

Company name: Jiangsu Yuyue Medical Equipment & Supply Co., Ltd.
ADD: No.1 Baisheng Road Development Zone, Danyang, Jiangsu province, 212300 China
TEL: +86 18252963550
FAX: +86-511-86900827
E-mail: qa.yuwell@yuyue.com.cn

Date: 2024/08/12

FEDERAL COMMUNICATIONS COMMISSIONS

Authorization and Evaluation Division
7435 Oakland Mills Road
Columbia, MD 21046

Subject: Description of Permissive Change


Dear Sir/Madam,

We, Jiangsu Yuyue Medical Equipment & Supply Co., Ltd. hereby authorize Bay Area Compliance Laboratories Corp. (Kunshan) to act as a laboratory for testing and test report generation for the following project(s):

FCC ID: 2A2JJYE650ARS

Model Name: YE650AR

Original Grant Date: 2024/05/21

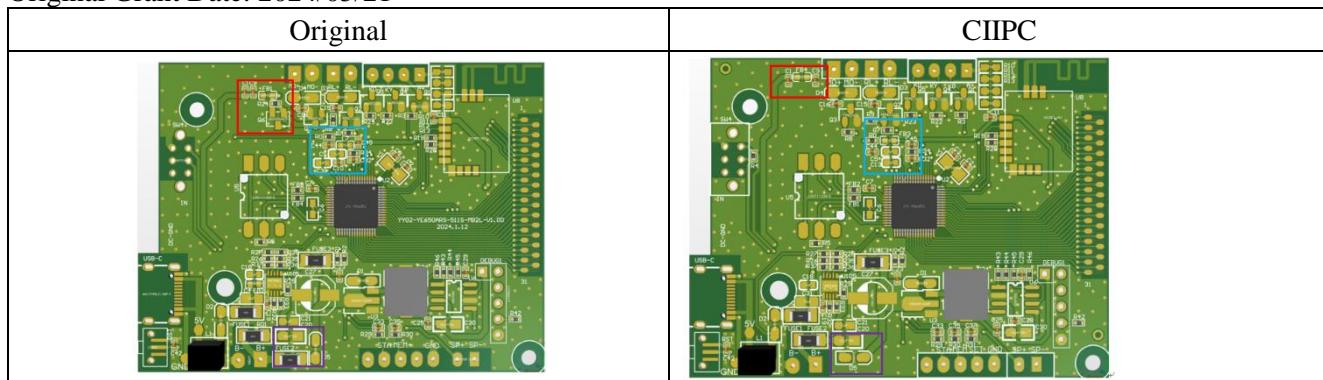

Detailed information:

1. The red part modifies the air pump control circuit and component layout, the blue part modifies the layout of microcontroller peripheral devices, the purple part modifies the fuse position and removes a $0\ \Omega$ resistor.
2. YE650AR IP classification is changed from IP20 to IP21, and its structure is adjusted as follows: reduced 0.45mm thickness for top cover buttons, and a 0.45mm thick, 2mm wide foam has been added to the panel button area.
3. Change the tested model from "YE650ARS" to "YE650AR".

We affirm that between Bay Area Compliance Laboratories Corp. (Kunshan) and Jiangsu Yuyue Medical Equipment & Supply Co., Ltd. any difference in understanding, including test plan, measurement methods, applicable standards and relevant procedures and processes have been resolved prior to commencement of testing activities.

This authorization is valid until further written notice from the applicant.

Sincerely,
Signature: *Caixia Yang*

Printed Name: Caixia Yang

Title: RA Engineer