


GBI Model: ITQ-MODULE
FCC ID: 2A3CW001

750-00600

MV11-94V-0

2003 R2.0

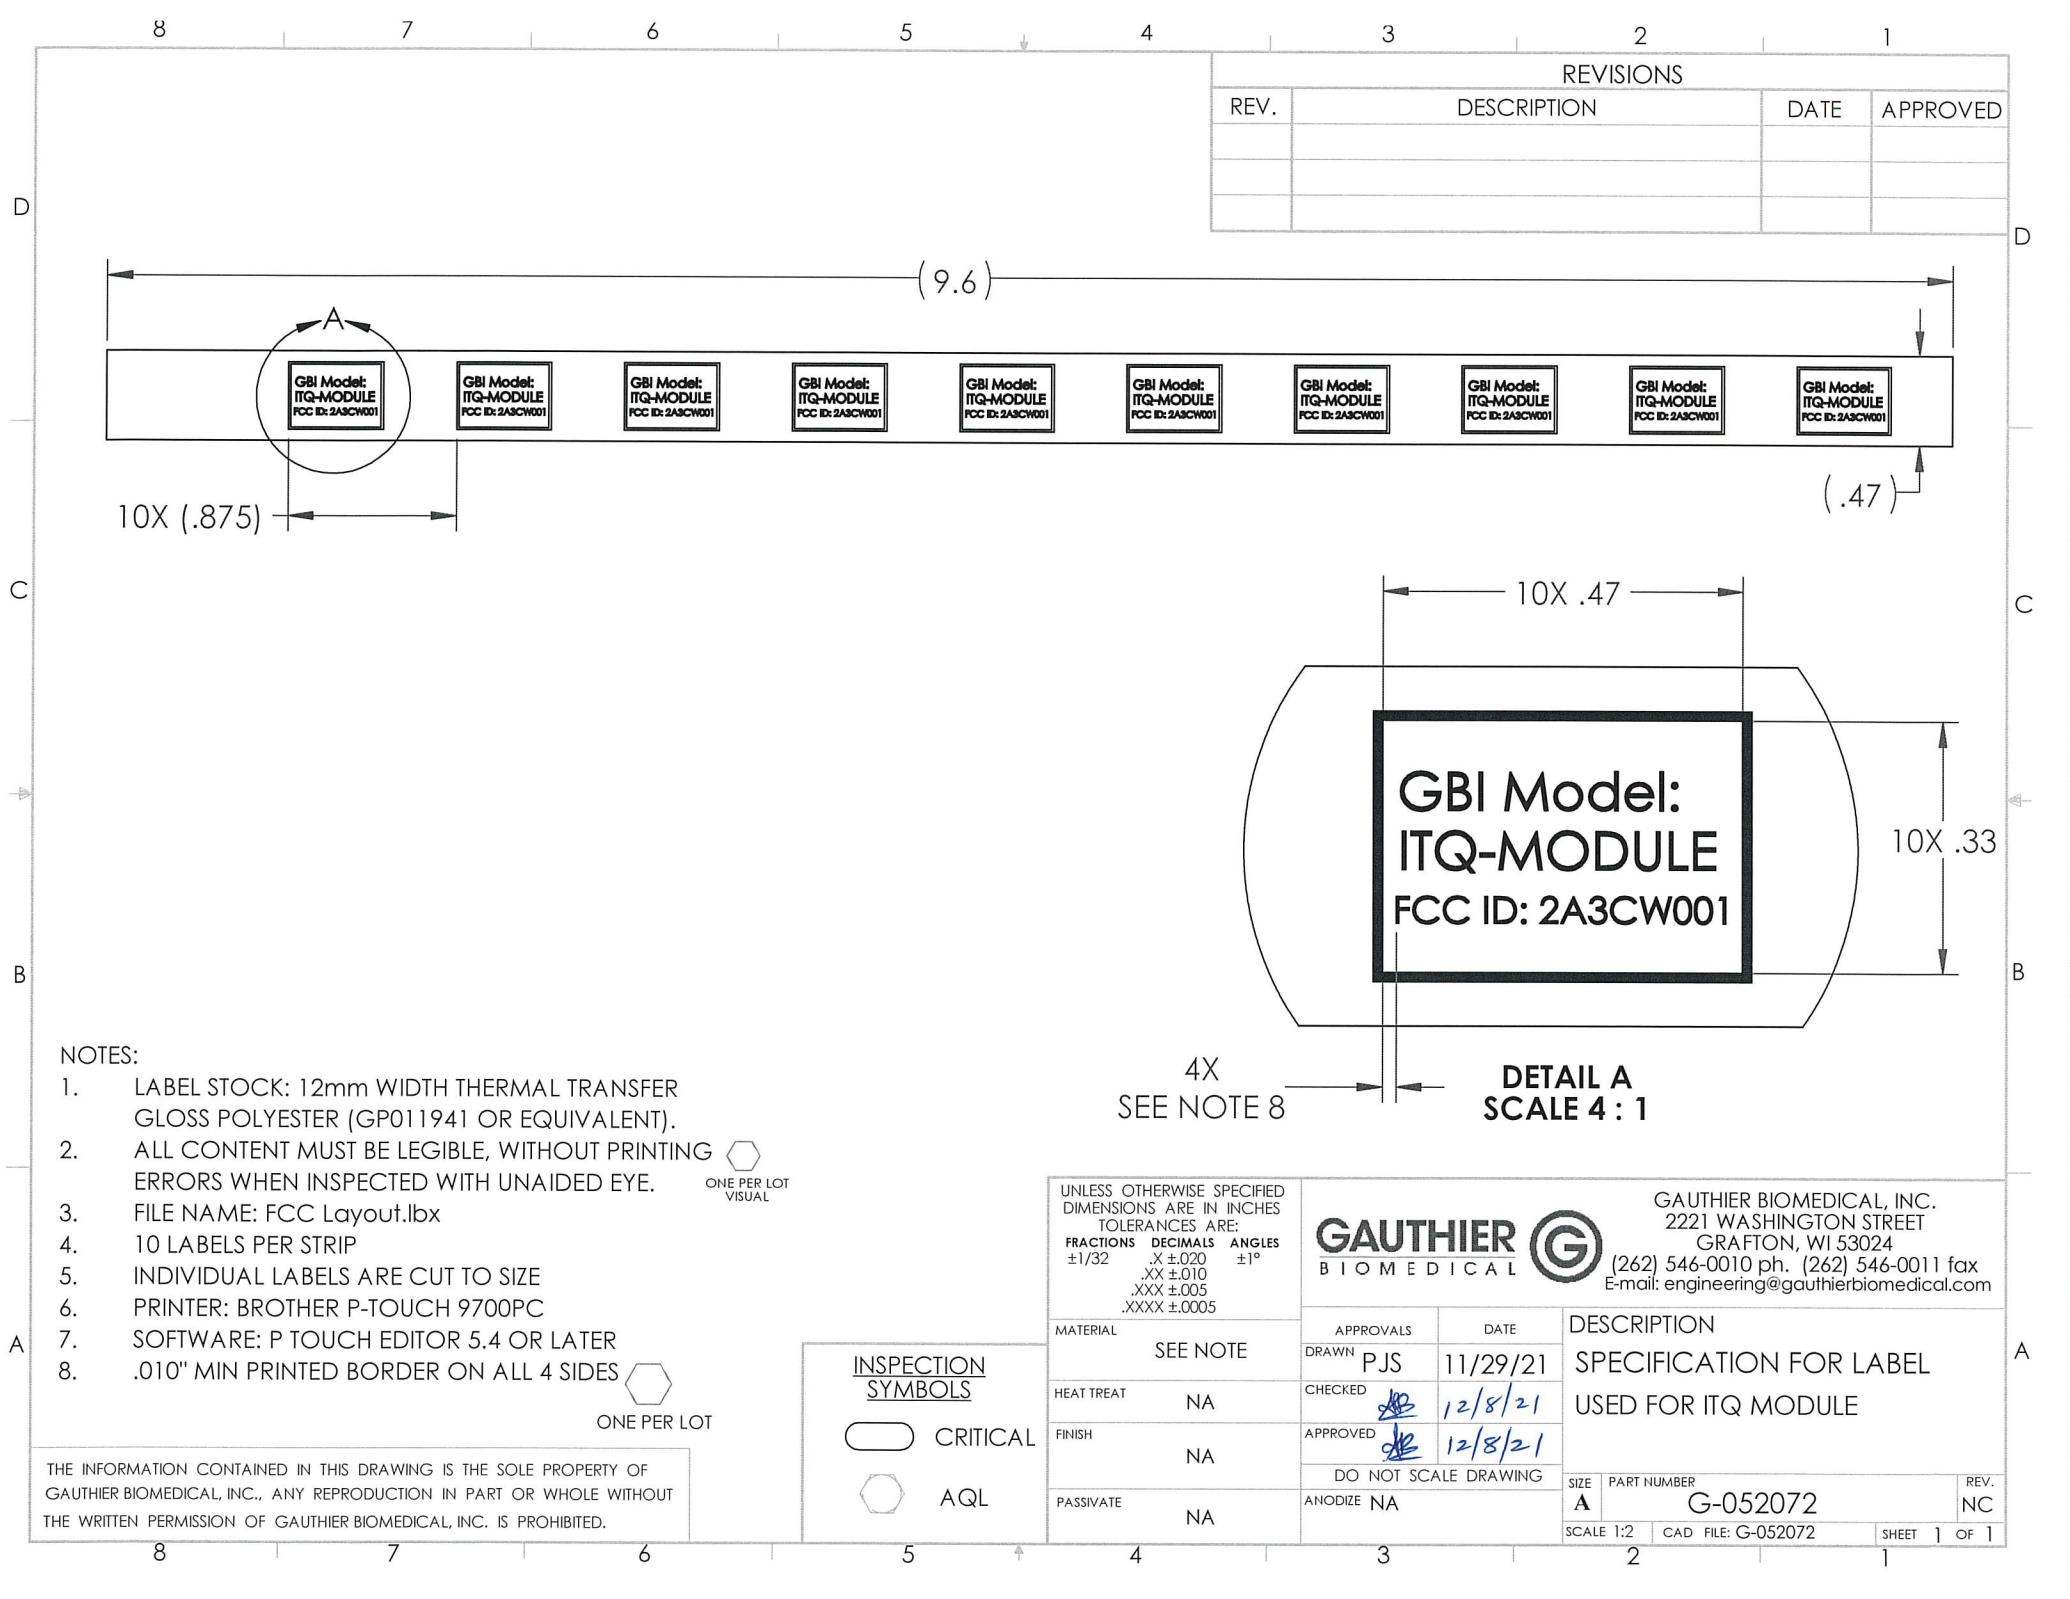

REVISIONS			
REV.	DESCRIPTION	DATE	APPROVED

NOTES:

1. LABEL STOCK: 12mm WIDTH THERMAL TRANSFER GLOSS POLYESTER (GP011941 OR EQUIVALENT).
2. ALL CONTENT MUST BE LEGIBLE, WITHOUT PRINTING ERRORS WHEN INSPECTED WITH UNAIDED EYE.  ONE PER LOT VISUAL
3. FILE NAME: FCC Layout.lbx
4. 10 LABELS PER STRIP
5. INDIVIDUAL LABELS ARE CUT TO SIZE
6. PRINTER: BROTHER P-TOUCH 9700PC
7. SOFTWARE: P TOUCH EDITOR 5.4 OR LATER
8. .010" MIN PRINTED BORDER ON ALL 4 SIDES  ONE PER LOT

THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF GAUTHIER BIOMEDICAL, INC., ANY REPRODUCTION IN PART OR WHOLE WITHOUT THE WRITTEN PERMISSION OF GAUTHIER BIOMEDICAL, INC. IS PROHIBITED.

INSPECTION
SYMBOLS



UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES
TOLERANCES ARE:
FRACTIONS DECIMALS ANGLES
±1/32 .X ±.020 ±1°
.XX ±.010
.XXX ±.005
.XXXX ±.0005

MATERIAL	SEE NOTE
HEAT TREAT	NA
FINISH	NA
PASSIVATE	NA

GAUTHIER 
BIOMEDICAL

GAUTHIER BIOMEDICAL, INC.
2221 WASHINGTON STREET
GRAFTON, WI 53024
(262) 546-0010 ph. (262) 546-0011 fax
E-mail: engineering@gauthierbiomedical.com

APPROVALS		DATE
DRAWN	PJS	11/29/21
CHECKED		12/8/21
APPROVED		12/8/21
DO NOT SCALE DRAWING		
ANODIZE	NA	

DESCRIPTION
SPECIFICATION FOR LABEL
USED FOR ITQ MODULE

SIZE A	PART NUMBER G-052072	REV. NC
SCALE 1:2	CAD FILE: G-052072	SHEET 1 OF 1