



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details



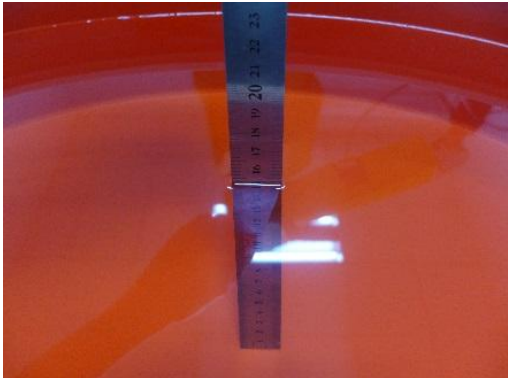


1. SAR measurement System





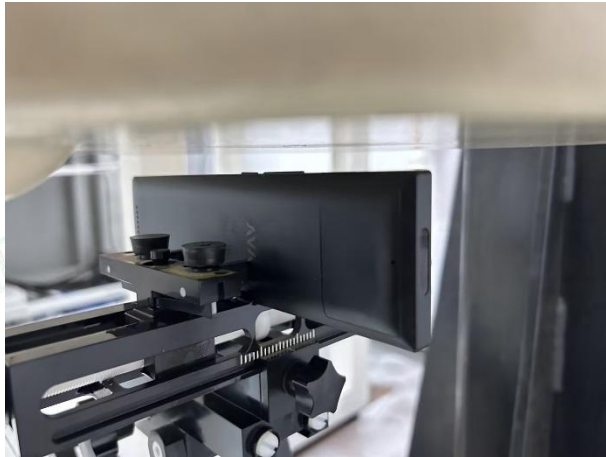
2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 5000
	





3. Photographs of EUT test position

Photo 3: Front side 10mm	Photo 4: Rear side 10mm
	
Photo 5: Left side 10mm	Photo 6: Right side 10mm
	
Photo 7: Bottom side 10mm	NA
	NA





4. EUT Constructional Details

Photo 8: Front View	Photo 9: Rear View
