

Appendix C for KSCR230500078901

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date	Due date of calibration
Dipole	☐	1	CLA150	4025	2021/04/26	2024/04/25
	☐	2	D450V3	1103	2021/04/21	2024/04/20
	☐	3	D750V3	1188	2022/03/29	2025/03/28
	☐	4	D835V2	4d114	2022/03/31	2025/03/30
	☐	5	D900V2	1d079	2022/06/07	2025/06/06
	☐	6	D1800V2	2d170	2022/03/31	2025/03/30
	☐	7	D1900V2	5d136	2022/06/07	2025/06/06
	☐	8	D2000V2	1041	2022/06/06	2025/06/05
	☐	9	D2300V2	1096	2022/03/31	2025/03/30
	☒	10	D2450V2	817	2022/04/01	2025/03/31
	☐	11	D2600V2	1158	2022/03/31	2025/03/30
	☐	12	D5GHzV2	1095	2022/06/01	2025/05/31
DAE	☒	13	DAE4	910	2022/07/14	2023/07/13
Probe	☒	14	EX3DV4	7767	2022/10/28	2023/10/27



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgsgroup.com.cn
 中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

1 Dipole

1.1 CLA150 - SN 4025

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Client: SGS-CN (Auden)		Certificate No: CLA150-4025_Apr21	
CALIBRATION CERTIFICATE			
Object: CLA150 - SN: 4025			
Calibration procedure(s): QA CAL-15-v9 Calibration Procedure for SAR Validation Sources below 700 MHz			
Calibration date: April 26, 2021			
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature $22 \pm 3^\circ\text{C}$ and humidity $< 70\%$.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 10476	09-Apr-21 (No. 217-03201/03202)	Apr-22
Power sensor NRP Z91	SN: 10344	09-Apr-21 (No. 217-03201)	Apr-22
Power sensor NRP Z91	SN: 10345	09-Apr-21 (No. 217-03202)	Apr-22
Reference 20 dB Attenuator	SN: C22862 (203)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310952 / 00357	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX30N4	SN: 3877	30-Dec-20 (No. EX3-3877_Dec20)	Dec-21
ENEA4	SN: 684	26-Jan-20 (No. D458-684_Jan20)	Jun-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter S44135	SN: G841203074	06-Apr-18 (in house check Jun-20)	In house check Jun-22
Power sensor E4113A	SN: MY41490807	06-Apr-18 (in house check Jun-20)	In house check Jun-22
Power sensor E4113A	SN: 000110210	06-Apr-18 (in house check Jun-20)	In house check Jun-22
RF generator HP 8464D	SN: U5846401709	04-Apr-18 (in house check Jun-20)	In house check Jun-22
Network Analyser Agilent E8363A	SN: U541000477	31-Mar-14 (in house check Oct-20)	In house check Oct-21
Calibrated by:	Name: Jeffrey Katsman	Function: Laboratory Technician	Signature:
Approved by:	Name: Kaja Polovic	Function: Technical Manager	Signature:
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: April 26, 2021			
Certificate No: CLA150-4025_Apr21		Page 1 of 6	

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Glossary:			
TSL: tissue simulating liquid			
ConvF: sensitivity in TSL / NORM x,y,z			
N/A: not applicable or not measured			
Calibration is Performed According to the Following Standards:			
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Technique", June 2013			
b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016			
c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010			
d) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
e) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.			
• Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: CLA150-4025_Apr21		Page 2 of 6	

Measurement Conditions DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELIA Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	$dx, dy = 4.0$ mm, $dz = 1.4$ mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz $\pm$ 1 MHz	

Head TSL parameters The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0°C	62.3	0.75 mho/m
Measured Head TSL parameters	$(22.0 \pm 0.2)^\circ\text{C}$	$61.1 \pm 6\%$	0.75 mho/m $\pm 6\%$
Head TSL temperature change during test	$< 0.5^\circ\text{C}$	---	---

SAR result with Head TSL		
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.90 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	$3.88\text{ W/kg} \pm 19.4\% (\text{kw2})$
SAR averaged over 10 cm^3 (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.60 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	$2.59\text{ W/kg} \pm 18.0\% (\text{kw2})$

Appendix (Additional assessments outside the scope of SCS 0108)	
Antenna Parameters with Head TSL	
Impedance, transformed to feed point	$47.9\Omega \pm 1.5\Omega$
Return Loss	-31.4 dB
Additional EUT Data	
Manufactured by	SPEAG

Certificate No: CLA150-4025_Apr21 Page 3 of 6


Certificate No: CLA150-4025_Apr21 Page 4 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 57355888 f(86-512) 57370818 www.sgs.com.cn
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

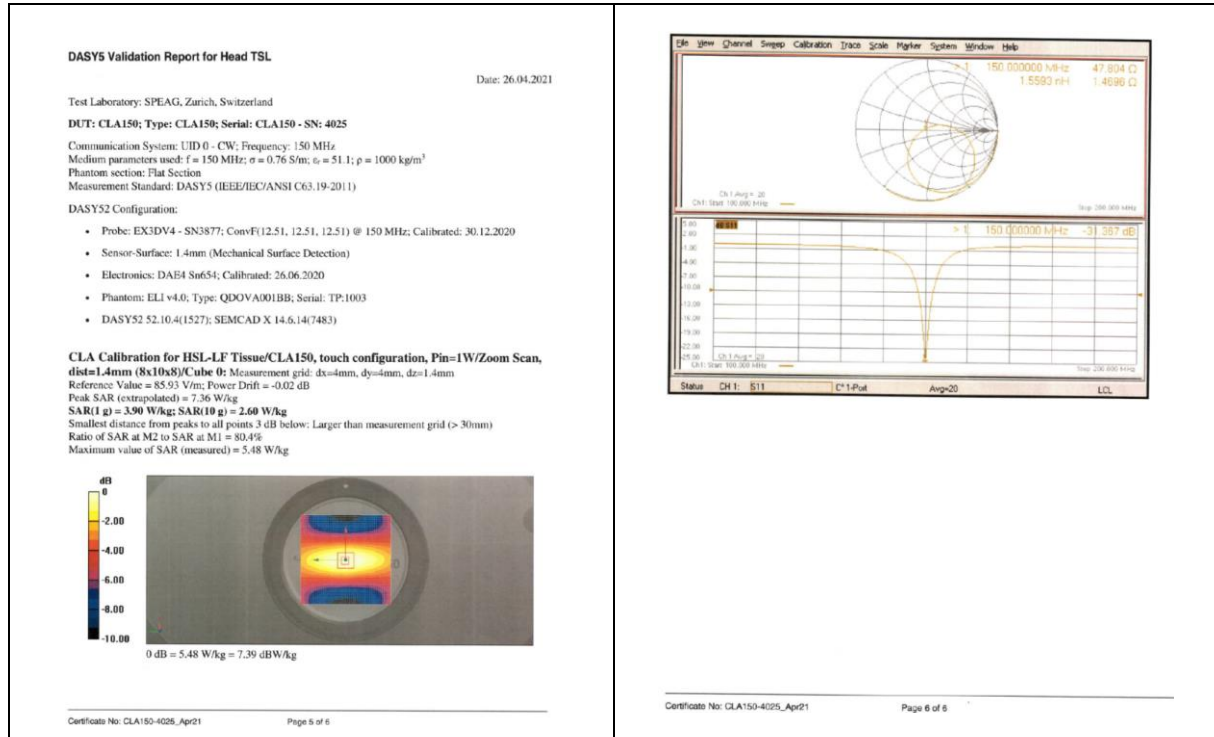

1.2 D450V3 - SN 1103

Calibration Laboratory of Schmid & Partner Engineering AG
Zweigschulstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aude)** Certificate No: **D450V3-1103_Apr21**

CALIBRATION CERTIFICATE

Object: **D450V3 - SN: 1103**

Calibration procedure(s): **QA CAL-15-v9**
Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 2) °C and humidity < 70%.

Calibration Equipment used (MPE: critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03201/03202)	Apr-22
Power sensor NRP-291	SN: 103244	09-Apr-21 (No. 217-03201)	Apr-22
Power sensor NRP-291	SN: 103245	09-Apr-21 (No. 217-03202)	Apr-22
Reference 20 dB Attenuator	SN: CG2852 (200)	09-Apr-21 (No. 217-03345)	Apr-22
Type-N mismatch combination	SN: 310852 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe E30309	SN: 3877	30-Dec-20 (No. E30-3877 Dec20)	Dec-21
DAEA	SN: 654	26-Jun-20 (No. D454-654-Jun20)	Jun-21

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E44198	SN: GB41200274	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
Power sensor E4412A	SN: MY41496047	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
Power sensor E4412A	SN: 00010010	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
RF generator HP 8548C	SN: L033400101700	06-Aug-09 (in house check Jun-20)	In house check: Jun-22
Network Analyzer Agilent E8358A	SN: U841080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21

Calibrated by: **Christoph Leubner** Function: **Laboratory Technician**

Approved by: **Krista Polovic** Technical Manager

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D450V3-1103_Apr21

Page 1 of 6

Calibration Laboratory of Schmid & Partner Engineering AG
Zweigschulstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No: **SCS 0106**

Glossary:

TSL: Issue simulating liquid sensitivity in TSL / NORM x,y,z

ConvF: not applicable or not measured

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC 61010-1:2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21

Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgsgroup.com.cn
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

Measurement Conditions

DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V82.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELJ4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.57 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	43.1 ± 6 %	0.07 mho/m ± 8 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.55 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	0.757 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg ± 17.6 % (k=2)

Certificate No: D450V3-1103_Apr21

Page 5 of 6

Appendix (Additional assessments outside the scope of SCS 0106)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	57.1 Ω - j2.6 jΩ
Return Loss	-23.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.346 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: D450V3-1103_Apr21

Page 4 of 6

DASY5 Validation Report for Head TSL

Test Laboratory: SPEAG, Zurich, Switzerland

Date: 21.04.2021

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103

Communication System: UTD 0 - CW; Frequency: 450 MHz

Medium parameters used: f = 450 MHz; α = 0.87 S/m; ε = 43.1; ρ = 1000 kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.64, 10.64, 10.64) @ 450 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 26.06.2020
- Phantom: ELJ v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue(d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 39.18 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 1.76 W/kg

SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.767 W/kg

Smallest distance from peaks to all points 3 dB below: Larger than measurement grid

Ratio of SAR at M2 to SAR at M1 = 64.9%

Maximum value of SAR (measured) = 1.53 W/kg

0 dB = 1.53 W/kg = 1.85 dBW/kg

Certificate No: D450V3-1103_Apr21

Page 5 of 6

File View Channel Sweep Calibration Trace Scale Marker System Window Help

Certificate No: D450V3-1103_Apr21

Page 4 of 6


1.3 D750V3 - SN 1188

TTL Speag CALIBRATION LABORATORY		CAICT																					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn																					
Client: SGS-CN		Certificate No: Z22-60103																					
CALIBRATION CERTIFICATE																							
Object: D750V3 - SN: 1188																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 28, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.																							
Calibration Equipment used (M&TE critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>104277</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP88</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX30V4</td><td>SN 7307</td><td>26-May-21(SPEAG.No.EX3-7307_May21)</td><td>May-22</td></tr><tr><td>D4E4</td><td>SN 1556</td><td>12-Jan-22(CTTL-SPEAG.No.Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	104277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP88	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX30V4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22	D4E4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	104277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Power sensor NRP88	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Reference Probe EX30V4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22																				
D4E4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator S4438C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY46110673</td><td>14-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator S4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator S4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Calibrated by: Zhao Jing SAR Test Engineer																							
Reviewed by: Lin Hao SAR Test Engineer																							
Approved by: Qi Dianyan SAR Project Leader																							
Issued: April 3, 2022																							
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-60103		Page 1 of 6																					

TTL Speag CALIBRATION LABORATORY		CAICT																						
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn																						
Measurement Conditions DASY system configuration, as far as not given on page 1:																								
<table border="1"><thead><tr><th>DASY Version</th><th>DASY52</th><th>V52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>750 MHz ± 1 MHz</td><td></td></tr></tbody></table>				DASY Version	DASY52	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz				
DASY Version	DASY52	V52.10.4																						
Extrapolation	Advanced Extrapolation																							
Phantom	Triple Flat Phantom 5.1C																							
Distance Dipole Center - TSL	15 mm	with Spacer																						
Zoom Scan Resolution	dx, dy, dz = 5 mm																							
Frequency	750 MHz ± 1 MHz																							
Head TSL parameters The following parameters and calculations were applied:																								
<table border="1"><thead><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>42.0</td><td>0.90 mho/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>41.4 ± 6 %</td><td>0.89 mho/m ± 6 %</td></tr><tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>---</td><td>---</td></tr></tbody></table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---					
	Temperature	Permittivity	Conductivity																					
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m																					
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %																					
Head TSL temperature change during test	<1.0 °C	---	---																					
SAR result with Head TSL																								
<table border="1"><thead><tr><th></th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR averaged over 1 cm² (1 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>2.07 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>8.27 W/kg ± 18.8 % (k=2)</td></tr><tr><td>SAR averaged over 10 cm² (10 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>1.37 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>5.48 W/kg ± 18.7 % (k=2)</td></tr></tbody></table>					Condition		SAR averaged over 1 cm ² (1 g) of Head TSL			SAR measured	250 mW input power	2.07 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL			SAR measured	250 mW input power	1.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)
	Condition																							
SAR averaged over 1 cm ² (1 g) of Head TSL																								
SAR measured	250 mW input power	2.07 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)																						
SAR averaged over 10 cm ² (10 g) of Head TSL																								
SAR measured	250 mW input power	1.37 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)																						
Certificate No: Z22-60103		Page 3 of 6																						

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• MY for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60103		Page 2 of 6	

TTL Speag CALIBRATION LABORATORY		CAICT					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn					
Appendix (Additional assessments outside the scope of CNAS L0570)							
Antenna Parameters with Head TSL							
<table border="1"><thead><tr><th>Impedance, transformed to feed point</th><th>53.60-1.13jΩ</th></tr><tr><th>Return Loss</th><th>-28.7dB</th></tr></thead></table>				Impedance, transformed to feed point	53.60-1.13jΩ	Return Loss	-28.7dB
Impedance, transformed to feed point	53.60-1.13jΩ						
Return Loss	-28.7dB						
General Antenna Parameters and Design							
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>0.947 ns</th></tr></thead></table>				Electrical Delay (one direction)	0.947 ns		
Electrical Delay (one direction)	0.947 ns						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.							
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.							
Additional EUT Data							
<table border="1"><thead><tr><th>Manufactured by</th><th>SPEAG</th></tr></thead></table>				Manufactured by	SPEAG		
Manufactured by	SPEAG						
Certificate No: Z22-60103		Page 4 of 6					

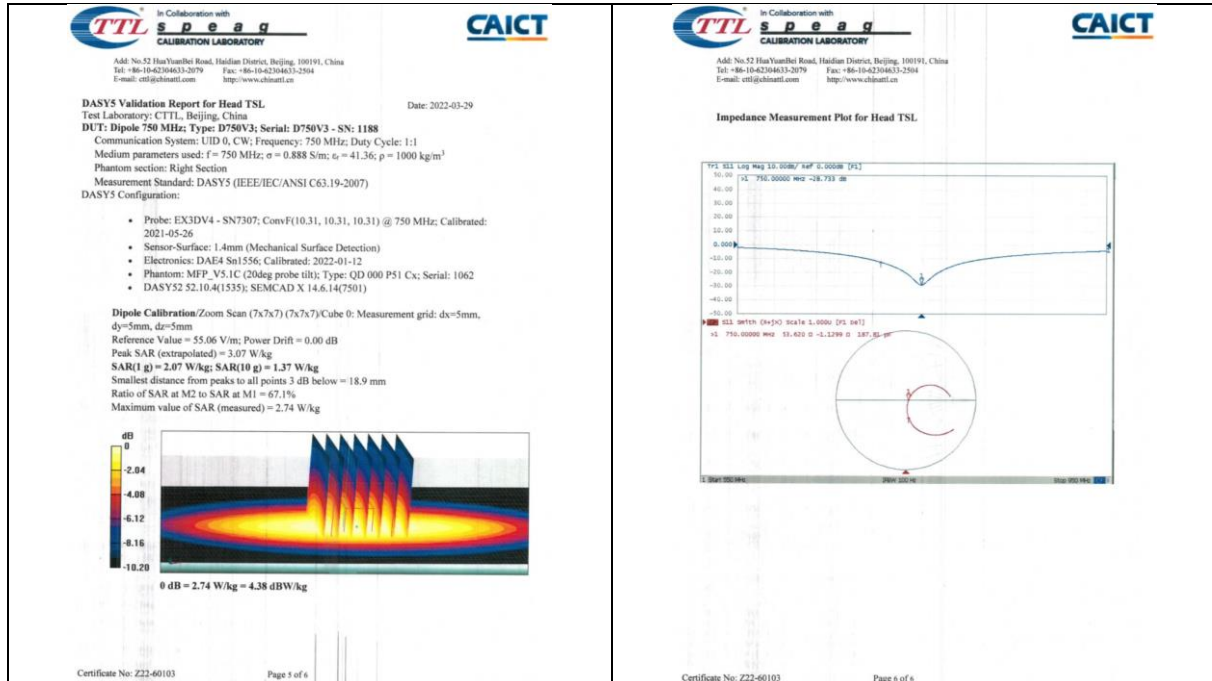

1.4 D835V2 - SN 4d114

TTS Calibration Laboratory		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62046131-2079 Fax: +86-10-62046131-2504 E-mail: cti@china.tts.com.cn http://www.china.tts.com.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62046131-2079 Fax: +86-10-62046131-2504 E-mail: cti@china.tts.com.cn http://www.china.tts.com.cn	
Client: SGS-CN		Certificate No: Z22-60104	
CALIBRATION CERTIFICATE			
Object: D835V2 - SN: 4d114			
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits			
Calibration date: March 31, 2022			
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRPBS	104261	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23
Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: [Signature]
Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: [Signature]
Approved by:	Name: Qi Diqian	Function: SAR Project Leader	Signature: [Signature]
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: Z22-60104 Page 1 of 6

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured


Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 665864, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:
c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:
• **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
• **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
• **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
• **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
• **SAR measured:** SAR measured at the stated antenna input power.
• **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
• **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60104 Page 2 of 6

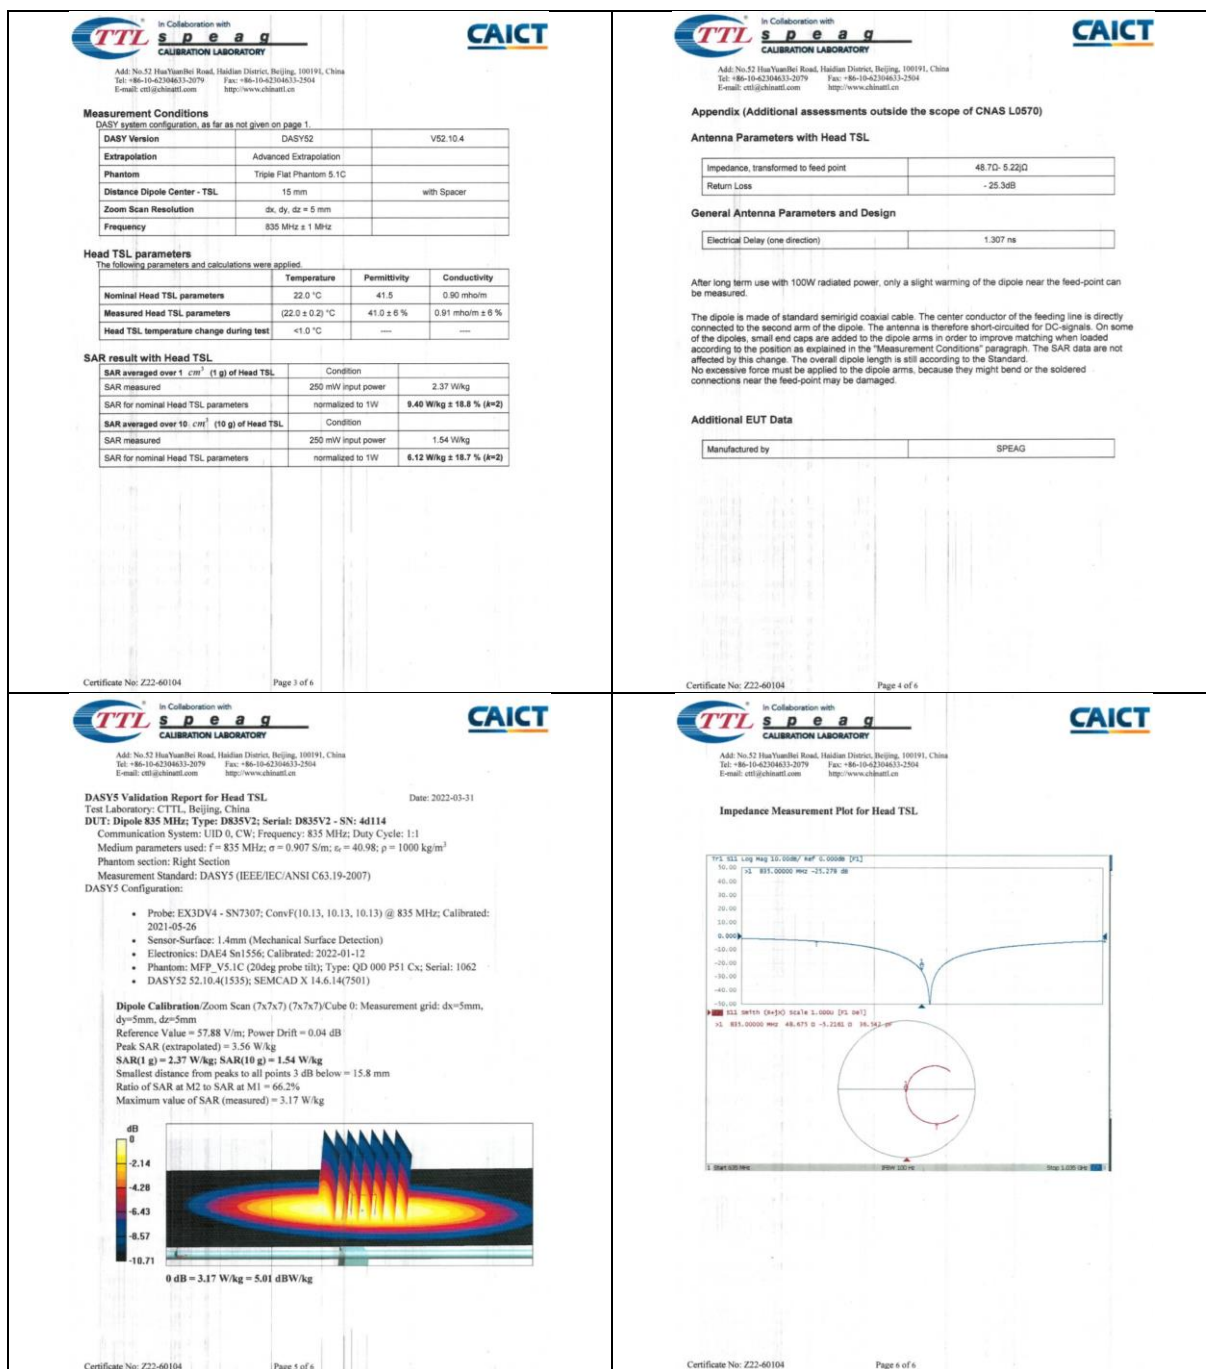

1.5 D900V2 - SN 1d079

In Collaboration with TTL CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn	
Client: SGS-CN		Certificate No: Z22-60184	
CALIBRATION CERTIFICATE			
Object: D900V2 - SN: 1d079			
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits			
Calibration date: June 7, 2022			
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±1)°C and humidity <70%.			
Calibration Equipment used (MATE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7464	28-Jan-22 (SPEAG No EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071450	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23
Calibrated by: Zhao Jing SAR Test Engineer			
Reviewed by: Lin Hao SAR Test Engineer			
Approved by: Qi Dianyuan SAR Project Leader			
Issued: June 13, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60184		Page 1 of 6	

In Collaboration with TTL CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn	
Certificate No: Z22-60184		Page 2 of 6	

In Collaboration with TTL CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dk, dy, dz = 5 mm		
Frequency	900 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.97 nholm
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 nholm ± 6 %
Head TSL temperature change during test	+1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.70 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.79 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60184		Page 3 of 6	

In Collaboration with TTL CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn	
Certificate No: Z22-60184		Page 4 of 6	


In Collaboration with TTL CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2117 E-mail: cti@china.com.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.10 - j8.49Ω		
Return Loss	-23.3 dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.312 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60184		Page 4 of 6	



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/terms-and-conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgs.com.cn
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

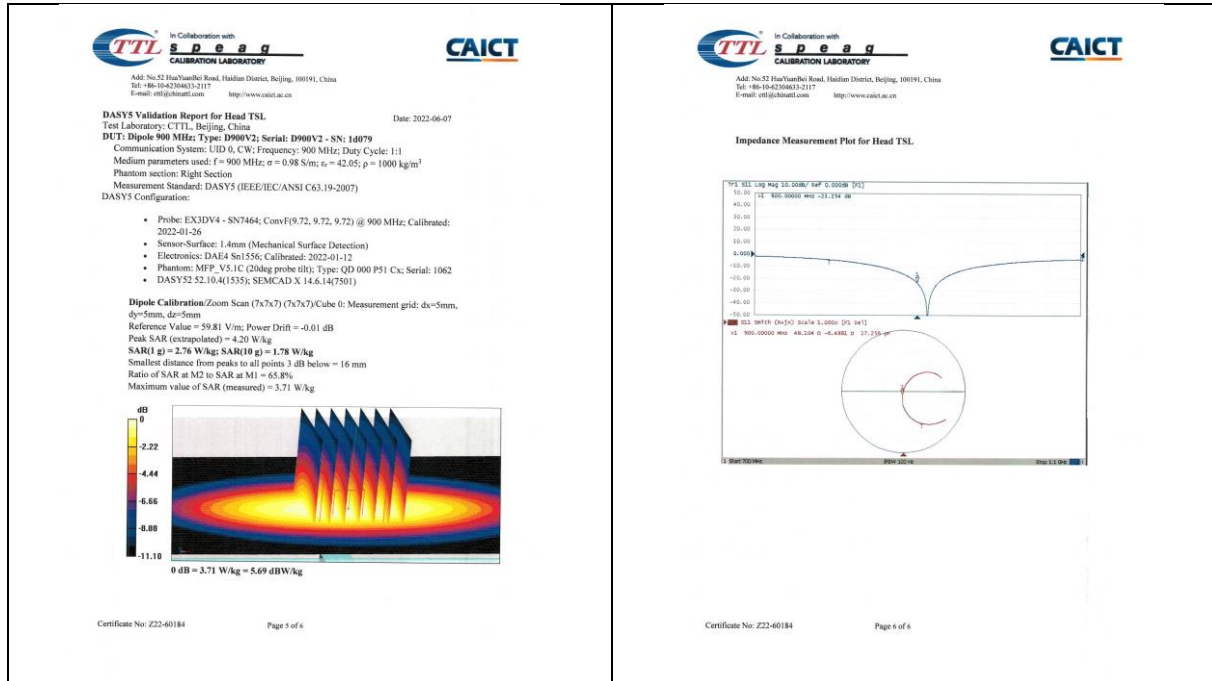

1.6 D1800V2 - SN 2d170

TTL In Collaboration with **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42304633-2117 Fax: +86-10-42304633-2118
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY46110573	14-Jan-22 (CTTL No.J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer

Reviewed by: **Lin Hao** SAR Test Engineer

Approved by: **Qi Diqian** SAR Project Leader

Issued April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

TTL In Collaboration with **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.


Certificate No: Z22-60105 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgsgroup.com.cn
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

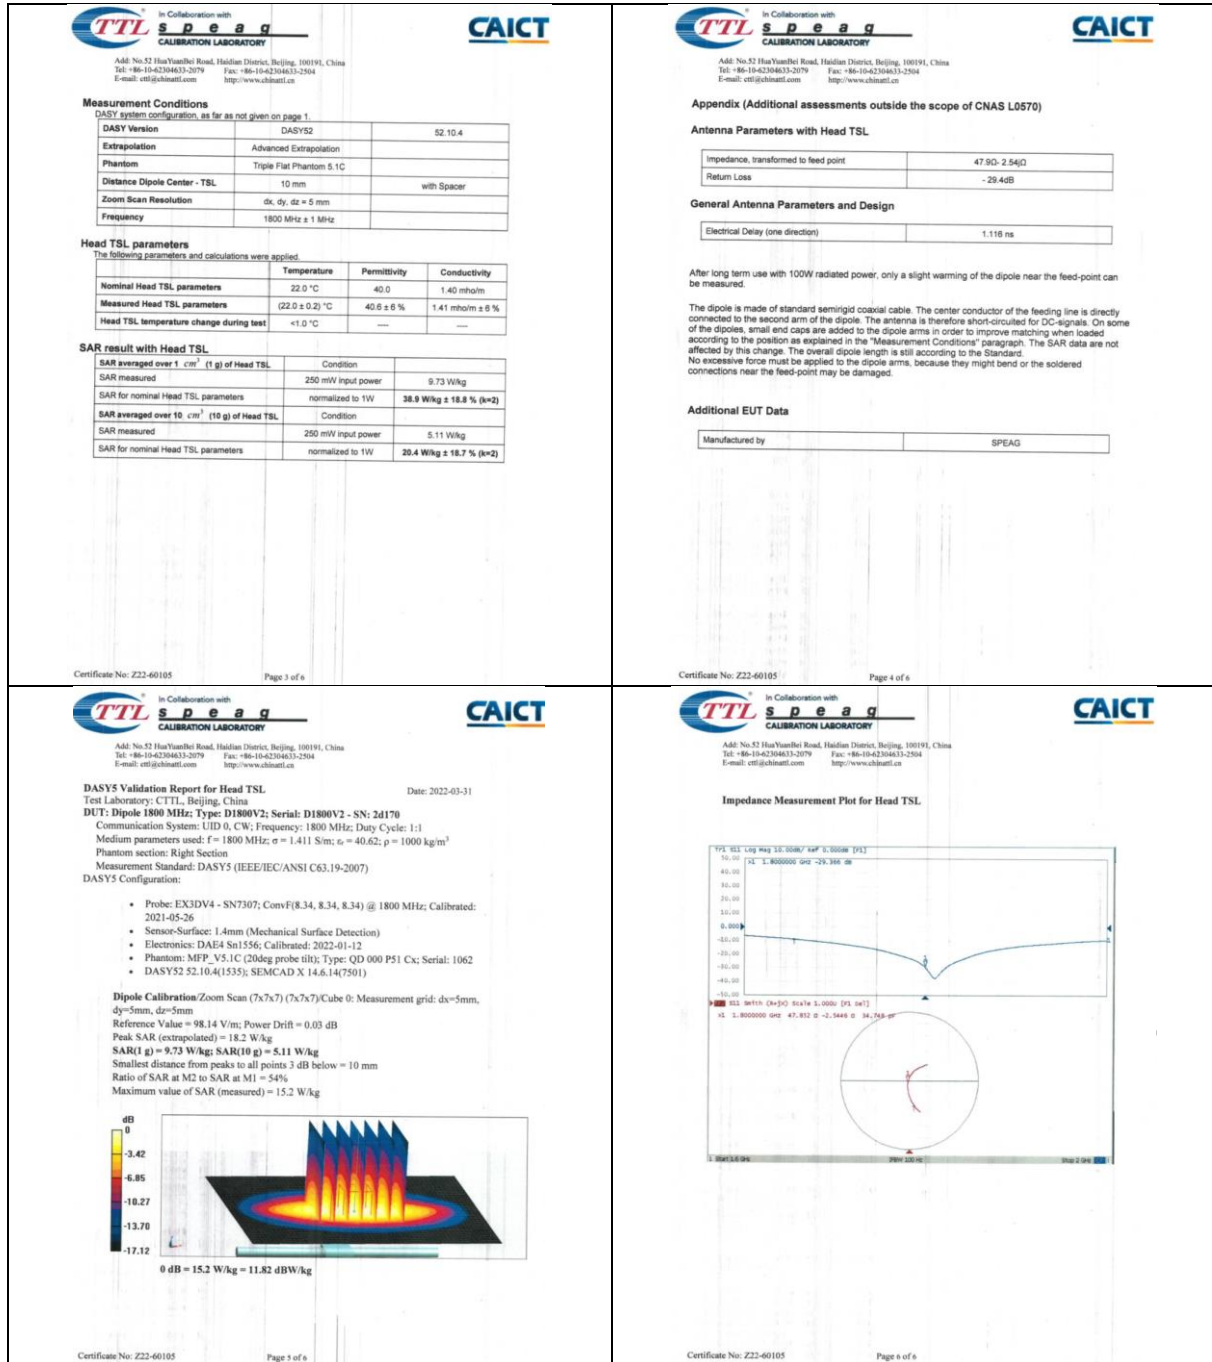

1.7 D1900V2 - SN 5d136

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42206033-2117 E-mail: cti@china.com.cn		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42206033-2117 E-mail: cti@china.com.cn	
Client: SGS-CN		Certificate No: Z22-60185	
CALIBRATION CERTIFICATE			
Object	D1900V2 - SN: 5d136		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	June 7, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±1)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP6S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EXSDV4	SN 7464	28-Jan-22 (SPEAG No EX3-7464_Jan22)	Jan-23
DAE4	SN 1656	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00409)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: June 13, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60185		Page 1 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42206033-2117 E-mail: cti@china.com.cn		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42206033-2117 E-mail: cti@china.com.cn	
Glossary:			
TSL	tissue simulating liquid		
ComF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865984, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60185		Page 2 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42206033-2117 E-mail: cti@china.com.cn		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42206033-2117 E-mail: cti@china.com.cn	
Measurement Conditions			
DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52		52.10.4
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm		with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	1900 MHz ± 1 MHz		
Head TSL parameters			
The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	32.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.3) °C	39.9 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL		Condition	
SAR measured		250 mW input power	9.65 W/kg
SAR for nominal Head TSL parameters		normalized to 1W	40.0 W/kg ± 16.8 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL		Condition	
SAR measured		250 mW input power	5.18 W/kg
SAR for nominal Head TSL parameters		normalized to 1W	20.8 W/kg ± 18.7 % (k=2)
Certificate No: Z22-60185		Page 3 of 6	


TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42206033-2117 E-mail: cti@china.com.cn		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42206033-2117 E-mail: cti@china.com.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	51.02 ± 7.56Ω		
Return Loss	-22.4dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.109 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60185		Page 4 of 6	




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/terms-and-conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgs.com.cn
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

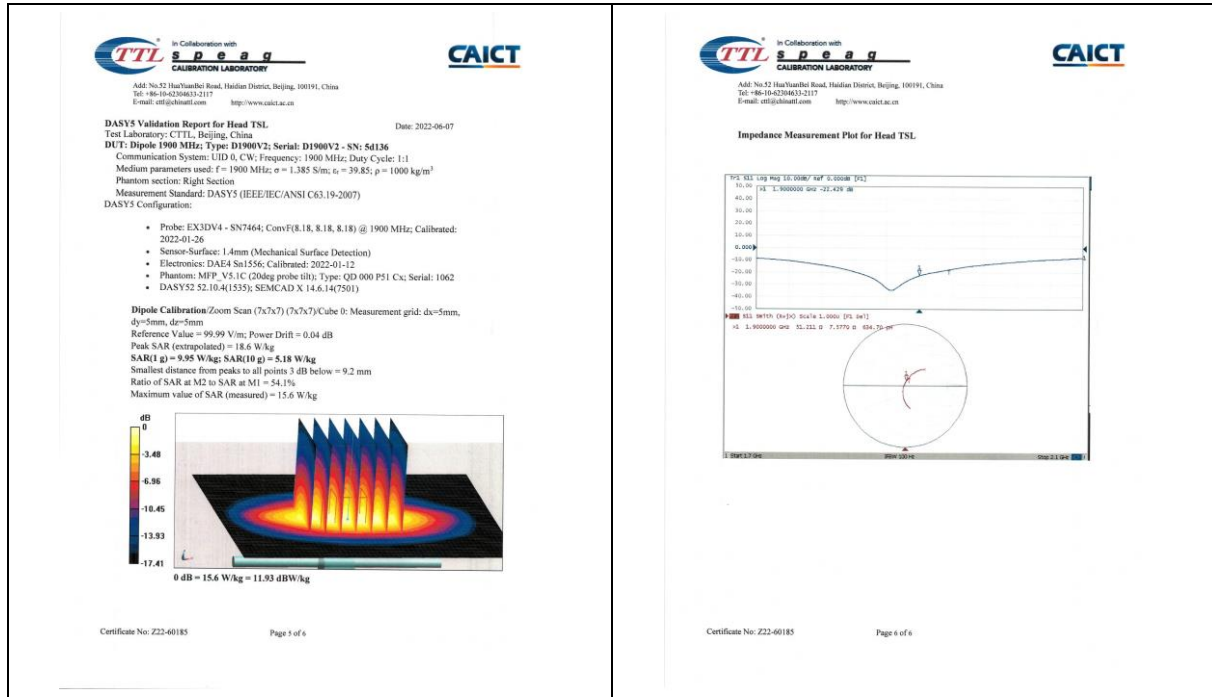

1.8 D2000V2 - SN 1041

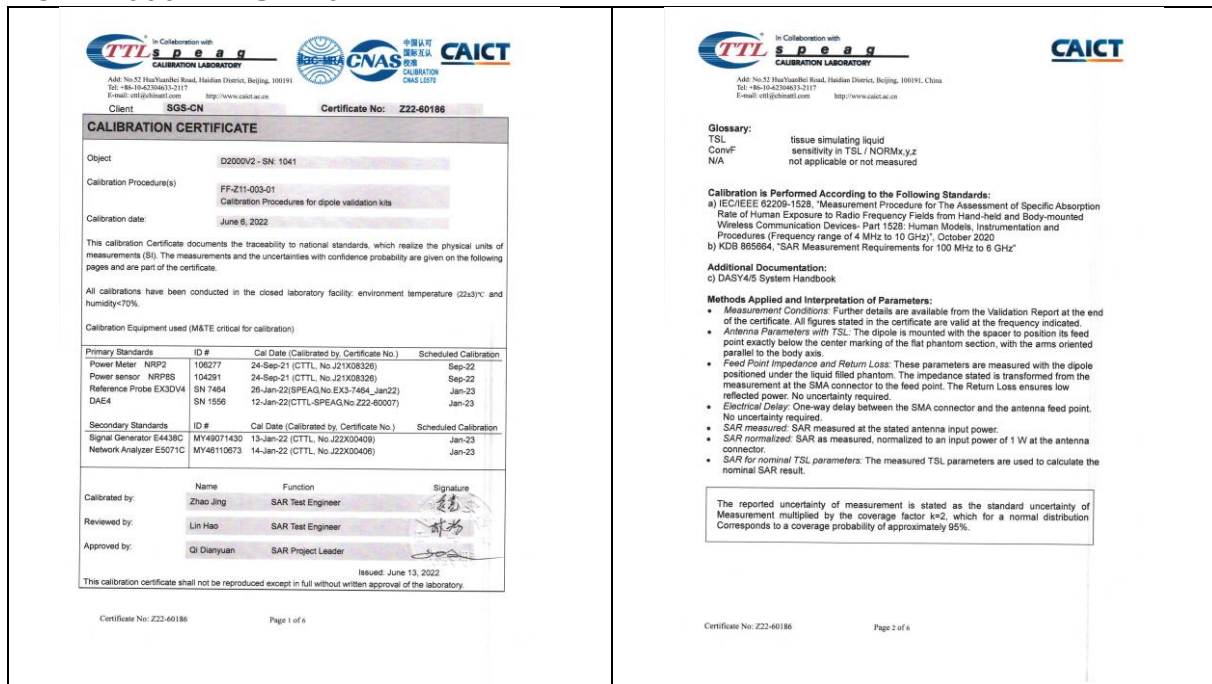

TTL In Collaboration with **CAICT**
SPeag
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62306633-2117
E-mail: cti@china.ttl.com http://www.caict.ac.cn

Measurement Conditions
DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom S.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2000 MHz ± 1 MHz	

Head TSL parameters
The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.4 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 16.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (k=2)

Certificate No: Z22-60186 Page 3 of 6

TTL In Collaboration with **CAICT**
SPeag
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62306633-2117
E-mail: cti@china.ttl.com http://www.caict.ac.cn

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.4Ω ± 0.74Ω
Return Loss	-34.9dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.088 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60186 Page 4 of 6


TTL In Collaboration with **CAICT**
SPeag
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62306633-2117
E-mail: cti@china.ttl.com http://www.caict.ac.cn

DASY5 Validation Report for Head TSL
Test Laboratory: CTTL, Beijing, China
DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041
Communication System: UTD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1
Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε_r = 40.21; ρ = 1000 kg/m³
Phantom section: Right Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(8.2, 8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sn1556; Calibrated: 2022-01-12
- Phantom: MPP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52: 52.10.4(1555); SEMCAD X 14.6(147501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 103.4 V/m; Power Drift = 0.03 dB
Peak SAR (extrapolated) = 19.6 W/kg
SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg
Smallest distance from peaks to all points 3 dB below = 9.1 mm
Ratio of SAR at M2 to SAR at M1 = 53.6%
Maximum value of SAR (measured) = 16.3 W/kg

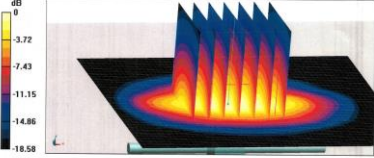


Certificate No: Z22-60186 Page 5 of 6

TTL In Collaboration with **CAICT**
SPeag
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62306633-2117
E-mail: cti@china.ttl.com http://www.caict.ac.cn

Impedance Measurement Plot for Head TSL

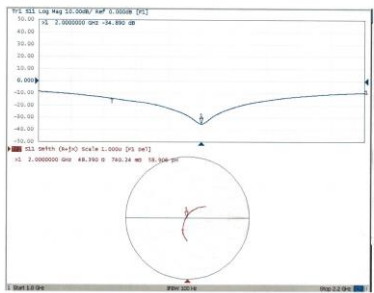


Certificate No: Z22-60186 Page 6 of 6

1.9 D2300V2 - SN 1096

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Client: SGS-CN		Certificate No: Z22-60106	
CALIBRATION CERTIFICATE			
Object: D2300V2 - SN: 1096			
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits			
Calibration date: March 31, 2022			
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards		ID # Cal Date (Calibrated by Certificate No.) Scheduled Calibration	
Power Meter NRP2		104277 24-Sep-21 (CTTL No.J21X08328) Sep-22	
Power sensor NRP8S		104291 24-Sep-21 (CTTL No.J21X08328) Sep-22	
Reference Probe EX30V4		SN 7307 26-May-21 (SPEAG No.EK3-7307_May21) May-22	
DAE4		SN 1556 12-Jan-22 (CTTL-SPEAG No.Z22-60007) Jan-23	
Secondary Standards		ID # Cal Date (Calibrated by Certificate No.) Scheduled Calibration	
Signal Generator E4438C		MY49071430 13-Jan-22 (CTTL No.J22X00406) Jan-23	
Network Analyzer E5071C		MY48110673 14-Jan-22 (CTTL No.J22X00406) Jan-23	
Calibrated by:		Name Function Signature	
Reviewed by:		Zhao Jing SAR Test Engineer	
Approved by:		Lin Hao SAR Test Engineer	
		Qi Dianyan SAR Project Leader	
		Issued: April 6, 2022	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60106		Page 1 of 6	
TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version		DASY2 52.10.4	
Extrapolation		Advanced Extrapolation	
Phantom		Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL		10 mm with Spacer	
Zoom Scan Resolution		dx, dy, dz = 5 mm	
Frequency		2300 MHz ± 1 MHz	
Head TSL parameters The following parameters and calculations were applied:			
Nominal Head TSL parameters		Temperature Permittivity Conductivity	
		22.0 °C 39.5 1.67 mho/m	
Measured Head TSL parameters		(22.0 ± 0.2) °C 39.8 ± 6 % 1.70 mho/m ± 6 %	
Head TSL temperature change during test		<1.0 °C — —	
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL		Condition	
SAR measured		250 mW input power 12.4 W/kg	
SAR for nominal Head TSL parameters		normalized to 1W 49.2 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL		Condition	
SAR measured		250 mW input power 5.88 W/kg	
SAR for nominal Head TSL parameters		normalized to 1W 23.4 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60106		Page 3 of 6	
TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point		49.20 - 4.56jΩ	
Return Loss		-26.6dB	
General Antenna Parameters and Design			
Electrical Delay (one direction)		1.083 ns	
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by		SPEAG	
Certificate No: Z22-60106		Page 4 of 6	



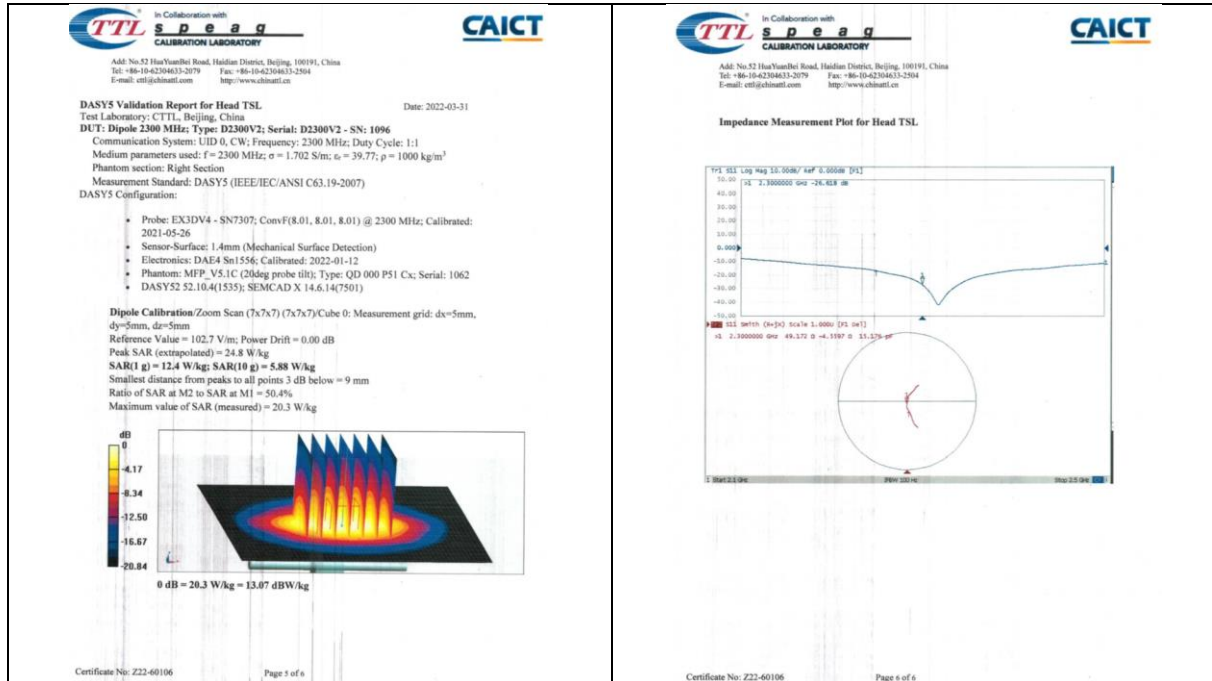

1.10 D2450V2 - SN 817

TTL In Collaboration with **CAICT**
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60107**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN: 817**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **April 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor: NRP8S	104291	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY46110873	14-Jan-22 (CTTL No.J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer Signature:

Reviewed by: **Lin Hao** SAR Test Engineer Signature:

Approved by: **Qi Dianyan** SAR Project Leader Signature:

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 6

TTL In Collaboration with **CAICT**
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.


Certificate No: Z22-60107 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/terms-and-conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgs.com
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

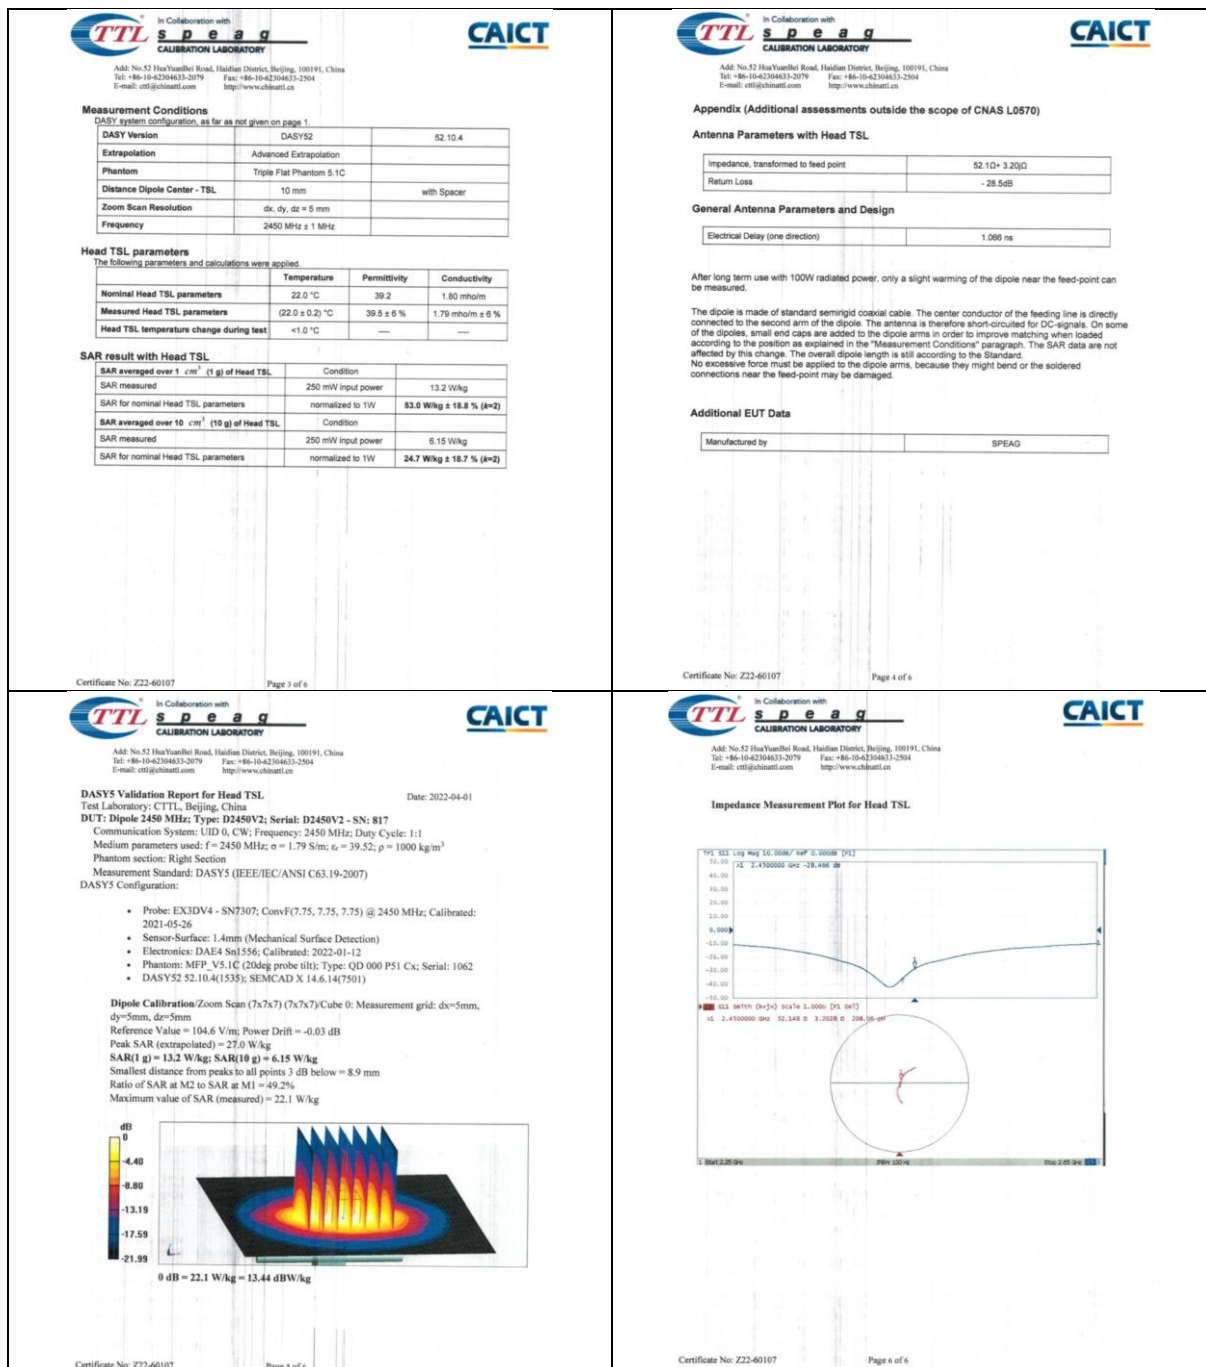


1.11 D2600V2 - SN 1158

TTL Speaq CALIBRATION LABORATORY		CAICT																					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn																					
Client: SGS-CN		Certificate No: Z22-40108																					
CALIBRATION CERTIFICATE																							
Object: D2600V2 - SN: 1158																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 31, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.																							
Calibration Equipment used (M&TE critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter: NRP2</td><td>106277</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor: NRPBS</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX3DVA</td><td>SN 7307</td><td>26-May-21 (SPEAG No EX3-7307_May21)</td><td>May-22</td></tr><tr><td>DAE4</td><td>SN 1556</td><td>12-Jan-22 (CTTL-SPEAG No Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor: NRPBS	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3DVA	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Power sensor: NRPBS	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Reference Probe EX3DVA	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22																				
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator E4438C</td><td>MY49071430</td><td>13-Jan-22 (CTTL No.J22X00406)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY48110673</td><td>14-Jan-22 (CTTL No.J22X00406)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23																				
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23																				
Calibrated by: Zhao Jing SAR Test Engineer																							
Reviewed by: Lin Hao SAR Test Engineer																							
Approved by: Qi Diaryuan SAR Project Leader																							
Issued: April 6, 2022																							
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-40108		Page 1 of 6																					

TTL Speaq CALIBRATION LABORATORY		CAICT																						
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn																						
Measurement Conditions DASY system configuration, as far as not given on page 1:																								
<table border="1"><thead><tr><th>DASY Version</th><th>DASY52</th><th>52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>2600 MHz ± 1 MHz</td><td></td></tr></tbody></table>				DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2600 MHz ± 1 MHz				
DASY Version	DASY52	52.10.4																						
Extrapolation	Advanced Extrapolation																							
Phantom	Triple Flat Phantom 5.1C																							
Distance Dipole Center - TSL	10 mm	with Spacer																						
Zoom Scan Resolution	dx, dy, dz = 5 mm																							
Frequency	2600 MHz ± 1 MHz																							
Head TSL parameters The following parameters and calculations were applied:																								
<table border="1"><thead><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>39.0</td><td>1.96 mho/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>36.7 ± 6 %</td><td>1.96 mho/m ± 6 %</td></tr><tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>---</td><td>---</td></tr></tbody></table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	36.7 ± 6 %	1.96 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---					
	Temperature	Permittivity	Conductivity																					
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m																					
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.7 ± 6 %	1.96 mho/m ± 6 %																					
Head TSL temperature change during test	<1.0 °C	---	---																					
SAR result with Head TSL																								
<table border="1"><thead><tr><th></th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR averaged over 1 cm² (1 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>13.7 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>54.8 W/kg ± 18.8 % (k=2)</td></tr><tr><td>SAR averaged over 10 cm² (10 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>6.12 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>24.6 W/kg ± 18.7 % (k=2)</td></tr></tbody></table>					Condition		SAR averaged over 1 cm ² (1 g) of Head TSL			SAR measured	250 mW input power	13.7 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL			SAR measured	250 mW input power	6.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg ± 18.7 % (k=2)
	Condition																							
SAR averaged over 1 cm ² (1 g) of Head TSL																								
SAR measured	250 mW input power	13.7 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)																						
SAR averaged over 10 cm ² (10 g) of Head TSL																								
SAR measured	250 mW input power	6.12 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg ± 18.7 % (k=2)																						
Certificate No: Z22-40108		Page 3 of 6																						

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn	
Glossary: TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.y.z N/A: not applicable or not measured			
Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation: c) DASY4/S System Handbook			
Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-40108		Page 2 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn					
Appendix (Additional assessments outside the scope of CNAS L0570)							
Antenna Parameters with Head TSL							
<table border="1"><thead><tr><th>Impedance, transformed to feed point</th><th>49.90-6.49jΩ</th></tr></thead><tbody><tr><td>Return Loss</td><td>-23.8dB</td></tr></tbody></table>				Impedance, transformed to feed point	49.90-6.49jΩ	Return Loss	-23.8dB
Impedance, transformed to feed point	49.90-6.49jΩ						
Return Loss	-23.8dB						
General Antenna Parameters and Design							
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>1.053 ns</th></tr></thead></table>				Electrical Delay (one direction)	1.053 ns		
Electrical Delay (one direction)	1.053 ns						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.							
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.							
Additional EUT Data							
<table border="1"><thead><tr><th>Manufactured by</th><th>SPEAG</th></tr></thead></table>				Manufactured by	SPEAG		
Manufactured by	SPEAG						
Certificate No: Z22-40108		Page 4 of 6					

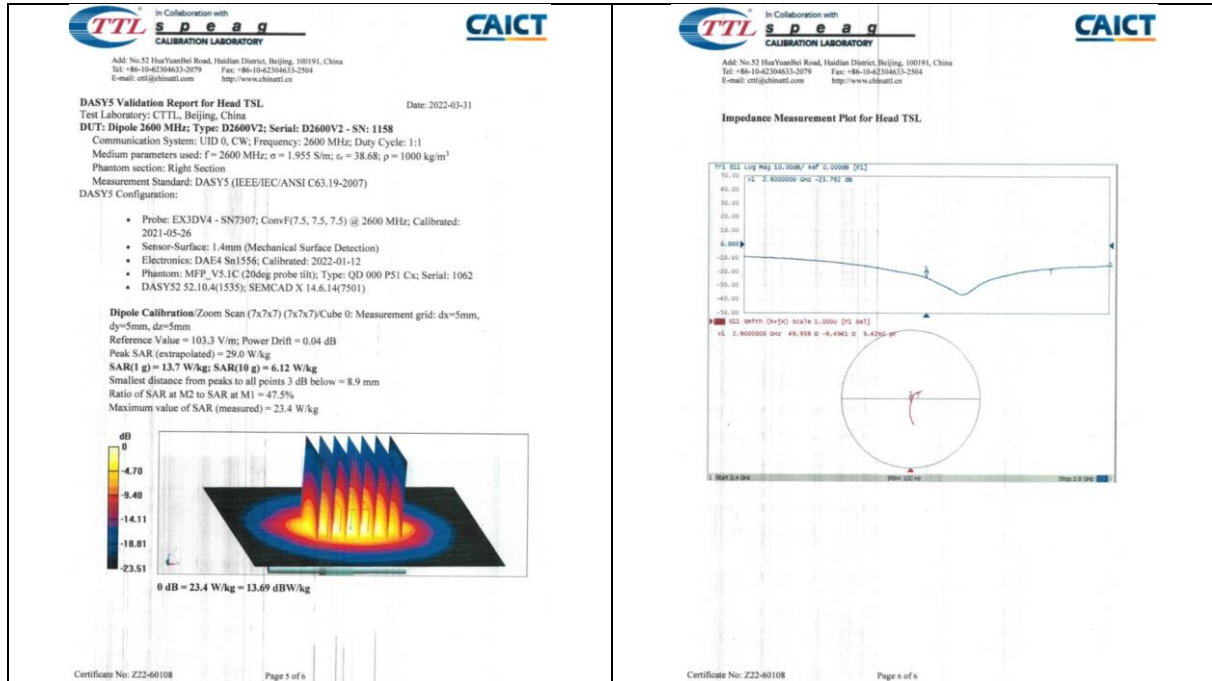

1.12 D5GHZV2 - SN 1095

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Client: SGS-CN Certificate No: Z22-60187

CALIBRATION CERTIFICATE

Object: D5GHZV2 - SN: 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464, Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyan SAR Project Leader

Issued: June 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Glossary:

TSL: Issue simulating liquid
sensitivity in TSL: / NORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.



The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 2 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 57355888 f(86-512) 57370818 www.sgs.com
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

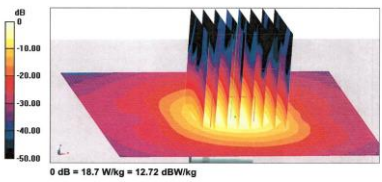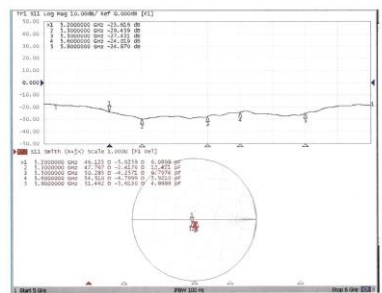In Collaboration with TTL s p e a q CALIBRATION LABORATORY CAICT Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cnlg@chinaetl.com http://www.caict.ac.cn General Antenna Parameters and Design <table border="1"><tr><td>Electrical Delay (one direction)</td><td>1.101 ns</td></tr></table> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data <table border="1"><tr><td>Manufactured by</td><td>SPEAG</td></tr></table> Certificate No: Z22-60187 Page 7 of 10	Electrical Delay (one direction)	1.101 ns	Manufactured by	SPEAG	In Collaboration with TTL s p e a q CALIBRATION LABORATORY CAICT Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cnlg@chinaetl.com http://www.caict.ac.cn DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-06-01 DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095 Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: $f = 5200 \text{ MHz}$; $\sigma = 4.62 \text{ S/m}$; $\epsilon = 35.39$; $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: $f = 5300 \text{ MHz}$; $\sigma = 4.73 \text{ S/m}$; $\epsilon = 35.19$; $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: $f = 5500 \text{ MHz}$; $\sigma = 4.939 \text{ S/m}$; $\epsilon = 34.83$; $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: $f = 5600 \text{ MHz}$; $\sigma = 5.051 \text{ S/m}$; $\epsilon = 34.69$; $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: $f = 5800 \text{ MHz}$; $\sigma = 5.247 \text{ S/m}$; $\epsilon = 34.42$; $\rho = 1000 \text{ kg/m}^3$ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA64 Sn1556; Calibrated: 2022-01-12 - Phantom: MPF_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 18.3 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg Certificate No: Z22-60187 Page 8 of 10
Electrical Delay (one direction)	1.101 ns				
Manufactured by	SPEAG				
In Collaboration with TTL s p e a q CALIBRATION LABORATORY CAICT Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cnlg@chinaetl.com http://www.caict.ac.cn Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.20 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.2 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg 0 dB = 16.7 W/kg = 12.72 dBW/kg  Certificate No: Z22-60187 Page 9 of 10	In Collaboration with TTL s p e a q CALIBRATION LABORATORY CAICT Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cnlg@chinaetl.com http://www.caict.ac.cn Impedance Measurement Plot for Head TSL  Certificate No: Z22-60187 Page 10 of 10				

2 DAE4 - SN 910

TTL Calibration Laboratory		CAICT	
In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn		中国计量科学研究院 CALIBRATION CNAS (L370)	
Client:	Auden	Certificate No:	Z22-60275
CALIBRATION CERTIFICATE			
Object	DAE4 - SN: 910		
Calibration Procedure(s)	FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAE)		
Calibration date:	July 14, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Process Calibrator 753	1971018	14-Jun-22 (CTTL, No.J22X04180)	Jun-23
Calibrated by:	Name	Function	Signature
	Yu Zongying	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued July 20, 2022 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60275		Page 1 of 3	

TTL Calibration Laboratory		CAICT	
In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn		中国计量科学研究院 CALIBRATION CNAS (L370)	
DC Voltage Measurement			
A/D Converter Resolution nominal High Range: 1LSB = 6.1μV, full range = -100...+300 mV Low Range: 1LSB = 61μV, full range = -1...+3mV DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec.			
Calibration Factors	X	Y	Z
High Range	403.347 ± 0.15% (k=2)	402.759 ± 0.15% (k=2)	403.242 ± 0.15% (k=2)
Low Range	3.98151 ± 0.7% (k=2)	3.94044 ± 0.7% (k=2)	3.94827 ± 0.7% (k=2)
Connector Angle			
Connector Angle to be used in DASY system		269° ± 1°	
Certificate No: Z22-60275		Page 2 of 3	

TTL Calibration Laboratory		CAICT	
In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn		中国计量科学研究院 CALIBRATION CNAS (L370)	
DC Voltage Measurement			
A/D Converter Resolution nominal High Range: 1LSB = 6.1μV, full range = -100...+300 mV Low Range: 1LSB = 61μV, full range = -1...+3mV DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec.			
Calibration Factors	X	Y	Z
High Range	403.347 ± 0.15% (k=2)	402.759 ± 0.15% (k=2)	403.242 ± 0.15% (k=2)
Low Range	3.98151 ± 0.7% (k=2)	3.94044 ± 0.7% (k=2)	3.94827 ± 0.7% (k=2)
Connector Angle			
Connector Angle to be used in DASY system		269° ± 1°	
Certificate No: Z22-60275		Page 3 of 3	




3 EX3DV4 - SN 7767

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst C Service suisse d'étalonnage S Swiss Calibration Service																																	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108																																	
Client: SGS-CN (Auden)	Certificate No: EX-7767_Oct22																																		
CALIBRATION CERTIFICATE																																			
Object: EX3DV4 - SN:7767																																			
Calibration procedures: QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v6, QA CAL-23.v5, QA CAL-25.v7 Calibration procedure for dosimetric E-field probes																																			
Calibration date: October 28, 2022																																			
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 1) °C and humidity < 70%. Calibration Equipment used (MATE critical for calibration)																																			
<table border="1"><thead><tr><th>Primary Standards</th><th>ID</th><th>Cal Date (Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power meter NRP</td><td>SN 102778</td><td>14-Apr-22 (No. 217-03558-05594)</td><td>Apr-23</td></tr><tr><td>Power sensor NRP-291</td><td>SN 102844</td><td>04-Apr-22 (No. 217-03558-05594)</td><td>Apr-23</td></tr><tr><td>DOF DAK-EX (imp/imp)</td><td>SN 1246</td><td>29-Oct-22 (DOF-DAK-EX-1246_Oct22)</td><td>Oct-23</td></tr><tr><td>DOF DAK-12</td><td>SN 1018</td><td>29-Oct-22 (DOF-DAK-12-1018_Oct22)</td><td>Oct-23</td></tr><tr><td>Reference 25 dB Attenuator</td><td>SN C22582 (20v)</td><td>04-Apr-22 (No. 217-03558-05594)</td><td>Apr-23</td></tr><tr><td>DAK4</td><td>SN 166</td><td>19-Oct-22 (No. 2464-480_Oct22)</td><td>Oct-23</td></tr><tr><td>Reference Probe E532V2</td><td>SN 3013</td><td>27-Dec-21 (No. E53-3013_Oct21)</td><td>Dec-22</td></tr></tbody></table>				Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN 102778	14-Apr-22 (No. 217-03558-05594)	Apr-23	Power sensor NRP-291	SN 102844	04-Apr-22 (No. 217-03558-05594)	Apr-23	DOF DAK-EX (imp/imp)	SN 1246	29-Oct-22 (DOF-DAK-EX-1246_Oct22)	Oct-23	DOF DAK-12	SN 1018	29-Oct-22 (DOF-DAK-12-1018_Oct22)	Oct-23	Reference 25 dB Attenuator	SN C22582 (20v)	04-Apr-22 (No. 217-03558-05594)	Apr-23	DAK4	SN 166	19-Oct-22 (No. 2464-480_Oct22)	Oct-23	Reference Probe E532V2	SN 3013	27-Dec-21 (No. E53-3013_Oct21)	Dec-22
Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration																																
Power meter NRP	SN 102778	14-Apr-22 (No. 217-03558-05594)	Apr-23																																
Power sensor NRP-291	SN 102844	04-Apr-22 (No. 217-03558-05594)	Apr-23																																
DOF DAK-EX (imp/imp)	SN 1246	29-Oct-22 (DOF-DAK-EX-1246_Oct22)	Oct-23																																
DOF DAK-12	SN 1018	29-Oct-22 (DOF-DAK-12-1018_Oct22)	Oct-23																																
Reference 25 dB Attenuator	SN C22582 (20v)	04-Apr-22 (No. 217-03558-05594)	Apr-23																																
DAK4	SN 166	19-Oct-22 (No. 2464-480_Oct22)	Oct-23																																
Reference Probe E532V2	SN 3013	27-Dec-21 (No. E53-3013_Oct21)	Dec-22																																
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID</th><th>Check Date (in house)</th><th>Scheduled Check</th></tr></thead><tbody><tr><td>Power meter E4418B</td><td>SN 0841938814</td><td>05-Apr-19 (in house check Jun-20)</td><td>In house check Jun-24</td></tr><tr><td>Power sensor E4418A</td><td>SN 14141486087</td><td>05-Apr-19 (in house check Jun-20)</td><td>In house check Jun-24</td></tr><tr><td>Power sensor E4415A</td><td>SN 100712510</td><td>05-Apr-19 (in house check Jun-20)</td><td>In house check Jun-24</td></tr><tr><td>RF generator HP 8448C</td><td>SN 106842001793</td><td>01-Apr-99 (in house check Jun-20)</td><td>In house check Jun-24</td></tr><tr><td>Network Analyzer E6396A</td><td>SN 1084108477</td><td>31-Mar-14 (in house check Oct-22)</td><td>In house check Oct-24</td></tr></tbody></table>				Secondary Standards	ID	Check Date (in house)	Scheduled Check	Power meter E4418B	SN 0841938814	05-Apr-19 (in house check Jun-20)	In house check Jun-24	Power sensor E4418A	SN 14141486087	05-Apr-19 (in house check Jun-20)	In house check Jun-24	Power sensor E4415A	SN 100712510	05-Apr-19 (in house check Jun-20)	In house check Jun-24	RF generator HP 8448C	SN 106842001793	01-Apr-99 (in house check Jun-20)	In house check Jun-24	Network Analyzer E6396A	SN 1084108477	31-Mar-14 (in house check Oct-22)	In house check Oct-24								
Secondary Standards	ID	Check Date (in house)	Scheduled Check																																
Power meter E4418B	SN 0841938814	05-Apr-19 (in house check Jun-20)	In house check Jun-24																																
Power sensor E4418A	SN 14141486087	05-Apr-19 (in house check Jun-20)	In house check Jun-24																																
Power sensor E4415A	SN 100712510	05-Apr-19 (in house check Jun-20)	In house check Jun-24																																
RF generator HP 8448C	SN 106842001793	01-Apr-99 (in house check Jun-20)	In house check Jun-24																																
Network Analyzer E6396A	SN 1084108477	31-Mar-14 (in house check Oct-22)	In house check Oct-24																																
Calibrated by: Name: Adonia Georgiadou Function: Laboratory Technician Signature: [Signature]																																			
Approved by: Even Kijhn Technical Manager Signature: [Signature]																																			
The calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																			
Certificate No: EX-7767_Oct22 Page 1 of 9																																			

EX3DV4 - SN:7767		October 28, 2022	
Parameters of Probe: EX3DV4 - SN:7767			
Basic Calibration Parameters			
	Sensor X	Sensor Y	Sensor Z
North (µV/(V/m)) ^A	0.87	5.89	0.56
DCP (mV) ^B	103.4	107.3	105.7
Unc (k = 2)			
			+10.1%
			+4.7%
Calibration Results for Modulation Responses			
USB ^C Communication System Name	A	B	C
	dB	dB	dB
0 CW	X 0.00	0.00	1.00
	Y 0.00	0.00	1.00
	Z 0.00	0.00	1.00
			186.7
			179.5
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. ^A The uncertainties of Item X1.2 do not affect the E-field uncertainty inside TSL (see Page 3). ^B Uncertainty for probe sensitivity for maximum specified field strength. ^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.			
Certificate No: EX-7767_Oct22 Page 3 of 9			

EX3DV4 - SN:7767		October 28, 2022	
Parameters of Probe: EX3DV4 - SN:7767			
Other Probe Parameters			
Sensor Arrangement			
Connector Angle	144.8°		
Mechanical Surface Detection Mode	enabled		
Optical Surface Detection Mode	disabled		
Probe Overall Length	337 mm		
Probe Body Diameter	10 mm		
Tip Diameter	8 mm		
Tip Length	2.5 mm		
Probe Tip to Sensor X Calibration Point	1 mm		
Probe Tip to Sensor Y Calibration Point	1 mm		
Probe Tip to Sensor Z Calibration Point	1 mm		
Recommended Measurement Distance from Surface	1.4 mm		
Note: Measurement distance from surface can be increased to 3-4 mm for all Area Scan Scans.			
Certificate No: EX-7767_Oct22 Page 4 of 9			



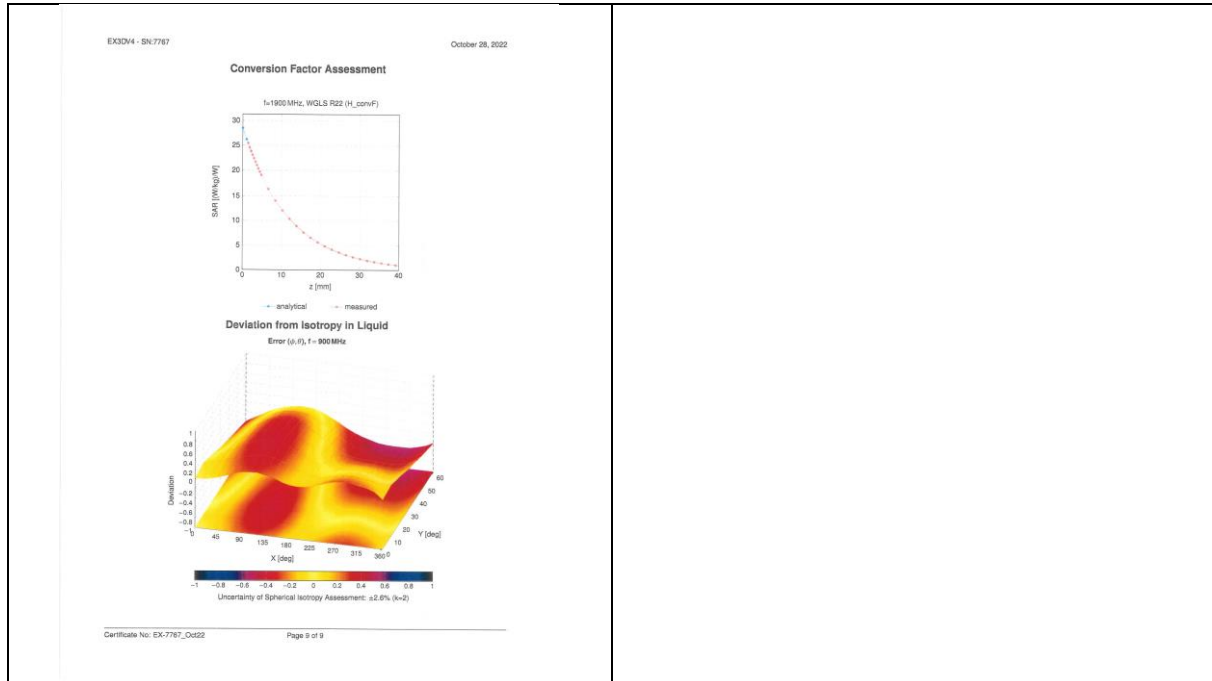

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgsgroup.com.cn
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2021/4/26	-31.4	/	47.8	/
2022/4/26	-32.5	-3.5%	47.1	0.7
2023/4/26	-32.3	-2.87%	46.5	1.3
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2021/4/21	-23	/	57.1	/
2022/4/26	-23.4	-1.74%	56.6	0.5
2023/4/26	-23.9	-3.91%	56.2	0.9
Dipole D750V3 SN 1188				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/29	-28.7	/	53.6	/
2023/3/29	-28.3	1.39%	53.2	0.4
Dipole D835V2 SN 4d114				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-25.3	/	48.7	/
2023/3/31	-24.6	2.77%	49.1	0.4
Dipole D900V2 SN 1d079				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/7	-23.3	/	48.1	/
2023/6/7	-23.6	-1.29%	48.3	0.2
Dipole D1800V2 SN 2d170				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-29.4	/	47.9	/
2023/3/31	-28.9	1.70%	47.2	0.7
Dipole D1900V2 SN 5d136				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/7	-22.4	/	51.2	/
Dipole D2000V2 SN 1041				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/6	-34.9	/	48.4	/
Dipole D2300V2 SN 1096				
Head Liquid				



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgs.com.cn
中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com

Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-26.6	/	49.2	/
2023/3/31	-27.1	-1.88%	49.4	0.2
Dipole D2450V2 SN 817				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/4/1	-28.5	/	52.1	/
2023/4/1	-28.0	1.75%	51.6	0.5
Dipole D2600V2 SN 1158				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-23.8	/	49.9	/
2023/3/31	-23.3	2.10%	50.3	0.4
Dipole D5GHzV2 SN 1095 for 5200				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-23.6	/	46.1	/
Dipole D5GHzV2 SN 1095 for 5300				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-29.5	/	47.8	/
Dipole D5GHzV2 SN 1095 for 5500				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-27.4	/	50.3	/
Dipole D5GHzV2 SN 1095 for 5600				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-24.0	/	54.5	/
Dipole D5GHzV2 SN 1095 for 5800				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-24.9	/	51.5	/



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10 Weiye Road, Development Zone, Kunshan, Jiangsu, China 215300 t(86-512) 5735 5888 f(86-512) 57370818 www.sgs.com.cn
 中国·江苏·昆山开发区伟业路10号 邮编: 215300 t(86-512) 57355888 f(86-512) 57370818 sgs.china@sgs.com