

**INFINIUM**

**TM1 Patient Monitor**  
**User's Manual**

**V1.0**

**Infinium Medical Inc.**

## Introduction

Thank you for choosing TM1 patient monitor

Before using the product, please read this manual carefully for proper use.

After reading, please properly keep this manual for reference at any time when needed.

**Product Name:** Patient Monitor

**Model Name:** TM1

### General Information:

This monitor can monitor the patient's ECG, Resp, Temp, SpO2, PR, NIBP, and IBP is used for monitoring, and the monitored information can be displayed, stored, and reviewed.

### Product Components:

This product consists of a host, a fixed base, a battery, a power adapter, and accessories (ECG lead wire, disposable electrode, blood oxygen probe, temperature probe, blood pressure sleeve and its extension tube, invasive pressure cable).

### Indications for Use:

The monitor is intended to monitor patients in medical institutions. It can also be used for transportation within and outside the hospital. This product must be used by clinical medical personnel who have undergone professional training.

**INFINIUM**

Infinium Medical Inc.

Website: [www.infiniummedical.com](http://www.infiniummedical.com)

Address: 12151 62nd St North #5 Largo Fl, 33773 USA

Toll Free (US call only): 866-918-8434

International: 1-727-531-8434

Fax: 1-727-531-8436

## Statement

Infinium hereby DISCLAIMS all warranties and conditions, either express, implied or statutory, including, but not limited to, any implied warranties or conditions of merchantability, of fitness for a particular purpose with regard to the materials.

Infinium shall not be liable for errors contained herein nor for incidental or consequential damages in connection with the furnishing, performance, or use of this manual. This manual may refer to information protected by copyrights or patents.

Release, amendment, reproduction, distribution, rental, adaption and translation of this manual in any manner whatsoever without the written permission of Infinium is strictly forbidden.

Contents of this manual are subject to changes without prior NOTE.

## 【Manufacturer Responsibility】

**Infinium** is responsible for the effects on safety, reliability and performance of this product, only if:

- All installation operations, expansions, changes, modifications and repairs of this product are conducted by Infinium authorized personnel;
- The electrical installation of the relevant room complies with the applicable national and local requirements;
- The product is used in accordance with the instructions for use.

## 【Note】

The equipment can't be used at home.



## WARNING

---

---

- This patient monitor is intended for use only by clinical professionals or at least under their guidance. It must only be used by trained personnel in its use. Anyone unauthorized or untrained must not perform any operation on it.

---

---

## Preface

### 【Manual Description】

This manual describes the uses, features, operations and safety messages of the patient monitor. Before using this equipment, observance of the manual is a prerequisite for proper performance and correct operation and ensures patient and user safety.

Keep this manual in the vicinity of the equipment so that it can be obtained conveniently when needed.

### 【Intended Audience of this Manual】

This manual is intended for clinical professionals. Clinical professionals are expected to have a working knowledge of medical procedures, practices and terminology, as required for the monitoring of all patients.

### 【Illustrations】

This manual uses illustrations for examples only. Illustrations in this manual may not necessarily reflect all system settings, features, configurations or data display.

### 【Convention】

*Italic*: used to indicate the cited chapter.

[Character]: Used to represent strings in software.

→: This symbol is used to represent the steps during the operation.

---

## Content

1 Safety .....	1
2 Monitor Description .....	6
3 Basic Operations .....	17
4 Setup .....	24
5 Display Mode .....	30
6 Alarm .....	33
7 ECG .....	41
8 Resp .....	58
9 SpO2 .....	63
10 Temp .....	70
11 NIBP .....	74
12 IBP .....	84
13 Managing Patients .....	91
14 Trends .....	94
15 Patient History Data .....	98
16 Freezing Waveforms .....	100
17 Internal Batteries .....	101
18 Care, Cleaning .....	105
19 Maintenance .....	107
20 Accessories .....	111
A Specifications .....	115
B Factory Defaults .....	129
C Alarm Messages .....	134
D EMC and Radio Regulatory Compliance .....	137

## 1 Safety

### 1.1 Safety Information



#### WARNING

- Indicates a potential hazard or unsafe practice that, if not avoided, could result in death or serious injury.



#### CAUTION

- Indicates a potential hazard or unsafe practice that, if not avoided, could result in minor personal injury or product/property damage.



#### NOTE

- Provides application tips or other useful information to ensure that you get the most from your product.

#### 1.1.1 Warning



#### WARNING

- — SINGLE PATIENT USE — This equipment is designed for use on one patient at a time.
- To avoid explosion hazard, do not use the equipment in the presence of flammable anesthetics, vapors or liquids.
- Do not use monitoring sensors during magnetic resonance imaging (MRI). Induced current could potentially cause burns. The sensor may affect the MRI image, and the MRI unit may affect the accuracy of the oximetry measurements.
- Before connecting the equipment to the power line, check that the voltage and frequency ratings of the power line are the same as those indicated on the equipment's label or in this manual.
- Before putting the system into operation, the operator must verify that the equipment, connecting cables and accessories are in correct working order and operating condition.
- Do not touch electrical equipment and the patient at the same time. This may cause an unsafe

electrical shock to the patient.

- Do not come into contact with patients during defibrillation. Otherwise, serious injury or death could occur.
- Do not use the equipment in the presence of flammable anesthetics, vapors or liquids.
- The waveforms, physiological data and alarm messages displayed on the equipment are for reference only and cannot be directly used for diagnostic interpretation.
- Wrap and secure excess cabling to reduce risk of entanglement or strangulation by patients or personnel.
- Batteries must be taken out when the equipment is not used.
- Do not disassemble the equipment on your own, otherwise electrical shock may occur. Maintenance should be carried out by manufacturer or authorized service personnel.
- The software copyright of the equipment is solely owned by the manufacturer. No organization or individual shall resort to juggling, copying, or exchanging it or to any other infringement on it in any form or by any means without due permission.

---

### 1.1.2 Caution

---

#### CAUTION

---

- To ensure patient safety, use only parts and accessories specified in this manual.
- Magnetic and electrical fields are capable of interfering with the proper performance of this equipment; Thus, this monitor shouldn't be operated with other High frequency equipment (especially high RF equipment) in the same site. High RF equipment shouldn't stay too close to this monitor, otherwise the normal function of this monitor might be affected.
- Do not lift the monitor by pulling on the sensor cable or power cord, as these cables may be disconnected from the monitor and the equipment may fall and injure the patient.
- Patient monitors are precision medical instruments. Always install or carry the equipment properly to avoid damage caused by drop, impact, strong vibration or other mechanical force. Do not pull, twist, or rub the lead wires.
- Please keep the lead wires and patient monitor dry to avoid the inaccurate measurement result, product damage or any potential risks that might harm the patient. Dry the equipment immediately when it gets wet.
- Some configurations are protected by passwords. If you need to use password to access these functions, please contact associated personnel.

---

- An indicated potential hazard or unsafe practice that, if not avoided, could result in minor personal injury, product malfunction, damage or property loss.
- Both the monitor and the devices that connected to this equipment, must be grounded together.
- Devices connected to the equipment must meet the requirements of the applicable IEC standards (e.g., IEC 60950 safety standards for information technology equipment and IEC 60601-1 safety standards for medical electrical equipment). The system configuration and all lead wires must meet the requirements of the IEC 60601-1 medical electrical systems standard.
- Any personnel who connect devices to the equipment's signal input/output port is responsible for providing evidence that the safety certification of the devices has been performed in accordance to the IEC 60601-1. If you have any question, please contact the manufacturer.
- Environment and patient condition must be considered to ensure the precision of measurement. For special safety instructions on these conditions, see chapters of this manual for reference accordingly.
- Chemical leakage from broken LCD is poisonous and adverse health consequences might occur once the leaking liquid enters human body. Please do take care when carrying patient monitors with broken LCD screens.
- Package material may contaminate the environment. Properly dispose of the package material according to applicable waste control regulations and keep it out of children's reach.
- At the end of its service life, the equipment, as well as its accessories, must be disposed of in compliance with the guidelines regulating the disposal of such products to avoid contaminating the environment.

---

### 1.1.3 Notes



---

- Put the equipment in a location where you can easily view, operate and maintain it.
- For proper operation, the operator shall stand in front of the equipment.
- Keep this manual in the vicinity of the equipment so that it can be obtained conveniently when needed.

---

## 1.2 Electromagnetic Interference

Due to the dramatic increase in the number of radio frequency transmitters or other sources of

## User's Manual for TM1 Patient Monitor

electronic interference (such as electronic surgical equipment, cell phones, two-way radar for vehicles, electronic devices, etc.) in medical care settings. The high level of interference caused by the immediate vicinity, or strong transmitter power of the interfering sources may interrupt the normal function of this equipment.


This monitor is designed for use within a specified electromagnetic environment. However, Certain electromagnetic interference may cause blurred or erroneous measurements, even worse, the malfunction of the equipment.

Interference may manifest itself in erratic readings, interruptions in operation or other functional errors. If this occurs, the working environment should be investigated to identify the source of the interference and eliminate it.

- Turn on and off the appliances in the vicinity to find out the interfering appliance.
- Redirect or relocate other receiving devices.
- Keep away from the interfering devices.

This patient monitor may generate or emit the energy of radio frequency, if not used properly according to the manual, it might cause harmful interference with other devices in the vicinity.

### 1.3 Equipment Symbols

Symbols	Explanation
	NOTE! Consult documents accompanying this monitor.
	Power ON/OFF (for a part of the equipment)
	Type CF applied part. Defibrillator-proof protection against electric shock.
	Type BF applied part. Defibrillator-proof protection against electric shock.
	Type BF applied part.
	Rechargeable battery
	Fuse replacement requirements
	Equipotential grounding

User's Manual for TM1 Patient Monitor

	Computer network
	Alternating current (AC)
	Battery indicator
	AC/DC dual-use
	Direct current (DC)
<b>SN</b>	Serial number
	Date of manufacture
	Manufacturer
	Fragile, handle with care
	This way up.
	Keep dry. Protect from rain.
	Stacking limit by number: Maximum number is 8 for the symbol in the illustration.
	Rotatable angle identification
	USB interface
<b>IPX1</b>	Waterproof grade identification
	Non ionizing radiation

## 2 Monitor Description

### 2.1 Intended Use

This device is intended to be used for monitoring, and recording of, and to generate alarms for, multiple physiological parameters of adults, pediatrics, and neonates. Critical physiological parameters include ECG(Electrocardiogram), Heart Rate (HR), Pulse Oxygen Saturation (SpO2), Pulse Rate (PR), Non-invasive Blood Pressure (NIBP), Respiration Rate (RR), Temperature (Temp), and Invasive Blood Pressure (IBP), the measurement can be displayed, stored and reviewed.

This monitor is intended for use in medical institutions, widely used in clinical departments such as internal medicine, surgery, operating rooms, ICU/CCU, emergency rooms, and obstetrics and gynecology. It can monitor important vital parameters of patients on a regular, continuous, and long-term basis, and has significant clinical value in ensuring patient safety. This device can also be used for transportation within and outside the hospital.



### WARNING

- This patient monitor is intended for use only by clinical professionals or under their guidance. It must only be used by persons who have received adequate training in its use. Operation by patient is not prohibited.

---

---

### 2.2 Operating Principle

The monitor operates based on the principle that various physiological changes are probed through sensor, amplified through signal booster, and ultimately turned into electrical information for analysis. The monitor software will calculate, analyze and edit the data, and display it in parameter area. You can also record and print it out as needed. When the measured data exceeds the alarm limit, it will trigger the alarm for action.

The software contains 4 parts: signal acquisition, analog processing, digital processing, information output.

### 2.3 Contraindications

Non invasive blood pressure (NIBP) cannot be measured on patients with sickle cell disease.

### 2.4 Components

The product consists of a host, portable handle frame, expansion base, battery, power adapter, and accessories (ECG cable, SpO2 sensor, NIBP cuff, IBP cables, C.O. cables, Temp sensor etc.).

## 2.5 Main Unit

### 2.5.1 Front View

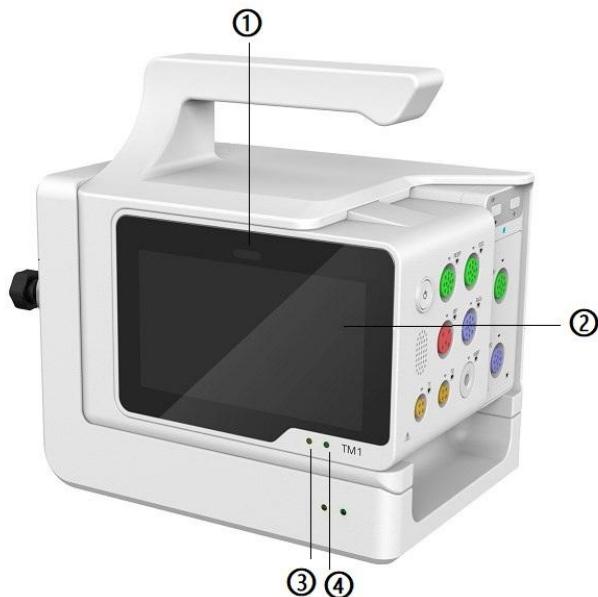


Figure 2-1 Front View

Number	Explanation	Symbol
1	<p><b>Alarm Indicator Lights:</b></p> <p>Indicate the level of technical and physiological alarms with different colors and flashing frequencies;</p> <p>High Level Alarm: Red, fast flashing frequency, 2 times on/off per second</p> <p>Medium Level Alarm: yellow, slow flashing frequency, 1 on/off per second</p> <p>Low Level Alarm: blue, constantly on without flashing</p>	
2	<b>Display Screen</b>	
3	<p><b>Battery Indicator:</b></p> <p><b>ON:</b> when the battery is being charged or already fully charged.</p> <p><b>Flash:</b> when the patient monitor operates on battery power.</p> <p><b>OFF:</b> when no battery is installed or no AC source is connected.</p>	
3	<p><b>AC Power Indicator:</b></p> <p><b>ON:</b> when AC power is connected.</p> <p><b>OFF:</b> when AC power is connected.</p>	

### 2.5.2 Rear View

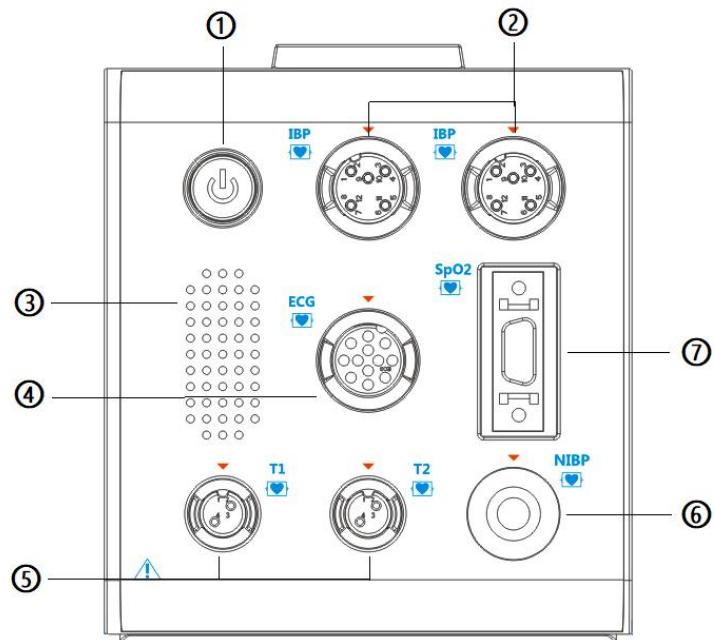


Figure 2-2 Rear View

Number	Explanation	Symbol
1	Power on/off Button: turn on/off the monitor	
2	IBP sensor interface	IBP
3	Speaker	
4	ECG cable interface	ECG
5	Temperature probe interface	T1/T2
6	NIBP Cuff interface	NIBP
7	SpO2 sensor interface	SpO2

### 2.6 Portable Handle

The portable handle is used to load the TM1 monitor.

### 2.6.1 Left View

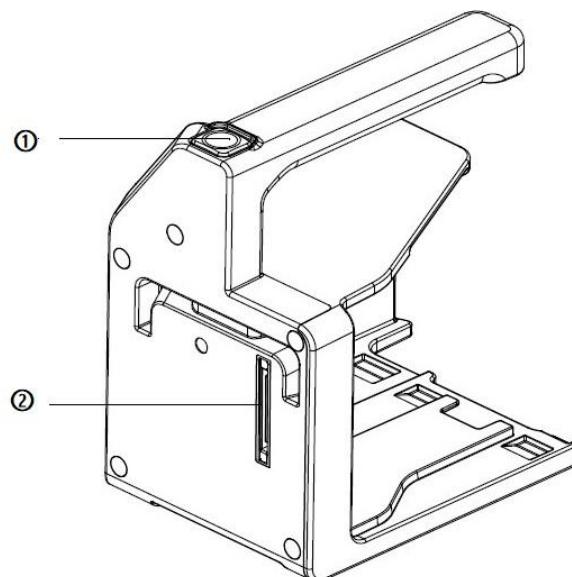


Figure 2-3 Left view of portable handle

Number	Explanation	Symbol
1	Unlock button: Press this button to unlock the portable handle frame and expansion base	
2	Multi pin connector: the interface for connecting the expansion base	

### 2.6.2 Right View

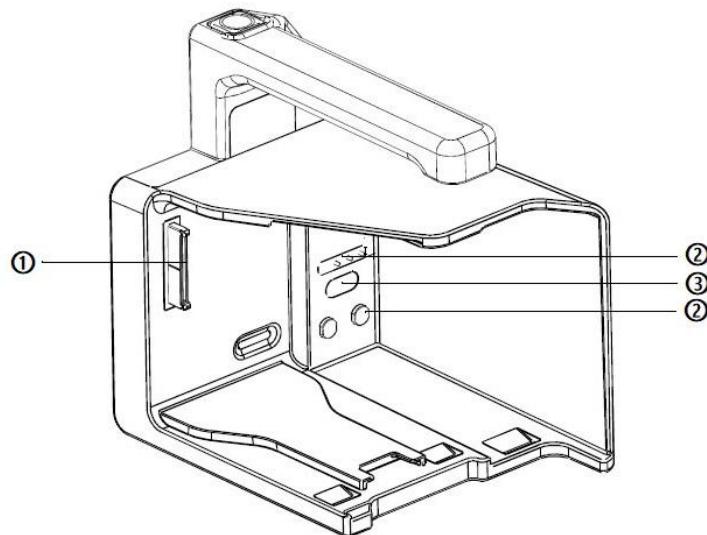


Figure 2-4 Right view of portable handle

Number	Explanation	Symbol
1	<b>Multi pin plug interface:</b> the interface for connecting the monitor	

2	<b>Contact:</b> Power supply and communication interface of external parameter measurement module	
3	Infrared communication interface	

## 2.7 Docking Station

The docking station is used to load a portable handle.

### 2.7.1 Left View

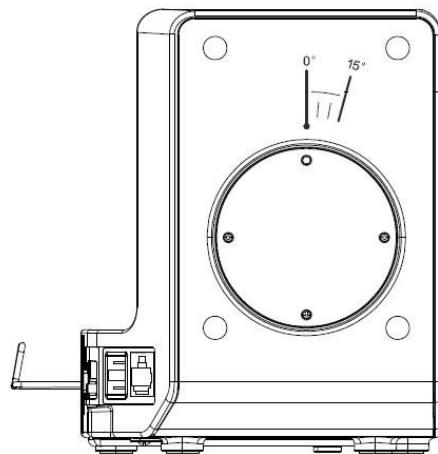


Figure 2-5 Left view of docking station

### 2.7.2 Right View

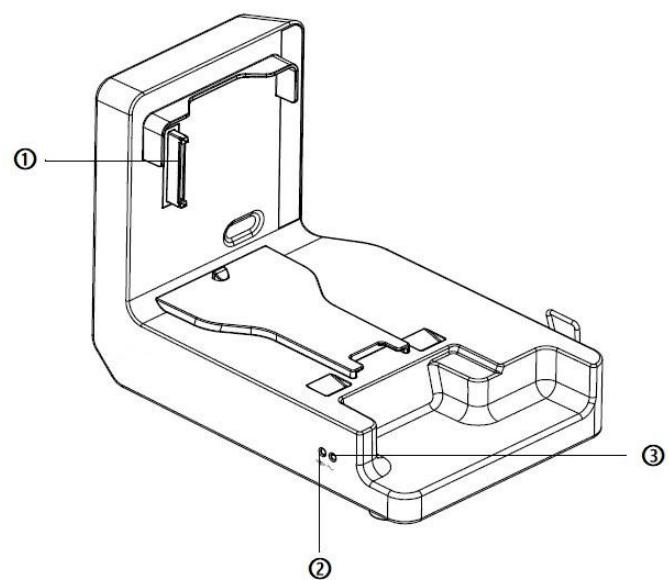


Figure 2-6 Right view of docking station

Number	Explanation	Symbol
1	<b>Multi pin interface:</b> enables power supply and data communication to the monitor when connecting to a portable handle frame	
2	<b>Connection status indicator light:</b> lights up when connected to the monitor normally	
3	<b>External power indicator light:</b> lights up when the external power is turned on	

### 2.7.3 Rear View

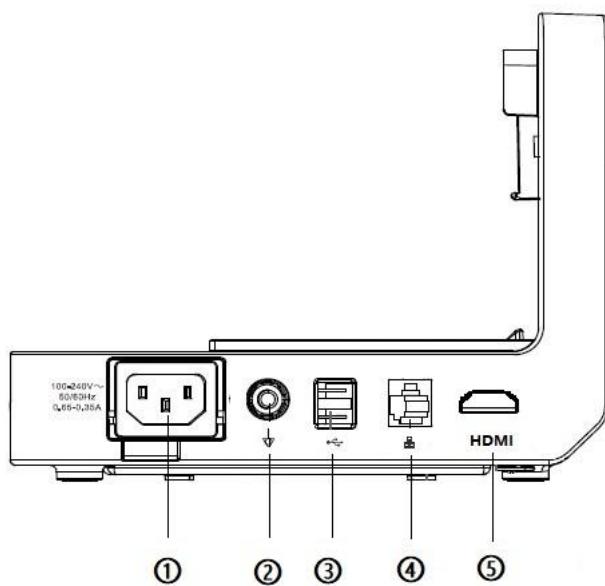


Figure 2-7 Right view of docking station

Number	Explanation	Symbol
1	<b>AC Power Input:</b> 100~240V AC 50/60Hz	100-240V 50/60Hz 1.3-0.5A
2	<b>Equipotential Grounding:</b> connecting other instruments and equipment with equipotential grounding system to eliminate the ground potential difference between different equipment to ensure safety	

3	USB Interface	USB
4	RJ45 Network Interface	
5	HDMI Extended Display Interface	HDMI

## 2.8 Display Screen

This patient monitor uses a high-resolution 5.7 inches LCD to display patient parameters and waveforms. A typical display screen is shown below.

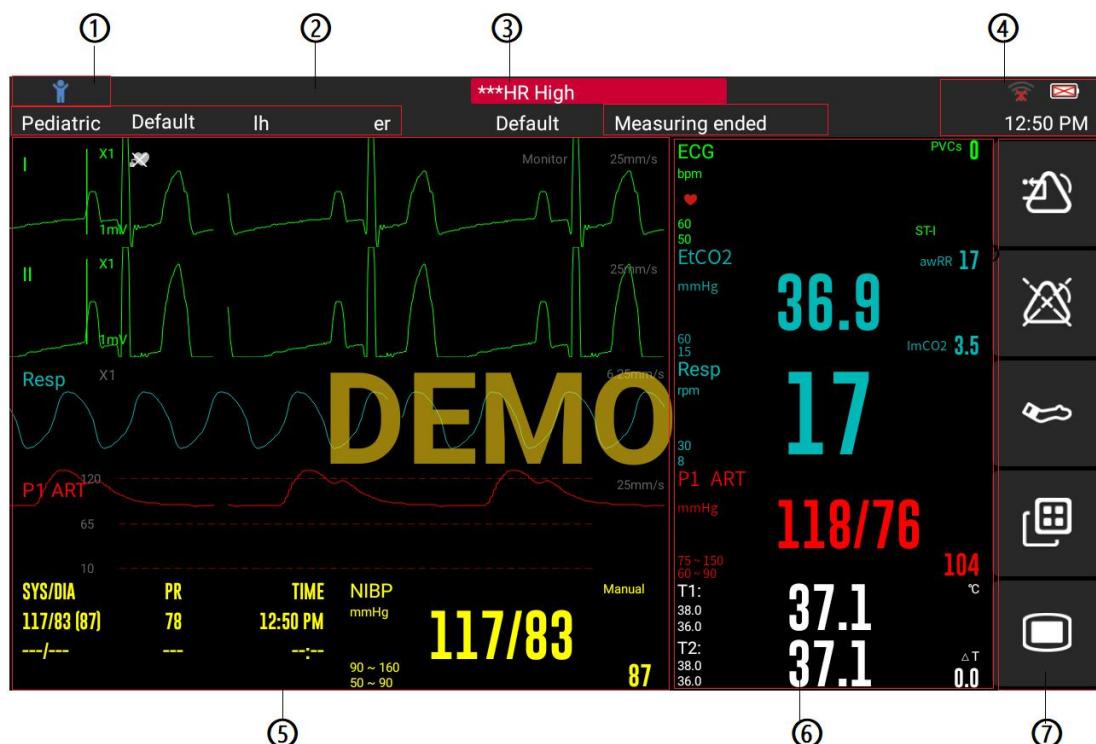


Figure 2-8 Normal Monitor View

Number	Explanation
1	<b>Patient Information Area</b> This area shows the patient information such as patient category, name, gender, ID.
2	<b>Technical Alarm Area</b> This area shows technical alarm messages and prompt messages. When multiple messages come, they will be displayed circularly. Select this area and the technical alarm list will be displayed.
3	<b>Physiological Alarm Area</b>

	This area shows physiological alarm messages. When multiple alarms occur, they will be displayed circularly. Select this area and the physiological alarm list will be displayed.
4	<b>System Status Bar:</b> Indicating time, network and battery status.
5	<b>Waveform Area:</b> This area shows measurement waveforms. The waveform name is displayed at the left upper corner of the waveform. The waveform position on display can be adjusted. Select this area and the corresponding measurement setup menu will be displayed.
6	<b>Parameter Area:</b> Displaying the real-time measurement value corresponding to each parameter module. Its waveform is displayed in the same row in the waveform area.
7	<b>Hot Keys Area:</b> The hotkey area has commonly used function hotkeys, including the Main Menu, Layout Management, NIBP Start/Stop, Alarm Pause, Alarm Reset, Trend Review, History Review, Configuration Management, Alarm Settings, and Standby.

### 2.8.1 Symbols

Symbols	Explanation	Symbols	Explanation
	Adult Patient, male		Adult Patient, female
	Pediatric Patient, male		Pediatric Patient, female
	Neonatal Patient, male		Neonatal Patient, female
	Patient monitor has no network connection		Patient monitor is connected to a wire network successfully.
	Wireless connection is working, the white bar indicates the network signal strength		
	Alarms are turned off.		Alarms are paused.
	Alarm audio is turned off.		Alarms audio is paused.
	Alarm reset		No battery is installed
	Battery failure		Full battery

	Batteries work correctly. The solid portion represents the current charge level of the batteries in proportion to its maximum charge level.		Low battery, needs to be charged
---	---	---	----------------------------------

## 2.8.2 Soft Keys

Soft Keys column is on the right of the screen, As shown in Figure 2-9

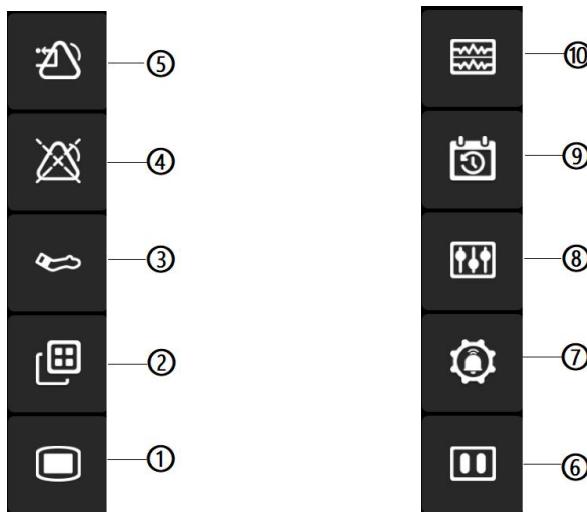


Figure 2-9 hot keys

- 1) **Main Menu:** Configure the system parameter.
- 2) **View Layout:** Set up the waveform in main display and parameter display layout.
- 3) **Start/Stop:** Start/Stop measuring the non-invasive blood pressure.
- 4) **Alarm Pause:** Pause the alarm system, and resume the alarm after time limit.
- 5) **Alarm Reset:** Reset the alarm system.
- 6) **Standby:** Pause current monitoring.
- 7) **Alarm Setup:** Set up alarm related settings, including general alarm settings and parameter alarm settings for each parameter module.
- 8) **Config Manager:** Manage configuration, including loading, deleting, saving, importing, exporting, etc.
- 9) **History Review:** Manage historical patients, including deleting, locking, unlocking, and opening trends for selected patients.
- 10) **Trend Review:** Enter the trend review page.

### 2.8.3 System Status Bar




Figure 2-10 System status display area

The system status bar is located in the upper right corner of the monitor, as shown in Figure 2-10.

- 1) Network status: display current network status (No connection, wired connection and wireless connection) and network signal strength.
- 2) Battery status: battery not in place, battery charging, battery failure, battery in place.
- 3) Battery level: display current battery level.
- 4) Current time: shown time format of either 24h or 12h.

### 2.8.4 Soft Keys Lists

Soft Keys Symbol	Soft Keys Name	Explanation	Soft Keys Symbol	Soft Keys Name	Explanation
	Setting	Enter setting menu		View Layout	Enter layout menu
	NIBP ON/OFF	Start/Stop NIBP		Alarm Paused	Pause current alarm
	Alarm Off	Turn off the alarm		Alarm Audio Paused	Pause the alarm sound
	Alarm Audio Off	Turn off the alarm audio		Alarm Reset	Reset the alarm system
	Display Paused	Pause current display		Alarm setting	Open alarm setting menu
	Config Manager	Open configuration management menu		History Review	Enter History Review window.

User's Manual for TM1 Patient Monitor

	Trend Review	Open trend review window for current patient.			
---	--------------	---	--	--	--

## 3 Basic Operations

### 3.1 Description

The following section describes the basic operations of the monitor before it is used.

### 3.2 Safety Precautions

#### **WARNING**

- Please use the installation accessories authorized by us.
- The software copyright of the equipment is solely owned by us. No organization or individual shall resort to juggling, copying, or exchanging it or to any other infringement on it in any form or by any means without due permission.
- Devices connected to the equipment must meet the requirements of the applicable IEC standards (e.g., IEC 60950 safety standards for information technology equipment and IEC 60601-1 safety standards for medical electrical equipment). The system configuration must meet the requirements of the IEC 60601-1-1 medical electrical systems standard. Any personnel who connect devices to the equipment's signal input/output port is responsible for providing evidence that the safety certification of the devices has been performed in accordance to the IEC 60601-1-1. If you have any question, please contact us.
- If it is not evident from the equipment specifications whether a particular combination with other devices is hazardous, for example, due to summation of leakage currents, please consult the manufacturers or else an expert in the field, to ensure the necessary safety of patients and all devices concerned will not be impaired by the proposed combination.
- **ACCURACY** - If the accuracy of any value displayed on the monitor, central station, or printed on a graph strip is questionable, determine the patient's vital signs by alternative means. Verify that all equipment is working correctly.
- **The operator should check whether the current alarm preset is applicable to the current patient before use.**

#### **CAUTION**

- Please keep the packaging material out of children's reach. When disposing of it, be sure to observe the applicable waste control regulations.
- The equipment might be contaminated during storage and transport. Before use, please verify

whether the packages are intact, especially the packages of single-use accessories. In case of any damage, do not apply it to patients.

- Make sure that the operating environment of the equipment meets the specific requirements. Otherwise, unexpected consequences, e.g., damage to the equipment, could result.
- Please read this manual thoroughly to ensure the proper use of the product and safety of both patient and operator.

---

 **NOTE**

---

- Put the equipment in a location where you can easily view, operate and maintain it.
- Keep this manual in the vicinity of the equipment so that it can be obtained conveniently when needed.
- Save the packing case and packaging material as they can be used if the equipment must be reshipped.

---

### **3.3 Installation**

#### **3.3.1 Unpacking and Checking**

Before unpacking, examine the packing case carefully for signs of damage. If any damage is detected, contact the carrier or the manufacturer. If the packing case is intact, open the package and remove the equipment and accessories carefully. Check all materials against the packing list and check for any mechanical damage. If you have any question, please contact us.

#### **3.3.2 Environmental Requirements**

The operating environment of the equipment must meet the requirements specified in this manual.

The environment where the equipment is used shall be reasonably free from noises, vibration, dust, corrosive, flammable and explosive substances. If the equipment is installed in a cabinet, sufficient space in front and behind shall be left for convenient operation, maintenance and repair. Moreover, to maintain good ventilation, the equipment shall be at least 2 inches (5 cm) away from around the cabinet.

When the equipment is moved from one place to another, condensation may occur as a result of temperature or humidity difference. In this case, never start the system before the condensation disappears.

## 3.4 Getting Started

Before using this monitor, please carefully read this manual and familiarize yourself with the performance, operating methods, and precautions of the instrument.

### 3.4.1 Connecting the power supply

When this monitor is connected to an AC adapter or expansion base, it can be powered by an AC power source. Before connecting to the AC power supply, please confirm that the voltage and frequency of the AC power supply are the same as the voltage and frequency indicated next to the AC adapter or expansion base power plug.

#### 3.4.1.1 Connect to AC Power Source using an AC adapter

1. Connect TM1 to one end of the AC adapter.
2. Connect the other end of the AC adapter to one end of the power cord.
3. Insert the other end of the power cord into an AC power outlet.
4. Check if the external power indicator light of TM1 is on and ensure that the power connection is normal.

The external power indicator light is located in the lower right corner of the display screen. When AC power is not connected, the indicator light does not light up; After connecting the AC power, the green indicator light will light up.

#### 3.4.1.2 Connect AC power supply using expansion dock

1. Connect TM1 to the expansion base.
2. Connect one end of the power cord to the AC power interface on the expansion base.
3. Insert the other end of the power cord into an AC power outlet.
4. Check if the AC power indicator light on the expansion base and the external power indicator light on TM1 are lit to ensure that the power connection is normal.



### WARNING

---

- Use the power cord provided in the product package for power connection.
- The adapter specified by our company must be used.
- Before connecting to the AC power supply, confirm that the voltage and frequency of the AC power supply are consistent with the specifications stated on the device label or manual.
- When using TM1 with the expansion base, please use AC power supply.
- When there are doubts about the integrity of the installation or wiring of external protective

wires, batteries should be used for power supply, otherwise it may cause injury to patients and operators due to electric shock.

---

---

### 3.5 Turning Power On

Before you turn on the monitor, please get ready for monitoring:

1. Check the patient monitor, and plug-in modules for any mechanical damage and make sure that cables, modules and accessories are properly connected.
2. Plug the power cord into the AC power source. If you run the patient monitor on battery power, ensure that the battery is sufficiently charged.

Press the Power **ON/OFF** button for 3s to turn on the equipment. The alarm light and the key backlight will illuminate, the welcoming screen will appear with a page indicating “**Loading System ...**” message, after 1-2min, the initialization of monitoring will begin after the with the **monitoring LOGO** on screen. Around 20s later, the initialization will be completed and the monitor enters the main screen. Now we could start monitoring.

### 3.6 Operation and Browse

All the elements required to operate the monitor are included on its screen, and almost every element on the screen is interactive. These screen elements include parameter measurement values, waveforms, hotkeys, information areas, alarm areas, and menus. Usually, you can access the same feature in different ways. For example, you can enter the setting menu for a certain parameter by selecting the parameter area or waveform area of the parameter, or by selecting the **【Main Menu】** hotkey on the main interface → selecting **【Parameter Setup】** from the **【Parameters】** column → selecting parameters.

#### 3.6.1 Using the Touchscreen

Select screen items by pressing them directly on the patient monitor's screen. You can access nearly all the functions by tapping directly on the screen, and almost every element on the screen is interactive, including parameter measurements, waveforms, soft keys, message areas, alarm areas, menus, etc. Information can be input using the touchscreen.

---



#### CAUTION

- Check the touchscreen for any possible damage before use. If it is broken, please to stop using the monitor immediately and contact your service personnel.
- If any sign of screen detachment occurs, please stop using the monitor immediately and contact service personnel.

---

### 3.6.2 Using the Mouse

This monitor can be connected to a mouse through the USB interface of the expansion base.

### 3.6.3 Using the Soft Keyboard

本监护仪提供软键盘，用于信息输入，软键盘功能如下：

This monitor provides a soft keyboard for information input, with the following functions:

- Select characters on the keyboard for input.
- Use the delete key  to delete the previous character.
- Use the uppercase and lowercase switch keys  to switch between English uppercase and lowercase letters.
- Use the confirm key  to confirm that the input is complete and close the soft keyboard.

## 3.7 Operating Modes

The monitor provides different operating modes. This section describes the monitoring mode and the standby mode.

### 3.7.1 Monitoring Mode

The monitoring mode is the most frequently used clinical mode for patient monitoring. When the monitor is turned on, it automatically enters the monitoring mode.

### 3.7.2 Standby Mode

You can temporarily stop patient monitoring without switching off the monitor by entering the standby mode.

#### 3.7.2.1 Entering the Standby Mode

Select the **Standby** quick key, or select the **Main Menu** quick key → from the Patient Management

column select **Standby**.

The monitor behaves as follows after entering the standby mode:

- Stops all parameter measurements.
- Disables all the alarms and prompt messages.

---

## **WARNING**

---

- Pay attention to the potential risk of placing the monitor to standby. In the standby mode, the

---

monitor stops all parameter measurements and disable all the alarm indications.

---

### 3.7.2.2 Exiting the Standby Mode

To exit the standby mode, choose any of the following ways:

- Select **Resume Monitor** to exit the standby mode and resume monitoring the current patient.
- Select **Discharge Patient** to discharge the current patient.

## 3.8 Configuring Your Monitor

Configure your monitor before putting it in use.

### 3.8.1 Setting the Date and Time

To set the system time, follow this procedure:

1. Select the **Main Menu** quick key → from the **System** column select **Time**.
2. Set Date and Time.
3. Set Date Format. Manually switch between 12 hour and 24 hour systems.



#### CAUTION

---

- Changing the date and time affects the storage of trends and events and may result in loss of data.

---

### 3.8.2 Adjusting the Screen Brightness

To adjust the screen brightness, follow this procedure:

1. Select the **Main Menu** quick key → from the **System** column select **Volume & Brightness**.
2. Set the **Brightness**.

### 3.8.3 Adjusting the Key Volume

To adjust the key volume, follow this procedure:

1. Select the **Main Menu** quick key → from the **System** column select **Volume & Brightness**.
1. Set the **Key Volume**.

## 3.9 Starting Monitoring

1. Enter the patient data.
2. Connect the required modules, patient cables and sensors.
3. Check that the patient cables and sensors are correctly connected.

4. Check that the patient settings such as [Alarm limit.], [Patient Cat.], [Paced], etc., are appropriate for your patient. Change setting according to your need for measurements.
5. Start Monitoring. Refer to the appropriate measurement section for details of how to perform the measurements you require.

### **3.10 Stopping Monitoring or Turning Off the Power**

To stop monitoring patient on a certain parameter:

1. Remove sensors from patient, and disconnect the patient cable from the sensor and module connector.
2. Do not reuse single-use disposable accessories.

If you want to turn off the monitor:

3. Confirm that the patient monitoring is finished.
4. Disconnect the patient cables and sensors from the patient monitor.
5. Press and hold the power **ON/OFF** button for above 3 seconds and confirm the operation in pop-up shut-down window.

You can unplug the monitor to cut off connection from AC power.



#### **CAUTION**

---

- Although not recommended, you can press and hold the power **ON/OFF** button for 10 seconds to force shutdown if needed. However, this may cause data loss.

---

## 4 Setup

To meet the patient needs in different clinical settings, you can set up the monitor accordingly in **General Menu**, **Module Menu**, **Config Manager**. For specific parameter measurement, the related alarm setting is complex, thus we'll introduce its setup in separate chapters. This chapter introduces only the monitor setup you need before use.

Select “**Main Menu**”  in the soft keys area → Enter “**General Menu**”, as illustrated in Figure 4-1.

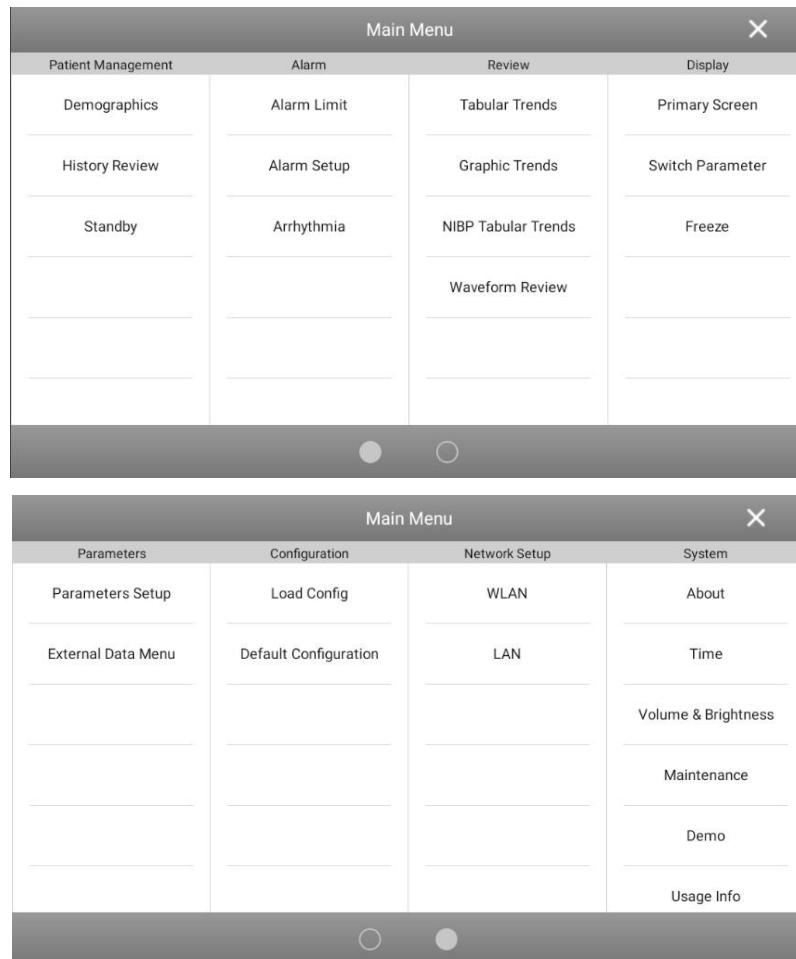


Figure 4-1: General Menu

### 4.1 Layout Setup

Click “**View/Layout**”  , Enter **View/Layout** configuration window, as illustrated in Figure 4-2.

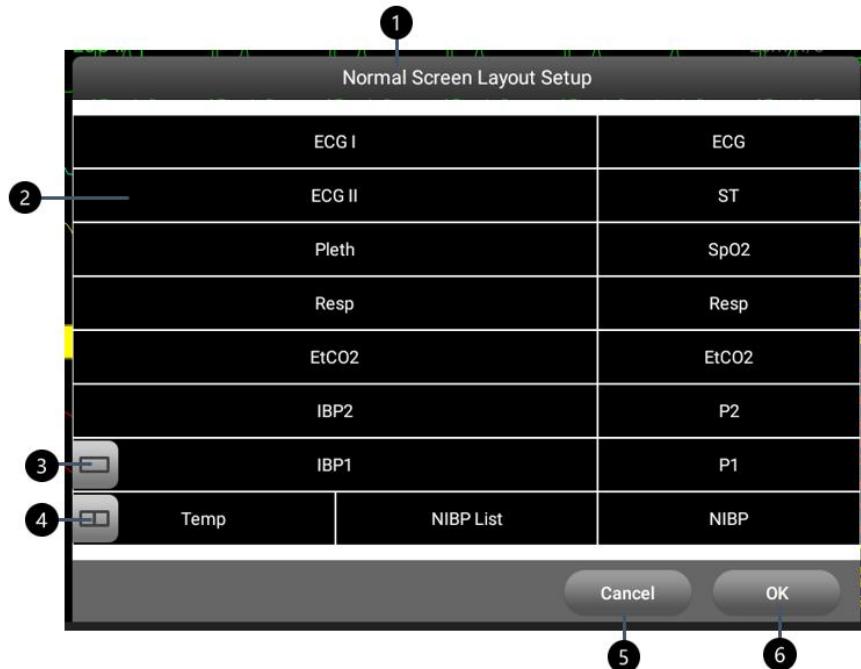


Figure 4-2: View/Layout

Number	Function Explanation
1	<b>Normal Screen Layout:</b> Display current layout: Normal View or Big Font View
2	<b>View/Layout:</b> Each cell in the table specifies the corresponding area, click the cell to fill in the selected parameters or waveforms for display.
3	<b>Layout Merge (One cell) :</b> Indicating that this one-cell waveform area is merged from 2 parameter areas.
4	<b>Layout Merge (Two cells) :</b> Click to merge 2 parameter area into one-cell waveform area.
5	<b>Cancel:</b> Click the button to cancel configuration changes and close the window
6	<b>OK:</b> Click the button, settings will be saved into configuration file and applied to monitor immediately, Normal Screen Layout will update.

### **NOTE**

- If the measurement module is not in place, corresponding parameters and waveforms can't be displayed.
- After the setup is completed, the system will save the current layout setting to the configuration file and automatically arrange the currently available waveforms and parameters to ensure the best display effect.

## 4.2 Switching On or Off a Parameter

You can manually switch on or off a parameter when its module is connected. To do so, follow this procedure:

1. Access Parameters On/Off by any of the following ways:
  - ◆ Select the **Screen Setup** quick key → select the Parameters On/Off tab.
  - ◆ Select the **Main Menu** quick key → from the Parameters column select **Parameters On/Off**.
2. Switch on or off desired parameters.

When a parameter is switched off, the monitor stops data acquisition and alarming for this measurement.

Its page is shown in Figure 4-3.

Tall Layout	Big Numerics	Switch Parameter
ECG	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/> Temp
Resp	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/> IBP1
SpO2	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/> IBP2
EtCO2	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/> Timer
NIBP	<input checked="" type="checkbox"/>	
NIBPList	<input checked="" type="checkbox"/>	

Figure 4-3: Parameter on/off page

## 4.3 External Data

Select the **Main Menu** quick key → select **External Data Menu** from the Parameters column, and enter the External Data menu, as shown in Figure 4-4.

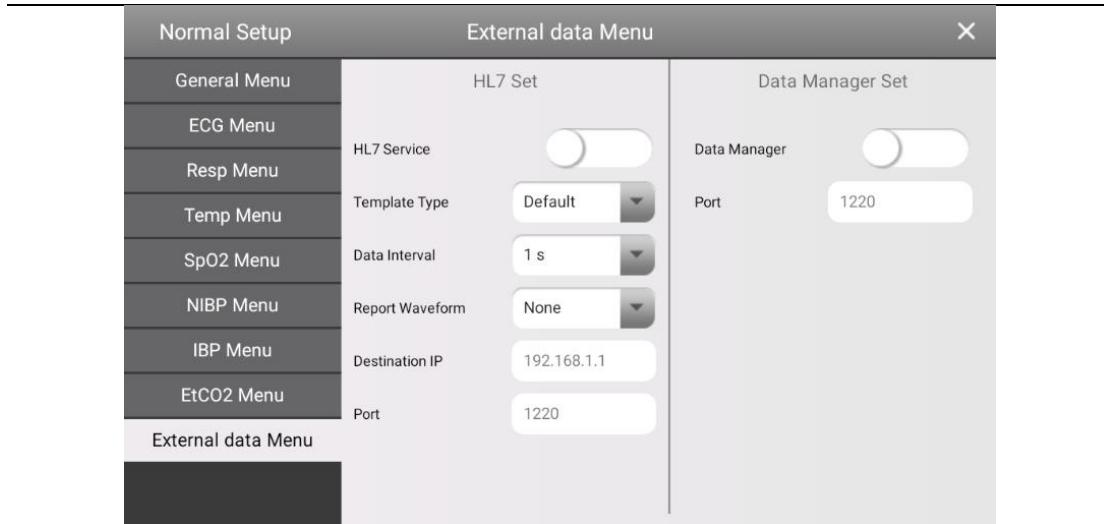


Figure 4-4: External Data Menu Page

On this page, the left side is for setting communication with HL7 Gateway, and the right side is for setting communication with DataManager. Each setting item needs to be set accordingly in order to communicate normally.

#### 4.3.1 HL7 Set

##### 1) HL7 Enable Service

Click “**HL7 Service**” button to turn **ON/OFF** HL7 Service, the default setting is **OFF**. When HL7 service is **OFF**, you could change HL7 settings. When HL7 service is **ON**, HL7 setting is disabled.

##### 2) Template Type

Select “**Template Type**” to set the Template Type and toggle between “**Default**” and “**EPIC**”. The default type is “**Default**”.

##### 3) Data Interval

Select “**Data Interval**” drop-down menu to set the data interval of HL7 message uploading. Selections are 1s, 5s, 10s, 15s, 20s, 25s, 30s, 1min. The default setting is **1s**.

##### 4) Report Waveform

Select “**Report Waveform**” drop-down menu to set HL7 waveform type for uploading. In ECG 3-lead mode, no setting is required. In 5-lead mode, Options are None, ECG I, ECG II, ECG III, ECG aVR, ECG aVF, ECG aVL, ECG V, All Leads. The default setting is **None**.

##### 5) Destination IP

The default IP address of remote receiving server for HL7 communication is 192.168.1.1. To communicate successfully, please setup the actual IP address of the remote server.

##### 6) Port

Configure the actual port of remote server. The default port is **1220**.

### 4.3.2 DataManager Set

#### 1) DataManager Enable/Disable

Select the **DataManager Enable/Disable** switch to turn on or off the DataManager service. The default setting is off. In the off state, the DataManager configuration information can be modified, while in the on state, it cannot be operated.

#### 2) Port

Configure the actual port of remote server. The default port is **1220**.

## 4.4 Net Setup


This monitor supports wireless WIFI and wired Ethernet network connections. Select **Main Menu** quick key → select **WLAN or LAN** from the **Network Setup** column to enter the corresponding network configuration page. The network defaults to DHCP to obtain the IP. If you need to set a static IP, you need to manually set it on the corresponding interface.

## 4.5 Config Manager

To meet the health care demand for different patient category, you can adjust the settings as required and then save it as a specific Config. Besides the default Config provided by default, you can create new local configurations or customize local configurations.

To access Configuration Management:

Select “**Config Manage**” in the extended soft keys area → **Configuration Management** window will appear, as illustrated in Figure 4-5.

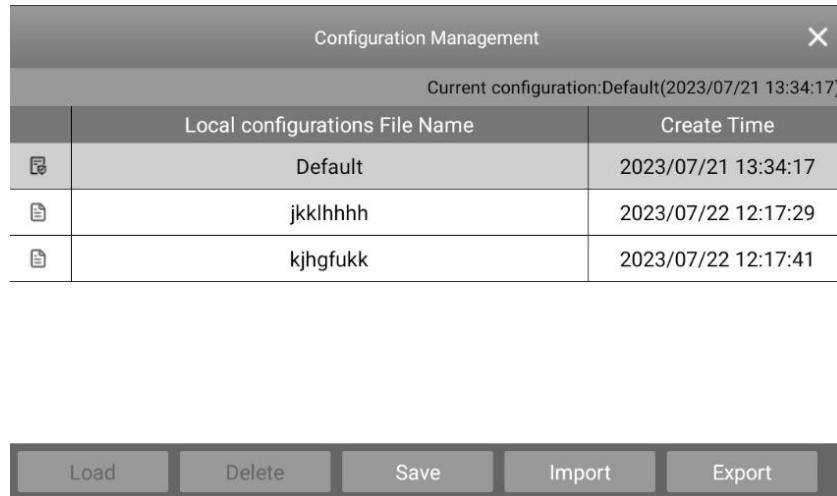

The screenshot shows a table titled "Configuration Management" with a header row: "Local configurations File Name" and "Create Time". Below the header, there are three data rows. The first row contains "Default" and "2023/07/21 13:34:17". The second row contains "jkkllhhhh" and "2023/07/22 12:17:29". The third row contains "kjhgfkukk" and "2023/07/22 12:17:41". At the bottom of the window, there is a row of buttons: "Load", "Delete", "Save", "Import", and "Export".

Configuration Management		
Current configuration:Default(2023/07/21 13:34:17)		
	Local configurations File Name	Create Time
Load	Default	2023/07/21 13:34:17
Delete	jkkllhhhh	2023/07/22 12:17:29
Save	kjhgfkukk	2023/07/22 12:17:41
Import		
Export		

Figure 4-5: Configuration Management

You need authorization to enter "**Config Manage**" and enter the password before you can operate the configuration.

Current **Configurations** are all displayed in configuration management window. In the Figure, data of each row are stored in corresponding configuration file. Default configuration can only be loaded, operations other than this are all disabled, such as delete, save as, export etc.

**1) Load**

Click “**Load**”, the selected configuration will be loaded and take effect immediately.

**2) Delete**

Click “**Delete**”, the selected configuration will be deleted, deletion will not trigger the configuration reload for current system.

**3) Save**

Click “**Save**”, Enter a name of your configuration in the pop-up window, and the configuration will be saved.

**4) Import**

Plug the USB drive with the configuration file to the equipment, click “**Import**”, and select the configuration file to be imported on the pop-up list. This function is used to share configuration files between devices of the same type.

**5) Export**

Select the row in configuration list (corresponding to the configuration file), click “**Export**” and the selected configuration will be exported to the specified USB drive.

## 4.6 Pause Display

Select “**Pause Display**”  in the soft keys area, the monitor will enter the **Pause Display** mode, the “**Pause Display**” window will appear, as illustrated in Figure 4-6.

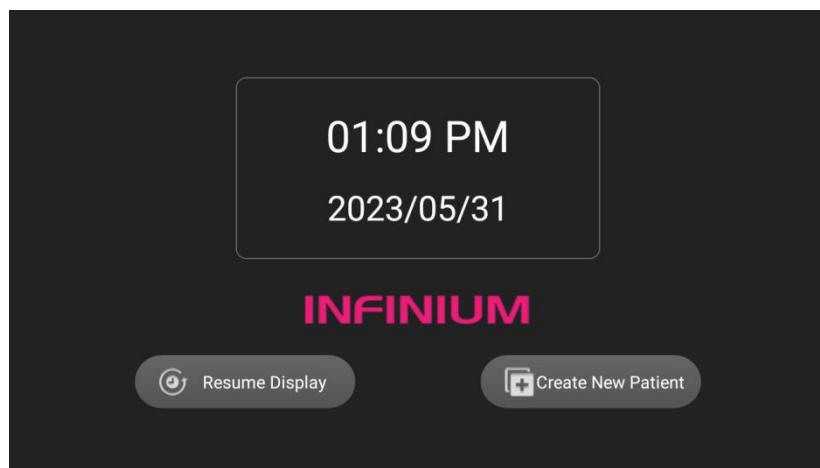


Figure 4-6: Pause Display

In this page, the following functions can be accessed:

**1) Resume Display**

Click “**Resume Display**” → The monitor will resume the display mode.

**2) Create New Patient**

Click “**Create New Case**” → The system will exit the current pause display mode. Create new patient profile by enter the patient information, after that the new monitoring procedure will start and monitoring data will be saved.

## 5 Display Mode

The TM1 patient monitor has five display modes: **Normal View**, **Big Font View**, **OxyCRG View**, **C.O. View**, and **BIS Real-time Trending View**, the display format of waveforms and parameters are different from each other in different display modes. For more details, see the explanation of each display mode.

### 5.1 Normal View

When the monitor is turned on, **Normal View** will be loaded by default, you can use two or more fingers to swipe left and right on the touch screen to switch between the **Normal View** and the **Big Font View**. In Normal View, select "View/Layout" to configure the **Normal View Layout**, as shown in Figure 5-1.

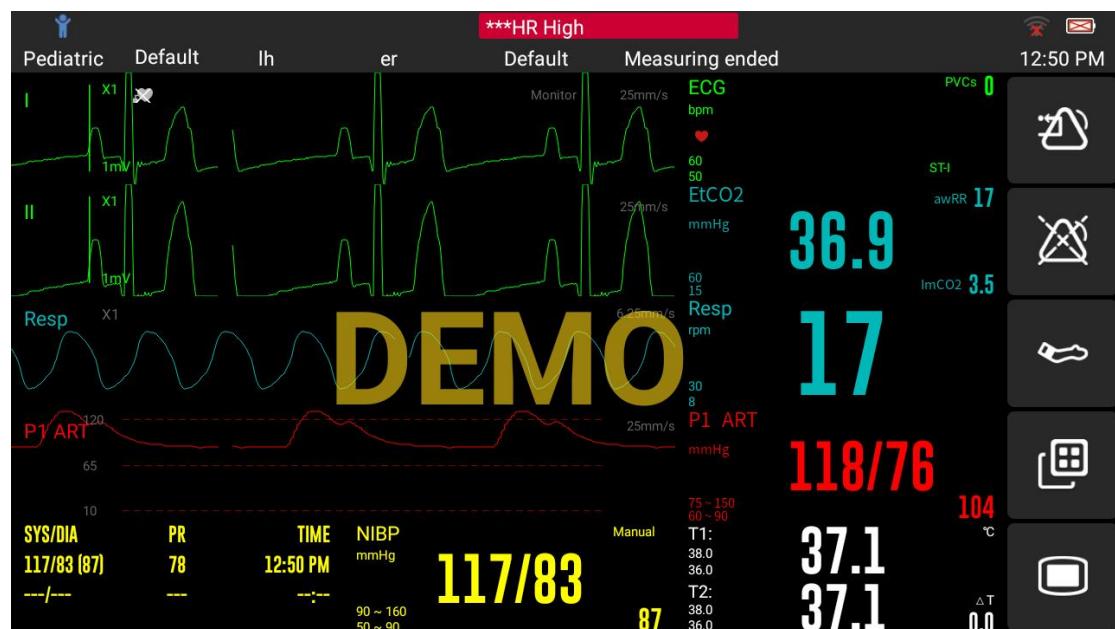


Figure 5-1: Normal View

The layout is demonstrated in Figure 5-2:

ECG I		ECG
ECG II		EtCO2
Resp		Resp
IBP1		IBP1
	NIBP List	NIBP
		Temp

Figure 5-2: Normal View Layout

In this mode, the screen could display 8 waveforms at most on main page simultaneously. And you could select from 13 waveforms: **ECG I, ECG II, ECG III, ECG AVR, ECG AVF, ECG AVL, ECG V, Pleth, Resp, IBP1, IBP2, BIS**. Therefore, this mode is suitable for monitoring situations where multiple waveforms are needed for observation at the same time.

You can customize the layout in left bottom side of the last 2 rows by merging 2 parameter areas to form a one-cell waveform area.

- Select parameter on the right column, the corresponding waveform will appear in the left cell. Vice versa, select waveform on the left column, the corresponding parameter will appear in the right cell. If the parameter does not have a waveform for display, you could choose ECG waveform for display in the corresponding space or leave it empty.
- The 2 rows and 3 columns at the bottom of the layout table is the mixed waveform-parameter area, which can flexibly meet your layout display demands. The 2 columns on the left can be merged into a waveform area, or the whole merging waveform area split into a 2-column parameter area.



### NOTE

---

- The first row of the waveform-parameter area is set to display the ECG waveform and ECG parameters. (No change can be made)

---

## 5.2 Big Font View

Swipe left and right on the touch screen using two or more fingers to switch between the **Normal View** and the **Big Font View**, as illustrated in Figure 5-3.

In Big Font View mode, select “View/Layout”  → **Big Font View Layout** window will pop up.

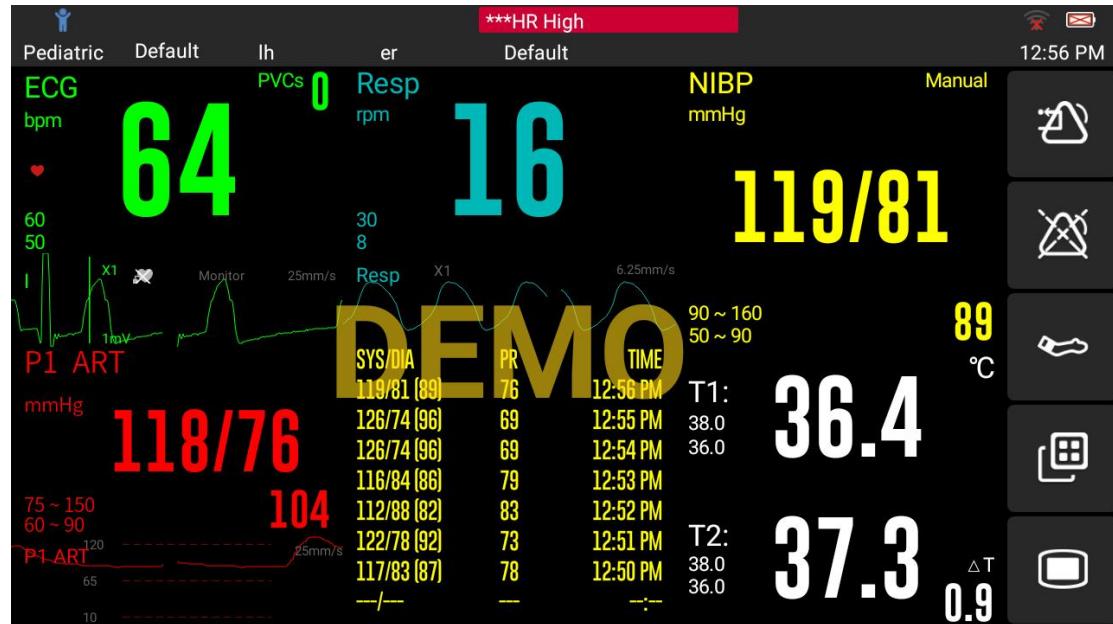


Figure 5-3: Big Font View

Figure 5-4 shows the layout setup of **Big Font View**, you could select 4 parameters with waveforms and 2 parameters without waveform in **Big Font View** mode. This mode suits the critical monitoring situation for more convenient observation.



Figure 5-4: Big Font Layout Setup

To customize the **Big Font Layout**:

- Cells in the first 2 rows and the first 2 columns in the layout table can display parameters and its waveform simultaneously. Cells in the last row could only display parameters.
- There are 6 display areas in screen.

## 6 Alarm

### 6.1 Description

Alarms, triggered by a vital sign that appears abnormal or by technical problems of the patient monitor, are indicated to the user by visual and audible alarm indications.

We'll introduce alarm settings and functions in this chapter.

### 6.2 Safety Precautions

---

---



#### WARNING

- A potential hazard can exist if different alarm presets are used for the same or similar equipment in any single area, e.g., an intensive care unit or cardiac operating room.
- Alarm setting may vary in different monitors to suit patient's needs. Before using the monitor, please ensure the previous alarm setting is suitable for this patient. Essential alarm limits should always be turned on.
- Setting alarm limits to extreme values may cause the alarm system to become ineffective.
- When the alarm sound is switched off, the patient monitor will give no audible alarm tones even if a new alarm occurs. Therefore, the user should be very careful about whether to switch off the alarm sound or not.
- Alarms must be set according to the patient's condition for those without continuous health care from medical professionals.
- Do not rely exclusively on the audible alarm system for patient monitoring. Adjustment of alarm volume to a low level or off during patient monitoring may result in a hazard to the patient. Always keep the patient under close surveillance.

---

---

### 6.3 About Alarms

#### 6.3.1 Alarm Categories

The alarms are classified into two categories: physiological alarms and technical alarms.

- **Physiological Alarms**

Physiological alarms, also called patient status alarms, are triggered by a monitored parameter value that violates set alarm limits or an abnormal patient condition.

- **Technical Alarms**

Technical alarms, also called system status alarms, are triggered by a device malfunction or a patient data distortion due to improper operation or mechanical problems. For example, Lead Wire Disconnection, Battery Too Low, Weak ECG Signal etc.

### 6.3.2 Alarm Levels

By severity, the patient monitor's alarms can be classified into three categories: high level, medium level and low level:

**High level:** Indicate that your patient is in a life-threatening situation or a severe device malfunction, an emergency treatment is demanded.

**Medium level:** Indicate that your patient's vital signs appear abnormal and an immediate treatment is required or a device malfunction. an immediate treatment is required.

**Low level:** Indicate that you patient's vital signs appear slightly abnormal, a device minor malfunction or an improper operation, an immediate treatment may be required.

### 6.3.3 Alarm Indicators

When an alarm occurs, the patient monitor will indicate it to the user through visual or audible alarm indications. Detailed indications are:

Alarm Indicator		High Level	Medium Level	Low Level	Reminder	Explanation
Alarm Lamp		Flashing Red Frequency: 2Hz Duty Ratio: 50%	Flashing Yellow Frequency: 0.5Hz Duty Ratio: 50%	Solid Blue-green Duty Ratio: 100%	/	/
Audible Alarm Tones	Default	Triple + Double + Triple + Double Beep.	Triple Beep.	Single Beep.	/	Alarm tone is set to be distinct from heartbeat and pulse sound for easy identification.
Alarm Message		Black Text with Red Background	Black Text with Yellow Background	Black Text with Blue-green Background	White Text	Alarm message appears on the top of the screen. You can click the area to view the alarm message list. The reminder appears at the bottom.
Alarm Level Symbol		***	**	*	/	The symbol will appear before the alarm message appear
Alarm Parameter		Flashing			/	/


**NOTE**

- When multiple alarms of different levels occur simultaneously, the patient monitor will select the alarm of the highest level and give visual and audible alarm indications accordingly.
- When multiple alarms of different levels occur simultaneously in the same area, only **high-level alarm** will be displayed.
- When multiple alarms of same levels occur simultaneously in the same area, the patient monitor give visual and audible alarm indications circularly.

### 6.3.4 Alarm Status Symbols

Apart from the aforementioned alarm indicators, the patient monitor still uses the following symbols telling the alarm status:



indicates alarm sound is silenced.



indicates alarm sound is paused.



indicates alarms are turned off.



indicates alarms are paused.



indicates alarm has been received, alarm is reset.

## 6.4 Check Alarm List

### 6.4.1 Check Technical Alarm List

In Normal View, to check technical alarm list:

- 1) Click “**Alarm List**” window;
- 2) Select “**Technical Alarms**” Tab.

### 6.4.2 Check Physiological Alarm List

In Normal View, to check physiological alarm list:

- 1) Click “**Alarm list**” window;
- 2) Select “**Physiological Alarms**” Tab.

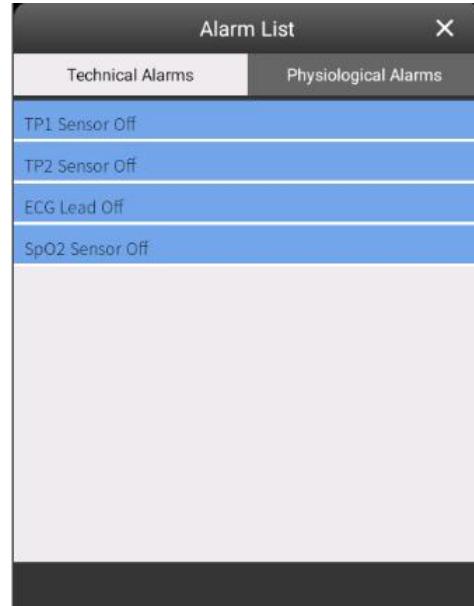


Figure 6-1: Alarm List

## 6.5 Alarm Setup

Select “**Alarm Setup**” in the extended soft key area → Enter **Alarm Setup** Menu

You need authorization to enter “**Alarm Setup**” and enter the password before you can change the configuration.

### 6.5.1 Set Alarm Properties for All Parameters

There are 3 ways to set alarm properties for the specified parameter:

1) Select “**Alarm Setup**” → “**XXX Alarm Menu**”, This patient monitor can also give alarms of these measured parameters.

In parameter specific menu, you must set **alarm ON/OFF**, **alarm limits**, **alarm level**, and **alarm record** separately on this monitor.

2) Select “**Main Menu**” → “**XXX Menu**” → “**Alarm Setup**”, in the alarm menu of the specified parameter, you could turn **ON/OFF** alarm or alarm recording, set the alarm level, high alarm limit, and low alarm limit.

3) Select the **parameter** on the screen → In the pop-up setup menu of the parameter, select “**Alarm Setup**”, in the alarm menu of the specified parameter, you could turn **ON/OFF** the alarm or alarm event saving, set the alarm level, High alarm limit, and Low alarm limit.

### 6.5.2 Alarm General Setup

Select “**Alarm Setup**” in the extended soft keys area → Select “**General Alarm Menu**”, You can set:

1) **Pause**: Select the drop-down menu to specify the pause mode for the soft key. You can toggle between “**Alarm Pause**” and “**Audio Pause**”, the default setting is “**Alarm Pause**”.

2) **Pause Time**: Set the alarm pause time as desired. Select drop-down menu to choose: **1min, 2min, 3min, infinite**, The default alarm pause time is **2 minutes**.

3) **Alarm Sound**: Set the alarm sound type.

4) **Minimum Volume**: The minimum volume determines the minimum value of the volume setting. The minimum volume range is **0 ~ 5**.

5) **High Alarm Interval**: Set the interval for high alarm lamps and alarm tones. Input interval value manually as you desired, valid input range is 3s~15s, the default setting is **10s**.

6) **Med Alarm Interval**: Set the interval for med alarm lamps and alarm tones. Input interval value manually as you desired, valid input range is 10s~20s, the default setting is **20s**.

7) **Low Alarm Interval**: Set the interval for low alarm lamps and alarm tones. Input interval value manually as you desired, valid input range is 20s~30s, the default setting is **20s**.

8) **Alarm Off Reminder**: When the alarm is off or the alarm sound is off, the monitor can provide periodic alarm prompt sound. This function is on by default.

9) **Reminder Interval**: The reminder interval can be set to 1min, 2min, 3min, 5min and 10min. The default is 5min. When the alarm is closed and alarm off reminder is on, the

---

configuration takes effect.

10) **Default:** This button can restore the default alarm configuration to the default state.

 **NOTE**

---

- Alarm sound volume can't exceed the system sound volume. When the system sound is switched off, the patient monitor will give no audible alarm tones even if a new alarm occurs, thus the user should be cautious for setting the system sound.

---

## 6.6 Pause Alarm and Pause Audio Alarm

### 6.6.1 Set the Pause Function

You can pause the alarm or pause the alarm sound according to your Pause setting. To set the pause function:

- 1) Select “**Alarm Setup**” in the extended soft key area → Click “**General Alarm Menu**” tab → Choose “**Alarm Pause**” or “**Audio Pause**”. The default setting is “**Alarm Pause**”.
- 2) Set “**Pause**” to “**Alarm Pause**” or “**Audio Pause**”, the default setting is “**Alarm Pause**”.

### 6.6.2 Alarm Pause

If the Pause soft key is set to “**Alarm Pause**”, you can select the button to pause alarm:

- All alarms are paused during the set alarm pause time.
- The remaining pause time and the alarm pause symbol will be displayed in the system status bar.

When the alarm pause session expires, the alarm paused status is automatically canceled and the alarm tone will sound. And you can cancel the “**Alarm Pause**” manually by reselecting the “**Alarm Pause**” soft key. The soft key’s name and symbol vary with the pre-defined pause function. (Alarm Pause or Audio Pause)

#### 6.6.2.1 Set Alarm Pause Time

You can select 1min, 2min, 3min or Infinite, the default alarm pause time is **2 min**. To set the alarm pause time:

- 1) Select “**Alarm Setup**” in the extended soft keys area → Select “**General Alarm Menu**” tab.
- 2) Select “**Pause Time**” as you desired.

#### 6.6.2.2 Turn Off the Alarms

If the “**Pause Time**” is set “**Infinite**” (For more details, please refer to the *6.6.2.1 Set alarm pause time*), Selecting “**Alarm Pause**” soft key will turn off all the alarms:

- No alarm lamps flash and no alarms are sounded.
- No alarm messages are shown.
- The “**alarm off**” message and **alarm off red symbol** are displayed in the system status bar.

You can cancel the “**Alarm Pause**” manually by reselecting the “**Alarm Pause**” soft key.



#### WARNING

- Alarm Pause and Alarm OFF may cause a potential hazard to patients. Please use the function

### 6.6.3 Silencing the Alarm Sound

If the pause function is set to “**Audio Pause**”, selecting “**Audio Pause**” will silence the alarm sound. When the alarm sound is muted:

- Both physiological alarms and technical alarms are off during the set alarm pause time.
- The remaining pause time and the alarm pause symbol will be displayed in the system status bar.

When the muted session expires, the alarm sound paused status will be automatically canceled and the alarm tone will sound. And you can cancel the “**Alarm Pause**” manually by reselecting the “**Alarm Pause**” soft key.

#### 6.6.3.1 Set Alarm Sound Pause Time

You can select 1min, 2min, 3min or Infinite. The default alarm sound pause time is fixed to be **2 min**.

To set the alarm sound pause time: please refer to *the 6.6.2.1*, setting steps are the same.

#### 6.6.3.2 Turn Off the Alarm Sound

If “**Pause**” is set to “**Infinite**”, Selecting “**Audio Pause**” soft key will turn off all alarm sounds:

- Both physiological and technical alarm sounds are off during the set alarm pause time.
- The “**Alarm Sound Off**” message and the **alarm sound pause red symbol** will be displayed in the system status bar.

To exit the “**Audio Pause**” status, please retap the “**Alarm Sound Off**” soft key.



#### WARNING

---

---

- Pausing or turning off alarm sound may cause a potential hazard to patients. Please use the function with careful consideration.

## 6.7 Alarm Reset

Select “**Alarm Reset**” soft key → Reset the alarm system. When the alarm system is reset successfully, the **Alarm Reset** symbol will appear in the system status bar.



### NOTE

- When monitor is in **Alarm Reset** state, if a new alarm occurs, the Alarm Reset symbol will disappear, alarm light and sound will be generated normally.

After alarm is reset:

- Current alarm sound and lamp will be blocked.
- “√” appears before the alarm message to indicate that this alarm has been received.
- Numerics stop flashing.

## 6.8 Testing Alarms

When the monitor starts up, a self-check is performed. In the meantime, alarm lamp is lit in red, yellow and blue respectively. This indicates that the alarm lamps indicators are working properly.

For further testing of a certain parameter measurement alarm, perform the measurement with a simulator. Adjust alarm limits and check that appropriate alarm behavior is observed.

## 6.9 Responding to an Alarm

When an alarm occurs, observe the following steps and take proper actions:

- Check the patient's condition.
- Confirm the alarming parameter or alarm category.
- Identify the source of the alarm.
- Take proper action to eliminate the alarm condition.
- Make sure the alarm condition is corrected.

For troubleshooting specific alarms, see appendix *Alarm Messages*.

---

## 7 ECG

### 7.1 ECG Description

The electrocardiogram (ECG) measures the electrical activity of the heart and displays it on the patient monitor as a waveform and a numeric. The monitor provides 3-lead/5-lead monitoring, ST segment and arrhythmia analysis.



Figure 7-1: ECG Display

### 7.2 ECG Safety

---



#### WARNING

---

- Direct cardiac contact with this monitor is prohibited.
- When connecting electrodes and/or patient cables, make sure that the connectors never come into contact with other conductive parts, or with earth. In particular, make sure that all of the ECG electrodes are attached to the patient.
- Use defibrillation-proof ECG cables during defibrillation.
- Do not touch the patient, or table, or instruments during defibrillation.
- To avoid burns to patients during high-frequency surgery, monitor cables, sensors must avoid contact with high-frequency electrosurgical equipment.
- Plug the ECG sensor into the ECG connector on the front panel of the monitor; Remember to align the protruding part of the sensor with the small slot of the connector when plugging it.

---

---



#### CAUTION

---

- Use only ECG electrodes and cables specified by this manual under its instruction. All warnings and notes must be followed.
- Periodically inspect the electrode application site to ensure skin quality. If the skin quality changes, replace the electrodes or change the application site.
- Interference from a non-grounded instrument near the patient and electrosurgery interference can cause problems with the waveform.

---

### 7.3 ECG Display

ECG waveform display area and parameter display area are shown in Figure 7-2.

## User's Manual for TM1 Patient Monitor

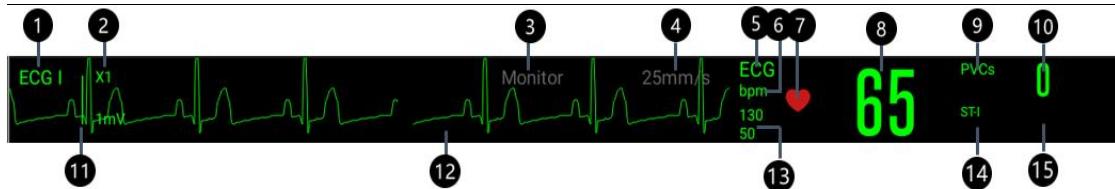


Figure 7-2: ECG Display

Number	Explanation	Number	Explanation
1	ECG Lead Label	9	PVCs Label
2	ECG Gain	10	PVCs Value
3	ECG Filter Label	11	ECG 1mV Calibration Bar
4	ECG Sweep Speed	12	ECG Waveform
5	ECG Name	13	ECG Alarm Limit
6	HR Unit	14	ST Parameter Label
7	Heart Beat Symbol	15	ST Value
8	HR Value		

### ⚠ NOTE

- For leads of different types and settings, the display of ECG parameter area and waveform area may vary.

## 7.4 Preparing to Monitor ECG

### 7.4.1 Prepare the Patient's Skin

Skin condition of the patient directly impact the ECG signal strength and the accuracy of the collected data. To properly prepare the skin, avoid bleeding or broken skin and choose flat, non-muscular areas for electrodes placement. Follow this procedure:

1. If necessary, shave hair from skin at chosen sites.
2. Gently rub skin surface at application sites to remove dead skin cells.
3. Thoroughly cleanse the site with a mild soap and water solution. We do not recommend using ether or pure alcohol, because this dries the skin and increases the resistance.
4. Dry the skin completely before applying the electrodes.

### 7.4.2 Electrode Placement

Please place the electrodes following the steps below:

1. Check whether the electrode package is intact within the expiration date. Tear off the protective paper on the back of the electrode sheet. Make sure the electrode gel is moist. Attach the clips or snaps to the electrodes before placing them.
2. Place the electrodes on the prepared skin. Squeeze out the air between the electrode and the patient's skin.
3. Attach the lead wires to the ECG trunk cable.
4. Plug the trunk cable into the equipment's ECG connector.



### NOTE

- Please store the electrodes in ambient temperature.
- Check that the patient cable or lead-wires are not damaged. Change them if necessary.
- Use the electrodes immediately once the conducting gel is unpacked.
- Use electrodes of the same brand. Using different brands with dissimilar composition can hinder an accurate ECG trace.
- When placing electrodes, choose a flat, non-muscular site where the signal will not be interfered with by either movement or bones. If you place electrodes in major muscle site, for example, the chest area, false Arrhythmia Alarm might be triggered due to the excessive muscle motion.

#### 7.4.3 Color and Letter Coding

There are two color coding standards for leads (IEC and AHA) :

Position On Body Surface	IEC		AHA	
	Inscription	Color	Inscription	Color
Right Arm	R	Red	RA	White
Left Arm	L	Yellow	LA	Black
Right Leg (Neutral)	N or RF	Black	RL	Green
Left Leg	F	Green	LL	Red
Chest 1	C1	White/Red	V1	Brown /Red
Chest 2	C2	White/Yellow	V2	Brown /Yellow
Chest 3	C3	White/Green	V3	Brown /Green
Chest 4	C4	White/Brown	V4	Brown /Blue

Chest 5	C5	White/Black	V5	Brown/Orange
Chest 6	C6	White/Purple	V6	Brown /Purple

#### 7.4.4 ECG Lead Placements

The electrode placement illustrations in this chapter adopt the AHA standard:

##### 1) 3-Leadwire Electrode Placement

Following is an electrode configuration when using 3 lead-wires:

- White Electrode (right arm) RA placement: directly below the clavicle and near the right shoulder.
- Black Electrode (left arm) LA placement: directly below the clavicle and near the left shoulder.
- Red Electrode (left leg) LL placement: on the left lower abdomen.

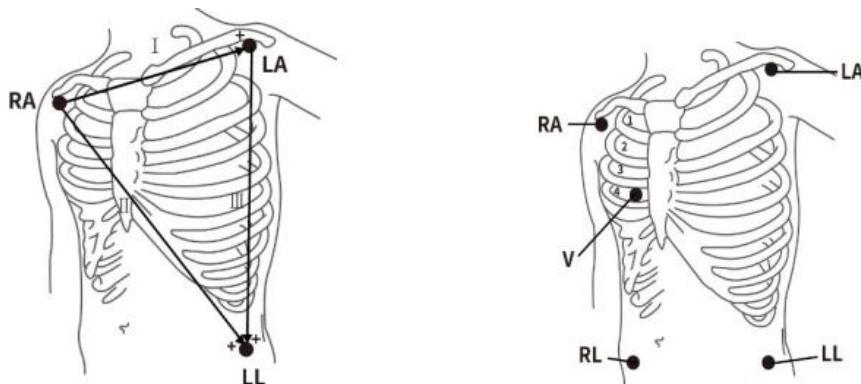



Figure 7-3: ECG Lead Placements

##### 2) 5-Leadwire Electrode Placement

Following is an electrode configuration when using 5 lead-wires:

- White Electrode (right arm) RA placement: directly below the clavicle and near the right shoulder.
- Black Electrode (left arm) LA placement: directly below the clavicle and near the left shoulder.
- Green Electrode (reference) RL placement: on the right lower abdomen.
- Red Electrode (left leg) LL placement: on the left lower abdomen.
- Brown Electrode (chest) V or C placement: on the chest.

The chest (V or C) electrode can be placed on one of the following positions:

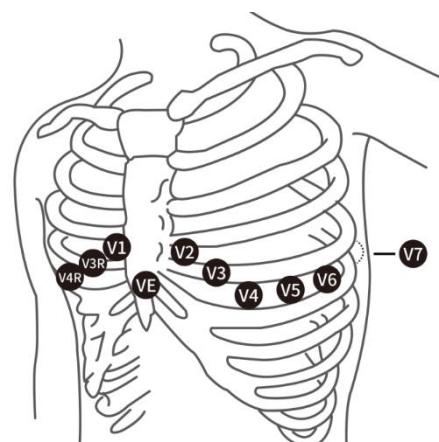

- V1 placement: on the fourth intercostal space at the right sternal border.
- V2 placement: on the fourth intercostal space at the left sternal border.
- V3 placement: midway between the V2 and V4 electrode positions.
- V4 placement: on the fifth intercostal space at the left midclavicular line.
- V5 placement: on the left anterior axillary line, horizontal with the V4 electrode position.
- V6 placement: on the left midaxillary line, horizontal with the V4 electrode position.
- V3R-V6R placement: on the right side of the chest in positions corresponding to those on the left.
- VE placement: over the xiphoid process.
- V7 placement: on posterior chest at the left posterior axillary line in the fifth intercostal space.
- V7R placement: on posterior chest at the right posterior axillary line in the fifth intercostal space.

#### **Lead Placement for Surgical Patients:**

The surgical site should be taken into consideration when placing electrodes on a surgical patient. e.g., for open-chest surgery, the chest electrodes can be placed on the lateral chest or back. To reduce artifacts and interference from electrosurgical units, you can place the limb electrodes close to the shoulders and lower abdomen and the chest electrodes on the left side of the mid-chest. Do not place the electrodes on the upper arm. Otherwise, the ECG waveform will be very small.

---

---



#### **WARNING**

---

- When using electrosurgical units (ESU), patient leads should be placed in a position that is equal distance from the electrosurgery electrotome and the grounding plate to avoid burns to the patient.
- Never entangle the ESU cable and the ECG cable together.
- When using electrosurgical units (ESU), never place ECG electrodes near to the grounding plate of the ESU, as this can cause a lot of interference on the ECG signal.

---

#### **7.4.5 Choosing ECG Lead Set**

To select ECG lead set:

1. Select ECG parameter area or waveform area → “ECG Menu”.
2. Select “Normal Setup”.
3. Set “Lead Set” according to the applied electrodes., the default type is “5-lead”.

#### **7.4.6 Checking Paced Status**

It is important to set the paced status correctly when you start monitoring ECG. The paced

symbol  is displayed when the “**Pace Detection**” is set to **ON**. The pace pulse markers “|” are shown on the ECG wave when the patient has a paced signal.

The paced symbol  will not be displayed when the “**Pace Detection**” is set to **OFF**.

To change the paced status:

1. Select ECG parameter area or waveform area → Enter “**ECG Menu**”.
2. Select “**Normal Setup**” tab.
3. Set “**Pace Detection**” to **[Yes]** or **[No]** according to patient’s need.

---

---



## WARNING

---

- For paced patients, you must set “**Pace Detection**” to **[Yes]**. Otherwise, the patient monitor could mistake a pace pulse for a QRS and fail to alarm when the ECG signal is too weak. For paced patients, Ventricular tachycardia may not always be detected
- Some heart pacemakers may cause false alarm on low heart rate or cardiac arrest due to pacemaker artifacts, for example, pacemaker overshoot may override the real QRS wave.
- Do not rely entirely on rate meter alarms when monitoring patients with pacemakers. Always keep these patients under close surveillance.
- For non-paced patients, you must set “**Pace Detection**” to **[No]**.

---

---

## 7.5 Changing ECG Settings

Select ECG parameter window or waveform area → Enter “ECG Menu” page, as shown in Figure 7-4.

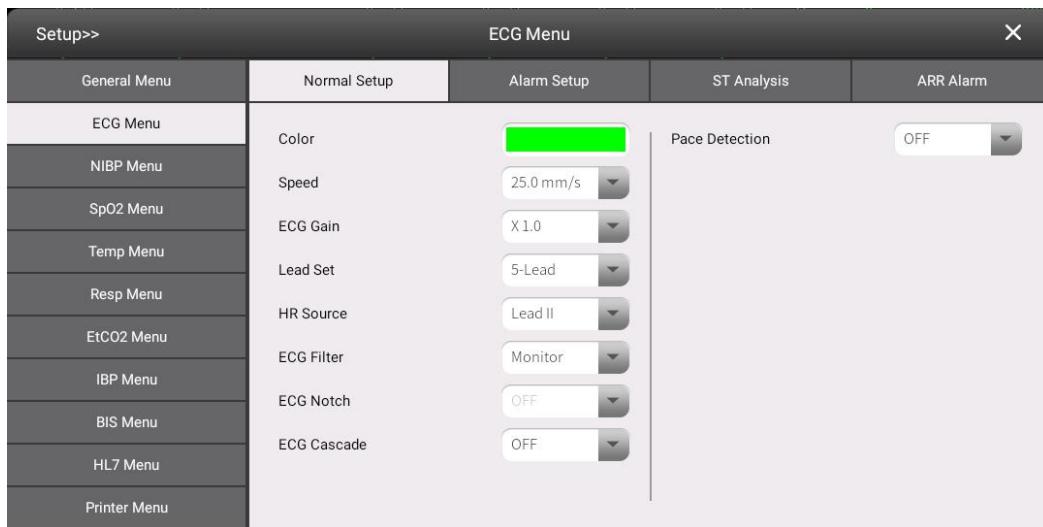


Figure 7-4: ECG Menu

### 7.5.1 ECG Normal Setup

In “ECG Menu” page, select “Normal Setup” tab to set:

#### 1) Color:

Select the drop-down menu of “Color” to set ECG waveform and parameter color. 32 colors are available, as shown in Figure 7-5. The default color is **Green**.

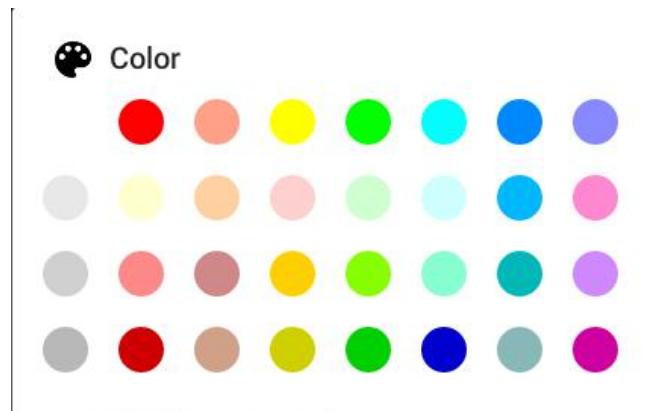


Figure 7-5: ECG Color Menu

#### 2) Speed

Select “Speed” drop-down menu, you can choose **12.5 mm/s**, **25mm/s** or **50mm/s**. The default speed is **25mm/s**. The larger the value, the faster the wave sweeps.

#### 3) ECG Gain

Select “ECG Gain” drop-down menu, you can choose **×0.25**, **×0.5**, **×1.0**, **×2.0**. ECG Gain change will adjust the waveform scale and waveform size. Higher ECG gain represents larger waveform size. The default Gain is **×1.0**.

#### 4) Lead Set

Select “**Lead Set**” drop-down menu, and toggle between **3 Leads** and **5 Leads** mode. The default setting is **5 Leads**.

#### 5) HR Source

Select “**HR Source**” drop-down menu, when lead set is **3 Leads**, you can choose **Lead I**, **Lead II** or **Lead III**. The default setting is **Lead II**.

When lead set is **5 Leads**, you can choose **Lead I**, **Lead II**, **Lead V**. The default setting is **Lead II**.

#### 6) ECG Filter

Select “**ECG Filter**” drop-down menu, you can choose **Monitor**, **Diagnose** or **Surgery**. The default setting is **Monitor**.

The ECG filter setting defines how ECG waves are smoothed:

- **[Monitor]**: Use under normal measurement conditions.
- **[Diagnostic]**: Use when diagnostic quality is required. The unfiltered ECG wave is displayed so that changes such as R-wave notching or discrete elevation or depression of the ST segment are visible.
- **[Surgery]**: Use when the signal is distorted by high frequency or low frequency interference. High frequency interference usually results in large amplitude spikes making the ECG signal look irregular. Low frequency interference usually leads to wandering or rough baseline. In the operating room, the surgery filter reduces artifacts and interference from electrosurgical units. Under normal measurement conditions, selecting **[Surgery]** may suppress the QRS complexes too much and then interfere with ECG analysis.

#### NOTE

---

- The **[Diagnostic]** filter is recommended when monitoring a patient in an environment with slight interference only.

#### 7) ECG Notch

Select “**ECG Notch**” drop-down menu to set Notch Freq. and then select **50Hz,60H or OFF** according to the power line frequency. The default “**Notch**” is **50Hz**.

#### NOTE

---

- When ECG Notch is set to **Diagnose** or **Surgeries** Notch setting is disabled with OFF shown on the button. Only when ECG Notch is set to **Monitor**, ECG Notch setting is allowed

#### 8) ECG Cascade

Select “**ECG Cascade**” drop-down menu and toggle between **ON/OFF**. When “**ECG Cascade**” is **ON**, A cascaded waveform is displayed in two waveform positions.

## ⚠ NOTE

- ECG Cascade only supports the first row of ECG waveforms.

### 9) Pace Detection

Select “Pace Detection” drop-down menu and toggle between **ON** and **OFF**. The default setting is **OFF**. When “Pace Detection” is **ON**, the pace pulse markers “|” are shown on the ECG wave when a paced signal has been detected. As shown in Figure 7-6, for more details, please refer to 7.4.6.



Figure 7-6: Pace Detection

### 10) ST 分析开关 (ST Analysis)

选择【ST 分析 (ST Analysis)】下拉选择菜单, 可关闭 (OFF) 或开启 (ON) ST 分析, 默认为关闭, 选择开启才会进行 ST 段分析。用户指定的导联上测得的 ST 段结果会以数字形式显示在 ECG 参数区。另可在趋势图或趋势列表菜单观查其以图形和列表方式显示的历史数据。

### 11) ARR 报警开关 (ARR Alarm)

选择【ARR 报警 (ARR Alarm)】下拉选择菜单, 可关闭 (OFF) 或开启 (ON) ARR 报警, 默认为关闭, 选择开启才会进行 ARR 报警。

## 7.5.2 ECG Alarm Setup

In “ECG Menu” page, select “Alarm Setup” tab, as shown in Figure 7-7.

Alarm Setup>>		ECG Menu					
		Name	Switch	Level	High Limit	Low Limit	Evt.Save
General Alarm Menu		HR	<input checked="" type="checkbox"/>	Medium	130	50	<input type="checkbox"/>
ECG Menu		ST-I	<input checked="" type="checkbox"/>	Medium	0.30	-0.30	<input type="checkbox"/>
NIBP Menu		ST-II	<input checked="" type="checkbox"/>	Medium	0.30	-0.30	<input type="checkbox"/>
SpO2 Menu		ST-III	<input checked="" type="checkbox"/>	Medium	0.30	-0.30	<input type="checkbox"/>
Temp Menu		ST-aVR	<input checked="" type="checkbox"/>	Medium	0.30	-0.30	<input type="checkbox"/>
Resp Menu		ST-aVL	<input checked="" type="checkbox"/>	Medium	0.30	-0.30	<input type="checkbox"/>
EtCO2 Menu		ST-aVF	<input checked="" type="checkbox"/>	Medium	0.30	-0.30	<input type="checkbox"/>
IBP1 Menu		ST-V	<input checked="" type="checkbox"/>	Medium	0.30	-0.30	<input type="checkbox"/>
IBP2 Menu		PVCs	<input checked="" type="checkbox"/>	Medium	10		<input type="checkbox"/>
BIS Menu							

Figure 7-7: ECG Alarm Setup Menu

You can configure the alarm setting for ECG parameters, including HR, ST-X (X represents

---

the following: I/II/II/aVR/aVL/aVF/V) and PVCS according to your needs.

## 7.6 ST Monitoring

The ST segment is an interval between ventricular depolarization and ventricular repolarization. It is identified as the end of the QRS complex to the beginning of the T wave. ST monitoring is intended to monitor the patient's oxygen supply and myocardial function. ST segment analysis calculates ST segment elevations and depressions for a given lead. As shown in Figure 7-8: As shown in the Figure below, the ST measured for each beat complex is the vertical difference between two measurement points with the R-wave peak as the baseline for the measurement.

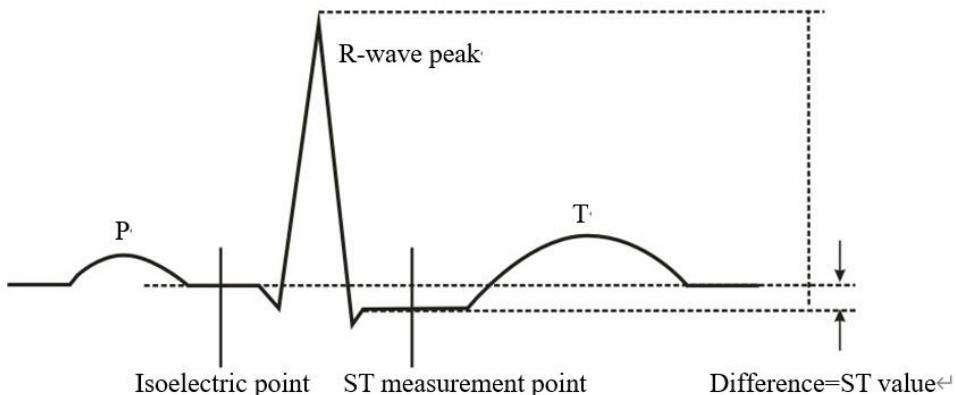


Figure 7-8: ST Segment

### 7.6.1 ST Security Information

---

#### WARNING

- Factors such as medications, metabolic or conduction disturbances may affect ST values.
- Since ST is calculated from a fixed delay after the J-point, it may be affected by heart rate variability.
- The data accuracy of the ST algorithm has been tested and its clinical significance should be determined by the physician.
- This monitor provides information on ST segment changes and the clinical significance of this information should be determined by the physician.

---



---

### 7.6.2 ST Display

Figure 7-9 shows ST numerics.

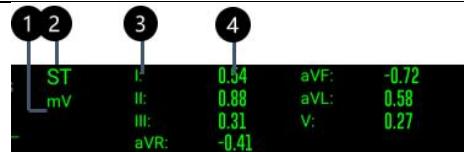


Figure 7-9: ST Numerics

Number	Explanation	Number	Explanation
1	ST Unit	3	Lead Name
2	ST Label	4	ST Value

ST parameters displayed in the ECG parameter area varies with the operating “**Lead Set**”:

When 3-lead is used for monitoring, only one ST parameter value is displayed in ECG parameter area, No ST parameter area will appear;

When 3-lead is used for monitoring, 7 ST parameters’ values are displayed in ST parameter area, they are: **ST-I, ST-II, ST-III, ST-aVR, ST-aVL, ST-aVF, ST-V**.

### 7.6.3 ST Setting

Select ECG waveform area or ECG parameter area on monitoring screen → Enter “**ECG Menu**” → Select “**ST Analysis**” tab, as shown in Figure 7-10.

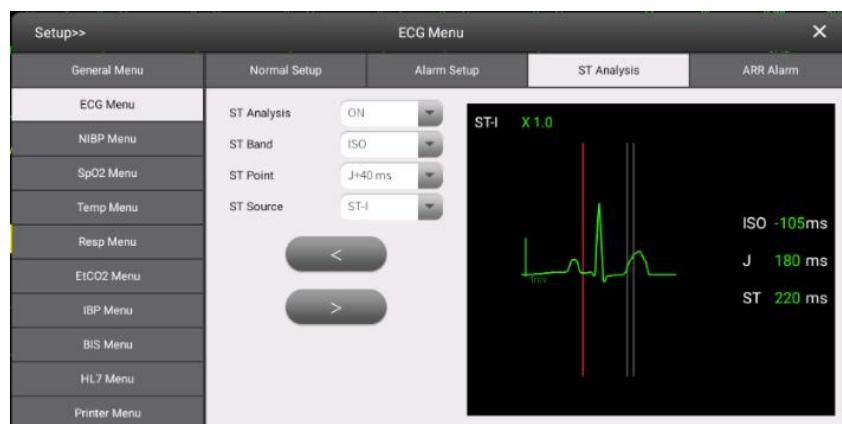


Figure 7-10: ST Setting

#### 1) Switching ST Analysis ON/OFF

Select “**ST Analysis**” drop-down menu and toggle between **OFF** and **ON**, by default, “**ST Analysis**” is **OFF**. When ST analysis is switched on, the measured ST numerics will be displayed in ECG parameter area. Also, history ST numerics can be accessed in graphical trend or tabular trend.

#### 2) ST Point

Select “**ST Band**” drop-down menu and toggle between “**ISO**”, “**J**” and “**ST**”, as shown in Figure 7-10: three vertical lines represent the ISO, J and ST point positions respectively. You can adjust the point position by using the touchscreen.

- **ISO (Reference Point)** : Set the baseline. Adjustment range is -500ms~0ms, default

setting is -105ms, indicating the reference point is located 105ms before the R-wave peak.

- **J or ST (Measurement Point)** : Specify the measurement point. Adjustment range is +460ms~+0ms, default setting is +180ms, indicating the reference point is located 180ms after the R-wave peak.

### 3) ST Source

Select “ST Source” drop-down menu to set ST Source.

When Lead Set is **3 Leads**, Options are **Lead I, Lead II and Lead III**. The default setting is **Lead II**.

When Lead Set is **5 Leads**, Options are **Lead I, Lead II, Lead III, Lead AVL, Lead AVR, Lead AVF, Lead V**. The default setting is **Lead II**.

#### 7.6.4 Additional Information

Exceptional QRS complex will not be considered in ST analysis. In some clinical situations where reliable ST monitoring can hardly be ensured, ST analysis should be switched off.

Possible situations are:

- You are unable to get a lead that is not noisy.
- Arrhythmias such as atrial fib/flutter cause irregular baseline.
- The patient is continuously ventricularly paced.
- The patient has left bundle branch block.

#### 7.6.5 Adjusting ST Measurement Points

The ST measurement (i.e., ST segment offset), refers to the vertical distance between the iso-location (ISO) and the ST point. The isotropic line is located between the end point of the P wave and the start point of the QRS complexes and provides the baseline for ST measurement. The ST point is located in the middle of the ST segment and the J point is the end point of the QRS complexes. Since the distance between the J point and the ST power is fixed, it can help to position ST point accurately.

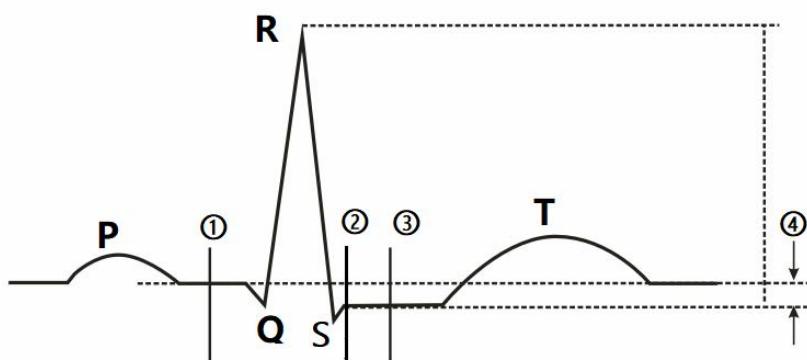


Figure 7-11: ST Measurement Adjustment

Number	Explanation	Number	Explanation
1	ISO Point	3	ST Point
2	J Point	4	ST Value

To adjust the ST measurement points:

1. In “**ECG Menu**”, Select “**ST Analysis**” tab;
2. Select corresponding setting page and then use the touchscreen to adjust the position of each point;
- The ISO-point cursor (1) positions the isoelectric point relative to the R-wave peak. Position the ISO-point in the middle of the flattest part of the baseline (between the P and Q waves or in front of the P wave).
- The J-point cursor (2) positions the J-point relative to the R-wave peak. It helps you to correctly position the ST-point. Position the J-point at the end of the QRS complex and the beginning of the ST segment.
- The ST-point is positioned a fixed distance from the J-point. Move the J-point to position the ST-point at the midpoint of the ST segment. You can select the following positions: J+40, J+60, J+80 or J+60/80. If the heart rate is greater than or equal to 120 bpm, it is recommended that the ST point is set to J + 60 ms. If the heart rate is less than 120 bpm, it is recommended that the ST point is set to J + 80 ms.

As shown in Figure 7-11 below:

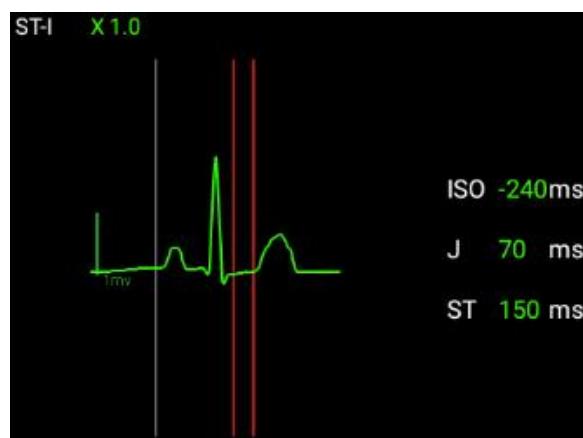


Figure 7-12: ST Measurement Points



## CAUTION

- If using ST analysis, the ST measurement points need to be adjusted when you start monitoring and if the patient's heart rate or ECG morphology changes significantly, as this may affect the size of the QT interval and thus the placement of the ST point. Artifactual ST segment depression or elevation may occur if the isoelectric point or the ST point is

incorrectly set.

- Always ensure that ST measurement points are appropriate for your patient.

---

## 7.7 Arrhythmia Analysis

Arrhythmia analysis is intended for adults, pediatrics and neonates. It can be used for both paced patient and non-paced patient monitor.

Arrhythmia analysis provides information on your patient's condition, including heart rate, PVC rate, rhythm, and ectopies. Healthcare professionals can use the analysis for patient treatment.

### 7.7.1 Safety Information

---



#### WARNING

---

- Arrhythmia may impact the Heart Rate. When patient with Arrhythmia is monitored, do not rely exclusively on the alarm messages based on HR value. Always keep the patient under close surveillance.
- Arrhythmia analysis program is intended to detect ventricular arrhythmias. It is not designed to detect atrial or supraventricular arrhythmias. It may incorrectly identify the presence or absence of an arrhythmia. Therefore, a physician must analyze the arrhythmia information with other clinical findings.

---

---



#### CAUTION

---

- The sensitivity and specificity of the arrhythmia algorithm cannot reach 100%. Sometimes false alarms or missed alarms may occur, which is especially obvious when ECG signal is severely interfered.
- ECG waveform amplitude and QRS threshold settings can affect the sensitivity of arrhythmia detection and heart rate calculation.
- If the QRS amplitude is too low, the monitor may not be able to calculate heart rate or may detect false arrests.

---

### 7.7.2 Arrhythmia Events

This monitor can detect 13 Arrhythmia events.

Number	Arrhythmia	Explanation
1	ASY	Asystole
2	FIB	Fibrillation
3	VTA	Ventricular Tachyarrhythmia
4	ROT	R_ON_T (R on T is detected)
5	RUN	VT>2 More than 2 consecutive PVCs within the last minute.
6	TPT	Irr. Rhythm Consistently irregular rhythm
7	CPT	Ventricular Couplet
8	PVC	Ventricular Premature Beats
9	BGM	Bigeminy
10	TGM	Trigeminy
11	TAC	Tachycardia
12	BRD	Bradycardia
13	MIS	Missed Beats

### 7.7.3 Changing Arrhythmia Alarm Settings

To change arrhythmia alarm settings, click “ECG Menu” → select “ARR Alarm” tab → Set the arrhythmia alarm for every arrhythmia condition according to your needs, as shown in Figure 7-12:

Name	Switch	Level	Record
ASY		High	
FIB		High	
VTA		High	
ROT		Medium	
RUN		Medium	
TPT		Medium	
CPT		Medium	
PVC		Medium	
BGM		Medium	
TGM		...	

Figure 7-13: Arrhythmia Alarm Setup Menu

## 7.8 ECG Troubleshooting

This section lists the problems that might occur. If you encounter problems when using the monitor or accessories, check the table below for troubleshooting. If the problem persists, contact your service personnel.

Problem	Corrective Action
ECG Artifact	<p>1. Check that electrodes are not detached or dry. Replace with fresh and moist electrodes if necessary.</p> <p>2. Check that leadwires are not defective. Replace leadwires if necessary.</p> <p>3. Check that patient cable or leadwires are routed too close to other electrical devices. Move the patient cable or leadwires away from electrical devices.</p>
Excessive Electrosurgical Interference	Use ESU-proof ECG cables.
Muscle Noise	<p>Inadequate skin preparation, tremors, tense subject, and/or poor electrode placement.</p> <p>1. Perform skin preparation again and re-place the electrodes. For more information, refer to 8.4 Preparing to Monitor ECG.</p> <p>2. Apply fresh, moist electrodes. Avoid muscular areas.</p>
Intermittent Signal	<p>1. Check that cables are properly connected.</p> <p>2. Check that electrodes are not detached or dry. Perform skin preparation again as described in 8.4 Preparing to Monitor ECG.</p> <p>3. Check that the patient cable or leadwires are not damaged. Change them if necessary.</p>
Excessive Alarms: heart rate, lead fault etc.	<p>1. Check that electrodes are not dry. Perform skin preparation again and replace the electrodes. For more information, refer to 8.4 Preparing to Monitor ECG.</p> <p>2. Check for excessive patient movement or muscle tremor. Reposition the electrodes. Replace with fresh and moist electrodes if necessary.</p>

User's Manual for TM1 Patient Monitor

Low Amplitude ECG Signal	<ol style="list-style-type: none"> <li>1. Check that the ECG gain is not set too low. Adjust the gain as required.</li> <li>2. Perform skin preparation again and re-place the electrodes.</li> <li>3. Check electrode application sites. Avoid bone or muscular area.</li> <li>4. Check that electrodes are not dry or used for a prolonged time. Replace with fresh and moist electrodes if necessary.</li> </ol>
No ECG Waveform	<ol style="list-style-type: none"> <li>1. Check that the ECG gain is not set too low. Adjust the gain as required.</li> <li>2. Check that the leadwires and patient cables are properly connected. Change cable and lead wires.</li> <li>3. Check that the patient cable or leadwires are not damaged. Change them if necessary.</li> </ol>
Base Line Wander	<ol style="list-style-type: none"> <li>1. Check for excessive patient movement or muscle tremor. Secure leadwires and cable.</li> <li>2. Check that electrodes are not detached or dry and replace with fresh and moist electrodes if necessary.</li> <li>3. Check for ECG filter setting. Set ECG Filter mode to <b>[Monitor]</b>.</li> </ol>

 **NOTE**

---

- For the physiological and technical alarm messages, refer to *Appendix C Alarm messages*

---

---

## 8 Resp

### 8.1 Description

Respiration is measured by thoracic impedance method. When the patient is breathing or ventilated, the volume of air changes in the lungs, resulting in impedance changes between the electrodes. Respiration rate (RR) is calculated from these impedance changes, and a respiration waveform appears on the patient monitor screen.

### 8.2 Resp Safety Information

---

---



#### WARNING

---

- When monitoring the patient's respiration, do not use ESU-proof ECG cables.
- The respiration measurement does not recognize the cause of apneas. It only indicates an alarm if no breath is detected when a pre-adjusted time has elapsed since the last detected breath. Therefore, it cannot be used for diagnostic purpose.
- If operating under conditions according to the EMC Standard EN 60601-1-2 (Radiated Immunity 3V/m), field strengths above 1V/m may cause erroneous measurements at various frequencies. Therefore, it is recommended to avoid the use of electrically radiating equipment in close proximity to the respiration measurement unit.
- When using the electrosurgery unit, ensure that the ESU return electrode is near the operating area. Also don't place ESU return electrode between the surgical area of the patient and the negative plate of the electrosurgery equipment to avoid burns at measurement sites.

---

---



#### CAUTION

---

- Use only the accessories specified by this manual and follow the guidance for operation. Adhere to all WARNING, CAUTION and NOTES.
- Respiration monitoring is not for use on the patients who are very active, as this will cause false alarms.

---

## 8.3 Resp Display

Resp waveform area and parameter area are shown as below in Figure 8-1.

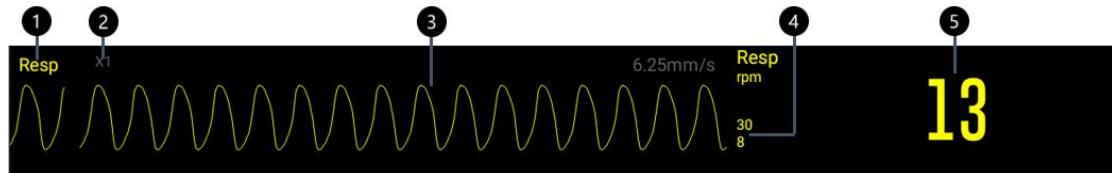


Figure 8-1: Resp Parameter and Waveform Display

Number	Explanation	Number	Explanation
1	Resp Label	4	Alarm Limit
2	Resp Gain	5	Resp Rate (RR)
3	Resp Waveform		

### ⚠ NOTE

- If ESU-proof ECG cables are used, the Resp waveform area will display the message “Check Leads. Please replace the ECG cables if necessary.

## 8.4 Preparing to Monitor Resp

### 8.4.1 Skin Preparation

Before monitoring Resp, prepare skin by the following steps:


- Shave hair from skin at chosen sites.
- Gently rub skin surface at sites to remove dead skin cells.
- Thoroughly cleanse the site with a mild soap and water solution. We do not recommend using ether or pure alcohol, because this dries the skin and increases the resistance.
- Dry the skin completely before applying the electrodes.

### ⚠ CAUTION

- As the skin is a poor conductor of electricity, preparing the skin is necessary to capture effective respiration signals.

### 8.4.2 Placing Resp Electrodes

As the Respiration measurement adopts the standard ECG electrode placement, you can use different ECG cables (3-lead, 5-lead). No additional electrodes are needed after ECG measurement. But the optimizing lead placement for Resp is essential. In clinical applications, some patients (especially neonates) expand their chests laterally, causing a negative intrathoracic pressure. In these cases, it is better to place the two respiration electrodes in the right midaxillary and the left lateral chest areas at the patient's maximum point of the breathing movement to optimize the respiratory waveform, as shown in below Figure.

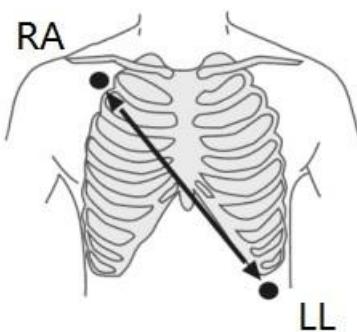

#### CAUTION

- Avoid the liver area and the ventricles of the heart in the line between the respiratory electrodes. This is particularly important for neonates.
- Some patients with restricted movement breathe mainly abdominally. In these cases, you may need to place the left leg electrode on the left abdomen at the point of maximum abdominal expansion to optimize the respiratory wave.
- In clinical applications, some patients (especially neonates) expand their chests laterally, causing a negative intrathoracic pressure. In these cases, it is best to place the two respiratory electrodes in the right midaxillary and left lateral chest areas at the patient's maximum point of breathing movement to optimize the respiratory wave
- To optimize the respiration waveform, place the RA and LL electrodes diagonally when using ECG Lead II.
- Periodically inspect the sensor application site, if skin irritations or lacerations occur, change the application site regularly.



#### NOTE

- Please store the electrodes in ambient temperature.
- Check whether the electrode package is intact and use the electrode before expiration date.

---

Don't use it if electrode conducting gel has dried out.

---

## 8.5 Setting Resp

Select Resp parameter area or waveform area → “**Resp Menu**” will pop up, as shown in Figure 8-2:

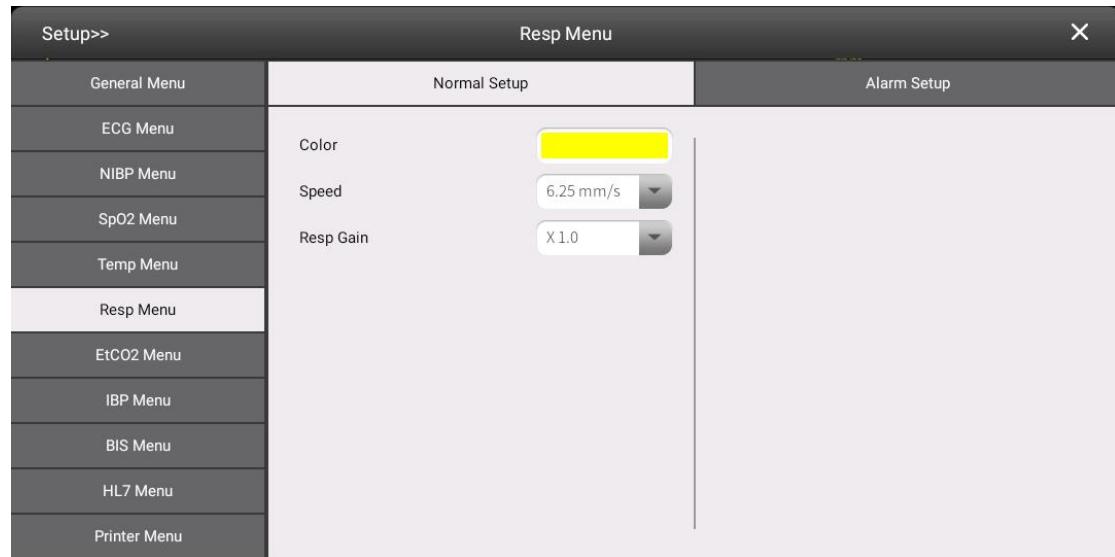


Figure 8-2: Resp Setup Menu

### 8.5.1 Resp Normal Setup

In “**Resp Menu**”, select “**Normal Setup**” tab, you can set:

**1) Resp waveform and parameter color (Color)**

Select “**Color**” → Color setting window will pop up → 32 colors are available to choose. The default color is **Cyan**.

**2) Resp Waveform Speed**

Select “**Speed**” drop-down menu → You can set speed to **6.25 mm/s, 12.5 mm/s, 25mm/s**. The default speed is **6.25mm/s**.

**3) Resp Gain**

Select “**Resp Gain**” drop-down menu → You can set Resp Gain to **×0.25, ×0.5, ×1.0, ×2.0**. Resp Gain change will change the waveform size. The default Gain is **×1.0**.

### 8.5.2 Resp Alarm Setup

Select “**Resp Menu**” → Select “**Alarm Setup**” tab, you can set alarm properties according to your need, the setup window is shown in Figure 8-3.

## User's Manual for TM1 Patient Monitor

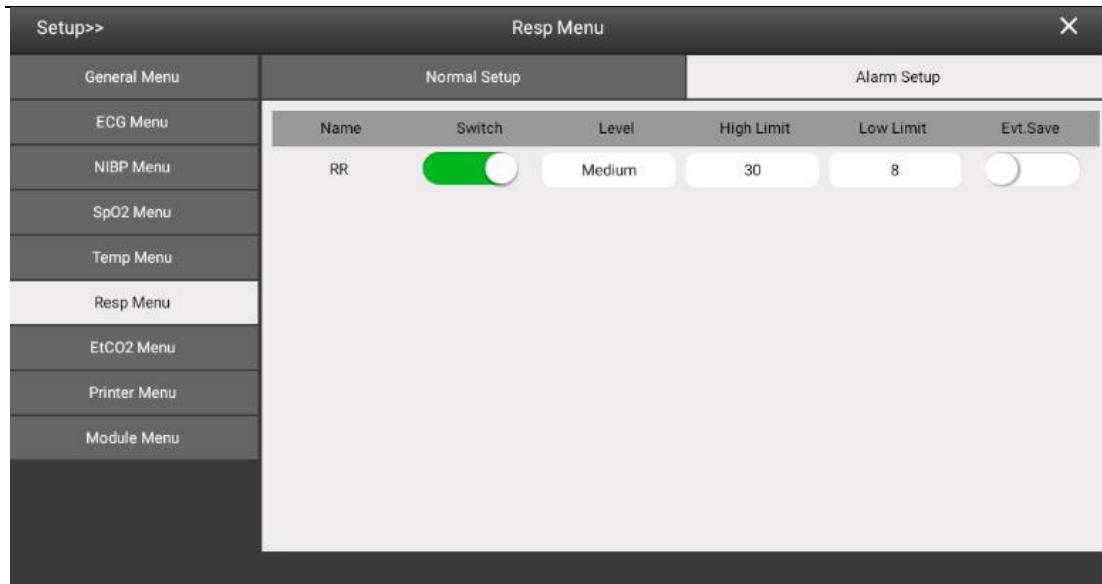


Figure 8-3 Resp Alarm Setup

### **NOTE**

---

- Apnea Alarm is set to ON by default. Change to apnea alarm is disabled.

---

## 8.6 Resp Troubleshooting

Please refer to *Appendix C alarm messages* for detailed information.

## 9 SpO2

### 9.1 SpO2 Description

SpO2(Oxygen saturation) is the percentage of saturated hemoglobin compared to total hemoglobin measured by a two-wavelength pulse oximeter (also called functional or In Vivo oxygen saturation). The SpO2 value is measured by light absorption technique: Red and infrared light is emitted from the emitter side of the sensor. The light is partly absorbed when it passes through the monitored tissue. The amount of transmitted light is detected in the detector side of the sensor. When the pulsative part of the light signal is examined, the amount of light absorbed by arterial hemoglobin is discovered and the saturation level can be calculated.

The SpO2 module processes the electrical signal and displays a “Pleth” waveform and digital values for SpO2 and pulse rate.

**This device is calibrated to display functional oxygen saturation.**

SpO2 measurement is applicable to adults, pediatrics and neonates.

This monitor supports Infinium SpO2 module, Nellcor SpO2 module and Masimo SpO2 module.

Infinium SpO2: No logo on the module;

Nellcor SpO2: Nellcor logo on the module;

Masimo SpO2: Masimo logo on the module.

#### **NOTE**

- Each SpO2 sensor connector can only be connected to the same type of extension cable. For example, Masimo SpO2 connector can only be connected to Masimo SpO2 extension cable.
- Functional testing equipment or SpO2 emulator can be used to evaluate the accuracy of PR (pulse rate) measurement.
- A functional tester or SpO2 emulator cannot be used to assess the accuracy of SpO2 sensor and pulse oximeter for monitor. They must be verified with clinical data.
- This monitor, and the SpO2 sensor, probe extension cable bundled with this equipment are all verified in compliance with ISO80601-2-61.

### 9.2 SpO2 Safety Information

#### **WARNING**

- When a trend toward patient deoxygenation is indicated, blood samples should be analyzed

by blood gas analyzer to completely understand the patient's condition.

- Do not use SpO<sub>2</sub> sensors during magnetic resonance imaging (MRI). Induced current could potentially cause burns. The sensor may affect the MRI image, and the MRI unit may affect the accuracy of the oximetry measurements.
- Prolonged continuous monitoring may increase the risk of undesirable changes in skin characteristics, such as irritation, reddening, blistering or burns. Inspect the sensor site every two hours and move the sensor if the skin quality changes. Change the application site every four hours. For neonates, or patients with poor peripheral blood circulation or sensitive skin, inspect the sensor site more frequently.
- Setting alarm limits to extreme values may cause the alarm system to become ineffective. For example, High oxygen levels may predispose a premature infant to retrorenal fibroplasia. If this is a consideration do NOT set the high alarm limit to 100%, which is equivalent to switching the alarm off.
- Each pulse oxygen probe and extension line used with the monitor are specially designed for the monitor.
- Before use, the responsible party or operator shall check the compatibility of the monitor with the probe and extension cable, otherwise it may cause patient injury.

---

---

## CAUTION

---

- Use only the SpO<sub>2</sub> sensors and other accessories specified in this manual. Follow this manual's instructions for use and adhere to all warnings and cautions.

---

### 9.3 SpO<sub>2</sub> Measurement Influencing Factors


Many factors may cause inaccurate measurement:

- Physiological characteristics that may interfere:
  - ◆ Cardiac arrest
  - ◆ Hypotension
  - ◆ Shock
  - ◆ Severe vasoconstriction
  - ◆ Severe anemia
  - ◆ Hypothermia
  - ◆ Venous pulsations
  - ◆ Darkly pigmented skin
  - ◆ Ventricular septal defects (VSDs)

- ◆ Low perfusion
- Interfering substances:
  - ◆ Intravascular dyes (such as indocyanine green, methylene blue, etc.)
  - ◆ Dysfunctional haemoglobin, such as carboxyhemoglobin (COHb) and methemoglobin (MetHb)
  - ◆ Presence of certain dyes on the measured site, such as methylene and indigo carmine
- Environmental conditions:
  - ◆ Excessive ambient light
  - ◆ Electrical interference
  - ◆ Electrosurgery
  - ◆ Defibrillation - May cause inaccurate reading for a short amount of time.
  - ◆ Excessive patient/sensor motion.
- Others
  - ◆ Incorrect sensor placement or incorrect SpO2 sensor is used.
  - ◆ Blood pressure cuff or other measuring sensor on the same limb as the SpO2 sensor

## 9.4 SpO2 Display

The SpO2 waveform area and parameter area as shown in Figure 9-1.

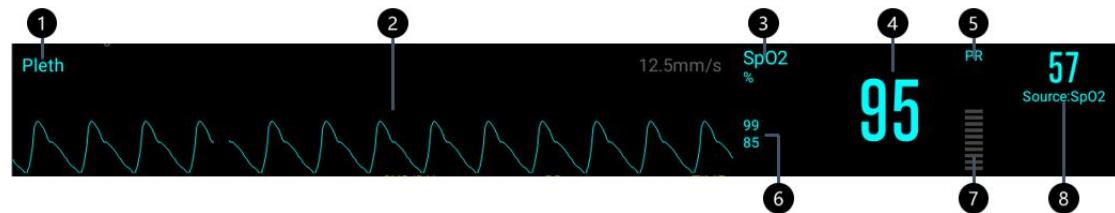

Number	Explanation	Number	Explanation
1	Pleth Label	5	PR Label
2	Pleth Waveform	6	SpO2 Alarm Range
3	SpO2 Label	7	Perfusion Indicator: the pulsatile portion of the measured signal caused by arterial pulsation.
4	SpO2 Value	8	Pulse Source: Options are SpO2, HR and IBP.

Figure 9-1: SpO2 Display

Note:

(1) The amplitude of pleth waveform can directly reflect the strength of the patient's pulse signal.

---

Pleth waveform is not normalized.

(2) The bar graph is directly proportional to the pulse intensity and can reflect the filling state of blood. As an indication of signal integrity, there are 15 grids in total. When it is less than 3 grids, the signal is weak and the measurement result may be inaccurate.

## 9.5 SpO<sub>2</sub> Measurement Preparation

To prepare:

1. Select an appropriate sensor according to the module type, patient category and weight.
2. Cleanse the surface of reusable sensor.
3. Remove colored nail polish from the application site.
4. Apply the sensor to the patient following "SpO<sub>2</sub> placement" guidelines.
5. Select an appropriate adapter cable according to the connector type and plug this cable into the SpO<sub>2</sub> connector.
6. Connect the sensor cable to the adapter cable.

---



### CAUTION

---

- Choose a sensor that matches the selected measurement site, too loose a sensor may cause light leakage, too tight a sensor may cause pulsation of the vein and make the measurement value inaccurate.
- In case of high ambient temperature, special attention should be paid to the selected measurement site with poor perfusion. High ambient temperatures can cause skin damage where the sensor placement positions for prolonged monitoring.
- Do not place sensor on a limb with the NIBP cuff, an intravenous infusion or arterial catheter in place.
- For neonatal patients, make sure that all sensor connectors and adapter cable connectors are outside the incubator. The humid atmosphere inside can cause inaccurate measurements.
- Plug the SpO<sub>2</sub> sensor into the socket/connector marked "SpO<sub>2</sub>" on the monitor panel. Remember to align the protruding part of the sensor plug with the small slot on the connector when plugging or removing it, otherwise it will cause unreliable measurements or damage to the sensor connector.
- Place the finger probe on the finger and align the finger with the direction of the finger indicated on the sensor.

---

## 9.6 Changing SpO2 Setting

Select SpO2 waveform area or parameter area → “SpO2 Menu”, as shown in Figure 9-2.



Figure 9-2: SpO2 Menu

### 9.6.1 SpO2 Normal Setup

Select “SpO2 Menu” page → select “Normal Setup” tab, to set:

#### 1) Color

Select the drop-down menu for “Color”, 2 colors are available, as shown in Figure 9-2. The default color is **Cyan**.

#### 2) Speed

Select “Speed” drop-down menu, you can choose 12.5 mm/s, 25mm/s or 50mm/s. The default speed is **25mm/s**. The larger the value is, the faster the wave sweep speed.

#### 3) Pulse Source

Select “PR Source” drop-down menu, you can choose SpO2, IBP1 or IBP2.

#### 4) FastSAT

You can set FastSat only when Masimo SpO2 module is used. Select “FastSAT” drop-down menu, and toggle between ON and OFF. The default setting is **OFF**.

#### 5) Sensitivity Mode

You can set “Sensitivity Mode” only when Masimo SpO2 module is used. Select “Sensitivity Mode” drop-down menu → Select Masimo mode, Normal mode or APOD mode. The default setting is **Normal mode**.

**Masimo mode** is used for critically ill patients that are difficult to obtain parameter values; **Normal mode** is suitable for most patients, and **APOD** (Adaptive Probe Dislodgement Detection) mode applies for cases where the probe contact with the patient is intermittent.

#### 6) Averaging Time

7) You can set **Averaging Time** only when Masimo SpO2 module is used. Select “Averaging Time” drop-down menu to set the **Averaging Time**, you can choose: 2-4s, 5-6s, 8s, 10s, 12s, 14s, 16s.

## 9.6.2 SpO2 Alarm Setup

Select “SpO2 Menu” → Select “Alarm Setup” tab, as shown in Figure 9-3.

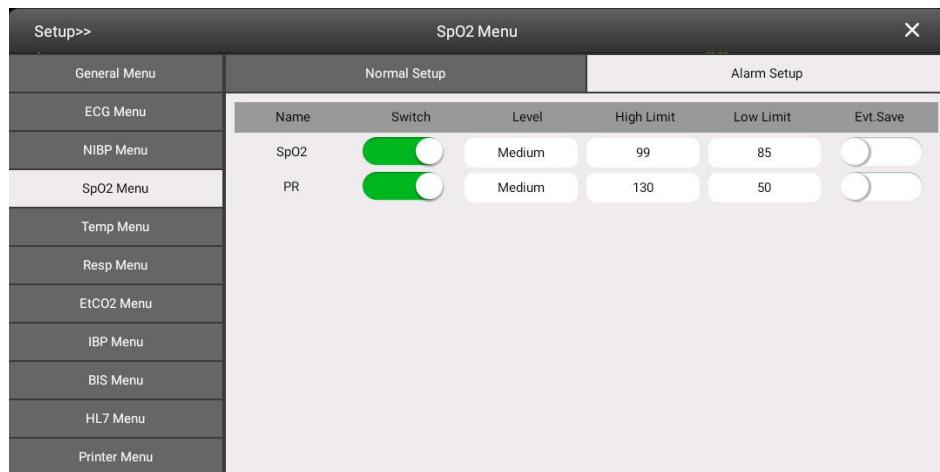


Figure 9-3: SpO2 Alarm Setup Menu

You can set the following alarm parameters for SpO2 module: SpO2, PR, PI, (PI setting is enabled only when Masimo SpO2 module is used. Set the alarm according to your needs)

## 9.7 SpO2 Troubleshooting

This section lists the problems that might occur. If you encounter problems when using the monitor or accessories, check the table below for troubleshooting. If the problem persists, contact your service personnel.

The following message may appear in “Pleth” waveform area:

Message	Explanation
“Long searching time”	SpO2 searching time is too long
“Searching pulse...”	This monitor is searching the pulse signal
“SpO2 sensor off”	The SpO2 sensor has become detached from the patient or the module
“SpO2 communication error”	There is a communication problem with the SpO2 measurement board

Problem	Corrective Action
No SpO2 parameter window and waveform area are displayed	1、Check if SpO2 module is plugged properly; 2、Check if the SpO2 parameter and waveform display is turned ON in “View Layout”. 3、Make sure SpO2 module and Main Unit of the monitor are connected.
“---” appears in SpO2 value	1、Check if the SpO2 sensor and adapter cable are connected tightly. Replace the SpO2 sensor or cable if necessary. 2、Check "SpO2 sensor off" alarm occurs, reconnect the sensor.

Pleth waveform size too low	1、NIBP cuff on the same limb as the SpO2 sensor. Change measured site if necessary. 2、PI value too low. Adjust the sensor position and connect to site with better perfusion. 3、Check sensor condition and sensor placement.
Inaccurate measurement	4、Check patient vital signs. 5、check for conditions that may cause inaccurate SpO2 readings. 6、check the monitor and the SpO2 module, cable, or sensor for proper functioning

 **NOTE**

---

- For physiological and technical alarm message, please refer to *Appendix C Alarm messages*.

---

## 10 Temp

### 10.1 Temp Description

Temperature of the human body is measured by the sensor that turns the temperature into an electrical signal, which is amplified and processed. Continuous temperature measurement uses thermistor method, based on the principle that the resistance of a thermistor changes with temperature. The thermistor measures the amount of change in resistance and thus calculates the temperature value.

The monitor can be used to measure the temperature of the patient's surface and cavity. This monitor supports 2 channel temperature measurement, the temperature of 2 channels (T1 and T2) can be displayed at the same time, and the temperature difference between two channels ( $\Delta T$ ) can be calculated and displayed.

Temp measurement is intended to use for adults, pediatrics and neonates.

### 10.2 Temp Display

Temp waveform area and parameter area are shown in Figure 10-1.



Figure 10-1: Temp Display

Number	Explanation	Number	Explanation
1	Temp Label	4	Temp Alarm Range
2	Temp Unit	5	$\Delta T$ Value: displaying the difference between two temperature values
3	T1&T2 Value		

### 10.3 Temp Measurement Preparation

Prepare for a Temp measurement by the following steps:

- 1) Select an appropriate probe according to patient type and measurement site.
- 2) Plug the Temp sensor into the "T1" or "T2" connector socket on the monitor panel.

---

3) Follow the manufacturer's instructions for probe application and instructions.

## 10.4 Temp Setting

Select Temp parameter area → “Temp Menu” will pop up, as shown in Figure 10-2.

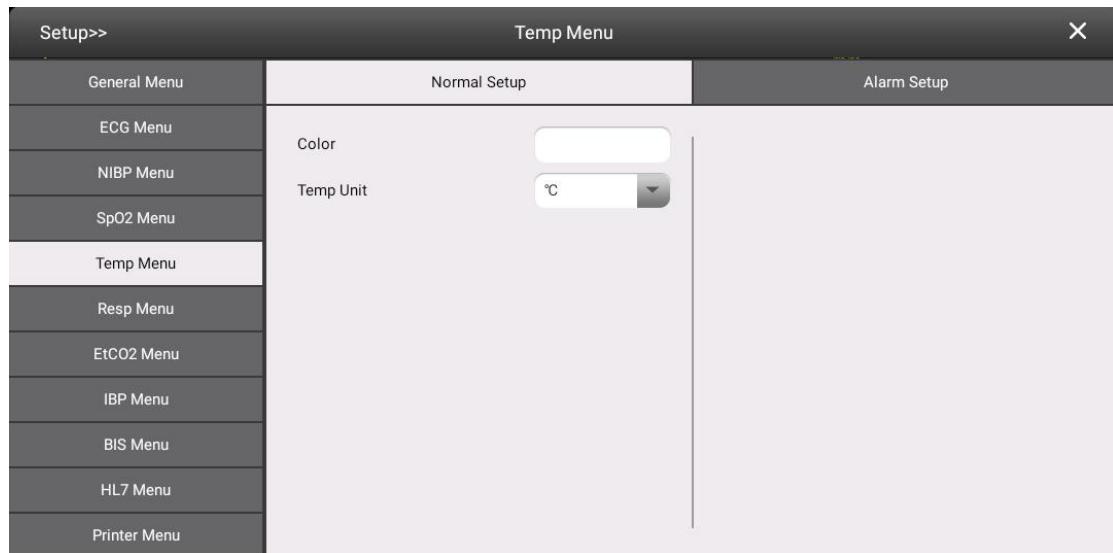


Figure 10-2: Temp Menu

### 10.4.1 Temp Normal Setup

In “Temp Menu” → Select “Normal Setup” tab:

#### 1) Color

Select “Color” → Color setting window will pop up → 32 colors are available to choose. The default color is **White**.

#### 2) Temp Unit

Select “Temp Unit” drop-down menu to set **Temp unit** and toggle between °C and °F. The default temp is °C;

### 10.4.2 Temp Alarm Setup

Select “Temp Menu” → Select “Alarm Setup” tab, as shown in Figure 10-3.

## User's Manual for TM1 Patient Monitor

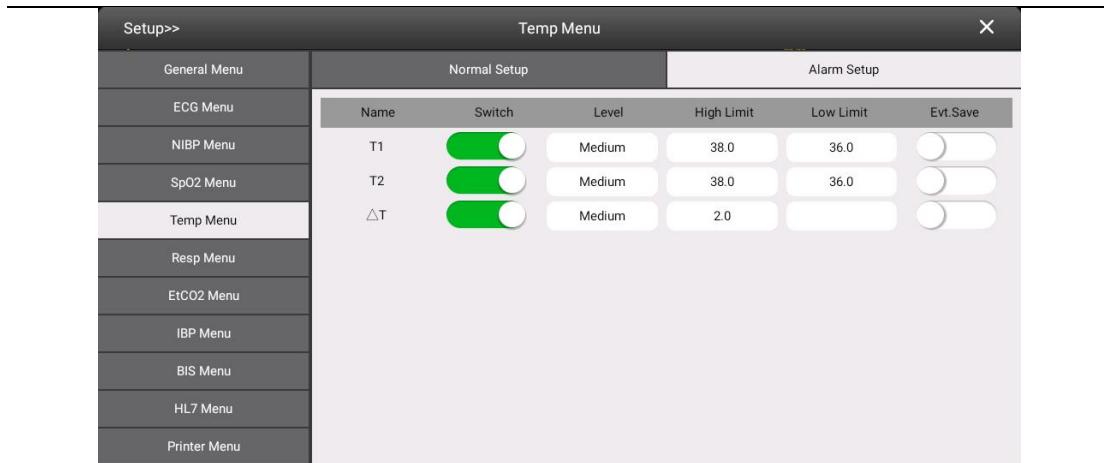


Figure 10-3: Temp Alarm Setup Menu

Temp alarm parameters are: T1, T2 and  $\Delta T$ . Set T1, T2 and  $\Delta T$  parameter according to your needs.

### 10.5 Temp Troubleshooting

This section lists the problems that might occur. If you encounter problems when using the monitor or accessories, check the table below for troubleshooting. If the problem persists, contact your service personnel.

Problem	Corrective Method
No Temp parameter area is display.	Check if Temp parameter is set to ON in “View Layout”
Measurement failure or “---” shown in Temp value	<ol style="list-style-type: none"> <li>If you are using a disposable probe, check whether the connection between the probe to the temperature cable is tight and secure.</li> <li>If any physical damage occurs on the probe, replace it with an intact one.</li> </ol>

#### NOTE

- For physiological and technical alarm message, please refer to *Appendix C Alarm Message*.



---

## 11 NIBP

### 11.1 NIBP Description

This monitor uses the oscillometric method for measuring the non-invasive blood pressure (NIBP). It is based on the principle that pulsatile blood flow through an artery creates oscillations of the arterial wall. Oscillometric devices use a blood pressure cuff to sense these oscillations that appear as tiny pulsations in cuff pressure. By measuring and analyzing at various cuff pressures, the amplitude (which changes based on the pressure within the cuff) and the frequency of these pulsations (which is dependent on the patient's heart rate), oscillometric devices can non-invasively determine blood pressure. Once the mean pressure is determined, the systolic and diastolic pressures are calculated with reference to the mean.

This measurement can be used for adults, pediatrics and neonates.



#### NOTE

---

- Blood pressure measurements determined with this device are equivalent to those obtained by a trained observer using the cuff/stethoscope auscultatory method or an intra-arterial blood pressure measurement device, within the deviations specified by IEC 60601-2-30.
- NIBP measurement can be performed during electro-surgery and discharge of defibrillator.

---

### 11.2 NIBP Safety Information

---

---



#### WARNING

---

- Be sure to select the correct patient category setting for your patient before measurement. Do not apply the higher adult settings for pediatric or neonatal patients. Otherwise, it may present a safety hazard.
- Do not measure NIBP on patients with sickle-cell disease or any condition where skin damage has occurred or is expected.
- Use clinical judgement to determine whether to perform frequent unattended blood pressure measurements on patients with severe blood clotting disorders because of the risk of hematoma in the limb fitted with the cuff.
- Do not use the NIBP cuff on a limb with an intravenous infusion or arterial catheter in place. This could cause tissue damage around the catheter when the infusion is slowed or blocked during cuff inflation.
- **Do not wear the cuff on the wound, otherwise it will cause further injury.**

---

---

- Avoid applying the cuff on the side of the mastectomy.
- **Cuff pressurization may cause temporary loss of the function of monitoring equipment used simultaneously on the same limb.**
- Kinked or otherwise restricted tubing can lead to a continuous cuff pressure, causing blood flow interference and potentially resulting in injury to the patient.
- The measurement site, patient's position (standing, sitting, lying down), exercise, or physiologic condition can all affect the NIBP readings. If you doubt the NIBP readings, determine the patient's vital signs by alternative means and then verify that the monitor is working correctly.
- Continuous non-invasive blood pressure measurements may cause purpura, ischemia and neuropathy in the limb with the cuff. Inspect the application site regularly to ensure skin quality and inspect the extremity of the cuffed limb for normal color, warmth and sensitivity. More frequent checks are required when performing automatic or continuous measurements. If any abnormality occurs, move the cuff to another site or stop the blood pressure measurements immediately. The 1 and 2-minute intervals are not recommended for extended periods of time.
- NIBP diagnostic significance must be decided by the doctor who performs the measurement.

---



## CAUTION

---

- Use only the modules and accessories specified in this manual. Follow this manual's instructions for use and adhere to all warnings and cautions.
- Accuracy of NIBP measurement depends on using a cuff of the proper size. It is essential to measure the circumference of the limb and choose the proper size cuff.

---

### 11.3 NIBP Measurement Influencing Factors

Measurements are impossible with heart rate extremes of less than 30bpm or greater than 300bpm, or if the patient is on a heart-lung machine.

The measurement may be inaccurate or impossible:

- If a regular arterial pressure pulse is hard to detect
- With excessive and continuous patient movement such as shivering or convulsions
- With cardiac arrhythmias
- Rapid blood pressure changes
- Severe shock or hypothermia that reduces blood flow to the peripheries

- Obesity, where a thick layer of fat surrounding a limb dampens the oscillations coming from the artery
- On an edematous extremity

 **NOTE**

- The NIBP feature is not validated for pregnant, including preeclamptic patients use.

## 11.4 Measurement Methods

There are three methods of measuring NIBP:

- **Manual:** measurement on demand.
- **Auto:** continually repeated measurements at set intervals.
- **STAT:** continually rapid series of measurements over a five-minute period, then return to the previous mode.

## 11.5 Understanding the NIBP Numerics

The NIBP display shows numeric only as below. Your display may be configured to look slightly different. We'll explain NIBP numerics on manual mode for illustration, as shown in Figure 11-1.



Figure 11-1: NIBP Numerics

Number	Explanation
1	<b>Unit of Pressure:</b> mmHg or kPa, the default unit is mmHg.
2	<b>Systolic / Diastolic Pressure:</b> if the real-time pressure value has risen above the high alarm limit or fallen below the low alarm limit, the numerics will flash.
3	<b>Measurement Method:</b> Indicating methods for current measurement. Methods are <b>Manual, Auto, STAT</b>

4	<b>Alarm Limits:</b> The upper digits are systolic alarm range; the bottom digits are diastolic alarm range.
5	<b>Mean Pressure:</b> Mean pressure obtained after the measurement and the real-time cuff pressure obtained during the measurement.

## 11.6 NIBP Measurement Preparation

### 11.6.1 NIBP Patient Preparation

When taking routine resting blood pressure, ensure that:

- The patient is comfortably seated, with their legs uncrossed and feet flat on the floor.
- The patient's arms and back are supported.
- The middle of the cuff is at the level of the right atrium of the patient's heart.



#### NOTE

---

- Ensure that the patient is relaxed and does not talk during the measurement.
- Allow 5 minutes to pass before taking the first measurement
- Other factors that cause high blood pressure measurements include dyspnea, bladder fullness, pain, etc.

---

### 11.6.2 NIBP Patient Connection

To place NIBP cuff:

1. Be sure to select the correct patient category setting for your patient before measurement. Verify the patient category and replace the cuff.
2. Connect the NIBP cuff hose to the module's NIBP connector.
3. Choose the appropriate cuff and make sure that the cuff has been completely deflated.

Position the NIBP cuff on the patient:

- a. Determine the patient's limb circumference.
- b. Select an appropriate cuff by referring to the limb circumference marked on the cuff. The width of the cuff should be 40% (50% for neonates) of the limb circumference, or 2/3 of the upper arm's length. The inflatable part of the cuff should be long enough to encircle at least 50% to 80% of the limb.
- c. Apply the cuff to an upper arm or leg of the patient and make sure the Φ marking on the cuff matches the artery location. Do not wrap the cuff too tightly around the limb. It may cause discoloration, and ischemia of the extremities. Make sure that the cuff edge falls within the marked range. If it does not, use a larger or smaller cuff that will fit better.
- d. Ensure that cuffed limb is supported to maintain the cuff at level of patient's heart.

Correcting the Measurement if Limb is not at Heart Level:

- Add 0.9 mmHg (0.12 kPa) for each centimeter higher, or
- Deduct 0.9 mmHg (0.12 kPa) for each centimeter lower.



## CAUTION

- Improper NIBP cuff size or compression of the cuff may lead to measurement inaccuracy.
- Avoid touching or squeezing the cuff and air tubing, otherwise the measurement may be inaccurate.
- Please be cautious about the accuracy when measuring other physiological parameters with NIBP cuff placement on the limb.

## 11.7 Starting/ Stopping NIBP Measurement

Task	Steps
Starting or Stopping a Single NIBP Measurement	<ol style="list-style-type: none"><li>1、Set NIBP measurement method to “<b>Manual</b>”</li><li>2、Start the measurement by selecting NIBP “<b>Start</b>”.</li><li>3、Stop the measurement by selecting NIBP “<b>Stop</b>”.</li><li>4、Measurement ends When the procedure is completed or measurement anomalies occur. You could also select “Stop” terminate the NIBP measurement manually.</li></ol>
Starting / Stopping NIBP Auto Measurement	<ol style="list-style-type: none"><li>1、Set NIBP measurement method to “<b>Auto</b>” and set the required interval.</li><li>2、Select NIBP “<b>Start</b>” → Start NIBP Auto measurement.</li><li>3、Start a measurement manually. The monitor will then automatically repeat NIBP measurements at the set time interval.</li><li>4、During the measurement, Select NIBP “<b>Stop</b>” at any time to terminate measurement procedure, and the count-down timer will be reset.</li></ol>
Starting / Stopping NIBP STAT Measurement	<ol style="list-style-type: none"><li>1、Set NIBP measurement method to “<b>STAT</b>”;</li><li>2、Select NIBP “<b>Start</b>”</li><li>3、In STAT mode, when the first measurement is complete, it</li></ol>

	<p>will continue the 2<sup>nd</sup> measurement. The automatic NIBP measurement process will stop after 5 measurements.</p> <p>4. During the measurement, Select NIBP “<b>Stop</b>” at any time to terminate measurement process.</p>
--	---

## 11.8 Changing NIBP Settings

Select the NIBP parameter area → “**NIBP Menu**” will pop up, as shown in Figure 11-2.

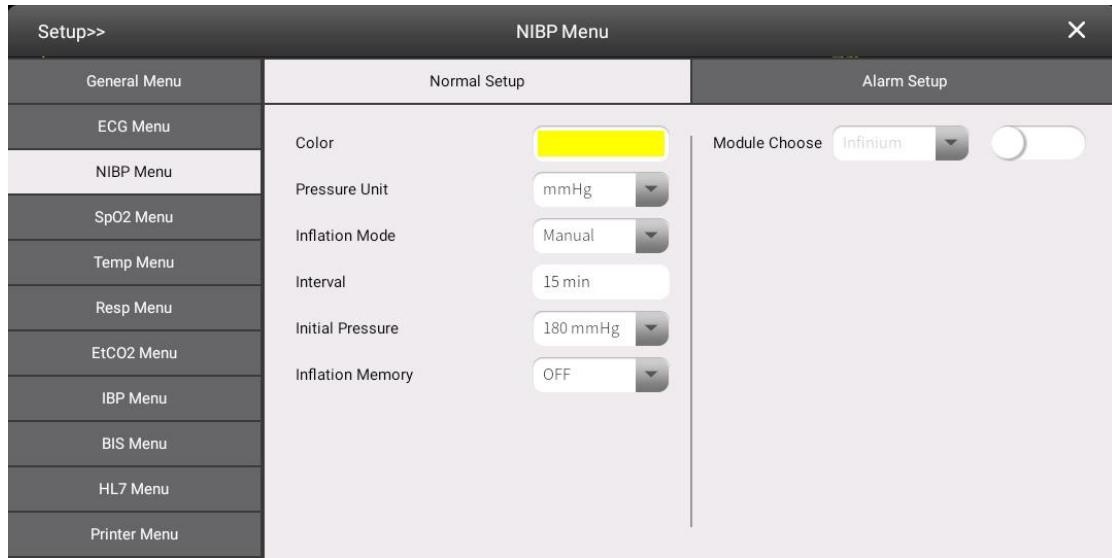


Figure 11-2: NIBP Setup Menu

### 11.8.1 NIBP Normal Setup

Select “**NIBP Menu**” → Select “**Normal Setup**” tab to set:

#### 1) Color

Select “**Color**” → Color setting window will pop up → 32 colors are available to choose. The default color is **Yellow**.

#### 2) Pressure Unit

Select “**Pressure Unit**” drop-down menu and toggle between **mmHg** and **kPa**. The default unit is **mmHg**.

#### 3) Inflation Mode

Select “**Inflation Mode**” drop-down menu → Set **Inflation Mode** for measurement method, you can select: Manual, Auto, STAT. The default “**Inflation Mode**” is **Manual**.

#### 4) Interval

When inflation mode is set to **Auto**, “**Interval**” setting will be enabled. Select “**Interval**” and then select a desired time interval. The interval range is 1 min — 4 hrs. The default Interval is **5 min**.

#### 5) Initial Pressure

Select “**Initial Pressure**” drop-down menu → Set the initial cuff inflation pressure manually, setting options may vary with the patient category.

- **Adult:**

Represents Adult Mode, during the initial measurement, the cuff is inflated to 180 mmHg, and if the blood pressure hasn't been captured, a second inflation, which is no more than 297mmHg, will start.

- **Pediatric:**

Represents Pediatrics Mode, during the initial measurement, the cuff is inflated to 140 mmHg, and if the blood pressure hasn't been captured, a second inflation, which is no more than 237mmHg, will start.

- **Neonate:**

Represents Neonates Mode, during the initial measurement, the cuff is inflated to 100 mmHg, and if the blood pressure hasn't been captured, a second inflation, which is no more than 147mmHg, will start.

#### 6) Inflation Memory

Select “**Inflation Memory**” drop-down menu → Turn **ON/OFF “Inflation Memory”**, When “**Inflation Memory**” is turned **ON**, the monitor will save the inflation pressure as baseline and set the inflation pressure as baseline + 30mmHg for next measurement automatically in order to reduce the measurement duration by decreasing the number of inflations. When “**Inflation Memory**” is turned **OFF**, then the monitor sets the inflation pressure automatically according to the previous measurement.

#### 7) NIBP Module Choose

Select “**NIBP Module Choose**” → Enter password (e.g., nbp...) to enable the drop-down menu → choose NIBP module type: **Infinium**, **SunTech Human** or **SunTech Animal**, the default setting is **Infinium**.

### 11.8.2 NIBP Alarm Setup

In “**NIBP Menu**” window → Select “**Alarm Setup**” tab, as shown in Figure 11-3.

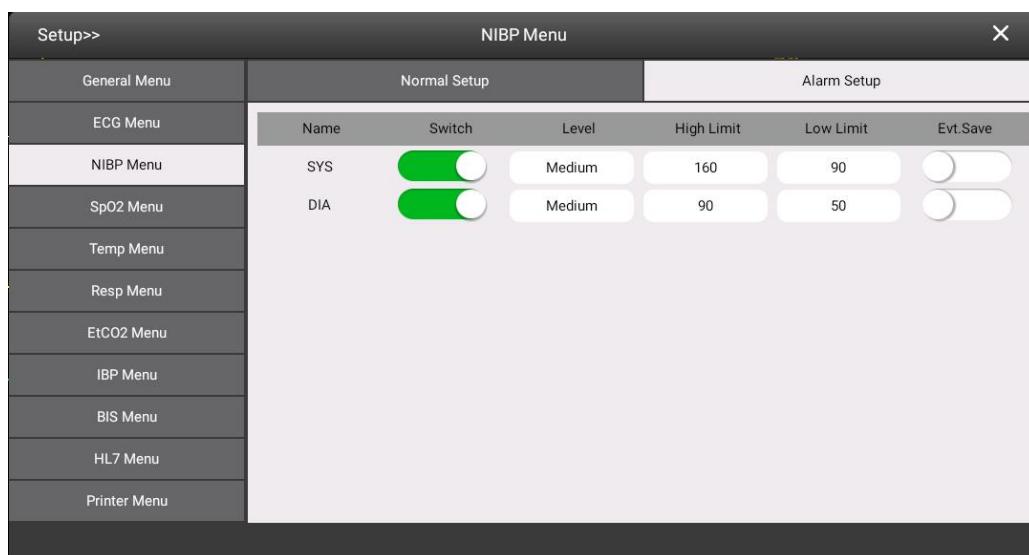


Figure 11-3: NIBP Alarm Setup Menu

You can set NIBP parameters: SYS and DIA alarm limits according to patient category

Patient Category \ Range	SYS High alarm limit (mmHg)	SYS Low alarm limit (mmHg)	DIA High alarm limit (mmHg)	DIA Low alarm limit (mmHg)
<b>Adult</b>	40~270 Factory Default Setting: 150	40~270 Factory default setting: 100	10~210 Factory default setting: 90	10~210 Factory default setting: 50
<b>Pediatric</b>	40~230 Factory default setting: 90	40~230 Factory default setting: 40	10~150 Factory default setting: 60	10~150 Factory default setting: 20
<b>Neonatal</b>	40~135 Factory default setting: 120	40~135 Factory default setting: 70	10~95 Factory default setting: 70	10~95 Factory default setting: 40

## 11.9 NIBP List

You can set “NIBP List” to be displayed in **View Layout** Menu. Then, multiple sets of most recent NIBP measurements will be displayed. And PR displayed is derived from NIBP.

SYS/DIA	PR	TIME
114/86 (84)	81	07:10 PM
122/78 (92)	73	07:05 PM
115/85 (85)	80	07:00 PM
115/85 (85)	80	06:55 PM
120/80 (90)	75	06:50 PM

Figure 11-4: NIBP List Display

Due to the screen size limit, The NIBP List displays only the most recent few NIBP measurements. The device can store a maximum 86,400 blood pressure measurement sets in its storage for NIBP List. To see more measurements, select the NIBP List display area → Enter the “NIBP Tabular Trends” Tab, as shown in Figure 11-4. Check the data by scrolling the data list, and you can manually set the number of viewable items on the current page by clicking the button to the right of "Number" according to your needs.





## **11.10 NIBP Maintenance**

### **11.10.1 NIBP Leakage Test**

The NIBP leakage test checks the integrity of the system and of the valve. It is required at least once every two years or when you doubt the measured NIBP. Leakage Test must be performed by your service personnel.

### **11.10.2 Calibrating NIBP**

NIBP is not user-calibrated. Cuff-pressure transducers must be verified and calibrated once every two years by a qualified service professional. Contact your service personnel when a calibration is necessary.

## **11.11 NIBP Troubleshooting**

Refer to *Appendix C alarm messages*

---

## 12 IBP

### 12.1 IBP Description

IBP is performed when real-time monitoring of blood pressure changes is required in critically ill patients such as shock patients, some cardiac surgeries and other major procedures. Invasive blood pressure (IBP) is generally monitored for: arterial blood pressure (ABP), central venous pressure (CVP), pulmonary artery pressure (PAP), left atrial pressure (LAP), and intracranial pressure (ICP).

The measurement principle is: First, the catheter is placed inside the blood vessel at the measured site by inserting a cannula needle in a suitable artery, and the outer end of the catheter is directly connected to the pressure transducer, due to pressure transmission effect of fluid, the blood pressure will be transmitted to the external pressure transducer through the fluid inside the catheter, so that a patient's blood pressure is constantly monitored beat-by-beat and the dynamic waveform of real-time blood pressure can be displayed. Through specific calculation methods, the systolic pressure, diastolic pressure and mean arterial pressure can be obtained.

You can measure and monitor two invasive blood pressures at the same time using a dual invasive blood pressure cable.

IBP measurement is suitable to use for adults, pediatrics, and neonates.

### 12.2 IBP Safety Information

---

---



#### WARNING

- Use only pressure transducers specified in this manual. Never reuse disposable pressure transducers.
- Make sure that the applied parts never come into contact with other electric devices.
- To reduce the hazard of burns during high-frequency surgical procedure, ensure that the monitor's cables and transducers never come into contact with the high-frequency surgical units.
- When using accessories, their operating temperature should be taken into consideration. For details, refer to instructions for use of accessories.
- All invasive procedures involve risks to the patient. Use aseptic technique. Follow catheter manufacturer's instructions.
- Mechanical shock to the invasive blood pressure transducer may cause severe shifts in zero balance and calibration, and cause erroneous readings.
- For physiological and technical alarm message, please refer to *Appendix C Alarm messages*.

---

---

## 12.3 IBP Measurement

### 12.3.1 IBP Device Connection

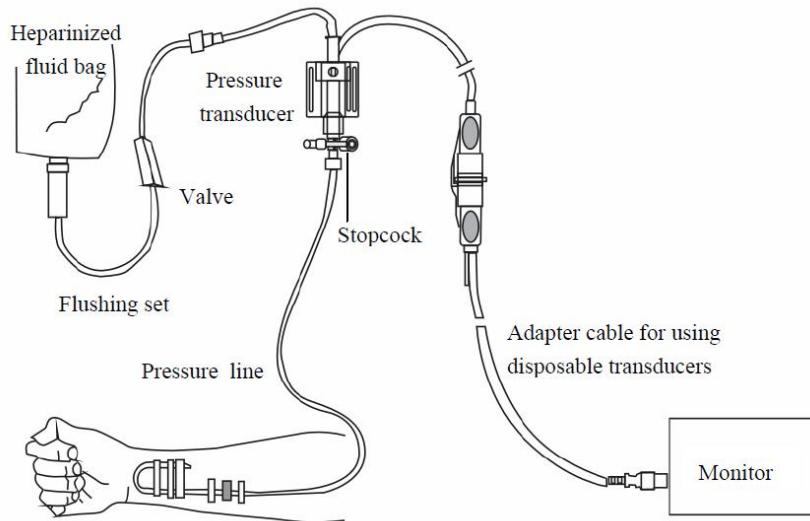


Figure 12-1: IBP Device Connection Diagram

### 12.3.2 Setting up IBP Measurement.

1. Plug the pressure cable into the IBP connector.
2. Plug the other side of the pressure cable into the IBP module.
3. Flush the system to exhaust all air from the tubing according to the IBP manufacturer's instructions. Ensure that the transducer and stopcocks are free of air bubbles.
4. Position the transducer so that it is level with the heart, approximately at the level of the midaxillary line.
5. Select the appropriate pressure label for measurement.
6. Zero the transducer. After a successful zeroing, turn off the stopcock to the atmosphere and turn on the stopcock to the patient.



#### CAUTION

- Before IBP measurement, make sure that all the transducers are zeroed correctly
- Ensure that the transducer and stopcocks are free of air bubbles. Air bubble may lead to wrong pressure reading.
- If measuring intracranial pressure (ICP) with a sitting patient, level the transducer with the top of the patient's ear. Incorrect leveling may give incorrect values.

### 12.3.3 Zeroing IBP Sensor

To avoid inaccurate pressure readings, the monitor requires a valid zero. Zero the transducer in accordance with your hospital policy (at least once per day). Zero whenever:

- A new transducer or adapter cable is used.
- You reconnect the transducer cable to the monitor.
- The monitor restarts.
- You doubt the readings.

Follow the below procedure to Zero the transducer:

1. Connect the pressure module with the transducer, and plug it into the monitor,
2. Turn off the stopcock to the patient and open the venting stopcock to air.
3. Select IBP waveform window or parameter area on screen → Enter “**IBP Menu**” → Select “**IBP1/IBP2 Setup**” tab → Select “**Zero IBP1/IBP2**”.
4. After the zero calibration is completed, close the stopcock to the air and open the stopcock to the patient.

Zeroing failure may occur when pressure fluctuates or exceeds the valid range of zeroing pressure. If zeroing fails, try the following methods:

1. Check the stopcock position to make it is vented to air.
2. Rezero the transducer and don't move the transducer and tubing to avoid motion artifacts.

## 12.4 IBP Display

The IBP measurement is displayed on the monitor as a waveform and numeric pressures. For ART pressure, Systolic, diastolic and mean pressure values of invasive blood pressures are displayed. For intravenous pressure, only mean blood pressure is displayed.

The Figure below shows the waveform and numerics for the ART pressure.



Figure 12-2: IBP Waveform and Parameter Display

Number	Explanation	Number	Explanation
1	IBP Label	5	P1 Label
2	IBP Waveform Scale	6	IBP Value (SYS/AID)
3	IBP Waveform	7	IBP Alarm Range
4	IBP Sweep Speed	8	IBP Value (MAP)



## 12.5 IBP Setting

Select IBP waveform window or parameter area → “IBP Menu” pops up, as shown in Figure 12-3.

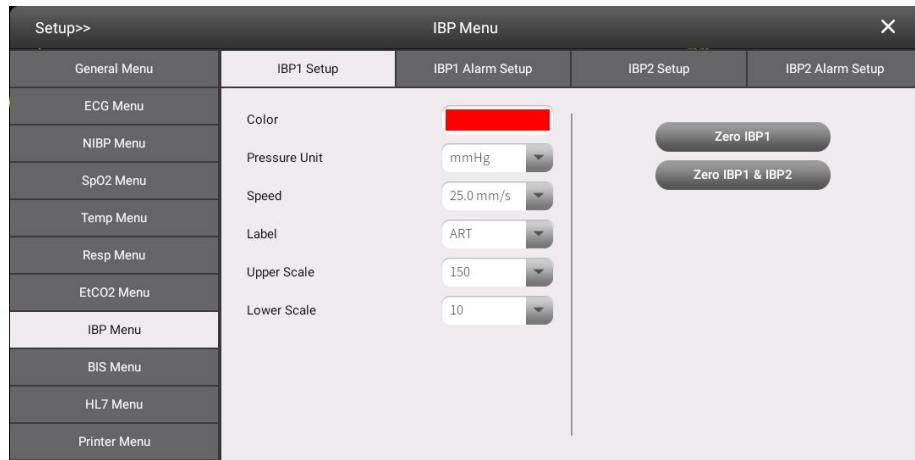


Figure 12-3: IBP Menu

### 12.5.1 IBP1/IBP2 Setup

In “IBP Menu” page → Select “IBP1/IBP2 Setup” tab to set:

#### 1) Color

Select “Color” → Color setting window will pop up → 32 colors are available to choose. The default color is **Red**.

#### 2) Pressure Unit

Select “Pressure Unit” drop-down menu to set Pressure Unit and toggle between **mmHg** and **kPa**. The default unit is **mmHg**.

#### 3) Speed

Select “Speed” drop-down menu to set speed: **12.5 mm/s**, **25 .0mm/s**. The default speed is **25.0mm/s**. The larger the speed value is, The faster the wave sweeps.

#### 4) Label

Select “Label” drop-down menu and then select your desired label from the list, IBP labels are Arterial blood pressure (**ART**), Pulmonary artery pressure (**PA**), Right atrial pressure (**RAP**), Central venous pressure (**CVP**), cranial pulse pressure (**ICP**) and left atrial pressure (**LAP**). The default is **ART**.

#### 5) Upper Scale

Select “Upper Scale” drop-down menu to set waveform Upper Scale for display, options are 180,150,120,100,75. The default **Upper Scale** is **150**.

#### 6) Lower Scale

Select “Lower Scale” drop-down menu to set waveform Lower Scale for display, options are 10, 0, -10, -20, -30. The default **Lower Scale** is **10**.

#### 7) Zero IBP1 or IBP2

Select “Zero IBP1/IBP2” → You can zero one channel at a time with selection Zero IBP1 or

Zero IBP2.

### 8) Zero IBP1 & IBP2 Simultaneously

Select “Zero IBP1& IBP2” to zero both of them.

## 12.5.2 IBP1/IBP2 Alarm Setup

In “IBP Menu” window → Select “IBP1/IBP2 Setup” tab, as shown in Figure 12-3.

Setup>>		IBP Menu							
General Menu		IBP1 Setup		IBP1 Alarm Setup		IBP2 Setup		IBP2 Alarm Setup	
ECG Menu		Name	Switch	Level	High Limit	Low Limit	Evt.Save		
IBP Menu		ART SYS	<input checked="" type="checkbox"/>	Medium	150	75	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
		ART DIA	<input checked="" type="checkbox"/>	Medium	90	60	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
		PA SYS	<input checked="" type="checkbox"/>	Medium	90	60	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
		PA DIA	<input checked="" type="checkbox"/>	Medium	75	45	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
		CVP MAP	<input checked="" type="checkbox"/>	Medium	30	10	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
		RAP MAP	<input checked="" type="checkbox"/>	Medium	30	10	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
		LAP MAP	<input checked="" type="checkbox"/>	Medium	30	10	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
		ICP MAP	<input checked="" type="checkbox"/>	Medium	30	10	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Figure 12-4: IBP Alarm Setup Menu

In this menu, you can set SYS, DIA and MAP properties for different pressure categories (ART, PA, CVP, RAP, LAP, ICP). Configure the alarm switch, alarm levels, high alarm limit and low alarm limit and alarm event recording for each parameter according to your needs.

## 12.6 IBP Troubleshooting

This section lists the problems that might occur. If you encounter problems when using the monitor or accessories, check the table below for troubleshooting. If the problem persists, contact your service personnel.

Problem	Corrective Method
No IBP parameter window and waveform area on screen	<p>1、Check if the IBP parameter and waveform display is turned ON in “View Layout”.</p> <p>2、Make sure the IBP module and monitor are connected.</p>
Invasive pressure readings seem unstable.	<p>1、Make sure there are no air bubbles in the transducer systems.</p> <p>2、Check if the transducer is fixed.</p> <p>3、Flush and zero.</p>

User's Manual for TM1 Patient Monitor

	4、 Replace the transducer.
Zeroing failure	<p>1、 Make sure that the transducer is vented to air, not to the patient, and try again.</p> <p>2、 Rezero the transducer and don't move the transducer and tubing when zeroing.</p> <p>3、 Replace the transducer if the rezeroing still fails.</p>

## 13 Managing Patients

### 13.1 Patient Information Setup

When you turn on the monitor and enters the normal screen, a prompt window will appear.

Select "**Create New Patient**" → Enter the patient information according to instructions shown on screen. When input is complete, click "**OK**" and the new patient is created.

If you select "**Continue Monitoring**", then this monitor will keep monitor the previous patient; Select "**Do Not Save**", then the patient is monitored as the **default patient**. During the monitoring process, touch the patient information area in the upper left corner of the main screen to view and modify the patient information, as shown in Figure 13-1.

Patient Management			
Room No	123	Gender	Male ►
Bed No	34	Height(cm)	168
ID	Default	Weight(kg)	65.0
First Name	er	Patient Type	Pediatric ►
Last Name	lh	Paced	OFF ►
Age	30		
		Cancel	OK

Figure 13-1: Patient Information

You can set:

#### 1) Department

Enter the patient department. User can enter a maximum of 18 characters.

#### 2) Bed NO.

Enter the patient number. User can enter a maximum of 18 characters.

#### 3) Patient ID

Enter the patient ID. User can enter a maximum of 18 characters, the patient ID cannot be empty and cannot be modified once the input is confirmed.

#### 4) Name

Patient name include First Name (Required) and Last Name (Optional) . User can enter a maximum of 18 characters.

#### 5) Gender

Set patient gender. The default setting is **Male**

#### 6) Birthday

Set patient birthday. The default setting is 01/01/2020.

#### 7) Height cm

Set patient height, the input range is 50~250cm.

#### 8) Weight kg

Set patient weight, the input range is 1~300kg.

#### 9) Patient Type

Set patient type: adult, pediatric or neonatal. The default setting is **adult**.

#### 10) Paced

Choose **ON** or **OFF**, the default setting is **OFF**.

## 13.2 Create New Patient

There are 2 methods to create new patient:

- Turn on the monitor, the “**Patient Management**” dialog window will pop up → Select “**Create New Patient**”.
- Select “**Pause Display**” in extended soft keys area → In the pop-up page, select “**Create New Patient**”.

---

---



### WARNING

---

- If you do not erase data from the previous patient, the new patient's data will be saved into the data of the previous patient. The monitor makes no distinction between the old and the new patient data.
- For paced patients, you must set “**Paced**” to **ON**. If it is incorrectly set to **NO**, the patient monitor could mistake a pace pulse for a QRS and fail to alarm when the ECG signal is too weak.
- For non-paced patients, you must set “**Paced**” to **OFF**.

---

---

## 13.3 Editing Patient Information

To edit the patient information:

Select the patient information area on the screen → “**Patient Information**” window will pop up, and you can make the required changes. Besides **Patient ID**, you can modify all the other information.

## 13.4 Deleting Patient Information

This monitor can save up to 20 patients' information. When trying to save more than 20 patients' information, message will appear: “**Full Patients, please go to the History Review to delete it from list, then you can create new patient**”!

To delete:

Select the “**History Review**” in the extended soft keys area → enter the “**History Review**”

User's Manual for TM1 Patient Monitor

---

page and select the patient ID you want to delete in the history patient list → Delete it.

If the patient ID is locked, you need to "**Unlock**" it first, then "**Delete**".

## 14 Trends

### 14.1 Description

During the patient monitoring process, the monitor will periodically collect current measurement data of each parameter and save it on the internal memory for data review, to help understand the patient's condition and health trend over a period of time. This monitor can save up to 120 hours (5 days, 24 hours per day) of monitoring data for a single patient, and display trend in graphic or tabular form to give you a picture of how your patient's condition is developing. You can export the saved monitoring data from the USB port.

The trend review page includes 4 tabs: **Graphic Trends**, **Tabular Trends**, **NIBP Tabular Trends**, and **Waveform Review**. They demonstrate the patient trend figure in different forms.

### 14.2 View Graphic Trends

Select “**Trend Review**” in the extended soft keys area → Select “**Graphic Trends**” tab, the graphic trends are shown in Figure 14-1.



Figure 14-1: Graphic Trends

Graphic trends page contains 3 fields for separate parameter graphic display. On the right side, value of each parameter, in correspondence to the cursor indicated time point (the red time line), is displayed.

#### Setting Up Trends:

##### 1) Timeline

Select “**Previous**” or “**Next**” to move the red timeline, you can position the timeline cursor in small and accurate step → Then you can simultaneously view 3 measurement value corresponding to the cursor position.

##### 2) Choose Parameters

Touch and select the parameter area on the right side of the screen → In the pop-up window,

choose parameters for monitor display as you required.

### 3) Trend Interval


Select the **Time Interval** (“5s” button in Figure 17-1) in the bottom of the page → Set the **Time Interval** in the pop-up window as you required, there are 12 options: 5s, 10s, 20s, 30s, 40s, 50s, 1min, 2min, 4min, 6min, 8min, 10min.

### 4) Trend Refresh

Select “**Refresh**” in the bottom of the page to refresh the graphic curve and parameter value.

## 14.3 View Tabular Trends

Select “**Trend Review**” in the extended soft keys area to enter the Trend review page → Select “**Tabular Trends**” tab to switch to the Tabular Trends window, as shown in Figure 14-2.

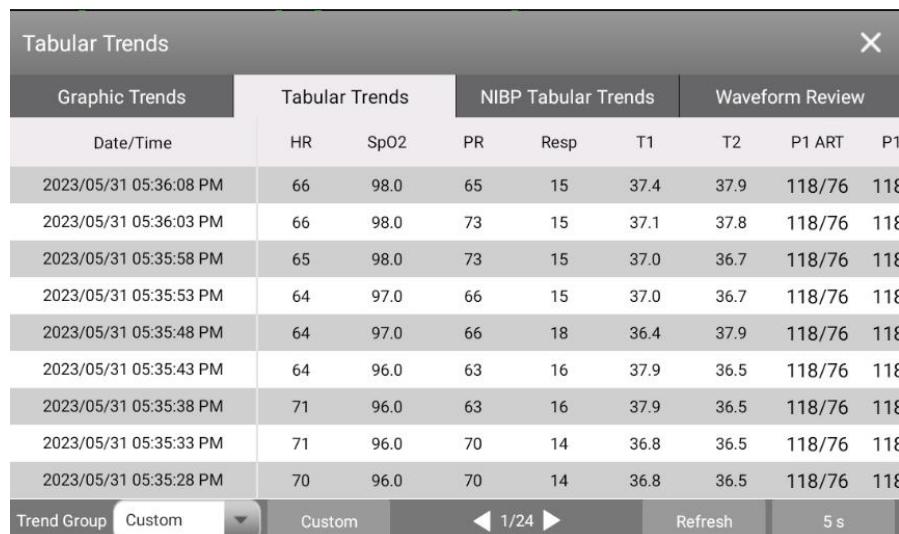

Tabular Trends								
Graphic Trends	Tabular Trends		NIBP Tabular Trends			Waveform Review		
Date/Time	HR	SpO2	PR	Resp	T1	T2	P1 ART	P1
2023/05/31 05:36:08 PM	66	98.0	65	15	37.4	37.9	118/76	118
2023/05/31 05:36:03 PM	66	98.0	73	15	37.1	37.8	118/76	118
2023/05/31 05:35:58 PM	65	98.0	73	15	37.0	36.7	118/76	118
2023/05/31 05:35:53 PM	64	97.0	66	15	37.0	36.7	118/76	118
2023/05/31 05:35:48 PM	64	97.0	66	18	36.4	37.9	118/76	118
2023/05/31 05:35:43 PM	64	96.0	63	16	37.9	36.5	118/76	118
2023/05/31 05:35:38 PM	71	96.0	63	16	37.9	36.5	118/76	118
2023/05/31 05:35:33 PM	71	96.0	70	14	36.8	36.5	118/76	118
2023/05/31 05:35:28 PM	70	96.0	70	14	36.8	36.5	118/76	118

Figure 14-2: Tabular Trends

Tabular Trends supports thermal printing.

### 1) Set Parameter

Select “**Trend Group**” drop-down menu → Select Parameters that you want to display by module or Select “**Custom**” to customize the parameters for Tabular Trends view.

### 2) Trend Interval

Select the **time interval** for trend (“5s” in Figure) in the bottom of the page → Set the required interval in the pop-up window, there are 12 options: 5s, 10s, 20s, 30s, 40s, 50s, 1min, 2mins, 4mins, 6mins, 8mins, 10mins.

### 3) Trend Refresh

Select “**Refresh**” in the bottom of the page to refresh data in tabular trend.

### 4) Browse Data

Each page displays 30 groups measurement data. You can view the all the data by scrolling the pages. There are 24 pages in total, you can Select   on the bottom to scroll left or right to navigate through the trend database.

## 14.4 View NIBP Tabular Trends

Select “Trend Review” in the extended soft keys area to enter the Trend review page → Select “NIBP Tabular Trends” tab to switch to the Tabular Trends page, as shown in Figure 14-3.

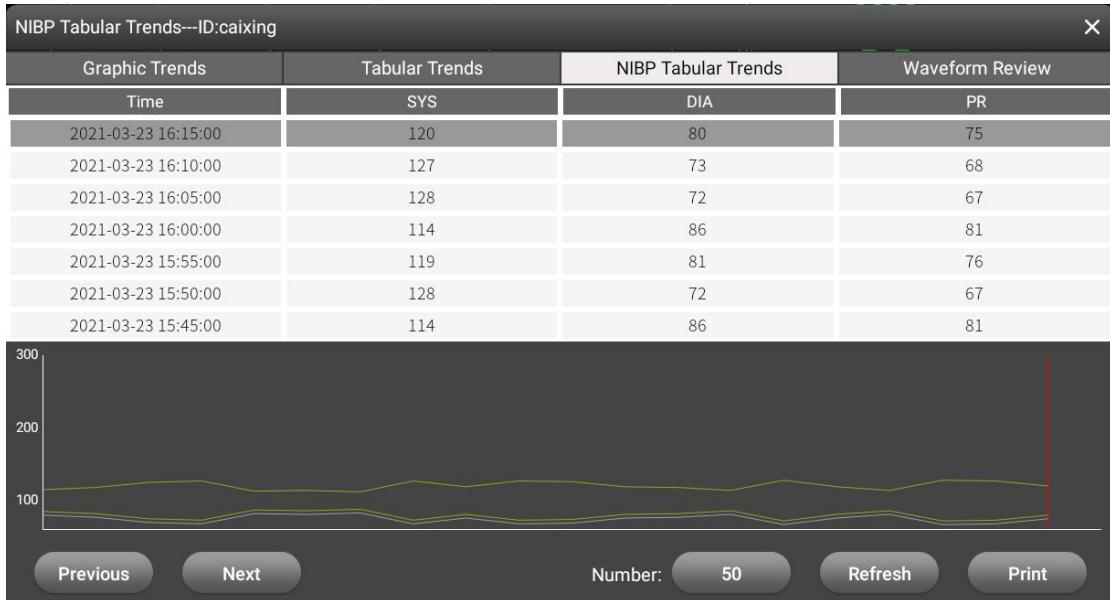


Figure14-3: NIBP Tabular Trends

NIBP measurements over a certain period of time are displayed in the form of a Graphic Trend and Tabular Trend simultaneously. Since the NIBP measurement data is not recorded and saved periodically, the NIBP trend curve is different from the other parameters' trend curves. Select a row of data in the NIBP tabular list, the red time line will navigate to the corresponding time point. Conversely, select a certain time by positioning the cursor (red time line) in the graphic trend, the corresponding row in the NIBP tabular list will be selected with gray background. By selecting the "Previous" or "Next" button at the bottom of the page, you can scroll the red time line left or right, and the row of the corresponding time point in the NIBP tabular list will be selected.

### 1) Trend Refresh

Select “Refresh” in the bottom of the page to refresh NIBP data in tabular list and graphic trend.

### 2) Maximum Number of Records from List for Display

Select the **number value** (to the right of “Number” label) → Set the maximum number of NIBP history records displayed on the current page.

### 3) Print/ Record

By selecting the “Print” button, you can print out the currently displayed data in NIBP tabular list.

## 14.5 Waveform Review

Select “Trend Review” in the extended soft keys area to enter the Trend review page → Select “Waveform Review” tab to switch to the waveform review page, as shown in Figure 14-4.

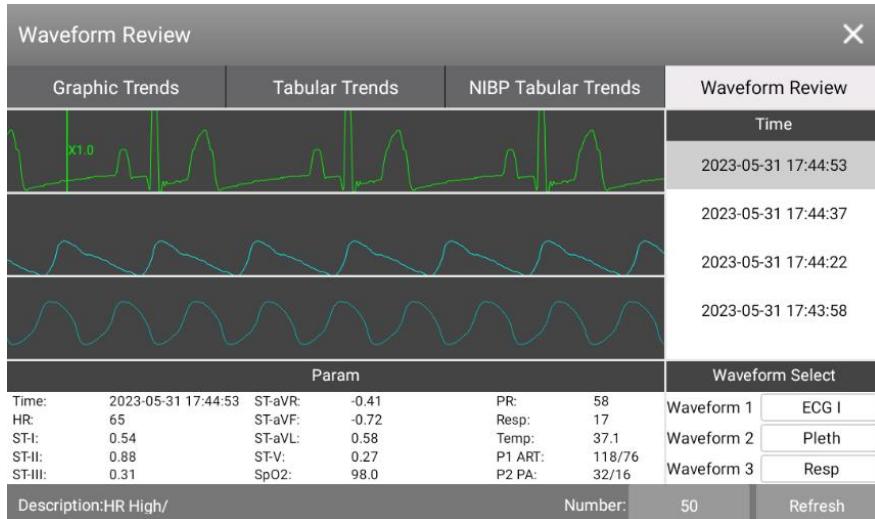


Figure 14-4: Waveform Review

This page shows the waveform and parameter values at a certain time point. The waveform and parameter data are indexed by the time points on the following:

- Waveforms freeze operation.
- Alarm event trigger.

### 1) Time

Select the record in “Time” list to load the saved data into waveform area and parameter area for display

### 2) Waveform

This page can display 3 waveforms simultaneously. To select the parameters whose waveforms you want to view, you can select “Waveform Select” in the bottom right side of the page → set “Waveform1 Waveform2 Waveform3”.

### 3) View Event Description

The “Description” in the bottom left side of the page indicates the trigger for current selected waveform and parameter recording.

### 4) Full Waveform

The waveform area shows the continuous waveforms 8s respectively before and after the currently selected time point, and you can scroll left or right to view the whole 16s waveform.

### 5) Refresh Data

Select “Refresh” in the bottom of the page to refresh waveform review list.

### 6) Number of Records for Display

Select the “Number” label → Set the maximum number of Waveform records displayed on the current page.

## 15 Patient History Data

## 15.1 Description

Patient History Data refers to the monitoring data of previous sessions when a new monitoring session starts. This monitor can save the data of the last 8 monitoring sessions at most, and you can select to view each session in the form of **Graphic Trends**, **Tabular Trends** or **Waveform Review**, and export the historical data for analysis.

## 15.2 History Data

Select “**History Review**” in the extended soft keys area to enter “**History Data**” page, as shown in Figure 15-1.

History Review					
Type	Patient ID		Start Time	Update Time	
Default	Default		2023-07-21 13:34:17	2023-05-31 17:57:39	
88767990	88767990		2023-07-22 12:16:34	2023-07-22 12:16:34	
987799009	987799009		2023-07-22 12:40:20	2023-07-29 07:37:40	
Default	Default		2023-08-02 13:42:31	2023-08-02 13:42:31	
Default	Default		2023-08-02	2023-08-02	
ID	88767990	First Name	hjkll	Weight	0.0
Gender	Male	Last Name	iyttghj	Height	56
				Age	110

Figure 15-1: History Data

You can:

### 1) Delete

Select “**Delete**” to delete the selected patient history data (When the data is locked, you are unable to delete it)

## 2) Lock/Unlock

Select “**Lock/Unlock**” to lock/unlock the selected patient history data. Once locked, the selected data can neither be overwritten nor be deleted.

### 3) Export

Select “**Export**” to export data. You can export the selected history data to the plugged USB drive.

#### 4) Open

Select “Open” in the bottom of the page → The selected data will be loaded into **Trend Review** display, as shown in Figure 15-2. For the page operations, please refer to *Chapter 14 Trend Review*.

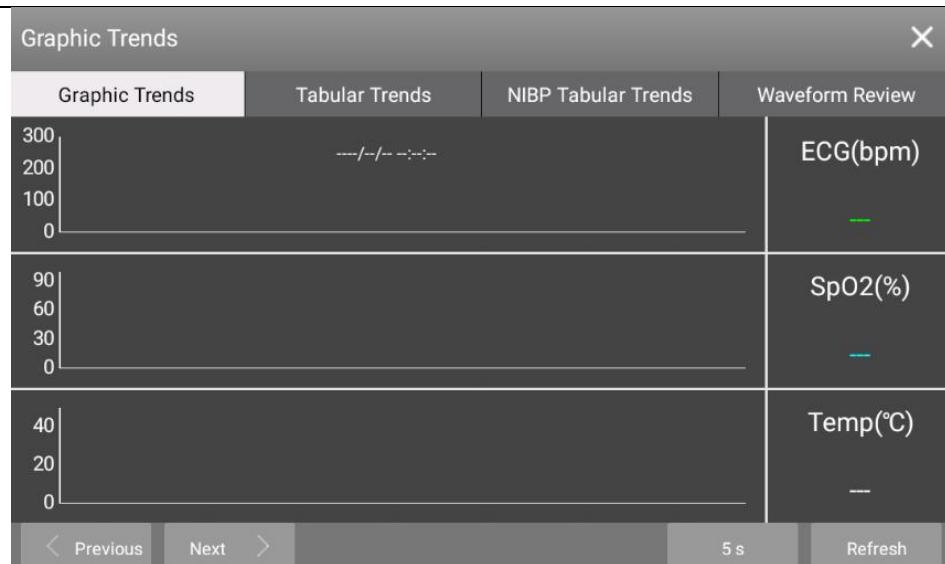


Figure 15-2: History Trend Review

## 16 Freezing Waveforms

### 16.1 Description

During patient monitoring, the freeze feature allows you to freeze the currently displayed waveforms on the screen so that you can have a close examination of the patient's status. Besides, you can select any frozen waveform for thermal printing.

### 16.2 Freezing Waveforms

When waveform is not frozen, select “Freeze”  soft keys to enter freezing process → Freeze window will pop up after the process is completed, as shown in Figure 16-1.



Figure 16-1: Freezing Waveforms

When you freeze waveforms, all the waveforms are frozen, no longer updating or sweeping. Measurement data will update normally in parameter area, real-time alarm messages will continue updating in the alarm area.

Therefore, no alarm will be missed and loss of monitoring data will not happen during the freezing operation.

### 16.3 Viewing Frozen Waveforms

When the moving waveforms are frozen, you can view the first 8 seconds and the last 8 seconds of the continuous waveform at the freeze point. and scroll the progress bar on the freeze setting page, the frozen waveform will scroll left or right accordingly, with a waveform movement step of 1 second. Therefore, you can observe the shape and other details of the entire waveform per second.

### 16.4 Saving Frozen Waveforms

Select “Save” in Freeze window to save the current frozen window into file. Also, you can review the saved waveforms in “Waveform Review” window under **Trend** page.

## 17 Internal Batteries

### 17.1 Description

The number of Lithium battery charge and discharge is more than 300 times (300-500 times, depending on the use of the situation). Battery lifespan depends on how frequent and how long it is used. If the battery is properly maintained and stored, its lifespan is about 3 years. If the battery is used improperly, its lifespan may decrease. When the battery is used frequently, replacing the lithium battery every 2 years is recommended; when it is not used frequently, it is recommended to replace the battery every 3 years.

The monitor is designed to operate on rechargeable Lithium-ion battery to ensure the normal operation of the monitor even when the AC power supply is interrupted. The patient monitor will prioritize the external AC as power source when available. If the AC power is cut off, the patient monitor will automatically run power from the internal batteries.

### 17.2 Safety Information



#### WARNING

- Keep the battery out of children's reach.
- Use only batteries specified in the chapter on "Accessories". Use of a different battery may present a risk of fire or explosion.
- Keep batteries in their original package until you are ready to use them.
- Do not expose batteries to liquids.
- Do not crush, drop or puncture batteries - mechanical abuse can lead to internal damage and internal short circuits which may not be visible externally. If a battery has been dropped or banged against a hard surface, whether damage is visible externally or not: discontinue use
- If the battery is damaged or leaking, replace it immediately.
- Extremely high ambient temperatures may cause the battery to overheat, resulting in interruption of power to the monitor.
- The lifespan of a lithium battery is two years. Replace the battery when its lifetime is expired. Failure to replace the battery on schedule may cause the battery to overheat during the monitoring process and cause serious damage to the device.
- Please install the battery into the equipment for charging before first use. When inserting the battery, Load the batteries in the chamber as indicated by the polarity symbols (+/-) marked inside, inserting the battery backward is not allowed.

- Do not open batteries, heat above 60°C (140°F), incinerate batteries, or cause them to short circuit. They may ignite, explode, leak or heat up, causing personal injury.

---

---



## CAUTION

---

- Take out the battery before the monitor is transported or will not be used for a long time.
- When using battery power, if the too many measurement modules are connected to the equipment for measurement, the monitor may automatically shut down due to excessive load.

---

## 17.3 Battery Installation

Batteries are not installed by default. Battery installation and replacement must be performed by our trained and authorized service personnel.

## 17.4 Battery Status

Battery Power Indicators, On-screen battery symbols and battery alarm message indicate the current status of the battery.

### 17.4.1 Battery Power Indicators

- Solid Green: Indicates that the batteries are charging.
- Green, Flashing: when the patient monitor operates on battery power.
- No light: when no battery is installed or no AC source is connected.

### 17.4.2 On-screen Battery Symbols

On-screen battery symbols indicate the battery status as follows:

-  Indicates that no batteries are installed
-  Indicates that batteries work correctly. The solid portion represents the current charge level of the batteries in proportion to its maximum charge level.
-  Indicates that the batteries have low charge level and need to be charged.
-  Indicates that the batteries are charging.
-  Indicates that the batteries are fully charged.
-  Indicates that the batteries malfunction.

### 17.4.3 Battery Level Indicator

The battery level indicator information is displayed on the right side of the battery icon, as shown in the following figure.



### 17.4.4 Battery Alarm

If the battery capacity is too low, a technical alarm will be triggered and the [Battery Too Low] message displayed. At this moment, apply AC power to the patient monitor. Otherwise, the patient monitor will power off automatically in 15s.

## 17.5 Charging a Battery

The battery is charged whenever the patient monitor is connected to an AC power source regardless of whether or not the patient monitor is currently on.

## 17.6 Conditioning a Battery

### 17.6.1 Optimizing Battery Performance

The performance of rechargeable batteries may deteriorate over time. Battery performance check is recommended to be performed every 3 months. If the battery is not optimized for a long time, it may cause the inaccuracy of battery indicator, resulting in a wrong judgment of the remaining battery operating time.

A battery needs at least two conditioning cycles when it is put into use for the first time. A battery conditioning cycle is one complete, uninterrupted charge of the battery, followed by an uninterrupted discharge of the battery. Batteries should be conditioned regularly to maintain their useful life.



#### NOTE

- Do not monitor patients when the batteries are conditioned.
- Do not stop charging or discharging cycle when batteries during conditioning.

### 17.6.2 Check Battery Performance

The performance of rechargeable batteries may deteriorate over time. Battery performance check must be performed every 3 months.

If you doubt that there is a battery malfunction, Check batter performance immediately.

The operating time of the battery reflects its performance directly. If the discharging time of a battery is noticeably shorter than that indicated in the specifications, replace the battery or contact

---

your service personnel.

If the battery condition is normal, Reconnect the monitor to mains power and charge the battery until it is full for use or charge to 40~60% for storage.



### NOTE

---

- The operating time depends on the configuration and operation. For example, Screen brightness too high or monitoring NIBP repeatedly will all shorten the operating time of the batteries.

---

## 17.7 Storing a Battery

When storing the battery, make sure the electrodes of the battery are not in contact with metal objects. If the battery needs to be stored for prolonged period, it should be placed in a cool environment and charged to 40%-60%.

Stored batteries should also be conditioned periodically.



### NOTE

---

- Remove the battery from the monitor when it is not used for a longer period of time, to avoid potential damage caused by battery leakage.
- Storing batteries in high temperatures for long periods of time will significantly reduce the battery lifespan.
- The temperature range for battery storage is -5°C~35°C. Storing the battery in a cool environment can slow down the battery aging. Ideally, batteries should be stored at 15°C.

---

## 17.8 Disposing of Used Batteries

Replace the used batteries and dispose them when:

- There is clear damage.
- There is a malfunction.
- Battery ages or the discharging time of a battery is noticeably shorter than that indicated in the specifications.
- Battery lifespan has expired.

Dispose of used batteries promptly and follow local government regulations in an environmentally-responsible manner.

## 18 Care, Cleaning

### 18.1 Description

In this chapter we only describe cleaning and disinfection of the main unit. For the cleaning and disinfection of reusable accessories, refer to instructions for use of corresponding accessories.

### 18.2 Safety Information



#### WARNING

- Use only the substances approved by us and methods listed in this chapter to clean or disinfect your equipment. Warranty does not cover damage caused by unapproved substances or methods.
- Do not mix disinfecting solutions (such as bleach and ammonia) as hazardous gases may result.
- We make no claims regarding the efficacy of the listed chemicals or methods as a means for controlling infection. For the method to control infection, consult your hospital's Infection Control Officer or Epidemiologist.
- The responsible hospital or institution shall carry out all cleaning and disinfection procedure specified in this chapter.



#### CAUTION

- Do not immerse part of the equipment into liquid.
- Any contact of disinfectant solutions with metal parts may cause corrosion.
- Do not allow liquid to enter the case.
- If you spill liquid on the equipment or accessories, please disconnect from power, erase the liquid and contact us or your service personnel immediately.
- Never use abrasive materials (such as steel wool or silver polish), or erosive cleaners (such as acetone or acetone-based cleaners).
- Dilute and use cleaning and disinfecting agents following instructions specified in product manual.
- After cleaning and disinfection, check the equipment carefully. Do not use if you see signs of deterioration or damage.

## 18.3 Cleaning

Your equipment should be cleaned on a regular basis. If there is heavy pollution or lots of dust and sand in your place, the equipment should be cleaned more frequently. Before cleaning the equipment, consult your hospital's regulations for cleaning the equipment.

Recommended **cleaning agents** are:

- Mild soap (diluted)
- Ammonia (diluted)
- Sodium hypochlorite bleach (diluted)
- Hydrogen peroxide (3%)
- Ethanol (70%)
- Isopropanol (70%)

To **clean your equipment**, follow these rules:

1. Shut down the patient monitor and disconnect it from the power line.
2. Clean the display screen using a soft, clean cloth dampened with a glass cleaner.
3. Clean the exterior surface of the equipment using a soft cloth dampened with the cleaner.
4. Wipe off all the cleaning solution with a dry cloth after cleaning if necessary.
5. Dry your equipment in a ventilated, cool place.

## 18.4 Disinfecting

Disinfection may cause damage to the equipment and is therefore not recommended for this patient monitor unless otherwise indicated in your hospital's servicing schedule. Cleaning equipment before disinfecting is recommended.

The recommended disinfectants include: ethanol 70%, isopropanol 70%, glutaraldehyde-type 2% liquid disinfectants

---



### NOTE

---

- Never use EtO or formaldehyde for disinfection.

---

## 19 Maintenance

### 19.1 Description

Regular maintenance of equipment and accessories is the key to ensure the normal operation of equipment. This chapter introduces the inspection and testing methods of the equipment.

### 19.2 Safety Information

#### WARNING

- Failure on the part of the responsible individual hospital or institution employing the use of this equipment to implement a satisfactory maintenance schedule may cause undue equipment failure, possible health hazards, and may endanger personal safety.
- The safety checks or maintenance involving any disassembly of the equipment should be performed by professional servicing personnel. Otherwise, undue equipment failure and possible health hazards could result.
- Personnel that is responsible for maintain this equipment must be qualified and familiar with the operation of the product.
- Do not disassemble the battery, store it in an environment above 60°C, incinerate it or short-circuit it, as these may cause battery burning, explosion, leakage or overheating, and serious injury or death could result.
- No changes should be made to this device itself.
- 为防止漏电流导致的电击,当发现本监护仪外壳破损后请停止使用。请联系维修人员处理。
- 使用本设备的医院或医疗机构应当建立完善的维护计划,否则可能造成设备失效和不可预期的后果,并可能危及人身安全。
- 不得自行对本设备进行更改。
- 本设备不含用户可维修部件。如需要维修请联系维修人员。
- 所有需要拆卸设备进行安全检查或维修工作应该由专业维修人员进行,非专业人员的操作可能造成设备失效,并可能危及人身安全。
- 请勿拆解电池,将其置于高于60°C的环境中或焚毁电池或使其短路。这样可能导致电池燃烧、爆炸、泄漏或发烫,造成人身伤害。
- 本设备维修人员必须具有合格的资质,并熟悉产品操作。



## CAUTION

---

- Maintenance and conditioning of the monitor are not allowed when the patient is monitored.
- If you discover a problem with any of the equipment, contact your service personnel or us.
- Do not use or store equipment outside the specified temperature, humidity, or altitude ranges.
- Disposal of packaging materials must comply with local regulations or the hospital's waste disposal policy.
- When the equipment and its accessories have reached the expiration date, they must be disposed of in accordance with local regulations. If you have any questions regarding the disposal, please contact our company.

---

---



## NOTE

---

- 如有必要, 请联系我公司获取产品电路图、部件清单、校准说明或其它设备维修相关的信息。

---

Before every use, after your patient monitor has been used for 6 to 12 months, or whenever your patient monitor is repaired or upgraded, a thorough inspection should be performed by qualified service personnel to ensure the reliability.

Follow these guidelines when inspecting the equipment:

- Make sure that the environment and power supply meet the requirements.
- Inspect the equipment and its accessories for mechanical damage.
- Inspect all power cords for damage, and make sure that their insulation is in good condition.
- Make sure that only specified accessories are applied.
- Inspect if the alarm system functions correctly.
- Make sure that the batteries meet the performance requirements.
- Make sure that the patient monitor is in good working condition.
- Make sure that the grounding resistance and leakage current meet the requirement.

In case of any damage or abnormality, do not use the patient monitor. Contact the hospital's biomedical engineers or your service personnel immediately.

## 19.3 Maintenance Plan

Ensure that maintenance tasks are performed in accordance with the maintenance plan or

local regulations. Before testing and maintenance, the equipment must be cleaned and disinfected.

Test and maintenance items and frequencies of recommend are as follows:

Test / maintenance items	Frequency of recommend	
Performance Testing		
Visual inspection	Before first use every day	
Parameter module performance test and calibration	1. When the user suspects that the measured value is inaccurate; 2. After maintenance or replacement of relevant modules; 3. Other modules shall be at least every two years.	
Security Testing		
Select test items based on the requirements of IEC60601-1	1. When the power module is repaired or replaced; 2. After the monitor falls; 3. At least once every two years or as required.	
Other Tests		
Startup inspection	Before each use	
Battery check	Functional testing	1. During the first installation; 2. After battery replacement.
	Performance testing	Every three months or when the running time of the battery is significantly reduced

## 19.4 Checking Version Information

监护仪维护时您可能需要监护仪和模块的版本信息。

选择【主菜单 (Main Menu)】热键→从【系统 (System)】列选择【关于 (About)】

查看系统软件版本信息。可以查看内核版本、系统版本、软件版本，模块软件和硬件版本。

You may be asked for information on monitor and module version.

To view system software version information, select the **Main Menu** quick key →from the **System** column select **About**.

You can check system kernel version, system version, software version, module hardware and software version.

## 19.5 Test methods and steps

Except for the following maintenance tasks, all testing and maintenance can only be completed by professional maintenance personnel approved by the company.

- Routine inspection, including visual inspection and startup inspection
- Battery inspection

When other tests and maintenance are required, please contact the maintenance

---

personnel in time.

### 19.5.1 Visual Inspection

Check the appearance of the equipment before use every day. In case of damage or failure of equipment and accessories, please stop using immediately and contact the equipment engineer of the hospital or the maintenance personnel of the company.

Visual inspection includes the following items:

- The environment and power supply meet the requirements
- The equipment shell shall be free of stains, and the panel and display screen shall not be broken or damaged
- The power supply is free of wear and has good insulation performance
- The interface, plug and cable shall be free from damage and winding
- Firmly connect the module and cable to the equipment

### 19.5.2 Startup Inspection

the monitor performs self-test after startup, and the startup inspection items are as follows:

- The equipment can be started normally
- Alarm system works normally
- The equipment displays normally

### 19.5.3 Battery check

Refer to 17.6.2 check battery performance.

## 19.6 Waste monitor

After the equipment reaches its service life, please dispose of the monitor and accessories according to local regulations.

---

---



### Warning

---

---

- For the disposal of components and accessories, if there are no corresponding regulations, the local regulations on the disposal of hospital waste can be followed.

---

---

## 20 Accessories

All accessories listed in this chapter meet the requirements of IEC 60601-1-2 when used with a monitor. Accessory materials in contact with the patient have been tested for biocompatibility and verified to meet the requirements of ISO 10993-1. Detailed information on accessories can be found in the relevant accessory manual.



### WARNING

- Use accessories specified in this chapter. Using other accessories may cause damage to the patient monitor or not meet the claimed specifications.
- The accessories should be used with this monitor only. It is the responsibility of the user to read this manual carefully (including accessories) or contact us to confirm the compatibility of the accessories with the device prior to use. Failure to do so may cause injury to patient.
- Single-use accessories are not designed to be reused. Reuse may cause a risk of contamination and affect the measurement accuracy.



### NOTE

- If accessories are used or stored outside of the specified temperature or humidity range, its performance may not reach the specifications claimed by this manual.
- Check the accessories and their packages for any sign of damage. Do not use them if any damage is detected.
- Do not use the expired accessories.
- Disposal of single-use accessories must comply with local regulations or hospital waste disposal policy.

See the accessory identification label for accessory information. If you need to buy, please contact the sales agent.

### 20.1 ECG Accessories

Name	Model	Patient Category	Remark	Manufacturer
Single use electrode	YY-W55	Adult	/	Qingdao Bright Medical Manufacturing Co Ltd

Name	Model	Type	Patient Category	Remark	Length	Manufacturer
Leadwire	M0202233	Clip Reusable	Adult	Individual set leads,3-lead	3.6m	Qingdao Bright Medical Manufacturing Co Ltd
	M0202232		Adult	Individual set leads,5-lead		
	M0202221	Snap Reusable	Adult	Integrated leads,5-lead		
	M0202227		Neonate	Individual set leads,3-lead		
	M0202222		Adult	Integrated leads,3-lead		

## 20.2 SpO<sub>2</sub> Accessories

Name	Model	Type	Patient Category	Remark	Manufacturer
Extension Cable	M05110 27	Reusable	Adult, Pediatric, Neonate	Length 3m	Qingdao Bright Medical Manufacturing Co Ltd

Name	Model	Type	Patient Category	Remark	Manufacturer
SpO <sub>2</sub> Sensors	DP400N /A-0901 03	Single use	Adult/ Neonate	Suitable for BCI module Length 1.6m	Beijing Rongrui-Century Science & Technology Co., Ltd.
	RSJ001 DA	Reusable	Adult		
	RSY001 DN		Neonate		

Wavelength emitted by pulse oximetry probe is 600 ~ 1000nm, The maximum photic output consumption of the sensor is less than 18 mW.

The information about the wavelength range and maximum photic output consumption can be especially useful to clinicians, for example, clinicians performing photodynamic therapy.

## 20.3 NIBP Accessories

Name	Model	Type	Patient Category	Remark	Manufacturer
Tubing	L340	Reusable	Adult, Pediatric, Neonate	Length 3.4m	Wuhan Infinium Electronics Co., Ltd.

Name	Model	Type	Patient Category	Remark	Manufacturer
Cuff	LF1101S	Reusable	Neonate	/	Lifemed Co., Ltd
	LF1102S		Pediatric		
	LF1103S		Adult		
	LF1204S		Adult		

## 20.4 Temp Accessories

Name	Model	Type	Patient Categor	Remark	Length	Manufacturer
Temp Probes	A-MR-01	Reusable	Adult	Esophageal/Rectal	3m	APK IMAGE CO., LTD
	A-MR-03		Adult	Skin		

## 20.5 IBP Accessories

Name	Model	Type	Patient	Remark	Manufacturer
IBP Cable	M0511023	Reusable	Adult	Length 3.1m	Qingdao Bright Medical Manufacturing Co., Ltd
IBP Sensor	SCW-Y-01	Disposable	Adult	/	SCW Medical LTD.

## 20.6 Other Accessories

Name	Model	Type	Patient Category	Remark	Manufacturer
Lithium battery	JQ146-03L	Reusable	/	/	ShenZhen New Light Energy Technology Co., Ltd
Direct power cord	/	/	/	Length 2m	/
Adapter power cord	/	/	/	Length 1m	/

## A Specifications

### A.1 Safety Specifications

#### A.1.1 Classifications

The patient monitor is classified, according to IEC60601-1:

Type of protection against electrical shock	I
Degree of protection against electrical shock	CF: ECG, NIBP, TEMP, IBP, SpO2
Mode of operation	Continuous
Degree of protection against harmful ingress of water	TM1Host: IPX2 Portable Handle and Expansion Base: IPX1
Mobile type	Portable

#### A.1.2 Environmental Specifications

Item	Temperature (°C)	Relative humidity	Barometric (kPa)
Operating conditions	5°C~40°C	15%~95%	80kPa~105kPa
Storage conditions	-20°C~55°C	10%~95%	80kPa~105kPa



#### WARNING

- Operation within the specified environmental specifications is a must. Otherwise, it may cause damage to the patient monitor or not meet the claimed specifications. If aging or any performance change that results from the environment condition, please contact the service personnel.



#### NOTE

- Unspecified modules' environment specifications are the same with the main unit's.

## A.2 Power Supply Specifications

### A.2.1 External AC Power

	Host	Dock	Adapter
AC waveform	/	Sine	Sine
Input Voltage	12V DC	100 ~ 240V	100 ~ 240V
Input Current	2A	1.5 ~ 0.5A	1.0 ~ 0.5A
Frequency	/	50/60 Hz	50/60 Hz

### A.2.2 Battery

W × D × H	145mm × 64mm × 21.5mm
Weight	340g
Type	Lithium-ion battery, rechargeable
Rated Voltage	10.89V DC
Volume	5200 mAh
Run Time	More than 2h in continuous operation (For new, fully-charge battery, with ambient temperature: 25°C)
Charge Time	Monitor ON or OFF: Charge 90% within 4 hours and full within 5 hours

## A.3 Physical specifications

Name	Model	Weight	Dimensions
Main Unit	TM1		
Battery	XHL18650-2S		
Dock	Dock		

## A.4 Hardware Specification

### A.4.1 Display Specification

Screen Type	TFT-LCD
Screen Size	12.5 inch
Resolution	1366x768 @ 60hz ( 24bit Colors )

#### A.4.2 LEDs on Main Units

Alarm Lamp	1 (3 colors: red, yellow, blue)
AC Power Indicator	1 (green)
Battery Status Indicator	1 (green)

#### A.4.3 Audio Indicator

Speaker	Give alarm tones (45 to 85 dB), reminder tones, key tones, QRS tones; Support PITCH TONE and multi-level tone modulation; alarm tones comply with IEC 60601-1-8.
---------	---

#### A.4.4 Interface

##### A.4.4.1 Interface of the Main Unit

DC power input connector	1
Multifunctional connector	1
Multi-pin connector	1
Communication interface	1
Infrared filter	1
Contact	2

##### A.4.4.2 Interface of the Dock

AC power input connector	1
Ethernet Port	1 1000M Ethernet port
USB	2 USB2.0 port
HDMI Port	1 HDMI 1.4 port
Equipotential End	1
Multi-pin connector	1
Host monitor connector	1
Infrared filter	1
Contact	2 个

#### A.4.5 Signal Outputs Specifications

Alarm output	
Alarm signal sound pressure level range	40 dB(A) to 80 dB(A) within a range of one meter

#### A.5 Software Specifications

General Specifications	
Channel	Up to 8 Channels are displayed.
Layout	<ol style="list-style-type: none"> <li>1) Up to 12 physiological parameters supported</li> <li>2) Waveform parameter customization</li> <li>3) Waveform area dynamic setup</li> <li>4) 32 sets of colors</li> <li>5) 2 display modes:           <ul style="list-style-type: none"> <li>● Normal View</li> <li>● Big Font View</li> </ul> </li> </ol>
Internal Storage	8 GB storage, usable size is 4.5GB
External File System	USB Flash Disk, FAT32 and NTFS format supported
Brightness	6 levels. Adjustable range is 0~5, 0 is the darkest, 5 is the brightest. Default setting is 3. Night mode brightness level is 0.
Sound Volume	6 levels. Adjustable range is OFF and 1~5, choose OFF to silence the audio, level 5 is the highest volume. Default setting is 2.
System Time	<p>24H/12H format supported:            24H: YYYY/MM/DD HH:MM            12H: YYYY/MM/DD H:MM AM/PM</p> <p>Turn on automatic synchronization, when the monitor is connected to WLAN. Time is automatically synchronized with network time.</p>
USB Extension	USB Keyboard USB Mouse USB Flash Disk <ul style="list-style-type: none"> <li>● USB Code Scanner</li> <li>● USB Hub (supported, connection with too many devices is not recommended)</li> </ul>
Patient Information Management	
Patient Setup	Supported, indexed with patient ID.
Trend Data Saving	<ul style="list-style-type: none"> <li>● 5×24h Parameter data saving</li> <li>● Waveform recording (ECG, SpO2, IBP, RESP etc.), 16s duration</li> </ul>

User's Manual for TM1 Patient Monitor

	per waveform.
Patient Review	Patient information display supported Sorting by time supported
Data Export	USB Flash Disk exportation supported Exportation through DataManager application within WLAN connection supported
Data Protection/ Deletion	<ul style="list-style-type: none"> <li>● Data protection supported to avoid accidental deletion or overwritten</li> <li>● Deletion confirmation window to avoid accidental deletion.</li> </ul>
Management Capacity	20 patient information sets at most
<b>Module Setup Management</b>	
General Module	ECG module Resp module Temp module SpO2module NIBP module IBP module
Config Manager	Up to 30 configurations supported.
Configuration Export/Import	Yes
Ethernet Setup	IPv4 address supported, DHCP and Static IP supported. The system default is DHCP.
WIFI	<ol style="list-style-type: none"> <li>1) WIFI SSID Scanning</li> <li>2) WIFI non-encryption/encryption connection supported, security certificates are:           <ul style="list-style-type: none"> <li>● WPA-PSK (recommended)</li> <li>● WPA2-PSK recommended)</li> <li>● WEP</li> </ul> </li> </ol> <p><b>Once connected, the system will save the password and connect to the WIFI automatically.</b></p>
WIFI Setup	IPv4 address supported, the system default is DHCP.
<b>Alarm Management</b>	
Alarm Levels	<p>Classified into 3 levels:</p> <ul style="list-style-type: none"> <li>● High: Flashing red with 2Hz frequency (twice per second)</li> <li>● Medium: Flashing yellow with 1Hz frequency (once per second)</li> <li>● Low: Solid blue</li> </ul> <p>You can set alarm sound type and alarm interval</p>

User's Manual for TM1 Patient Monitor

Physiological Parameters	HR, PVCs, ST, ARR, RR, TP, SpO2, PR, PI(Masimo), NIBP-SYS, NIBP-DIA, IBP-ART-SYS, IBP-ART-DIA, IBP-PA-SYS, IBP-PA-DIA, IBP-CVP-MAP, IBP-RAP-MAP, IBP-LAP-MAP, IBP-ICP-MAP
Physiological Alarm Events Recordings	<p>Physiological Alarm can trigger the recording the waveform when the alarm event occurs. You can turn off the trigger function.</p> <p>Event recordings are:</p> <ol style="list-style-type: none"> <li>1. 16s waveform data (8s respectively before and after the alarm event occurring moment)</li> <li>2. Physiological measurement data</li> </ol>
Physiological Alarm List	<p>Summary of current physiological alarms for review.</p> <p>Summary of history alarms for a specific parameter in Alarm Review, capacity: 100 sets.</p>
Physiological Alarm	Sensor Off, Low Battery, Hardware malfunction, Module Disconnection, Signal out of range
Technical Alarm List	<p>Current technical alarm list for review.</p> <p>History alarm list for technical alarms in Alarm Review, <b>Capacity:</b> 100 sets.</p>
<b>Data Communication</b>	
View Other Monitored Patients	<p>Searching and remote view patient monitors within the same network are supported</p> <p>Patient Monitor ↔ Patient Monitor</p>
Health Level 7 Standards	<ol style="list-style-type: none"> <li>1、 HL7 two-way communication supported</li> <li>2、 HL7 patient management supported</li> <li>3、 HL7 view report</li> </ol> <p>For more information about the HL7 standards process, please refer to the HL7 standards process document that we provide</p>
Data Transmission	<p>Data export/import mode through network supported</p> <p>Exportation content: Patient data and config</p> <p>Importation content: Config</p>
History Patient Data Export	<p>Installation of our DataManager software on PC allows you to view historical patient data stored in different devices within the LAN.</p> <p>When the DataManager Service is enabled on the monitor, your PC can connect to the monitor through the DataManager software and export the history patient data from the device, including measurement data and alarm recordings.</p>
<b>Smart Upgrade</b>	

System Firmware Upgrade	Yes
Automated Upgrade by Network	Yes

## A.6 Measurement Specifications

### A.6.1 ECG

ECG	
Standards	ANSI-AAMI EC13, IEC 6061-2-27:2011
Lead Set	3-lead: I, II, III 5-lead: I, II, III, AVR, AVF, AVL, V
ECG Standard	IEC
Display Sensitivity	Gain: 2.5mm/mV ( $\times 0.25$ ), 5mm/mV ( $\times 0.5$ ), 10mm/mV ( $\times 1$ ), 20mm/mV ( $\times 2$ ); error $\leq \pm 10\%$
Speed	12.5 mm/s, 25 mm/s, 50 mm/s; error $\leq \pm 5\%$
Mode	Diagnostic mode Monitor mode Surgical mode
Common Mode Rejection Ratio (With Notch Off)	>90dB
Notch	Diagnostic mode: Notch is 50/60Hz, nonadjustable Monitor and surgical mode: 50Hz/60 Hz/OFF, manual adjustment
Differential Input Impedance	$\geq 5M\Omega$
Accuracy of Reappearing Input Signal	Use A and B methods based on EC13 or IEC60601-2-27 to determine system total error and frequency response.
Electrode Offset Potential Tolerance	$\leq \pm 300\text{mV}$
Lead-off Detection Current	Measuring electrode: $< 0.1\mu\text{A}$ Drive electrode: $< 1\mu\text{A}$
Baseline Recovery Time	$< 5\text{s}$
Patient Leakage Current	$< 10\mu\text{A}$
Calibration Signal	1mV (peak-to-peak value) $\pm 10\%$
ESU Protection	Cut mode: 300W Coagulate mode: 100W Recovery time: $\leq 10\text{s}$
PACE Pulse	

User's Manual for TM1 Patient Monitor

Pace Pulse Markers	Pace pulses meeting the following conditions are labeled with a PACE marker:  Amplitude: $\pm 2$ to $\pm 700$ mV Width: 0.1 to 2 ms Rise time: 10 to 100 $\mu$ s
Pace Pulse Rejection	When tested in accordance with the ANSI/AAMI EC13-2002: Sections 4.1.4.1 and 4.1.4.3, the heart rate meter rejects all pulses meeting the following conditions.  Amplitude: $\pm 2$ to $\pm 700$ mV Width: 0.1 to 2 ms Rise time: 10 to 100 $\mu$ s
Pacemaker Pulse Rejection of Fast ECG Signals	25V/s $\pm 15\%$ RTI
<b>HR</b>	
Measurement Range	30bpm~300bpm
Resolution	1bpm
Accuracy	$\pm 1$ bpm or $\pm 1\%$ , whichever is greater.
HR Averaging Method	In compliance with the requirements in Clause 4.1.2.1 d) of ANSI/AAMI EC13-2002, the following method is used:  the 4 most recent RR intervals are averaged to compute the HR.  The HR value displayed on the monitor screen is updated every second.
Response to Irregular Rhythm	In compliance with the requirements in Clause 4.1.2.1 e) of ANSI/AAMI EC13-2002,  the heart rate after 20 seconds of stabilization is displayed as follows:  Ventricular bigeminy (3a): $-80 \pm 1$ bpm Slow alternating ventricular bigeminy (3b): $-60 \pm 1$ bpm Rapid alternating ventricular bigeminy (3c): $-120 \pm 1$ bpm Bidirectional systoles (3d): $-90 \pm 2$ bpm
Response Time to Heart Rate Change	From 80 to 120bpm: less than 12 s From 80 to 40bpm: less than 12s
Response to Tachycardia	$\leq 12$ s
Tall T-Wave Rejection Capability	When the test is performed based on part 4.1.2.1 c) of

User's Manual for TM1 Patient Monitor

	ANSI/AAMI EC 13-2002, the heart rate meter will reject all 100 ms QRS complexes with less than 0.8 mV of amplitude, and T waves with T-wave interval of 180 ms and those with Q-T interval of 350 ms.
<b>ST Segment Analysis</b>	
Measurement Range	-2.00mV ~ +2.00mV
Resolution	0.01mV
Accuracy	±15% or ±0.05mV whichever is greater
<b>Arrhythmia</b>	
Asystole (ASY)	Yes
Fibrillation (FIB)	Yes
Ventricular Tachycardia (VTA)	Yes
R On T (ROT)	Yes
Ventricular Run (RUN)	Yes
Ventricular Triplet (TPT)	Yes
Ventricular Couplet (CPT)	Yes
Ventricular Premature Beat (VPB)	Yes
Bigeminy (BGM)	Yes
Trigeminy (TGM)	Yes
Tachycardia (TAC)	Yes
Bradycardia (BRD)	Yes
Missed Beat (MIS)	Yes
<b>Alarm Limit</b>	
HR Alarm High	(Low limit + 2) ~300 bpm Default value: 130 bpm (Adult) 160bpm (Pediatric) 200bpm (Neonate)
HR Alarm Low	30~ (high limit - 2) bpm Default value: 50bpm (Adult) 75bpm (Pediatric) 100 bpm (Neonate)
ST Alarm High	(Low limit - 0.20) ~ 2.00mV Default value: 0.30mV
ST Alarm Low	-2.00~ (high limit - 0.20) mV

	Default value: -0.30mV
--	------------------------

### A.6.2 Resp

Resp	
Technique	Trans-thoracic impedance
Lead	Lead II
Resp Measurement Range	0rpm~120rpm
Resolution	1rpm
Accuracy	7rpm~120rpm: $\leq \pm 2\text{rpm}$ 0rpm~6rpm: Not specified
Speed	6.25mm/s, 12.5mm/s, 25.0mm/s
Display Gain	$\times 0.25$ , $\times 0.5$ , $\times 1.0$ , $\times 2.0$
Apnea Alarm Delay	10s~60s, Default value: 20s
Alarm Limit	
RR High	(Low limit + 2) ~120 rpm Default value: 30rpm
RR Low	0~(high limit -2) rpm Default value: 6rpm

### A.6.3 Temp

Temp		
Standard	ISO 80601-2-56:2018	
Measurement method	Thermal Resistance	
Operating mode	Direct mode	
Measurement range	0°C~50°C (32°F~122°F)	
Resolution	0.1°C	
Unit	°C/°F	
Error	Temp range	Error
	0°C~34.9°C	±0.2°C
	35.0°C~39.9°C	±0.1°C
	40.0°C~44.9°C	±0.2°C
	45.0°C~50.0°C	±0.3°C
Channel	2 channels	

User's Manual for TM1 Patient Monitor

Minimum time for accurate measurement	Body surface: <100 s Body cavity: <80 s
Refreshing rate	1s
Temp Difference Calculation	Yes
<b>Alarm Limit</b>	
T1/T2 Alarm High	(Low limit + 1) ~50°C Default value: 38.0°C
T1/T2 Alarm Low	0~ (high limit - 1) °C Default value: 36.0°C
△T High	0~50°C Default value: 2.0°C

#### A.6.4 SpO2

<b>General Specification</b>	
Standard	ISO 80601-2-61:2017
<p>*Measurement accuracy verification: The SpO2 accuracy has been verified in human experiments by comparing with arterial blood sample reference measured with a CO-oximeter. Pulse oximeter measurements are statistically distributed and about two-thirds of the measurements are expected to come within the specified accuracy range compared to CO-oximeter measurements.</p>	
SpO2	
Measurement Range	0%~100%
Resolution	1%
Accuracy	70%~100%: $\leq\pm 2\%$ 0%~69%: Not specified
Speed	12.5mm/s, 25.0mm/s
Refreshing Rate	1s
Response time	$\leq 30$ s (normal perfusion, no disturbance, SpO2 value sudden change within 70% – 100%)
Low Perfusion Conditions	0.3%~20%
PR	
Measurement Range	30bpm~250bpm
Resolution	1bpm
Accuracy	$\leq\pm 2$ bpm (measured without motion) $\leq\pm 3$ bpm (measured with motion)
Alarm Limit	Range

User's Manual for TM1 Patient Monitor

SpO2 Alarm High	(Low limit + 1) ~100% Default value: 99%
SpO2 Alarm Low	0~(high limit - 1) % Default value: 85%
PR Alarm High	(High limit + 2) ~300bpm
PR Alarm Low	30~(low limit - 2) bpm
SpO2 Alarm Response Time	<b>≤12s</b>

### A.6.5 NIBP

General Specification			
Standard	ISO 80601-2-30:2019		
Measurement Method	Oscillometry		
Mode of Operation	Manual, Auto and STAT		
Auto Mode Repetition Intervals	2min~240min		
Number of STAT Mode Cycle	5		
Total Number of NIBP Listings	1024		
Measurement Type	Adult, Pediatric, Neonate		
Initial Cuff Inflation Pressure	Adult options: 80mmHg 100mmHg 120mmHg 140mmHg 150mmHg 160mmHg <b>180mmHg</b> <b>(Default)</b> 200mmHg 220mmHg 240mmHg	Pediatric options: 80mmHg 100mmHg 120mmHg <b>140mmHg</b> <b>(Default)</b> 160mmHg 180mmHg 200mmHg 220mmHg 240mmHg	Neonate options: 60mmHg 70mmHg 80mmHg <b>100mmHg</b> <b>(Default)</b> 120mmHg
Inflation Memory Mode	Yes		
Alarm Limit			
Sys High	Adult: (low limit + 5) ~270mmHg Pediatric: (low limit + 5) ~230mmHg Neonate: (low limit + 5) ~135mmHg		

User's Manual for TM1 Patient Monitor

	<p>Default value: 160mmHg (Adult) 120mmHg (Pediatric) 90mmHg (Neonate)</p>
Sys Low	<p>40~ (high limit - 5) mmHg Default value: 90mmHg (Adult) 70mmHg (Pediatric) 40mmHg (Neonate)</p>
Día High	<p>Adult: (low limit + 5) ~210mmHg Pediatric: (low limit + 5) ~150mmHg Neonate: (low limit + 5) ~95mmHg Default value: 90mmHg (Adult) 70mmHg (Pediatric) 60mmHg (Neonate)</p>
Dia Low	<p>10~ (high limit - 5) mmHg Default value: 50mmHg (Adult) 40mmHg (Pediatric) 20mmHg (Neonate)</p>
<b>Infinium Module</b>	
Standard	ISO80601-2-30:2019
Measurement Method	Upper arm, Oscillometry
Mode of Operation	Manual, Auto and STAT
Max Measurement Time	180s (Adult/Pediatric) 90s (Neonate)
Static Pressure Measurement Range	0~300mmHg
Accuracy	±3mmHg
Dynamic Pressure Measurement Range	<p><b>Adult:</b> SYS: 40mmHg~270mmHg DIA: 10mmHg~210mmHg</p> <p><b>Pediatric:</b> SYS: 40mmHg~230mmHg DIA: 10mmHg~150mmHg</p> <p><b>Neonate:</b> SYS: 40mmHg~135mmHg</p>

User's Manual for TM1 Patient Monitor

	DIA: 10mmHg~95mmHg
Dynamic Pressure Accuracy	Max mean error: $\pm 5\text{mmHg}$ Max standard deviation: 8mmHg
Resolution	1mmHg
Software Overpressure Protection	Adult: $297\text{mmHg} \pm 3\text{mmHg}$ Pediatric: $237\text{mmHg} \pm 3\text{mmHg}$ Neonate: $147\text{mmHg} \pm 3\text{mmHg}$
PR Measurement Range	40~240bpm
PR Accuracy	2% or $\pm 3\text{bpm}$ , whichever is greater

### A.6.6 IBP

General Specification	
Standard	IEC 60601-2-34:2011
Measurement Method	Direct invasive measurement
Measurement Range	-30mmHg~300mmHg
Resolution	1mmHg
Accuracy	$\geq -10\text{mmHg}$ : $\pm 1\text{mmHg}$ or 2%, whichever is greater $< -10\text{mmHg}$ : $\pm 3\text{mmHg}$ or 4%, whichever is greater
Number Of Channels	2Channels
Zeroing Range	$\leq 120\text{mmHg}$
Excitement Voltage	5V DC, $\pm 2\%$
Sensitivity	5uV/V/mmHg
Impedance Range	$300\Omega \sim 3K\Omega$
Sweep Speed	12.5mm/s, 25.0mm/s
Waveform Scale	-30mmHg~300mmHg, manual input required
Waveform Optimization Mode	Manual / Auto (In manual mode, optimization varies with waveform scale)
Pressure Label	ART (Arterial Blood Pressure) PA (Pulmonary Artery Pressure) CVP (Central Venous Pressure) RAP (Right Arterial Pressure) LAP (Left Arterial Pressure) ICP (Intracranial Pressure)
Alarm Limit	
ART Alarm High	(Low limit + 2) ~300mmHg

User's Manual for TM1 Patient Monitor

	Default value: 150mmHg
ART Alarm Low	0~ (high - 2) mmHg Default value: 75mmHg
PA Alarm High	(Low limit + 2) ~200mmHg Default value: 90mmHg
PA Alarm Low	-30~ (high limit - 2) mmHg Default value: 60mmHg
CVP/RAP/LAP/ICP Alarm High	(Low limit + 2) ~60mmHg Default value: 30mmHg
CVP/RAP/LAP/ICP Alarm Low	-30~ (high limit - 2) mmHg Default value: 10mmHg

## B Factory Defaults

### B.1 ECG, Arrhythmia, ST Factory Default Settings

#### B.1.1 ECG Setup

ECG Setup	Factory Default Settings				
HR	Alarm ON/OFF		ON		
	Alarm High	Adult	130bpm		
		Pediatric	160bpm		
		Neonate	200bpm		
	Alarm Low	Adult	50bpm		
		Pediatric	75bpm		
		Neonate	100bpm		
	Alarm Level	Medium			
	Alarm Record	OFF			
	Alarm Source	HR			
Color					
Speed	25.0 mm/s				
ECG Gain	×1.0				
Lead Set	5-lead				
ECG Filter	Monitor				
ECG Notch	50Hz/60Hz				
ECG Cascade	ON				
Paced	OFF				

#### B.1.2 Arrhythmia Alarm Setup

User's Manual for TM1 Patient Monitor

Item	Alarm ON/OFF	Alarm Level	Alarm Record
ASY	ON	High	ON
FIB	ON	High	OFF
VTA	ON	High	OFF
ROT	ON	Medium	OFF
RUN	ON	Medium	OFF
TPT	ON	Medium	OFF
CPT	ON	Medium	OFF
PVC	ON	Medium	OFF
BGM	ON	Medium	OFF
TGM	ON	Medium	OFF
TAC	ON	Medium	OFF
BRD	ON	Medium	OFF
MIS	ON	Medium	OFF

### B.1.3 ST Segment Setup

Item	Factory Default Settings	
ST Alarm Mode	Real-time	
ST-I, ST-II, ST-III, ST-aVR ST-aVL, ST-aVF, ST-V	Alarm ON/OFF	ON
	Alarm High	0.30mV
	Alarm Low	-0.30mV
	Alarm Level	Medium
	Alarm Record	OFF
ST Analysis	ON	
ST Segment	Auto	
ST Point	J+40ms	
ST Point adjustment	ON	
ISO Point	-105ms	
J Point	180ms	

### B.2 Resp Setup

Item	Factory Default Settings	
RR	Alarm ON/OFF	ON
	Alarm High	Adult 30rpm
		Pediatric 30rpm
		Neonate 100rpm

User's Manual for TM1 Patient Monitor

	Alarm Low	Adult	8rpm
		Pediatric	8rpm
		Neonate	30rpm
	Alarm Level	Medium	
	Alarm Record	OFF	
Apnea	Alarm ON/OFF	ON (Cannot be set)	
	Alarm Level	High (Cannot be set)	
	Alarm Record	ON (Cannot be set)	
RR Source		Resp	
Color			
Speed		6.25mm/s	
Gain		×1.0	

### B.3 SpO2 Setup

Item	Factory Default Settings		
SpO2	Alarm ON/OFF	ON	
	Alarm High	99%	
	Alarm Low	85%	
	Alarm Level	Medium	
	Alarm Record	OFF	
PR	Alarm ON/OFF	ON	
	Alarm High	Adult	130bpm
		Pediatric	160bpm
		Neonate	200bpm
	Alarm Low	Adult	50bpm
		Pediatric	75bpm
		Neonate	100bpm
	Alarm Level	Medium	
	Alarm Record	OFF	
Color			
Speed		12.5mm/s	
PR Source		SpO2	

### B.4 Temp Setup

Item	Factory Default Settings	
T1/T2	Alarm ON/OFF	ON

User's Manual for TM1 Patient Monitor

	Alarm High	38°C
	Alarm Low	36°C
	Alarm Level	Medium
	Alarm Record	OFF
△T	Alarm ON/OFF	ON
	Alarm High	2.0°C
	Alarm Level	Medium
	Alarm Record	OFF
Color		White
Temperature Unit		°C

## B.5 NIBP Setup

Item	Factory Default Settings		
NIBP-SYS	Alarm ON/OFF	ON	
	Alarm High	Adult	160mmHg
		Pediatric	120mmHg
		Neonate	90mmHg
	Alarm Low	Adult	90mmHg
		Pediatric	70mmHg
		Neonate	40mmHg
NIBP-DIA	Alarm Level	Medium	
	Alarm Record	OFF	
	Alarm ON/OFF	ON	
	Alarm High	Adult	90mmHg
		Pediatric	70mmHg
		Neonate	60mmHg
	Alarm Low	Adult	50mmHg
		Pediatric	40mmHg
		Neonate	20mmHg
	Alarm Level	Medium	
	Alarm Record	OFF	
	Color		
	Pressure Unit	mmHg	
	Mode of Operation	Manual	
	Initial Pressure	Adult	180mmHg
		Pediatric	140mmHg

	Neonate	100mmHg
--	---------	---------

## B.6 IBP Setup

Item	Factory Default Settings		
IBP-SYS	Alarm ON/OFF		ON
	ART	Alarm High	150mmHg
		Alarm Low	75mmHg
	PA	Alarm High	90mmHg
		Alarm Low	60mmHg
	Alarm Level		Medium
	Alarm Record		OFF
IBP-DIA	Alarm ON/OFF		ON
	ART	Alarm High	90 mmHg
		Alarm Low	60 mmHg
	PA	Alarm High	75 mmHg
		Alarm Low	45 mmHg
	Alarm Level		Medium
	Alarm Record		OFF
IBP-MAP	Alarm ON/OFF		ON
	CVP, RAP	Alarm High	30 mmHg
		Alarm Low	10 mmHg
	Alarm Level		Medium
	Alarm Record		OFF
Color			
Pressure Unit	mmHg		
Speed	25.0mm/s		
Parameter Label	IBP1 — ART IBP2 — PA		
Parameter Ruler	IBP1 — 10~150mmHg IBP2 — 10~75mmHg		

## C Alarm Messages

### C.1 Physiological Alarm Messages

#### General Physiological Alarm

Alarm Messages	Default Level	Cause and Solution
XXX Too High	Medium	XX value has risen above the high alarm limit or fallen below the low alarm limit. Check the patient's condition and check if the patient category and alarm limit settings are correct.
XXX Too Low	Medium	
Resp Apnea	High	Patient can't respirate or the respiration signal was so weak that the monitor cannot perform respiration analysis. Check the patient's Condition, electrode placement and the Resp connections.

Note: XXX represents Physiological parameter, like HR, ST, RR, SpO2, PR, ART-SYS, ART-DIA etc.

#### Arrhythmia Alarm messages

Alarm Messages	Default Level
Asystole	High
V-Fib/V-Tach	High
V-Tach	High
R on T	Medium
RUN	Medium
Vent Rhythm	Medium
Couplet	Medium

PVC	Medium
Bigeminy	Medium
Trigeminy	Medium
Tachy	Medium
Brady	Medium
Missed Beats	Medium

## C.2 Technical Alarm Messages

Module	Alarm Messages	Default Level	Cause and Solution
ECG	ECG Lead Off	Low	The electrode has become detached from the patient or the lead wire has become disconnected from the adapter cable. Check the connections of the electrodes and leadwires.
	ECG Lead LA Off	Low	
	ECG Lead RA Off	Low	
	ECG Lead LL Off	Low	
	ECG Lead V Off	Low	
	ECG Lead V2 Off	Low	
	ECG Lead V3 Off	Low	
	ECG Lead V4 Off	Low	
	ECG Lead V5 Off	Low	
	ECG Lead V6 Off	Low	
SpO2	ECG Invalid Signal	Medium	Electrode-to-Skin Impedance too high, and reposition the electrode.
	HR Overrange	Medium	If HR>300bpm, Check patient's condition.
	SpO2 Sensor Off	Low	The SpO2 sensor has become detached from the patient or the module, check the connection. If the alarm persists, replace it with a new sensor.
	SpO2 Sensor Fault	Low	Troubleshoot the problem with instructions specified by the
	SpO2 No Sensor	Low	

User's Manual for TM1 Patient Monitor

	SpO2 Unrecognized Sensor	Low	manual that comes with Masimo SpO2 module.
	SpO2 Sensor Incompatible	Low	
	SpO2 Too Much Ambient Light	Low	
	SpO2 Low Signal	Low	
	SpO2 Weak Signal	Low	
	SpO2 Weak Pulse	Low	
	SpO2 Interference	Low	
	SpO2 Board Fault	Low	
Temp	TP1 Sensor Off	Low	Check the sensor connections. Reconnect the sensor.
	TP2 Sensor Off	Low	
NIBP	NIBP Self-check Error	Low	Check NIBP module or replace it.
	NIBP Cuff Off	Low	Reconnect the cuff.
	NIBP Loose Cuff or Pneumatic Leak	Low	Check the leakage in cuff or airway.
	NIBP Weak Signal	Low	The patient's pulse is weak or the cuff is loose. Check the patient's condition and change the cuff application site.
	NIBP Overrange	Low	The measured NIBP value is not within the specified range. Check the patient's condition.
	NIBP Excessive Motion	Low	Please keep quiet and remeasure.
	NIBP Overpressure	Low	The NIBP airway may be occluded. Check the airway and measure again. If the alarm persists, replace it with a new sensor.
	NIBP Signal Saturated	Low	The NIBP signal is saturated due to excess motion or other sources.
	NIBP Air Leak	Low	Check the NIBP cuff and pump for leakages.
	NIBP System Error	Low	Re-plug the module or restart the monitor.
	NIBP Timeout	Low	An error occurred during NIBP measurement and therefore the monitor cannot perform analysis correctly.

			Check the patient's condition and NIBP connections, or replace the cuff.
IBP	IBP1 Sensor Off	Low	Check the sensor connection and reconnect the sensor.
	IBP2 Sensor Off	Low	
	IBP3 Sensor Off	Low	
	IBP4 Sensor Off	Low	
Battery	Battery Low	Low	Battery Low, please charge the battery.
	Battery Too Low	High	Battery Too Low, please charge it immediately, otherwise, the monitor will shut down automatically.

## D EMC and Radio Regulatory Compliance

The product is in radio-interference protection class A in accordance with EN55011. The product complies with the requirement of standard EN60601-1-2:2007 “Electromagnetic Compatibility – Medical Electrical Equipment”.



### NOTE

- Using accessories, transducers and cables other than those specified may result in increased electromagnetic emission or decreased electromagnetic immunity of the patient monitoring equipment.
- The device or its components should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the device or its components should be observed to verify normal operation in the configuration in which it will be used.
- The device needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided below.
- Other devices may affect this monitor even though they meet the requirements of CISPR.
- When the inputted signal is below the minimum amplitude provided in technical specifications, erroneous measurements could result.
- Portable and mobile communication devices can affect their performance.
- Other devices containing RF emission may affect this device (e. g., mobile phone, PAD, computer with wireless functionality).

### Monitor Performance Specifications:

User's Manual for TM1 Patient Monitor

Item	Performance Specifications
ECG	HR Range: 30~300bpm 3-lead: I, II, III 5-lead: I, II, III, V, aVR, aVF, aVL Input Signal Range: $\pm 5\text{mV}$
SpO <sub>2</sub>	Measurement Range: 0~100%
NIBP	Measurement Range: Adult: SYS (40~270) mmHg DIA (10~210) mmHg Pediatric: SYS (40~230) mmHg DIA (10~150) mmHg Neonate: SYS (40~135) mmHg DIA (10~95) mmHg Mode of operation: Auto, Manual, STAT
Resp	Measurement Range: 0~120rpm
Temp	Measurement Range: 0~50°C
PR	Measurement Range: 30~250bpm
Display	12.5-inch multi-colored display, Resolution: 1366*768
Operation method	Use touchscreen
Alarm Indicator	Audio alarm, Lamp alarm
Data Communication	Ethernet supported
Power Supply	AC power: 100~220V, 50/60Hz, 1.3~0.5A DC power: Battery power supplied 10.89V/5200mAh Lithium chargeable battery

Guidance and Declaration - Electromagnetic Emissions		
The device is suitable for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.		
Emission tests	Compliance	Electromagnetic Environment - Guidance
Radio frequency (RF) emissions CISPR 11	1 Group	The device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.

RF emissions CISPR 11	Class A	The device is suitable for use in all establishments other than domestic and those indirectly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC61000-3-2	Class A	
Voltage Fluctuations/Flicker Emissions IEC 61000-3-3	Complies	



## WARNING

- This equipment is expected to be operated by medical professionals, as it may cause electromagnetic interference or interfere with other devices in the vicinity. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the equipment or shielding the relevant electromagnetic site.

Guidance and Declaration - Electromagnetic Immunity			
The device is suitable for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.			
Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV differential Mode ±2 kV differential Mode	±1 kV differential Mode ±2 kV differential Mode	Mains power quality should be that of a typical commercial or hospital environment.

### Guidance and Declaration - Electromagnetic Immunity

The device is suitable for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<p>&lt;5 % UT (&gt;95 % dip in UT) for 0.5 cycle</p> <p>40 % UT (60 % dip in UT) for 5 cycles</p> <p>70 % UT (30 % dip in UT) for 25 cycles</p> <p>&lt;5 % UT (&gt;95 % dip in UT) for 5 s</p>	<p>&lt;5 % UT (&gt;95 % dip in UT) for 0.5 cycle</p> <p>40 % UT (60 % dip in UT) for 5 cycles</p> <p>70 % UT (30 % dip in UT) for 25 cycles</p> <p>&lt;5 % UT (&gt;95 % dip in UT) for 5 s</p>	Mains power quality should be that of a typical commercial or hospital environment. If the user of our product requires continued operation during power mains interruptions, it is recommended that our product be powered from an uninterruptible power supply or a battery.
Power frequency (50/60Hz) magnetic Field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at level typical location in a commercial or hospital environment.

Note:  $U_T$  is the AC mains voltage prior to application of the test level.

### Guidance and Declaration - Electromagnetic Immunity

The device is suitable for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.

Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	3 Vrms	<p>Portable and mobile RF communications equipment should be used no closer to any part of the device, including cables, than the recommended separation distance, which can be calculated using the formula applicable to the frequency of the transmitter.</p> <p>The formulas for calculating the recommended separation distance are as follows:</p> $d = 1.2\sqrt{P}$
-------------------------------	-----------------------------	--------	--

User's Manual for TM1 Patient Monitor

<p>Radiated RF IEC 61000-4-3</p> <p>Only ISA CO2 is tested at 20 V/m</p>	<p>3 V/m 80%AM@2Hz 80 MHz to 2.5 GHz</p> <p>20 V/m 80%AM@1kHz 80 MHz to 2.5 GHz</p>	<p>3 V/m</p> <p>20 V/m</p>	<p><math>d = 1.2\sqrt{P}</math> 80 MHz to 800 MHz</p> <p><math>d = 2.3\sqrt{P}</math> 800 MHz to 2.5 GHz</p> <p>Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey <sup>a)</sup>, should be less than the compliance level in each frequency range <sup>b)</sup>. Interference may occur in the vicinity of equipment marked with the following symbol:</p> 
<p><i>[NOTE 1]:</i> At 80 MHz and 800 MHz, the higher frequency range applies.</p> <p><i>[NOTE 2]:</i> These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.</p> <p>a). Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio and TV broadcasters cannot be accurately predicted theoretically. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be conducted. If the measured field strength in the location in which the device is used exceeds the applicable RF compliance level, verify that the device works normally. If you observe abnormal performance, you may need to reorient or relocate the device.</p> <p>b). Over the frequency range of 150 kHz to 80 MHz, field strengths should be less than 3V/m.</p>			

**Recommended Separation Distances between Portable and Mobile RF Communications Equipment and the device**

## User's Manual for TM1 Patient Monitor

The device is suitable for use in an electromagnetic environment in which radiated RF disturbance are controlled. The customer or the user of the device can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the device as recommended below, according to the maximum output power of the communication equipment.

Rated Maximum Output power of Transmitter Watts (W)	Separation distance according to frequency of transmitter [m]		
	150 kHz to 80 MHz	80 MHz to 800 MHz	800 MHz to 2.5 GHz
	$d = 1.2 \sqrt{P}$	$d = 1.2 \sqrt{P}$	$d = 2.3 \sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.20	1.20	2.30
10	3.80	3.80	7.30
100	12.00	12.00	23.00

For transmitters at a maximum output power not listed above, the separation distance can be estimated using the equation in the corresponding column, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

Note 1: From 80 MHz to 800 MHz, the separation distance for the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

## Radio Management Compliance

### RF Parameter

<b>Project</b>	<b>IEEE 802.11b/g/n (2.4G)</b>
<b>Operating Frequency</b>	IEEE 802.11b/g/n(HT20): 2412MHz to 2462MHz IEEE 802.11n(HT40): 2422MHz to 2452MHz
<b>Modulation</b>	IEEE for 802.11b: DSSS(CCK, DQPSK, DBPSK) IEEE for 802.11g: OFDM(64QAM, 16QAM, QPSK, BPSK) IEEE for 802.11n(HT20 and HT40): OFDM (64QAM,

	16QAM, QPSK, BPSK)
<b>Effective Radiation Power (dBm)</b>	<20dBm (Average value) <30dBm (Peak)

## FCC

---



### FCC WARNING

Any Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions:

- (1) This device may not cause harmful interference, and
- (2) this device must accept any interference received, including interference that may cause undesired operation.

Note: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

-Reorient or relocate the receiving antenna.

-Increase the separation between the equipment and receiver.

-Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.

-Consult the dealer or an experienced radio/TV technician for help.

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment. This equipment should be installed and operated with minimum distance 20cm between the radiator & your body.

---

---

# INFINIUM

Infinium Medical Inc.

Website: [www.infiniummedical.com](http://www.infiniummedical.com)

Address: 12151 62nd St North #5 Largo Fl, 33773 USA

Toll Free (US call only): 866-918-8434

International: 1-727-531-8434

Fax: 1-727-531-8436 Infinium Medical Inc.