

## Head Tissue Simulating Liquids

<b>Application</b>	Specific absorption rate according to standards (e.g., IEC 62209-x, IEEE 1528)		
<b>Packaging</b>	Plastic container of 10 liters with nozzle		
<b>Life Time</b>	Life time and stability of the liquid depend on usage, storage, and handling of tissue simulating liquid		
<b>Options</b>	Tissue simulating liquids for frequencies outside the below listed ranges are available upon request (please contact <a href="mailto:info@speag.swiss">info@speag.swiss</a> )		
<b>Head Tissue</b>	Parameters according to IEEE 1528 / IEC 62209-1/ IEC 62209-2 / FCC KDB 865664		
<b>Narrow-Band Solutions (±5% Tolerance)</b>	<b>Product</b>	<b>Test Frequency (MHz)</b>	<b>Main Ingredients</b>
	HSL300V2	300	Water, Sugar
	HSL450V2	450	Water, Sugar
	HSL750V2	750	Water, Sugar
	HSL900V2	835, 900	Water, Sugar
<b>Broad-Band Solutions (±5% Tolerance)</b>	<b>Product</b>	<b>Test Frequency (MHz)</b>	<b>Main Ingredients</b>
	HBBL1350-1850V3	1450 - 1800	Water, Tween
	HBBL1550-1950V3	1750 - 1850	Water, Tween
	HBBL1900-3800V3	1950 - 3000	Water, Tween
	HBBL3500-5800V5	3500 - 5800	Water, Oil
<b>Broad-Band Solutions (±10% Tolerance)</b>	<b>Product</b>	<b>Test Frequency (MHz)</b>	<b>Main Ingredients</b>
	HBBL4-250V3	4 - 250	Water, Tween
	HBBL1350-1850V3	1300 - 1850	Water, Tween
	HBBL1550-1950V3	1550 - 1950	Water, Tween
	HBBL1900-3800V3	1900 - 3800	Water, Tween
	HBBL600-10000V6	600 - 10000	Water, Oil

## Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HBL600-10000V6)
Product No.	SL AAH U16 BD (Batch: 180208-1)
Manufacturer	SPEAG

### Measurement Method

TSL dielectric parameters measured using calibrated DAK probe.

### Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

### Test Condition



Ambient Condition 22°C ; 30% humidity  
 TSL Temperature 22°C  
 Test Date 8-Feb-18  
 Operator WM

### Additional Information

TSL Density  
 TSL Heat-capacity

### Results

	Measured			Target		Diff.to Target [%]	
f [MHz]	e'	e''	sigma	eps	sigma	Δ-eps	Δ-sigma
800	44.1	20.3	0.90	41.7	0.90	5.8	0.3
825	44.1	19.9	0.91	41.6	0.91	6.0	0.4
835	44.1	19.7	0.92	41.5	0.91	6.1	0.9
850	44.0	19.4	0.92	41.5	0.92	6.0	0.4
900	43.9	18.7	0.94	41.5	0.97	5.8	-3.1
1400	42.9	14.9	1.16	40.6	1.18	5.7	-1.6
1450	42.8	14.7	1.18	40.5	1.20	5.7	-1.7
1600	42.6	14.2	1.26	40.3	1.28	5.7	-1.9
1625	42.6	14.1	1.28	40.3	1.30	5.8	-1.4
1640	42.6	14.1	1.29	40.3	1.31	5.8	-1.2
1650	42.5	14.1	1.29	40.2	1.31	5.6	-1.8
1700	42.4	14.0	1.32	40.2	1.34	5.6	-1.6
1750	42.3	13.9	1.35	40.1	1.37	5.5	-1.5
1800	42.3	13.8	1.38	40.0	1.40	5.7	-1.4
1810	42.3	13.8	1.39	40.0	1.40	5.7	-0.7
1825	42.3	13.7	1.40	40.0	1.40	5.7	0.0
1850	42.2	13.7	1.41	40.0	1.40	5.5	0.7
1900	42.1	13.6	1.44	40.0	1.40	5.3	2.9
1950	42.0	13.6	1.47	40.0	1.40	5.0	5.0
2000	42.0	13.5	1.51	40.0	1.40	5.0	7.9
2050	41.9	13.5	1.54	39.9	1.44	5.0	6.6
2100	41.8	13.5	1.57	39.8	1.49	5.0	5.4
2150	41.8	13.5	1.61	39.7	1.53	5.2	5.0
2200	41.7	13.4	1.64	39.6	1.58	5.2	3.9
2250	41.6	13.4	1.68	39.6	1.62	5.2	3.6
2300	41.6	13.4	1.72	39.5	1.67	5.4	3.2
2350	41.5	13.4	1.76	39.4	1.71	5.4	2.9
2400	41.4	13.5	1.80	39.3	1.76	5.4	2.5
2450	41.4	13.5	1.84	39.2	1.80	5.6	2.2
2500	41.3	13.5	1.88	39.1	1.85	5.5	1.4
2550	41.2	13.5	1.92	39.1	1.91	5.4	0.6
2600	41.1	13.6	1.96	39.0	1.96	5.4	-0.2
3500	39.6	14.1	2.75	37.9	2.91	4.3	-5.5
3700	39.2	14.3	2.94	37.7	3.12	4.1	-5.7

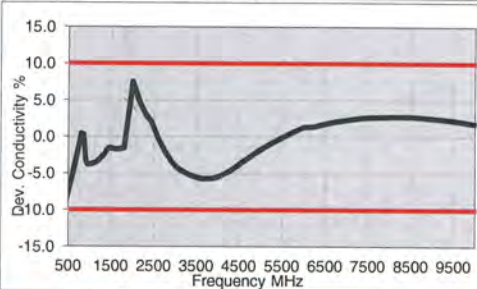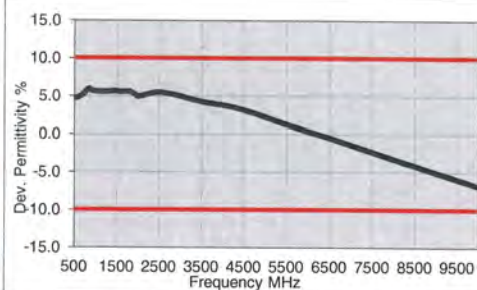

5200	36.7	15.9	4.61	36.0	4.66	1.9	-1.0
5250	36.6	16.0	4.67	35.9	4.71	1.8	-0.9
5300	36.5	16.0	4.72	35.9	4.76	1.7	-0.7
5500	36.1	16.2	4.96	35.6	4.96	1.3	-0.1
5600	35.9	16.3	5.08	35.5	5.07	1.1	0.2
5700	35.7	16.4	5.19	35.4	5.17	0.9	0.5
5800	35.6	16.5	5.31	35.3	5.27	0.8	0.8
6000	35.2	16.6	5.55	35.1	5.48	0.4	1.3
6500	34.3	17.1	6.18	34.5	6.07	-0.5	1.8
7000	33.4	17.5	6.81	33.9	6.65	-1.4	2.3
7500	32.5	17.8	7.43	33.3	7.24	-2.3	2.7
8000	31.7	18.1	8.06	32.7	7.84	-3.2	2.8
8500	30.8	18.4	8.68	32.1	8.45	-4.2	2.8
9000	30.0	18.6	9.31	31.5	9.08	-5.1	2.6
9500	29.1	18.8	9.93	31.0	9.71	-5.9	2.2
10000	28.3	19.0	10.55	30.4	10.36	-6.9	1.8