


Impedance Plot for D450V3-SN:1113


450 Head

Calibrated impedance: $55.7\Omega - 5.3j\Omega$; Measurement impedance: $58.4\Omega + 6.5j\Omega$ (within 5Ω)

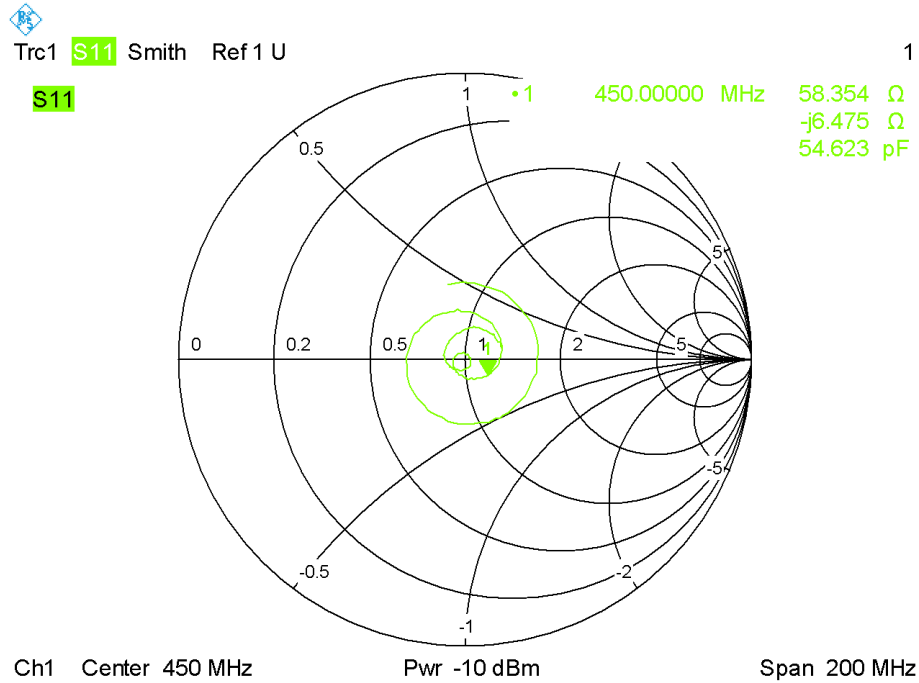

Date: 26.MAY.2023 09:16:28

Calibrated return loss: -22.6dB; Measurement return loss: -22.7dB (within 20%)

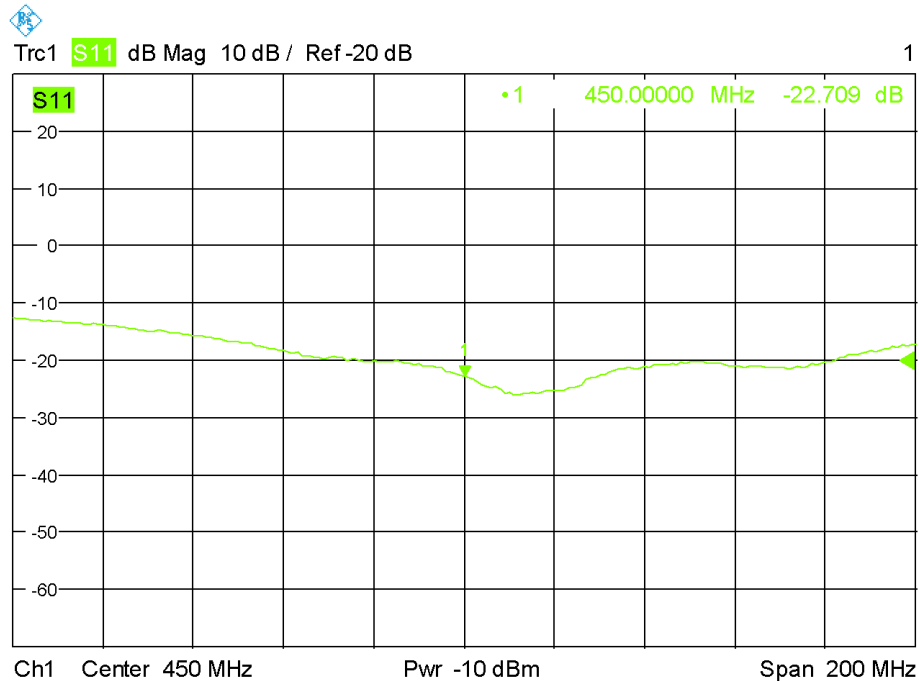

Date: 26.MAY.2023 09:18:16