









INSTRUCTION MANUAL

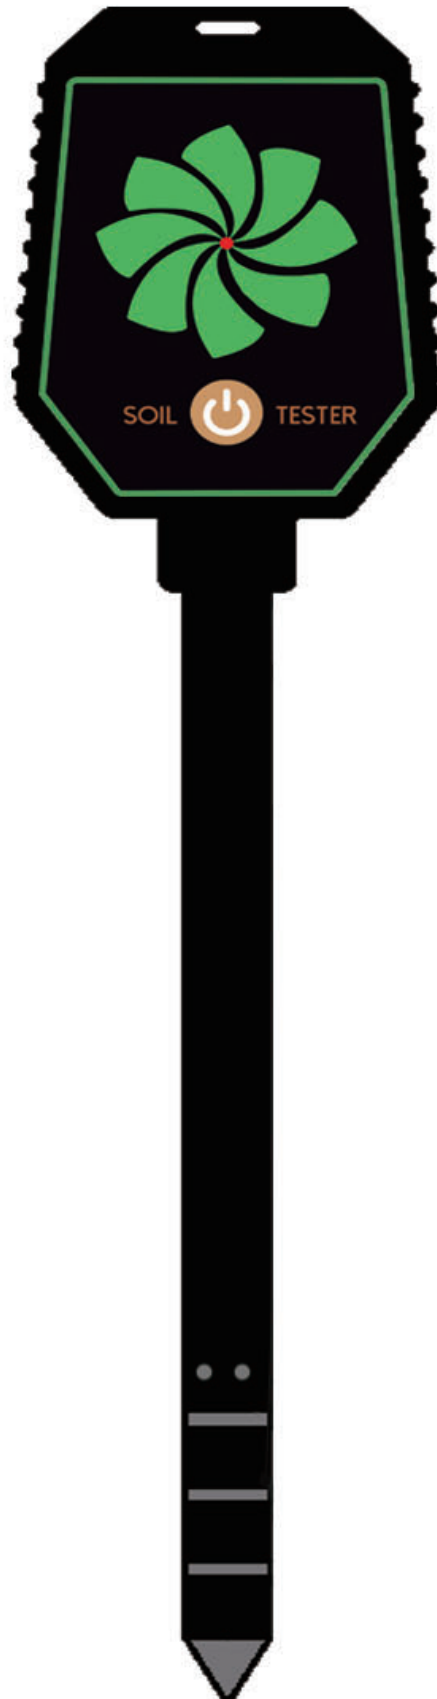

8-in-1 Soil Meter

PARAMETER

pH	Range	0.0-14.0pH
	Resolution	0.1pH
	Accuracy	±0.1pH
	Calibration	7.0,4.0,10.0
EC	Range	0.01-9.99mS/cm
	Resolution	0.01mS/cm
	Accuracy	±0.01mS/cm
	Calibration	1413µS/cm
SALT	Range	0-5110mg/L
	Resolution	1mg/L
	Accuracy	±2%F.S.
Fertility	Range	0-99%
	Resolution	1%
	Accuracy	±2%F.S.
Air Humidity	Range	0-100%RH
	Resolution	1%RH
	Accuracy	±2%RH/Year
Temperature	Range	0.0-50.0°C/32.0-122.0°F
	Resolution	0.1°C/0.1°F
	Accuracy	±0.5°C/±0.1°F
Light Intensity	Dark	
	Normal	
	Bright	
Soil Moist	Dry	
	Normal	
	Wet	
	Wet+	

PRODUCT INTRODUCTION

LIGHT RECEIVER SENSOR

ON/OFF

PILOT LAMP

SOIL TESTER

PH REFERENCE ELECTRODE

EC & MOISTURE ELECTRODE

PH MEASURING ELECTRODE

METAL SPEAR TIP

DOWNLOAD THE APP

Use your smartphone to scan QR code, or search "yinmik" app in Google Play Store or APP Store to download and install.



YINMIK





(IOS)





(Android)

For the first time using the app, please follow the system prompts to enable Bluetooth and location permissions.

Android:

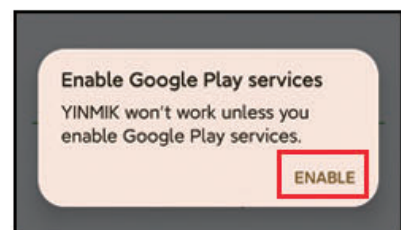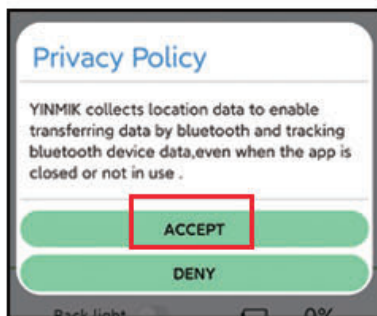


IOS:

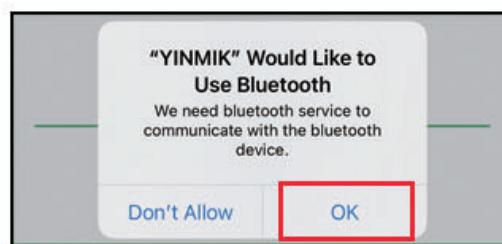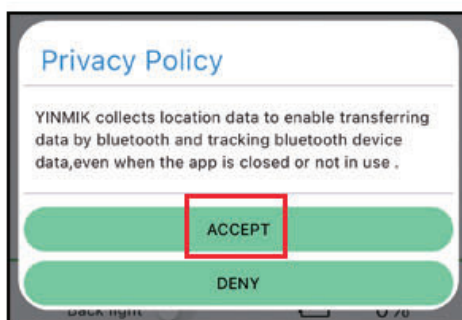




APP CONNECTION

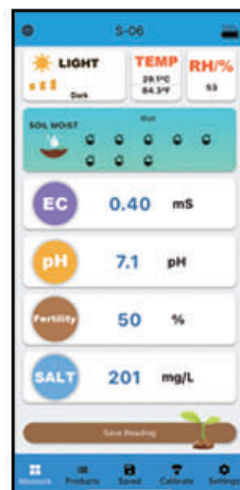
- 1, Turn on the meter by pressing "ON/OFF". The red indicator light on the product is flashing.
- 2, Open the app and wait for automatic connection. APP will match the meter model automatically.
- 3, All testing results can be viewed on the APP. Model number display on top of the screen.
- 4, The product connection is successful, and the indicator light is off.




APP OPERATION

MEASURE

- 1, Click  can switch between Chinese and English.
- 2, Click  to save data Manually.
- 3, Click  to save measurement data.

×	S-06	
Date: 2024-09-20 15:15:47		
pH: 0.00		
EC: 0.00 mS/cm		
SALT: 0 mg/L		
MOIST: 0.00 mS/cm		
LIGHT: 0		
RH: 56%		
FERTILITY: 0.0%		
Temperature: 28.6°C(83.5°F)		
Notes:		
<div></div>		

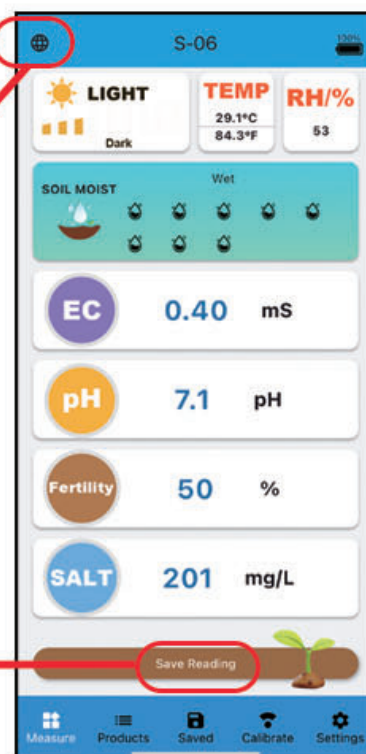


SAVED

1,Manually saved data is displayed in black.

2,Auto saved data is displayed in blue.

3,click  to share the file. If connect to the printer, the testing records can be printed.

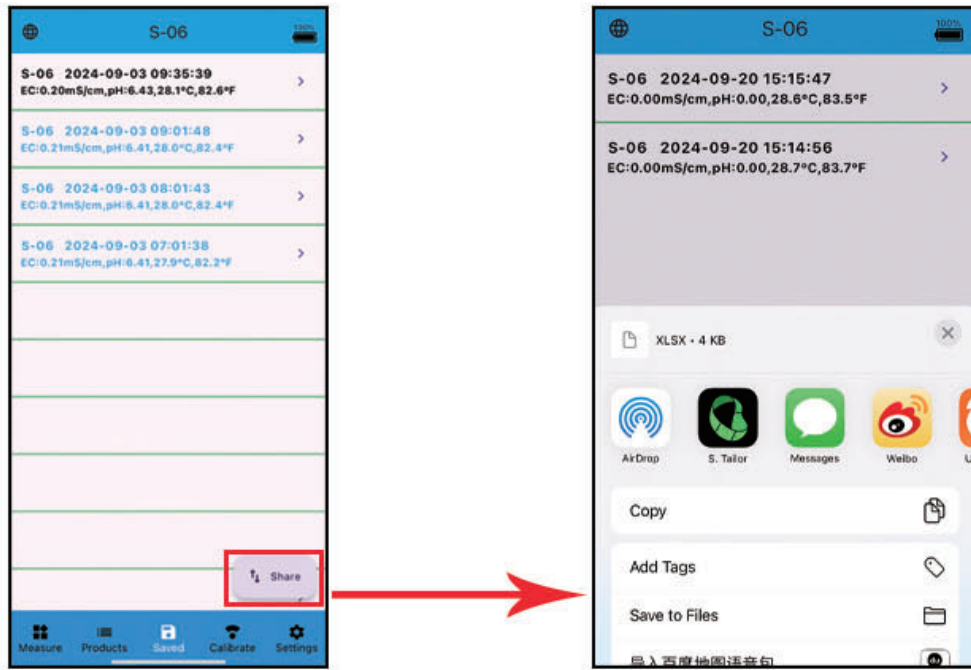

CALIBRATE


1,The pH calibration sequence is 7.0-4.0-10.0.

2,EC calibration uses 1413 μ S/cm calibration solution.


3,Please refer to the calibration introduction for specific calibration procedures. (Page 8).



SETTINGS

1, Click  to open auto save. Auto Saved time interval can be set (between 1-99 hours).


2, Set pH/EC Max or Min Limit values according to user's requirement. If testing results are out of range, the digits will display in red.

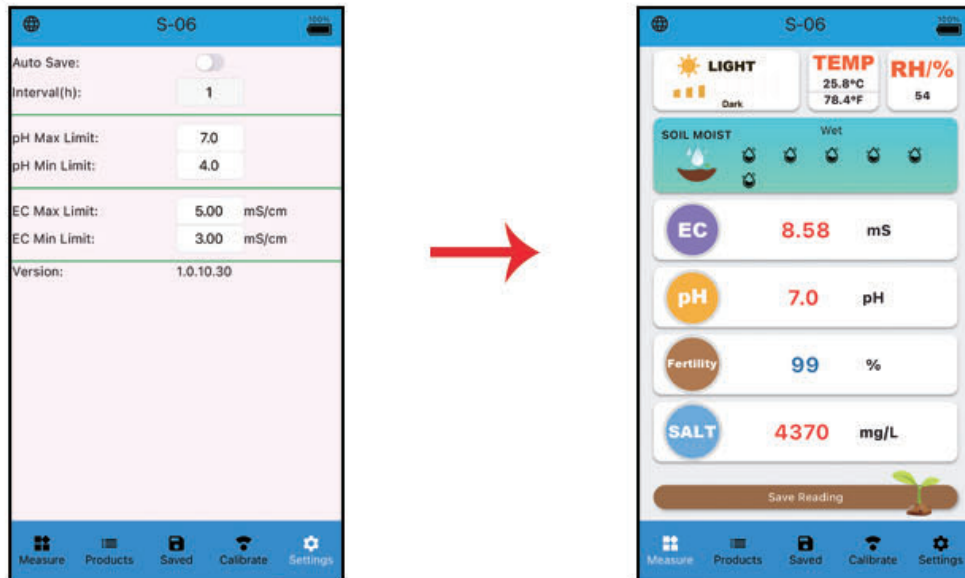

REPLACING THE BATTERY


1, The device battery level is displayed in the upper right corner of the APP homepage. Please replace the battery according to the battery level prompt.

2, Open the protective cover of the battery compartment, remove the old battery, and arrange 4 new batteries, paying attention to the placement of the positive and negative electrodes.

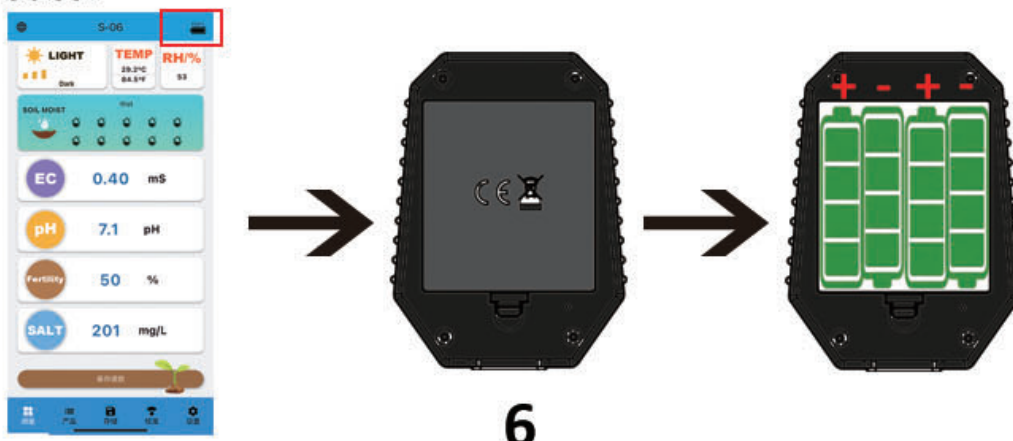


MEASUREMENT STEPS

- 1, Turn on the meter by pressing "ON/OFF". The red indicator light on the product is flashing.
- 2, Open the app and wait for automatic connection. APP will match the meter model automatically.
- 3, All testing results can be viewed on the APP. Model number display on top of the screen.
- 4, The product connection is successful, and the indicator light is off.
- 5, Slowly insert electrode into the soil, the insertion depth is at least 6cm. Make sure that the pH reference electrode (two white dots) is submerged in the soil.

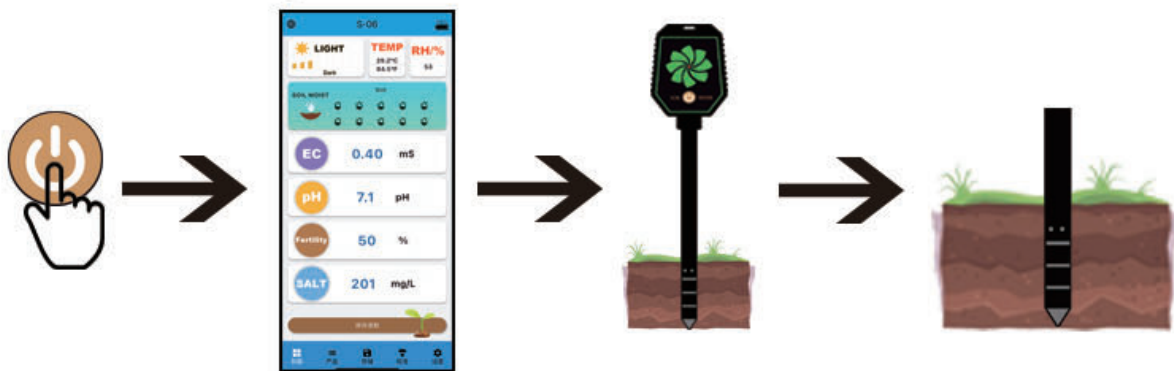

- 6, Pull out the electrode and wash the electrode with clean water. Use the brush to clean the residual soil on the electrode.

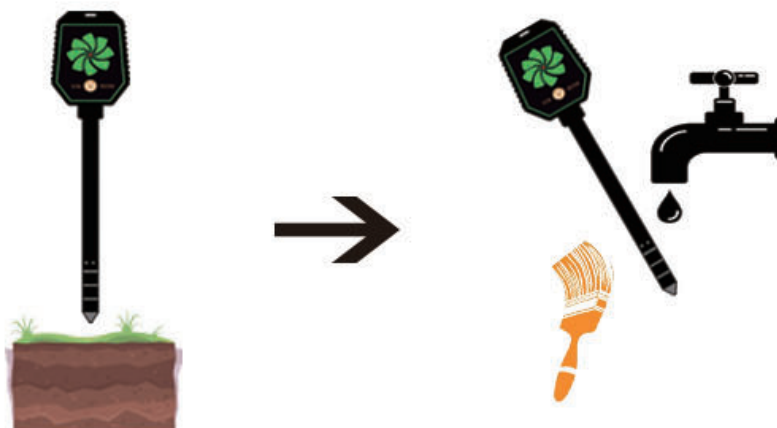

PH CALIBRATION


Tips:

1,PH Solution: Dissolve each buffersolution into 3 cups which is filled with250ml distilled water .


2,The calibration sequence is 7.0-4.0-10.0.

STEP 7.0


1,Turn on the meter by pressing "ON/OFF".Bluetooth connection to mobile app.



2, Put the pH probe into the pH7.0 buffer solution.Make sure that the pH reference electrode (two white dots) is submerged in the buffer solution.

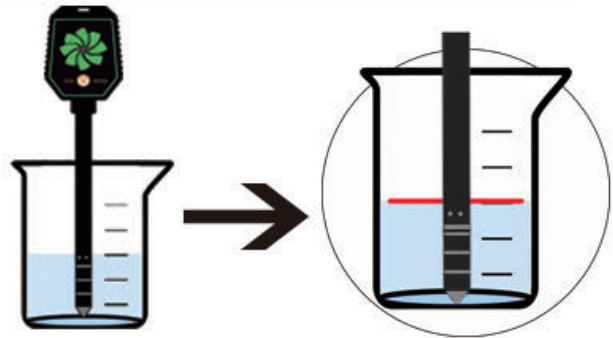

3, Wait for the screen value to stabilize and approach 7.0, then click on the calibration page and select pH calibration.

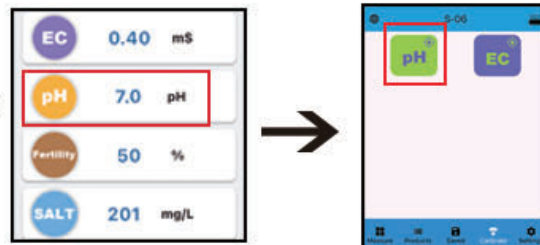


4,Click on "7.0" to calibrate, and the calibration record will be displayed after the calibration is completed.




5,Wash the electrode with pure water and wipe dry it.

STEP 4.0


- 1, Put the pH probe into the pH4.0 buffer solution. Make sure that the pH reference electrode (two white dots) is submerged in the buffer solution.

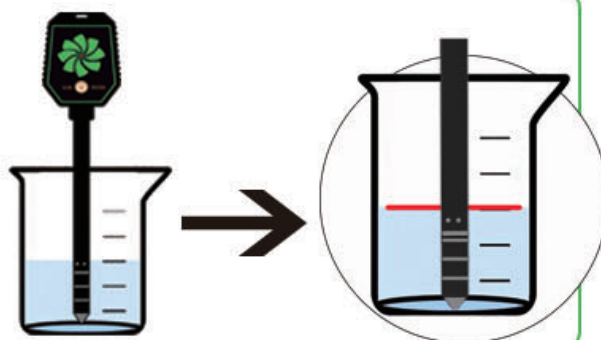

- 2, Wait for the screen value to stabilize and approach 4.0, then click on the calibration page and select pH calibration.

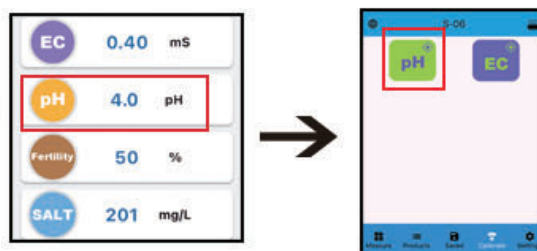


- 3, Click on "4.0" to calibrate, and the calibration record will be displayed after the calibration is completed.

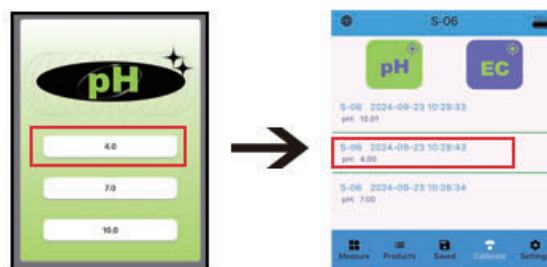


- 4, Wash the electrode with pure water and wipe dry it.

STEP 10.0

- 1, Put the pH probe into the pH10.0 buffer solution. Make sure that the pH reference electrode (two white dots) is submerged in the buffer solution.

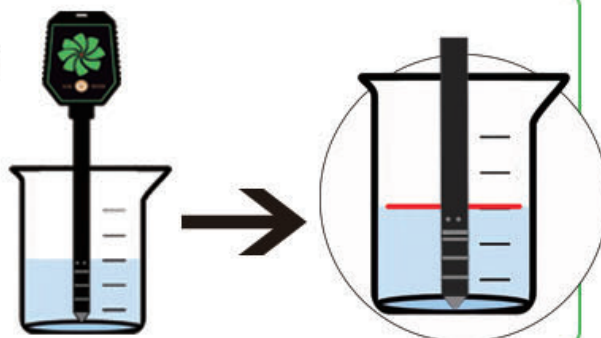

2, Wait for the screen value to stabilize and approach 10.0, then click on the calibration page and select pH calibration.

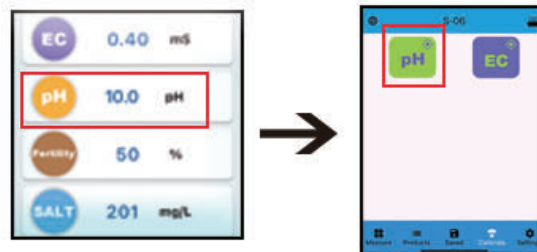

3, Click on "10.0" to calibrate, and the calibration record will be displayed after the calibration is completed.




4, Wash the electrode with pure water and wipe dry it.

EC CALIBRATION


Tips:

- 1, The tester has been calibrated before leaving the factory, and there is no need for recalibration.
- 2, EC calibration requires 1413 μ S/cm calibration solution.


1, Turn on the meter by pressing "ON/OFF". Bluetooth connection to mobile app.




2, Put the pH probe into the 1413 μ S/cm buffer solution. Make sure that the pH reference electrode (two white dots) is submerged in the buffer solution.

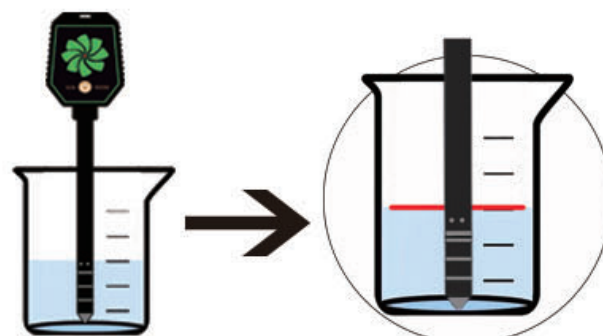

3, Wait for the screen value to stabilize and approach 1413 μ S/cm, then click on the calibration page and select EC calibration.

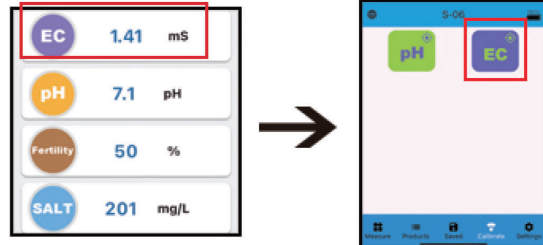

4, Click to enter 1.41, and the calibration record will be displayed after the calibration is completed.

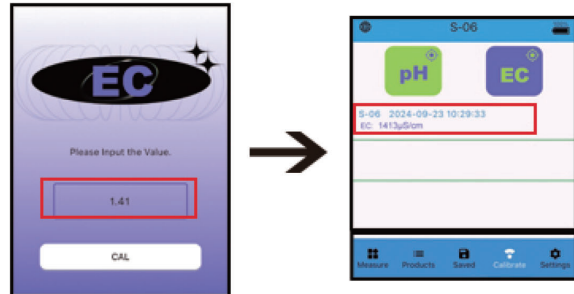

5, Wash the electrode with pure water and wipe dry it.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Any changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation.

If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

The device has been evaluated to meet general RF exposure requirement. The device can be used in portable exposure condition without restriction