


LUNDERG.[®]

Under Mattress Early-Alert Sensor Pad


START
HERE

Quick Guide Video

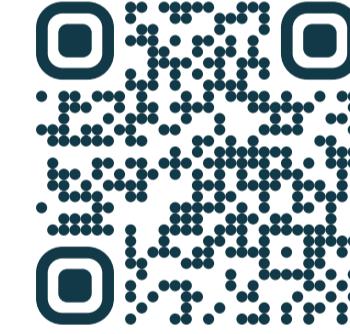


Lunderg.com/undervideo

Quick Guide PDF

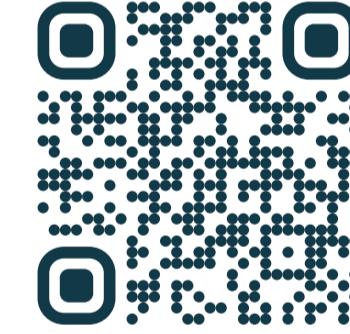

Lunderg.com/underguide


Full Guide Video

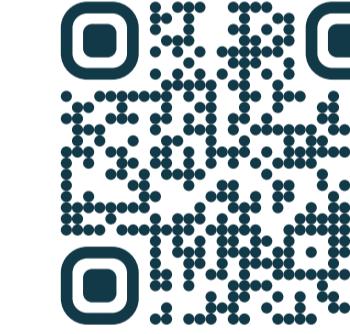

Lunderg.com/underfullvideo

Questions? Contact us at questions@Lunderg.com
We reply within 24 hours, 7 days a week!

↑ THIS SIDE MUST FACE UP ↑

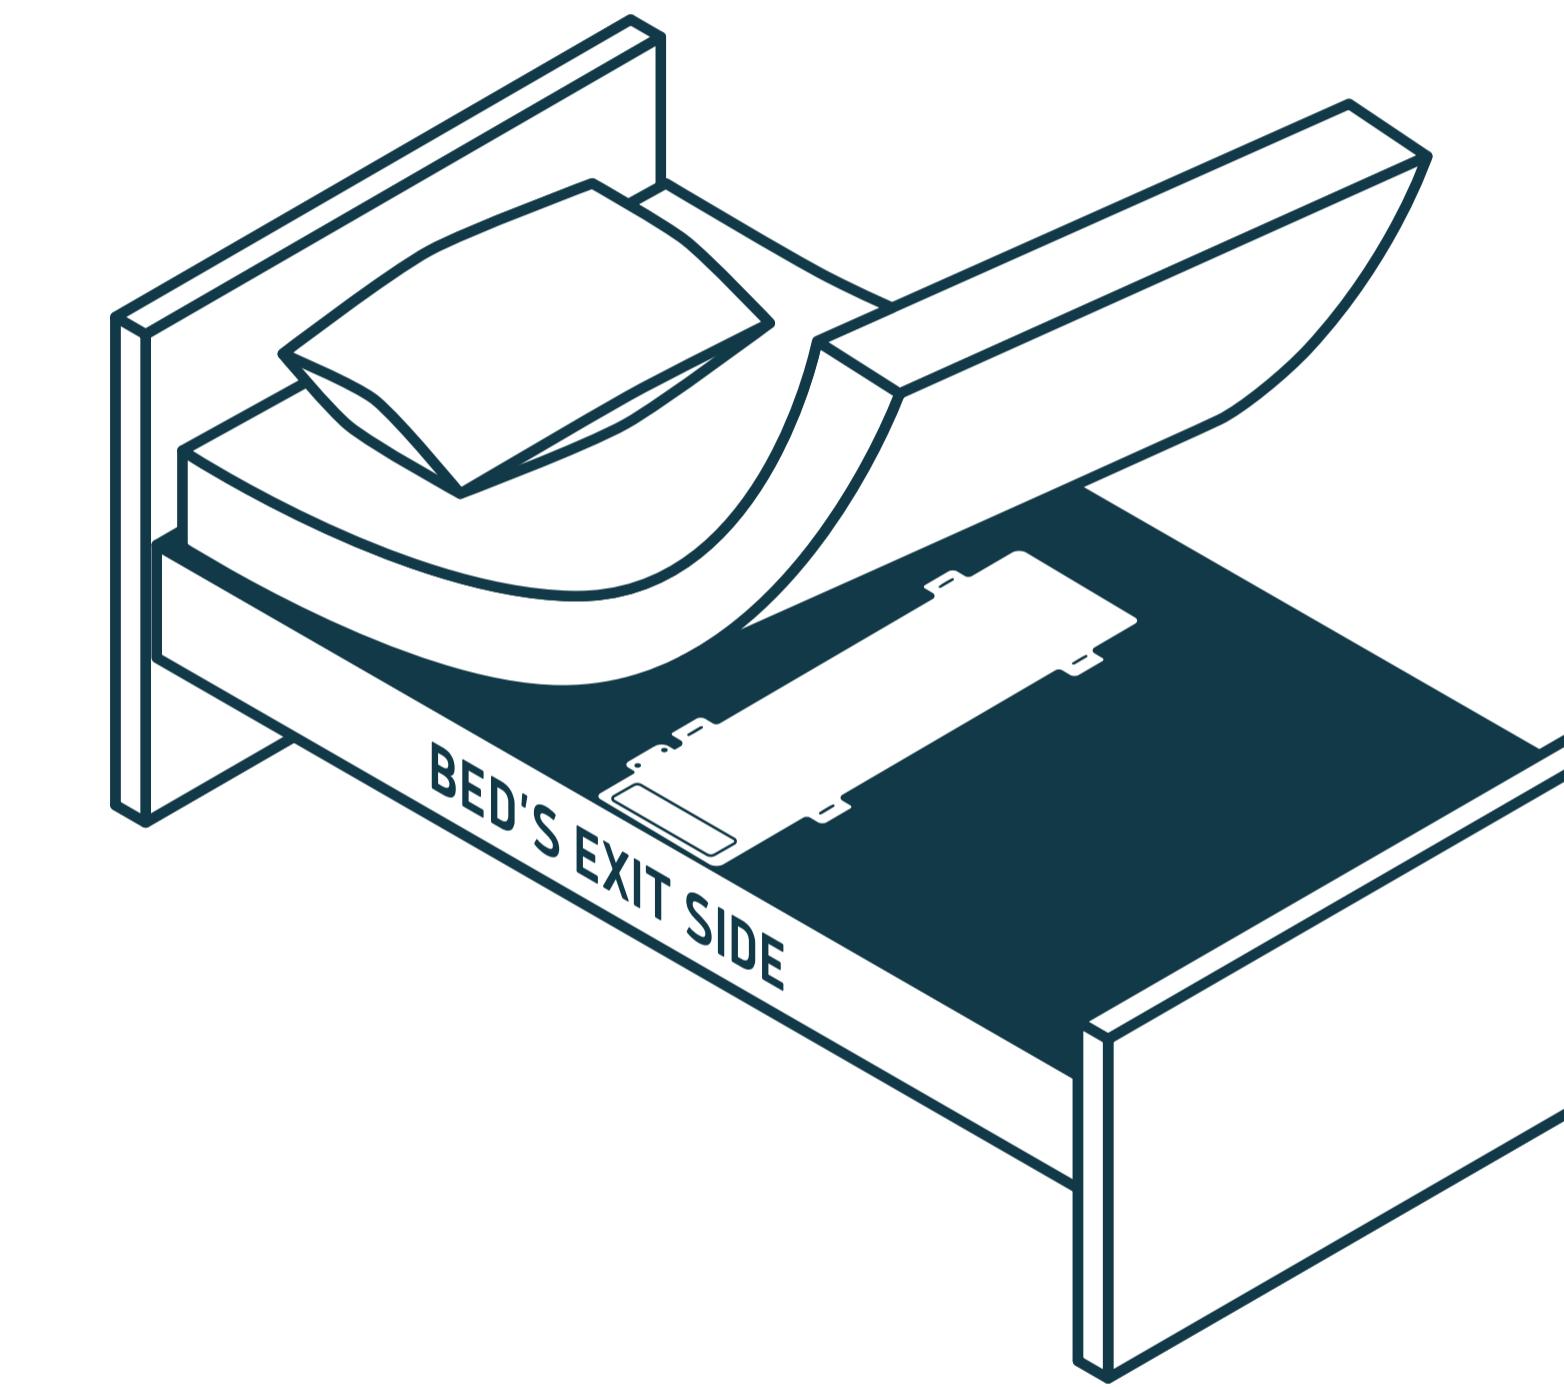

Normal OFF Early-Alert

POCKET

EARLY ALERT

→ FACE TOWARDS THE BED'S EXIT SIDE →

LUNDERG®

Under Mattress Early-Alert Sensor Pad

UPC-LUN-UNDERBED-KIT

For safety, replace this pad after 24 months of use.

CAUTION: Technology alone cannot prevent falls or injury. In addition to professional caregivers, this device is solely meant to supplement a facility or home patient management system.

Start Date	End Date

Use start date to track pad use.

Battery Input 3V 2 x CR2477 - Batteries can't be replaced
Protected by US Patent #s: 11,412,996 / 7,924,163 / 9,253,891
/ 7,557,719 / 8,085,154 / 7,474,224
FCC ID: 2AB3B-LUN-UMB / IC: 28964-LUNUMB
This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
[1] This device may not cause harmful interference, and
[2] this device must accept any interference received,
including interference that may cause undesired operation.



IP21
IEC/EN 60601-1
IEC/EN 60601-1-6
IEC/EN 60601-1-11
Designed in the USA - Made in P.R.C.

Care & Maintenance Instructions:

- Use disinfectant wipes or antibacterial cleansers to clean the pad.
- **DO NOT** immerse the sensor pad in any liquid.
- **DO NOT** expose the sensor pad to high-temperature sanitizers.

Storage:

- Move the switch inside the pocket to OFF.
- Always keep the sensor pad flat when in storage.
- Storage temperature: 32°F -122°F (0°C - 50°C).

PROBLEMS OR QUESTIONS?

Contact us directly at questions@lunderg.com or
request a call back at (800) 652-4905
We reply to every message within 24 hours!