

RADIO TEST REPORT

Report ID:

REP021632

Project number:

PRJ0041478

Type of assessment:

SAR Exemption report

Applicant:

MedRx Inc.

Product description:

Hearing Aid Analyzer

Model (HVIN):

MedRx WREM

FCC identifier:

2A6UNMEDRXWREM

ISED certification number:

28531-MEDRXWREM

Specifications:

- ◆ FCC 47 CFR Part 2 Subpart J, §2.1093
- ◆ FCC KDB 447498 D01 General RF Exposure Guidance v06
- ◆ ISED Canada RSS-102 Issue 5 Amendment 1, (February 2021)
- ◆ RSS-102, Issue 5, Supplementary Procedure SPR-002, Issue 1

Attestation:

I attest that the testing was performed or supervised by me; that the test measurements were made in accordance with the above-mentioned departmental standard(s), and that the radio equipment identified in this application has been subject to all applicable test conditions specified in the departmental standards and all of the requirements of the standards have been met.

Date of issue: **January 3, 2024****Tarek Elkholy, EMC/RF Specialist**

Prepared by



Signature

Nemko Canada Inc., a testing laboratory, is accredited by ANSI National Accreditation Board (ANAB).

The tests included in this report are within the scope of this accreditation.

The ANAB symbol is an official symbol of the ANSI National Accreditation Board, used under licence.

ANAB File Number: AT-3195 (Ottawa/Almonte); AT-3193 (Pointe-Claire); AT-3194 (Cambridge)

Lab locations

Company name	Nemko Canada Inc.			
Facilities	<i>Ottawa site:</i> 303 River Road Ottawa, Ontario Canada K1V 1H2 Tel: +1 613 737 9680 Fax: +1 613 737 9691	<i>Montréal site:</i> 292 Labrosse Avenue Pointe-Claire, Québec Canada H9R 5L8 Tel: +1 514 694 2684 Fax: +1 514 694 3528	<i>Cambridge site:</i> 1-130 Saltsman Drive Cambridge, Ontario Canada N3E 0B2 Tel: +1 519 650 4811	<i>Almonte site:</i> 1500 Peter Robinson Road West Carleton, Ontario Canada K0A 1L0 Tel: +1 613 256-9117
Test site identifier	Organization	Ottawa/Almonte	Montreal	Cambridge
	FCC:	CA2040	CA2041	CA0101
	ISED:	2040A-4	2040G-5	24676
Website	www.nemko.com			

Limits of responsibility

Note that the results contained in this report relate only to the items tested and were obtained in the period between the date of initial receipt of samples and the date of issue of the report.

This test report has been completed in accordance with the requirements of ISO/IEC 17025. All results contained in this report are within Nemko Canada's ISO/IEC 17025 accreditation.

Copyright notification

Nemko Canada Inc. authorizes the applicant to reproduce this report provided it is reproduced in its entirety and for use by the company's employees only. Any use which a third party makes of this report, or any reliance on or decisions to be made based on it, are the responsibility of such third parties. Nemko Canada Inc. accepts no responsibility for damages, if any, suffered by any third party as a result of decisions made or actions based on this report.
© Nemko Canada Inc.

Table of Contents

Table of Contents	3
Evaluation summary	4
1.1 SAR exemption for standalone transmission	4
1.2 Nerve Stimulation test, Wireless charger	7

Section 1

Evaluation summary

1.1 SAR exemption for standalone transmission

Section 1.1.1 References, definitions and limits

FCC §2.1093

- (2) The SAR limits for general population/uncontrolled exposure are 0.08 W/kg, as averaged over the whole body, and a peak spatial-average SAR of 1.6 W/kg, averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the parts of the human body treated as extremities, such as hands, wrists, feet, ankles, and pinnae, where the peak spatial-average SAR limit is 4 W/kg, averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube). Exposure may be averaged over a time period not to exceed 30 minutes to determine compliance with general population/uncontrolled SAR limits.

FCC KDB 447498 D01

4.3.1 Standalone SAR test exclusion considerations

The SAR-based exemption formula of §1.1307(b)(3)(i)(B), repeated here, applies for single fixed, mobile, and portable RF sources with available maximum time-averaged power or effective radiated power (ERP), whichever is greater, of less than or equal to the threshold P_{th} (mW).

This method shall only be used at separation distances from 0.5 cm to 40 cm and at frequencies from 0.3 GHz to 6 GHz (inclusive). P_{th} is given by formula

$$P_{th}(mW) = \begin{cases} ERP_{20\text{ cm}} \left(\frac{d}{20\text{ cm}} \right)^x & d \leq 20\text{ cm} \\ ERP_{20\text{ cm}} & 20\text{ cm} < d \leq 40\text{ cm} \end{cases}$$

where

$$x = -\log_{10} \left(\frac{60}{ERP_{20\text{ cm}} \sqrt{f}} \right)$$

Table 1.1-1: Example Power Thresholds (mW)

Separation:	5 mm	10 mm	15 mm	20 mm	25 mm	30 mm	35 mm	40 mm	45 mm	50 mm
300 MHz	39	65	88	110	129	148	166	184	201	217
450 MHz	22	44	67	89	112	135	158	180	203	226
835 MHz	9	25	44	66	90	116	145	175	207	240
1900 MHz	3	12	26	44	66	92	122	157	195	236
2450 MHz	3	10	22	38	59	83	111	143	179	219
3600 MHz	2	8	18	32	49	71	96	125	158	195
5800 MHz	1	6	14	25	40	58	80	106	136	169

Notes: Values in the table are in mW

For mobile devices that are not exempt per Table 1 [of §1.1307(b)(1)(i)(C)] at distances from 20 cm to 40 cm and in 0.3 GHz to 6 GHz, evaluation of compliance with the exposure limits in §1.1310 is necessary if the ERP of the device is greater than ERP 20 cm in Formula below [repeated from §2.1091(c)(1); also in §1.1307(b)(1)(i)(B)].

$$P_{th}(mW) = ERP_{20\text{ cm}}(mW) = \begin{cases} 2040f & 0.3\text{ GHz} \leq f < 1.5\text{ GHz} \\ 3060 & 1.5\text{ GHz} \leq f \leq 6\text{ GHz} \end{cases}$$

Table 1.1-2: Thresholds for single RF sources subject to routine environmental evaluation

Table 1	RF Source Frequency			Minimum Distance			Threshold ERP
	f_L (MHz)		f_H (MHz)	$\lambda_L / 2\pi$		$\lambda_H / 2\pi$	(W)
	0.3	–	1.34	159 m	–	35.6 m	1,920 R ²
	1.34	–	30	35.6 m	–	1.6 m	3,450 R ² /f ²
	30	–	300	1.6 m	–	159 mm	3.83 R ²
	300	–	1,500	159 mm	–	31.8 mm	0.0128 R ² f
	1,500	–	100,000	31.8 mm	–	0.5 mm	19.2 R ²

References, definitions and limits, continued

RSS-102, Section 2.5.1

SAR evaluation is required if the separation distance between the user and/or bystander and the antenna and/or radiating element of the device is less than or equal to 20 cm, except when the device operates at or below the applicable output power level (adjusted for tune-up tolerance) for the specified separation distance defined in table below

Table 1.1-3: Exemption limits for routine evaluation based on frequency and separation distance

Separation:	≤5 mm	10 mm	15 mm	20 mm	25 mm	30 mm	35 mm	40 mm	45 mm	≥50 mm
≤300 MHz	71	101	132	162	193	223	254	284	315	345
450 MHz	52	70	88	106	123	141	159	177	195	213
835 MHz	17	30	42	55	67	80	92	105	117	130
900 MHz	7	10	18	34	60	99	153	225	316	431
2450 MHz	4	7	15	30	52	83	123	173	235	309
3500 MHz	2	6	16	32	55	86	124	170	225	290
5800 MHz	1	6	15	27	41	56	71	85	97	106

Notes: Values in the table are in mW

Output power level shall be the higher of the maximum conducted or equivalent isotropically radiated power (e.i.r.p.) source-based, time-averaged output power. For controlled use devices where the 8 W/kg for 1 gram of tissue applies, the exemption limits for routine evaluation in the table above are multiplied by a factor of 5. For limb-worn devices where the 10 gram value applies, the exemption limits for routine evaluation in the table above are multiplied by a factor of 2.5. If the operating frequency of the device is between two frequencies located in Table 1, linear interpolation shall be applied for the applicable separation distance. For test separation distance less than 5 mm, the exemption limits for a separation distance of 5 mm can be applied to determine if a routine evaluation is required.

For medical implants devices, the exemption limit for routine evaluation is set at 1 mW. The output power of a medical implants' device is defined as the higher of the conducted or e.i.r.p to determine whether the device is exempt from the SAR evaluation.

1.1.1 EUT technical information, Bluetooth

Type of EUT use	head or body
Minimum separation distance	1 cm
Highest operating frequency	2.442 GHz
Antenna type	Integral
Antenna gain	0.5 dBi
Maximum transmitter conducted power	6.3 dBm (4.3 mW)
Maximum system ERP	4.65 dBm (2.9 mW)
Duty cycle	100 %

1.1.2 Justification for Standalone SAR test exclusion

SAR exemption verification for FCC:

Nominal RF power (mW):	4.8	INPUTS
Duty cycle (%):	100	
Frequency (GHz):	2.442	
Distance (cm):	1	
Time averaged power (mW):	4.8	Calculated

Frequency (GHz)	λ (cm)	Power (mW)	Distance (cm)	Exemption ERP _{20cm} (mW)	x	P _{threshold} (mW)	Result	Ratio
2.442	12.3	5	1	3060	1.90	10.28	EXEMPT	0.47

Table 1.1-4: SAR exemption verification for ISED Canada

Transmit frequency, MHz	Maximum EIRP, mW	Separation distance, mm	Limit, mW	Margin, dB
2442	4.8	10	7.015	1.7

Note: Margin was calculated as follows: $10 \times \log_{10}(\text{Limit} / \text{Maximum EIRP})$

1.1.3 Verdict

The calculation is below the threshold, therefore, the product exempt from the SAR test requirements.

1.2 Nerve Stimulation test, Wireless charger

1.2.1 References, definitions, and limits

This evaluation of the instantaneous requirements for Radio Frequency (RF) field strengths (reference levels) based on the effects of internal electric fields was done in accordance with SPR-002, Issue 1. The limits for Uncontrolled Environment are found in RSS 102, Issue 5, Table 4 (Instantaneous).

Table 4: RF Field Strength Limits for Devices Used by the General Public (Uncontrolled Environment)				
Frequency Range (MHz)	Electric Field (V/m rms)	Magnetic Field (A/m rms)	Power Density (W/m ²)	Reference Period (minutes)
0.003-10 ²¹	83	90	-	Instantaneous*
0.1-10	-	0.73/ <i>f</i>	-	6 ^{**}
1.1-10	87/ <i>f</i> ^{0.5}	-	-	6 ^{**}
10-20	27.46	0.0728	-2	6
20-48	58.07/ <i>f</i> ^{0.25}	0.1540/ <i>f</i> ^{0.25}	8.944/ <i>f</i> ^{0.5}	6
48-300	22.06	0.05852	1.291	6
300-6000	3.142 <i>f</i> ^{0.3417}	0.008335 <i>f</i> ^{0.3417}	0.02619 <i>f</i> ^{0.6834}	6
6000-15000	61.4	0.163	10	6
15000-150000	61.4	0.163	10	616000/ <i>f</i> ^{1.2}
150000-300000	0.158 <i>f</i> ^{0.5}	4.21 x 10 ⁻⁴ <i>f</i> ^{0.5}	6.67 x 10 ⁻⁵ <i>f</i>	616000/ <i>f</i> ^{1.2}
Note: <i>f</i> is frequency in MHz. * Based on nerve stimulation (NS). ** Based on specific absorption rate (SAR).				

Start date October 5, 2022

1.2.2 Observations, settings and special notes

The testing was performed as per SPR-002, Issue 1.

- The measurement probe is set a fixed separation distance of 20 cm
- The instantaneous E-Field is assessed over the average 180 cm human body height, measuring 5 points in 40 cm intervals, starting 20 cm above the ground. The maximum field was measured at 20 cm height and is used as reference for calculations.
- The instantaneous H-Field is assessed by measuring 8 points in an evenly spaced rectangular pattern measuring 60 cm tall by 30 cm wide. The maximum field was measured at 20 cm height and is used as reference for calculations.
- The X, Y, and Z axis are measured simultaneously, and summed by the measurement probe software
- The maximum emission level is measured using an appropriate resolution bandwidth.
- Worst case measurement are recorded in the tables in the test data section.

1.2.3 Test data

Table 1.2-2: Equipment list

Equipment	Manufacturer	Model no.	Test Software	Asset no.	Cal cycle	Next cal.
Isotropic probe	Narda	EHP200A	EHP200-TS	FA003103	2 years	July 14, 2023

Type of evaluation	Nerve Stimulation Exposure Evaluation (SPR-002)					
Nerve Stimulation Evaluation (SPR-002)	Evaluated against exposure limits: ☒ General Public Use ☐ Controlled Use					
	Measurement distance:		0.1	m		
	Field Strength:		4.7	☒ V/m (electric)	☐ A/m (magnetic)	
				☒ Measured	☐ Computed	☐ Calculated
	Field Strength:		0.5	☐ V/m (electric)	☒ A/m (magnetic)	
			☒ Measured	☐ Computed	☐ Calculated	
Exposure condition:		☒ Whole body/Torso/Head		☐ Leg		
		☒ Arm		☐ Hand/Foot		

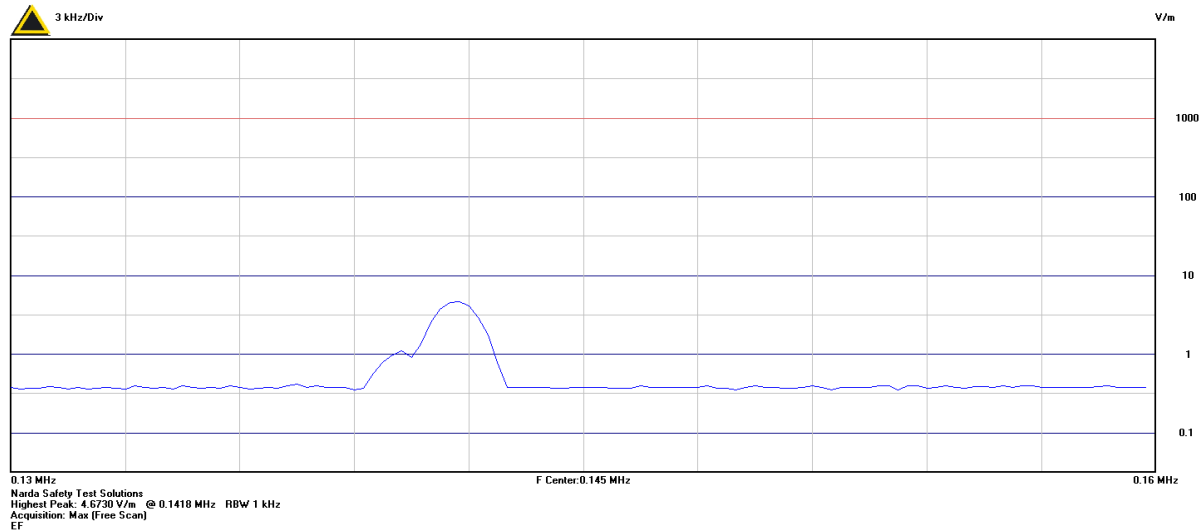


Table 1.2-3 - Instantaneous E-Field measurements over 180 cm height

Frequency, MHz	Measurement distance cm	Measured Electric Field Strength V/m (r.m.s) instantaneous	RSS-102 Limit Electric Field Strength V/m (r.m.s) instantaneous	Margin, dB
0.1418	10	4.67	83.00	78.33

Notes: Limit taken from RSS 210, Issue 5, Table 4 for Uncontrolled Exposure, Maximum E-Field emission measured at 20 cm

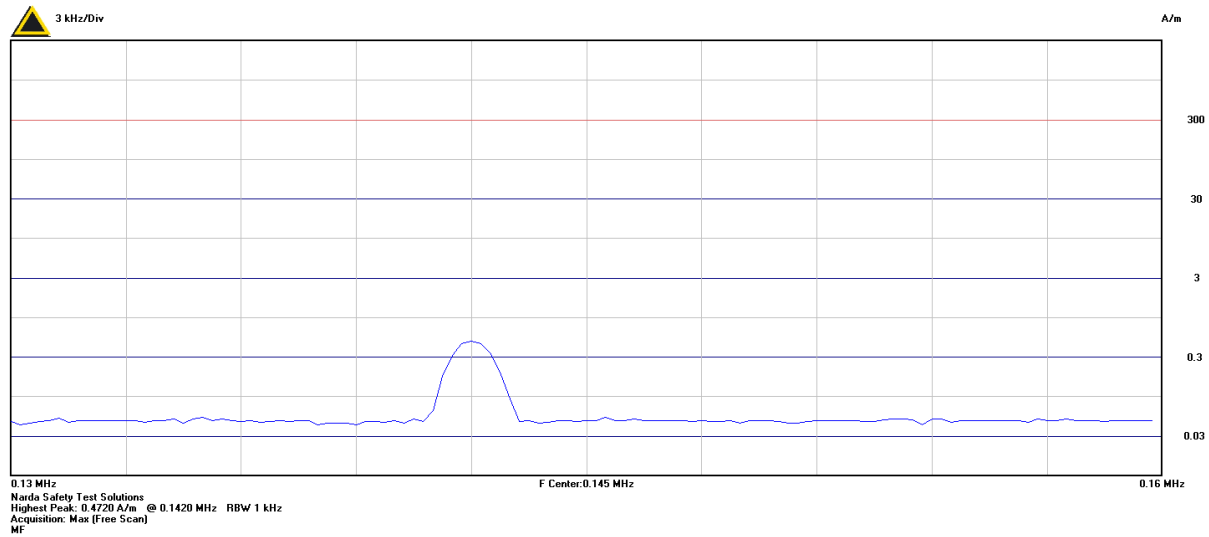


Table 1-2.4 - Maximum instantaneous H-Field

Frequency, MHz	Antenna Position referencing EUT	Measurement distance cm	Measured Magnetic Field Strength A/m (r.m.s) instantaneous	RSS-102 Limit Magnetic Field Strength A/m (r.m.s) instantaneous	Margin, dB
0.1420	All sides	10	0.47	90.00	89.53

1.2.4 Test setup photos



End of the test report