



FCC 47 CFR § 2.1093  
IEC/IEEE 62209-1528

**SAR REPORT (NFC evaluation)  
FOR**

**Wireless Charger + NFC**

**MODEL NUMBER: WCMIT31A**

**FCC ID: 2A6WXWCMIT31A**

**REPORT NUMBER: S-4791776982-S2V2**

**ISSUE DATE: 2025-07-29**

*Prepared for*  
**BH EVS Co.,Ltd**  
**5, Magokjungang 8-ro 5-gil, Gangseo-gu,**  
**Seoul, 07794 Republic of Korea**

*Prepared by*  
**UL Korea, Ltd.**

**26th floor, 152, Teheran-ro, Gangnam-gu Seoul, 06236, Korea**

**Suwon Test Site: UL Korea, Ltd. Suwon Laboratory**  
**218 Maeyeong-ro, Yeongtong-gu,**  
**Suwon-si, Gyeonggi-do, 16675, Korea**  
**TEL: (031) 337-9902**  
**FAX: (031) 213-5433**



**Testing Laboratory**

**TL-637**

**Revision History**

Rev.	Date	Revisions	Revised By
V1	2025-07-10	Initial Issue	--
V1	2025-07-29	Deleted in Sec 10	Jeongyeon Won

**Table of Contents**


<b>1. Attestation of Test Results .....</b>	<b>4</b>
<b>2. Test Specification, Methods and Procedures.....</b>	<b>5</b>
<b>3. Facilities and Accreditation .....</b>	<b>5</b>
<b>4. SAR Measurement System &amp; Test Equipment .....</b>	<b>6</b>
4.1. <i>SAR Measurement System.....</i>	6
4.2. <i>SAR Scan Procedures.....</i>	7
4.3. <i>Test Equipment.....</i>	9
<b>5. Measurement Uncertainty.....</b>	<b>10</b>
5.1. <i>DECISION RULE.....</i>	10
<b>6. Device Under Test (DUT) Information .....</b>	<b>11</b>
6.1. <i>DUT Description .....</i>	11
6.2. <i>Wireless Technologies.....</i>	11
<b>7. RF Exposure Conditions (Test Configurations) .....</b>	<b>11</b>
<b>8. Dielectric Property Measurements &amp; System Check .....</b>	<b>12</b>
8.1. <i>Dielectric Property Measurements .....</i>	12
8.2. <i>System Check.....</i>	13
<b>9. Measured SAR Results .....</b>	<b>15</b>
9.1. <i>NFC.....</i>	15
<b>Appendices .....</b>	<b>16</b>
S-4791776982-S2 FCC SAR App A Test photos .....	16
S-4791776982-S2 FCC SAR App B Test Plots .....	16
S-4791776982-S2 FCC SAR App C System Plots .....	16
S-4791776982-S2 FCC SAR App D SAR Tissue .....	16
S-4791776982-S2 FCC SAR App E Probe Certi.....	16
S-4791776982-S2 FCC SAR App F Source Certi .....	16

## 1. Attestation of Test Results

Applicant Name	BH EVS Co.,Ltd.
FCC ID	2A6WXWCMIT31A
Model Number	WCMIT31A
Applicable Standards	FCC 47 CFR § 2.1093 IEC/IEEE 62209-1528 Published RF exposure KDB procedures
Exposure Category	SAR Limits (W/Kg) Peak spatial average 1g SAR
General population / Uncontrolled exposure	1.6
RF Exposure Conditions	Equipment Class - The Highest SAR (W/kg) NFC
Standalone at 0mm	<0.10
Simultaneous Tx	N/A
Date Tested	2025-06-19
Test Results	Pass

UL Korea, Ltd. tested the above equipment in accordance with the requirements set forth in the above standards. All indications of Pass/Fail in this report are opinions expressed by UL Korea, Ltd. based on interpretations and/or observations of test results. Measurement Uncertainties were not taken into account and are published for informational purposes only. The test results show that the equipment tested is capable of demonstrating compliance with the requirements as documented in this report.

**Note:** The results documented in this report apply only to the tested sample, under the conditions and modes of operation as described herein. This document may not be altered or revised in any way unless done so by UL Korea, Ltd. and all revisions are duly noted in the revisions section. Any alteration of this document not carried out by UL Korea, Ltd. will constitute fraud and shall nullify the document. This report must not be used by the client to claim product certification, approval, or endorsement by IAS, any agency of the Federal Government, or any agency of any government.

Approved & Released By:	Prepared By:
	
Justin Park Operations Leader UL Korea, Ltd. Suwon Laboratory	Jeongyeon Won Laboratory Engineer UL Korea, Ltd. Suwon Laboratory

## 2. Test Specification, Methods and Procedures

The tests documented in this report were performed in accordance with IEEE Std 62209-1528:

In addition to the above, the following information was used:

- 447498 D04 Interim General RF Exposure Guidance v01

## 3. Facilities and Accreditation

The test sites and measurement facilities used to collect data are located at

Suwon
SAR 4 Room

UL Korea, Ltd. is accredited by IAS, Laboratory Code TL-637.


The full scope of accreditation can be viewed at;

<https://www.iasonline.org/wp-content/uploads/2017/05/TL-637-cert-New.pdf>.

## 4. SAR Measurement System & Test Equipment

### 4.1. SAR Measurement System

The DASY6 & 8 system used for performing compliance tests consists of the following items:

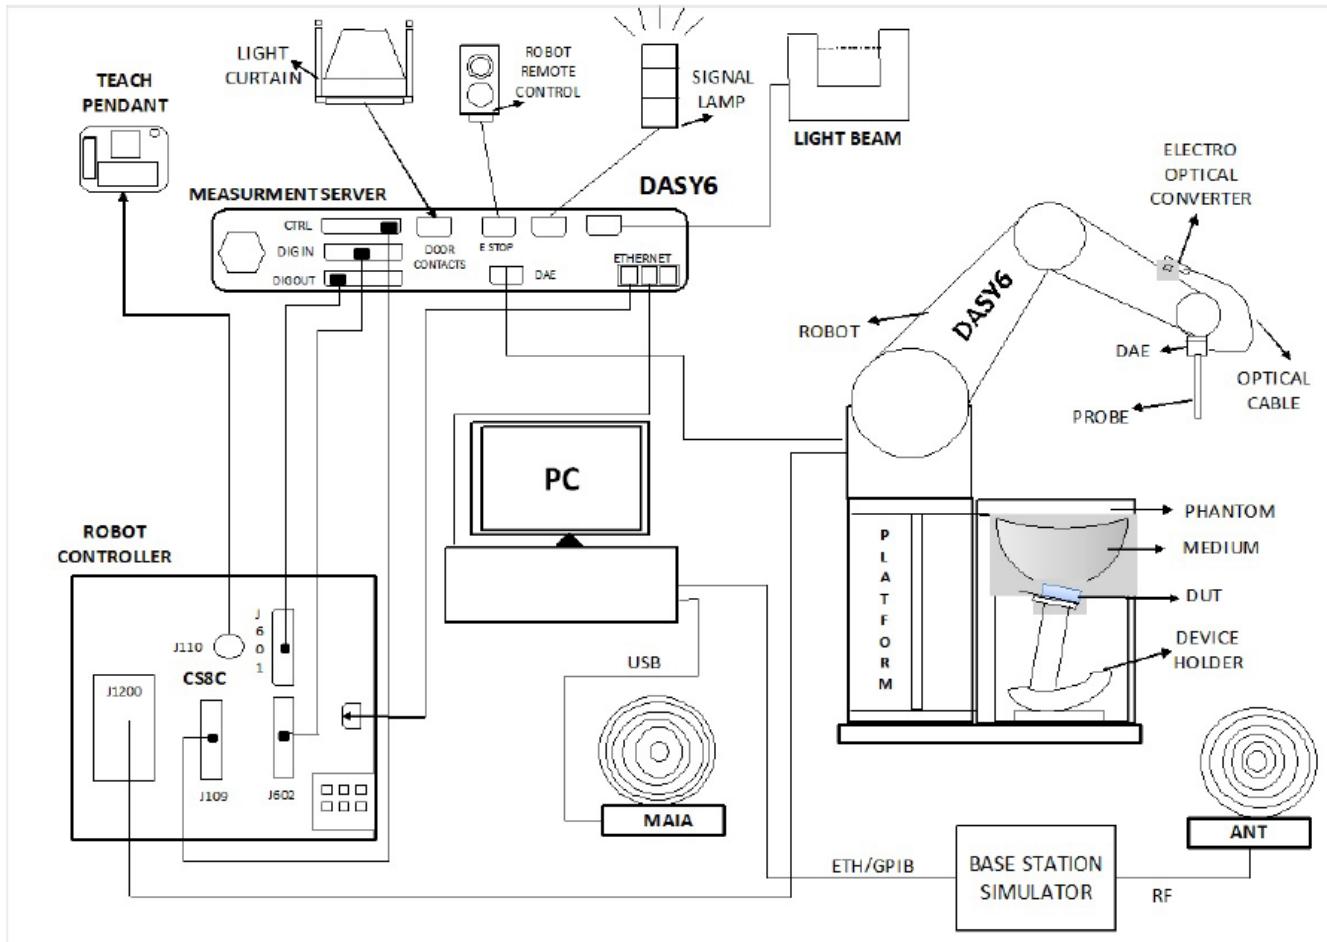

- A standard high precision 6-axis robot with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- An isotropic Field probe optimized and calibrated for the targeted measurement.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running Win10 and the DASY6 or 8 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.

## 4.2. SAR Scan Procedures

### Step 1: Power Reference Measurement

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 2.1 mm. This distance cannot be smaller than the distance of sensor calibration points to probe tip as defined in the probe properties.

### Step 2: Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values, before doing a fine measurement around the hot spot. The sophisticated interpolation routines implemented in DASY software can find the maximum locations even in relatively coarse grids. When an Area Scan has measured all reachable points, it computes the field maximal found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing. For example, a 2 dB range is required in IEEE Standard 1528 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan). If only one Zoom Scan follows the Area Scan, then only the absolute maximum will be taken as reference. For cases where multiple maximums are detected, the number of Zoom Scans has to be increased accordingly.

Area Scan Parameters extracted from IEC/IEEE Standard 62209-1528

**Table 3 – Area scan parameters**

Parameter	DUT transmit frequency being tested	
	$f \leq 3 \text{ GHz}$	$3 \text{ GHz} < f \leq 10 \text{ GHz}$
Maximum distance between the measured points (geometric centre of the sensors) and the inner phantom surface ( $z_{M1}$ in Figure 20 in mm)	$5 \pm 1$	$\delta \ln(2)/2 \pm 0,5^{\text{a}}$
Maximum spacing between adjacent measured points in mm (see O.8.3.1) <sup>b</sup>	20, or half of the corresponding zoom scan length, whichever is smaller	$60/f$ , or half of the corresponding zoom scan length, whichever is smaller
Maximum angle between the probe axis and the phantom surface normal ( $\alpha$ in Figure 20) <sup>c</sup>	$5^{\circ}$ (flat phantom only) $30^{\circ}$ (other phantoms)	$5^{\circ}$ (flat phantom only) $20^{\circ}$ (other phantoms)
Tolerance in the probe angle	$1^{\circ}$	$1^{\circ}$

<sup>a</sup>  $\delta$  is the penetration depth for a plane-wave incident normally on a planar half-space.

<sup>b</sup> See Clause O.8 on how  $\Delta x$  and  $\Delta y$  may be selected for individual area scan requirements.

<sup>c</sup> The probe angle relative to the phantom surface normal is restricted due to the degradation in the measurement accuracy in fields with steep spatial gradients. The measurement accuracy decreases with increasing probe angle and increasing frequency. This is the reason for the tighter probe angle restriction at frequencies above 3 GHz.

### Step 3: Zoom Scan

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The Zoom Scan measures points (refer to table below) within a cube whose base faces are centered on the maxima found in a preceding area scan job within the same procedure. When the measurement is done, the Zoom Scan evaluates the averaged SAR for 1 g and 10 g and displays these values next to the job's label.

Zoom Scan Parameters extracted from IEC/IEEE Standard 62209-1528

**Table 4 – Zoom scan parameters**

Parameter	DUT transmit frequency being tested	
	$f \leq 3$ GHz	$3 \text{ GHz} < f \leq 10$ GHz
Maximum distance between the closest measured points and the phantom surface ( $z_{M1}$ in Figure 20 and Table 3, in mm)	5	$\delta \ln(2)/2$ <sup>a</sup>
Maximum angle between the probe axis and the phantom surface normal ( $\alpha$ in Figure 20)	5° (flat phantom only) 30° (other phantoms)	5° (flat phantom only) 20° (other phantoms)
Maximum spacing between measured points in the x- and y-directions ( $\Delta x$ and $\Delta y$ , in mm)	8	$24/f$ <sup>b</sup>
For uniform grids: Maximum spacing between measured points in the direction normal to the phantom shell ( $\Delta z_1$ in Figure 20, in mm)	5	$10/(f - 1)$
For graded grids: Maximum spacing between the two closest measured points in the direction normal to the phantom shell ( $\Delta z_1$ in Figure 20, in mm)	4	$12/f$
For graded grids: Maximum incremental increase in the spacing between measured points in the direction normal to the phantom shell ( $R_z = \Delta z_2/\Delta z_1$ in Figure 20)	1,5	1,5
Minimum edge length of the zoom scan volume in the x- and y-directions ( $L_z$ in O.8.3.2, in mm)	30	22
Minimum edge length of the zoom scan volume in the direction normal to the phantom shell ( $L_h$ in O.8.3.2 in mm)	30	22
Tolerance in the probe angle	1°	1°

<sup>a</sup>  $\delta$  is the penetration depth for a plane-wave incident normally on a planar half-space.

<sup>b</sup> This is the maximum spacing allowed, which might not work for all circumstances.

### Step 4: Power drift measurement

The Power Drift Measurement measures the field at the same location as the most recent power reference measurement within the same procedure, and with the same settings. The Power Drift Measurement gives the field difference in dB from the reading conducted within the last Power Reference Measurement. This allows a user to monitor the power drift of the device under test within a batch process. The measurement procedure is the same as Step 1.

### 4.3. Test Equipment

The measuring equipment used to perform the tests documented in this report has been calibrated in accordance with the manufacturers' recommendations, and is traceable to recognized national standards.

#### Dielectric Property Measurements

Name of Equipment	Manufacturer	Type/Model	Serial No.	Cal. Due Date
Dielectric Assessment Kit	SPEAG	DAK-12	1158	2025-10-21
Shorting block	SPEAG	DAK-12 Short	SM DAK 220 AD	N/A
Thermometer	LKM	DTM3000	3851	2025-07-23

#### System Check & SAR Probe & DAE & Dipole

Name of Equipment	Manufacturer	Type/Model	Serial No.	Cal. Due Date
MXG Analog Signal Generator	Keysight	N5173B	MY59101083	2025-07-23
Power Sensor	KEYSIGHT	U2000A	MY61010006	2025-07-23
Power Sensor	KEYSIGHT	U2000A	MY54260007	2025-07-25
Power Amplifier	Sambo	BA00T60W2D	S3010-0001	2026-01-02
Directional Coupler	MINI-CIRCUITS	ZMDC-30-1+	SF569102123	2025-07-24
Attenuator	KEYSIGHT	BW-N10W5+	N/A	2025-07-23
Attenuator	KEYSIGHT	8491B020	MY39272300	2025-07-23
E-Field Probe	SPEAG	EX3DV4	7313	2026-02-24
Data Acquisition Electronics	SPEAG	DAE4	1591	2026-02-18
System Validation Dipole	SPEAG	CLA -13	1015	2025-08-22
Thermometer	Lutron	MHB-382SD	AJ.45903	2026-01-06

#### Note(s):

1. All equipments were used until Cal.Due data.

## 5. Measurement Uncertainty

### Measurement Uncertainty of 9MHz to 19MHz

#### Measurement uncertainty for 9 MHz to 19 MHz

(According to IEEE 62209-1528)

a	b	c		d	e f(d,k)	f	g	h = cxf/e	i = cxg/e	k		
Uncertainty component	Reference	Tol. 1 g (±%)	Tol. 10 g (±%)	Prob. Dist.	Div.	ci (1 g)	ci (10 g)	1 g ui (± %)	10 g ui (± %)	vi		
<b>Measurement System Errors</b>												
Probe Calibration	8.4.1.1	13.3		Normal	2	1	1	6.7	6.7	∞		
Probe Calibration Drift	8.4.1.2	1.7		Rectangular	1.732	1	1	1.0	1.0	∞		
Probe Linearity	8.4.1.3	4.7		Rectangular	1.732	1	1	2.7	2.7	∞		
Broadband Signal	8.4.1.4	0.8		Rectangular	1.732	1	1	0.5	0.5	∞		
Probe Isotropy	8.4.1.5	7.6		Rectangular	1.732	1	1	4.4	4.4	∞		
Data Acquisition	8.4.1.6	0.3		Normal	1	1	1	0.3	0.3	∞		
RF Ambient	8.4.1.7	1.8		Normal	1	1	1	1.8	1.8	∞		
Probe Positioning	8.4.1.8	0.006		Normal	1	0.14	0.14	0.10	0.10	∞		
Data Processing	8.4.1.9	1.2		Normal	1	1	1	1.2	1.2	∞		
<b>Phantom and Device Errors</b>												
Conductivity (meas.)DAK	8.4.2.1	2.5		Normal	1	0.78	0.71	2.0	1.8	∞		
Conductivity (temp.)BB	8.4.2.2	5.4		Rectangular	1.732	0.78	0.71	2.4	2.2	∞		
Phantom Permittivity	8.4.2.3	14.0		Rectangular	1.732	0	0	0.0	0.0	∞		
Distance DUT -TSL	8.4.2.4	2.0		Normal	1	2	2	4.0	4.0	∞		
Device Positioning	8.4.2.5	1.0	2.3	Normal	1	1	1	1.0	2.3	40		
Device Holder	8.4.2.6	3.6		Normal	1	1	1	3.6	3.6	∞		
DUT Modulation	8.4.2.7	2.4		Rectangular	1.732	1	1	1.4	1.4	∞		
Time-average SAR	8.4.2.8	1.7		Rectangular	1.732	1	1	1.0	1.0	∞		
DUT drift	8.4.2.9	5.0		Normal	1	1	1	5.0	5.0	∞		
<b>Correction to the SAR results</b>												
Deviation to Target	8.4.3.1	1.9		Normal	1	1	0.84	1.9	1.6	∞		
Combined Standard Uncertainty $U_c(y) =$	RSS							12.16	12.23			
Expanded Uncertainty $U$ , Coverage Factor = 2, > 95 % Confidence =							<b>24.33</b>	<b>24.47</b>				

## 5.1. DECISION RULE

Measurement Uncertainty is not applied when providing statements of conformity in accordance with IEC Guide 115:2023, 4.3.3.

## 6. Device Under Test (DUT) Information

### 6.1. DUT Description

Device Dimension	Refer to Appendix A.		
Test Sample information	No. 1	S/N Proto Type	Notes SAR

### 6.2. Wireless Technologies

Wireless technologies	Frequency bands	Operating mode	Duty Cycle used for SAR testing
NFC	13.56 MHz	Factory Test Mode	100%

## 7. RF Exposure Conditions (Test Configurations)

Refer to Appendix A for the specific details of the antenna-to-antenna and antenna-to-edge(s) distances.

### Folder Closed (Phablet mode)

Wireless technologies	Antennaa	DUT-to-User Separation	Test Positions					
			Rear	Front	Top	Left	Bottom	Right
NFC	NFC Ant.	0 mm	No	Yes	Yes	Yes	Yes	Yes

### **Notes:**

This device is a WPT (including NFC) installed in a vehicle. The Rear side is generally not in contact with the user. So Rear SAR test excluded.

## 8. Dielectric Property Measurements & System Check

### 8.1. Dielectric Property Measurements

The temperature of the tissue-equivalent medium used during measurement must also be within 18°C to 25°C and within  $\pm 2^\circ\text{C}$  of the temperature when the tissue parameters are characterized.

The dielectric parameters must be measured before the tissue-equivalent medium is used in a series of SAR measurements. The Tissue Dielectric parameters (100MHz to 6GHz) should be re-measured after each 3 – 4 days of use; or earlier if the dielectric parameters can become out of tolerance; for example, when the parameters are marginal at the beginning of the measurement series.

Tissue dielectric parameters were measured at the low, middle and high frequency of each operating frequency range of the test device.

For The Tissue Dielectric parameters (4MHz to 30MHz). The parameters must be measured before 24 hours.

#### Tissue Dielectric Parameters (4MHz to 30MHz)

Target Frequency (MHz)	Head	
	$\epsilon_r$	$\sigma$ (S/m)
4	55.0	0.75
13	55.0	0.75
30	55.0	0.75

#### IEC\_IEEE Std 62209-1528 : 2020

Refer to Table 2 within the IEC\_IEEE Std 62209-1528 : 2020.

#### Dielectric Property Measurements Results:

##### SAR 4 Room

Date	Freq. (MHz)	Liquid Parameters			Measured	Target	Delta (%)	Limit $\pm$ (%)
2025-06-19	Head 13	e'	56.6100	Relative Permittivity ( $\epsilon_r$ ):	56.61	55.00	2.93	5
		e"	1018.1000	Conductivity ( $\sigma$ ):	0.74	0.75	-1.88	5
	Head 12	e'	56.7200	Relative Permittivity ( $\epsilon_r$ ):	56.72	55.00	3.13	5
		e"	1102.0100	Conductivity ( $\sigma$ ):	0.74	0.75	-1.96	5
	Head 14	e'	56.5300	Relative Permittivity ( $\epsilon_r$ ):	56.53	55.00	2.78	5
		e"	945.9700	Conductivity ( $\sigma$ ):	0.74	0.75	-1.82	5

## 8.2. System Check

SAR system verification is required to confirm measurement accuracy, according to the tissue dielectric media, probe calibration points and other system operating parameters required for measuring the SAR of a test device. The system verification must be performed for each frequency band and within the valid range of each probe calibration point required for testing the device. The same SAR probe(s) and tissue-equivalent media combinations used with each specific SAR system for system verification must be used for device testing. When multiple probe calibration points are required to cover substantially large transmission bands, independent system verifications are required for each probe calibration point. A system verification must be performed before each series of SAR measurements using the same probe calibration point and tissue-equivalent medium. Additional system verification of 100MHz to 6GHz frequency range should be considered according to the conditions of the tissue-equivalent medium and measured tissue dielectric parameters, typically every three to four days when the liquid parameters are re-measured or sooner when marginal liquid parameters are used at the beginning of a series of measurements.

For The System verification of 4MHz to 30MHz frequency range, The System verification must be performed before 24 hours.

### System Performance Check Measurement Conditions (100MHz to 6GHz):

- The measurements were performed in the flat section of the TWIN SAM or ELI phantom, shell thickness: 2.0  $\pm 0.2$  mm (bottom plate) filled with Body or Head simulating liquid of the following parameters.
- The depth of tissue-equivalent liquid in a phantom must be  $\geq 15.0$  cm for SAR measurements  $\leq 3$  GHz and  $\geq 10.0$  cm for measurements  $> 3$  GHz.
- The DASY system with an E-Field Probe was used for the measurements.
- The dipole was mounted on the small tripod so that the dipole feed point was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10 mm (above 1 GHz) and 15 mm (below 1 GHz) from dipole center to the simulating liquid surface.
- The coarse grid with a grid spacing of 15 mm was aligned with the dipole.  
For 5 GHz band - The coarse grid with a grid spacing of 10 mm was aligned with the dipole.
- Special 7x7x7 (below 3 GHz) and/or 8x8x7 (above 3 GHz) fine cube was chosen for the cube.
- Distance between probe sensors and phantom surface was set to 2.5 mm.  
For 5 GHz band - Distance between probe sensors and phantom surface was set to 1.4 mm
- The dipole input power (forward power) was 100 mW.
- The results are normalized to 1 W input power.

### System Performance Check Measurement Conditions (4MHz to 30MHz):

- The measurements were performed in the flat section of the TWIN SAM or ELI phantom, shell thickness: 2.0  $\pm 0.2$  mm (bottom plate) filled with Body or Head simulating liquid of the following parameters.
- The depth of tissue-equivalent liquid in a phantom must be  $\geq 15.0$  cm for SAR measurements
- The DASY system with an E-Field Probe was used for the measurements.
- The CLA(Confined Loop Antennas) was mounted on the small tripod so that the CLA feed point was positioned below the center marking of the flat phantom section and the CLA was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 0 mm separation distance from CLA center to the Phantom surface.
- The CLA input power (forward power) was 100 mW.
- The results are normalized to 1 W input power.

### Reference Target SAR Values

The reference SAR values can be obtained from the calibration certificate of system validation dipoles.

System Dipole	Serial No.	Cal. Date	Cal.due date	Target SAR Values (W/kg)	
				1g/10g	Head
CLA-13	1015	2024-8-22	2025-8-22	1g	0.537
				10g	0.333

### System Check Results

The 1-g and 10-g SAR measured with a reference dipole, using the required tissue-equivalent medium at the test frequency, must be within 10% of the manufacturer calibrated dipole SAR target.

#### SAR 4 Room

Date Tested	System Dipole		T.S. Liquid		Measured Results		Target (Ref. Value)	Delta ±10 %	Plot No.
	Type	Serial #			Zoom Scan to 100 mW	Normalize to 1 W			
2025-6-19	CLA-13	1015	Head	1g	0.05	0.5	0.54	0.56	1
				10g	0.03	0.3	0.33	-0.90	

## 9. Measured SAR Results

### 9.1. NFC

Antenna	Frequency Band	RF Exposure Conditions	Dist. (mm)	Test Position	Freq. (MHz)	1-g SAR (W/kg)	Plot No.
						Meas.	
NFC	13.56MHz	Standalone	0	Front	13.56	0.026	1
				Top	13.56	0.000	
				Bottom	13.56	0.000	
				Left	13.56	0.000	
				Right	13.56	0.000	

## Appendices

Refer to separated files for the following appendixes.

**S-4791776982-S2 FCC SAR App A Test photos**

**S-4791776982-S2 FCC SAR App B Test Plots**

**S-4791776982-S2 FCC SAR App C System Plots**

**S-4791776982-S2 FCC SAR App D SAR Tissue**

**S-4791776982-S2 FCC SAR App E Probe Certi**

**S-4791776982-S2 FCC SAR App F Source Certi**

**END OF REPORT**