



Allengers
Medical Systems Limited

FDA Hall, Unit-2, Bhankarpur, Mubarakpur Road,
Derabassi, Distt Mohali-140507, India



Flat Panel Detector
G4336RWC
22-26V $\approx$ 1.5A
FCC ID:2A77600002

UDI

SN



IPX6

Rx Only

NON
STERILE



www.allengers.com



Allengers
Medical Systems Limited

FDA Hall, Unit-2, Bhankarpur, Mubarakpur Road,
Derabassi, Distt Mohali-140507, India



Flat Panel Detector
G4336RWG
22-26V $\approx$ 1.5A
FCC ID:2A77600002

UDI

SN



IPX6

Rx Only

NON
STERILE



www.allengers.com



Allengers
Medical Systems Limited

FDA Hall, Unit-2, Bhankarpur, Mubarakpur Road,
Derabassi, Distt Mohali-140507, India



Flat Panel Detector
T4336RWC
22-26V $\approx$ 1.5A
FCC ID:2A77600002

UDI

SN



IPX6

Rx Only

NON
STERILE



www.allengers.com



Allengers
Medical Systems Limited

FDA Hall, Unit-2, Bhankarpur, Mubarakpur Road,
Derabassi, Distt Mohali-140507, India



Flat Panel Detector
T4336RWG
22-26V $\approx$ 1.5A
FCC ID:2A77600002

UDI

SN



IPX6

Rx Only

NON
STERILE



www.allengers.com





Allengers
Medical Systems Limited

FDA Hall, Unit-2, Bhankarpur, Mubarakpur Road,
Derabassi, Distt Mohali-140507, India



Flat Panel Detector
G4343RWC
22-26V === 1.5A
FCC ID:2A77600002

UDI

SN



IPX6

Rx Only

NON
STERILE

MAX
300 Kg
660 lb



www.allengers.com



Allengers
Medical Systems Limited

FDA Hall, Unit-2, Bhankarpur, Mubarakpur Road,
Derabassi, Distt Mohali-140507, India



Flat Panel Detector
G4343RWG
22-26V === 1.5A
FCC ID:2A77600002

UDI

SN



IPX6

Rx Only

NON
STERILE


MAX
300 Kg
660 lb



www.allengers.com



Identification label

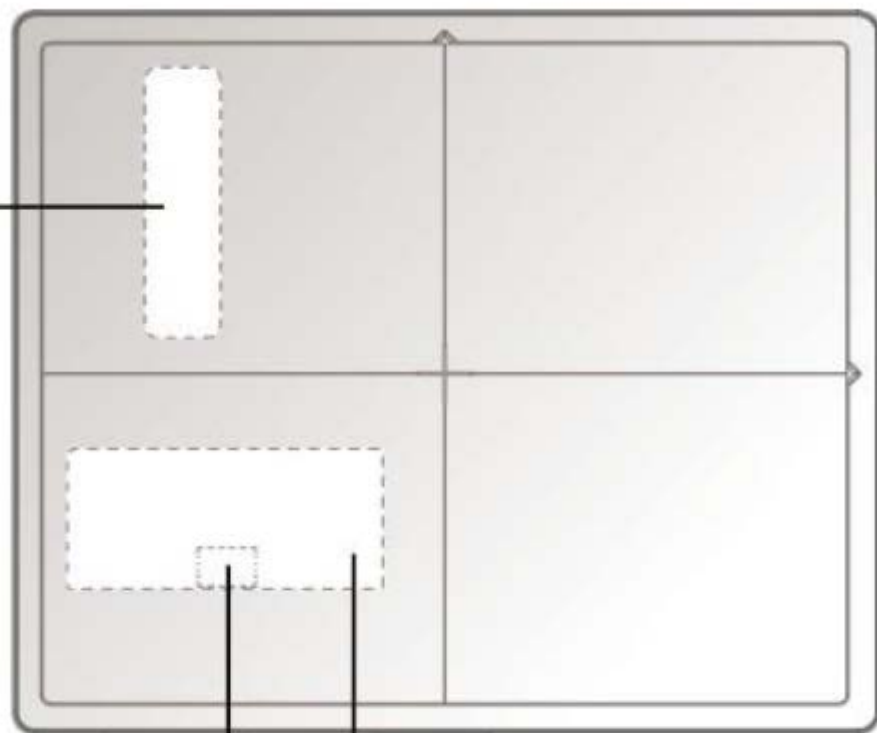

Battery label

Battery polarity label