


1.11 D2600V2 - SN 1158

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Client: SGS-CN		Certificate No: Z22-60108	
CALIBRATION CERTIFICATE			
Object: D2600V2 - SN: 1158			
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits			
Calibration date: March 31, 2022			
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards		ID # Cal Date (Calibrated by Certificate No.) Scheduled Calibration	
Power Meter NRP2		102377 24-Sep-21 (CTTL No.J21X08326) Sep-22	
Power sensor NRP8S		104291 24-Sep-21 (CTTL No.J21X08326) Sep-22	
Reference Probe EX3DVA		SN 7307 26-May-21(SPEAG.No.EX3-7307_May21) May-22	
DAE4		SN 1556 12-Jan-22(CTTL-SPEAG.No.Z22-60007) Jan-23	
Secondary Standards		ID # Cal Date (Calibrated by Certificate No.) Scheduled Calibration	
Signal Generator E4438C		MY49071430 13-Jan-22 (CTTL No.J22X00406) Jan-23	
Network Analyzer E5071C		MY48110673 14-Jan-22 (CTTL No.J22X00406) Jan-23	
Calibrated by: Zhao Jing SAR Test Engineer		Signature	
Reviewed by: Lin Hao SAR Test Engineer		Signature	
Approved by: Qi Dianyan SAR Project Leader		Signature	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60108		Page 1 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1.		Appendix (Additional assessments outside the scope of CNAS L0570)	
DASY Version: DASY2		Antenna Parameters with Head TSL	
Extrapolation: Advanced Extrapolation		Impedance, transformed to feed point: 49.90-6.49jΩ	
Phantom: Triple Flat Phantom 5.1C		Return Loss: -23.8dB	
Distance Dipole Center - TSL: 10 mm with Spacer		General Antenna Parameters and Design	
Zoom Scan Resolution: 0.1, 0.2, 0.5 mm		Electrical Delay (one direction): 1.053 ns	
Frequency: 2600 MHz ± 1 MHz		After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.	
Head TSL parameters The following parameters and calculations were applied:		The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.	
Nominal Head TSL parameters: 22.0 °C 39.0 1.96 mho/m		Additional EUT Data	
Measured Head TSL parameters: (22.0 ± 0.2) °C 36.7 ± 6 % 1.96 mho/m ± 6 %		Manufactured by: SPEAG	
Head TSL temperature change during test: <1.0 °C ---			
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL			
SAR measured: 250 mW input power 13.7 W/kg			
SAR for nominal Head TSL parameters: normalized to 1W 54.8 W/kg ± 18.8 % (k=2)			
SAR averaged over 10 cm² (10 g) of Head TSL			
SAR measured: 250 mW input power 6.12 W/kg			
SAR for nominal Head TSL parameters: normalized to 1W 24.6 W/kg ± 18.7 % (k=2)			
Certificate No: Z22-60108		Page 3 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Glossary:		TSL: tissue simulating liquid	
ConvF: sensitivity in TSL / NORMx.y.z			
N/A: not applicable or not measured			
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/S System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60108		Page 2 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1.		Appendix (Additional assessments outside the scope of CNAS L0570)	
DASY Version: DASY2		Antenna Parameters with Head TSL	
Extrapolation: Advanced Extrapolation		Impedance, transformed to feed point: 49.90-6.49jΩ	
Phantom: Triple Flat Phantom 5.1C		Return Loss: -23.8dB	
Distance Dipole Center - TSL: 10 mm with Spacer		General Antenna Parameters and Design	
Zoom Scan Resolution: 0.1, 0.2, 0.5 mm		Electrical Delay (one direction): 1.053 ns	
Frequency: 2600 MHz ± 1 MHz		After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.	
Head TSL parameters The following parameters and calculations were applied:		The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.	
Nominal Head TSL parameters: 22.0 °C 39.0 1.96 mho/m		Additional EUT Data	
Measured Head TSL parameters: (22.0 ± 0.2) °C 36.7 ± 6 % 1.96 mho/m ± 6 %		Manufactured by: SPEAG	
Head TSL temperature change during test: <1.0 °C ---			
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL			
SAR measured: 250 mW input power 13.7 W/kg			
SAR for nominal Head TSL parameters: normalized to 1W 54.8 W/kg ± 18.8 % (k=2)			
SAR averaged over 10 cm² (10 g) of Head TSL			
SAR measured: 250 mW input power 6.12 W/kg			
SAR for nominal Head TSL parameters: normalized to 1W 24.6 W/kg ± 18.7 % (k=2)			
Certificate No: Z22-60108		Page 3 of 6	

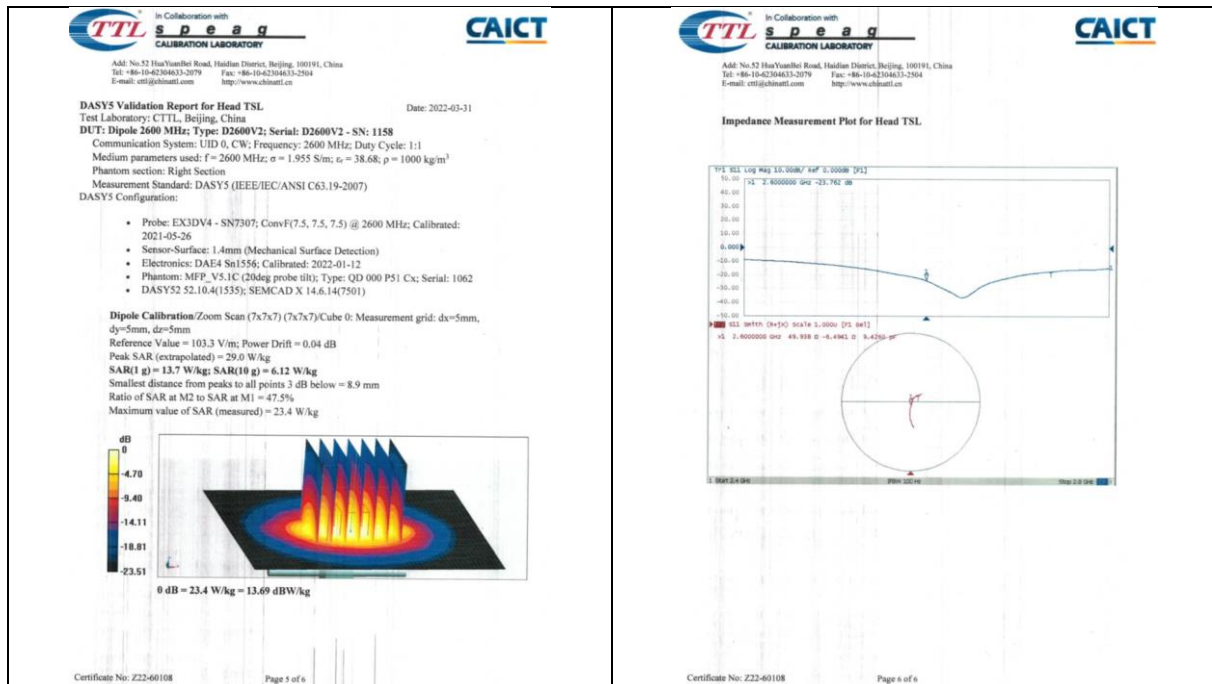

1.12 D5GHZV2 - SN 1095

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Client: SGS-CN Certificate No: Z22-60187

CALIBRATION CERTIFICATE

Object: D5GHZV2 - SN: 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21008328)	Sep-22
Power sensor NRP8S	104201	24-Sep-21 (CTTL No.J21008328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464, Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22000408)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22000406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyan SAR Project Leader

Issued: June 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Glossary:

TSL: Issue simulating liquid

ComF: sensitivity in TSL / NORMx,y,z

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 2 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62362117 E-mail: cnlg@chinaetl.com http://www.caict.ac.cn			
Measurement Conditions GSEY system configuration, as far as not given on page 1.			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz		
Head TSL parameters at 5200MHz The following parameters and calculations were applied.			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5200MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	7.79 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	77.8 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.22 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)	
Certificate No: Z22-60187 Page 3 of 10			

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62362117 E-mail: cnlg@chinaetl.com http://www.caict.ac.cn			
Head TSL parameters at 5300MHz The following parameters and calculations were applied.			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5300MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	7.94 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.27 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)	
Head TSL parameters at 5500MHz The following parameters and calculations were applied.			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.8	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5500MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	8.29 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	82.6 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.34 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)	
Certificate No: Z22-60187 Page 4 of 10			

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62362117 E-mail: cnlg@chinaetl.com http://www.caict.ac.cn			
Head TSL parameters at 5600MHz The following parameters and calculations were applied.			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5600MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	8.12 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.30 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)	
Head TSL parameters at 5800MHz The following parameters and calculations were applied.			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5800MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	7.71 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.16 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	21.6 W/kg ± 24.2 % (k=2)	
Certificate No: Z22-60187 Page 5 of 10			

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62362117 E-mail: cnlg@chinaetl.com http://www.caict.ac.cn			
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL at 5200MHz			
Impedance, transformed to feed point	48.1D-5.03jΩ		
Return Loss	-23.6dB		
Antenna Parameters with Head TSL at 5300MHz			
Impedance, transformed to feed point	47.8D-2.42jΩ		
Return Loss	-28.5dB		
Antenna Parameters with Head TSL at 5500MHz			
Impedance, transformed to feed point	50.3D-4.26jΩ		
Return Loss	-27.4dB		
Antenna Parameters with Head TSL at 5600MHz			
Impedance, transformed to feed point	54.5D-4.80jΩ		
Return Loss	-24.0dB		
Antenna Parameters with Head TSL at 5800MHz			
Impedance, transformed to feed point	51.5D-5.61jΩ		
Return Loss	-24.9dB		
Certificate No: Z22-60187 Page 6 of 10			





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

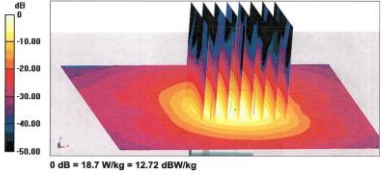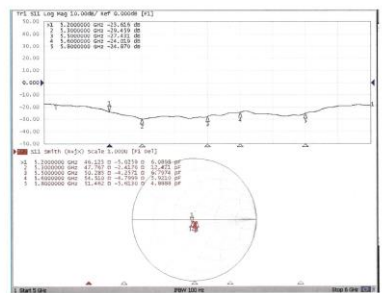In Collaboration with TTL s p e a q CALIBRATION LABORATORY CAICT Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62502117 E-mail: cti@chinaetl.com http://www.caict.ac.cn General Antenna Parameters and Design Electrical Delay (one direction) 1.101 ns After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data Manufactured by SPEAG Certificate No: Z22-60187 Page 7 of 10	In Collaboration with TTL s p e a q CALIBRATION LABORATORY CAICT Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62502117 E-mail: cti@chinaetl.com http://www.caict.ac.cn DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-06-01 DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095 Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: $f = 5200 \text{ MHz}$; $\sigma = 4.62 \text{ S/m}$; $\epsilon_r = 35.19$; $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: $f = 5300 \text{ MHz}$; $\sigma = 4.73 \text{ S/m}$; $\epsilon_r = 35.19$; $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: $f = 5500 \text{ MHz}$; $\sigma = 4.939 \text{ S/m}$; $\epsilon_r = 34.83$; $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: $f = 5600 \text{ MHz}$; $\sigma = 5.051 \text{ S/m}$; $\epsilon_r = 34.89$; $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: $f = 5800 \text{ MHz}$; $\sigma = 5.247 \text{ S/m}$; $\epsilon_r = 34.42$; $\rho = 1000 \text{ kg/m}^3$ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA64 Sn1556; Calibrated: 2022-01-12 - Phantom: MPF_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 18.3 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg Certificate No: Z22-60187 Page 8 of 10
In Collaboration with TTL s p e a q CALIBRATION LABORATORY CAICT Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62502117 E-mail: cti@chinaetl.com http://www.caict.ac.cn Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.28 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.2 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg  Certificate No: Z22-60187 Page 9 of 10	In Collaboration with TTL s p e a q CALIBRATION LABORATORY CAICT Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62502117 E-mail: cti@chinaetl.com http://www.caict.ac.cn Impedance Measurement Plot for Head TSL  Certificate No: Z22-60187 Page 10 of 10

2 DAE4 - SN 1245

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9770 www.spgs.ch, info@spgs.ch s p e a g IMPORTANT NOTICE USAGE OF THE DAE4 The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points: Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE to wear out. Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an anti-static bag. This anti-static bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside. E-stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements. Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect. DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file. Important Note: Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer. Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure. Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE. TN_EH190306AE_DAE4.docx 07.03.2019	Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108 Client: SGS-CN (Auden) Certificate No.: DAE4-1245_May22 CALIBRATION CERTIFICATE Object: DAE4 - SD 000 D04 BM - SN: 1245 Calibration procedure(s): QA CAL-06 v30 Calibration procedure for the data acquisition electronics (DAE) Calibration date: May 30, 2022 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3) °C and humidity < 70%. Calibration Equipment used (MATE critical for calibration) <table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Kelvin Multimeter Type 2001</td><td>SN: 0810276</td><td>31-Aug-21 (No.31368)</td><td>Aug-22</td></tr></tbody></table> <table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Check Date (in house)</th><th>Scheduled Check</th></tr></thead><tbody><tr><td>Auto DAE Calibration Unit</td><td>SE LWS 003 AA 1001</td><td>24-Jan-22 (in house check)</td><td>In house check: Jan-23</td></tr><tr><td>Calibrator Blue V2.1</td><td>SE LWS 006 AA 1002</td><td>24-Jan-22 (in house check)</td><td>In house check: Jan-23</td></tr></tbody></table> Calibrated by: Dominique Stettin Function: Laboratory Technician Signature: <i>[Signature]</i> Approved by: Ben Kohn Technical Manager Signature: <i>[Signature]</i> This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: May 30, 2022 Certificate No: DAE4-1245_May22 Page 1 of 5	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Kelvin Multimeter Type 2001	SN: 0810276	31-Aug-21 (No.31368)	Aug-22	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Auto DAE Calibration Unit	SE LWS 003 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23	Calibrator Blue V2.1	SE LWS 006 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																		
Kelvin Multimeter Type 2001	SN: 0810276	31-Aug-21 (No.31368)	Aug-22																		
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																		
Auto DAE Calibration Unit	SE LWS 003 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23																		
Calibrator Blue V2.1	SE LWS 006 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23																		
Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108 Glossary DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system. Methods Applied and Interpretation of Parameters • DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. • Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. • The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty. • DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. • Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. • Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage. • AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage. • Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. • Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance. • Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement. • Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. • Power consumption: Typical value for information. Supply currents in various operating modes. Certificate No: DAE4-1245_May22 Page 2 of 5	DC Voltage Measurement AD - Converter Resolution nominal High Range: 1LSB = 6.1 μV, full range = -190...+320 mV Low Range: 1LSB = 61 μV, full range = -1...+3 mV DASY measurement parameters: Auto Zero-Time: 3 sec; Measuring time: 3 sec <table border="1"><thead><tr><th>Calibration Factors</th><th>X</th><th>Y</th><th>Z</th></tr></thead><tbody><tr><td>High Range</td><td>405.265 ± 0.02% (k=2)</td><td>403.974 ± 0.02% (k=2)</td><td>406.092 ± 0.02% (k=2)</td></tr><tr><td>Low Range</td><td>3.99534 ± 1.50% (k=2)</td><td>3.99508 ± 1.50% (k=2)</td><td>4.01015 ± 1.50% (k=2)</td></tr></tbody></table> Connector Angle <table border="1"><thead><tr><th>Connector Angle to be used in DASY system</th><th>30.0° ± 1°</th></tr></thead></table> Certificate No: DAE4-1245_May22 Page 3 of 5	Calibration Factors	X	Y	Z	High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)	Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)	Connector Angle to be used in DASY system	30.0° ± 1°						
Calibration Factors	X	Y	Z																		
High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)																		
Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)																		
Connector Angle to be used in DASY system	30.0° ± 1°																				



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	19994.45	1.52	0.00
Channel X - Input	20004.58	2.22	0.01
Channel X + Input	-20001.14	1.12	-0.01
Channel Y + Input	19994.72	1.58	0.00
Channel Y - Input	20001.22	-1.00	-0.00
Channel Y + Input	-20003.05	-1.57	0.01
Channel Z + Input	19992.44	0.19	0.00
Channel Z - Input	20003.09	0.58	0.00
Channel Z + Input	-20001.73	-0.27	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2001.91	0.41	0.02
Channel X - Input	202.54	0.65	0.32
Channel X + Input	-197.86	0.07	-0.04
Channel Y + Input	2002.05	0.58	0.03
Channel Y - Input	201.27	-0.57	-0.28
Channel Y + Input	-196.23	-0.06	0.03
Channel Z + Input	2001.96	0.08	0.00
Channel Z - Input	200.09	-1.53	-0.76
Channel Z + Input	-199.85	-1.57	0.79

2. Common mode sensitivity

Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X	-5.87	-7.69
-200	9.12	7.79
Channel Y	-8.68	-9.28
-200	8.52	6.36
Channel Z	-5.36	-5.60
-200	3.58	3.06

3. Channel separation

Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	4.07
Channel Y	200	9.36	-
Channel Z	200	7.14	-

Certificate No: DAE4-1245, May22

Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15984	17040
Channel Y	16562	16768
Channel Z	16035	15668

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input (mV)	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	1.00	-0.15	1.93	0.45
Channel Y	-0.18	-1.28	0.94	0.45
Channel Z	-0.58	-2.81	0.58	0.60

6. Input Offset Current

Nominal input circuitry offset current on all channels: <25nA

7. Input Resistance (Typical values for information)

	Zeroing (Ohm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+8	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1245, May22

Page 5 of 5

3 EX3DV4 - SN 7346

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zugstrasse 6, 8664 Zurich, SwitzerlandS Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration ServiceAccredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client: Auden

Certificate No: EX3-7346_Mar22

CALIBRATION CERTIFICATE

Object: EX3DV4 - SN 7346
Calibration procedure(s): QA CAL-01 v8, QA CAL-14 v6, QA CAL-23 v5, QA CAL-25 v7
Calibration procedure for dosimetric E-field probes

Calibration date: March 30, 2022

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closest laboratory facility: environment temperature (22 ± 3) °C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration):

Primary Standards	ISI	Cal Date (Certificate No.)	Scheduled Calibration
Power meter MNP	SN 10478	08-Apr-21 (No. 217-02501-02502)	Apr-22
Power sensor MNP-291	SN 10304	08-Apr-21 (No. 217-02501)	Apr-22
Power sensor MNP-291	SN 10343	08-Apr-21 (No. 217-02502)	Apr-22
Reference 20 dB attenuator	SN C2253 (20)	08-Apr-21 (No. 217-02503)	Apr-22
DAEA	SN 460	13-Dec-21 (No. DAE4-489, 04031)	Dec-22
Reference Probe (S3302)	SN 3013	27-Dec-21 (No. E53-3013, Dec21)	Dec-22

Secondary Standards	ISI	Check Date (in house)	Scheduled Calibration
Power meter E4413B	SN G84123074	08-Apr-21 (in house check Jun-20)	In house check Jun-22
Power sensor E4413A	SN MY4148887	08-Apr-21 (in house check Jun-20)	In house check Jun-22
Power sensor E4413A	SN 40011816	08-Apr-21 (in house check Jun-20)	In house check Jun-22
RF generator HP 8446C	SN US340101709	04-Apr-20 (in house check Jun-20)	In house check Jun-22
Network Analyzer E5730A	SN US41030477	31-Mar-14 (in house check Dec-20)	In house check Dec-22

Calibrated by: Name: Sven Kuhn, Function: Laboratory Technician, Signature: [Signature]
Approved by: Sven Kuhn, Deputy Manager, Signature: [Signature]

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-7346_Mar22

Page 1 of 24

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zugstrasse 6, 8664 Zurich, SwitzerlandS Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration ServiceAccredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary:

TSL: Issue simulating liquid
NORM_{M,y,z}: sensitivity in free space
ConF: sensitivity in TSL / NORM_{M,y,z}
DCP: diode compression point
CF: crest factor (10µs, cycle) of the RF signal
A, B, C, D: modulation dependent linearization parameters
Polarization: ϕ rotation around probe axis
Polarization: θ rotation around an axis that is in the plane normal to probe axis (at measurement center).
i.e., θ = 0 is normal to probe axis
Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62233-1:2018, Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1:333, Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz); October 2020
b) KOB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{M,y,z}: Assessed for E-field polarization $\theta = 0$ if $f < 900$ MHz in TEM-cell; $f > 900$ MHz: R22 waveguide. NORM_{M,y,z} are only intermediate values, i.e., the uncertainties of NORM_{M,y,z} do not affect the E-field uncertainty inside TSL (see below ConF).
- NORM_{M,y,z} = NORM_{M,y,z} * Frequency response (see Frequency Response Chart). This linearization is implemented in DASY4 software version later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConF.
- DCP_{M,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAC: PAC is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A_{M,y,z}, B_{M,y,z}, C_{M,y,z}, D_{M,y,z}, V_{M,y,z}: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. V_{M,y,z} is the maximum calibration range expressed in RMS voltage across the diode.
- ConF and Boundary Effect Parameters: Assessed in far phantom using E-field or Temperature Transfer Standard for $f < 900$ MHz and inside waveguide using analytical field distributions based on power measurements for $f > 900$ MHz. The same values are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are implemented in DASY4 software to ensure the accuracy close to the boundary. The separability in TSL corresponds to NORM_{M,y,z} * ConF, whereby the uncertainty corresponds to that given for ConF. A frequency dependent ConF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy / DCP deviation from isotropy: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM_M (no uncertainty required).

Certificate No: EX3-7346_Mar22

Page 2 of 24



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300


t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

EX3DV4 - SN:7346									
March 30, 2022									
DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346									
Basic Calibration Parameters									
Norm. $\mu V/(V/m)^2$		Sensor X		Sensor Y		Sensor Z		Unc. (k=2)	
DCP (mV) ²		0.45		0.47		0.61		± 10.1 %	
		101.4		106.0		106.9			
Calibration Results for Modulation Response									
UID	Communication System Name	A	B	C	D	VR	Max. dev.	Max. Unc ¹	
		dB	dB-μV	dB	dB	mV			
0	CW	X: 0.00	0.00	1.00	0.00	143.5	± 3.5 %	± 4.1 %	
		Y: 0.00	0.00	1.00	0.00	139.3			
		Z: 0.00	0.00	1.00	0.00	139.0			
10035-AAA	Pulse Waveform (200Hz, 10%)	X: 3.33	68.90	11.66	10.00	60.0	± 3.5 %	± 9.6 %	
		Y: 4.03	79.70	12.35	60.0				
		Z: 1.63	61.25	6.76	60.0				
10035-AAA	Pulse Waveform (200Hz, 20%)	X: 3.30	79.65	11.31	6.99	85.0	± 2.4 %	± 9.6 %	
		Y: 11.31	81.32	14.72	85.0				
		Z: 5.83	69.90	5.11	85.0				
10035-AAA	Pulse Waveform (200Hz, 40%)	X: 7.41	79.85	12.51	3.98	95.0	± 2.7 %	± 9.6 %	
		Y: 26.93	81.42	15.51	95.0				
		Z: 0.18	138.38	0.01	95.0				
10035-AAA	Pulse Waveform (200Hz, 60%)	X: 22.77	71.13	9.52	2.32	120.0	± 1.7 %	± 9.6 %	
		Y: 20.90	91.58	16.29	120.0				
		Z: 7.84	138.51	16.47	120.0				
10035-AAA	GRK Waveform, 1 MHz	X: 1.47	64.88	13.82	1.00	150.0	± 4.2 %	± 9.6 %	
		Y: 1.96	66.27	14.65	0.00	150.0			
		Z: 0.43	67.88	11.05	150.0				
10088-AAA	GRK Waveform, 10 MHz	X: 1.96	66.27	14.65	0.00	150.0	± 1.1 %	± 9.6 %	
		Y: 2.08	67.33	15.38	150.0				
		Z: 2.41	64.75	13.18	150.0				
10088-AAA	64-QAM Waveform, 100 MHz	X: 2.43	68.51	18.25	3.01	150.0	± 1.0 %	± 9.6 %	
		Y: 2.41	68.51	18.25	150.0				
		Z: 1.70	64.72	15.99	150.0				
10088-AAA	64-QAM Waveform, 40 MHz	X: 3.38	66.29	15.25	0.00	150.0	± 2.0 %	± 9.6 %	
		Y: 3.38	66.29	15.25	150.0				
		Z: 2.70	65.72	14.74	150.0				
10014-AAA	WLAN CDDF, 64-QAM, 40MHz	X: 4.11	69.35	17.77	0.00	150.0	± 3.6 %	± 9.6 %	
		Y: 4.70	65.54	15.41	150.0				
		Z: 3.83	66.16	15.28	150.0				
Note: For details on UID parameters see Appendix									
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.									
* The uncertainties of Norm. V, Z do not affect the E-field uncertainty within T10, (see Pages 5 and 6)									
* Numerical simulation parameter, uncertainty not required									
* Uncertainty is determined using the noise deviation from linear response applying rectangular distribution and is expressed for the square of the field value.									
Certificate No: EX3-7346_Mar22 Page 3 of 34									

EX3DV4 - SN:7346									
March 30, 2022									
DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346									
Sensor Model Parameters									
C1	C2	a	T1	T2	T3	T4	T5	T6	
IP	IP	V ²	ms.V ²	ms.V ²	ms	V ²	V ²	V ²	
X	39.2	291.80	35.10	5.63	5.02	1.42	0.12	1.01	
Y	37.1	270.84	34.12	6.29	6.01	1.82	0.05	1.01	
Z	9.7	69.74	33.37	4.96	0.00	4.94	0.61	0.00	1.00
Other Probe Parameters									
Sensor Arrangement									
Triangular									
Connector Angle (°)									
-166.1									
Mechanical Surface Detection Mode									
enabled									
Optical Surface Detection Mode									
disabled									
Probe Overall Length									
337 mm									
Probe Body Diameter									
10 mm									
Tip Length									
9 mm									
Tip Diameter									
2.5 mm									
Probe Tip to Sensor X Calibration Point									
1 mm									
Probe Tip to Sensor Y Calibration Point									
1 mm									
Probe Tip to Sensor Z Calibration Point									
1 mm									
Recommended Measurement Distance from Surface									
1.4 mm									
Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.									
Certificate No: EX3-7346_Mar22 Page 4 of 34									

EX3DV4 - SN:7346									
March 30, 2022									
DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346									
Calibration Parameter Determined in Head Tissue Simulating Media									
f (MHz)	Relative Permittivity ¹	Conductivity (S/m) ²	ConvF X	ConvF Y	ConvF Z	Alpha ³	Depth ⁴ (mm)	Unc. (k=2)	
750	41.9	0.69	10.56	10.56	10.56	0.55	0.85	± 12.0 %	
835	41.5	0.90	10.12	10.12	10.12	0.42	0.96	± 12.0 %	
900	41.5	0.97	10.10	10.10	10.10	0.53	0.80	± 12.0 %	
1430	40.5	1.20	9.26	9.26	9.26	0.50	0.80	± 12.0 %	
1750	40.1	1.37	8.63	8.63	8.63	0.34	0.86	± 12.0 %	
1900	40.0	1.40	8.48	8.48	8.48	0.35	0.86	± 12.0 %	
2000	40.0	1.40	8.35	8.35	8.35	0.34	0.86	± 12.0 %	
2300	39.5	1.67	7.86	7.86	7.86	0.39	0.90	± 12.0 %	
2450	39.2	1.80	7.63	7.63	7.63	0.41	0.90	± 12.0 %	
2600	39.0	1.96	7.33	7.33	7.33	0.44	0.90	± 12.0 %	
3300	38.2	2.71	7.15	7.15	7.15	0.30	1.35	± 13.1 %	
3500	37.8	2.81	7.14	7.14	7.14	0.30	1.35	± 13.1 %	
3750	37.7	3.12	6.85	6.85	6.85	0.30	1.35	± 13.1 %	
3900	37.5	3.32	6.71	6.71	6.71	0.40	1.60	± 13.1 %	
4100	37.2	3.53	6.58	6.58	6.58	0.40	1.60	± 13.1 %	
4200	37.1	3.63	6.30	6.30	6.30	0.40	1.70	± 13.1 %	
4400	36.9	3.64	6.24	6.24	6.24	0.40	1.70	± 13.1 %	
4600	36.7	4.04	6.11	6.11	6.11	0.40	1.70	± 13.1 %	
4800	36.4	4.25	6.08	6.08	6.08	0.40	1.80	± 13.1 %	
4900	36.3	4.40	5.84	5.84	5.84	0.40	1.80	± 13.1 %	
5200	36.0	4.66	5.25	5.25	5.25	0.40	1.80	± 13.1 %	
5300	35.9	4.78	5.12	5.12	5.12	0.40	1.80	± 13.1 %	
5500	35.6	4.96	4.85	4.85	4.85	0.40	1.80	± 13.1 %	
5600	35.5	5.07	4.70	4.70	4.70	0.40	1.80	± 13.1 %	
5800	35.3	5.27	4.75	4.75	4.75	0.40	1.80	± 13.1 %	
* Frequency validity above 300 MHz is ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.									
* At frequencies 5-10 GHz, the validity of tissue parameters (ε and σ) can be related to ± 10% if liquid compensation formula is applied to measured DCP values. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.									
* Alpha/Depth are determined during calibration. SP-ECG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz, below ± 2% for frequencies between 3-6 GHz, and below ± 4% for frequencies between 6-10 GHz at any distance larger than half the probe diameter from the boundary.									
Certificate No: EX3-7346_Mar22 Page 5 of 34									

EX3DV4 - SN:7346									
March 30, 2022									
DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346									
Calibration Parameter Determined in Head Tissue Simulating Media									
f (MHz)	Relative Permittivity ¹	Conductivity (S/m) ²	ConvF X	ConvF Y	ConvF Z	Alpha ³	Depth ⁴ (mm)	Unc. (k=2)	
6500	34.5	6.07	5.30	5.30	5.30	0.20	2.50	± 18.6 %	
* Frequency validity above 3 GHz is ± 700 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.									
* At frequencies 5-10 GHz, the validity of tissue parameters (ε and σ) can be related to ± 10% if liquid compensation formula is applied to measured DCP values. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.									
* Alpha/Depth are determined during calibration. SP-ECG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz, below ± 2% for frequencies between 3-6 GHz, and below ± 4% for frequencies between 6-10 GHz at any distance larger than half the probe diameter from the boundary.									
Certificate No: EX3-7346_Mar22 Page 6 of 34									

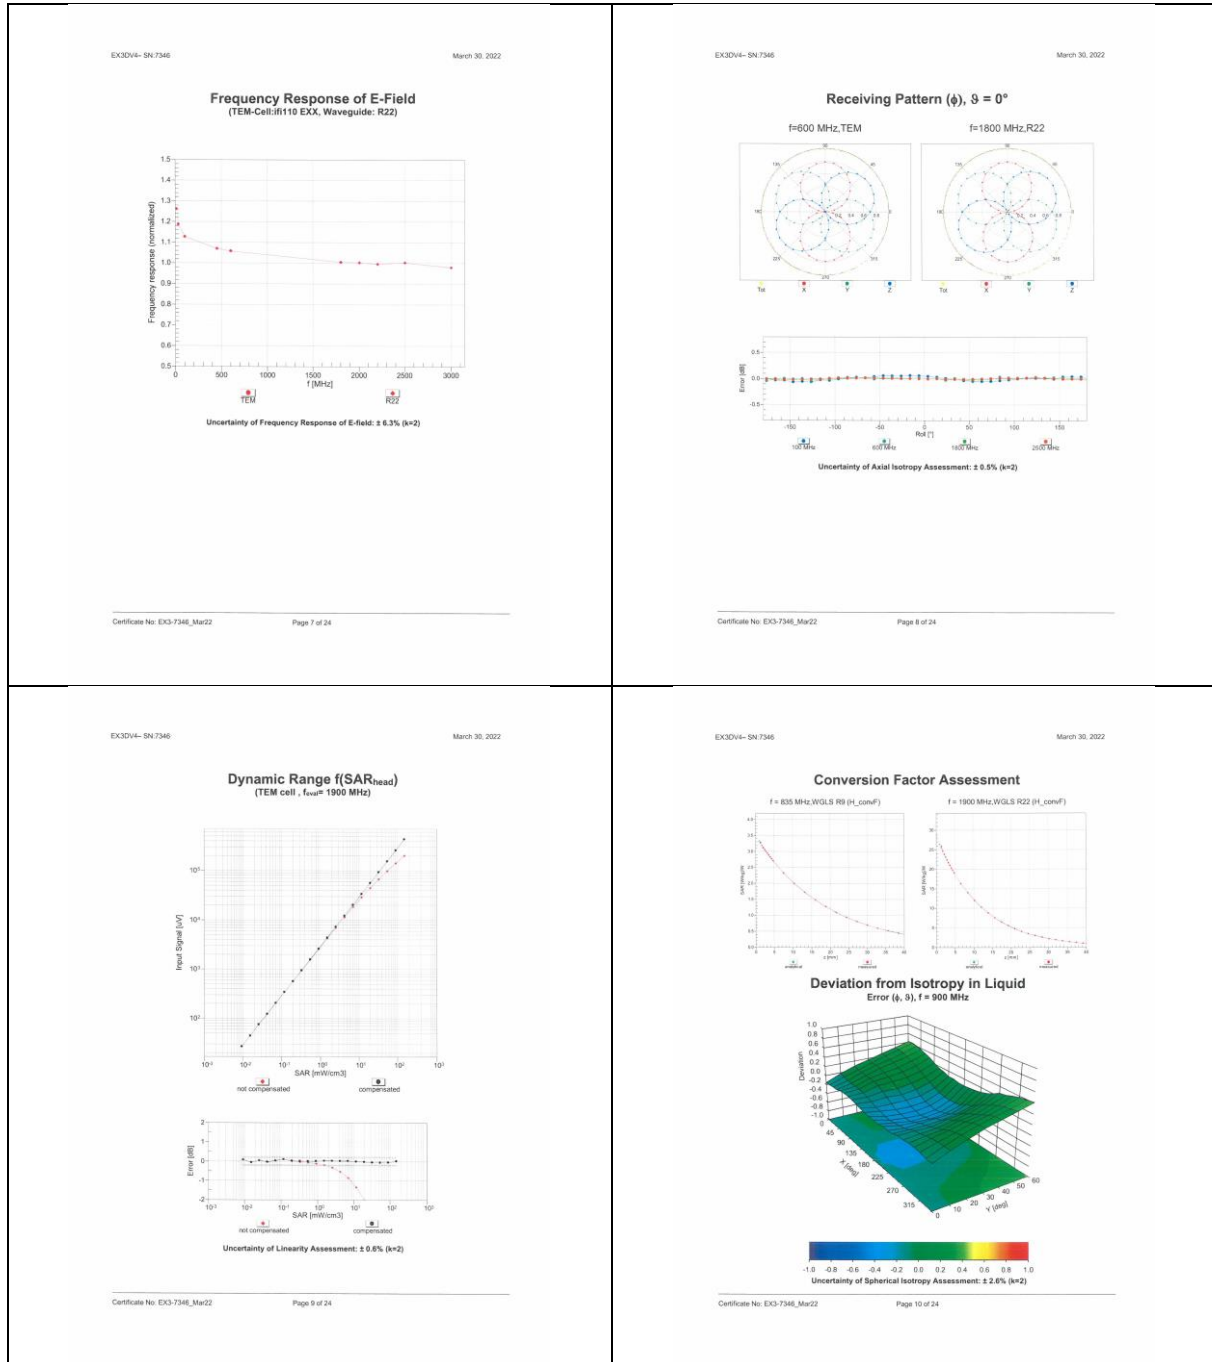

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

EXD04A-SN7346

March 30, 2022

Uplink	Rev	Communication System Name	Group	PAR	Unc (%)
0	-	CW	CW	0.00	4.7 %
10010	CAA	BAR Validation (Square, 100ms, 10ms)	Test	0.00	4.7 %
10011	CAE	LMTS-FDD (HSPA)	WCDMA	2.81	5.9 %
10012	CAE	IEEE 802.11b WIF 2.4 GHz (DSSS, 1 Mbps)	WLAN	1.87	5.9 %
10013	CAE	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 54 Mbps)	WLAN	1.87	5.9 %
10021	DAC	GSM-FDD (TMA, GSM)	GSM	9.39	5.9 %
10023	DAC	GPRS-FDD (TMA, GSM, TN 0)	GSM	9.57	5.9 %
10024	DAC	EDGE-FDD (TMA, GSM, TN 0-1)	GSM	9.56	5.9 %
10025	DAC	EDGE-FDD (TMA, BPSK, TN 0-1)	GSM	12.62	5.9 %
10027	DAC	GPRS-FDD (TMA, GSM, TN 0-2)	GSM	4.80	4.8 %
10028	DAC	EDGE-FDD (TMA, GSM, TN 0-2-3)	GSM	3.55	4.8 %
10029	DAC	EDGE-FDD (TMA, BPSK, TN 0-2-3)	GSM	7.78	5.9 %
10030	CAA	IEEE 802.11s Bluetooth (GFSK, DHT)	Bluetooth	5.30	5.9 %
10031	CAA	IEEE 802.11s Bluetooth (GFSK, DHT)	Bluetooth	1.05	5.9 %
10033	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	7.54	5.9 %
10034	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.53	5.9 %
10035	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	3.83	5.9 %
10036	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	8.01	5.9 %
10037	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.77	5.9 %
10038	CAF	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.15	5.9 %
10039	CAB	CDMA2000 1X RTT, RCT	CDMA2000	4.57	5.9 %
10040	CAB	IS-54/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	7.78	5.9 %
10041	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	6.98	5.9 %
10042	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	13.88	5.9 %
10043	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	10.79	5.9 %
10044	CAE	LMTS-TDD (SC-FDMA, 1.28 Mbps)	TD-SCDMA	11.07	5.9 %
10050	CAD	EDGE-FDD (TMA, BPSK, TN 0-1-2-3)	GSM	6.52	5.9 %
10055	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 1 Mbps)	WLAN	2.72	5.9 %
10060	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 5.5 Mbps)	WLAN	3.96	5.9 %
10061	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	3.96	5.9 %
10062	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	8.68	5.9 %
10063	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	8.63	5.9 %
10064	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	6.98	5.9 %
10065	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.00	5.9 %
10066	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.38	5.9 %
10067	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.32	5.9 %
10068	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.24	5.9 %
10069	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.95	5.9 %
10071	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	9.80	5.9 %
10072	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	8.62	5.9 %
10073	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	9.36	5.9 %
10074	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.30	5.9 %
10075	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.77	5.9 %
10076	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.90	5.9 %
10077	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	11.00	5.9 %
10081	CAB	CDMA2000 1X RTT, RCT	CDMA2000	3.87	5.9 %
10082	CAB	IS-54/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	4.77	5.9 %
10083	DAC	GPRS-FDD (TMA, GSM, TN 0-1)	GSM	6.98	5.9 %
10084	CAB	LMTS-FDD (HSPA)	WCDMA	3.08	5.9 %
10089	CAB	LMTS-FDD (HSPA, Subnet 2)	WCDMA	3.98	5.9 %
10090	CAD	EDGE-FDD (TMA, BPSK, TN 0-1)	GSM	3.55	5.9 %

Certificate No: EXD-7346_Mar22

Page 11 of 24

EXD04A-SN7346

March 30, 2022

Uplink	Rev	Communication System Name	Group	PAR	Unc (%)
0	-	CW	CW	0.00	4.7 %
10010	CAA	BAR Validation (Square, 100ms, 10ms)	Test	0.00	4.7 %
10011	CAE	LMTS-FDD (HSPA)	WCDMA	2.81	5.9 %
10012	CAE	IEEE 802.11b WIF 2.4 GHz (DSSS, 1 Mbps)	WLAN	1.87	5.9 %
10013	CAE	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 54 Mbps)	WLAN	1.87	5.9 %
10021	DAC	GSM-FDD (TMA, GSM)	GSM	9.39	5.9 %
10023	DAC	GPRS-FDD (TMA, GSM, TN 0)	GSM	9.57	5.9 %
10024	DAC	EDGE-FDD (TMA, GSM, TN 0-1)	GSM	9.56	5.9 %
10025	DAC	EDGE-FDD (TMA, BPSK, TN 0-1)	GSM	12.62	5.9 %
10027	DAC	GPRS-FDD (TMA, GSM, TN 0-2)	GSM	4.80	4.8 %
10028	DAC	EDGE-FDD (TMA, GSM, TN 0-2-3)	GSM	3.55	4.8 %
10029	DAC	EDGE-FDD (TMA, BPSK, TN 0-2-3)	GSM	7.78	5.9 %
10030	CAA	IEEE 802.11s Bluetooth (GFSK, DHT)	Bluetooth	5.30	5.9 %
10031	CAA	IEEE 802.11s Bluetooth (GFSK, DHT)	Bluetooth	1.05	5.9 %
10033	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	7.54	5.9 %
10034	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.53	5.9 %
10035	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	3.83	5.9 %
10036	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	8.01	5.9 %
10037	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.77	5.9 %
10038	CAF	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.15	5.9 %
10039	CAB	CDMA2000 1X RTT, RCT	CDMA2000	4.57	5.9 %
10040	CAB	IS-54/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	7.78	5.9 %
10041	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	6.98	5.9 %
10042	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	13.88	5.9 %
10043	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	10.79	5.9 %
10044	CAE	LMTS-TDD (SC-FDMA, 1.28 Mbps)	TD-SCDMA	11.07	5.9 %
10050	CAD	EDGE-FDD (TMA, BPSK, TN 0-1-2-3)	GSM	6.52	5.9 %
10055	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 1 Mbps)	WLAN	2.72	5.9 %
10060	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 5.5 Mbps)	WLAN	3.96	5.9 %
10061	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	3.96	5.9 %
10062	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	8.68	5.9 %
10063	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	8.63	5.9 %
10064	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	6.98	5.9 %
10065	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.00	5.9 %
10066	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.38	5.9 %
10067	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.32	5.9 %
10068	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.24	5.9 %
10069	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.95	5.9 %
10071	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	9.80	5.9 %
10072	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	8.62	5.9 %
10073	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	9.36	5.9 %
10074	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.30	5.9 %
10075	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.77	5.9 %
10076	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.90	5.9 %
10077	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	11.00	5.9 %
10081	CAB	CDMA2000 1X RTT, RCT	CDMA2000	3.87	5.9 %
10082	CAB	IS-54/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	4.77	5.9 %
10083	DAC	GPRS-FDD (TMA, GSM, TN 0-1)	GSM	6.98	5.9 %
10084	CAB	LMTS-FDD (HSPA)	WCDMA	3.08	5.9 %
10089	CAB	LMTS-FDD (HSPA, Subnet 2)	WCDMA	3.98	5.9 %
10090	CAD	EDGE-FDD (TMA, BPSK, TN 0-1)	GSM	3.55	5.9 %

Certificate No: EXD-7346_Mar22

Page 12 of 24

EXD04A-SN7346

March 30, 2022

Uplink	Rev	Communication System Name	Group	PAR	Unc (%)
0	-	CW	CW	0.00	4.7 %
10010	CAA	BAR Validation (Square, 100ms, 10ms)	Test	0.00	4.7 %
10011	CAE	LMTS-FDD (HSPA)	WCDMA	2.81	5.9 %
10012	CAE	IEEE 802.11b WIF 2.4 GHz (DSSS, 1 Mbps)	WLAN	1.87	5.9 %
10013	CAE	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 54 Mbps)	WLAN	1.87	5.9 %
10021	DAC	GSM-FDD (TMA, GSM)	GSM	9.39	5.9 %
10023	DAC	GPRS-FDD (TMA, GSM, TN 0)	GSM	9.57	5.9 %
10024	DAC	EDGE-FDD (TMA, GSM, TN 0-1)	GSM	9.56	5.9 %
10025	DAC	EDGE-FDD (TMA, BPSK, TN 0-1)	GSM	12.62	5.9 %
10027	DAC	GPRS-FDD (TMA, GSM, TN 0-2)	GSM	4.80	4.8 %
10028	DAC	EDGE-FDD (TMA, GSM, TN 0-2-3)	GSM	3.55	4.8 %
10029	DAC	EDGE-FDD (TMA, BPSK, TN 0-2-3)	GSM	7.78	5.9 %
10030	CAA	IEEE 802.11s Bluetooth (GFSK, DHT)	Bluetooth	5.30	5.9 %
10031	CAA	IEEE 802.11s Bluetooth (GFSK, DHT)	Bluetooth	1.05	5.9 %
10033	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	7.54	5.9 %
10034	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.53	5.9 %
10035	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	3.83	5.9 %
10036	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	8.01	5.9 %
10037	CAA	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.77	5.9 %
10038	CAF	IEEE 802.11s Bluetooth (PIA-QPSK, DHT)	Bluetooth	4.15	5.9 %
10039	CAB	CDMA2000 1X RTT, RCT	CDMA2000	4.57	5.9 %
10040	CAB	IS-54/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	7.78	5.9 %
10041	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	6.98	5.9 %
10042	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	13.88	5.9 %
10043	CAE	IS-97/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	10.79	5.9 %
10044	CAE	LMTS-TDD (SC-FDMA, 1.28 Mbps)	TD-SCDMA	11.07	5.9 %
10050	CAD	EDGE-FDD (TMA, BPSK, TN 0-1-2-3)	GSM	6.52	5.9 %
10055	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 1 Mbps)	WLAN	2.72	5.9 %
10060	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 5.5 Mbps)	WLAN	3.96	5.9 %
10061	CAB	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	3.96	5.9 %
10062	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	8.68	5.9 %
10063	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	8.63	5.9 %
10064	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	6.98	5.9 %
10065	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.00	5.9 %
10066	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.38	5.9 %
10067	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.32	5.9 %
10068	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.24	5.9 %
10069	CAD	IEEE 802.11b WIF 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.95	5.9 %
10071	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	9.80	5.9 %
10072	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	8.62	5.9 %
10073	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	9.36	5.9 %
10074	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.30	5.9 %
10075	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.77	5.9 %
10076	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	10.90	5.9 %
10077	CAB	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	11.00	5.9 %
10081	CAB	CDMA2000 1X RTT, RCT	CDMA2000	3.87	5.9 %
10082	CAB	IS-54/IS-130 FDD (TMA/FDMA, PIA-QPSK, FullRate)	AMPS	4.77	5.9 %
10083	DAC	GPRS-FDD (TMA, GSM, TN 0-1)	GSM	6.98	5.9 %
10084	CAB	LMTS-FDD (HSPA)	WCDMA	3.08	5.9 %
10089	CAB	LMTS-FDD (HSPA, Subnet 2)	WCDMA	3.98	5.9 %
10090	CAD	EDGE-FDD (TMA, BPSK, TN 0-1)	GSM	3.55	5.9 %

Certificate No: EXD-7346_Mar22

Page 13 of 24

EXD04A-SN7346

March 30, 2022

Uplink	Rev	Communication System Name	Group	PAR	Unc (%)
0	-	CW	CW	0.00	4.7 %
10010	CAA	BAR Validation (Square, 100ms, 10ms)	Test	0.00	4.7 %
10011	CAE	LMTS-FDD (HSPA)	WCDMA	2.81	5.9 %
10012	CAE	IEEE 802.11b WIF 2.4 GHz (DSSS, 1 Mbps)	WLAN	1.87	5.9 %
10013	CAE	IEEE 802.11g WIF 2.4 GHz (DSSS-OFDM, 54 Mbps)	WLAN	1.87	5.9 %
10021	DAC	GSM-FDD (TMA, GSM)	GSM	9.39	5.9 %
10023	DAC	GPRS-FDD (TMA, GSM, TN 0)	GSM	9.57	5.9 %
10024	DAC	EDGE-FDD (TMA, GSM, TN 0-1)	GSM	9.56	5.9 %
10025	DAC	EDGE-FDD (TMA, BPSK, TN 0-1)	GSM	12.62	5.9 %
10027	DAC	GPRS-FDD (TMA, GSM, TN 0-2)	GSM	4.80	4.8 %
10028	DAC	EDGE-FDD (TMA, GSM, TN 0-2-3)	GSM	3.55	4.8 %
10029	DAC	EDGE-FDD (TMA, BPSK, TN 0-2-3			

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>, and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is deemed to have read, understood and accepted the Terms and Conditions of the document and to have agreed to follow the Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is strictly prohibited and may result in severe civil or criminal penalties. Unless otherwise stated, the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

**Attention: To check the authenticity of testing /inspection rep
or email: CN.Doccheck@sgs.com**

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn

f(86-512)57370818 sqs.china@sqs.com



EX3034-SN-7346				March 30, 2022			
10414	AAA	WLAN CDF4 64-QAM 40MHz	Generic	8.54	± 0.6 %		
10415	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps, R90c-d)	WLAN	1.54	± 0.6 %		
10416	AAA	IEEE 802.11g WFI 2.4 GHz (OFDM, 5.5 Mbps, R90c-d)	WLAN	8.23	± 0.6 %		
10417	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 6 Mbps, R90c-d)	WLAN	8.23	± 0.6 %		
10418	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 6 Mbps, R90c-Long)	WLAN	8.14	± 0.6 %		
10419	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 6 Mbps, R90c-Short)	WLAN	8.19	± 0.6 %		
10420	AAC	IEEE 802.11n HT Overhead, 7.2 Mbps, R90c-d	WLAN	8.32	± 0.6 %		
10421	AAC	IEEE 802.11n HT Overhead, 6.3 Mbps, 16-QAM	WLAN	8.47	± 0.6 %		
10424	AAC	IEEE 802.11n HT Overhead, 7.2 Mbps, 64-QAM	WLAN	8.40	± 0.6 %		
10425	AAC	IEEE 802.11n HT Overhead, 14 Mbps, R90c-d	WLAN	8.41	± 0.6 %		
10428	AAC	IEEE 802.11n HT Overhead, 30 Mbps, 16-QAM	WLAN	8.45	± 0.6 %		
10427	AAC	IEEE 802.11n HT Overhead, 130 Mbps, 64-QAM	WLAN	8.41	± 0.6 %		
10430	AAD	LTE-FDD (FDDMA, 5 MHz, E-TRP 3.1)	LTE-FDD	8.28	± 0.6 %		
10431	AAD	LTE-FDD (FDDMA, 10 MHz, E-TRP 3.1)	LTE-FDD	8.38	± 0.6 %		
10432	AAC	LTE-FDD (FDDMA, 15 MHz, E-TRP 3.1)	LTE-FDD	8.34	± 0.6 %		
10433	AAC	LTE-FDD (FDDMA, 20 MHz, E-TRP 3.1)	LTE-FDD	8.34	± 0.6 %		
10434	AAA	WCDMA (BS Test Model 1, 64 QPSK)	WCDMA	8.80	± 0.6 %		
10435	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %		
10447	AAD	LTE-FDD (FDDMA, 5 MHz, E-TRP 3.1, Clipping 44%)	LTE-FDD	7.86	± 0.6 %		
10448	AAD	LTE-FDD (FDDMA, 10 MHz, E-TRP 3.1, Clipping 44%)	LTE-FDD	7.93	± 0.6 %		
10449	AAC	LTE-FDD (FDDMA, 15 MHz, E-TRP 3.1, Clipping 44%)	LTE-FDD	7.91	± 0.6 %		
10450	AAC	LTE-FDD (FDDMA, 20 MHz, E-TRP 3.1, Clipping 44%)	LTE-FDD	7.88	± 0.6 %		
10451	AAA	WCDMA (BS Test Model 1, 64 QPSK, Clipping 44%)	WCDMA	7.89	± 0.6 %		
10452	AAD	Validation (Spurs, 10ms, 1ms)	Test	10.00	± 0.6 %		
10458	AAC	IEEE 802.11ac WFI (160MHz, 64-QAM, R90c-d)	WLAN	8.63	± 0.6 %		
10457	AAA	UMTS FDD (SC-FDMA)	WCDMA	6.62	± 0.6 %		
10459	AAA	CDMA2000 (1xEV-DO Rev. B, 3 carriers)	CDMA2000	8.18	± 0.6 %		
10459	AAA	CDMA2000 (1xEV-DO Rev. B, 3 carriers)	CDMA2000	8.25	± 0.6 %		
10462	AAA	UMTS FDD (HSPA, R90c-d)	WCDMA	2.39	± 0.6 %		
10461	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %		
10462	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Sub)	LTE-TDD	8.30	± 0.6 %		
10463	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL Sub)	LTE-TDD	8.30	± 0.6 %		
10464	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %		
10465	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10466	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10467	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	7.82	± 0.6 %		
10468	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10469	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10470	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10474	AAC	LTE-TDD (SC-FDMA, 1 RB, 10 Mbps, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10475	AAC	LTE-TDD (SC-FDMA, 1 RB, 10 Mbps, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10477	AAF	LTE-TDD (SC-FDMA, 1 RB, 20 Mbps, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10478	AAF	LTE-TDD (SC-FDMA, 1 RB, 20 Mbps, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %		
10479	AAB	LTE-TDD (SC-FDMA, 50% RB, 4.4 Mbps, QPSK, UL Sub)	LTE-TDD	7.74	± 0.6 %		
10480	AAB	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Sub)	LTE-TDD	8.18	± 0.6 %		
10481	AAC	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM, UL Sub)	LTE-TDD	8.18	± 0.6 %		
10482	AAC	LTE-TDD (SC-FDMA, 50% RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.71	± 0.6 %		
10483	AAC	LTE-TDD (SC-FDMA, 50% RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.39	± 0.6 %		
10484	AAC	LTE-TDD (SC-FDMA, 50% RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.47	± 0.6 %		
10485	AAF	LTE-TDD (SC-FDMA, 50% RB, 5.5 Mbps, QPSK, UL Sub)	LTE-TDD	7.89	± 0.6 %		
10486	AAF	LTE-TDD (SC-FDMA, 50% RB, 5.5 Mbps, 16-QAM, UL Sub)	LTE-TDD	8.28	± 0.6 %		
10487	AAF	LTE-TDD (SC-FDMA, 50% RB, 5.5 Mbps, 64-QAM, UL Sub)	LTE-TDD	8.40	± 0.6 %		
10488	AAF	LTE-TDD (SC-FDMA, 50% RB, 10 Mbps, QPSK, UL Sub)	LTE-TDD	7.70	± 0.6 %		

Certificate No. EX3-7346_Mar22

Page 15 of 24

EX3034-SN-7346				March 30, 2022			
10487	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.49	± 0.6 %		
10488	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.37	± 0.6 %		
10489	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.39	± 0.6 %		
10490	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.39	± 0.6 %		
10491	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.39	± 0.6 %		
10492	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.42	± 0.6 %		
10493	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.42	± 0.6 %		
10494	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.48	± 0.6 %		
10495	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.47	± 0.6 %		
10496	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.50	± 0.6 %		
10497	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %		
10498	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %		
10499	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.53	± 0.6 %		
10500	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.53	± 0.6 %		
10501	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.56	± 0.6 %		
10502	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.69	± 0.6 %		
10503	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.77	± 0.6 %		
10504	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 9 Mbps, R90c-d)	WLAN	8.25	± 0.6 %		
10505	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 12 Mbps, R90c-d)	WLAN	8.45	± 0.6 %		
10506	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 18 Mbps, R90c-d)	WLAN	8.13	± 0.6 %		
10507	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 24 Mbps, R90c-d)	WLAN	8.09	± 0.6 %		
10508	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 36 Mbps, R90c-d)	WLAN	8.37	± 0.6 %		
10509	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 48 Mbps, R90c-d)	WLAN	8.10	± 0.6 %		
10510	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 54 Mbps, R90c-d)	WLAN	8.30	± 0.6 %		
10511	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps, R90c-d)	WLAN	1.99	± 0.6 %		
10512	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 2 Mbps, R90c-d)	WLAN	1.99	± 0.6 %		
10513	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 5.5 Mbps, R90c-d)	WLAN	1.98	± 0.6 %		
10514	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 11 Mbps, R90c-d)	WLAN	1.98	± 0.6 %		
10515	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 6 Mbps, R90c-d)	WLAN	8.89	± 0.6 %		
10516	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 9 Mbps, R90c-d)	WLAN	8.80	± 0.6 %		
10517	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 12 Mbps, R90c-d)	WLAN	8.79	± 0.6 %		
10518	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 18 Mbps, R90c-d)	WLAN	8.49	± 0.6 %		
10519	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 24 Mbps, R90c-d)	WLAN	8.49	± 0.6 %		
10520	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 36 Mbps, R90c-d)	WLAN	8.76	± 0.6 %		
10521	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 48 Mbps, R90c-d)	WLAN	8.35	± 0.6 %		
10522	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 54 Mbps, R90c-d)	WLAN	8.35	± 0.6 %		
10523	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 6 Mbps, R90c-d)	WLAN	8.87	± 0.6 %		
10524	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 9 Mbps, R90c-d)	WLAN	8.89	± 0.6 %		
10525	AAA	IEEE 802.11n WFI 2.4 GHz (DSSS-OFDM, 12 Mbps, R90c-d)	WLAN	8.70	± 0.6 %		
10526	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 9 Mbps, R90c-d)	WLAN	8.49	± 0.6 %		
10527	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 12 Mbps, R90c-d)	WLAN	8.36	± 0.6 %		
10528	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 18 Mbps, R90c-d)	WLAN	8.76	± 0.6 %		
10529	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 24 Mbps, R90c-d)	WLAN	8.76	± 0.6 %		
10530	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 36 Mbps, R90c-d)	WLAN	8.67	± 0.6 %		
10531	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 48 Mbps, R90c-d)	WLAN	8.61	± 0.6 %		
10532	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 54 Mbps, R90c-d)	WLAN	8.79	± 0.6 %		
10533	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 6 Mbps, R90c-d)	WLAN	8.84	± 0.6 %		
10534	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 9 Mbps, R90c-d)	WLAN	8.74	± 0.6 %		
10535	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 12 Mbps, R90c-d)	WLAN	8.74	± 0.6 %		
10536	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.83	± 0.6 %		
10537	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.79	± 0.6 %		
10538	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10539	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10540	AAD	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10541	AAD	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10542	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10543	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10544	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10545	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10546	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10547	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10548	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.86	± 0.6 %		
10549	AAA	LTE-TDD (SC-FDMA, 1 RB, 5.1 MHz, QPSK, UL Sub+2.7)	LTE-TDD	11.96	± 0.6 %		
10550	AAA	CDMA2000 (1xEV-DO Rev. B, 3 carriers)	CDMA2000	3.45	± 0.6 %		
10551	AAC	LTE-TDD (SC-FDMA, 1 RB, 5.1 MHz, E-TRP 3.1, Clipping 44%)	LTE-TDD	6.91	± 0.6 %		
10552	AAC	LTE-TDD (SC-FDMA, 1 RB, 5.1 MHz, E-TRP 3.1, Clipping 44%)	LTE-TDD	7.42	± 0.6 %		
10553	AAC	LTE-TDD (SC-FDMA, 1 RB, 5.1 MHz, E-TRP 3.1, Clipping 44%)	LTE-TDD	6.96	± 0.6 %		
10554	AAC	LTE-TDD (SC-FDMA, 1 RB, 5.1 MHz, E-TRP 3.1, Clipping 44%)	LTE-TDD	7.21	± 0.6 %		
10555	AAA	Pulse Waveform (200Hz, 10%)	Test	10.00	± 0.6 %		
10556	AAA	Pulse Waveform (200Hz, 20%)	Test	6.99	± 0.6 %		

Units are otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>, and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its issue, and does not constitute a warranty. The Company's sole responsibility is to its Client, and this document does not exonerate parties to a transaction from exercising all their rights and obligations under its transaction documents. This document cannot be reproduced, except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this document refer only to the sample/s tested and such sample/s as is/are retained for re-analysis.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.DCcheck@sgs.com

No. 10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300	t(86-512)57355888	f(86-512)57370818	www.sgsgroup.com.cn
中国 · 江苏 · 昆山市留学生创业园伟业路10号 邮编 215300	t(86-512)57355888	f(86-512)57370818	sgs.china@sgs.com

EX3DV4 – SN 7346

March 30, 2022

10985	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.6 %
10986	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
10987	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
10988	AAA	SG NR DL (CP-OPDM, TN 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.56	± 9.6 %
10989	AAA	SG NR DL (CP-OPDM, TN 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
10990	AAA	SG NR DL (CP-OPDM, TN 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %

* Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4 – SN 7346

March 30, 2022

10991	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.6 %
10992	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
10993	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
10994	AAA	SG NR DL (CP-OPDM, TN 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.56	± 9.6 %
10995	AAA	SG NR DL (CP-OPDM, TN 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
10996	AAA	SG NR DL (CP-OPDM, TN 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
10997	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.6 %
10998	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
10999	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11000	AAA	SG NR DL (CP-OPDM, TN 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.56	± 9.6 %
11001	AAA	SG NR DL (CP-OPDM, TN 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11002	AAA	SG NR DL (CP-OPDM, TN 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11003	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.6 %
11004	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11005	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11006	AAA	SG NR DL (CP-OPDM, TN 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.56	± 9.6 %
11007	AAA	SG NR DL (CP-OPDM, TN 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11008	AAA	SG NR DL (CP-OPDM, TN 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11009	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.6 %
11010	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11011	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11012	AAA	SG NR DL (CP-OPDM, TN 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.56	± 9.6 %
11013	AAA	SG NR DL (CP-OPDM, TN 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11014	AAA	SG NR DL (CP-OPDM, TN 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11015	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.6 %
11016	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11017	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11018	AAA	SG NR DL (CP-OPDM, TN 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.56	± 9.6 %
11019	AAA	SG NR DL (CP-OPDM, TN 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11020	AAA	SG NR DL (CP-OPDM, TN 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11021	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.6 %
11022	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11023	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11024	AAA	SG NR DL (CP-OPDM, TN 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.56	± 9.6 %
11025	AAA	SG NR DL (CP-OPDM, TN 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.53	± 9.6 %
11026	AAA	SG NR DL (CP-OPDM, TN 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %
11027	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.54	± 9.6 %
11028	AAA	SG NR DL (CP-OPDM, TN 3.1, 60 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD	9.50	± 9.6 %

Certificate No. EX3-7346_Mar22

Page 23 of 24

Certificate No. EX3-7346_Mar22

Page 24 of 24

4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2021/4/26	-31.4	/	47.8	/
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2021/4/21	-23	/	57.1	/



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is deemed to have read, understood and accepted the Terms and Conditions of the document and to have agreed to follow the Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or expiration date of this document will render it null and void. The original document or a copy thereof, otherwise stated, is the only valid version. The results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sqs.china@sqs.com