


NOTES:

1. Use 3M adhesive 467MP or 9667MP.
2. Subsurface printing only.
3. Background is white.
4. Match colors of graphics with provided graphic file.
5. One label per lot is to be inspected.
6. Perform inspection using SID-0000000212.
7. A Certificate of Conformance and RoHS statement is required for the material.

(xx) Denotes Incoming Inspection dimensions.

All material must be RoHS compliant

Boarder Key
 ----- Kiss-cut tab
 ——— Label edge

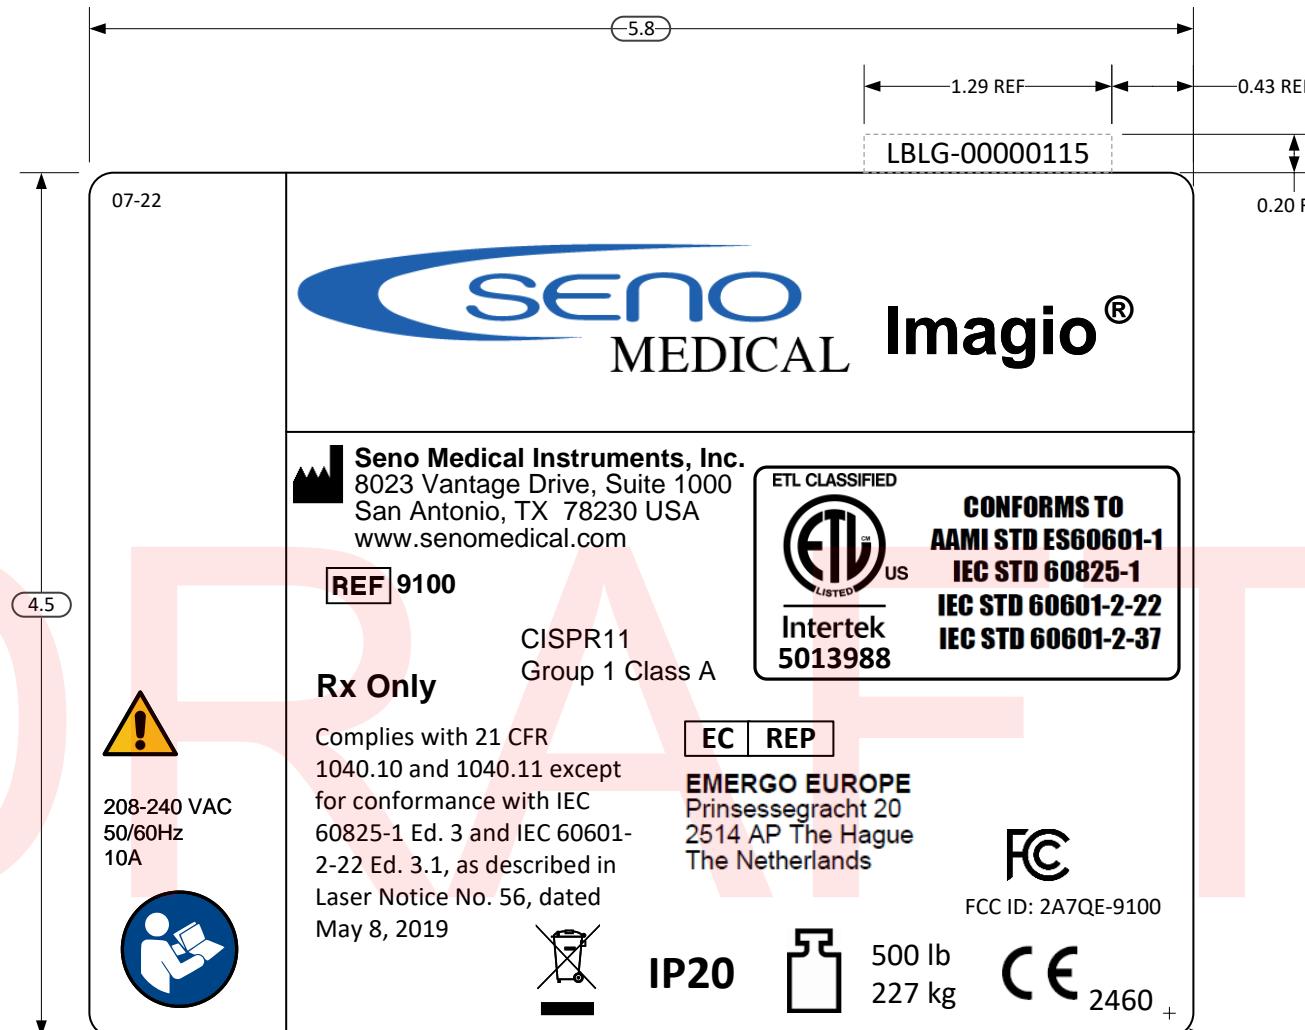

REVISION HISTORY		
REV	DESCRIPTION	DATE
1	INITIAL RELEASE	10/27/2020
2	UPDATED REF NUMBER	2/5/2021
3	REMOVED DUPLICATE VOLTAGE INFO, ADDED IP RATING NUMBER, UPDATE TOLERANCES	4/7/2021
4	REMOVED CE MARK AND EMERGO EUROPE INFORMATION	6/29/2021
5	ADDED FCC MARK AND ID	--
6	ADDED CE MARK AND EMERGO EUROPE INFORMATION	--

UNLESS OTHERWISE SPECIFIED DIMENSIONAL UNITS: INCHES TOLERANCES FRACTIONAL +/- 1/32 ANGULAR: MACH +/- 1/2 DEGREE ONE DECIMAL PLACE +/- 0.1 TWO DECIMAL PLACES +/- 0.06 THREE DECIMAL PLACES +/- 0.005		PROPRIETARY AND CONFIDENTIAL THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF SENO MEDICAL INSTRUMENTS. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF SENO MEDICAL INSTRUMENTS IS PROHIBITED.	
		Drawn By V. Pacheco	MATERIAL 0.007" Thk Polycarbonate
FINISH N/A	Made From Part No. N/A	Previous number N/A	PROPRIETARY AND CONFIDENTIAL THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF SENO MEDICAL INSTRUMENTS. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF SENO MEDICAL INSTRUMENTS IS PROHIBITED.
DWG. NO. LBLG-00000115	REV. 6	SCALE: N/A	DRAWN IN VISO Sheet 1 of 1