




# **Appendix D**


## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System

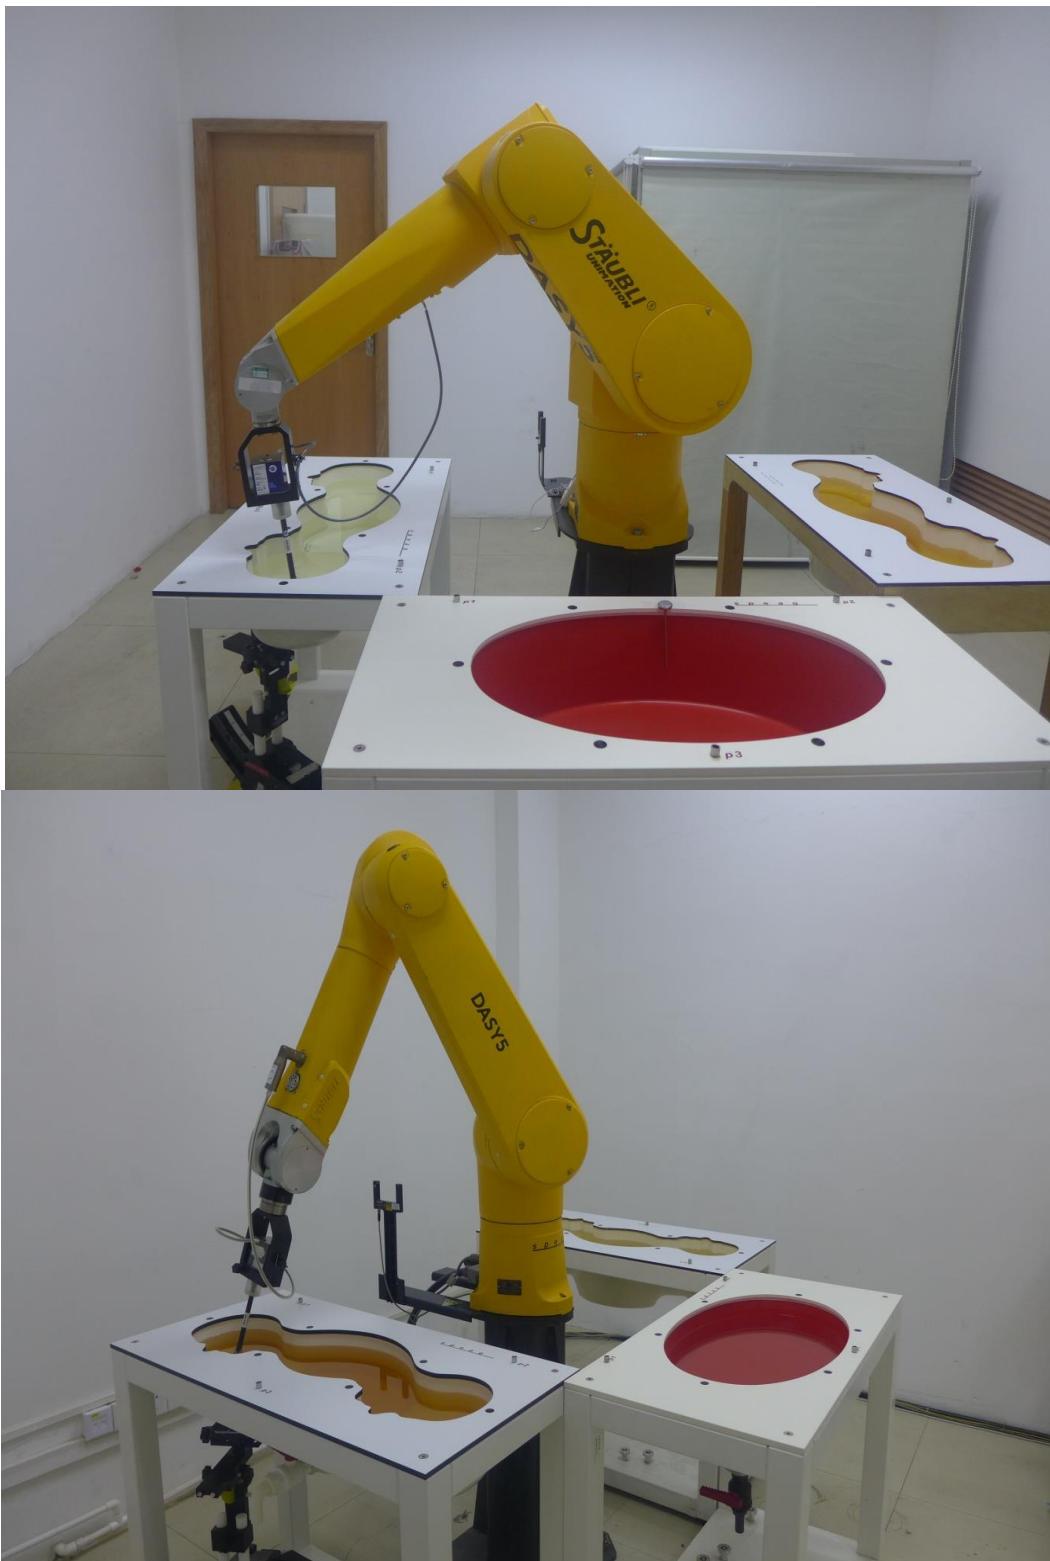

## 2. Photographs of Tissue Simulate Liquid

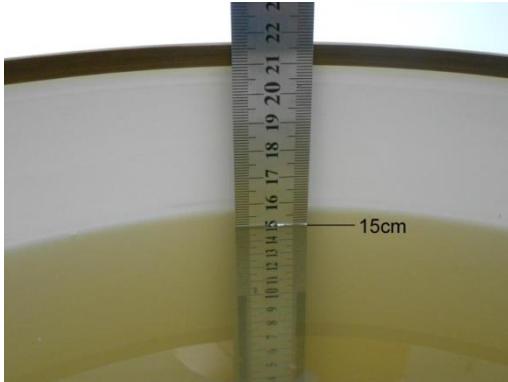Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	N/A
	N/A

### 3. Photographs of EUT test position

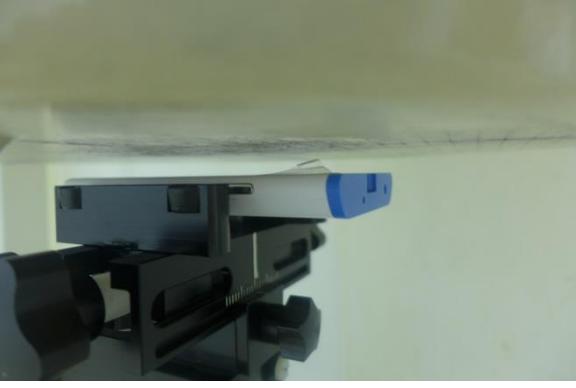
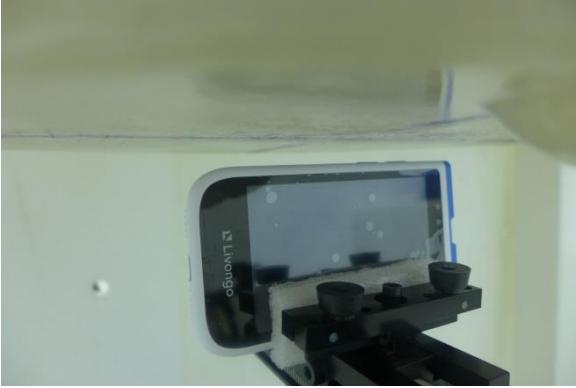
Photo 6: Front side 15mm	Photo 7: Back side 15mm
	
Photo 8: Front side 10mm	Photo 9: Back side 10mm
	
Photo 10: Left side 10mm	Photo 11: Right side 10mm
	

Photo 12: Top side 10mm	Photo 13: Bottom side 10mm
	

**4. EUT Constructional Details**

Photo 14: Front View	Photo 15: Back View
 A photograph of the smartphone's front view. The device is white with a black screen. The screen displays the 'Livongo' logo. A clear plastic ruler is placed next to the phone, showing measurements from 1 to 10 inches on the left and 1 to 10 centimeters on the right. The phone is positioned vertically, with its top edge aligned with the 10-inch/10-centimeter mark on the ruler.	 A photograph of the smartphone's back view. The device is white and appears to be made of a matte material. A circular camera lens is visible on the top left. A clear plastic ruler is placed next to the phone, showing measurements from 1 to 10 inches on the left and 1 to 10 centimeters on the right. The phone is positioned vertically, with its top edge aligned with the 10-inch/10-centimeter mark on the ruler.