

## Extended Dipole Calibrations

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.




Head						
Date of measurement	Return-loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary impedance (ohm)	Delta (ohm)
2014-07-24	-28.92		48.84		3.34	
2015-07-23	-28.70	-0.76	50.34	1.50	3.24	-0.1
2016-07-25	-28.81	-0.38	50.16	1.32	3.28	-0.06

Body						
Date of measurement	Return-loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary impedance (ohm)	Delta (ohm)
2014-07-24	-23.03		50.91		7.08	
2015-07-23	-24.64	7.00	48.52	-2.39	6.25	-0.83
2016-07-25	-23.86	3.60	48.95	-1.96	6.70	-0.38

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5ohm of prior calibration.

Therefore the verification result should support extended calibration.

## 1.3. D1900V2 Dipole Calibration Certificate

 <b>TMC</b> In Collaboration with <b>s p e a g</b> CALIBRATION LABORATORY	Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 E-mail: Info@emcite.com	Fax: +86-10-62304633-2504 Http://www.emcite.com	 IAC-MRA	 CNAS 校准 CNAS L0442																																																							
Client	CIQ SZ (Auden)		Certificate No: J15-2-3052																																																								
<b>CALIBRATION CERTIFICATE</b>																																																											
<table border="0" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 20%;">Object</td> <td colspan="4">D1900V2 - SN: 5d150</td> </tr> <tr> <td>Calibration Procedure(s)</td> <td colspan="4"> TMC-OS-E-02-194  Calibration procedure for dipole validation kits </td> </tr> <tr> <td>Calibration date:</td> <td colspan="4">December 12, 2015</td> </tr> <tr> <td colspan="5"> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> </td> </tr> <tr> <td colspan="2" style="text-align: left;">Primary Standards</td> <td style="text-align: left;">ID #</td> <td colspan="2" style="text-align: left;">Cal Date(Calibrated by, Certificate No.)</td> </tr> <tr> <td colspan="2"> Power Meter NRVD  Power sensor NRV-Z5  Reference Probe ES3DV3  DAE4  Signal Generator E4438C  Network Analyzer E8362B </td> <td>102083 100595 SN 3149 SN 777 MY49070393 MY43021135</td> <td colspan="2"> 11-Sep-15 (TMC, No.JZ13-443)  11-Sep-15 (TMC, No. JZ13-443)  5- Sep-15 (SPEAG, No.ES3-3149_Sep13)  22-Feb-15 (SPEAG, DAE4-777_Feb13)  13-Nov-15 (TMC, No.JZ13-394)  19-Oct-15 (TMC, No.JZ13-278) </td> </tr> <tr> <td colspan="2" style="text-align: left;">Calibrated by:</td> <td style="text-align: left;">Name</td> <td style="text-align: left;">Function</td> <td style="text-align: left;">Signature</td> </tr> <tr> <td colspan="2" style="text-align: left;">Reviewed by:</td> <td style="text-align: left;">Qi Dianyuan</td> <td style="text-align: left;">SAR Project Leader</td> <td style="text-align: left;"></td> </tr> <tr> <td colspan="2" style="text-align: left;">Approved by:</td> <td style="text-align: left;">Lu Bingsong</td> <td style="text-align: left;">Deputy Director of the laboratory</td> <td style="text-align: left;"></td> </tr> <tr> <td colspan="5" style="text-align: right; padding-right: 20px;">Issued: December 17, 2015</td> </tr> <tr> <td colspan="5" style="text-align: center; border-top: 1px solid black; border-bottom: 1px solid black;"> This calibration certificate shall not be reproduced except in full without written approval of the laboratory. </td> </tr> </table>					Object	D1900V2 - SN: 5d150				Calibration Procedure(s)	TMC-OS-E-02-194 Calibration procedure for dipole validation kits				Calibration date:	December 12, 2015				<p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p>					Primary Standards		ID #	Cal Date(Calibrated by, Certificate No.)		Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV3 DAE4 Signal Generator E4438C Network Analyzer E8362B		102083 100595 SN 3149 SN 777 MY49070393 MY43021135	11-Sep-15 (TMC, No.JZ13-443) 11-Sep-15 (TMC, No. JZ13-443) 5- Sep-15 (SPEAG, No.ES3-3149_Sep13) 22-Feb-15 (SPEAG, DAE4-777_Feb13) 13-Nov-15 (TMC, No.JZ13-394) 19-Oct-15 (TMC, No.JZ13-278)		Calibrated by:		Name	Function	Signature	Reviewed by:		Qi Dianyuan	SAR Project Leader		Approved by:		Lu Bingsong	Deputy Director of the laboratory		Issued: December 17, 2015					This calibration certificate shall not be reproduced except in full without written approval of the laboratory.				
Object	D1900V2 - SN: 5d150																																																										
Calibration Procedure(s)	TMC-OS-E-02-194 Calibration procedure for dipole validation kits																																																										
Calibration date:	December 12, 2015																																																										
<p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p>																																																											
Primary Standards		ID #	Cal Date(Calibrated by, Certificate No.)																																																								
Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV3 DAE4 Signal Generator E4438C Network Analyzer E8362B		102083 100595 SN 3149 SN 777 MY49070393 MY43021135	11-Sep-15 (TMC, No.JZ13-443) 11-Sep-15 (TMC, No. JZ13-443) 5- Sep-15 (SPEAG, No.ES3-3149_Sep13) 22-Feb-15 (SPEAG, DAE4-777_Feb13) 13-Nov-15 (TMC, No.JZ13-394) 19-Oct-15 (TMC, No.JZ13-278)																																																								
Calibrated by:		Name	Function	Signature																																																							
Reviewed by:		Qi Dianyuan	SAR Project Leader																																																								
Approved by:		Lu Bingsong	Deputy Director of the laboratory																																																								
Issued: December 17, 2015																																																											
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																																											



Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: [info@emcite.com](mailto:info@emcite.com) [Http://www.emcite.com](http://www.emcite.com)

**Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.



Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: Info@emcite.com [Http://www.emcite.com](http://www.emcite.com)

#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.7.1137
Extrapolation	Advanced Extrapolation	
Phantom	Twin Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz $\pm$ 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.9 $\pm$ 6 %	1.42 mho/m $\pm$ 6 %
Head TSL temperature change during test	<0.5 °C	---	---

#### SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.71 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	38.3 mW /g $\pm$ 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.08 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.2 mW /g $\pm$ 20.4 % (k=2)

#### Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	53.7 $\pm$ 6 %	1.53 mho/m $\pm$ 6 %
Body TSL temperature change during test	<0.5 °C	---	---

#### SAR result with Body TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.98 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	39.9 mW /g $\pm$ 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.26 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.0 mW /g $\pm$ 20.4 % (k=2)



Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: Info@emcite.com [Http://www.emcite.com](http://www.emcite.com)

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.3Ω+ 3.17jΩ
Return Loss	-30.0dB

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.8Ω+ 3.92jΩ
Return Loss	-27.7dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.048 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
-----------------	-------



Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: Info@emcite.com [Http://www.emcite.com](http://www.emcite.com)

**DASY5 Validation Report for Head TSL**

Date: 12.12.2015

Test Laboratory: TMC, Beijing, China

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d150**

Communication System: CW; Frequency: 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.416$  mho/m;  $\epsilon_r = 38.91$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3149; ConvF(5.06,5.06,5.06); Calibrated: 2015/9/5
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 22/2/2015.
- Phantom: SAM 1186; Type: QD000P40CC;
- DASY52 52.8.7(1137); SEMCAD X Version 14.6.10 (7164)

**Dipole Calibration for Head Tissue/Pin=250mW, d=10mm/Zoom Scan**


(7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 90.054 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 17.9 W/kg

**SAR(1 g) = 9.71 W/kg; SAR(10 g) = 5.08 W/kg**

Maximum value of SAR (measured) = 11.8 W/kg

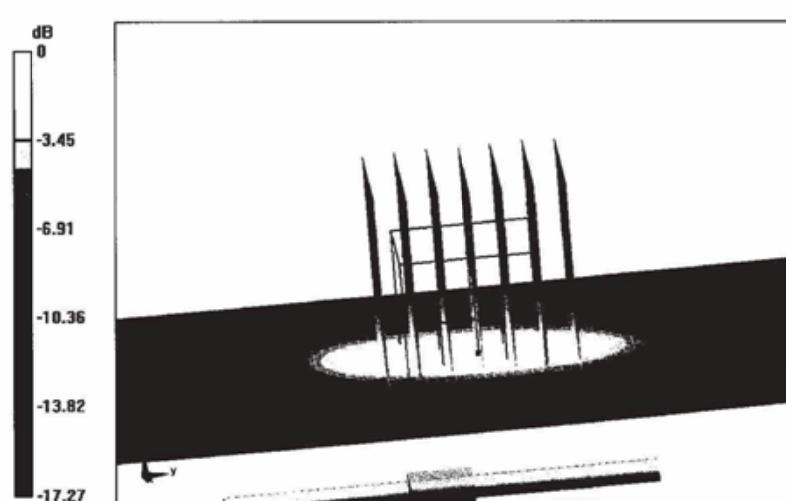


0 dB = 11.8 W/kg = 10.72 dBW/kg



Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: Info@emcite.com [Http://www.emcite.com](http://www.emcite.com)

**Impedance Measurement Plot for Head TSL**

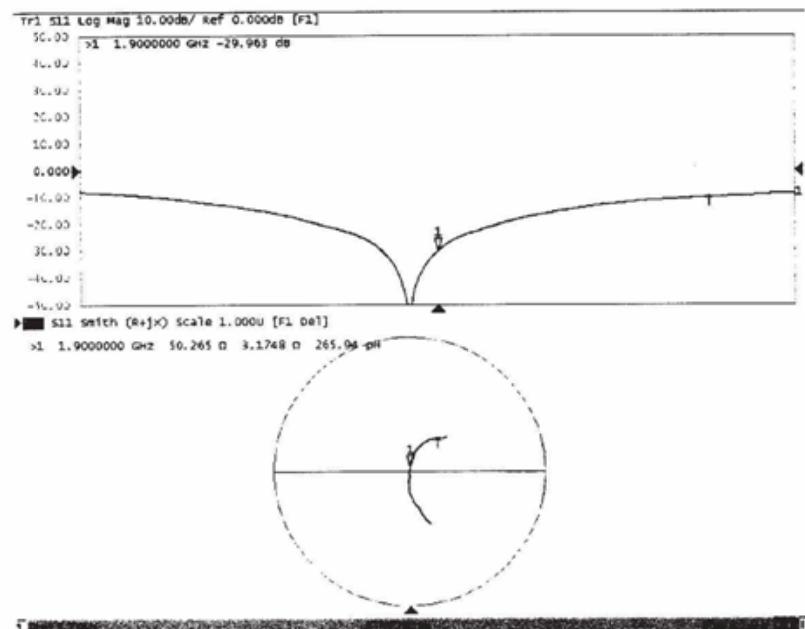



Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: Info@emcite.com [Http://www.emcite.com](http://www.emcite.com)

**DASY5 Validation Report for Body TSL**

Date: 12.10.2015

Test Laboratory: TMC, Beijing, China

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d150**

Communication System: CW; Frequency: 1900 MHz;

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.528$  mho/m;  $\epsilon_r = 53.74$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Phantom

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3149; ConvF(4.72,4.72,4.72) ; Calibrated: 2015/9/5
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 22/2/2015
- Phantom: SAM1186; Type: QD000P40CC;
- DASY52 52.8.7(1137); SEMCAD X Version 14.6.10 (7164)

**Dipole Calibration for Body Tissue/Pin=250mW, d=10mm/Zoom Scan**


**(7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**

Reference Value = 83.606 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 17.7 W/kg

**SAR(1 g) = 9.98 W/kg; SAR(10 g) = 5.26 W/kg**

Maximum value of SAR (measured) = 12.1 W/kg

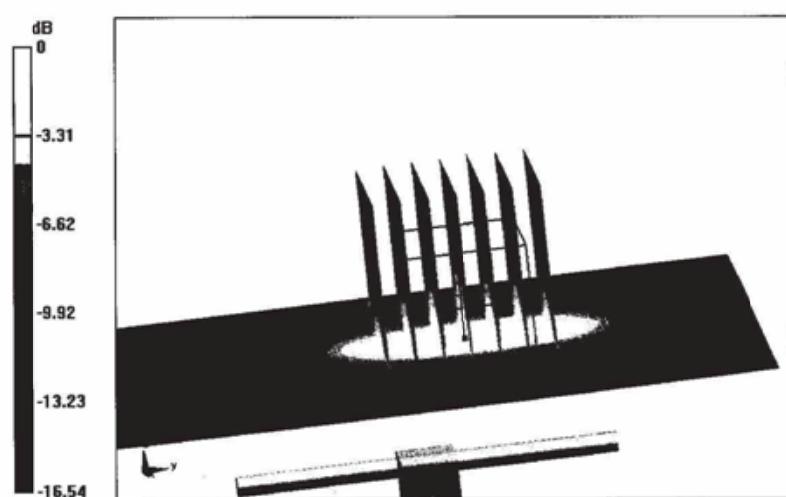

0 dB = 12.1 W/kg = 10.83 dBW/kg


Certificate No: J15-2-3052

Page 7 of 8



Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: Info@emcite.com [Http://www.emcite.com](http://www.emcite.com)



**Impedance Measurement Plot for Body TSL**

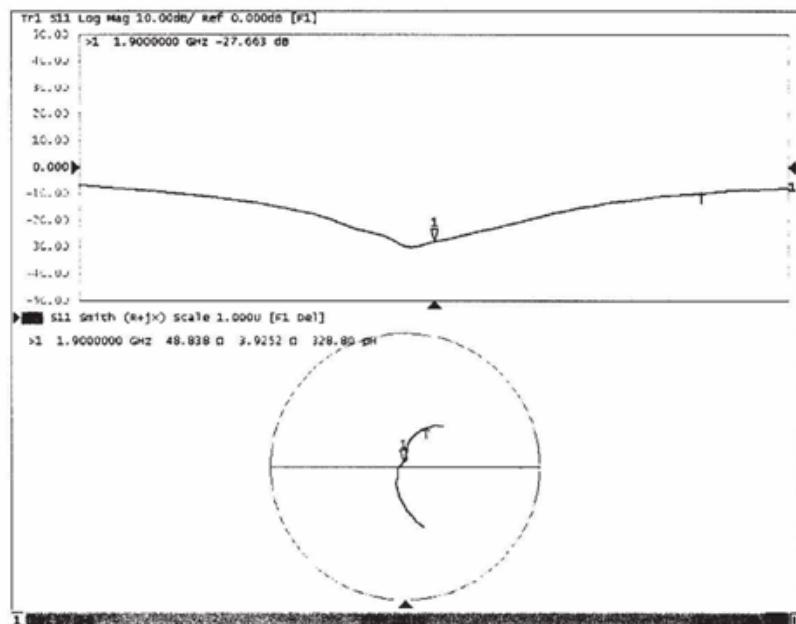

Certificate No: J15-2-3052

Page 8 of 8

## 1.4. D2450V2 Dipole Calibration Certificate

 In Collaboration with <b>s p e a g</b> CALIBRATION LABORATORY		  CALIBRATION No. L0570																													
Client	CIQ-SZ(Auden)																														
Certificate No: Z15-97070																															
<b>CALIBRATION CERTIFICATE</b>																															
Object	D2450V2 - SN: 884																														
Calibration Procedure(s)	TMC-OS-E-02-194 Calibration procedure for dipole validation kits																														
Calibration date:	September 1, 2015																														
<p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature(<math>22\pm3</math>)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date(Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRV</td> <td>102083</td> <td>11-Sep-14 (TMC, No.JZ13-443)</td> <td>Sep-15</td> </tr> <tr> <td>Power sensor NRV-Z5</td> <td>100595</td> <td>11-Sep-14 (TMC, No. JZ13-443)</td> <td>Sep-15</td> </tr> <tr> <td>Reference Probe ES3DV3</td> <td>SN 3149</td> <td>5- Sep-14 (SPEAG, No.ES3-3149_Sep13)</td> <td>Sep-15</td> </tr> <tr> <td>DAE3</td> <td>SN 536</td> <td>23-Jan-15 (SPEAG, DAE3-536_Jan14)</td> <td>Jan -16</td> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49070393</td> <td>13-Nov-14 (TMC, No.JZ13-394)</td> <td>Nov-15</td> </tr> <tr> <td>Network Analyzer E8362B</td> <td>MY43021135</td> <td>19-Oct-14 (TMC, No.JZ13-278)</td> <td>Oct-15</td> </tr> </tbody> </table> <p>Calibrated by:  Name: Zhao Jing Function: SAR Test Engineer</p> <p>Reviewed by:  Name: Qi Dianyuan Function: SAR Project Leader</p> <p>Approved by:  Name: Lu Bingsong Function: Deputy Director of the laboratory</p> <p>Issued: September 4, 2015</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>				Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRV	102083	11-Sep-14 (TMC, No.JZ13-443)	Sep-15	Power sensor NRV-Z5	100595	11-Sep-14 (TMC, No. JZ13-443)	Sep-15	Reference Probe ES3DV3	SN 3149	5- Sep-14 (SPEAG, No.ES3-3149_Sep13)	Sep-15	DAE3	SN 536	23-Jan-15 (SPEAG, DAE3-536_Jan14)	Jan -16	Signal Generator E4438C	MY49070393	13-Nov-14 (TMC, No.JZ13-394)	Nov-15	Network Analyzer E8362B	MY43021135	19-Oct-14 (TMC, No.JZ13-278)	Oct-15
Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration																												
Power Meter NRV	102083	11-Sep-14 (TMC, No.JZ13-443)	Sep-15																												
Power sensor NRV-Z5	100595	11-Sep-14 (TMC, No. JZ13-443)	Sep-15																												
Reference Probe ES3DV3	SN 3149	5- Sep-14 (SPEAG, No.ES3-3149_Sep13)	Sep-15																												
DAE3	SN 536	23-Jan-15 (SPEAG, DAE3-536_Jan14)	Jan -16																												
Signal Generator E4438C	MY49070393	13-Nov-14 (TMC, No.JZ13-394)	Nov-15																												
Network Analyzer E8362B	MY43021135	19-Oct-14 (TMC, No.JZ13-278)	Oct-15																												

Certificate No: Z15-97070

Page 1 of 8



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: [ctl@chinattl.com](mailto:ctl@chinattl.com) [Http://www.chinattl.cn](http://www.chinattl.cn)



CALIBRATION  
No. L0570

### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

### Additional Documentation:

- DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:* SAR measured at the stated antenna input power.
- SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.



In Collaboration with  
**s p e a g**  
 CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: [ctl@chinattl.com](mailto:ctl@chinattl.com) [Http://www.chinattl.cn](http://www.chinattl.cn)



CALIBRATION  
 No. L0570

#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.8.1222
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.84 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

#### SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.1 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	52.1 mW /g ± 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.17 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.6 mW /g ± 20.4 % (k=2)

#### Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.3 ± 6 %	2.00 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	---	---

#### SAR result with Body TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.1 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	51.6 mW /g ± 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	6.11 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	24.2 mW /g ± 20.4 % (k=2)

Certificate No: Z15-97070

Page 3 of 8



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: [cttl@chinattl.com](mailto:cttl@chinattl.com) [Http://www.chinattl.cn](http://www.chinattl.cn)



CALIBRATION  
No. L0570

### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	58.3Ω- 0.76jΩ
Return Loss	- 22.3dB

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	58.1Ω+ 2.61jΩ
Return Loss	- 22.1dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.224 ns
----------------------------------	----------


After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.


No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.


#### Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

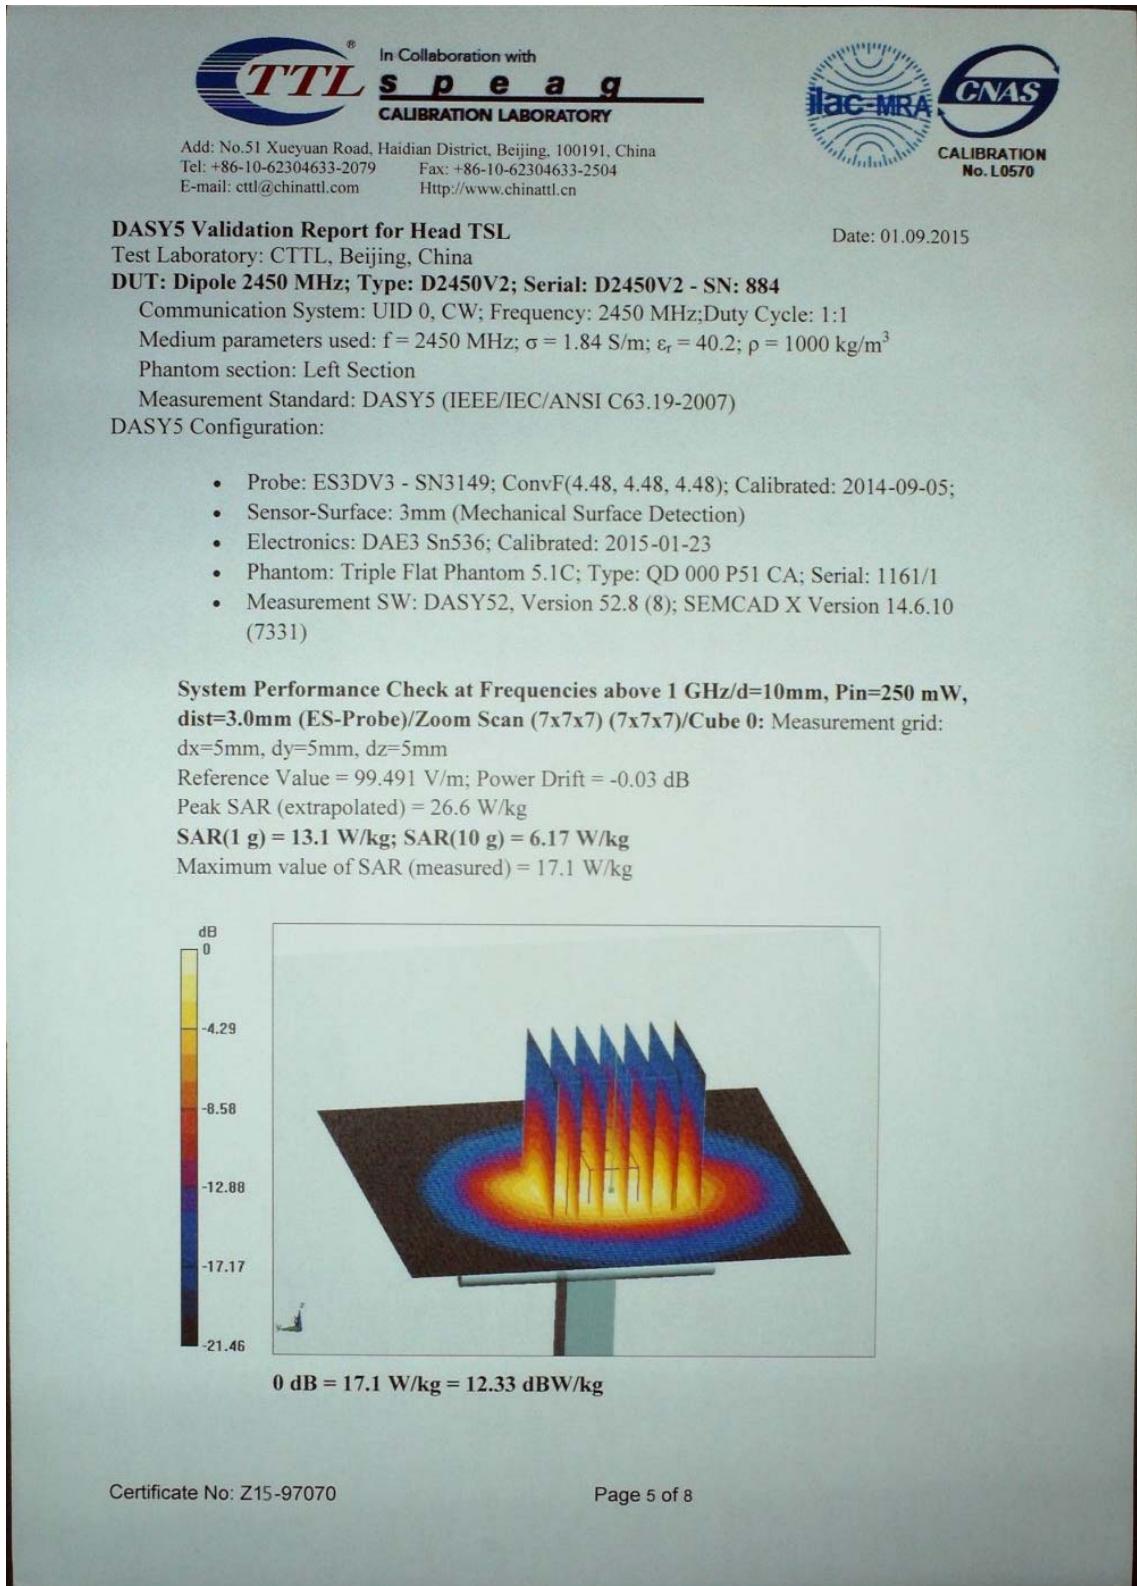


## Appendix A: Calibration Certificate

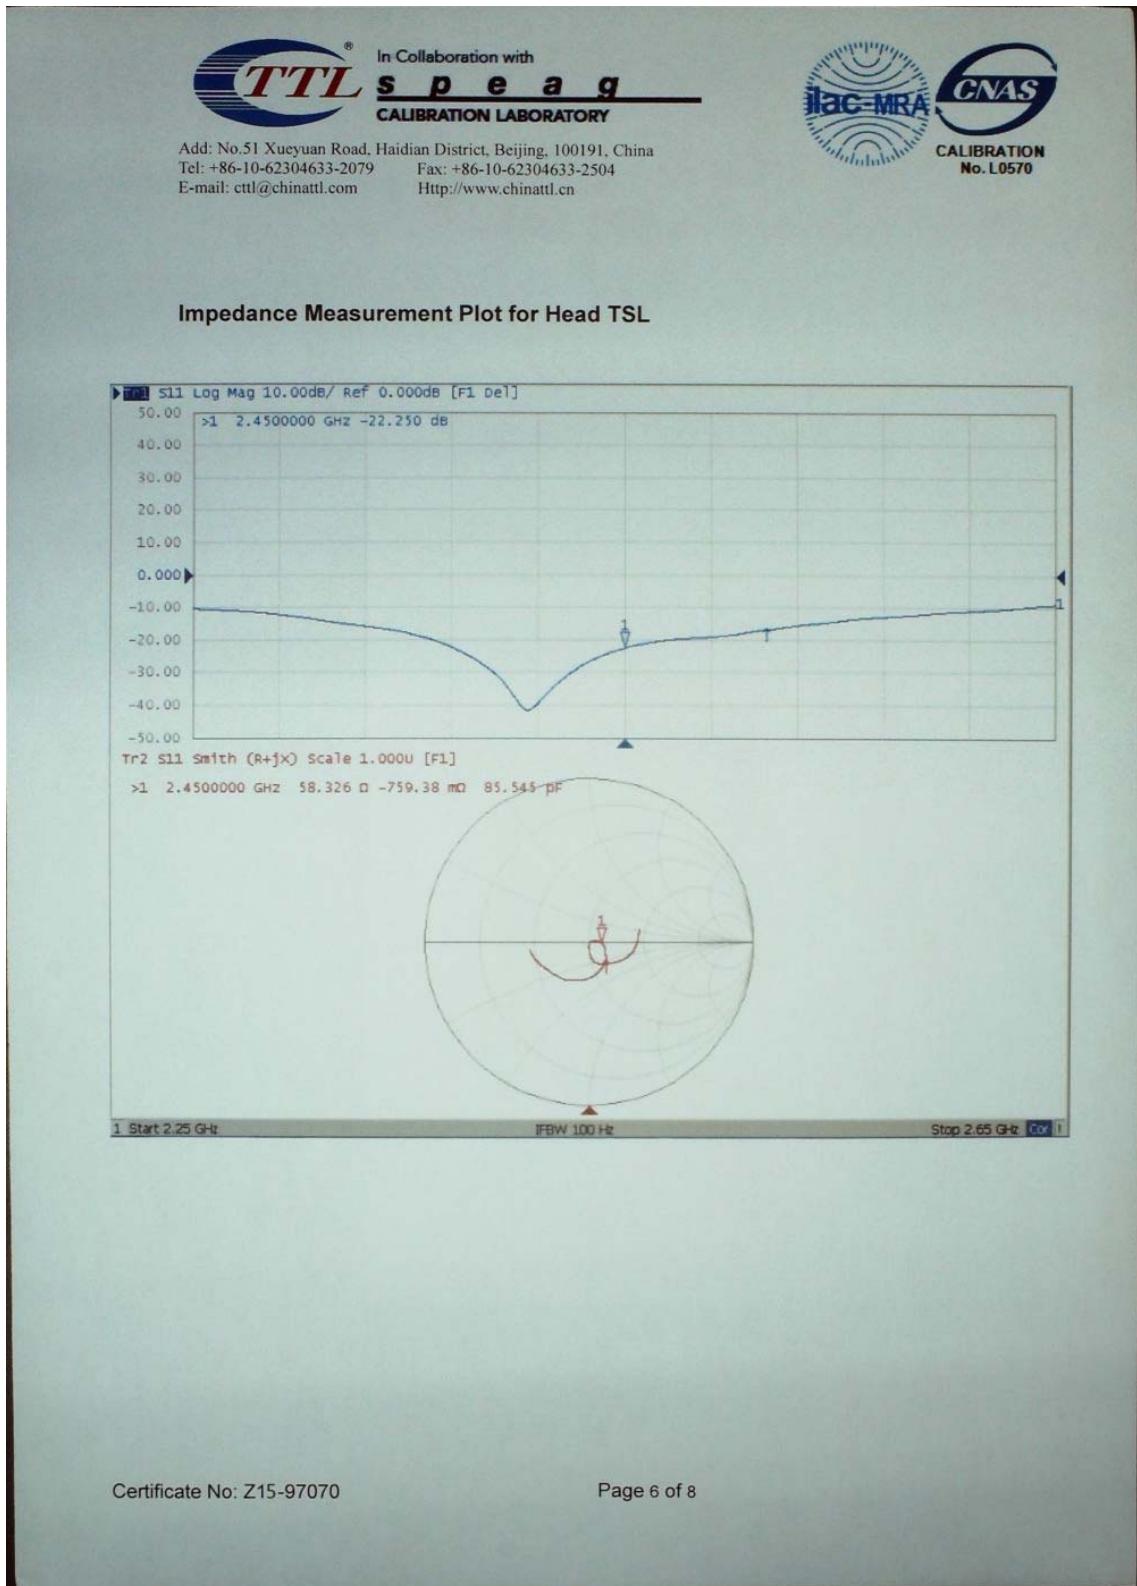

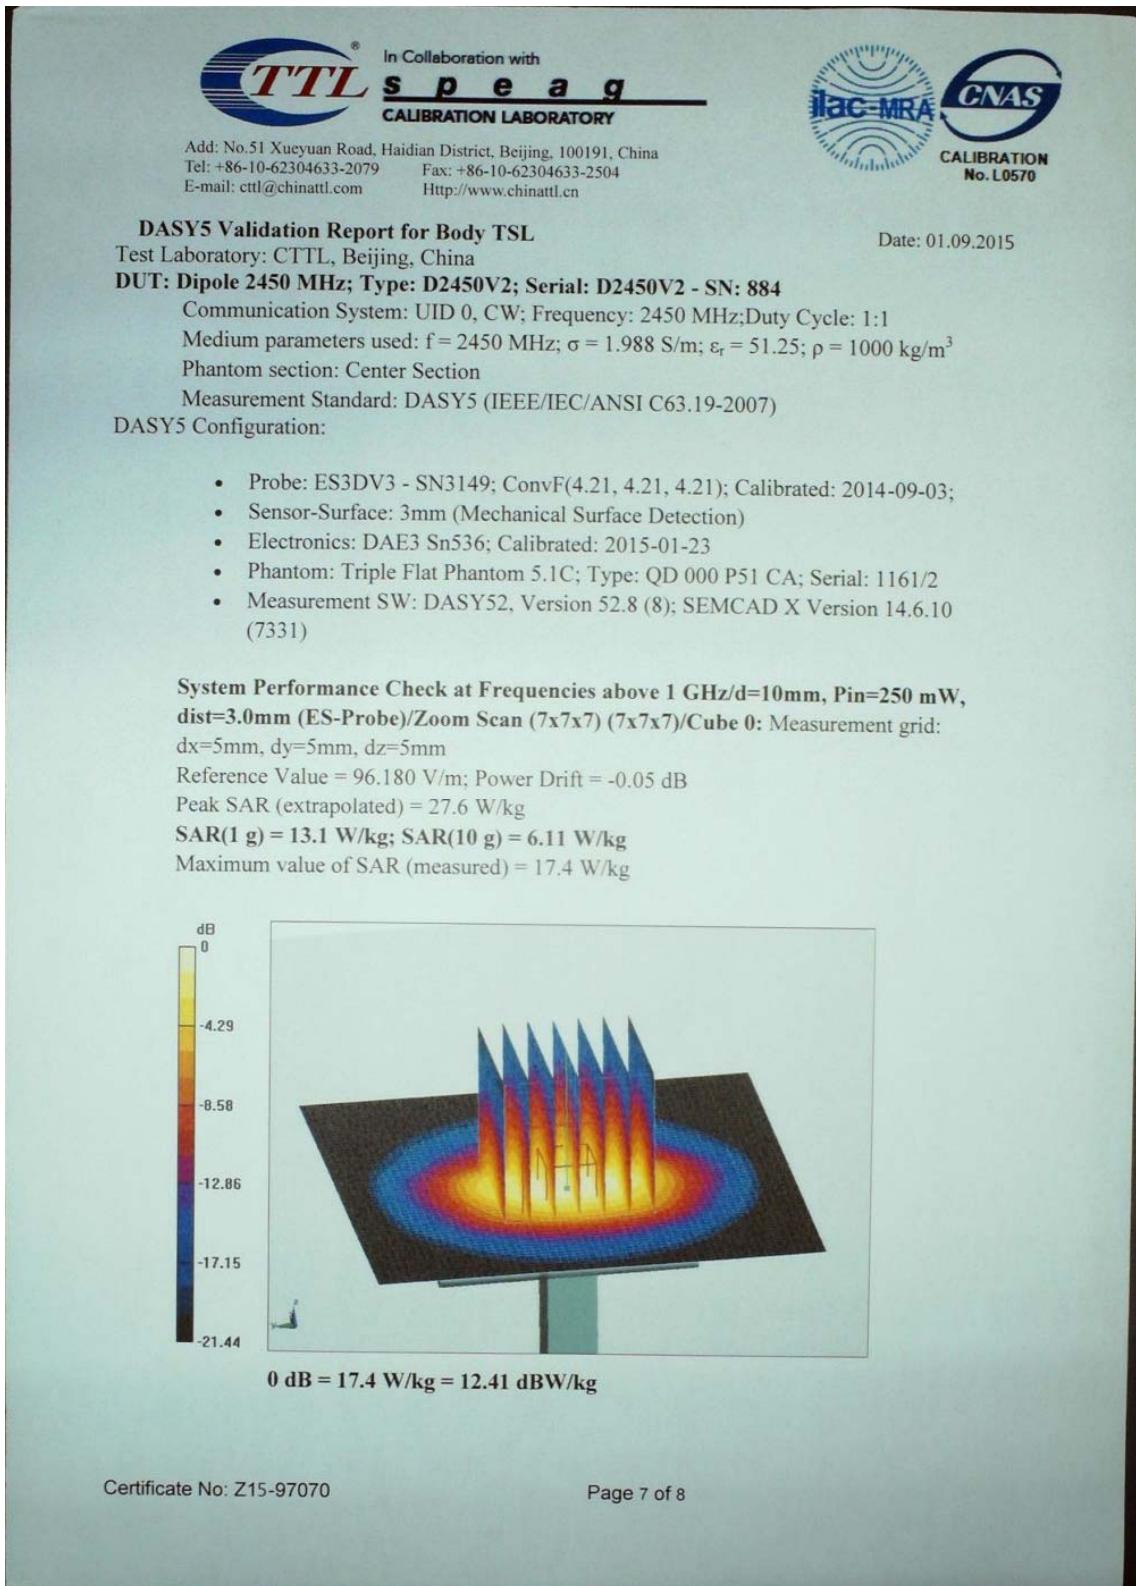

## Appendix A: Calibration Certificate

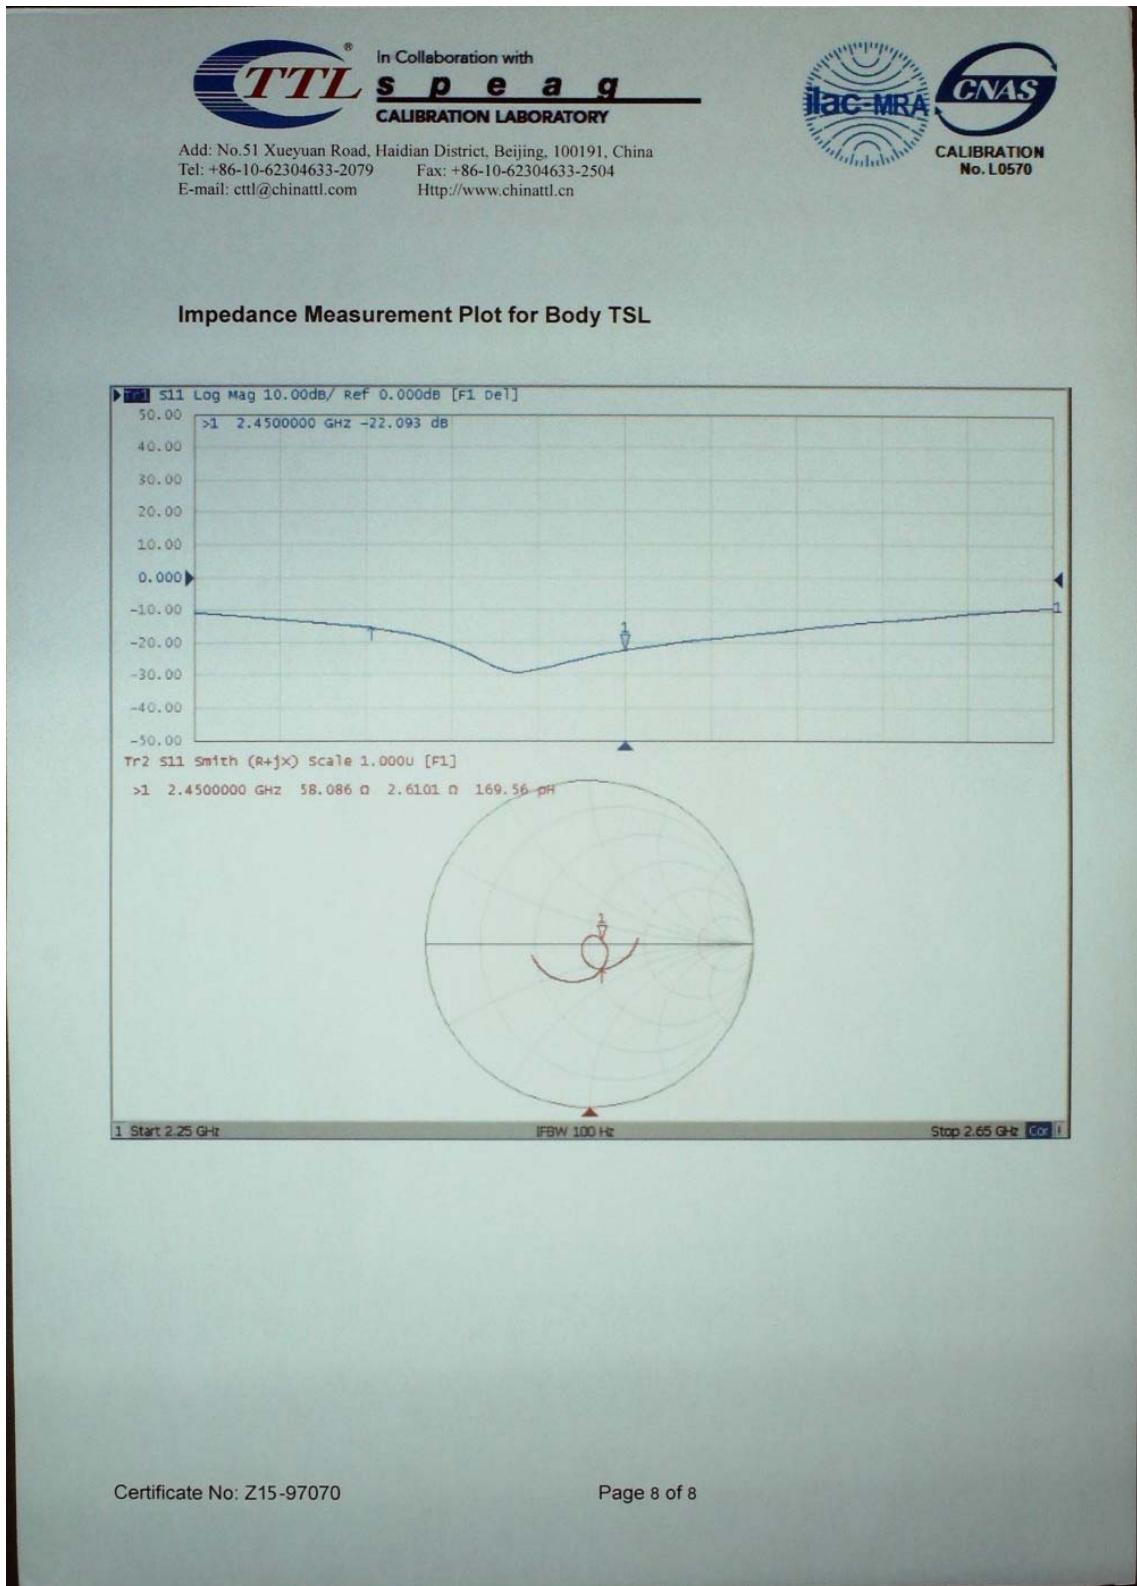

## Extended Dipole Calibrations

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Head						
Date of measurement	Return-loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary impedance (ohm)	Delta (ohm)
2015-09-01	-22.3		58.3		-0.76	
2016-08-31	-21.8	2.24	58.5	0.2	-0.68	0.08

Body						
Date of measurement	Return-loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary impedance (ohm)	Delta (ohm)
2015-09-01	-22.1		58.1		2.61	
2016-08-31	-21.5	2.71	59.0	0.9	2.36	-0.25

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5ohm of prior calibration. Therefore the verification result should support extended calibration.

## 1.5. DAE4 Calibration Certificate





 In Collaboration with  
**speag**  
 CALIBRATION LABORATORY
 


**MRA**  
**CNAS**  
 中国认可  
 国际互认  
 校准  
 CALIBRATION  
 CNAS L0570

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2218  
 Fax: +86-10-62304633-2209  
 E-mail: ctll@chinattl.com  
<http://www.chinattl.cn>

Client : **CIQ(Shenzhen)**      Certificate No: Z16-97120

**CALIBRATION CERTIFICATE**

Object	DAE4 - SN: 1315		
Calibration Procedure(s)	<b>FD-Z11-2-002-01</b> Calibration Procedure for the Data Acquisition Electronics (DAE4)		
Calibration date:	July 26, 2016		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature( $22\pm3$ )°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Process Calibrator 753	1971018	27-June-16 (CTTL, No:J16X04778)	June-17
Calibrated by:	Name Yu Zongying	Function SAR Test Engineer	Signature 
Reviewed by:	Name QI Dianyuan	Function SAR Project Leader	Signature 
Approved by:	Name Lu Bingsong	Function Deputy Director of the laboratory	Signature 
Issued: July 27, 2016 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2218 Fax: +86-10-62304633-2209  
E-mail: [cttl@chinattl.com](mailto:cttl@chinattl.com) [Http://www.chinattl.cn](http://www.chinattl.cn)

**Glossary:**

DAE data acquisition electronics  
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

**Methods Applied and Interpretation of Parameters:**

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2218 Fax: +86-10-62304633-2209  
E-mail: ctli@chinattl.com Http://www.chinattl.cn

#### DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB =  $6.1\mu V$ , full range =  $-100...+300 mV$   
Low Range: 1LSB =  $61nV$ , full range =  $-1.....+3mV$

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	$405.179 \pm 0.15\% (k=2)$	$405.018 \pm 0.15\% (k=2)$	$404.98 \pm 0.15\% (k=2)$
Low Range	$3.99015 \pm 0.7\% (k=2)$	$3.98549 \pm 0.7\% (k=2)$	$3.98861 \pm 0.7\% (k=2)$

#### Connector Angle

Connector Angle to be used in DASY system	$20.5^\circ \pm 1^\circ$
---	--------------------------