



Keep Track of Your Injections

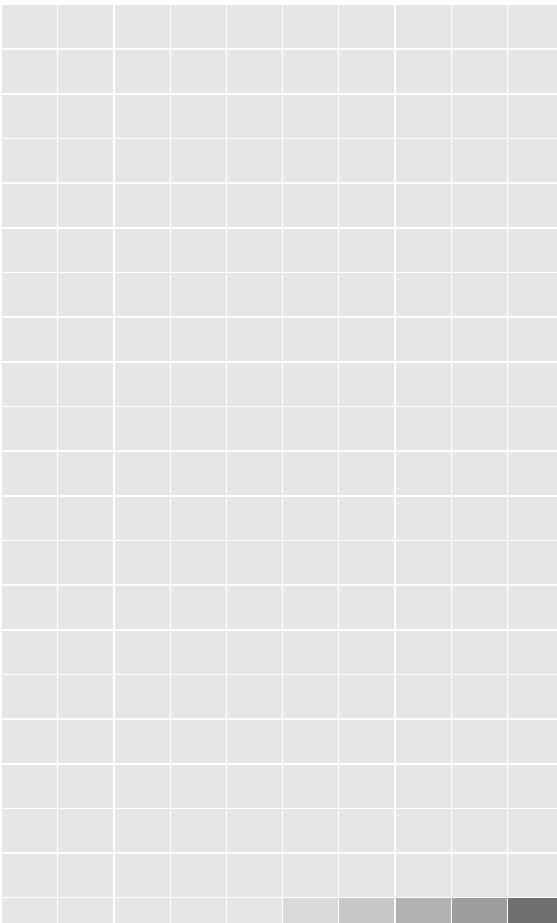

8020100530_04
#02 2024-08-27

This is your
Instructions for Use

- For quick overview of steps, read your Quick Reference Guide
- For training video, go to www.skytrofa.com



Instructions
for Use



Quick
Reference Guide



Training
Video

www.skytrofa.com

Ascendis Pharma Customer Support



1-844-44ASCENDIS
(1-844-442-7236)



Distributed by:

Ascendis Pharma Endocrinology Inc.
Princeton, NJ 08540
USA



Phillips-Medisize A/S
Gimsinglundvej 20
DK-7600 Struer
Denmark

This Instructions for Use has been approved by

[Placeholder]

Approved: Month, Year

Instructions for Use

Skytrofa® Auto-Injector

For SKYTROFA cartridges

Single-patient use



Watch Video



www.skytrofa.com

Parts Overview



Getting Started

How to Use



Troubleshooting and Care

Product Information

Status Icons



Green Check Mark
Injection successfully completed



Green Eye
Mixed medicine is ready for inspection in window



Green Mixing
Medicine mixing is in progress

► Read more about status icons on pages 26-45 (and pages 52-63 for troubleshooting)



Constant Green
► Battery is fully charged
► The auto-injector is ready to use



Flashing Green
► At least 1 injection remaining, but charging recommended after use



Flashing Orange
► Battery needs charging

► Read more about battery status icons on page 25