

Annex C: Calibration Reports

Tested Model: DT080-MS-W10

Report Number:

FCC17060478A



SAR Reference Dipole Calibration Report

Ref: ACR.176.6.15.SATU.A

WORLD STANDARDIZATION CERTIFICATION & TESTING CO.,LTD

BLOCK A, BAO SHI SCIENCE PARK,BAO SHI ROAD, BAO'AN DISTRICT SHENZHEN 518108,P.R. CHINA

MVG COMOSAR REFERENCE DIPOLE

FREQUENCY: 2450 MHZ

SERIAL NO.: SN 14/13 DIP 2G450-238

Calibrated at MVG US

2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 7/25/2016

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



	Name Fund		Date	Signature	
Prepared by:	J ér ôme LUC	Product Manager	7/25/2016	JES	
Checked by:	J á âme LUC	Product Manager	7/25/2016	JE	
Approved by :	Kim RUTKOWSKI	Quality Manager	7/25/2016	frem Puthowski	

Ø	Customer Name		
	World		
Distribution	Standardization		
Distribution :	Certification &		
	Testing Co.,Ltd		

Issue	Date	Modifications	
A	7/25/2016	Initial release	
497			



TABLE OF CONTENTS

1	Intro	luction	
2	Devic	e Under Test	
3	Produ	act Description	
	3.1	General Information	4
4	Meas	urement Method	
	4.1	Return Loss Requirements	5
	4.2	Mechanical Requirements	5
5	Meas	urement Uncertainty	
	5.1	Return Loss	5
	5.2	Dimension Measurement	5
	5.3	Validation Measurement	5
6	Calibr	ration Measurement Results	
	6.1	Return Loss and Impedance In Head Liquid	6
	6.2	Return Loss and Impedance In Body Liquid	6
	6.3	Mechanical Dimensions	6
7	Valida	ation measurement	
	7.1	Head Liquid Measurement	7
	7.2	SAR Measurement Result With Head Liquid	8
	7.3	Body Liquid Measurement	9
	7.4	SAR Measurement Result With Body Liquid	10
8	List o	f Equipment11	



1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEEE 1528, FCC KDBs and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

Device Under Test			
Device Type COMOSAR 2450 MHz REFERENCE DIPOL			
Manufacturer	MVG		
Model SID2450			
Serial Number SN 14/13 DIP 2G450-238			
Product Condition (new / used) Used			

A yearly calibration interval is recommended.

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, FCC KDBs and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – MVG COMOSAR Validation Dipole



4 MEASUREMENT METHOD

The IEEE 1528, FCC KDBs and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constucted as outlined in the fore mentioned standards.

4.2 MECHANICAL REQUIREMENTS

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

Frequency band	Expanded Uncertainty on Return Loss
400-6000MHz	0.1 dB

5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

Length (mm)	Expanded Uncertainty on Length		
3 - 300	0.05 mm		

5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEEE 1528, FCC KDBs, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.


Scan Volume	Expanded Uncertainty
1g	20.3 %



10 g	20.1 %
I .	


6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

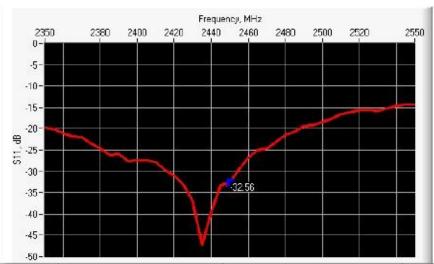

Frequency (MHz)	Return Loss (dB)	Requirement (dB)	Impedance
2450	-32.56	-20	48.3 Ω - 1.6 j

6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

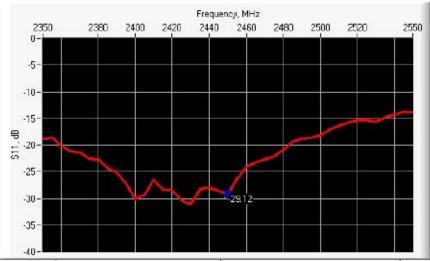

Frequency (MHz)	Return Loss (dB)	Requirement (dB)	Impedance
2450	-29.12	-20	$0.0 \Omega + 11.0 j$

6.3 MECHANICAL DIMENSIONS

Frequency MHz	L mm		h mm		d mm	
	required	measured	required	measured	required	measured
300	420.0 ±1 %.		250.0 ±1 %.		6.35 ±1 %.	

Page: 6/11



290.0 ±1 %.		166.7 ±1 %.		6.35 ±1 %.	
176.0 ±1 %.		100.0 ±1 %.		6.35 ±1 %.	
161.0 ±1 %.		89.8 ±1 %.		3.6 ±1 %.	
149.0 ±1 %.		83.3 ±1 %.		3.6 ±1 %.	
89.1 ±1 %.		51.7 ±1 %.		3.6 ±1 %.	
80.5 ±1 %.		50.0 ±1 %.		3.6 ±1 %.	
79.0 ±1 %.		45.7 ±1 %.		3.6 ±1 %.	
75.2 ±1 %.		42.9 ±1 %.		3.6 ±1 %.	
72.0 ±1 %.		41.7 ±1 %.		3.6 ±1 %.	
68.0 ±1 %.		39.5 ±1 %.		3.6 ±1 %.	
66.3 ±1 %.		38.5 ±1 %.		3.6 ±1 %.	
64.5 ±1 %.		37.5 ±1 %.		3.6 ±1 %.	
61.0 ±1 %.		35.7 ±1 %.		3.6 ±1 %.	
55.5 ±1 %.		32.6 ±1 %.		3.6 ±1 %.	
51.5 ±1 %.	PASS	30.4 ±1 %.	PASS	3.6 ±1 %.	PASS
48.5 ±1 %.		28.8 ±1 %.		3.6 ±1 %.	
41.5 ±1 %.		25.0 ±1 %.		3.6 ±1 %.	
37.0±1 %.		26.4 ±1 %.		3.6 ±1 %.	
34.7±1 %.		26.4 ±1 %.		3.6 ±1 %.	
	176.0 ±1 %. 161.0 ±1 %. 149.0 ±1 %. 89.1 ±1 %. 80.5 ±1 %. 79.0 ±1 %. 72.0 ±1 %. 68.0 ±1 %. 66.3 ±1 %. 61.0 ±1 %. 55.5 ±1 %. 48.5 ±1 %. 41.5 ±1 %. 37.0±1 %.	176.0 ±1 %. 161.0 ±1 %. 149.0 ±1 %. 89.1 ±1 %. 80.5 ±1 %. 79.0 ±1 %. 72.0 ±1 %. 68.0 ±1 %. 66.3 ±1 %. 61.0 ±1 %. 55.5 ±1 %. 51.5 ±1 %. 41.5 ±1 %. 37.0±1 %.	176.0 ±1 %. 100.0 ±1 %. 161.0 ±1 %. 89.8 ±1 %. 149.0 ±1 %. 83.3 ±1 %. 89.1 ±1 %. 51.7 ±1 %. 80.5 ±1 %. 50.0 ±1 %. 79.0 ±1 %. 45.7 ±1 %. 72.0 ±1 %. 41.7 ±1 %. 68.0 ±1 %. 39.5 ±1 %. 66.3 ±1 %. 37.5 ±1 %. 61.0 ±1 %. 35.7 ±1 %. 55.5 ±1 %. 32.6 ±1 %. 48.5 ±1 %. 28.8 ±1 %. 41.5 ±1 %. 25.0 ±1 %. 37.0±1 %. 26.4 ±1 %.	176.0 ±1 %. 100.0 ±1 %. 161.0 ±1 %. 89.8 ±1 %. 149.0 ±1 %. 83.3 ±1 %. 89.1 ±1 %. 51.7 ±1 %. 80.5 ±1 %. 50.0 ±1 %. 79.0 ±1 %. 45.7 ±1 %. 75.2 ±1 %. 42.9 ±1 %. 72.0 ±1 %. 41.7 ±1 %. 68.0 ±1 %. 39.5 ±1 %. 66.3 ±1 %. 38.5 ±1 %. 64.5 ±1 %. 35.7 ±1 %. 55.5 ±1 %. 32.6 ±1 %. 70.0 ±1 %. 28.8 ±1 %. 41.5 ±1 %. 25.0 ±1 %. 37.0 ±1 %. 26.4 ±1 %.	176.0 ±1 %. 100.0 ±1 %. 6.35 ±1 %. 161.0 ±1 %. 89.8 ±1 %. 3.6 ±1 %. 149.0 ±1 %. 83.3 ±1 %. 3.6 ±1 %. 89.1 ±1 %. 51.7 ±1 %. 3.6 ±1 %. 80.5 ±1 %. 50.0 ±1 %. 3.6 ±1 %. 79.0 ±1 %. 45.7 ±1 %. 3.6 ±1 %. 75.2 ±1 %. 42.9 ±1 %. 3.6 ±1 %. 72.0 ±1 %. 41.7 ±1 %. 3.6 ±1 %. 68.0 ±1 %. 39.5 ±1 %. 3.6 ±1 %. 66.3 ±1 %. 36.5 ±1 %. 3.6 ±1 %. 61.0 ±1 %. 35.7 ±1 %. 3.6 ±1 %. 55.5 ±1 %. 32.6 ±1 %. 3.6 ±1 %. 48.5 ±1 %. 28.8 ±1 %. 3.6 ±1 %. 41.5 ±1 %. 25.0 ±1 %. 3.6 ±1 %. 37.0±1 %. 3.6 ±1 %. 3.6 ±1 %.

7 VALIDATION MEASUREMENT

The IEEE Std. 1528, FCC KDBs and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 HEAD LIQUID MEASUREMENT

Frequency MHz	Relative peri	Relative permittivity (-/')		ity (σ) S/m
	required	measured	required	measured
300	45.3 ±5 %		0.87 ±5 %	
450	43.5 ±5 %		0.87 ±5 %	
750	41.9 ±5 %		0.89 ±5 %	
835	41.5 ±5 %		0.90 ±5 %	
900	41.5 ±5 %		0.97 ±5 %	
1450	40.5 ±5 %		1.20 ±5 %	
1500	40.4 ±5 %		1.23 ±5 %	
1640	40.2 ±5 %		1.31 ±5 %	
1750	40.1 ±5 %		1.37 ±5 %	

Page: 7/11



1800	40.0 ±5 %		1.40 ±5 %	
1900	40.0 ±5 %		1.40 ±5 %	
1950	40.0 ±5 %		1.40 ±5 %	
2000	40.0 ±5 %		1.40 ±5 %	
2100	39.8 ±5 %		1.49 ±5 %	
2300	39.5 ±5 %		1.67 ±5 %	
2450	39.2 ±5 %	PASS	1.80 ±5 %	PASS
2600	39.0 ±5 %		1.96 ±5 %	
3000	38.5 ±5 %		2.40 ±5 %	
3500	37.9 ±5 %		2.91 ±5 %	

7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.


Software	OPENSAR V4
Phantom	SN 20/09 SAM71
Probe	SN 18/11 EPG122
Liquid	Head Liquid Values: eps': 38.3 sigma: 1.80
Distance between dipole center and liquid	10.0 mm
Area scan resolution	dx=8mm/dy=8mm
Zoon Scan Resolution	dx=5mm/dy=5mm/dz=5mm
Frequency	2450 MHz
Input power	20 dBm
Liquid Temperature	21 ℃
Lab Temperature	21 ℃
Lab Humidity	45 %

Frequency MHz	1 g SAR (V	V/kg/W)	10 g SAR (W/kg/W)
	required	measured	required	measured
300	2.85		1.94	
450	4.58		3.06	
750	8.49		5.55	
835	9.56		6.22	
900	10.9		6.99	
1450	29		16	
1500	30.5		16.8	
1640	34.2		18.4	
1750	36.4		19.3	1
1800	38.4		20.1	

Page: 8/11



1900	39.7		20.5	
1950	40.5		20.9	
2000	41.1		21.1	
2100	43.6		21.9	
2300	48.7		23.3	
2450	52.4	53.41 (5.34)	24	23.95 (2.40)
2600	55.3		24.6	
3000	63.8		25.7	
3500	67.1		25	

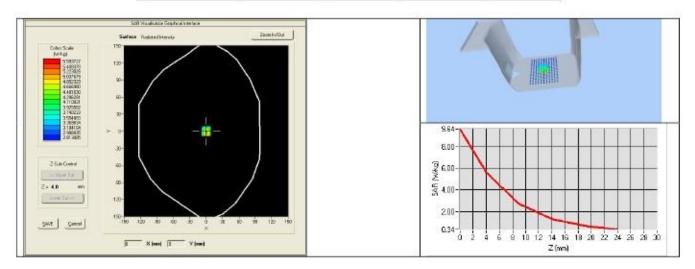

7.3 BODY LIQUID MEASUREMENT

Frequency MHz	Relative perr	mittivity (-/)	Conductiv	ity (σ) S/m
	required	measured	required	measured
150	61.9 ±5 %		0.80 ±5 %	
300	58.2 ±5 %		0.92 ±5 %	
450	56.7 ±5 %		0.94 ±5 %	
750	55.5 ±5 %		0.96 ±5 %	
835	55.2 ±5 %		0.97 ±5 %	
900	55.0 ±5 %		1.05 ±5 %	
915	55.0 ±5 %		1.06 ±5 %	
1450	54.0 ±5 %		1.30 ±5 %	
1610	53.8 ±5 %		1.40 ±5 %	
1800	53.3 ±5 %		1.52 ±5 %	
1900	53.3 ±5 %		1.52 ±5 %	
2000	53.3 ±5 %		1.52 ±5 %	
2100	53.2 ±5 %		1.62 ±5 %	
2450	52.7 ±5 %	PASS	1.95 ±5 %	PASS

Page: 9/11




2600	52.5 ±5 %	2.16 ±5 %
3000	52.0 ±5 %	2.73 ±5 %
3500	51.3 ±5 %	3.31 ±5 %
5200	49.0 ±10 %	5.30 ±10 %
5300	48.9 ±10 %	5.42 ±10 %
5400	48.7 ±10 %	5.53 ±10 %
5500	48.6 ±10 %	5.65 ±10 %
5600	48.5 ±10 %	5.77 ±10 %
5800	48.2 ±10 %	6.00 ±10 %

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

Software	OPENSAR V4	
Phantom	SN 20/09 SAM71	
Probe	SN 18/11 EPG122	
Liquid	Body Liquid Values: eps': 52.7 sigma: 1.94	
Distance between dipole center and liquid	10.0 mm	
Area scan resolution	dx=8mm/dy=8mm	
Zoon Scan Resolution	dx=5mm/dy=5mm/dz=5mm	
Frequency	2450 MHz	
Input power	20 dBm	
Liquid Temperature	21 ℃	
Lab Temperature	21 ℃	
Lab Humidity	45 %	

Frequency MHz	1 g SAR (W/kg/W)	10 g SAR (W/kg/W)
	measured	measured
2450	51.39 (5.14)	23.63 (2.36)

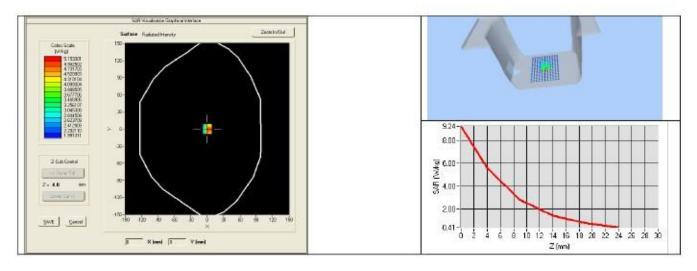

Page: 10/11



8 LIST OF EQUIPMENT

Equipment Summary Sheet					
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date	
SAM Phantom	MVG	SN-20/09-SAM71	Validated. No cal required.	Validated. No cal required.	
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.	
Network Analyzer	Rhode & Schwarz ZVA	SN100132	02/2015	02/2018	
Calipers	Carrera	CALIPER-01	12/2013	12/2016	
Reference Probe	MVG	EPG122 SN 18/11	06/2016	06/2017	
Multimeter	Keithley 2000	1188656	12/2013	12/2016	
Signal Generator	Agilent E4438C	MY49070581	12/2013	12/2016	
Amplifier	Aethercomm	SN 046	Characterized prior to Class. No cal required. tes		
Power Meter	HP E4418A	US38261498	12/2013	12/2016	
Power Sensor	HP ECP-E26A	US37181460	12/2013	12/2016	
Directional Coupler	Narda 4216-20	01386	Characterized prior to Characterized prior to test. No cal required. test. No cal required.		
Temperature and Humidity Sensor	Control Company	11-661-9	12/2014	12/2017	



SAR Reference Waveguide Calibration Report

Ref: ACR.176.9.16.SATU.A

WORLD STANDARDIZATION CERTIFICATION & TESTING CO.,LTD

BLOCK A, BAO SHI SCIENCE PARK,BAO SHI ROAD, BAO'AN DISTRICT SHENZHEN 518108,P.R. CHINA

MVG COMOSAR DOSIMETRIC E-FIELD PROBE

FREQUENCY: 5000-6000 MHZ SERIAL NO.: SN 14/13 EPG239

Calibrated at MVG US 2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 7/25/2016

Summary:

This document presents the method and results from an accredited SAR reference waveguide calibration performed in MVG USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.





	Name	Function	Date	Signature
Prepared by :	Jérôme LUC	Product Manager	7/25/2016	JS
Checked by:	Jérôme LUC	Product Manager	7/25/2016	JES
Approved by:	Kim RUTKOWSKI	Quality Manager	7/25/2016	thim Puthowski

	Customer Name
	World
Distribution :	Standardization
	Certification &
	Testing Co .,Ltd

Issue	Date	Modifications
A	7/25/2016	Initial release






TABLE OF CONTENTS

1	Introduction4	
2	Device Under Test4	
3	Product Description4	
	3.1 General Information	4
4	Measurement Method4	
	Return Loss Requirements	4
	Mechanical Requirements	4
5	Measurement Uncertainty5	
	Return Loss	5
	ension Measurement	Dim 5
	Validation Measurement	
6	Calibration Measurement Results5	
	Return Loss_	5
	Mechanical Dimensions	6
7	Validation measurement7	
	Head Liquid Measurement	7
	surement Result_	Mea 7
	Body Measurement Result	10
8	List of Equipment	



1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEEE 1528 and CEI/IEC 62209 standards for reference waveguides used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

	Device Under Test
Device Type	COMOSAR 5000-6000 MHz REFERENCE WAVEGUIDE
Manufacturer	MVG
Model	SWG5500
Serial Number	SN 14/13 EPG239
Product Condition (new / used)	Used

A yearly calibration interval is recommended.

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Waveguides are built in accordance to the IEEE 1528 and CEI/IEC 62209 standards.

4 MEASUREMENT METHOD

The IEEE 1528 and CEI/IEC 62209 standards provide requirements for reference waveguides used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

RETURN LOSS REQUIREMENTS

The waveguide used for SAR system validation measurements and checks must have a return loss of -8 dB or better. The return loss measurement shall be performed with matching layer placed in the open end of the waveguide, with the waveguide and matching layer in direct contact with the phantom shell as outlined in the fore mentioned standards.

MECHANICAL REQUIREMENTS

The IEEE 1528 and CEI/IEC 62209 standards specify the mechanical dimensions of the validation waveguide, the specified dimensions are as shown in Section 6.2. Figure 1 shows how the dimensions relate to the physical construction of the waveguide.



5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

RETURN LOSS

The following uncertainties apply to the return loss measurement:

Frequency band	Expanded Uncertainty on Return Loss		
400-6000MHz	0.1 dB		

DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

Length (mm)	Expanded Uncertainty on Length
3 - 300	0.05 mm


VALIDATION MEASUREMENT

The guidelines outlined in the IEEE 1528 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

Scan Volume	Expanded Uncertainty
1 g	20.3 %
10 g	20.1 %

6 CALIBRATION MEASUREMENT RESULTS

RETURN LOSS IN HEAD LIQUID

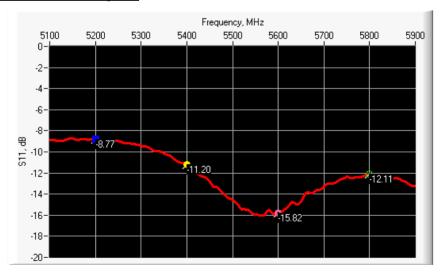


Page: 5/13



SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Frequency (MHz)	Return Loss (dB)	Requirement (dB)	Impedance
5200	-8.77	-8	$25.52 \Omega + 13.34 j\Omega$
5400	-11.20	-8	$85.09 \Omega + 12.81 j\Omega$
5600	-15.82	-8	36.65 Ω - 4.32 jΩ
5800	-12.11	-8	$53.20 \Omega + 26.19 j\Omega$

RETURN LOSS IN BODY LIQUID

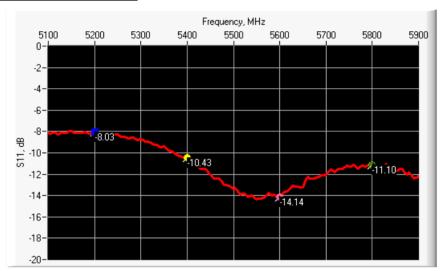

Frequency (MHz)	Return Loss (dB)	Requirement (dB)	Impedance
5200	-8.03	-8	$24.31 \Omega + 15.75 j\Omega$
5400	-10.43	-8	$92.67 \Omega + 5.39 j\Omega$
5600	-14.14	-8	33.81 Ω - 2.99 jΩ
5800	-11.10	-8	$57.11 \Omega + 30.17 j\Omega$

MECHANICAL DIMENSIONS

Г	L (mm)		W (mm)		L_{f} (mm)		W _f (mm)		T (mm)	
Frequenc	Require	Measure	Require	Measure	Require	Measure	Require	Measure	Require	Measure
y (MHz)	d	d	d	d	d	d	d	d	d	d
5200	40.39 ± 0.13	PASS	20.19 ± 0.13	PASS	81.03 ± 0.13	PASS	61.98 ± 0.13	PASS	5.3*	PASS
5800	40.39 ± 0.13	PASS	20.19 ± 0.13	PASS	81.03 ± 0.13	PASS	61.98 ± 0.13	PASS	4.3*	PASS

^{*} The tolerance for the matching layer is included in the return loss measurement.



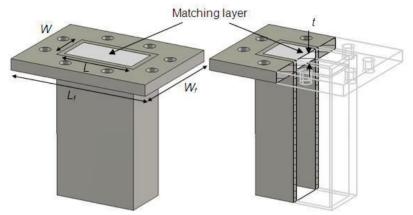


Figure 1: Validation Waveguide Dimensions

7 VALIDATION MEASUREMENT

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference waveguide meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed with the matching layer placed in the open end of the waveguide, with the waveguide and matching layer in direct contact with the phantom shell.

HEAD LIQUID MEASUREMENT

Frequency MHz	Relative perr	mittivity (ε _r ')	Conductivi	ity (σ) S/m
	required	measured	required	measured
5000	36.2 ±10 %		4.45 ±10 %	
5100	36.1 ±10 %		4.56 ±10 %	
5200	36.0 ±10 %	PASS	4.66 ±10 %	PASS
5300	35.9 ±10 %		4.76 ±10 %	
5400	35.8 ±10 %	PASS	4.86 ±10 %	PASS
5500	35.6 ±10 %		4.97 ±10 %	
5600	35.5 ±10 %	PASS	5.07 ±10 %	PASS
5700	35.4 ±10 %		5.17 ±10 %	
5800	35.3 ±10 %	PASS	5.27 ±10 %	PASS
5900	35.2 ±10 %		5.38 ±10 %	
6000	35.1 ±10 %		5.48 ±10 %	

SAR MEASUREMENT RESULT WITH HEAD LIQUID

At those frequencies, the target SAR value can not be generic. Hereunder is the target SAR value defined by MVG, within the uncertainty for the system validation. All SAR values are normalized to 1 W net power. In bracket, the measured SAR is given with the used input power.




SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Software	OPENSAR V4
Phantom	SN 20/09 SAM71
Probe	SN 18/11 EPG122
Liquid	Head Liquid Values 5200 MHz: eps' :35.64 sigma : 4.67 Head Liquid Values 5400 MHz: eps' :36.44 sigma : 4.87 Head Liquid Values 5600 MHz: eps' :36.66 sigma : 5.17 Head Liquid Values 5800 MHz: eps' :35.31 sigma : 5.31
Distance between dipole waveguide and liquid	0 mm
Area scan resolution	dx=8mm/dy=8mm
Zoon Scan Resolution	dx=4mm/dy=4m/dz=2mm
Frequency	5200 MHz 5400 MHz 5600 MHz 5800 MHz
Input power	20 dBm
Liquid Temperature	21 °C
Lab Temperature	21 °C
Lab Humidity	45 %


Frequency (MHz)	1 g SAR (W/kg)		$\begin{array}{c ccccccccccccccccccccccccccccccccccc$		R (W/kg)
	required measured		required	measured	
5200	159.00	164.05 (16.41)	56.90	57.03 (5.70)	
5400	166.40	171.66 (17.17)	58.43	59.33 (5.93)	
5600	173.80	177.81 (17.78)	59.97	60.90 (6.09)	
5800	181.20	185.02 (18.50)	61.50	62.43 (6.24)	


SAR MEASUREMENT PLOTS @ 5200 MHz

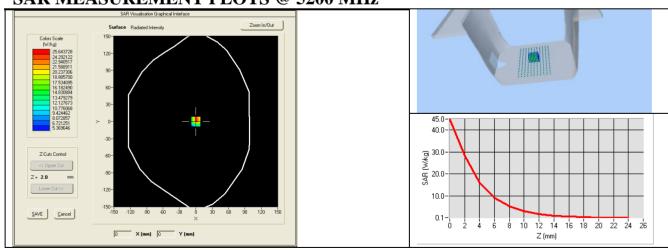





SAR MEASUREMENT PLOTS @ 5400 MHz







SAR MEASUREMENT PLOTS @ 5600 MHz





SAR MEASUREMENT PLOTS @ 5800 MHz

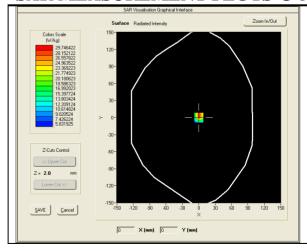



Page: 9/13



SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

BODY LIQUID MEASUREMENT

Frequency MHz	Relative permittivity (ϵ_{r} ')		Conductivity (σ) S/m		
	required	required measured		measured	
5200	49.0 ±10 %	PASS	5.30 ±10 %	PASS	
5300	48.9 ±10 %		5.42 ±10 %		
5400	48.7 ±10 %	PASS	5.53 ±10 %	PASS	
5500	48.6 ±10 %		5.65 ±10 %		
5600	48.5 ±10 %	PASS	5.77 ±10 %	PASS	
5800	48.2 ±10 %	PASS	6.00 ±10 %	PASS	


SAR MEASUREMENT RESULT WITH BODY LIQUID


Software	OPENSAR V4
Phantom	SN 20/09 SAM71
Probe	SN 18/11 EPG122
Liquid	Body Liquid Values 5200 MHz: eps':48.64 sigma: 5.51 Body Liquid Values 5400 MHz: eps':46.52 sigma: 5.77 Body Liquid Values 5600 MHz: eps':46.79 sigma: 5.77 Body Liquid Values 5800 MHz: eps':47.04 sigma: 6.10
Distance between dipole waveguide and liquid	0 mm
Area scan resolution	dx=8mm/dy=8mm
Zoon Scan Resolution	dx=4mm/dy=4m/dz=2mm
Frequency	5200 MHz 5400 MHz 5600 MHz 5800 MHz
Input power	20 dBm
Liquid Temperature	21 °C
Lab Temperature	21 °C
Lab Humidity	45 %

Frequency (MHz)	1 g SAR (W/kg)	10 g SAR (W/kg)
	measured	measured
5200	163.36 (16.34)	57.09 (5.71)
5400	166.22 (16.62)	57.22 (5.72)
5600	172.11 (17.21)	58.61 (5.86)
5800	177.10 (17.71)	59.95 (5.99)





BODY SAR MEASUREMENT PLOTS @ 5200 MHz







BODY SAR MEASUREMENT PLOTS @ 5400 MHz





BODY SAR MEASUREMENT PLOTS @ 5600 MHz






Page: 11/13



BODY SAR MEASUREMENT PLOTS @ 5800 MHz

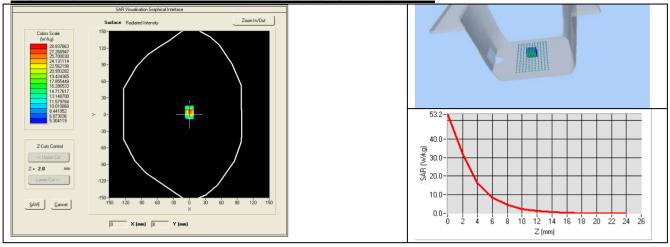





8 LIST OF EQUIPMENT

Equipment Summary Sheet						
Equipment Manufacturer / Description Model		Identification No.	Current Calibration Date	Next Calibration Date		
Flat Phantom	MVG	SN-20/09-SAM71	Validated. No cal required.	Validated. No cal required.		
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.		
Network Analyzer	Rhode & Schwarz ZVA	SN100132	02/2015	02/2018		
Calipers	Carrera	CALIPER-01	12/2013	12/2016		
Reference Probe	MVG	EPG122 SN 18/11	10/2015	10/2016		
Multimeter	Keithley 2000	1188656	12/2013	12/2016		
Signal Generator	Agilent E4438C	MY49070581	12/2013	12/2016		
Amplifier	Aethercomm	SN 046	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.		
Power Meter	HP E4418A	US38261498	12/2013	12/2016		
Power Sensor	HP ECP-E26A	US37181460	12/2013	12/2016		
Directional Coupler	Narda 4216-20	01386	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.		
Temperature and Humidity Sensor	Control Company	150798832	10/2014	10/2017		



COMOSAR E-Field Probe Calibration Report

Ref: ACR.176.8.15.SATU.A

WORLD STANDARDIZATION CERTIFICATION & TESTING CO .,LTD

BLOCK A, BAO SHI SCIENCE PARK,BAO SHI ROAD, BAO'AN DISTRICT

SHENZHEN 518108,P.R. CHINA

MVG COMOSAR DOSIMETRIC E-FIELD PROBE

SERIAL NO.: SN 07/15 EP252

Calibrated at MVG US 2105 Barrett Park Dr. - Kennesaw, GA 30144





Calibration Date: 7/25/2016

Summary:

This document presents the method and results from an accredited COMOSAR Dosimetric E-Field Probe calibration performed in MVG USA using the CALISAR / CALIBAIR test bench, for use with a COMOSAR system only. All calibration results are traceable to national metrology institutions.



	Name	Function	Date	Signature
Prepared by:	J ér âme LUC	Product Manager	7/25/2016	JES
Checked by:	J ér ôme LUC	Product Manager	7/25/2016	JES
Approved by :	Kim RUTKOWSKI	Quality Manager	7/25/2016	Jum Puthowski

8	Customer Name		
	World		
Distriction	Standardization		
Distribution :	Certification &		
	Testing Co.,Ltd		

Issue	Date	Modifications
A	7/25/2016	Initial release
eve .		



TABLE OF CONTENTS

I	Device Under Test4	
2	Product Description4	
	2.1 General Information	4
3	Measurement Method4	
	Linearity	4
	Sensitivity	
	Lower Detection Limit	5
	Isotropy	5
	Boundary Effect	5
4	Measurement Uncertainty5	
5	Calibration Measurement Results6	
	Sensitivity in air	6
	Linearity	
	Sensitivity in liquid	7
	Isotropy	8
6	List of Equipment9	



1 DEVICE UNDER TEST

Device Under Test			
Device Type COMOSAR DOSIMETRIC E FIELD PROB			
Manufacturer	MVG		
Model	SSE5		
Serial Number	SN 07/15 EP252		
Product Condition (new / used)	New		
Frequency Range of Probe	0.7 GHz-6GHz		
Resistance of Three Dipoles at Connector	Dipole 1: R1=0.217 MΩ		
	Dipole 2: R2=0.215 MΩ		
	Dipole 3: R3=0.215 M Ω		

A yearly calibration interval is recommended.

2 PRODUCT DESCRIPTION

2.1 <u>GENERAL INFORMATION</u>

MVG's COMOSAR E field Probes are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards.



Figure 1 – MVG COMOSAR Dosimetric E field Dipole

Probe Length	330 mm
Length of Individual Dipoles	4.5 mm
Maximum external diameter	8 mm
Probe Tip External Diameter	5 mm
Distance between dipoles / probe extremity	2.7 mm

3 MEASUREMENT METHOD

The IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards provide recommended practices for the probe calibrations, including the performance characteristics of interest and methods by which to assess their affect. All calibrations / measurements performed meet the fore mentioned standards.

LINEARITY

The evaluation of the linearity was done in free space using the waveguide, performing a power sweep to cover the SAR range 0.01W/kg to 100W/kg.



SENSITIVITY

The sensitivity factors of the three dipoles were determined using a two step calibration method (air and tissue simulating liquid) using waveguides as outlined in the standards.

LOWER DETECTION LIMIT

The lower detection limit was assessed using the same measurement set up as used for the linearity measurement. The required lower detection limit is 10 mW/kg.

ISOTROPY

The axial isotropy was evaluated by exposing the probe to a reference wave from a standard dipole with the dipole mounted under the flat phantom in the test configuration suggested for system validations and checks. The probe was rotated along its main axis from 0 - 360 degrees in 15 degree steps. The hemispherical isotropy is determined by inserting the probe in a thin plastic box filled with tissue-equivalent liquid, with the plastic box illuminated with the fields from a half wave dipole. The dipole is rotated about its axis $(0^{\circ}-180^{\circ})$ in 15° increments. At each step the probe is rotated about its axis $(0^{\circ}-360^{\circ})$.

BOUNDARY EFFECT

The boundary effect is defined as the deviation between the SAR measured data and the expected exponential decay in the liquid when the probe is oriented normal to the interface. To evaluate this effect, the liquid filled flat phantom is exposed to fields from either a reference dipole or waveguide. With the probe normal to the phantom surface, the peak spatial average SAR is measured and compared to the analytical value at the surface.

4 MEASUREMENT UNCERTAINTY

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty associated with an E-field probe calibration using the waveguide technique. All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

Uncertainty analysis of the probe calibration in waveguide						
ERROR SOURCES	Uncertainty value (%)	Probability Distribution	Divisor	ci	Standard Uncertainty (%)	
Incident or forward power	3.00%	Rectangular	$\sqrt{3}$	1	1.732%	
Reflected power	3.00%	Rectangular	\\sqrt{3}_	1	1.732%	
Liquid conductivity	5.00%	Rectangular	\[\ldots \sqrt{3}\]	1	2.887%	
Liquid permittivity	4.00%	Rectangular		1	2.309%	
Field homogeneity	3.00%	Rectangular		1	1.732%	
Field probe positioning	5.00%	Rectangular	$\sqrt{3}$	1	2.887%	



Field probe linearity	3.00%	Rectangular	$\sqrt{3}$	1	1.732%
Combined standard uncertainty					5.831%
Expanded uncertainty 95 % confidence level k = 2					12.0%

5 CALIBRATION MEASUREMENT RESULTS

Calibration Parameters		
Liquid Temperature	21 °C	
Lab Temperature	21 °C	
Lab Humidity	45 %	


SENSITIVITY IN AIR

	Normy dipole	
$1 \left(\mu V / (V/m)^2 \right)$	$2 \left(\mu V / (V/m)^2 \right)$	$3 (\mu V/(V/m)^2)$
6.43	5.43	7.19

DCP dipole 1	DCP dipole 2	DCP dipole 3
(mV)	(mV)	(mV)
93	91	96

Calibration curves ei=f(V) (i=1,2,3) allow to obtain H-field value using the formula:

$$E = \sqrt{E_1^2 + E_2^2 + E_3^2}$$

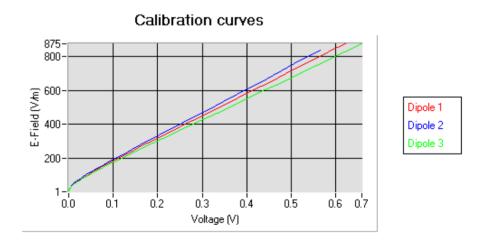


Page: 6/9

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



LINEARITY

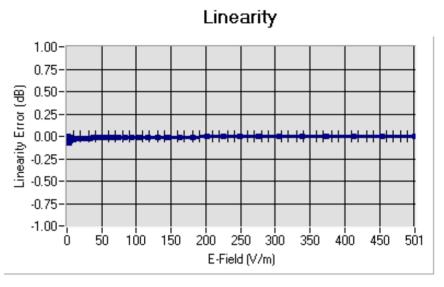

Linearity:[I+/-1.58% (+/-0.07dB)

SENSITIVITY IN LIQUID

<u>Liquid</u>	Frequency	Permittivity	Epsilon (S/m)	ConvF
	<u>(MHz +/-</u>			
	100MHz)			
HL450	450	42.17	0.86	5.29
BL450	450	57.65	0.95	5.43
HL750	750	40.03	0.93	4.74
BL750	750	56.83	1.00	4.85
HL850	835	42.19	0.90	4.93
BL850	835	54.67	1.01	5.07
HL900	900	42.08	1.01	4.65
BL900	900	55.25	1.08	4.83
HL1800	1800	41.68	1.46	4.01
BL1800	1800	53.86	1.46	4.16
HL1900	1900	38.45	1.45	4.63
BL1900	1900	53.32	1.56	4.78
HL2000	2000	38.26	1.38	4.16
BL2000	2000	52.70	1.51	4.25
HL2450	2450	37.50	1.80	4.00
BL2450	2450	53.22	1.89	4.11
HL2600	2600	39.80	1.99	3.92
BL2600	2600	52.52	2.23	4.07
HL5200	5200	35.90	4.71	4.95
BL5200	5200	48.90	5.36	4.40
HL5600	5600	35.50	5.07	4.66
BL5600	5600	48.50	5.77	3.90
HL5800	5800	35.30	5.27	4.66
BL5800	5800	48.20	6.00	4.02


LOWER DETECTION LIMIT: 8mW/kg



ISOTROPY


HL900 MHz

- Axial isotropy: 0.04 dB- Hemispherical isotropy: 0.06 dB



HL1800 MHz

- Axial isotropy: 0.05 dB- Hemispherical isotropy: 0.06 dB





6 LIST OF EQUIPMENT

Equipment Summary Sheet				
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date
Flat Phantom	MVG	SN-20/09-SAM71	Validated. No cal required.	Validated. No cal required.
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.
Network Analyzer	Rhode & Schwarz ZVA	SN100132	02/2015	02/2018
Reference Probe	MVG	EP 94 SN 37/08	06/2016	06/2017
Multimeter	Keithley 2000	1188656	12/2013	12/2016
Signal Generator	Agilent E4438C	MY49070581	12/2013	12/2016
Amplifier	Aethercomm	SN 046	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Power Meter	HP E4418A	US38261498	12/2013	12/2016
Power Sensor	HP ECP-E26A	US37181460	12/2013	12/2016
Directional Coupler	Narda 4216-20	01386	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Waveguide	Mega Industries	069Y7-158-13-712	Validated. No cal required.	Validated. No cal required.
Waveguide Transition	Mega Industries	069Y7-158-13-701	Validated. No cal required.	Validated. No cal required.
Waveguide Termination	Mega Industries	069Y7-158-13-701	Validated. No cal required.	Validated. No cal required.
Temperature / Humidity Sensor	Control Company	11-661-9	12/2014	12/2017



COMOSAR E-Field Probe Calibration Report

Ref: ACR.351.8.16.SATU.A

WORLD STANDARDIZATION CERTIFICATION & TESTING CO .,LTD

BLOCK A, BAO SHI SCIENCE PARK,BAO SHI ROAD, BAO'AN DISTRICT SHENZHEN 518108,P.R. CHINA

MVG COMOSAR DOSIMETRIC E-FIELD PROBE

SERIAL NO.: SN 08/16 EPGO292

Calibrated at MVG US 2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 12/09/2016

Summary:

This document presents the method and results from an accredited COMOSAR Dosimetric E-Field Probe calibration performed in MVG USA using the CALISAR / CALIBAIR test bench, for use with a COMOSAR system only. All calibration results are traceable to national metrology institutions.



	Name	Function	Date	Signature
Prepared by :	Jérôme LUC	Product Manager	12/16/2016	Jez
Checked by:	Jérôme LUC	Product Manager	12/16/2016	JES
Approved by:	Kim RUTKOWSKI	Quality Manager	12/16/2016	thim Puthowshi

	Customer Name
Distribution:	World Standardization Certification & Testing Co .,Ltd

Issue	Date	Modifications
A	12/16/2016	Initial release



TABLE OF CONTENTS

1	Devi	Device Under Test4			
2	Prod	uct Description4			
	2.1	General Information	4		
3	Meas	surement Method4			
	3.1	Linearity	4		
	3.2	Sensitivity	5		
	3.3	Lower Detection Limit	5		
	3.4	Isotropy	5		
	3.5	Boundary Effect	5		
4	Meas	surement Uncertainty5			
5	Calib	oration Measurement Results6			
	5.1	Sensitivity in air	6		
	5.2	Linearity	7		
	5.3	Sensitivity in liquid	7		
	5.4	Isotropy			
6	List	of Equipment9			



1 DEVICE UNDER TEST

Device Under Test		
Device Type	COMOSAR DOSIMETRIC E FIELD PROBE	
Manufacturer	MVG	
Model	SSE2	
Serial Number	SN 08/16 EPGO292	
Product Condition (new / used)	New	
Frequency Range of Probe	0.7 GHz-6GHz	
Resistance of Three Dipoles at Connector	Dipole 1: R1=0.194 MΩ	
	Dipole 2: R2=0.198 MΩ	
	Dipole 3: R3=0.192 MΩ	

A yearly calibration interval is recommended.

2 PRODUCT DESCRIPTION

2.1 GENERAL INFORMATION

MVG's COMOSAR E field Probes are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards.



Figure 1 – MVG COMOSAR Dosimetric E field Dipole

Probe Length	330 mm
Length of Individual Dipoles	2 mm
Maximum external diameter	8 mm
Probe Tip External Diameter	2.5 mm
Distance between dipoles / probe extremity	1 mm

3 MEASUREMENT METHOD

The IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards provide recommended practices for the probe calibrations, including the performance characteristics of interest and methods by which to assess their affect. All calibrations / measurements performed meet the fore mentioned standards.

3.1 LINEARITY

The evaluation of the linearity was done in free space using the waveguide, performing a power sweep to cover the SAR range 0.01W/kg to 100W/kg.



3.2 SENSITIVITY

The sensitivity factors of the three dipoles were determined using a two step calibration method (air and tissue simulating liquid) using waveguides as outlined in the standards.

3.3 LOWER DETECTION LIMIT

The lower detection limit was assessed using the same measurement set up as used for the linearity measurement. The required lower detection limit is 10 mW/kg.

3.4 ISOTROPY

The axial isotropy was evaluated by exposing the probe to a reference wave from a standard dipole with the dipole mounted under the flat phantom in the test configuration suggested for system validations and checks. The probe was rotated along its main axis from 0 - 360 degrees in 15 degree steps. The hemispherical isotropy is determined by inserting the probe in a thin plastic box filled with tissue-equivalent liquid, with the plastic box illuminated with the fields from a half wave dipole. The dipole is rotated about its axis $(0^{\circ}-180^{\circ})$ in 15° increments. At each step the probe is rotated about its axis $(0^{\circ}-360^{\circ})$.

3.5 BOUNDARY EFFECT

The boundary effect is defined as the deviation between the SAR measured data and the expected exponential decay in the liquid when the probe is oriented normal to the interface. To evaluate this effect, the liquid filled flat phantom is exposed to fields from either a reference dipole or waveguide. With the probe normal to the phantom surface, the peak spatial average SAR is measured and compared to the analytical value at the surface.

4 MEASUREMENT UNCERTAINTY

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty associated with an E-field probe calibration using the waveguide technique. All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

Uncertainty analysis of the probe calibration in waveguide					
ERROR SOURCES	Uncertainty value (%)	Probability Distribution	Divisor	ci	Standard Uncertainty (%)
Incident or forward power	3.00%	Rectangular	$\sqrt{3}$	1	1.732%
Reflected power	3.00%	Rectangular	$\sqrt{3}$	1	1.732%
Liquid conductivity	5.00%	Rectangular	$\sqrt{3}$	1	2.887%
Liquid permittivity	4.00%	Rectangular	$\sqrt{3}$	1	2.309%
Field homogeneity	3.00%	Rectangular	$\sqrt{3}$	1	1.732%
Field probe positioning	5.00%	Rectangular	$\sqrt{3}$	1	2.887%



Field probe linearity	3.00%	Rectangular	$\sqrt{3}$	1	1.732%
Combined standard uncertainty					5.831%
Expanded uncertainty 95 % confidence level k = 2					12.0%

5 CALIBRATION MEASUREMENT RESULTS

Calibration Parameters			
Liquid Temperature	21 °C		
Lab Temperature	21 °C		
Lab Humidity	45 %		


5.1 <u>SENSITIVITY IN AIR</u>

Normx dipole		
$1 (\mu V/(V/m)^2)$	$2 (\mu V/(V/m)^2)$	$3 (\mu V/(V/m)^2)$
0.76	0.63	0.72

DCP dipole 1	DCP dipole 2	DCP dipole 3
(mV)	(mV)	(mV)
91	94	97

Calibration curves ei=f(V) (i=1,2,3) allow to obtain H-field value using the formula:

$$E = \sqrt{E_1^2 + E_2^2 + E_3^2}$$

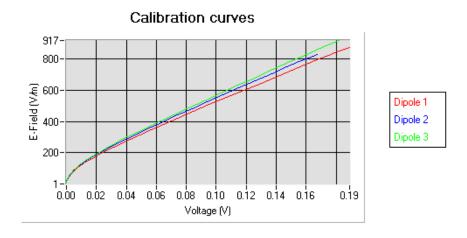


Page: 6/9

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



5.2 **LINEARITY**

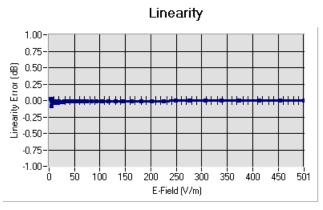

Linearity: I+/-1.83% (+/-0.08dB)

5.3 <u>SENSITIVITY IN LIQUID</u>

<u>Liquid</u>	Frequency	<u>Permittivity</u>	Epsilon (S/m)	<u>ConvF</u>
	MHz +/-			
	<u>100MHz)</u>			
HL5200	5200	35.64	4.67	1.91
BL5200	5200	48.64	5.51	1.97
HL5300	5300	35.98	4.74	1.96
BL5300	5300	47.55	5.62	2.02
HL5600	5600	36.66	5.17	2.00
BL5600	5600	46.79	5.77	2.05
HL5800	5800	35.31	5.31	1.86
BL5800	5800	47.04	6.10	1.91


LOWER DETECTION LIMIT: 8mW/kg



5.4 <u>ISOTROPY</u>

<u>HL5600 MHz</u>

- Axial isotropy: 0.06 dB - Hemispherical isotropy: 0.10 dB





6 LIST OF EQUIPMENT

Equipment Summary Sheet						
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date		
Flat Phantom	MVG	SN-20/09-SAM71	Validated. No cal required.	Validated. No cal required.		
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.		
Network Analyzer	Rhode & Schwarz ZVA	SN100132	02/2016	02/2019		
Reference Probe	MVG	EP 94 SN 37/08	10/2016	10/2017		
Multimeter	Keithley 2000	1188656	12/2013	12/2016		
Signal Generator	Agilent E4438C	MY49070581	12/2013	12/2016		
Amplifier	Aethercomm	SN 046	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.		
Power Meter	HP E4418A	US38261498	12/2013	12/2016		
Power Sensor	HP ECP-E26A	US37181460	12/2013	12/2016		
Directional Coupler	Narda 4216-20	01386	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.		
Waveguide	Mega Industries	069Y7-158-13-712		Validated. No cal required.		
Waveguide Transition	Mega Industries	069Y7-158-13-701	Validated. No cal required.	Validated. No cal required.		
Waveguide Termination	Mega Industries	069Y7-158-13-701	Validated. No cal required.	Validated. No cal required.		
Temperature / Humidity Sensor	Control Company	150798832	10/2015	10/2017		