FCCID: 2ABCS-A6102

Date of Issue : January 8, 2014

ANSI/IEEE Std. C95.1-1992 In accordance with the requirements of FCC Report and Order: ET Docket 93-62; FCC 47 CFR Part 2 (2.1093)

FCC SAR TEST REPORT

For

Product Name: 3D PAD Brand Name: TRULY Model No.: A6102

Series Model: A6100, N103D **Test Report Number:** C131230S02-SF

Issued for

Truly Industrial (ShanWei) Ltd Truly Industrial Area, Shanwei City, Guangdong Province, People's Republic of China

Issued by

Compliance Certification Services Inc.

Kun shan Laboratory

No.10 Weiye Rd., Innovation park, Eco&Tec, Development Zone, Kunshan City, Jiangsu, China

> TEL: 86-512-57355888 FAX: 86-512-57370818



Note: This report shall not be reproduced except in full, without the written approval of Compliance Certification Services Inc. This document may be altered or revised by Compliance Certification Services Inc. personnel only, and shall be noted in the revision section of the document. The client should not use it to claim product endorsement by A2LA or any government agencies. The test results in the report only apply to the tested sample.

Revision History

Revision	REPORT NO.	Date	Page Revised	Contents
Original	C130922R01-SF	November 22, 2013	N/A	N/A
Update	C131230S02-SF	December 31, 2013	All report	Add 802.11 a mode test data and related information
1	C131230S02-SF	January 8, 2014	All report	Add GPRS850 Edge1 test data and Plots of Performance Check
1	C131230S02-SF	January 8, 2014	7	Add simulating liquid For 5G

TABLE OF CONTENTS

1.	CERTIFICATE OF COMPLIANCE (SAR EVALUATION)	4
2.	EUT DESCRIPTION	5
3.	REQUIREMENTS FOR COMPLIANCE TESTING DEFINED BY THE FCC	6
4.	TEST METHODOLOGY	6
5.	DOSIMETRIC ASSESSMENT SETUP	
	5.1 MEASUREMENT SYSTEM DIAGRAM	8
	5.2 SYSTEM COMPONENTS	9
6.	EVALUATION PROCEDURES	12
7.	MEASUREMENT UNCERTAINTY	16
8.	EXPOSURE LIMIT	17
9.	EUT ARRANGEMENT	18
10.	MEASUREMENT RESULTS	19
	10.1 TEST LIQUIDS CONFIRMATION	19
	10.2 LIQUID MEASUREMENT RESULTS	20
	10.3 PROBE CALIBRATION PROCEDURE	21
	10.4 SYSTEM PERFORMANCE CHECK	26
	10.5 EUT TUNE-UP PROCEDURES AND TEST MODE	28
	10.6 SAR TEST CONFIGURATIONS	
	10.7 BODY TEST EXCLUSION THRESHOLDS	
	10.8 EUT SETUP PHOTOS	
	10.9 SAR MEASUREMENT RESULTS	
	10.10 REPEATED SAR MEASUREMENT	
	10.11 SAR HANDSETS MULTI XMITER ASSESSMENT	
	EUT PHOTO	
12.		
13.	FACILITIES	48
14.	REFERENCES	48
15.	ATTACHMENTS	49
App	pendix A: Plots of Performance Check	50
App	pendix B: DASY Calibration Certificate	56
Δnr	pendix C: Plots of SAR Test Result	114

1. CERTIFICATE OF COMPLIANCE (SAR EVALUATION)

		-				
Product Name:	3D PAD	3D PAD				
Brand Name:	TRULY					
Model Name.:	A6102	A6102				
Series Model:	A6100 · N103D					
Devices supporting GPRS:	Class B					
Description Test Modes(worst case):	SIM Card					
Device Category:	PORTABLE DEVICES					
Exposure Category:	GENERAL POPULATION/UNCONTROLLED EXPOSURE					
Date of Test:	November 10, 2013 to January 8, 2014					
Applicant:	Truly Industrial (ShanWei Truly Industrial Area,Shan of China) Ltd wei City,Guangdong Province,People's Republic				
Manufacturer:	Truly Industrial (ShanWei Truly Industrial Area,Shan of China) Ltd wei City,Guangdong Province,People's Republic				
Application Type:	Certification					
AF	PLICABLE STANDARDS A	ND TEST PROCEDURES				
STANDARDS AND TEST PROCEDURES TEST RESULT						
KDB	KDB 865664 No non-compliance noted					
Deviation from Applicable Standard						
None						

The device was tested by Compliance Certification Services Inc. in accordance with the measurement methods and procedures specified in KDB 865664 The test results in this report apply only to the tested sample of the stated device/equipment. Other similar device/equipment will not necessarily produce the same results due to production tolerance and measurement uncertainties.

Approved by:

Jeff fang

Tested by:

Jeff Fang RF Manager

Compliance Certification Services Inc.

Luck.Fu Test Engineer

Compliance Certification Services Inc.

nek Fu

2. EUT DESCRIPTION

Product Name:	3D PAD					
Brand Name:	TRULY	TRULY				
Model Name.:	A6102					
Series Model:	A6100 [,] N103D					
Model Discrepancy:	The motherboard is the same ,only diff	ferent models .				
FCC ID:	2ABCS-A6102					
Power reduction:	NO					
DTM Description:	N/A					
Device Category:	Production unit					
Frequency Range:	GPRS850: 850: 824.2 ~ 848.8 MHz GPRS1900: 1850.2 ~ 1909.8 MHz WCDMA Band II: 1852.4~1907.6MHz WCDMA Band V: 826.4~846.6 MHz 802.11 a:5745 MHz ~5825 MHz 802.11b/g: 2412 ~ 2462 MHz 802.11n HT20: 2412 ~ 2462 MHz 802.11n HT40: 2422 ~ 2452 MHz Bluetooth: 2402 ~ 2480 MHz					
Transmit Power (Average Max)::	GPRS 850:33 dBm EDGE 850:33 dBm GPRS 1900:30 dBm EDGE 1900:30 dBm WCDMA Band II: 21.5 dBm Band II HSDPA:21.5 dBm Band II HSUPA:21 dBm WCDMA Band V:23 dBm	IEEE 802.11a:15 dBm IEEE 802.11b:13.5 dBm IEEE 802.11g:11.5 dBm IEEE 802.11n HT20:11.5 dBm IEEE 802.11n HT40:10.5 dBm Bluetooth:3 dBm Band V HSDPA:23 dBm Band V HSUPA:22 dBm				
Max.SAR(Scaled 1-g):	Body: GPRS 850: 0.792 W/kg GPRS 1900: 0.858 W/kg : WCDMA BandII: 0.753 W/kg WCDMA BandII: 0.746 W/kg IEEE 802.11a:0.743 W/kg					
Modulation Technique:	IEEE 802.11b: 0.169 W/kg GPRS: GMSK WCDMA: QPSK EDGE: GMSK,8PSK IEEE 802.11a: OFDM IEEE 802.11b: DSSS (CCK, DQPSK, DBPSK) IEEE 802.11g/n: OFDM (BPSK, 16-QAM, 64-QAM) Bluetooth: GFSK + π/4DQPSK+8DPSK LE4.0: GFSK					
Accessories:	Power supply and ADP (rating): Model Name: KSA20A0500250D5 Battery (rating): Capacitance: 7000mAb					
Antenna Specification:	GSM: PIFA antenna WCDMA: PIFA antenna Bluetooth : PIFA antenna					
Operating Mode:	Maximum continuous output					
	I.					

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

3. REQUIREMENTS FOR COMPLIANCE TESTING DEFINED BY THE FCC

The US Federal Communications Commission has released the report and order "Guidelines for Evaluating the Environmental Effects of RF Radiation", ET Docket No. 93-62 in August 1996. The order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 1.6 mW/g for an uncontrolled environment and 8.0 mW/g for an occupational/controlled environment as recommended by the ANSI/IEEE standard C95.1-1992.

4. TEST METHODOLOGY

The Specific Absorption Rate (SAR) testing specification, method and procedure for this device is in accordance with the following standards:

□ ANSI/IEEE C95.1-1992

KDB 648474 D04 v01 Handset SAR

☑ KDB 865664 D01 v01r02 SAR Measurement 100 MHz to 6 GHz

X KDB 941225 D06 v01r01 Hotspot Mode SAR

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

5. DOSIMETRIC ASSESSMENT SETUP

These measurements were performed with the automated near-field scanning system DASY 5 from ATTENNESSA. The system is based on a high precision robot (working range greater than 0.9 m), which positions the probes with a positional repeatability of better than ± 0.02 mm. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines to the data acquisition unit. The SAR measurements were conducted with the E-field PROBE EX3DV4 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe has been calibrated according to the procedure described in [7] with accuracy of better than ±10%. The spherical isotropy was evaluated with the procedure described in [8] and found to be better than ±0.25 dB. The phantom used was the SAM Twin Phantom as described in FCC supplement C, IEE P1528 and CENELEC EN 62209.

Ingredients	Frequency (MHz)									
(% by weight)	450		835		915		1900		2450	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5
Conductivity (S/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78


Simulating Liquids for 5 GHz, Manufactured by SPEAG

Ingredients	(% by weight)
Water	78
Mineral oil	11
Emulsifiers	9
Additives and Salt	2

FCCID: 2ABCS-A6102

Date of Issue : January 8, 2014

5.1 MEASUREMENT SYSTEM DIAGRAM

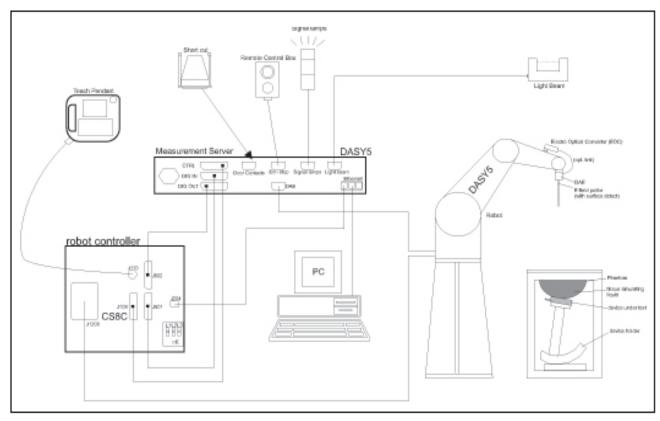

The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (St"aubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal
 multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision
 detection, etc. The unit is battery powered with standard or rechargeable batteries. The
 signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion between optical and electrical
 of the signals for the digital communication to the DAE and for the analog signal from the
 optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 7.
- DASY5 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing validating the proper functioning of the system.

5.2 SYSTEM COMPONENTS



The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz intel ULV celeron, 128MB chip-disk and 128 MB RAM. The necessary circuits for communication with either the DAE4(or DAE3) electronic box as well as the 16-bit AD-converter system for optical detection and digital I/O interface are contained on the DASY5 I/O-board, which is directly connected to the PC/104 bus of the CPU board.

The measurement server performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation.



The PC-operating system cannot interfere with these time critical processes. All connections are supervised by a watchdog, and disconnection of any of the cables to the measurement server will automatically disarm the robot and disable all program-controlled robot movements. Furthermore, the measurement server is equipped with two expansion slots which are reserved for future applications. Please note that the expansion slots do not have a standardized pinout and therefore only the expansion cards provided by SPEAG can be inserted. Expansion cards from any other supplier could seriously damage the measurement server. Calibration: No calibration required.

Data Acquisition Electronics (DAE)



The data acquisition electronics (DAE4) consists of a highly sensitive electrometer grade preamplifier with auto-zeroing, a channel and gainswitching multiplexer, a fast 16 bit AD converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock. The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection. The input impedance of the DAE4 box is 200MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.

EX3DV4 Isotropic E-Field Probe for Dosimetric Measurements



Construction: Symmetrical design with triangular core

Built-in shielding against static charges

PEEK enclosure material (resistant to organic solvents,

e.g., DGBE)

Calibration: Basic Broad Band Calibration in air: 10-3000 MHz.

Conversion Factors (CF) for HSL 900 and HSL 1800 CF-Calibration for other liquids and frequencies upon

request.

Frequency: 10 MHz to > 6 GHz; Linearity: ± 0.2 dB (30 MHz to 3

GHz)

Directivity: ± 0.3 dB in HSL (rotation around probe axis)

± 0.5 dB in HSL (rotation normal to probe axis)

Dynamic Range: 10 μW/g to > 100 mW/g; Linearity: ± 0.2 dB

(noise: typically $< 1 \mu W/g$)



Report No. C131230S02-SF FCCID: 2ABCS-A6102 Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Dimensions: Overall length: 337 mm (Tip: 9 mm)

Tip diameter: 2.5 mm (Body: 10 mm)
Distance from probe tip to dipole centers:

1 mm

Application: High precision dosimetric measurements

in any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6

GHz with precision of better 30%.




Interior of probe

SAM Twin Phantom

Construction:

The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (SAM) phantom defined in IEEE 1528-200X, CENELEC 50360 and IEC 62209. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points with the robot.



Dimensions: Height: 850mm; Length: 1000mm; Width:

750mm

SAM Phantom (ELI4 v4.0)

Description Construction:

Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI4 is fully compatible with the latest draft of the standard IEC 62209 Part II and all known tissue simulating liquids. ELI4 has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is supported by software version DASY4/DASY5.5 and higher and is compatible with all SPEAG dosimetric probes and dipoles

Shell Thickness: $2.0 \pm 0.2 \text{ mm (sagging: } <1\%)$

Filling Volume: Approx. 25 liters

Dimensions: Major ellipse axis: 600 mm

Minor axis: 400 mm 500mm





Report No: C131230S02-SF FCCID: 2ABCS-A6102 Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Device Holder for SAM Twin Phantom

Construction: In combination with the Twin SAM Phantom, the

Mounting Device (made from POM) enables the rotation of the mounted transmitter in spherical coordinates, whereby the rotation point is the ear opening. The devices can be easily and accurately positioned according to IEC, IEEE, CENELEC, FCC or other specifications. The device holder can be locked at different phantom locations (left head, right head, and flat phantom).



System Validation Kits for SAM Twin Phantom

Construction: Symmetrical dipole with I/4 balun Enables

measurement of feedpoint impedance with NWA Matched for use near flat phantoms filled with brain simulating solutions Includes distance

holder and tripod adaptor.

Frequency: 900,1800,2450,5800 MHz

Return loss: > 20 dB at specified validation position **Power capability:** > 100 W (f < 1GHz); > 40 W (f > 1GHz)

Dimensions:

D835V2: dipole length: 161 mm; overall height: 340 mm D1800V2: dipole length: 72.5 mm; overall height: 300 mm D1900V2: dipole length: 67.7 mm; overall height: 300 mm D2450V2: dipole length: 51.5 mm; overall height: 290 mm D5GHzV2: dipole length: 20.6 mm; overall height: 300mm



System Validation Kits for ELI4 phantom

Construction: Symmetrical dipole with I/4 balun Enables

measurement of feedpoint impedance with NWA Matched for use near flat phantoms filled with brain simulating solutions Includes distance

holder and tripod adaptor.

Frequency: 900, 1800, 2450, 5800 MHz

Return loss: > 20 dB at specified validation position **Power capability:** > 100 W (f < 1GHz); > 40 W (f > 1GHz)

Dimensions:

D835V2: dipole length: 161 mm; overall height: 340 mm D1800V2: dipole length: 72.5 mm; overall height: 300 mm D1900V2: dipole length: 67.7 mm; overall height: 300 mm D2450V2: dipole length: 51.5 mm; overall height: 290 mm D5GHzV2: dipole length: 20.6 mm; overall height: 300 mm



Report No. C131230S02-SF FCCID: 2ABCS-A6102 Date of Issue :January 8,

Reference No.: C130922R01-SI

6. EVALUATION PROCEDURES

DATA EVALUATION

The DASY 5 post processing software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters: - Sensitivity Norm_i, a_{i0} , a_{i1} , a_{i2}

- Conversion factor ConvF_i

- Diode compression point dcpi

Device parameters: - Frequency f

- Crest factor cf

Media parameters: - Conductivity σ

- Density ho

These parameters must be set correctly in the software. They can be found in the component documents or be imported into the software from the configuration files issued for the DASY 5 components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with V_i = Compensated signal of channel i(i = x, y, z)

 U_i = Input signal of channel i (i = x, y, z)

cf = Crest factor of exciting field (DASY 5 parameter)

 dcp_i = Diode compression point (DASY 5 parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:

$$E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

H-field probes: $H_i = \sqrt{Vi} \cdot \frac{a_{i10} + a_{i11}f + a_{i12}f^2}{f}$

with V_i = Compensated signal of channel i(i = x, y, z)

 $Norm_i$ = Sensor sensitivity of channel i (i = x, y, z)

 $\mu V/(V/m)^2$ for E0field Probes

ConvF = Sensitivity enhancement in solution

aij = Sensor sensitivity factors for H-field probes

f = Carrier frequency (GHz)

Ei = Electric field strength of channel i in V/m

Hi = Magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with SAR = local specific absorption rate in mW/g

 E_{tot} = total field strength in V/m

 σ = conductivity in [mho/m] or [Siemens/m]

 ρ = equivalent tissue density in g/cm³

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid.

The power flow density is calculated assuming the excitation field as a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

with P_{pwe} = Equivalent power density of a plane wave in mW/cm²

 E_{tot} = total electric field strength in V/m

 H_{tot} = total magnetic field strength in A/m

SAR EVALUATION PROCEDURES

The procedure for assessing the peak spatial-average SAR value consists of the following steps:

Power Reference Measurement

The reference and drift jobs are useful jobs for monitoring the power drift of the device under test in the batch process. Both jobs measure the field at a specified reference position, at a selectable distance from the phantom surface. The reference position can be either the selected section's grid reference point or a user point in this section. The reference job projects the selected point onto the phantom surface, orients the probe perpendicularly to the surface, and approaches the surface using the selected detection method.

Area Scan

The area scan is used as a fast scan in two dimensions to find the area of high field values, before doing a finer measurement around the hot spot. The sophisticated interpolation routines implemented in DASY 5 software can find the maximum locations even in relatively coarse grids. The scan area is defined by an editable grid. This grid is anchored at the grid reference point of the selected section in the phantom. When the area scan's property sheet is brought-up, grid was at to 15 mm by 15 mm and can be edited by a user.

Zoom Scan

Zoom scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default zoom scan measures 5 x 5 x 7 points within a cube whose base faces are centered around the maximum found in a preceding area scan job within the same procedure. If the preceding Area Scan job indicates more then one maximum, the number of Zoom Scans has to be enlarged accordingly (The default number inserted is 1).

Power Drift measurement

The drift job measures the field at the same location as the most recent reference job within the same procedure, and with the same settings. The drift measurement gives the field difference in dB from the reading conducted within the last reference measurement. Several drift measurements are possible for one reference measurement. This allows a user to monitor the power drift of the device under test within a batch process. In the properties of the Drift job, the user can specify a limit for the drift and have DASY 5 software stop the measurements if this limit is exceeded.

The Z Scan job measures points along a vertical straight line. The line runs along the Z-axis of a one-dimensional grid. A user can anchor the grid to the current probe location. As with any other grids, the local Z-axis of the anchor location establishes the Z-axis of the grid.

SPATIAL PEAK SAR EVALUATION

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1529 standard. It can be conducted for 1 g and 10 g.

The DASY 5 system allows evaluations that combine measured data and robot positions, such as:

- · maximum search
- extrapolation
- · boundary correction
- · peak search for averaged SAR

During a maximum search, global and local maximum searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

Extrapolation

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation.

Extrapolation routines require at least 10 measurement points in 3-D space. They are used in the Cube Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation. For a grid using 5x5x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1 g and 10 g cubes.

Boundary effect

For measurements in the immediate vicinity of a phantom surface, the field coupling effects between the probe and the boundary influence the probe characteristics. Boundary effect errors of different dosimetric probe types have been analyzed by measurements and using a numerical probe model. As expected, both methods showed an enhanced sensitivity in the immediate vicinity of the boundary. The effect strongly depends on the probe dimensions and disappears with increasing distance from the boundary. The sensitivity can be approximately given as:

$$S \approx S_o + S_b exp(-\frac{z}{a})cos(\pi \frac{z}{\lambda})$$

Since the decay of the boundary effect dominates for small probes (a $<<\lambda$), the cos-term can be omitted. Factors Sb (parameter Alpha in the DASY 5 software) and a (parameter Delta in the DASY 5 software) are assessed during probe calibration and used for numerical compensation of the boundary effect. Several simulations and measurements have confirmed that the compensation is valid for different field and boundary configurations.

This simple compensation procedure can largely reduce the probe uncertainty near boundaries. It works well as long as:

- the boundary curvature is small
- the probe axis is angled less than 30 to the boundary normal
- the distance between probe and boundary is larger than 25% of the probe diameter
- the probe is symmetric (all sensors have the same offset from the probe tip)

Since all of these requirements are fulfilled in a DASY 5 system, the correction of the probe boundary effect in the vicinity of the phantom surface is performed in a fully automated manner via the measurement data extraction during post processing.

7. MEASUREMENT UNCERTAINTY

UNCERTAIN	ITY BUDGE	ACCORDING	G TO IEE	EE 152	28-2003	
Error Description	Uncertainty Value ±%	Probability distribution	Divisor	C₁ 1g	Standard unc.(1g) ±%	V ₁ or V _{eff}
Measurement System						
Probe calibration	±5.5	normal	1	1	±5.5	∞
Axial isotropy of probe	±4.7	rectangular	√3	0.7	±1.9	∞
Hemispherical Isotropy of probe	±9.6	rectangular	√3	0.7	±3.9	∞
Probe linearity	±4.7	rectangular	√3	1	±2.7	∞
Detection Limit	±1.0	rectangular	√3	1	±0.6	∞
Boundary effects	±1.0	rectangular	√3	1	±0.6	∞
Readout electronics	±0.3	normal	1	1	±0.3	∞
Response time	±0.8	rectangular	√3	1	±0.5	∞
Integration time	±2.6	rectangular	√3	1	±1.5	∞
Probe positioning	±2.9	rectangular	√3	1	±1.7	∞
Probe positioner	±0.4	rectangular	√3	1	±0.2	∞
RF ambient Noise	±3.0	rectangular	√3	1	±1.7	∞
RF ambient Reflections	±3.0	rectangular	√3	1	±1.7	∞
Max.SAR Eval	±1.0	rectangular	√3	1	±0.6	∞
Test Sample Related						
Device positioning	±2.9	normal	1	1	±2.9	145
Device holder uncertainty	±3.6	normal	1	1	±3.6	5
Power drift	±5.0	rectangular	√3	1	±2.9	∞
Phantom and Set up						
Phantom uncertainty	±4.0	rectangular	√3	1	±2.3	∞
Liquid conductivity(target)	±5.0	rectangular	√3	0.64	±1.8	∞
Liquid conductivity(meas.)	±2.5	rectangular	1	0.64	±1.6	∞
Liquid permittivity(target)	±5.0	rectangular	√3	0.6	±1.7	∞
Liquid permittivity(meas.)	±2.5	rectangular	1	0.6	±1.5	∞
Combined Standard Uncertainty					±10.7	387
Coverage Factor for 95%		kp=2				
Expanded Standard Uncertainty					±21.4	

Table: Worst-case uncertainty for DASY5 assessed according to IEEE1528-2003.

The budge is valid for the frequency range 300 MHz to 6G Hz and represents a worst-case analysis.

8. EXPOSURE LIMIT

(A). Limits for Occupational/Controlled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and Ankles
0.4	8.0	20.0

(B). Limits for General Population/Uncontrolled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and Ankles
0.08	1.6	4.0

Note: Whole-Body SAR is averaged over the entire body, partial-body SAR is averaged over any 10 gram of tissue defined as a tissue volume in the shape of a cube. SAR for hands, wrists, feet and ankles is averaged over any 1 grams of tissue defined as a tissue volume in the shape of a cube.

Population/Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure.

Occupational/Controlled Environments are defined as locations where there is exposure that may be incurred by people who are aware of the potential for exposure, (i.e. as a result of employment or occupation).

> **NOTE** GENERAL POPULATION/UNCONTROLLED EXPOSURE **PARTIAL BODY LIMIT** 1.6 W/kg

9. EUT ARRANGEMENT

This EUT was tested in four different positions. They are reverse side of tablet, Edge 1; Edge 3 and Edge 4.In these positions, the surface of EUT is touching with phantom 0cm.

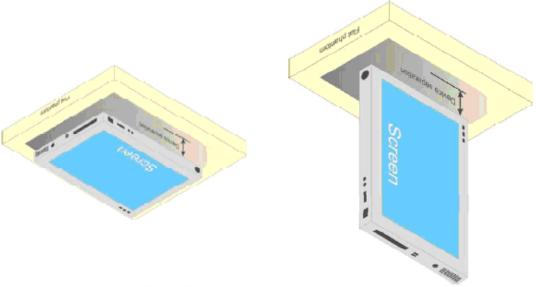


Fig Illustration for Lap-touching Position

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

10. MEASUREMENT RESULTS

10.1 TEST LIQUIDS CONFIRMATION

SIMULATED TISSUE LIQUID PARAMETER CONFIRMATION

The dielectric parameters were checked prior to assessment using the HP85070C dielectric probe kit. The dielectric parameters measured are reported in each correspondent section.

KDB865664 RECOMMENDED TISSUE DIELECTRIC PARAMETERS

The tissue dielectric parameters recommended by the KDB865664 have been incorporated in the following table.

Target Frequency	He	ad	Body		
(MHz)	ϵ_{r}	σ (S/m)	ε _r	σ (S/m)	
150	52.3	0.76	61.9	0.80	
300	45.3	0.87	58.2	0.92	
450	43.5	0.87	56.7	0.94	
835	41.5	0.90	55.2	0.97	
900	41.5	0.97	55.0	1.05	
915	41.5	0.98	55.0	1.06	
1450	40.5	1.20	54.0	1.30	
1610	40.3	1.29	53.8	1.40	
1800-2000	40.0	1.40	53.3	1.52	
2450	39.2	1.80	52.7	1.95	
3000	38.5	2.40	52.0	2.73	
5800	45.3	5.27	48.2	6.00	

(ε_r = relative permittivity, σ = conductivity and ρ = 1000 kg/m³)

10.2 LIQUID MEASUREMENT RESULTS

The following table show the measuring results for simulating liquid:

Liquid Type	Liquid Temp. (°C)	Parameters	Target	Measured	Deviation (%)	Limited (%)	Measured Date
Body835	21.5	Permitivity(ε)	55.20	54.329	-1.58	± 5	2013-11-10
Бойуозэ	21.5	Conductivity(σ)	0.97	0.97	0.00	± 5	2013-11-10
Body1900	21.5	Permitivity(ε)	53.30	53.263	-0.07	± 5	2013-11-11
B00y1900 21.5	Conductivity(σ)	1.52	1.537	1.12	± 5	2013-11-11	
Body2450	Body2450 21.5	Permitivity(ε)	52.70	51.332	-2.60	± 5	2013-11-13
B00y2430	21.5	Conductivity(σ)	1.95	2.012	3.18	± 5	2013-11-13
Body5800	21.4	Permitivity(ε)	48.2	46.98	-2.53	± 5	2013-12-26
Бойуэооо 21.4	Conductivity(σ)	6	6.17	2.83	± 5	2013-12-20	
Dody925	21.5	Permitivity(ε)	55.20	53.03	-3.93	± 5	2014-1-8
Body835	21.5	Conductivity(σ)	0.97	0.954	-1.65	± 5	2014-1-0

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

10.3 PROBE CALIBRATION PROCEDURE

For the calibration of E-field probes in lossy liquids, an electric field with an accurately known field strength must be produced within the measured liquid. For standardization purposes it would be desirable if all measurements which are necessary to assess the correct field strength would be traceable to standardized measurement procedures. In the following two different calibration techniques are summarized:

Transfer Calibration with Temperature Probes

In lossy liquids the specific absorption rate (SAR) is related both to the electric field (E) and the temperature gradient (dT/dt) in the liquid.

$$SAR = \frac{\sigma}{\rho}|E|^2 = c\frac{dT}{dt}$$

whereby σ is the conductivity, ρ the density and c the heat capacity of the liquid.

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Hence, the electric field in lossy liquid can be measured indirectly by measuring the temperature gradient in the liquid. Non-disturbing temperature probes (optical probes or thermistor probes with resistive lines) with high spatial resolution (<1-2 mm) and fast reaction time (<1 s) are available and can be easily calibrated with high precision [2]. The setup and the exciting source have no influence on the calibration; only the relative positioning uncertainties of the standard temperature probe and the E-field probe to be calibrated must be considered. However, several problems limit the available accuracy of probe calibrations with temperature probes:

- The temperature gradient is not directly measurable but must be evaluated from temperature measurements at different time steps. Special precaution is necessary to avoid measurement errors caused by temperature gradients due to energy equalizing effects or convection currents in the liquid. Such effects cannot be completely avoided, as the measured field itself destroys the thermal equilibrium in the liquid. With a careful setup these errors can be kept small.
- The measured volume around the temperature probe is not well defined. It is difficult to calculate the energy transfer from a surrounding gradient temperature field into the probe. These effects must be considered, since temperature probes are calibrated in liquid with homogeneous temperatures. There is no traceable standard for temperature rise measurements.
- The calibration depends on the assessment of the specific density, the heat capacity and the conductivity of the medium. While the specific density and heat capacity can be measured accurately with standardized procedures ($\sim 2\%$ for c; much better for ρ), there is no standard for the measurement of the conductivity. Depending on the method and liquid, the error can well exceed $\pm 5\%$.
- Temperature rise measurements are not very sensitive and therefore are often performed at a higher power level than the E-field measurements. The nonlinearities in the system (e.g., power measurements, different components, etc.) must be considered.

Considering these problems, the possible accuracy of the calibration of Efield probes with temperature gradient measurements in a carefully designed setup is about $\pm 10\%$ (RSS) [4]. Recently, a setup which is a combination of the waveguide techniques and the thermal measurements was presented in

[7]. The estimated uncertainty of the setup is $\pm 5\%$ (RSS) when the same liquid is used for the calibration and for actual measurements and $\pm 7.9\%$ (RSS) when not, which is in good agreement with the estimates given in [4].

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Calibration with Analytical Fields

In this method a technical setup is used in which the field can be calculated analytically from measurements of other physical magnitudes (e.g., input power). This corresponds to the standard field method for probe calibration in air; however, there is no standard defined for fields in lossy liquids.

When using calculated fields in lossy liquids for probe calibration, several points must be considered in the assessment of the uncertainty:

- The setup must enable accurate determination of the incident power.
- The accuracy of the calculated field strength will depend on the assessment of the dielectric parameters of the liquid.
- Due to the small wavelength in liquids with high permittivity, even small setups might be above the resonant cutoff frequencies. The field distribution in the setup must be carefully checked for conformity with the theoretical field distribution.

In the following section a setup which allows the analytical calculation of the SAR will be introduced.

New Waveguide Setup for Probe Calibration

Rectangular waveguides are self-contained systems. In the frequency band in which only the dominant TE₀₁ mode exists, highly accurate fields can be generated for calibration purposes if reflections can be minimized or compensated for. Considerable standing waves unavoidably occur if a lossy liquid is inserted in the waveguide. However, the cross sectional field distribution which is defined only by the geometry is not modified by these standing waves, a fact which can be utilized for generating well defined fields inside lossy liquid.

Three different standard waveguides (R9, R14 and R22) with overlapping frequency ranges were realized covering the frequency range of interest, i.e., from 800 up to 2500 MHz. In each waveguide, a planar, dielectric slab (ϵ_r = 3.3) was introduced to minimize reflections (return loss < -10 dB). The lossy tissue simulating liquid in which the probe had to be calibrated was

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

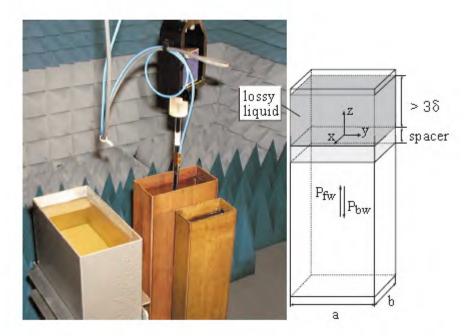


Figure 5.1: Experimental setup for assessment of the conversion factor when using a vertically rectangular waveguide.

The here presented waveguide system is a robust and easy-to-use setup enabling calibration of dosimetric E-field probes with high precision. Even more important is that the calibration of the setup can be reduced to power measurements which can be traced to a standard calibration procedure. The practical limitation given by the waveguide size to the frequency band between 800 and 2500 MHz is not severe in the context of compliance testing, since the most important operational frequencies of mobile communications systems are covered. The presented waveguide system is therefore well suited for implementation as a standard calibration technique for dosimetric probes in this frequency range. For frequencies below 800 MHz, transfer calibration with temperature probes remains the most practical way to achieve calibration with decent precision.

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

filled into the vertically standing waveguide. The medium depth had to be chosen such that the standing waves within the liquid were negligible, i.e., larger than three times the skin depth (<-50 dB at the interface liquid-slab). The attenuation of the waveguide adapters was determined to be 0.05 dB by the transmission method using two identical adapters. Table 5.1 gives an overview of some of the construction details.

	R9	R14	R22
WG cross section*	248×124	165×82.5	109×54.7
Spacer height*	50	30	25
Liquid height*	150	130	80

^{*} all dimensions in mm

Table 5.1: Description of the waveguide systems.

With these setups, the total power absorbed by the lossy liquid can be accurately determined by measurement of the forward and reflected powers. Since all power entering the lossy liquid is absorbed by the liquid, the volume SAR can be determined as:

$$SAR^{V} = \frac{4(P_{fw} - P_{bw})}{ab\delta} \cos^{2}(\pi \frac{y}{a}) e^{(-2z/\delta)}$$
 (5.2)

The here presented waveguide system is a robust and easy-to-use setup enabling calibration of dosimetric E-field probes with high precision. Even more important is that the calibration of the setup can be reduced to power measurements which can be traced to a standard calibration procedure. The practical limitation given by the waveguide size to the frequency band between 800 and 2500 MHz is not severe in the context of compliance testing, since the most important operational frequencies of mobile communications systems are covered. The presented waveguide system is therefore well suited for implementation as a standard calibration technique for dosimetric probes in this frequency range. For frequencies below 800 MHz, transfer calibration with temperature probes remains the most practical way to achieve calibration with decent precision.

FCCID: 2ABCS-A6102


Date of Issue :January 8, 2014

10.4 SYSTEM PERFORMANCE CHECK

The system performance check is performed prior to any usage of the system in order to guarantee reproducible results. The system performance check verifies that the system operates within its specifications of $\pm 10\%$. The system performance check results are tabulated below. And also the corresponding SAR plot is attached as well in the SAR plots files.

SYSTEM PERFORMANCE CHECK MEASUREMENT CONDITIONS

- The measurements were performed in the flat section of the SAM twin phantom filled with head and body simulating liquid of the following parameters.
- The DASY5 system withan E-fileld probe EX3DV4 SN: 3798 was used for the measurements.
- The dipole was mounted on the small tripod so that the dipole feed point was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15 mm (below 1 GHz) and 10 mm (above 1 GHz) from dipole center to the simulating liquid surface.
- The coarse grid with a grid spacing of 10mm was aligned with the dipole.
- Special 7x7x7 fine cube was chosen for cube integration (dx= 5 mm, dy= 5 mm, dz= 5 mm).
- Distance between probe sensors and phantom surface was set to 2 mm.
- The dipole input power was 1W±3%.
- The results are normalized to 1 W input power.





- Note: For SAR testing, less than 3G the liquid depth is 15cm shown above
- Note: For SAR testing, above than 3G the liquid depth is 10cm shown above

SYSTEM PERFORMANCE CHECK RESULTS

Liquid Type	Ambient Temp. (°C)	Liquid Temp. (°C)	Input Power (W)	Measured SAR1g (W/Kg)	1W Target SAR1g(W/Kg)	1W Normalized SAR1g(W/Kg)	Deviation (%)	Limited (%)	Date
Body835	22	21.5	0.25	2.32	9.53	9.28	-2.62	± 10	2013-11-10
Body1900	22	21.5	0.25	9.73	40.50	38.92	-3.90	± 10	2013-11-11
Body2450	22	21.5	0.25	12.90	49.20	51.60	4.88	± 10	2013-11-13
Body5800	22.7	21.4	0.1	7.21	75.00	72.1	-3.87	± 10	2013-12-26
Body835	22	21.5	0.25	2.41	9.53	9.64	1.15	± 10	2014-1-8

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

10.5 EUT TUNE-UP PROCEDURES AND TEST MODE

The following procedure had been used to prepare the EUT for the SAR test.

To setup the desire channel frequency and the maximum output power. A Radio Communication Tester "CMU200" was used to program the EUT.

GPRS 850/EDGE 850:

Network Support: GPRS/EDGE

Main Service: Circuit Switched/Packet data

Power Setting: 33dBm/33dBm

GPRS 1900/EDGE1900:

Network Support: GPRS/EDGE

Main Service: Circuit Switched/Packet data

Power Setting: 30dBm/30dBm Conducted output power(dBm):

Band		GSM 850			GSM 1900				
Channel	128	190	251	512	661	810			
Frequency(MHz)	824.2	836.6	848.8	1850.2	1880	1909.8			
Maximum Burst-Averaged Output Power									
GPRS 8 (1 Uplink)	32.23	32.29	32.35	29.52	29.64	29.78			
GPRS 10 (2 Uplink)	31.51	31.54	31.59	28.98	28.96	29.05			
GPRS 11 (3 Uplink)	29.81	29.85	29.89	27.23	27.24	27.30			
GPRS 12 (4 Uplink)	29.00	29.01	29.09	26.42	26.45	26.53			
EDGE 8 (1 Uplink)	32.21	32.28	32.34	29.47	29.59	29.72			
EDGE 10 (2 Uplink)	31.52	31.52	31.57	28.91	28.91	29.01			
EDGE 11 (3 Uplink)	29.83	29.81	29.85	27.17	27.21	27.25			
EDGE 12 (4 Uplink)	28.96	28.98	28.99	26.36	26.42	26.43			
Ма	ximum Fra	me-Averaç	ged Output	Power					
GPRS 8 (1 Uplink)	23.21	23.27	23.33	20.50	20.62	20.76			
GPRS 10 (2 Uplink)	25.49	25.52	25.57	22.96	22.94	23.03			
GPRS 11 (3 Uplink)	25.55	25.59	25.63	22.97	22.98	23.04			
GPRS 12 (4 Uplink)	25.99	26.00	26.08	23.41	23.44	23.52			
EDGE 8 (1 Uplink)	23.18	23.25	23.31	20.44	20.56	20.69			
EDGE 10 (2 Uplink)	25.50	25.50	25.55	22.89	22.89	22.99			
EDGE 11 (3 Uplink)	25.57	25.55	25.59	22.91	22.95	22.99			
EDGE 12 (4 Uplink)	25.95	25.97	25.98	23.35	23.41	23.42			

Remark: The frame-averaged power is linearly scaled the maximum burst-averaged power based on time slots. The calculated methods are shown as below:

Frame-averaged power = Burst-averaged power (1 Uplink) - 9.03 dBm Frame-averaged power = Burst averaged power (2 Uplink) - 6.02 dBm Frame-averaged power = Burst-averaged power (3 Uplink) - 4.26 dBm Frame-averaged power = Burst averaged power (4 Uplink) - 3.01 dBm

Note: Per KDB 447498 D01v05r01, the maximum output power channel is used for SAR testing and for further SAR test reduction.

3102

Date of Issue : January 8, 2014

WCDMA Conducted output power(dBm):

As the SAR body tests for WCDMA **BandII**, we established the radio link through call processing. The maximum output power were verified on high, middle and low channels for each test band according to 3GPP TS 34.121 with the following configuration:a 12.2kbps RMC, 64,144,384 kbps RMC with TPC set to all "all '1's" Test loop Mode 1

The following procedures had been used to prepare the EUT for the SAR test.

HSDPA Setup Configuration:

Table C.10.1.4: β values for transmitter characteristics tests with HS-DPCCH

Sub-test	βα	βd	β _d (SF)	β⊌βа	βнs (Note1, Note 2)	CM (dB) (Note 3)	MPR (dB) (Note 3)
1	2/15	15/15	64	2/15	4/15	0.0	0.0
2	12/15 (Note 4)	15/15 (Note 4)	64	12/15 (Note 4)	24/15	1.0	0.0
3	15/15	8/15	64	15/8	30/15	1.5	0.5
4	15/15	4/15	64	15/4	30/15	1.5	0.5

Note 1: Δ_{ACK} , Δ_{NACK} and $\Delta_{CQI} = 30/15$ with $\beta_{Im} = 30/15 * \beta_c$

Note 2: For the HS-DPCCH power mask requirement test in clause 5.2C, 5.7A, and the Error Vector Magnitude (EVM) with HS-DPCCH test in clause 5.13.1A, and HSDPA EVM with phase discontinuity in clause 5.13.1AA, Δ_{ACK} and Δ_{NACK} = 30/15 with β_{hs} = 30/15 * β_c , and Δ_{CQI} = 24/15

with B = 24/15 * B ...

Note 3: CM = 1 for β_o/β_d =12/15, β_{hb}/β_c=24/15. For all other combinations of DPDCH, DPCCH and HS-DPCCH the MPR is based on the relative CM difference. This is applicable for only UEs that support HSDPA in release 6 and later releases.

Note 4: For subtest 2 the β_c/β_d ratio of 12/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signalled gain factors for the reference TFC (TF1, TF1) to β_c = 11/15 and β_d = 15/15.

HSUPA Setup Configuration:

Table C.11.1.3: β values for transmitter characteristics tests with HS-DPCCH and E-DCH

- 1	ub- est	βε	βd	β _đ (SF)	βε/βα	βнs (Note f)	βec	βed (Note 5) (Note 6)	βed (SF)	β _{ed} (Codes)	CM (dB) (Note 2)	MPR (dB) (Note 2)	AG Index (Note 6)	E- TFCI
	1	11/15 (Note 3)	15/15 (/Vote 3)	64	11/15 (Note 3)	22/15	209/2 25	1309/225	4	1	1.0	0.0	20	75
	2	6/15	15/15	64	6/15	12/15	12/15	94/75	4	1	3.0	2.0	12	67
	3	15/15	9/15	64	15/9	30/15	30/15	β _{cd} 1: 47/15	4	2	2.0	1.0	15	92
								β _{cd} 2: 47/15	4					
	4	2/15	15/15	64	2/15	4/15	2/15	56/75	4	1	3.0	2.0	17	71
	5	15/15	15/15	64	15/15	30/15	24/15	134/15	4	1	1.0	0.0	21	81
		(Note 4)	(Note 4)		(Note 4)									

Note 1: Λ_{ACK} , Λ_{NACK} and Λ_{CQI} = 30/15 with β_{ks} = 30/15 * β_s .

Note 2: CM = 1 for β_c/β_d =12/15, β_{ns}/β_c =24/15. For all other combinations of DPDCH, DPCCH, HS- DPCCH, E-DPDCH and E-DPCCH the MPR is based on the relative CM difference.

Note 3: For subtest 1 the β_c/β_d ratio of 11/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signalled gain factors for the reference TFC (TF1, TF1) to β_c = 10/15 and β_d = 15/15.

Note 4: For subtest 5 the μ_c/μ_d ratio of 15/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signalled gain factors for the reference TFC (TF1, TF1) to β_d = 14/15 and β_d = 15/15.

Note 5: In case of testing by UE using E-DPDCH Physical Layer category 1, Sub-test 3 is omitted according to TS25.306 Table 5.1g.

Note 6: β_{cd} can not be set directly, it is set by Absolute Grant Value.

Band	W	WCDMA Band II			WCDMA Band V			
Channel	9262	9400	9538	4132	4182	4233		
Frequency(MHz)	1852.4	1880	1907.6	826.4	836.6	846.6		
RMC12.2K	21.38	21.24	21.12	22.80	22.41	22.67		
HSDPA Subtest-1	21.31	21.22	21.18	22.59	22.23	22.43		
HSDPA Subtest-2	21.30	21.17	21.14	22.61	22.21	22.41		
HSDPA Subtest-3	21.28	21.14	21.11	22.56	22.24	22.39		
HSDPA Subtest-4	21.21	21.09	21.02	22.53	22.21	22.40		
HSUPA Subtest-1	20.50	20.45	20.32	21.72	21.59	21.55		
HSUPA Subtest-2	19.46	19.21	19.12	20.54	20.04	20.44		
HSUPA Subtest-3	20.47	20.25	20.11	21.79	21.59	21.63		
HSUPA Subtest-4	19.52	19.28	19.21	20.28	20.16	20.26		
HSUPA Subtest-5	20.46	20.26	20.22	21.74	21.61	21.68		

Note:

Per KDB 941225 D01, RMC 12.2kbps setting is used to evaluate SAR. If HSDPA/HSUPA output power is < 0.25dB higher than RMC, HSDPA/HSUPA SAR evaluation can be excluded.

WLAN Conducted output power(dBm):

Mode	Channel	Frequence	Average power(dBm) Date Rate(bps) 6M
	149	5745 MHZ	14.05
	153	5765 MHZ	14.32
802.11 a	157	5785 MHZ	14.10
	161	5805 MHZ	14.37
	165	5825 MHZ	14.45

			Average power(dBm)
Mode	Channel	Frequence	Date Rate(bps)
			1M
	1	2412 MHZ	13.12
802.11 b	6	2437 MHZ	13.18
	11	2462 MHZ	13.15

			Average power(dBm)	
Mode	Channel	Frequence	Date Rate(bps)	
			6 M	
	1	2412 MHZ	11.18	
802.11 g	6	2437 MHZ	11.21	
	11	2462 MHZ	11.11	

			Average power(dBm)	
Mode	Channel	Frequence	Date Rate(bps)	
			6.5 M	
	1	2412 MHZ	9.87	
802.11 n HT20	6	2437 MHZ	9.92	
	11	2462 MHZ	9.82	

			Average power(dBm)	
Mode	Channel	Frequence	Date Rate(bps)	
			6.5 M	
	3	2422 MHZ	9.74	
802.11 n HT40	6	2437 MHZ	9.89	
	9	2452 MHZ	9.77	

Per KDB 248227, choose the highest output power channel to test SAR and determine further SAR exclusion

FCCID: 2ABCS-A6102 Date of Issue :January 8, 2014

2. Per KDB 248227, 11g, 11n-HT20 and 11n-HT40 output power is less than 0.25dB higher than 11b mode, the SAR test can be excluded.

Bluetooth Conducted output power(dBm)

Date Rate(Mbps)	Channel	Frequence	Average power(dBm)
	0	2402 MHZ	2.47
1	39	2441 MHZ	1.96
	78	2480 MHZ	2.41
	0	2402 MHZ	0.42
2	39	2441 MHZ	0.33
	78	2480 MHZ	0.35
	0	2402 MHZ	0.98
3	39	2441 MHZ	0.82
	78	2480 MHZ	0.89

BT LE4.0

Date Rate(Mbps)	Channel	Frequence	Average power(dBm)
	0	2402 MHZ	3.41
1	19	2440 MHZ	3.15
	39	2480 MHZ	3.22

According to KDB447498 D01:The 1-g and 10-g SAR test exclusion thresholds fsor 100 MHz to 6 GHz at *test separation distances* ≤ 50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance,

- mm)] $\cdot [\sqrt{f_{(GHz)}}] \le 3.0$ for 1-q SAR and ≤ 7.5 for 10-q extremity SAR,24 where
 - f(GHz) is the RF channel transmit frequency in GHz
 - Power and distance are rounded to the nearest mW and mm before calculation25
 - The result is rounded to one decimal place for comparison
 - 3.0 and 7.5 are referred to as the numeric thresholds in the step 2 below
 - If the test separation distance (antenna-user) is < 5mm, 5mm is used for excluded SAR calculation

	Wireless Interface	Bluetooth
Tune-up Maximum power (dBm)		4
Tune-up Maximum rated power (mW)		2.512
	Antenna to user (mm)	5
Body	Frequency(GHz)	2.402
	SAR exclusion threshold	3

Per KDB 447498 D01v05r01 exclusion thresholds is 0.778< 3, RF exposure evaluation is not required.

The Turn-up Maximum Power

Mode	The Turn-up Maximum Power(Customer Declared)(dBm)	Range	Measured Conduct Maximum Power(dBm)
GPRS 850-1TS	32+/-1	31-33	32.35
GPRS 850-2TS	31+/-1	30-32	31.59
GPRS 850-3TS	29+/-1	28-30	29.89
GPRS 850-4TS	28.5+/-1	27.5~29.5	29.09
EDGE 850-1TS	32+/-1	31~33	32.34
EDGE 850-2TS	31+/-1	30~32	31.57
EDGE 850-3TS	29+/-1	28~30	29.85
EDGE 850-4TS	28.5+/-1	27.5~29.5	28.99
GPRS 1900-1TS	29+/-1	28~30	29.78
GPRS 1900-2TS	28.5+/-1	27.5~29.5	29.05
GPRS 1900-3TS	27+/-1	26~28	27.30
GPRS 1900-4TS	26+/-1	25~27	26.53
EDGE 1900-1TS	29+/-1	28~30	29.72
EDGE 1900-2TS	28.5+/-1	27.5~29.5	29.01
EDGE 1900-3TS	27+/-1	26~28	27.25
EDGE 1900-4TS	26+/-1	25~27	26.43
WCDMA Band II	20.5+/-1	19.5~21.5	21.38
HSDPA Band II Sub-1	20.5+/-1	19.5~21.5	21.31
HSDPA Band II Sub-2	20.5+/-1	19.5~21.5	21.30
HSDPA Band II Sub-3	20.5+/-1	19.5~21.5	21.28
HSDPA Band II Sub-4	20.5+/-1	19.5~21.5	21.21
HSUPA Band II Sub-1	20+/-1	19~21	20.50
HSUPA Band II Sub-2	19+/-1	18~20	19.46
HSUPA Band II Sub-3	20+/-1	19~21	20.47
HSUPA Band II Sub-4	19+/-1	18~20	19.52
HSUPA Band II Sub-5	20+/-1	19~21	20.46
WCDMA Band V	22+/-1	21~23	22.80
HSDPA Band V Sub-1	22+/-1	21~23	22.59
HSDPA Band V Sub-2	22+/-1	21~23	22.61
HSDPA Band V Sub-3	22+/-1	21~23	22.56
HSDPA Band V Sub-4	22+/-1	21~23	22.53
HSUPA Band V Sub-1	21+/-1	20~22	21.72
HSUPA Band V Sub-2	20+/-1	19~21	20.54
HSUPA Band V Sub-3	21+/-1	20~22	21.79
HSUPA Band V Sub-4	19.5+/-1	18.5~20.5	20.28




Compliance Certification Services Inc. Report No: C131230S02-SF FCCID: 2ABCS-A6102 Date of Issue :Ja Reference No.: C130922R01-SF

Date of Issue :January 8, 2014

HSUPA Band V Sub-5	21+/-1	20~22	21.74
IEEE 802.11a	14+/-1	13~15	14.45
IEEE 802.11b	12.5+/-1	11.5~13.5	13.18
IEEE 802.11g	10.5+/-1	9.5~11.5	11.21
IEEE 802.11n(20M)	9.5+/-1	9.5~11.5	9.92
IEEE 802.11n(40M)	9.5+/-1	8.5~10.5	9.89
BT 1M	2+/-1	1~3	2.47
BT 2M	0+/-1	-1~1	0.42
BT 3M	0.5+/-1	-0.5~1.5	0.98
BT LE4.0	3+/-1	2~4	3.41

So, they are in tune-up range and complied.

10.6 SAR TEST CONFIGURATIONS

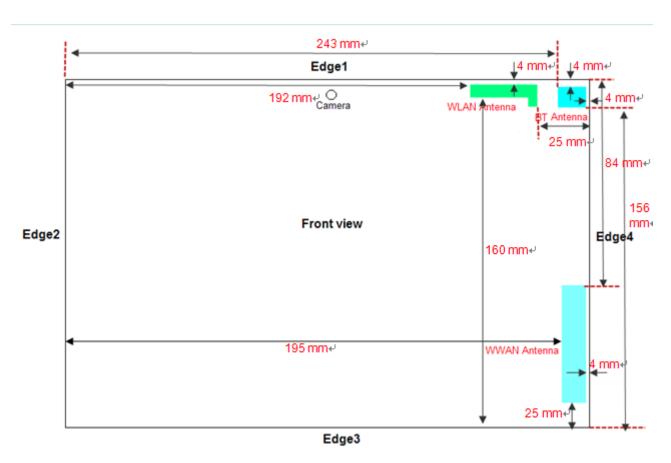

evice dimensions (H v W v D): 263 v 171 v 13 mm

Device dimensions (H X W X D): 263 X 171 X 13 mm			
Antennas	Wireless Interface		
WWAN antenna	GPRS850 GPRS1900 WCDMA Bnad II WCDMA Bnad V		
WLAN antenna	WLAN 2.4G;WLAN 5.8G		
Bluetooth antenna	Bluetooth		

Test Mode

1 COL INCAC				
GSM 850/PCS1900	Data transmission mode(GPRS)/Voice mode(GSM)			
WCDMA Band II/V	Data transmission mode(12.2kRMC)			
WLAN	Data transmission mode(IEEE 802.11 b) Data transmission mode(IEEE 802.11 5.8G)			

10.7 BODY TEST EXCLUSION THRESHOLDS

The following SAR test exclusion Thresholds based on KDB 447498 D01 General RF Exposure Guidance v05r01) 4.3.1)

		WWAN			WLAN	
Exposure	Wireless Interface	GPRS 850 Class 12	GPRS1900 Class12	WCDMA Band II	WCDMA Band V	802.11 b
Position	Maximum power	29.5	27	21.5	23	13.5
	Maximum rated power(mW)	891.25	501.19	141.25	199.53	22.39
_	Antenna to user (mm)	5			5	
Rear view	SAR exclusion threshold	16.27	10.88	10.88	16.27	9.58
	SAR testing required?	Yes	Yes	Yes	Yes	Yes
	Antenna to user (mm)	84			5	
Edge1	SAR exclusion threshold	356.67	539.67	539.67	356.67	9.58
	SAR testing required?	Yes	No	No	No	Yes
Antenna to user (mm)		195			192	
Edge2	SAR exclusion threshold	985.67	1945.67	1945.67	985.67	2415.33
	SAR testing required?	No	No	No	No	No
Antenna to user (mm)			25			160
Edge3	SAR exclusion threshold	81.35	54.41	54.41	81.35	1892.67
	SAR testing required?	Yes	Yes	Yes	Yes	No
	Antenna to user (mm)	5			25	
Edge4	SAR exclusion threshold	16.27	10.88	10.88	16.27	47.92
	SAR testing required?	Yes	Yes	Yes	Yes	No

-	Wireless Interface	WLAN 802.11 a
Exposure Position	Maximum power	15
	Maximum rated power(mW)	31.62
_	Antenna to user (mm)	5
Rear view	SAR exclusion threshold	6.23
	SAR testing required?	Yes
	Antenna to user (mm)	5
Edge1	SAR exclusion threshold	6.23
	SAR testing required?	Yes
	Antenna to user (mm)	192
Edge2	SAR exclusion threshold	1482.28
	SAR testing required?	No
Edge3	Antenna to user (mm)	160
	SAR exclusion threshold	1162.28
	SAR testing required?	No
	Antenna to user (mm)	25
Edge4	SAR exclusion threshold	31.14
	SAR testing required?	Yes

Note:

- 1. Maximum power is the source-based time-average power and represents the maximum RF output power among production units
- 2. Per KDB 447498 D01v05r01, for larger devices, the test separation distance of adjacent edge configuration is determined by the closest separation between the antenna and the user.
- 3. Per KDB 447498 D01v05r01, standalone SAR test exclusion threshold is applied; If the distance of the antenna to the user is < 5mm, 5mm is used to determine SAR exclusion threshold
- 4. Per KDB 447498 D01v05r01, the 1-g and 10-g SAR test exclusion thresholds for 100 MHz to 6 GHz at test separation distances ≤ 50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)] · [√f(GHz)] ≤ 3.0 for 1-g SAR and ≤ 7.5 for 10-g extremity SAR

f(GHz) is the RF channel transmit frequency in GHz

Power and distance are rounded to the nearest mW and mm before calculation


The result is rounded to one decimal place for comparison

For < 50 mm distance, we just calculate mW of the exclusion threshold value (3.0) to do compare.

This formula is [3.0] / $[\sqrt{f(GHz)}] \cdot [(min. test separation distance, mm)] = exclusion threshold of mW.$

- 5. Per KDB 447498 D01v05r01, at 100 MHz to 6 GHz and for test separation distances > 50 mm, the SAR test exclusion threshold is determined according to the following
 - a) [Threshold at 50 mm in step 1) + (test separation distance 50 mm)·(f(MHz)/150)] mW. at 100 MHz to 1500 MHz
 - b) [Threshold at 50 mm in step 1) + (test separation distance 50 mm) 10] mW at > 1500 MHz and ≤ 6 GHz
- 6. When the minimum test separation distance is < 5 mm, a distance of 5 mm according to 5) in section 4.1 is applied to determine SAR test exclusion.

10.8 EUT SETUP PHOTOS

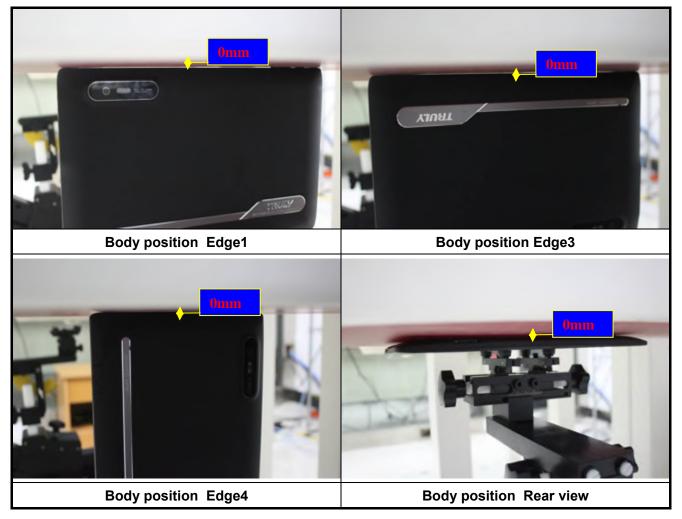

10.9 SAR MEASUREMENT RESULTS

Body worn SAR Test Results

GSM SAR

Band	Mode	Test Position	Dist. (mm)	Ch.	Freq. (MHZ)	max Power (dBm)	Turn- Up Limit (dBm)	Scaled Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
GPRS850	GPRS 4slots	Rear	0	251	848.8	29.09	29.5	1.099	0.11	0.721	0.792
GPRS850	GPRS 4slots	Edge 1	0	251	848.8	29.09	29.5	1.099	-0.06	0.461	0.507
GPRS850	GPRS 4slots	Edge 3	0	251	848.8	29.09	29.5	1.099	-0.13	0.685	0.753
GPRS850	GPRS 4slots	Edge 4	0	251	848.8	29.09	29.5	1.099	0.00	0.212	0.233
GPRS 1900	GPRS 4slots	Rear	0	810	1909.8	26.53	27	1.114	0.06	0.770	0.858
GPRS 1900	GPRS 4slots	Edge 3	0	810	1909.8	26.53	27	1.114	0.05	0.526	0.586
GPRS 1900	GPRS 4slots	Edge 4	0	810	1909.8	26.53	27	1.114	0.14	0.175	0.195
GPRS 1900	GPRS 4slots	Rear	0	512	1850.2	29.00	29.5	1.122	0.11	0.644	0.723
GPRS 1900	GPRS 4slots	Rear	0	661	1880	29.01	29.5	1.119	0.10	0.762	0.853

WCDMA SAR

Band	Mode	Test Position	Dist. (mm)	Ch.	Freq. (MHZ)	max Power (dBm)	Turn- Up Limit (dBm)	Scaled Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
Band II	RMC 12.2k	Rear	0	9262	1852.4	21.38	21.5	1.028	-0.14	0.732	0.753
Band II	RMC 12.2k	Edge 3	0	9262	1852.4	21.38	21.5	1.028	-0.16	0.577	0.593
Band II	RMC 12.2k	Edge 4	0	9262	1852.4	21.38	21.5	1.028	-0.15	0.194	0.199
Band V	RMC 12.2k	Rear	0	4132	826.4	22.80	23	1.047	0.10	0.712	0.746
Band V	RMC 12.2k	Edge 3	0	4132	826.4	22.80	23	1.047	-0.01	0.618	0.647
Band V	RMC 12.2k	Edge 4	0	4132	826.4	22.80	23	1.047	0.01	0.118	0.124

WLAN SAR

Band	Mode	Test Position	Dist. (mm)	Ch.	Freq. (MHZ)	max Power (dBm)	Turn- Up Limit (dBm)	Scaled Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
WLAN 2.4G	802.11b	Rear	0	6	2437	13.18	13.5	1.076	0.09	0.157	0.169
WLAN 2.4G	802.11b	Edge 1	0	6	2437	13.18	13.5	1.076	-0.02	0.041	0.044

Band	Mode	Test Position	Dist. (mm)	Ch.	Freq. (MHZ)	max Power (dBm)	Turn- Up Limit (dBm)	Scaled Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
WLAN 5.8G	802.11a	Rear	0	153	5765	14.32	15	1.169	0.00	0.307	0.359
WLAN 5.8G	802.11a	Rear	0	161	5805	14.37	15	1.156	0.00	0.238	0.275
WLAN 5.8G	802.11a	Rear	0	165	5825	14.45	15	1.135	0.00	0.225	0.255
WLAN 5.8G	802.11a	Edge 1	0	153	5765	14.32	15	1.169	0.00	0.635	0.743
WLAN 5.8G	802.11a	Edge 1	0	161	5805	14.37	15	1.156	-0.19	0.593	0.686
WLAN 5.8G	802.11a	Edge 1	0	165	5825	14.45	15	1.135	-0.16	0.587	0.666
WLAN 5.8G	802.11a	Edge 4	0	153	5765	14.32	15	1.169	0.00	0.278	0.325
WLAN 5.8G	802.11a	Edge 4	0	161	5805	14.37	15	1.156	0.00	0.189	0.219

FCCID: 2ABCS-A6102 Date of Issue : January 8, 2014

10.10 REPEATED SAR MEASUREMENT

Note:

Per KDB 865664 D01v01r01, for each frequence band, repeated SAR measurement is not required when the measured SAR is < 0.8W/Kg.

10.11 SAR HANDSETS MULTI XMITER ASSESSMENT

	Position	Applicable Combination
Simultaneous Transmission	Body-worn	WWAN (data) + WLAN WWAN (data) + BT

Note:

- 2.4GHz WLAN and BT share the same antenna, and cannot transmit simultaneously.
- The reported SAR summation is calculated based on the same configuration and test position.
- For simultaneous transmission analysis, Bluetooth SAR is estimated per KDB 447498 D01v05 based on the formula below.

(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)] • [√f(GHz)/x] W/kg for test separation distances \leq 50 mm; where x = 7.5 for 1-g SAR, and x = 18.75 for 10-g SAR.

0.4 W/kg for 1-g SAR and 1.0 W/kg for 10-g SAR, when the test separation distances is > 50 mm.

Bluetooth	Max power	Body (5mm distance)
Estimated SAR (W/kg)	4dBm	0.104 W/kg

- Per KDB 447498 D01v05, simultaneous transmission SAR is compliant if,
 - 1) Scalar SAR summation < 1.6W/kg.
 - 2) SPLSR = (SAR1 + SAR2)1.5 / (min. separation distance, mm), and the peak separation distance is determined from the square root of [(x1-x2)2 + (y1-y2)2 + (z1-z2)2], where (x1, y1, z1) and (x2, y2, z2) are the coordinates of the extrapolated peak SAR locations in the zoom scan
 - If SPLSR \leq 0.04, simultaneously transmission SAR is compliant
 - 3) Simultaneously transmission SAR measurement, and the reported multi-band SAR < 1.6W/kg

Result of SUM ∑SAR1g of Body-worn

SUM ∑SAR1g (GPRS850+WLAN(2.4G) or Bluetooth)										
Position	Distance	Stand	alone SAR(1g) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]				
1 Osition	[mm]	GSM850	WLAN 2.4G	Bluetoooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth				
Rear	0	0.792	0.169	0.104	0.961	0.896				

SUM ∑SAR1g (GPRS1900+WLAN(2.4G) or Bluetooth)										
Position	Distance	Stand	alone SAR(1g)	[W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]				
	[mm]	PCS 1900	WLAN 2.4G	Bluetoooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth				
Rear	0	0.858	0.169	0.104	1.027	0.962				

SUM ∑SAR1g (WCDMA Band II+WLAN(2.4G) or Bluetooth)										
Position	Distance	Stand a	lone SAR(1g) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]				
	[mm]	WCDMA II	WLAN 2.4G	Bluetoooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth				
Rear	0	0.753	0.169	0.104	0.922	0.857				

SUM ∑SAR1g (WCDMA Band V+WLAN(2.4G) or Bluetooth)										
Position	Distance	Stand a	lone SAR(1g) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]				
	[mm]	WCDMA V	WLAN 2.4G	Bluetoooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth				
Rear	0	0.746	0.169	0.104	0.915	0.85				

SUM ∑SAR1g (GPRS850+WLAN(5.8G) or Bluetooth)										
Position	Distance	Stand	alone SAR(1g) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]				
1 Osition	[mm]	GSM850	WLAN 5.8G	Bluetoooth	WWAN + WLAN(5.8G)	WWAN + Bluetooth				
Rear	0	0.792	0.359	0.104	1.151	0.896				
Edge4	0	0.233	0.519	0.104	0.752	0.337				

SUM ∑SAR1g (GPRS1900+WLAN(5.8G) or Bluetooth)							
Position	Distance	Stand alone SAR(1g) [W/kg]			SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]	
	[mm]	PCS 1900	00 WLAN 5.8G Bluetoooth		WWAN + WLAN(5.8G)	WWAN + Bluetooth	
Rear	0	0.858	0.359	0.104	1.217	0.962	
Edge4	0	0.195	0.519	0.104	0.714	0.299	



SUM ∑SAR1g (WCDMA Band II+WLAN(5.8G) or Bluetooth)								
Position	Distance	Stand alone SAR(1g) [W/kg]			SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]		
	[mm]	WCDMA II	WLAN 5.8G	Bluetoooth	WWAN + WLAN(5.8G)	WWAN + Bluetooth		
Rear	0	0.753	0.359	0.104	1.112	0.857		
Fdge4	0	0.199	0.519	0.104	0.718	0.303		

SUM ∑SAR1g (WCDMA Band V+WLAN(5.8G) or Bluetooth)							
Position	Distance	Stand alone SAR(1g) [W/kg]			SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]	
	[mm]	WCDMA V	WCDMA V WLAN 5.8G Bluetoooth		WWAN + WLAN(5.8G)	WWAN + Bluetooth	
Rear	0	0.746	0.359	0.104	1.105	0.850	
Edge4	0	0.124	0.519	0.104	0.643	0.228	

EUT PHOTO



















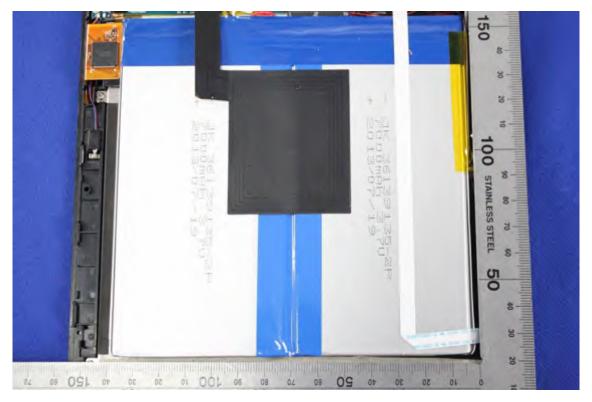

EQUIPMENT LIST & CALIBRATION STATUS

Name of Equipment	Manufacturer	Type/Model	Serial Number	Last Calibration	Calibration Due
PC	HP	Core(rm)3.16G	CZCO48171H	N/A	N/A
Signal Generator	Agilent	E8257C	MY43321570	05/13/2013	05/12/2014
S-Parameter Network Analyzer	Agilent	E5071B	MY42301382	03/11/2013	03/10/2014
Wireless Communication Test Set	R&S	CMU200	SN:109525	01/23/2013	01/22/2014
Power Meter	Agilent	E4416A	GB41292714	03/16/2013	03/15/2014
Peak & Average sensor	Agilent	E9327A	CF0001	03/16/2013	03/15/2014
E-field PROBE	SPEAG	EX3DV4	3798	07/26/2013	07/25/2014
DAE	SPEAG	DEA4	1245	07/25/2013	07/24/2014
DIPOLE 835MHZ ANTENNA	SPEAG	D835V2	4d114	07/30/2013	07/29/2014
DIPOLE 1900MHZ ANTENNA	SPEAG	D1900V2	5d136	07/22/2013	07/21/2014
DIPOLE 2450MHZ ANTENNA	SPEAG	D2450V2	817	07/31/2013	07/30/2014
DIPOLE 5GHZ ANTENNA	SPEAG	D5GHzV2	1095	05/31/2013	05/30/2014
DUMMY PROBE	SPEAG	DP_2	SPDP2001AA	N/A	N/A
SAM PHANTOM (ELI4 v4.0)	SPEAG	QDOVA001BB	1102	N/A	N/A
Twin SAM Phantom	SPEAG	QD000P40CD	1609	N/A	N/A
ROBOT	SPEAG	TX60	F10/5E6AA1/A101	N/A	N/A
ROBOT KRC	SPEAG	CS8C	F10/5E6AA1/C101	N/A	N/A
LIQUID CALIBRATION KIT	ANTENNESSA	41/05 OCP9	00425167	N/A	N/A

Reference No.: C130922R01-SF

FCCID: 2ABCS-A6102

Date of Issue : January 8, 2014

13. FACILITIES

All measurement facilities used to collect the measurement data are located at

No.10, Weiye Rd., Innovation Park, Eco & Tec. Development Part, Kunshan City, Jiangsu Province, China.

14. REFERENCES

- [1] Federal Communications Commission, \Report and order: Guidelines for evaluating the environ-mental effects of radiofrequency radiation", Tech. Rep. FCC 96-326, FCC, Washington, D.C. 20554, 1996.
- [2] David L. Means Kwok Chan, Robert F. Cleveland, \Evaluating compliance with FCC guidelines for human exposure to radiofrequency electromagnetic fields", Tech. Rep., Federal Communication Commission, O_ce of Engineering & Technology, Washington, DC, 1997.
- [3] Thomas Schmid, Oliver Egger, and Niels Kuster, \Automated E-_eld scanning system for dosimetric assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp. 105{113, Jan. 1996.
- [4] Niels Kuster, Ralph K.astle, and Thomas Schmid, \Dosimetric evaluation of mobile communications equipment with known precision", IEICE Transactions on Communications, vol. E80-B, no. 5, pp. 645{652, May 1997.
- [5] CENELEC, \Considerations for evaluating of human exposure to electromagnetic fields (EMFs) from mobile telecommunication equipment (MTE) in the frequency range 30MHz 6GHz", Tech. Rep., CENELEC, European Committee for Electrotechnical Standardization, Brussels, 1997.
- [6] ANSI, ANSI/IEEE C95.1-1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, The Institute of Electrical and Electronics Engineers, Inc., New York, NY 10017, 1992.
- [7] Katja Pokovic, Thomas Schmid, and Niels Kuster, \Robust setup for precise calibration of E-_eld probes in tissue simulating liquids at mobile communications frequencies", in ICECOM _ 97, Dubrovnik, October 15{17, 1997, pp. 120{124.
- [8] Katja Pokovic, Thomas Schmid, and Niels Kuster, \E-_eld probe with improved isotropy in brain simulating liquids", in Proceedings of the ELMAR, Zadar, Croatia, 23{25 June, 1996, pp. 172{175.
- [9] Volker Hombach, Klaus Meier, Michael Burkhardt, Eberhard K. uhn, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 900 MHz", IEEE Transactions on Microwave Theory and Techniques, vol. 44, no. 10, pp. 1865{1873, Oct. 1996.
- [10] Klaus Meier, Ralf Kastle, Volker Hombach, Roger Tay, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 1800 MHz", IEEE Transactions on Microwave Theory and Techniques, Oct. 1997, in press.
- [11] W. Gander, Computermathematik, Birkhaeuser, Basel, 1992.
- [12] W. H. Press, S. A. Teukolsky, W. T. Vetterling, and B. P. Flannery, Numerical Recepies in C, The Art of Scientific Computing, Second Edition, Cambridge University Press, 1992.. Dosimetric Evaluation of Sample device, month 1998 9
- [13] NIS81 NAMAS, \The treatment of uncertainity in EMC measurement", Tech. Rep., NAMAS Executive, National Physical Laboratory, Teddington, Middlesex, England, 1994.
- [14] Barry N. Taylor and Christ E. Kuyatt, \Guidelines for evaluating and expressing the uncertainty of NIST measurement results", Tech. Rep., National Institute of Standards and Technology, 1994. Dosimetric Evaluation of Sample device, month 1998 10

ATTACHMENTS 15.

Exhibit	Content
1	System Performance Check Plots
2	Dipole calibration report D835V2 SN:4d114
3	Dipole calibration report D1900V2-SN:5d136
4	Dipole calibration report D2450V2 SN: 817
5	Dipole calibration report D5GHzV2 SN: 1095
6	Probe calibration report EX3DV4 SN3798
7	DAE calibration report DEA4 SD000D04BJ SN:1245
8	SAR Test Plots

APPENDIX A: PLOTS OF PERFORMANCE CHECK

The plots are showing as followings.

Reference No.: C130922R01-SF

FCCID: 2ABCS-A6102 Date of Issue : January 8, 2014

Test Laboratory: Compliance Certification Services Inc. Date: 11/10/2013

System Performance Body Check-D835

DUT: Dipole 835 MHz; Type: D835V2; Serial: SN4d092

Communication System: CW; Communication System Band: D835 (835.0 MHz); Frequency: 835

MHz; Duty Cycle: 1:1

Medium parameters used: f = 835 MHz; σ = 0.97 S/m; ϵ_r = 54.329; ρ = 1000 kg/m³

Room Ambient Temperature: 22.9°C; Liquid Temperature: 21.5°C

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY Configuration:

- Probe: EX3DV4 SN3798; ConvF(9.27, 9.27, 9.27); Calibrated: 7/26/2013;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1245; Calibrated: 7/25/2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1102
- DASY52 52.8.5(1059);
- SEMCAD X Version 14.6.8 (7028)

System Performance Check at Frequencies Low 1 GHz/d=15mm, Pin=250 mW, dist=3.0mm (EX-Probe)/Area Scan (7x12x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 1.98 W/kg


System Performance Check at Frequencies Low 1 GHz/d=15mm, Pin=250 mW, dist=3.0mm (EX-**Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:**

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 45.917 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 2.33 W/kg

SAR(1 g) = 2.32 W/kg; SAR(10 g) = 1.56 W/kgMaximum value of SAR (measured) = 2.02 W/kg

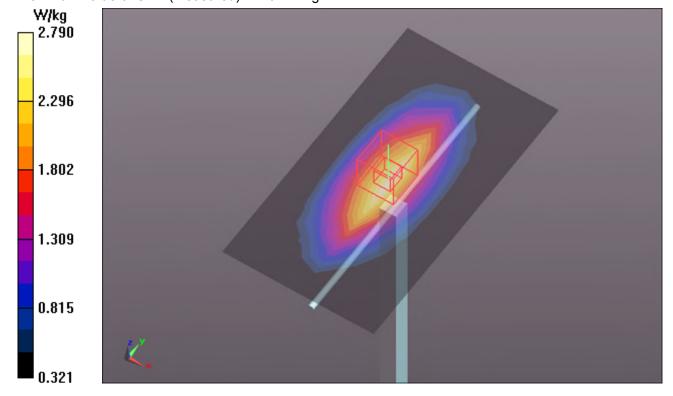

Reference No.: C130922R01-SF

Test Laboratory: Compliance Certification Services Inc. Date: 11/11/2013

System Performance Check-Body D1900

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: SN:5d142

Communication System: CW; Communication System Band: D1900 (1900.0 MHz); Frequency: 1900

MHz; Duty Cycle: 1:1

Medium parameters used: f = 1900 MHz; σ = 1.537 S/m; ϵ_r = 53.263; ρ = 1000 kg/m³

Room Ambient Temperature: 22.3; Liquid Temperature: 21.2°C

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY Configuration:

- Probe: EX3DV4 SN3798; ConvF(7.32, 7.32, 7.32); Calibrated: 7/26/2013;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1245; Calibrated: 7/25/2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1102
- DASY52 52.8.5(1059);
- SEMCAD X Version 14.6.8 (7028)

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Area Scan (7x7x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 10.2 W/kg

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 83.104 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 14.2 W/kg

SAR(1 g) = 9.73 W/kg; SAR(10 g) = 4.39 W/kg

Maximum value of SAR (measured) = 11.1 W/kg

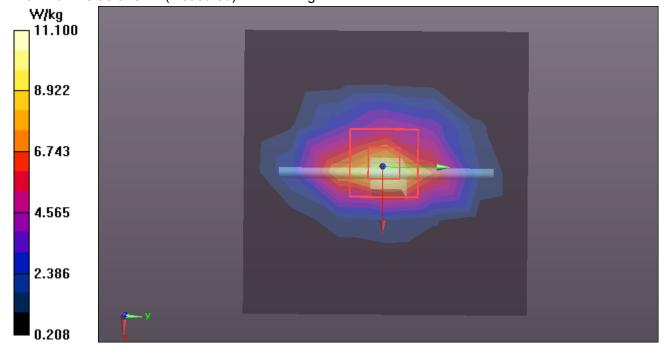

Test Laboratory: Compliance Certification Services Inc. Date: 11/13/2013

SystemPerformance Body Check-D2450

DUT: Dipole 2450 MHz; Type: D24500V2; Serial: 817

Communication System: CW; Communication System Band: D2450 (2450.0 MHz); Frequency: 2450

MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz; $\sigma = 2.012 \text{ S/m}$; $\varepsilon_r = 51.332$; $\rho = 1000 \text{ kg/m}^3$

Room Ambient Temperature: 23.4°C; Liquid Temperature: 21.8°C

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY Configuration:

- Probe: EX3DV4 SN3798; ConvF(7.08, 7.08, 7.08); Calibrated: 7/26/2013;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1245; Calibrated: 7/20/2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1102
- DASY52 52.8.5(1059);
- SEMCAD X Version 14.6.8 (7028)

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Area Scan (8x9x1):

Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 18.6 W/kg

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 90.233 V/m; Power Drift = 0.11 dB

Peak SAR (extrapolated) = 26.7 W/kg

SAR(1 g) = 12.9 W/kg; SAR(10 g) = 6.68 W/kg

Maximum value of SAR (measured) = 20.1 W/kg

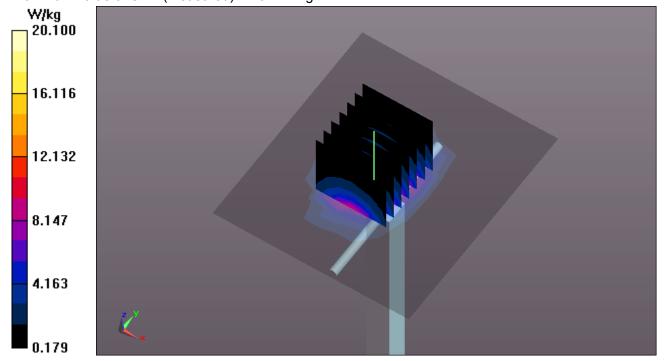

Reference No.: C130922R01-SF

FCCID: 2ABCS-A6102 Date of Issue :January 8, 2014

Test Laboratory: Compliance Certification Services Inc. Date: 12/26/2013

System check_ MSL5800

DUT: Dipole 5GHz; Type: D5GHz V2; Serial: 1095

Communication System: CW; Communication System Band: D5GHz; Frequency: 5800 MHz;Duty Cycle: 1:1 Medium parameters used (interpolated): f = 5800 MHz; $\sigma = 6.17$ S/m; $\epsilon_r = 46.782$; $\rho = 1000$ kg/m³

Room Ambient Temperature: 22.7°C; Liquid Temperature: 21.4°C

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY Configuration:

- Probe: EX3DV4 SN3798; ConvF(4.24, 4.24, 4.24); Calibrated: 7/26/2013;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1245; Calibrated: 7/25/2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: 1102
- DASY52 52.8.5(1059);
- SEMCAD X Version 14.6.8 (7028)


Configuration/Pin=100mW,d=10mm/Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 7.09 W/kg

Configuration/Pin=100mW,d=10mm/Zoom Scan (7x7x15)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 35.165 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 26.2 W/kg

SAR(1 g) = 7.21 W/kg; SAR(10 g) = 2.1 W/kgMaximum value of SAR (measured) = 8.50 W/kg

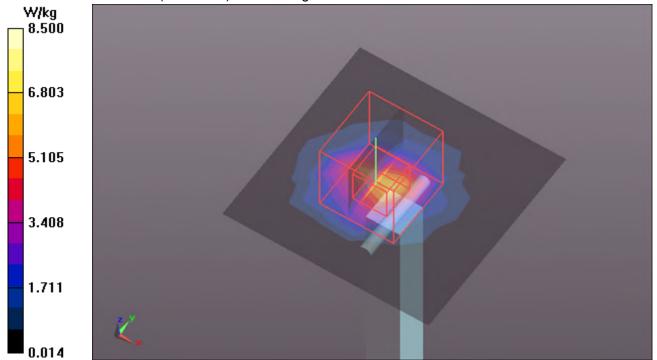

Date: 1/8/2014

Test Laboratory: Compliance Certification Services Inc.

System Performance Check-Body D835

DUT: Dipole 835 MHz D835V2; Type: D835V2; Serial: D835V2 - SN4d114

Communication System: CW; Communication System Band: D835 (835.0 MHz); Frequency: 835

MHz; Duty Cycle: 1:1

Medium parameters used: f = 835 MHz; σ = 0.954 S/m; ε_r = 53.03; ρ = 1000 kg/m³

Room Ambient Temperature: 22°C; Liquid Temperature: 21.5°C

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY Configuration:

- Probe: EX3DV4 SN3798; ConvF(9.27, 9.27, 9.27); Calibrated: 7/26/2013;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1245; Calibrated: 7/25/2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: 1102
- DASY52 52.8.5(1059);
- SEMCAD X Version 14.6.8 (7028)

System Performance Check at Frequencies Low 1 GHz/d=15mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (measured) = 2.77 W/kg

System Performance Check at Frequencies Low 1 GHz/d=15mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.903 V/m; Power Drift = -0.11 dB

Peak SAR (extrapolated) = 3.26 W/kg

SAR(1 g) = 2.41 W/kg; SAR(10 g) = 1.47 W/kgMaximum value of SAR (measured) = 2.78W/kg

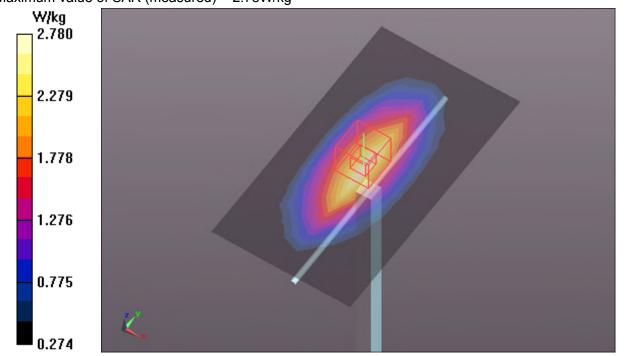

Reference No.: C130922R01-SF

Date of Issue :January 8, 2014

APPENDIX B: DASY CALIBRATION CERTIFICATE

The DASY Calibration Certificates are showing as followings .



Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kallbrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Accreditation No.: SCS 108

C

Certificate No: D835V2-4d114 Jul13

CALIBRATION CERTIFICATE

Object

D835V2 - SN: 4d114

Calibration procedure(s)

QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

July 30, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37292783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe ES3DV3	SN: 3206	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
	Name	Function	Signature
Calibrated by:	Claudio Leubler	Laboratory Technician	

Issued: July 30, 2013

This calibration certificate shall not be reproduced except in full without written approval of the faboratory

Katja Pokovio

Certificate No: D835V2-4d114_Jul13

Approved by:

Page 1 of 8

Technical Manager

Compliance Certification Services Inc.

Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausetrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étatonnege
Servizio sylzzero di teratura
S Swise Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)",

February 2005

c) Federal Communications Commission Office of Engineering & Technology (FCC OET). "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D835V2-4d114_Jul13

Page 2 of 8

Measurement Conditions

DASY system configuration, as far as not given on page 1.

2317401
with Spacer

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.8 ± 6 %	0.92 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	2000	100

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.41 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.50 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.58 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.24 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.9 ± 6 %	1.00 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	-	-

SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.44 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.53 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.61 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.32 W/kg ± 16.5 % (k=2)

Certificate No: D835V2-4d114_Jul13

Page 3 of 8

Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.1 Ω - 1.3 jΩ	
Return Loss	- 32.1 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.2 Ω - 3.0 μΩ	
Return Loss	- 29.1 dB	

General Antenna Parameters and Design

Electrical Delay (one direction) 1.399 ns	3
---	---

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	June 29, 2010

Certificate No: D835V2-4d114_Jul13

Reference No : C130922R01-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

DASY5 Validation Report for Head TSL

Date: 30.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: f = 835 MHz; $\sigma = 0.92 \text{ S/m}$; $\varepsilon_r = 41.8$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section


Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(6.05, 6.05, 6.05); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)


Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 56.702 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 3.60 W/kg SAR(1 g) = 2.41 W/kg; SAR(10 g) = 1.58 W/kg Maximum value of SAR (measured) = 2.81 W/kg

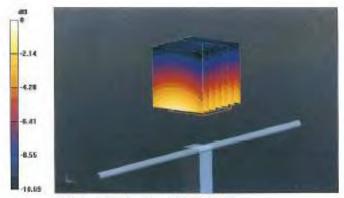

0 dB = 2.81 W/kg = 4.49 dBW/kg

Impedance Measurement Plot for Head TSL

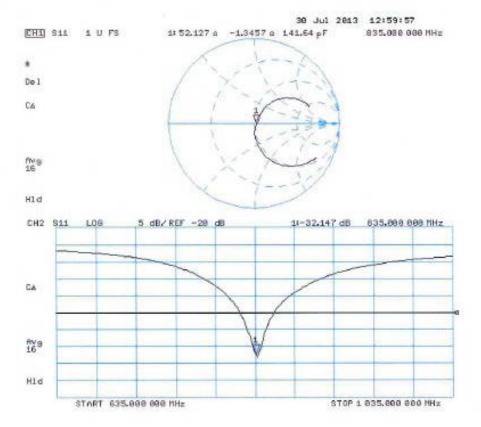

Certificate No: DB35V2-4d114_Jul13

Page 6 of 8

DASY5 Validation Report for Body TSL

Date: 22.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: f = 835 MHz; $\sigma = 1$ S/m; $\varepsilon_r = 54.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(6.04, 6.04, 6.04); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 54.853 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 3.56 W/kg SAR(1 g) = 2.44 W/kg; SAR(10 g) = 1.61 W/kgMaximum value of SAR (measured) = 2.83 W/kg



0 dB = 2.83 W/kg = 4.52 dBW/kg

Reference No.: C130922R01-SF

Impedance Measurement Plot for Body TSL

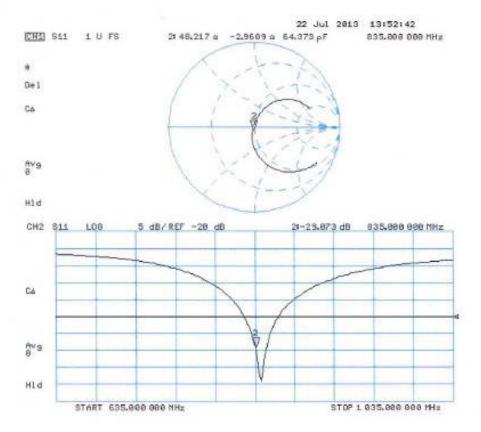



Report No. C 13 1230502-5F

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Calibration Laboratory of

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlocher Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Accreditation No.: SCS 108

Certificate No: D1900V2-5d136 Jul13

CALIBRATION CERTIFICATE

Object

D1900V2 - SN: 5d136

Calibration procedure(s)

Schmid & Partner

QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

July 22, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%,

Calibration Equipment used (M&TE critical for calibration)

ID#	Cal Date (Certificate No.)	Scheduled Calibration
GB37480704	01-Nov-12 (No. 217-01640)	Oct-13
US37292783	01-Nov-12 (No. 217-01640)	Oct-13
SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
ID#	Check Date (in house)	Scheduled Check
MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
US37390585 S4206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
Name	Function	Signature
Jeton Kastrati	Laboratory Technician	1 19
W-8- H-1	* *****	me
Katja Pokovic	Technical Manager	Jak lly
	GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206	GB37480704 01-Nov-12 (No. 217-01640) US37292783 01-Nov-12 (No. 217-01640) SN: 5058 (20k) 04-Apr-13 (No. 217-01736) SN: 5047.3 / 06327 04-Apr-13 (No. 217-01739) SN: 3205 28-Dec-12 (No. ES3-3205_Dec12) SN: 601 25-Apr-13 (No. DAE4-601_Apr13) ID # Check Date (in house) MY41092317 18-Oct-02 (in house check Oct-11) 100005 04-Aug-99 (in house check Oct-11) US37390585 S4206 18-Oct-01 (in house check Oct-12) Name Function Jeton Kastrati Laboratory Technician

Certificate No: D1900V2-5d136_Jul13

Page 1 of 8

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Issued: July 22, 2013

Compliance Certification Services Inc.

Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zoughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kallbrierdienst Service suisse d'étalonnage Servizio svizzero di taretura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multileteral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)",

February 2005

c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay; One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d135_Jul13

Page 2 of 8

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Messured Head TSL parameters	(22.0 ± 0.2) °C	38.9 ± 6 %	1.36 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	-	nema)

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.0 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.29 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 16.5 % (k=2)

Body TSL parameters

e following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.4 ± 6 %	1.49 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	(asser)	

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10,0 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	40.5 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.37 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.6 W/kg ± 16.5 % (k=2)

Certificate No: D1900V2-5d136_Jul13

Page 3 of 8

FCCID: 2ABCS-A6102

Date of Issue : January 8, 2014

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.9 Ω + 7.2 jΩ	
Return Loss	- 22.5 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.7 Ω + 7.3 jΩ	
Return Loss	- 22.1 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.203 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	April 14, 2010	

Certificate No: D1900V2-5d136_Jul13

DASY5 Validation Report for Head TSL

Date: 22.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d136

Communication System: UID 0 - CW ; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz; $\sigma = 1.36 \text{ S/m}$; $\varepsilon_r = 38.9$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.98, 4.98, 4.98); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0;


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 95.803 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 18.1 W/kg SAR(1 g) = 10 W/kg; SAR(10 g) = 5.29 W/kgMaximum value of SAR (measured) = 12.4 W/kg

dB -5.00 -10.00-15.00-20.00

0 dB = 12.4 W/kg = 10.93 dBW/kg

25.00

Impedance Measurement Plot for Head TSL

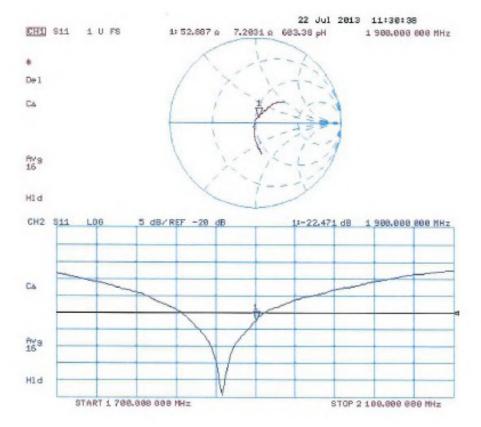

Reference No.: C130922R01-SF

DASY5 Validation Report for Body TSL

Date: 22.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d136

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz; $\sigma = 1.49 \text{ S/m}$; $\epsilon_r = 53.4$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)


DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.6, 4.6, 4.6); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 95.803 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 17.0 W/kg SAR(1 g) = 10 W/kg; SAR(10 g) = 5.37 W/kg

Maximum value of SAR (measured) = 12.5 W/kg

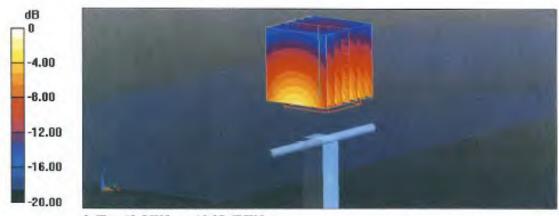

0 dB = 12.5 W/kg = 10.97 dBW/kg

Impedance Measurement Plot for Body TSL

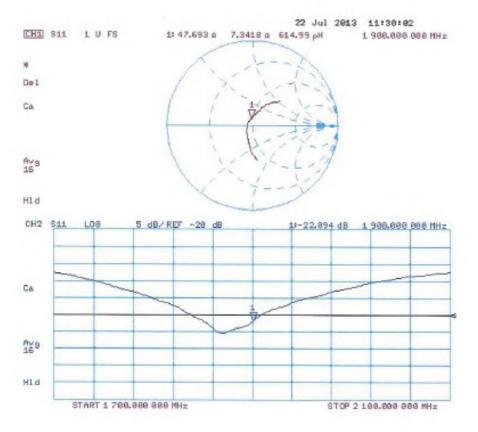

Certificate No: D1900V2-5d136_Jul13

Page 8 of 8



Report No: C131230502-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibriordienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Accreditation No.: SCS 108

C

Certificate No: D2450V2-817_Jul13

CALIBRATION CERTIFICATE

Object

D2450V2 - SN: 817

Calibration procedure(s)

QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

July 31, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (Si). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%,

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Call Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	01-Nav-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37292783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe ES3DV3	SN: 3206	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13:
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
	Name	Function	Signature
Calibrated by:	Israe El-Naoug	Laboratory Technician	Orran Cl-Dagos of
Approved by:	Katja Pokovic	Technical Manager	0000

Issued: July 31, 2013

This calibration conficate shall not be reproduced except in full without written approval of the laboratory

Certificate No: D2450V2-817_Jul13

Page 1 of 8

Compliance Certification Services Inc.

Report No: C131230502-5F

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Calibration Laboratory of Schmid & Partner Engineering AG

Zoughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlscher Kalibnerdienst Scrylce suisse d'étalonnage Scrylzio sylzzero di tareture S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multitateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-817_Jul13

Page 2 of 8

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.8 ± 6 %	1.81 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		-

SAR result with Head TSL

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.18 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 16.5 % (k=2)

Body TSL parameters

e following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.5 ± 6 %	2.01 mho/m ± 8 %
Body TSL temperature change during test	< 0.5 °C	****	(man)

SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.8 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	49.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.87 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.1 W/kg ± 16.5 % (k=2)

Certificate No: D2450V2-817_Jul13

Page 3 of 8

FCCID: 2ABCS-A6102

Date of Issue : January 8, 2014

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$53.5 \Omega + 2.9 j\Omega$	
Return Loss	- 27.1 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.7 Ω + 4.5 Ω	
Return Loss	- 27.0 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.159 ns
Electrical Delay (one direction)	1.138115

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 23, 2007

Certificate No: D2450V2-817_Jul13

Reference No.: C130922R01-SF

FCCID: 2ABCS-A6102

Date of Issue : January 8, 2014

DASY5 Validation Report for Head TSL

Date: 31.07.2013

Rev. UT

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz; $\sigma = 1.81 \text{ S/m}$; $\epsilon_r = 37.8$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)


DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.52, 4.52, 4.52); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 99.781 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 27.7 W/kgSAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.18 W/kg

Maximum value of SAR (measured) = 16.8 W/kg

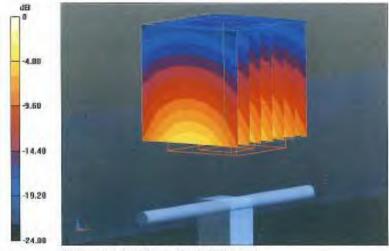

0 dB = 16.8 W/kg = 12.25 dBW/kg

Impedance Measurement Plot for Head TSL

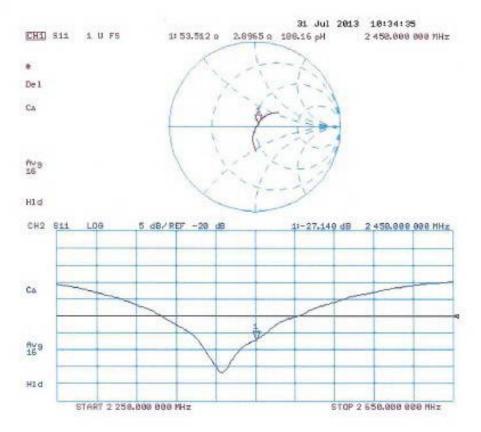

DASY5 Validation Report for Body TSL

Date: 31.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz; $\sigma = 2.01 \text{ S/m}$; $\varepsilon_r = 50.5$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section


Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.42, 4.42, 4.42); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 94.151 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 26.3 W/kg SAR(1 g) = 12.6 W/kg; SAR(10 g) = 5.87 W/kg Maximum value of SAR (measured) = 16.7 W/kg

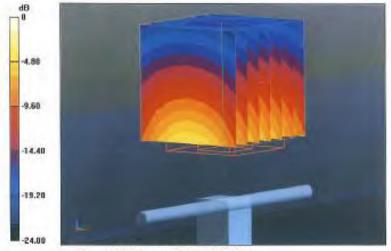

0 dB = 16.7 W/kg = 12.23 dBW/kg


Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Impedance Measurement Plot for Body TSL

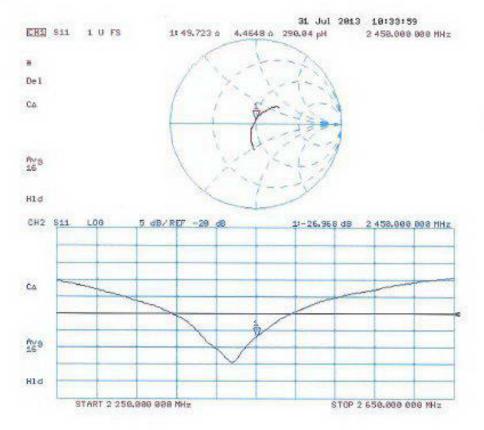

Compliance Certification Services Inc.

Report No: C131230502-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Calibration Laboratory of Schmid & Partner Engineering AG Zoughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Accreditation No.: SCS 108

Certificate No: D5GHzV2-1095_May13

CALIBRATION CERTIFICATE

Object

D5GHzV2 - SN: 1095

Calibration procedure(s)

QA CAL-22.v2

Calibration procedure for dipole validation kits between 3-6 GHz

Calibration date:

May 31, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37292783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe EX3DV4	SN: 3503	28-Dec-12 (No. EX3-3503_Dec12)	Dec-13
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	412

Certificate No: D5GHzV2-1095_May13

Page 1 of 16

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Issued: May 31, 2013



Reference No.: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Calibration Laboratory of Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di tareture

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC 62209-2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", March 2010
- b) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D5GHzV2-1095 May13

Page 2 of 16

Measurement Conditions

DASY Version	DASY5	V52.8.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.5 ± 6 %	4.50 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	****	

SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.94 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.6 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.7 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1095_May13

Page 3 of 16

Reference No.: C130922R01-SF

Date of Issue :January 8, 2014

Head TSL parameters at 5300 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.3 ± 6 %	4.60 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	3444	****

SAR result with Head TSL at 5300 MHz

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.1 W / kg ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.37 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.7 W/kg ± 19.5 % (k=2)

Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.1 ± 6 %	4.79 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	****	444

SAR result with Head TSL at 5500 MHz

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.42 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	84.3 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.40 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.0 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1095_May13

Page 4 of 16

Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.0 ± 6 %	4.89 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	Add.	

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.24 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	82.5 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 19.5 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.7 ± 6 %	5.11 mha/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	and .	

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.86 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	78.7 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.23 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.3 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1095_May13

Page 5 of 16

Body TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	49.0	5.30 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.6 ± 6 %	5.41 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	****	

SAR result with Body TSL at 5200 MHz

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.44 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	74.6 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.08 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.9 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5300 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.42 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.4 ± 6 %	5.53 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	4164	****

SAR result with Body TSL at 5300 MHz

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.58 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	76.0 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.12 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.3 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1095_May13

Page 6 of 16

Body TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.65 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.1 ± 6 %	5.80 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	****	ines.

SAR result with Body TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.89 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	79.1 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.19 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	22.0 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.0 ± 6 %	5.80 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		****

SAR result with Body TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.76 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	77.8 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.15 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.6 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1095_May13

Page 7 of 16

Body TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.6 ± 6 %	6.24 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.47 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	75.0 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.06 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.7 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1095_May13

Page 8 of 16

Appendix

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	50.2 Ω - 6.4 jΩ
Return Loss	- 23.9 dB

Antenna Parameters with Head TSL at 5300 MHz

Impedance, transformed to feed point	50.2 Ω - 3.3 jΩ	
Return Loss	- 29.6 dB	

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	53.2 Ω - 2.2 jΩ	
Return Loss	- 28.5 dB	

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	56.0 Ω - 1.1 jΩ	
Return Loss	- 24.8 dB	

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	55.4 Ω - 2.8 jΩ	
Return Loss	- 24.8 dB	

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	50.7 Ω - 5.3 jΩ	
Return Loss	- 25.5 dB	

Antenna Parameters with Body TSL at 5300 MHz

Impedance, transformed to feed point	50.8 Ω - 1.5 jΩ	
Return Loss	- 35.5 dB	

Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	53.8 Ω - 1.2 jΩ	
Return Loss	- 28.4 dB	

Certificate No: D5GHzV2-1095_May13

Page 9 of 16

Report No. C131230502-5F

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	56.2 Ω + 1.1 jΩ	
Return Loss	- 24.5 dB	

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	55.6 Ω + 0.3 jΩ	
Return Loss	- 25.5 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.208 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 24, 2010

Certificate No: D5GHzV2-1095_May13

Page 10 of 16

Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

DASY5 Validation Report for Head TSL

Date: 30.05.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used: f = 5200 MHz; σ = 4.5 S/m; ϵ_r = 36.5; ρ = 1000 kg/m³, Medium parameters used: f = 5300 MHz; σ = 4.6 S/m; ϵ_r = 36.3; ρ = 1000 kg/m³, Medium parameters used: f = 5500 MHz; σ = 4.79 S/m; ϵ_r = 36.1; ρ = 1000 kg/m³, Medium parameters used: f = 5600 MHz; σ = 4.89 S/m; ϵ_r = 36; ρ = 1000 kg/m³, Medium parameters used: f = 5800 MHz; σ = 5.11 S/m; ϵ_r = 35.7; ρ = 1000 kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.41, 5.41, 5.41); Calibrated: 28.12.2012, ConvF(5.1, 5.1, 5.1);
 Calibrated: 28.12.2012, ConvF(4.91, 4.91, 4.91); Calibrated: 28.12.2012, ConvF(4.76, 4.76, 4.76);
 Calibrated: 28.12.2012, ConvF(4.81, 4.81, 4.81); Calibrated: 28.12.2012;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.6(1115); SEMCAD X 14.6.9(7117)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.153 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 29.3 W/kg

SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg

Maximum value of SAR (measured) = 18.3 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.596 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 31.2 W/kg

SAR(1 g) = 8.3 W/kg; SAR(10 g) = 2.37 W/kg

Maximum value of SAR (measured) = 19.3 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.084 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 33.1 W/kg

SAR(1 g) = 8.42 W/kg; SAR(10 g) = 2.4 W/kg

Maximum value of SAR (measured) = 20.0 W/kg

Certificate No: D5GHzV2-1095_May13

Page 11 of 16

Reference No.: C130922R01-SF

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 64.341 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 32.9 W/kg

SAR(1 g) = 8.24 W/kg; SAR(10 g) = 2.34 W/kg Maximum value of SAR (measured) = 19.9 W/kg


Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.473 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 32.8 W/kg

SAR(1 g) = 7.86 W/kg; SAR(10 g) = 2.23 W/kg Maximum value of SAR (measured) = 19.2 W/kg

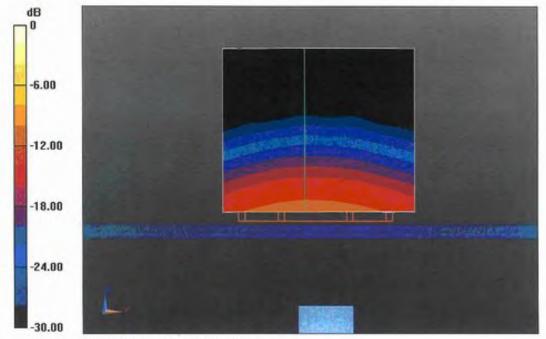

0 dB = 19.2 W/kg = 12.83 dBW/kg


Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Impedance Measurement Plot for Head TSL

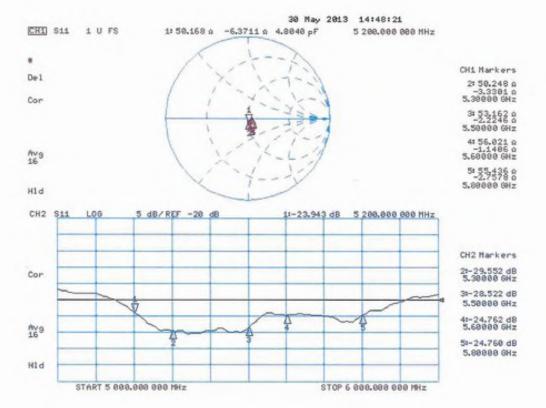

Certificate No: D5GHzV2-1095_May13

Page 13 of 16

Report No: C131230S02-SF Reference No.: C130922R01-SF Date of Issue : January 8, 2014

DASY5 Validation Report for Body TSL

Date: 31.05.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500

MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used: f = 5200 MHz; $\sigma = 5.41 \text{ S/m}$; $\varepsilon_r = 49.6$; $\rho = 1000 \text{ kg/m}^3$, Medium parameters used: f = 5300 MHz; $\sigma = 5.53$ S/m; $\varepsilon_r = 49.4$; $\rho = 1000$ kg/m³, Medium parameters used: f = 5500 MHz; $\sigma =$ 5.8 S/m; $\varepsilon_r = 49.1$; $\rho = 1000 \text{ kg/m}^3$, Medium parameters used: f = 5600 MHz; $\sigma = 5.8 \text{ S/m}$; $\varepsilon_r = 49$; $\rho = 1000 \text{ mHz}$ kg/m³, Medium parameters used: f = 5800 MHz; $\sigma = 6.24 \text{ S/m}$; $\varepsilon_r = 48.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(4.91, 4.91, 4.91); Calibrated: 28.12.2012, ConvF(4.67, 4.67, 4.67); Calibrated: 28.12.2012, ConvF(4.43, 4.43, 4.43); Calibrated: 28.12.2012, ConvF(4.22, 4.22, 4.22); Calibrated: 28.12.2012, ConvF(4.38, 4.38, 4.38); Calibrated: 28.12.2012;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.6(1115); SEMCAD X 14.6.9(7117)

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.744 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 29.0 W/kg

SAR(1 g) = 7.44 W/kg; SAR(10 g) = 2.08 W/kg

Maximum value of SAR (measured) = 17.0 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.871 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 30.4 W/kg

SAR(1 g) = 7.58 W/kg; SAR(10 g) = 2.12 W/kg

Maximum value of SAR (measured) = 17.5 W/kg

Dipole Calibration for Body Tissuc/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.666 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 33.6 W/kg

SAR(1 g) = 7.89 W/kg; SAR(10 g) = 2.19 W/kg

Maximum value of SAR (measured) = 18.7 W/kg

Certificate No: D5GHzV2-1095 May13

Page 14 of 16

Reference No.: C130922R01-SF

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.108 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 34.2 W/kg

SAR(1 g) = 7.76 W/kg; SAR(10 g) = 2.15 W/kg

Maximum value of SAR (measured) = 18.5 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan,


dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 55.451 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 34.6 W/kg

SAR(1 g) = 7.47 W/kg; SAR(10 g) = 2.06 W/kg


Maximum value of SAR (measured) = 18.2 W/kg

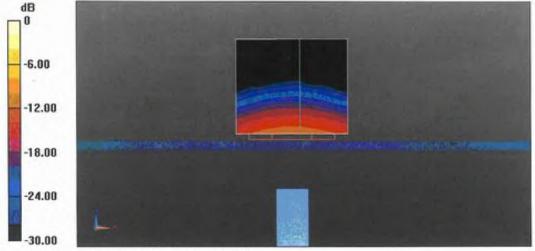

0 dB = 18.2 W/kg = 12.60 dBW/kg

Reference No.: C130922R01-SF

Impedance Measurement Plot for Body TSL

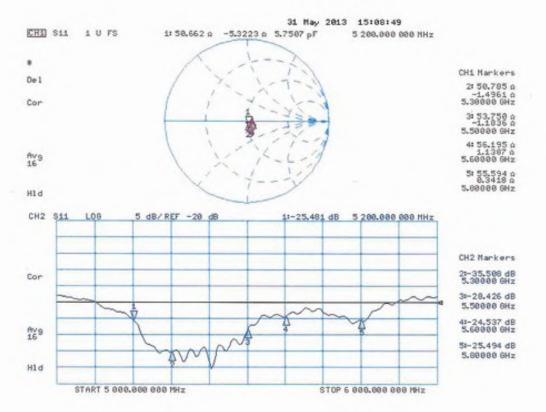

Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Schmid & Partner Engineering AG

s p e a q

Zeughausstrasse 43, 9004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

1245

IMPORTANT NOTICE

USAGE OF THE DAE 4

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

Battery Exchange: The battery cover of the DAE4 unit is closed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.

Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.

E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

Important Note:

Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.

Important Note:

Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the Estop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.

Important Note:

To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.

Schmid & Partner Engineering

TN_BR040315AD DAE4.doc

11.12.2009

Compliance Certification Services Inc.

Reference No.: C130922R01-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kallbrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Accreditation No.: SCS 108

Certificate No: DAE4-1245 Jul 13

C

CALIBRATION CERTIFICATE DAE4 - SD 000 D04 BM - SN: 1245 Object QA CAL-06.v26 Calibration procedure(s) Calibration procedure for the data acquisition electronics (DAE) July 25, 2013 Calibration date: This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (\$1). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) ID # Cal Date (Certificate No.) Scheduled Calibration Primary Standards Keithley Multimeter Type 2001 SN: 0810278 02-Oct-12 (No:12728) Oct-13 Check Date (in house) Scheduled Check Secondary Standards SE UWS 053 AA 1001 07-Jan-13 (in house check) In house check: Jan-14 Auto DAE Calibration Unit Calibrator Box V2.1 SE UMS 008 AA 1002 07-Jan-13 (in house check) In house check: Jan-14 Function Signature Name Dominique Steffen Technician Calibrated by: Approved by: Fin Bomholt Deputy Technical Manager Issued: July 25, 2013 This calibration cartificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: DAE4-1245_Jul13

Page 1 of 5

Compliance Certification Services Inc.

Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with Inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-1245_Jul13

Page 2 of 5

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range:

1LSB =

6.1µV.

full range = -100...+300 mV full range = -1......+3mV

Low Range:

1LSB =

61nV,

DASY measurement parameters; Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	Z
High Range	405.940 ± 0.02% (k=2)	404.664 ± 0.02% (k=2)	405.801 ± 0.02% (k=2)
Low Range	4.00386 ± 1.50% (k=2)	3.98278 ± 1.50% (k=2)	4.02487 ± 1.50% (k=2)

Connector Angle

nector Angle to be used in DASY system	30.5°±1°	
nector Angle to be used in DASY system	30.5)°±1°

Certificate No: DAE4-1245 Jul 13

Page 3 of 5

Appendix

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	199992.97	-4.47	-0.00
Channel X + Input	20001.91	0.89	0.00
Channel X - Input	-19999.11	1.66	-0.01
Channel Y + Input	199994.30	-3.32	-0.00
Channel Y + Input	20001.64	0.75	0.00
Channel Y - Input	-20000.51	0.28	-0.00
Channel Z + Input	199995.90	-1.30	-0.00
Channel Z + Input	20000.30	-0.60	-0.00
Channel Z - Input	-19999.90	0.89	-0.00

Low Range	Reading (µV)	Difference (μV)	Error (%)
Channel X + Input	2001.51	0.38	0.02
Channel X + Input	201.72	0.21	0.11
Channel X - Input	-198.76	-0.28	0.14
Channel Y + Input	2000.72	-0.41	-0.02
Channel Y + Input	199.98	-1.50	-0.74
Channel Y - Input	-198.85	-0.28	0.14
Channel Z + Input	2000.21	-0.84	-0.04
Channel Z + Input	200.77	-0.56	-0.28
Channel Z - Input	-199.95	-1.29	0.65

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec: Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-8.24	-10.01
	- 200	10.27	8.63
Channel Y	200	-7.32	-7.74
	- 200	6.53	6.34
Channel Z	200	-5.94	-6.42
	- 200	5.13	4.65

3. Channel separation

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (μV)
Channel X	200	-	4.16	-2.61
Channel Y	200	8.79	-	3.99
Channel Z	200	9.96	7.22	-

Certificate No: DAE4-1245_Jul13

Page 4 of 5

Peference No : C130022P01-SE

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15874	16183
Channel Y	16451	15694
Channel Z	15932	15717

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MO

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)	
Channel X	0.94	-0.24	2.04	0.48	
Channel Y	-0.42	-1.91	0.54	0.47	
Channel Z	-0.83	-2.62	0.57	0.60	

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)		
Channel X	200	200		
Channel Y	200	200		
Channel Z	200	200		

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)	
Supply (+ Vcc)	+0.01	+6	+14	
Supply (- Vcc)	-0.01	-8	-9	

Certificate No: DAE4-1245_Jul13

Page 5 of 5



FCCID: 2ABCS-A6102

Date of Issue : January 8, 2014

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Accreditation No.: SCS 108

Certificate No. EX3-3798_Jul13

CALIBRATION CERTIFICATE

Object

EX3DV4 - SN:3798

Calibration procedure(s)

QA CAL-01.v8, QA CAL-14.v3, QA CAL-23.v4, QA CAL-25.v4

Calibration procedure for dosimetric E-field probes

Calibration date:

July 26, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)*C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	04-Apr-13 (No. 217-01733)	Apr-14
Power sensor E4412A	MY41498087	94-Apr-13 (No. 217-01733)	Apr-14
Reference 3 dB Attenuator	SN: S5054 (3c)	04-Apr-13 (No. 217-01737)	Apr-14
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-13 (No. 217-01735)	Apr-14
Reference 30 dB Attenuator	SN: S5129 (30b)	04-Apr-13 (No. 217-01738)	Apr-14
Reference Probe ES3DV2	SN: 3013	28-Dec-12 (No. ES3-3013_Dec12)	Dec-13
DAE4	SN: 680	31-Jan-13 (No. DAE4-660_Jan13)	Jan-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 864BC	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-15
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-12)	In house check: Oct-13

Name Function Calibrated by: Dimce lliev Laboratory Technician Approved by: Katja Pokovic Technical Manager

Issued: July 26, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: EX3-3798_Jul13

Page 1 of 11



Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zoughausstrasse 43, 8004 Zurich, Switzerland





C

Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C, D modulation dependent linearization parameters

Polarization φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

 IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

Techniques", December 2003

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz; R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z; A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage scross the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset. The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: EX3-3798 Jul 13

Page 2 of 11

EX3DV4 - SN:3798

July 26, 2013

Probe EX3DV4

SN:3798

Manufactured: April 5, 2011

Calibrated: July 26, 2013

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3798_Jul13

Page 3 of 11

FCCID: 2ABCS-A6102

Date of Issue : January 8, 2014

Reference No.: C130922R01-SF

EX3DV4-SN:3798

July 26, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²) ^A	0.54	0.51	0.59	± 10.1 %
DCP (mV) ⁸	95.9	98.8	98.6	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBõV	С	dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	164.4	±3.0 %
		Y	0.0	0.0	1.0		168.1	
		Z	0.0	0.0	1.0		130.9	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: EX3-3798_Jul13

A The uncertainties of NormX,Y,Z do not affect the E3-field uncertainty inside TSL (see Pages 5 and 6).

<sup>Numerical linearization parameter: uncertainty not required.

Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the</sup>

EX3DV4-SN:3798

July 26, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	41.5	0.90	9.16	9.16	9.16	0.35	0.94	± 12.0 %
900	41.5	0.97	9.01	9.01	9.01	0.35	0.93	± 12.0 %
1810	40.0	1.40	7.79	7.79	7.79	0.73	0.59	± 12.0 %
1900	40.0	1.40	7.73	7.73	7.73	0.68	0.62	± 12.0 %
2000	40.0	1.40	7.73	7.73	7.73	0.80	0.58	± 12.0 %
2450	39.2	1.80	7.08	7.08	7.08	0.66	0.62	± 12.0 %
5200	36.0	4.66	4.85	4.85	4.85	0.37	1.80	± 13.1 %
5300	35.9	4.76	4.71	4.71	4.71	0.38	1.80	± 13.1 %
5500	35.6	4.96	4.76	4.76	4.76	0.36	1.80	± 13.1 %
5600	35.5	5.07	4.51	4.51	4.51	0.42	1.80	± 13.1 %
5800	35.3	5.27	4.48	4.48	4.48	0.40	1.80	± 13.1 %

Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS

Certificate No: EX3-3798_Jul13

of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

At frequencies below 3 GHz, the validity of tissue parameters (c and c) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and c) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and c) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

EX3DV4-SN:3798

July 26, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	55.2	0.97	9.27	9.27	9.27	0.49	0.84	± 12.0 %
900	55.0	1.05	9.11	9.11	9.11	0.80	0.62	± 12.0 %
1810	53.3	1.52	7.45	7.45	7.45	0.37	88.0	± 12.0 %
1900	53.3	1.52	7.32	7.32	7.32	0.37	0.86	± 12.0 %
2000	53.3	1.52	7.54	7.54	7.54	0.29	1.01	± 12.0 %
2450	52.7	1.95	7.08	7.08	7.08	0.80	0.57	± 12.0 %
5200	49.0	5.30	4.38	4.38	4.38	0.41	1.90	± 13.1 %
5300	48.9	5.42	4.22	4.22	4.22	0.41	1.90	± 13.1 %
5500	48.6	5.65	3.93	3.93	3.93	0.46	1.90	± 13.1 %
5600	48.5	5.77	3.92	3.92	3.92	0.38	1.90	± 13.1 %
5800	48.2	6.00	4.24	4.24	4.24	0.46	1.90	± 13.1 %

Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS.

Certificate No: EX3-3798_Jul13

of the ConvF uncertainty at calibration frequency and the uncertainty for the hidicated frequency band.

At frequencies below 3 GHz, the validity of tissue parameters (c and c) can be relaxed to ± 10% if iguid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and c) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Report No: C131230S02-SF

FCCID: 2ABCS-A6102


Date of Issue :January 8, 2014

Reference No.: C130922R01-SF

EX3DV4-SN:3798

July 26, 2013

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

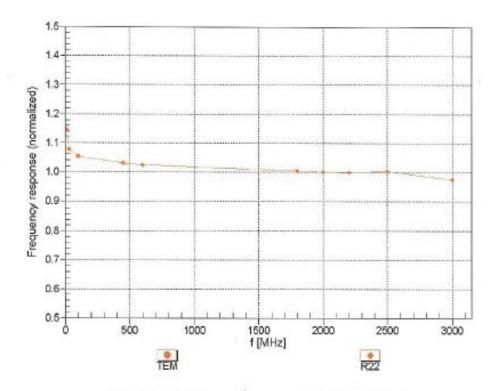

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: EX3-3798_Jul13

Page 7 of 11

Report No: C131230S02-SF

FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014


Reference No.: C130922R01-SF

EX3DV4-SN:3798


July 26, 2013


Receiving Pattern (φ), 9 = 0°

f=600 MHz,TEM



f=1800 MHz,R22



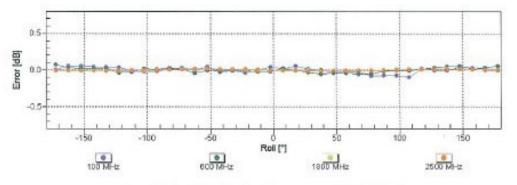

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3798_Jul13


Page 8 of 11


Reference No.: C130922R01-SF

EX3DV4-SN:3798

July 26, 2013

Dynamic Range f(SAR_{head}) (TEM cell, f = 900 MHz)

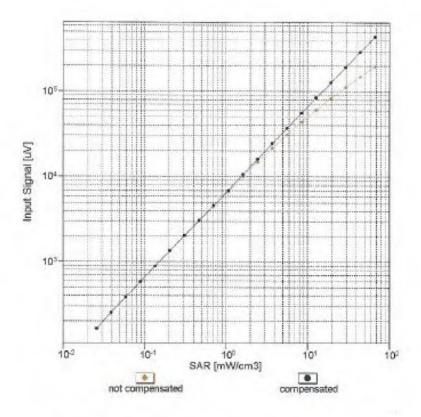

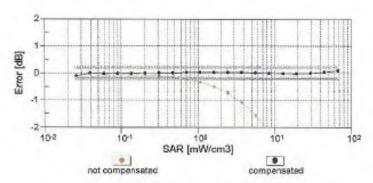

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: EX3-3798_Jul13

Page 9 of 11


FCCID: 2ABCS-A6102

Date of Issue :January 8, 2014


Reference No.: C130922R01-SF


EX3DV4-SN:3798 July 26, 2013

Conversion Factor Assessment

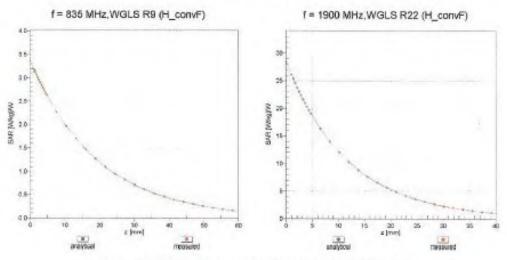

Deviation from Isotropy in Liquid Error (6, 8), f = 900 MHz

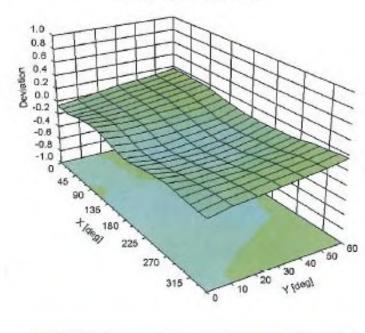



Certificate No: EX3-3798_Jul13

Page 10 of 11

EX3DV4-SN:3798

July 26, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-42,4
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

Certificate No: EX3-3798_Jul13

Page 11 of 11

Reference No.: C130922R01-SF

Date of Issue :January 8, 2014

APPENDIX C: PLOTS OF SAR TEST RESULT

The plots are showing in the file named Appendix C Plots of SAR Test Result

END REPORT