Channel 11

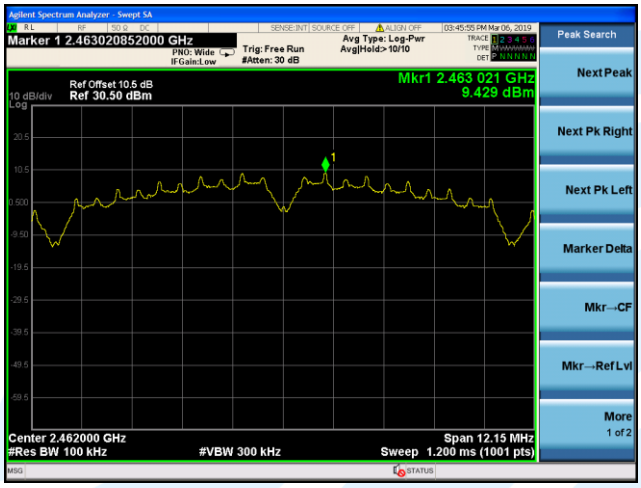
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.463020852000 GHz
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Mkr1 2.463 021 GHz
9.429 dBm
Center 2.462000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 12.15 MHz
Sweep 1.200 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

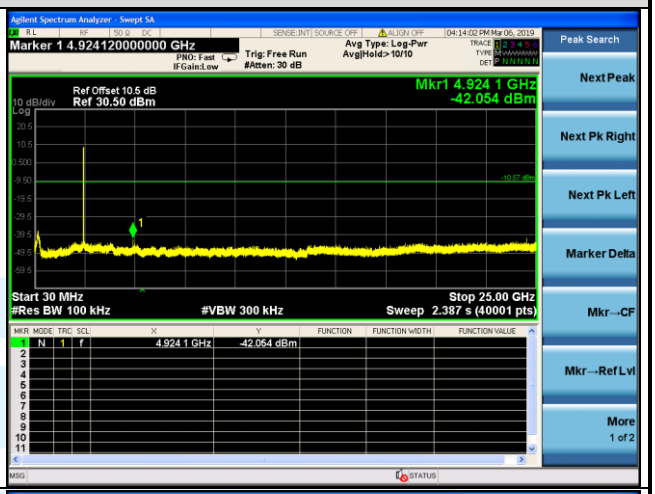
Agilent Spectrum Analyzer - Swept SA
Marker 1 4.924120000000 GHz
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Mkr1 4.924 1 GHz
-42.054 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 2.483 500 GHz
-46.294 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
Normal
Delta
Fixed
Off
Properties
More
1 of 2

Channel 12

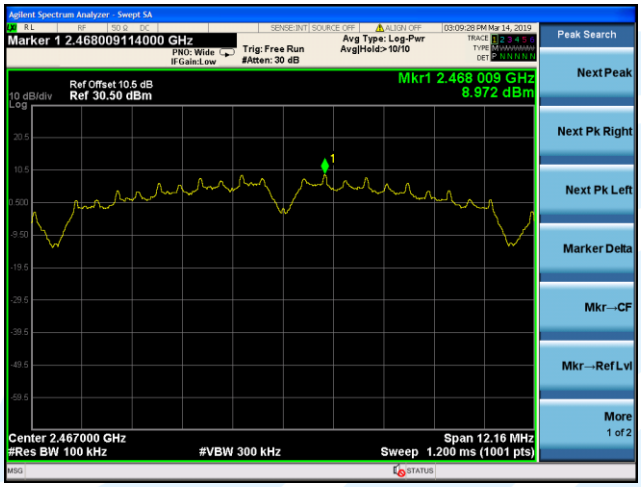
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.468009114000 GHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
03:09:28 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Log
Mkr1 2.468 009 GHz
8.972 dBm
Center 2.467000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 12.16 MHz
Sweep 1.200 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

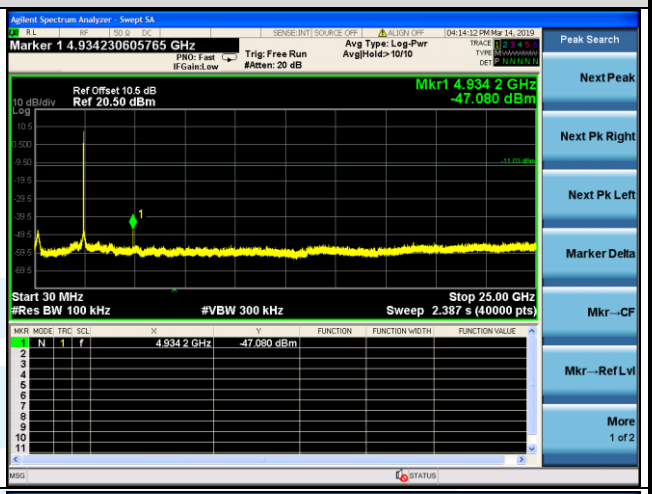
Agilent Spectrum Analyzer - Swept SA
Marker 1 4.934230605765 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
04:14:12 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 4.934 2 GHz
-47.080 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40000 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
04:15:22 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 2.483 500 GHz
-44.841 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
1
Normal
Delta
Fixed
Off
Properties
More
1 of 2

Channel 13

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.473008616000 GHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
03:10:43 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Log
Mkr1 2.473 009 GHz
5.543 dBm
Center 2.472000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 12.15 MHz
Sweep 1.200 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

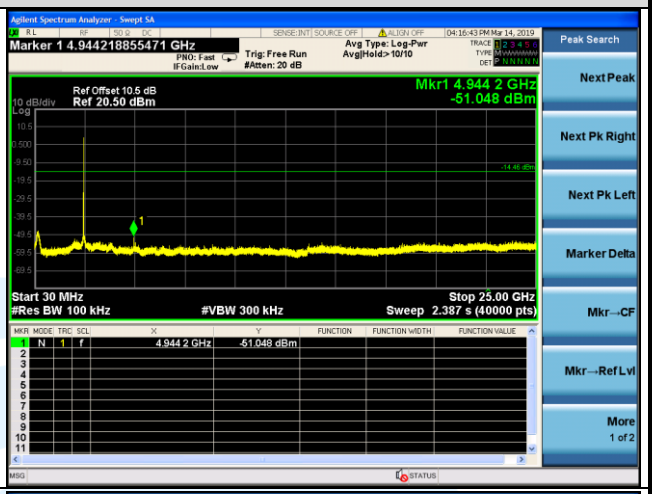
Agilent Spectrum Analyzer - Swept SA
Marker 1 4.944218855471 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
04:16:43 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 4.944 2 GHz
-51.048 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40000 pts)
1 N 1 f 4.944 2 GHz -51.048 dBm
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

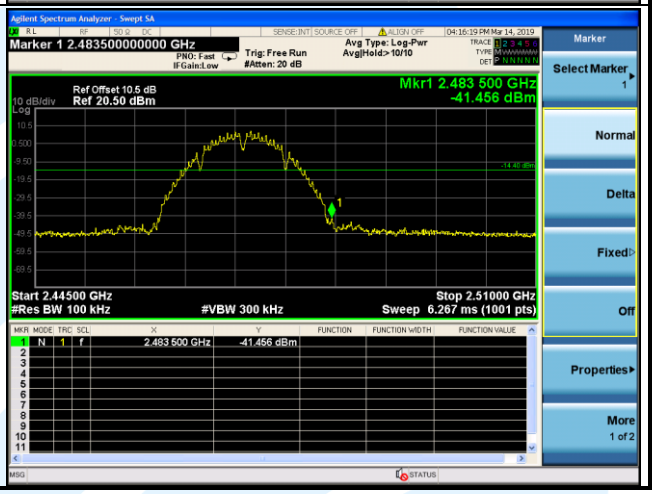
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
04:16:19 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 2.483 500 GHz
-41.456 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
1 N 1 f 2.483 500 GHz -41.456 dBm
Marker
Select Marker
1
Normal
Delta
Fixed
Off
Properties
More
1 of 2

IEEE 802.11g	
In-Band Reference Level	**Out of Band Emission**
Channel 1	
	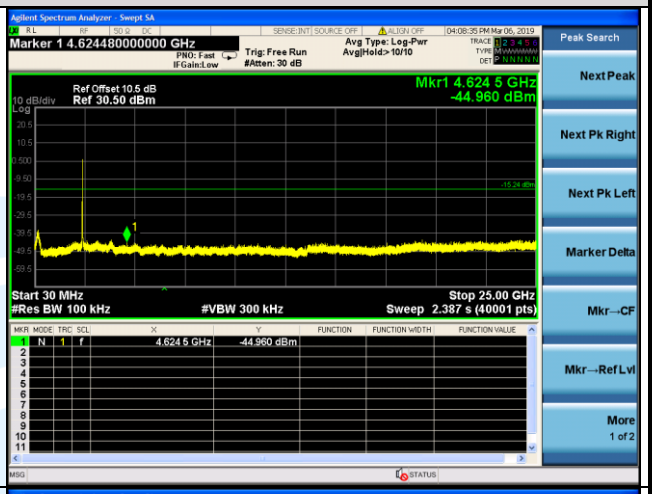 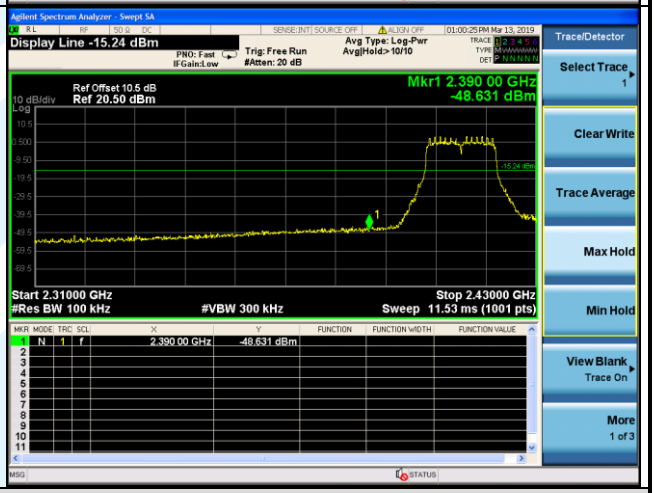
Channel 6	
	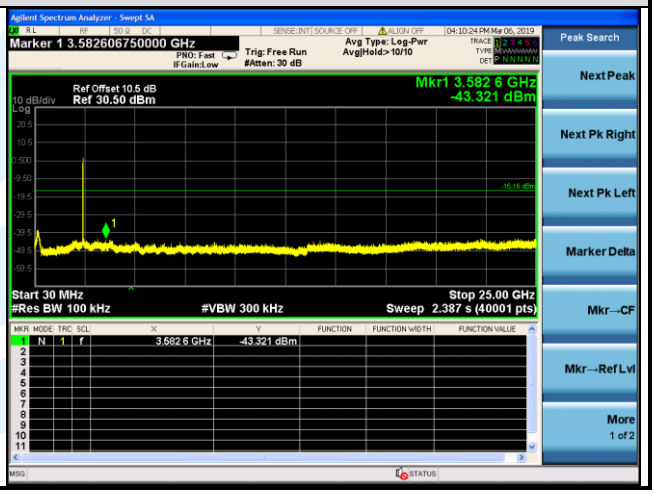

Channel 11

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.463284660000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:> 10/10
03:49:39 PM Mar 06, 2019
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Log
Mkr1 2.463 285 GHz
3.376 dBm
Center 2.46200 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 23.79 MHz
Sweep 2.333 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

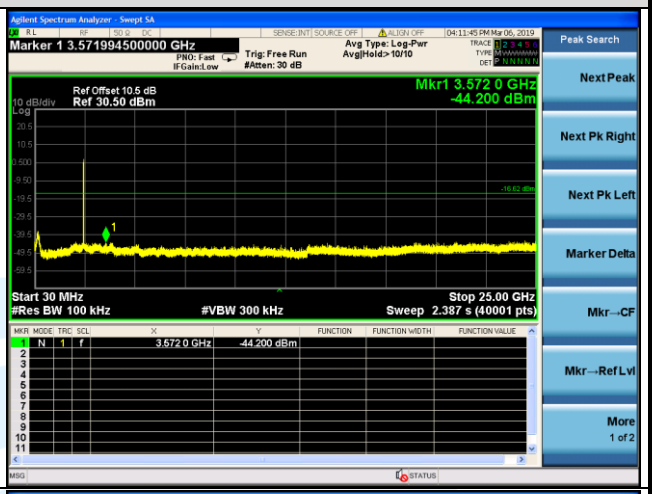
Agilent Spectrum Analyzer - Swept SA
Marker 1 3.571994500000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:> 10/10
04:11:45 PM Mar 06, 2019
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Log
Mkr1 3.572 0 GHz
-44.200 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:> 10/10
01:04:56 PM Mar 13, 2019
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 2.483 500 GHz
-44.941 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
1
Normal
Delta
Fixed
Off
Properties
More
1 of 2

Channel 12

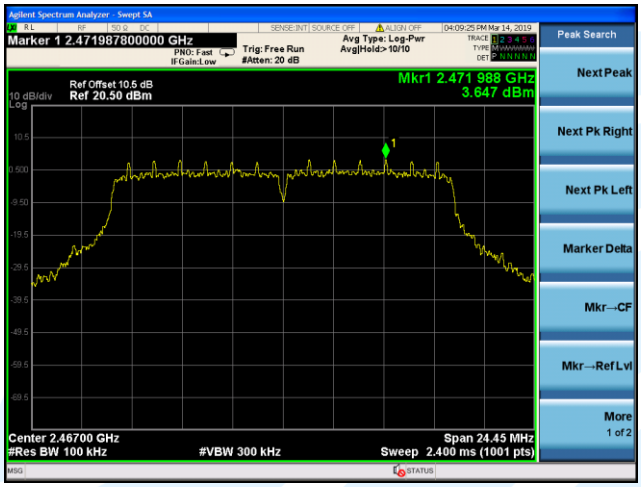
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.471987800000 GHz
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 2.471 988 GHz
3.647 dBm
Center 2.46700 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 24.45 MHz
Sweep 2.400 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

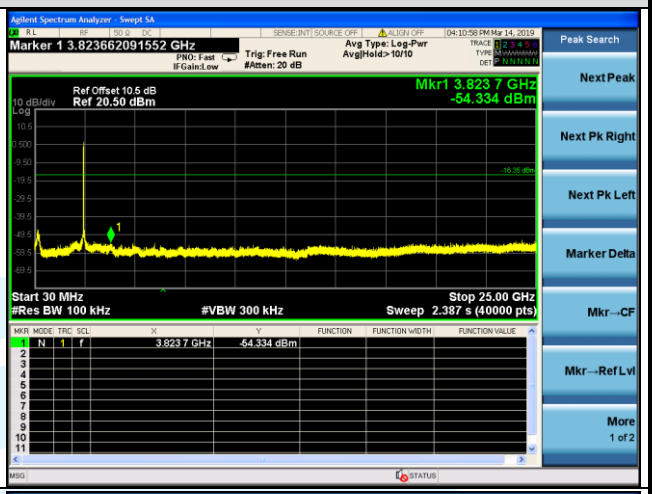
Agilent Spectrum Analyzer - Swept SA
Marker 1 3.823662091552 GHz
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 3.823 7 GHz
-54.334 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40000 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

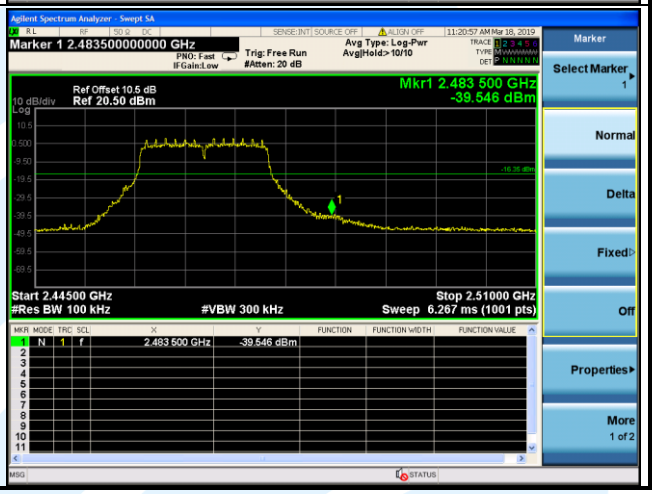
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 2.483 500 GHz
-39.546 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
Normal
Delta
Fixed
Off
Properties
More
1 of 2

Channel 13

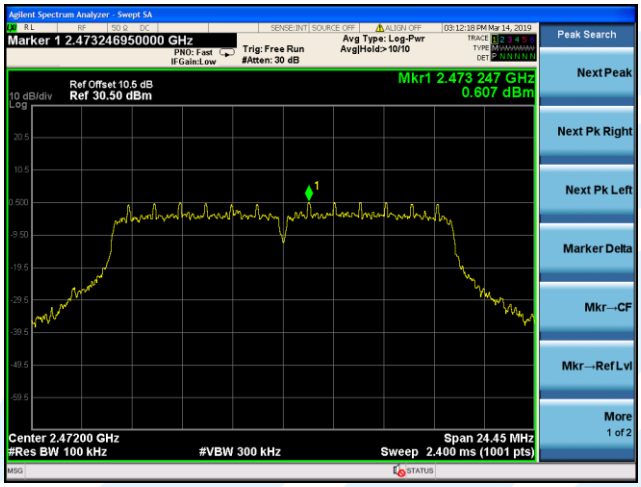
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.473246950000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
03:12:18 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Log
Mkr1 2.473 247 GHz
0.607 dBm
Center 2.47200 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 24.45 MHz
Sweep 2.400 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

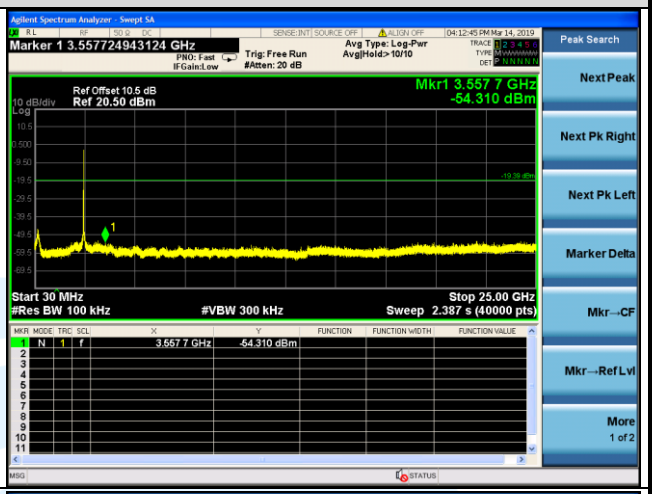
Agilent Spectrum Analyzer - Swept SA
Marker 1 3.557724943124 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
04:12:45 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 3.557 7 GHz
-54.310 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40000 pts)
3.557 7 GHz
-54.310 dBm
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

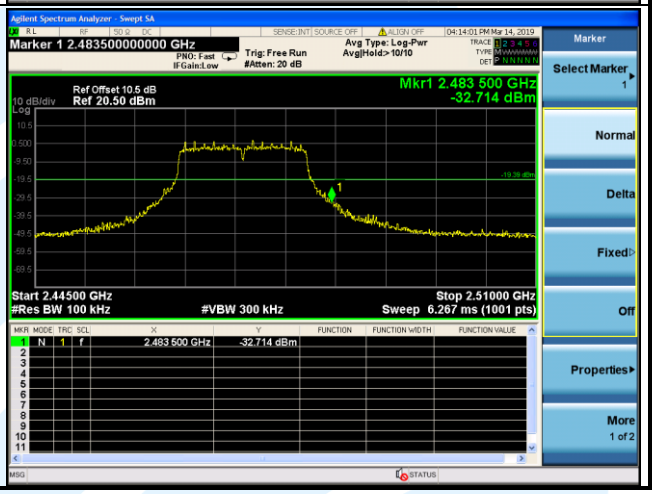
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
04:14:01 PM Mar 14, 2019
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 2.483 500 GHz
-32.714 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
2.483 500 GHz
-32.714 dBm
Marker
Select Marker
1
Normal
Delta
Fixed
Off
Properties
More
1 of 2

IEEE 802.11n-HT20	
In-Band Reference Level	**Out of Band Emission**
Channel 1	
	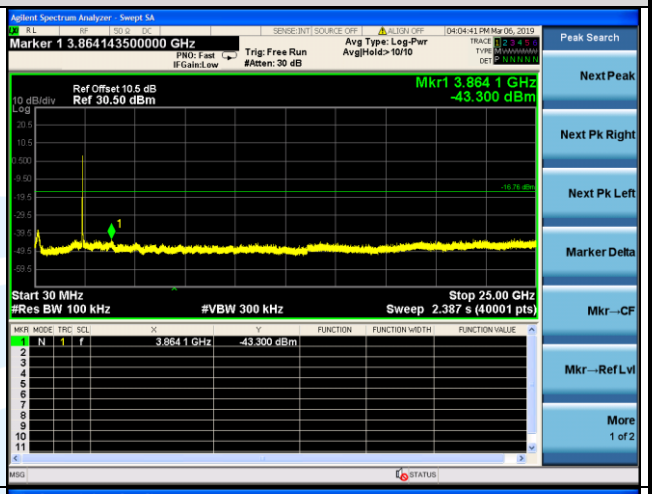 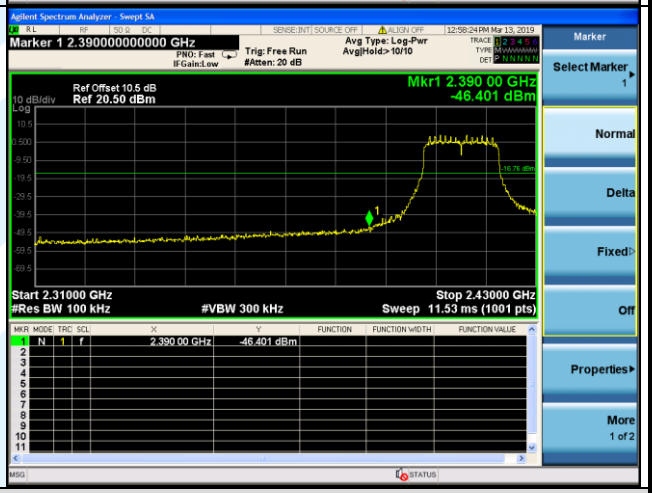
Channel 6	
	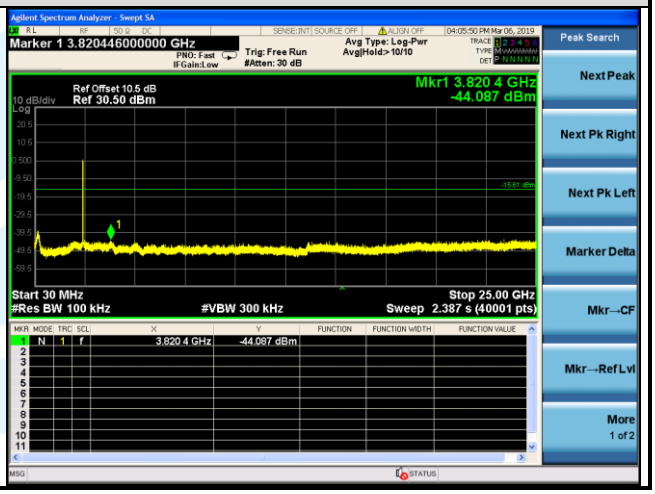

Channel 11

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.467049765000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:> 10/10
03:53:30 PM Mar 06, 2019
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Log
Mkr1 2.467 050 GHz
4.013 dBm
Center 2.46200 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 24.40 MHz
Sweep 2.333 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

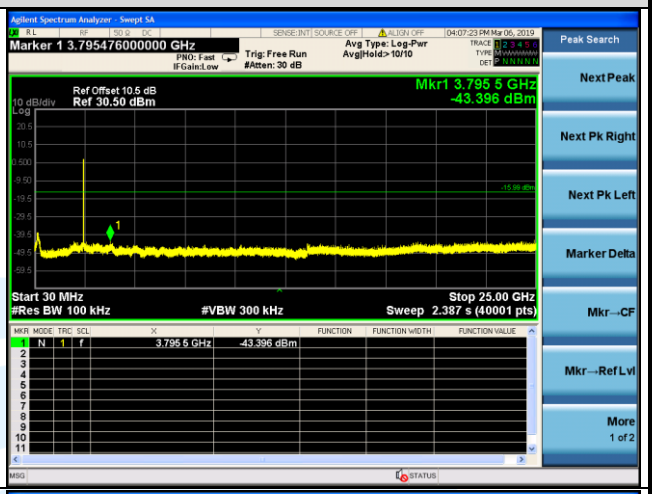
Agilent Spectrum Analyzer - Swept SA
Marker 1 3.795476000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:> 10/10
04:07:23 PM Mar 06, 2019
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Log
Mkr1 3.795 5 GHz
-43.396 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40001 pts)
3.795 5 GHz
-43.396 dBm
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

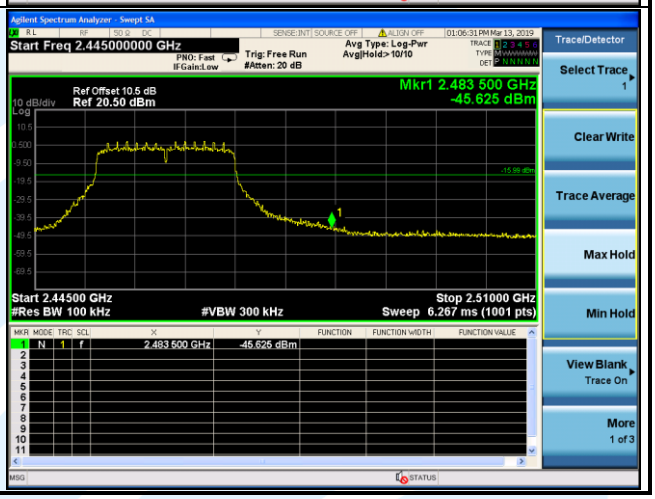
Agilent Spectrum Analyzer - Swept SA
Start Freq 2.445000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:> 10/10
01:06:31 PM Mar 13, 2019
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 2.483 500 GHz
-45.625 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
2.483 500 GHz
-45.625 dBm
Trace/Detector
Select Trace
1
Clear Write
Trace Average
Max Hold
Min Hold
View Blank
Trace On
More
1 of 3

Channel 12

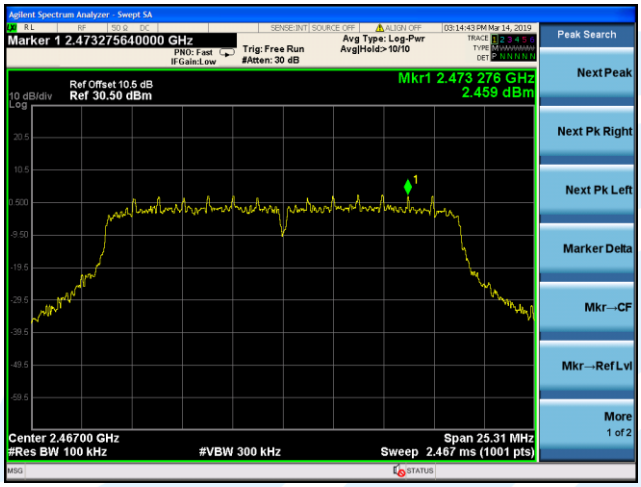
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.473275640000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Mkr1 2.473 276 GHz
2.459 dBm
Center 2.46700 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 25.31 MHz
Sweep 2.467 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

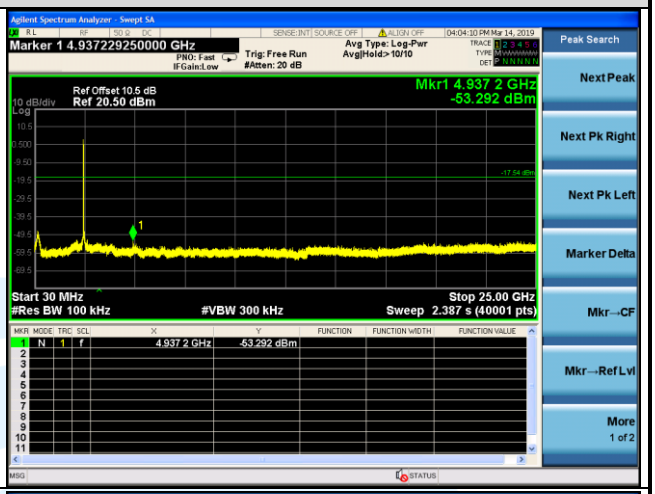
Agilent Spectrum Analyzer - Swept SA
Marker 1 4.937229250000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 4.937 2 GHz
-53.292 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 2.483 500 GHz
-39.322 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
Normal
Delta
Fixed
Off
Properties
More
1 of 2

Channel 13

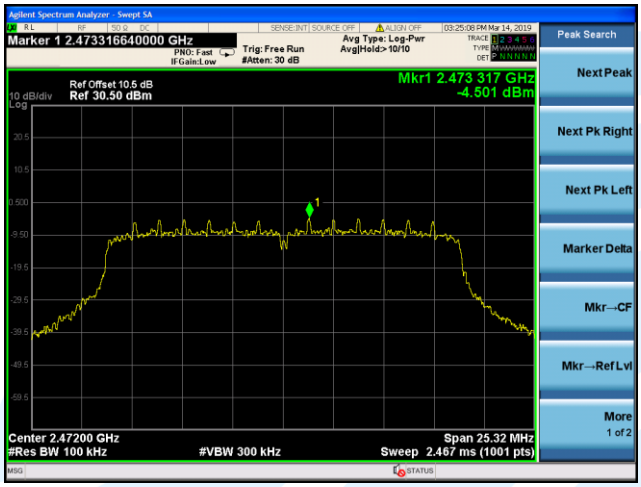
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.473316640000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Mkr1 2.473 317 GHz
-4.501 dBm
Center 2.47200 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 25.32 MHz
Sweep 2.467 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

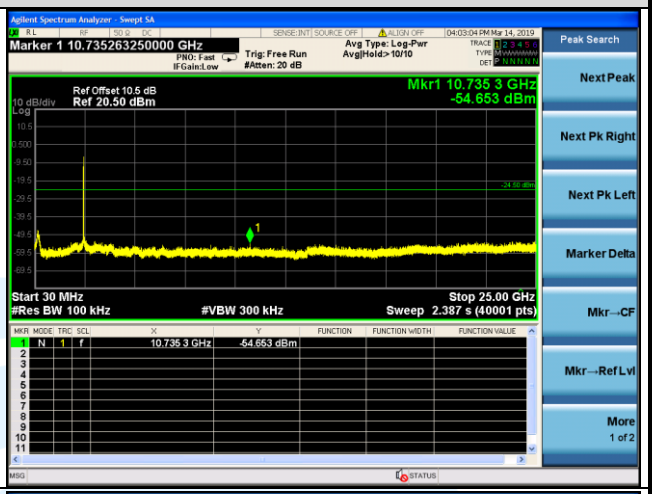
Agilent Spectrum Analyzer - Swept SA
Marker 1 10.735263250000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 10.735 3 GHz
-54.653 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

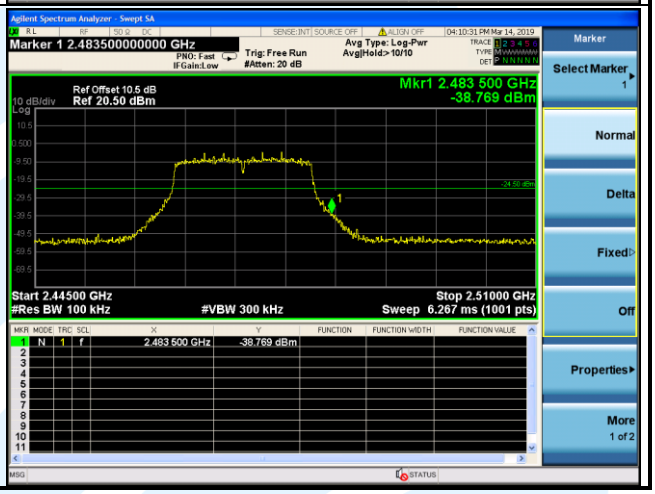
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 2.483 500 GHz
-38.769 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
Normal
Delta
Fixed
Off
Properties
More
1 of 2

IEEE 802.11n-HT40	
In-Band Reference Level	**Out of Band Emission**
Channel 3	
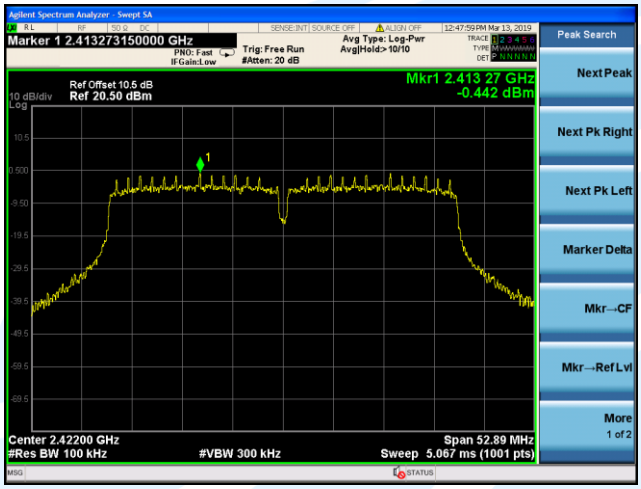	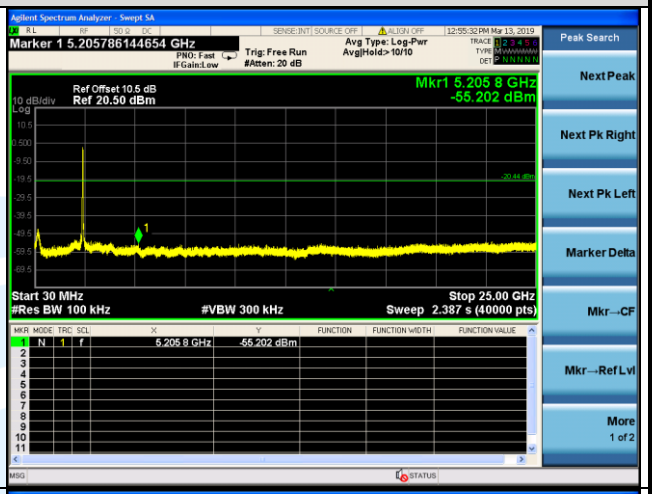
Channel 6	
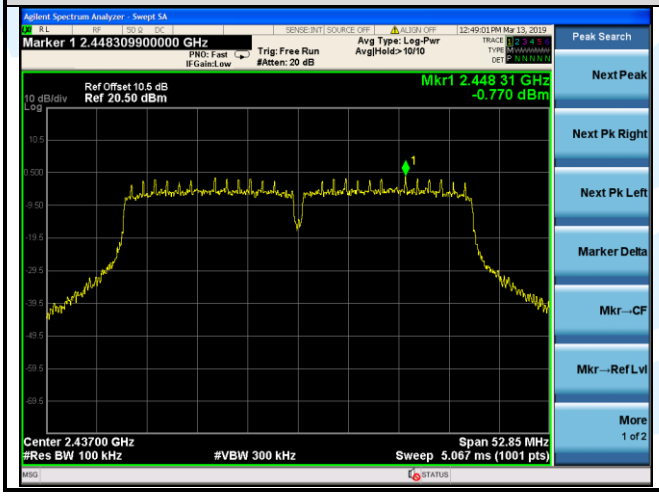	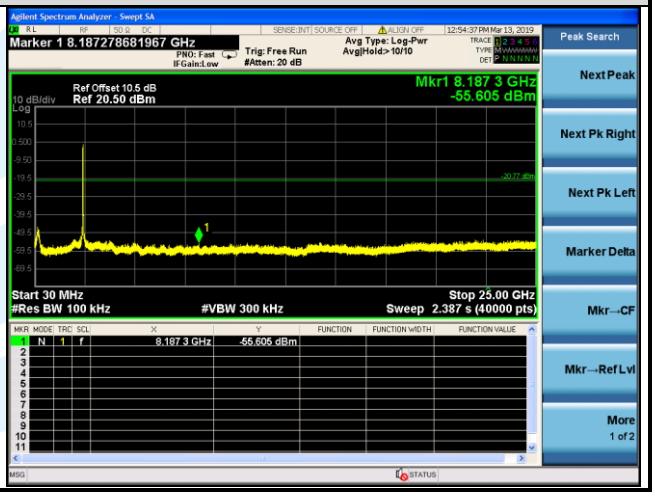

Channel 9

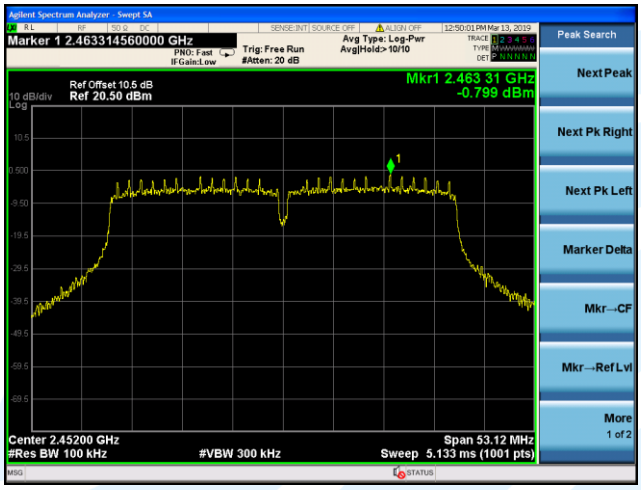
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.463314560000 GHz
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 2.463 31 GHz
-0.799 dBm
Center 2.45200 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 53.12 MHz
Sweep 5.133 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

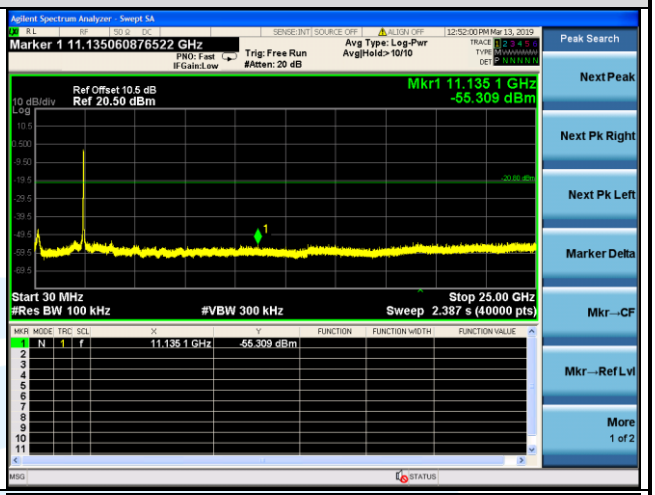
Agilent Spectrum Analyzer - Swept SA
Marker 1 11.135060876522 GHz
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 11.135 1 GHz
-55.309 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40000 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 2.483 500 GHz
-41.733 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
Normal
Delta
Fixed
Off
Properties
More
1 of 2

Channel 10

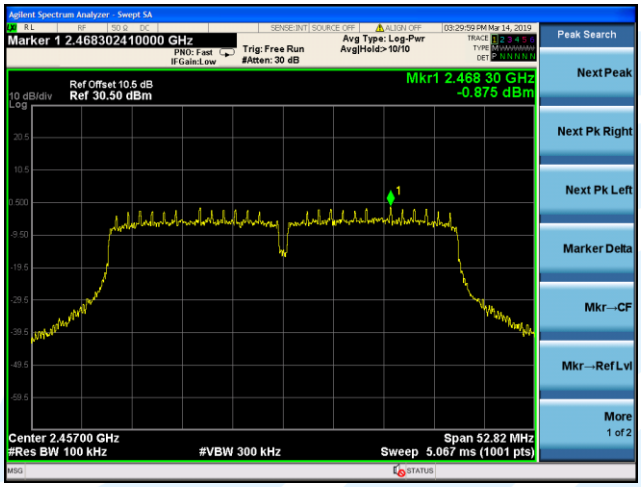
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.468302410000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Mkr1 2.468 30 GHz
-0.875 dBm
Center 2.45700 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 52.82 MHz
Sweep 5.067 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

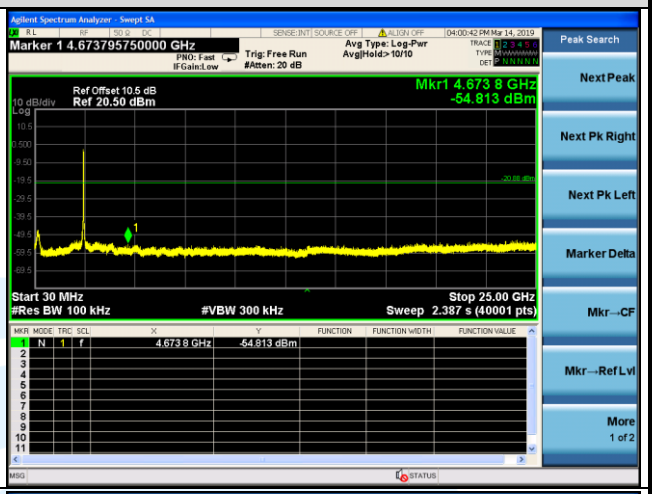
Agilent Spectrum Analyzer - Swept SA
Marker 1 4.673795750000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 4.673 8 GHz
-54.813 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Mkr1 2.483 500 GHz
-42.768 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
Normal
Delta
Fixed
Off
Properties
More
1 of 2

Channel 11

Agilent Spectrum Analyzer - Swept SA
Marker 1 2.473315250000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 30.50 dBm
Log
Mkr1 2.473 32 GHz
-7.547 dBm
Center 2.46200 GHz
#Res BW 100 kHz
#VBW 300 kHz
Span 52.88 MHz
Sweep 5.067 ms (1001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

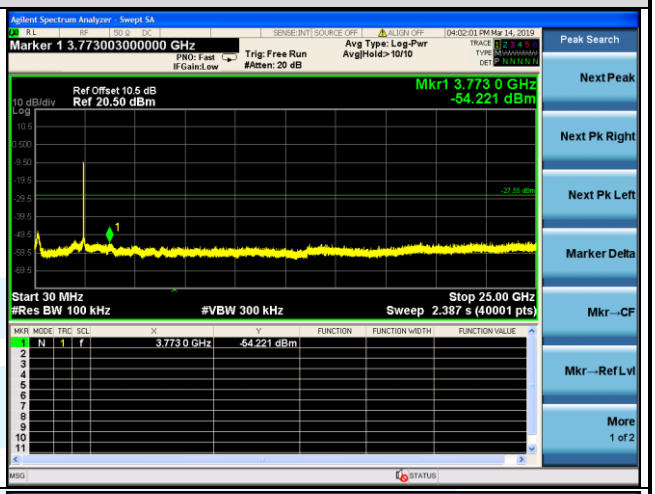
Agilent Spectrum Analyzer - Swept SA
Marker 1 3.773003000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 3.773 0 GHz
-54.221 dBm
Start 30 MHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.00 GHz
Sweep 2.387 s (40001 pts)
Peak Search
Next Peak
Next Pk Right
Next Pk Left
Marker Delta
Mkr→CF
Mkr→Ref Lvl
More
1 of 2

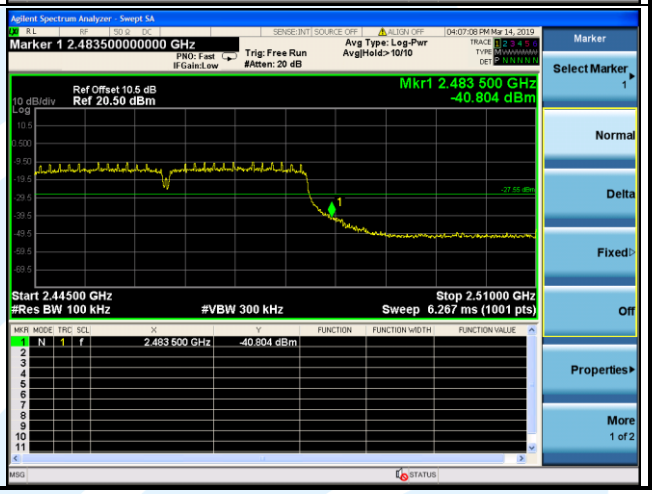
Agilent Spectrum Analyzer - Swept SA
Marker 1 2.483500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: Log-Pwr
Avg|Hold:>10/10
Ref Offset 10.5 dB
10 dB/div Ref 20.50 dBm
Log
Mkr1 2.483 500 GHz
-40.804 dBm
Start 2.44500 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 2.51000 GHz
Sweep 6.267 ms (1001 pts)
Marker
Select Marker
1
Normal
Delta
Fixed
Off
Properties
More
1 of 2

SISO_ Chain 1_ IEEE 802.11b	
In-Band Reference Level	**Out of Band Emission**
Channel 1	
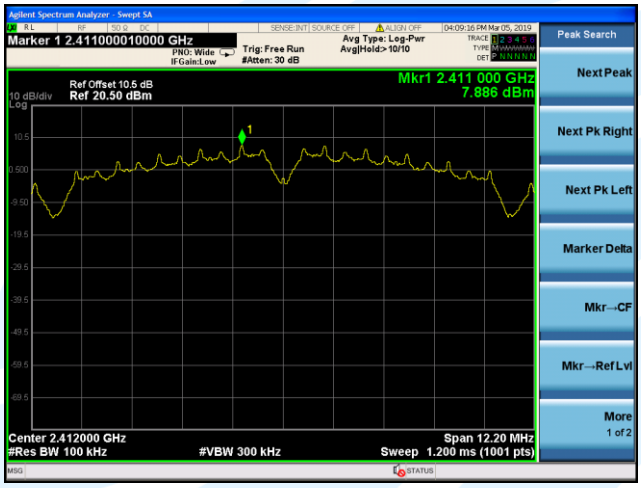	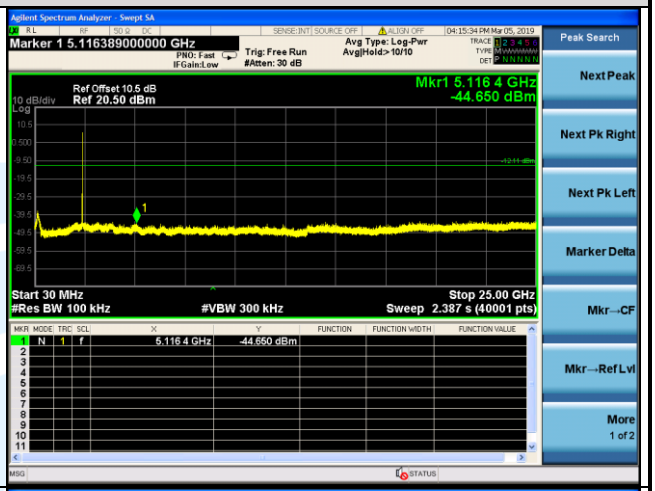 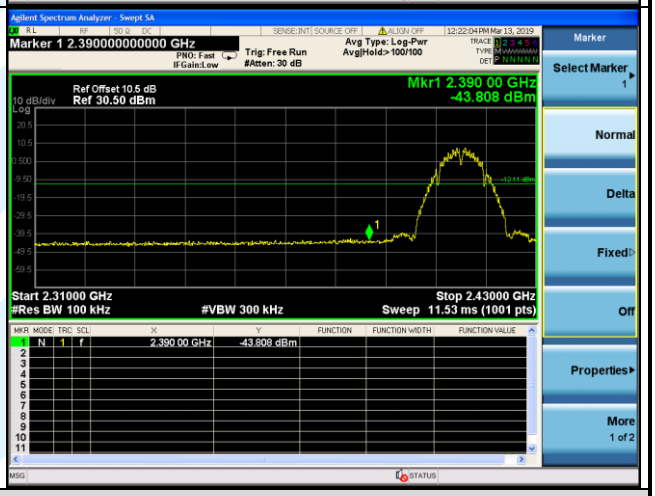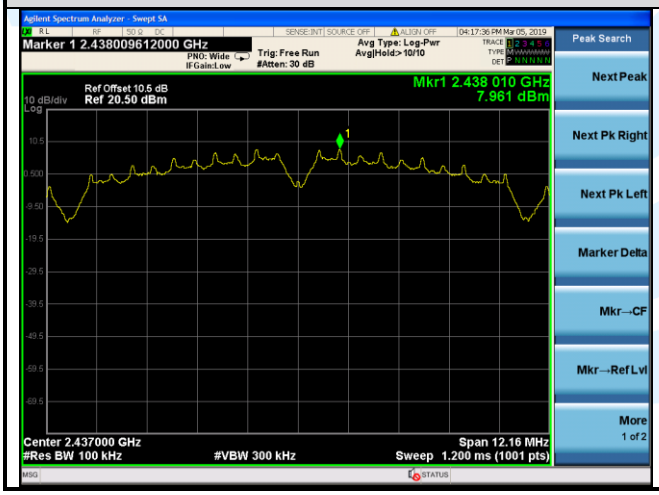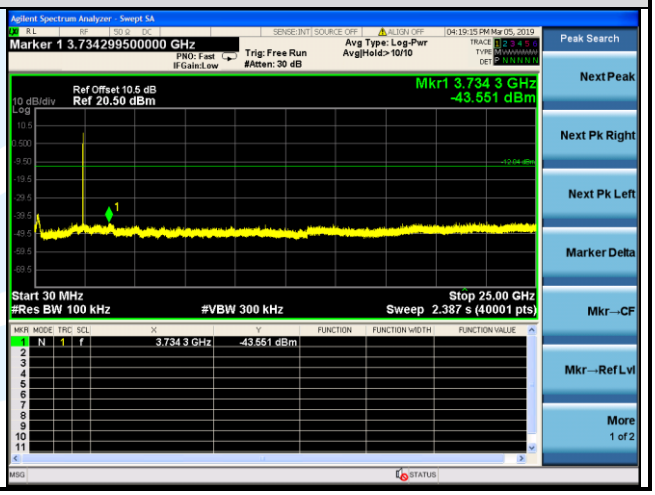
Channel 6