

## ANNEX F System Validation

The SAR system must be validated against its performance specifications before it is deployed. When SAR probes, system components or software are changed, upgraded or recalibrated, these must be validated with the SAR system(s) that operates with such components.

**Table F.1: System Validation for 3846**

| Probe SN. | Liquid name  | Validation date | Frequency point | Status (OK or Not) |
|-----------|--------------|-----------------|-----------------|--------------------|
| 3846      | Head 750MHz  | July 20,2024    | 750MHz          | OK                 |
| 3846      | Head 900MHz  | July 20,2024    | 900MHz          | OK                 |
| 3846      | Head 1450MHz | July 20,2024    | 1450MHz         | OK                 |
| 3846      | Head 1750MHz | July 20,2024    | 1750MHz         | OK                 |
| 3846      | Head 1900MHz | July 20,2024    | 1900MHz         | OK                 |
| 3846      | Head 2100MHz | July 21,2024    | 2100MHz         | OK                 |
| 3846      | Head 2300MHz | July 21,2024    | 2300MHz         | OK                 |
| 3846      | Head 2450MHz | July 21,2024    | 2450MHz         | OK                 |
| 3846      | Head 2600MHz | July 21,2024    | 2600MHz         | OK                 |
| 3846      | Head 3300MHz | July 22,2024    | 3300MHz         | OK                 |
| 3846      | Head 3500MHz | July 22,2024    | 3500MHz         | OK                 |
| 3846      | Head 3700MHz | July 22,2024    | 3700MHz         | OK                 |
| 3846      | Head 3900MHz | July 22,2024    | 3900MHz         | OK                 |
| 3846      | Head 4100MHz | July 22,2024    | 4100MHz         | OK                 |
| 3846      | Head 4200MHz | July 22,2024    | 4200MHz         | OK                 |
| 3846      | Head 4400MHz | July 22,2024    | 4400MHz         | OK                 |
| 3846      | Head 4600MHz | July 22,2024    | 4600MHz         | OK                 |
| 3846      | Head 4800MHz | July 22,2024    | 4800MHz         | OK                 |
| 3846      | Head 4950MHz | July 22,2024    | 4950MHz         | OK                 |
| 3846      | Head 5250MHz | July 23,2024    | 5250MHz         | OK                 |
| 3846      | Head 5600MHz | July 23,2024    | 5600MHz         | OK                 |
| 3846      | Head 5750MHz | July 23,2024    | 5750MHz         | OK                 |

**Table F.1: System Validation for 7673**

| Probe SN. | Liquid name  | Validation date | Frequency point | Status (OK or Not) |
|-----------|--------------|-----------------|-----------------|--------------------|
| 7673      | Head 750MHz  | July.30,2024    | 750 MHz         | OK                 |
| 7673      | Head 900MHz  | July.30,2024    | 900 MHz         | OK                 |
| 7673      | Head 1750MHz | July.30,2024    | 1750 MHz        | OK                 |
| 7673      | Head 1900MHz | July.30,2024    | 1900 MHz        | OK                 |
| 7673      | Head 2000MHz | July.30,2024    | 2000 MHz        | OK                 |
| 7673      | Head 2300MHz | July.30,2024    | 2300 MHz        | OK                 |
| 7673      | Head 2450MHz | July.30,2024    | 2450 MHz        | OK                 |
| 7673      | Head 2600MHz | July.30,2024    | 2600 MHz        | OK                 |
| 7673      | Head 3500MHz | July.30,2024    | 3500 MHz        | OK                 |
| 7673      | Head 3700MHz | July.30,2024    | 3700 MHz        | OK                 |
| 7673      | Head 5250MHz | July.30,2024    | 5250 MHz        | OK                 |
| 7673      | Head 5600MHz | July.30,2024    | 5600 MHz        | OK                 |
| 7673      | Head 5750MHz | July.30,2024    | 5750 MHz        | OK                 |



No. 24T04Z102293-001

## ANNEX G Probe Calibration Certificate

### Probe 3846 Calibration Certificate



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn http://www.caict.ac.cn



中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L0570

Client **CTTL**Certificate No: **24J02Z000266**

#### CALIBRATION CERTIFICATE

Object **EX3DV4 - SN : 3846**Calibration Procedure(s) **FF-Z11-004-02  
Calibration Procedures for Dosimetric E-field Probes**Calibration date: **June 19, 2024**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards        | ID #               | Cal Date(Calibrated by, Certificate No.)  | Scheduled Calibration |
|--------------------------|--------------------|-------------------------------------------|-----------------------|
| Power Meter NRP2         | 106277             | 19-Oct-23(CTTL, No.J23X11026)             | Oct-24                |
| Power sensor NRP8S       | 104291             | 19-Oct-23(CTTL, No.J23X11026)             | Oct-24                |
| Power sensor NRP8S       | 104292             | 19-Oct-23(CTTL, No.J23X11026)             | Oct-24                |
| Reference 10dBAttenuator | 18N50W-10dB        | 19-Jan-23(CTTL, No.J23X00212)             | Jan-25                |
| Reference 20dBAttenuator | 18N50W-20dB        | 19-Jan-23(CTTL, No.J23X00211)             | Jan-25                |
| Reference Probe EX3DV4   | SN 7464            | 22-Jan-24(SPEAG, No.EX-7464_Jan24)        | Jan-25                |
| DAE4                     | SN 1555            | 24-Aug-23(SPEAG, No.DAE4-1555_Aug23)      | Aug-24                |
| Secondary Standards      | ID #               | Cal Date(Calibrated by, Certificate No.)  | Scheduled Calibration |
| SignalGenerator MG3700A  | 6201052605         | 12-Jun-24(CTTL, No.24J02X005419)          | Jun-25                |
| SignalGenerator APSIN26G | 181-33A6D0700-1959 | 26-Mar-24(CTTL, No.24J02X002468)          | Mar-25                |
| Network Analyzer E5071C  | MY46110673         | 25-Dec-23(CTTL, No.J23X13425)             | Dec-24                |
| Reference 10dBAttenuator | BT0520             | 11-May-23(CTTL, No.J23X04061)             | May-25                |
| Reference 20dBAttenuator | BT0267             | 11-May-23(CTTL, No.J23X04062)             | May-25                |
| OCP DAK-12               | SN 1174            | 25-Oct-23(SPEAG, No.OCP-DAK12-1174_Oct23) | Oct-24                |


|                | Name        | Function           | Signature |
|----------------|-------------|--------------------|-----------|
| Calibrated by: | Yu Zongying | SAR Test Engineer  |           |
| Reviewed by:   | Lin Jun     | SAR Test Engineer  |           |
| Approved by:   | Qi Dianyuan | SAR Project Leader |           |

Issued: June 30, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: 24J02Z000266

Page 1 of 9



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

### Glossary:

|                       |                                                                                                                                             |
|-----------------------|---------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                   | tissue simulating liquid                                                                                                                    |
| NORM <sub>x,y,z</sub> | sensitivity in free space                                                                                                                   |
| ConvF                 | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                  |
| DCP                   | diode compression point                                                                                                                     |
| CF                    | crest factor (1/duty_cycle) of the RF signal                                                                                                |
| A,B,C,D               | modulation dependent linearization parameters                                                                                               |
| Polarization $\Phi$   | $\Phi$ rotation around probe axis                                                                                                           |
| Polarization $\theta$ | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i<br>$\theta=0$ is normal to probe axis |


Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>:** Assessed for E-field polarization  $\theta=0$  ( $f \leq 900\text{MHz}$  in TEM-cell;  $f > 1800\text{MHz}$ : waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>:** DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>:** A,B,C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f > 800\text{MHz}$ ) and inside waveguide using analytical field distributions based on power measurements for  $f > 800\text{MHz}$ . The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50\text{MHz}$  to  $\pm 100\text{MHz}$ .
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle:** The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:3846

### Basic Calibration Parameters

|                                      | Sensor X | Sensor Y | Sensor Z | Unc ( $k=2$ ) |
|--------------------------------------|----------|----------|----------|---------------|
| Norm( $\mu V/(V/m)^2$ ) <sup>A</sup> | 0.39     | 0.47     | 0.48     | $\pm 10.0\%$  |
| DCP(mV) <sup>B</sup>                 | 100.4    | 101.0    | 102.4    |               |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A dB | B dB $\sqrt{\mu V}$ | C   | D dB | VR mV | Unc <sup>E</sup> ( $k=2$ ) |
|-----|---------------------------|---|------|---------------------|-----|------|-------|----------------------------|
| 0   | CW                        | X | 0.0  | 0.0                 | 1.0 | 0.00 | 153.1 | $\pm 2.0\%$                |
|     |                           | Y | 0.0  | 0.0                 | 1.0 |      | 174.2 |                            |
|     |                           | Z | 0.0  | 0.0                 | 1.0 |      | 173.4 |                            |

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X, Y, Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 4).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:3846

### Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 41.9                               | 0.89                            | 9.89    | 9.89    | 9.89    | 0.20               | 1.25                    | ± 12.7%     |
| 900                  | 41.5                               | 0.97                            | 9.38    | 9.38    | 9.38    | 0.15               | 1.49                    | ± 12.7%     |
| 1450                 | 40.5                               | 1.20                            | 8.62    | 8.62    | 8.62    | 0.17               | 1.16                    | ± 12.7%     |
| 1750                 | 40.1                               | 1.37                            | 8.25    | 8.25    | 8.25    | 0.29               | 0.99                    | ± 12.7%     |
| 1900                 | 40.0                               | 1.40                            | 7.95    | 7.95    | 7.95    | 0.28               | 1.10                    | ± 12.7%     |
| 2100                 | 39.8                               | 1.49                            | 7.80    | 7.80    | 7.80    | 0.25               | 1.09                    | ± 12.7%     |
| 2300                 | 39.5                               | 1.67                            | 7.69    | 7.69    | 7.69    | 0.66               | 0.69                    | ± 12.7%     |
| 2450                 | 39.2                               | 1.80                            | 7.43    | 7.43    | 7.43    | 0.66               | 0.70                    | ± 12.7%     |
| 2600                 | 39.0                               | 1.96                            | 7.28    | 7.28    | 7.28    | 0.66               | 0.70                    | ± 12.7%     |
| 3300                 | 38.2                               | 2.71                            | 6.96    | 6.96    | 6.96    | 0.54               | 0.88                    | ± 13.9%     |
| 3500                 | 37.9                               | 2.91                            | 6.81    | 6.81    | 6.81    | 0.44               | 1.05                    | ± 13.9%     |
| 3700                 | 37.7                               | 3.12                            | 6.71    | 6.71    | 6.71    | 0.46               | 1.05                    | ± 13.9%     |
| 3900                 | 37.5                               | 3.32                            | 6.65    | 6.65    | 6.65    | 0.40               | 1.25                    | ± 13.9%     |
| 4100                 | 37.2                               | 3.53                            | 6.57    | 6.57    | 6.57    | 0.35               | 1.30                    | ± 13.9%     |
| 4200                 | 37.1                               | 3.63                            | 6.45    | 6.45    | 6.45    | 0.35               | 1.35                    | ± 13.9%     |
| 4400                 | 36.9                               | 3.84                            | 6.37    | 6.37    | 6.37    | 0.40               | 1.25                    | ± 13.9%     |
| 4600                 | 36.7                               | 4.04                            | 6.33    | 6.33    | 6.33    | 0.45               | 1.27                    | ± 13.9%     |
| 4800                 | 36.4                               | 4.25                            | 6.26    | 6.26    | 6.26    | 0.45               | 1.25                    | ± 13.9%     |
| 4950                 | 36.3                               | 4.40                            | 6.05    | 6.05    | 6.05    | 0.50               | 1.19                    | ± 13.9%     |
| 5250                 | 35.9                               | 4.71                            | 5.45    | 5.45    | 5.45    | 0.45               | 1.40                    | ± 13.9%     |
| 5600                 | 35.5                               | 5.07                            | 4.75    | 4.75    | 4.75    | 0.55               | 1.20                    | ± 13.9%     |
| 5750                 | 35.4                               | 5.22                            | 4.90    | 4.90    | 4.90    | 0.50               | 1.30                    | ± 13.9%     |

<sup>C</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequency up to 6 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.




In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

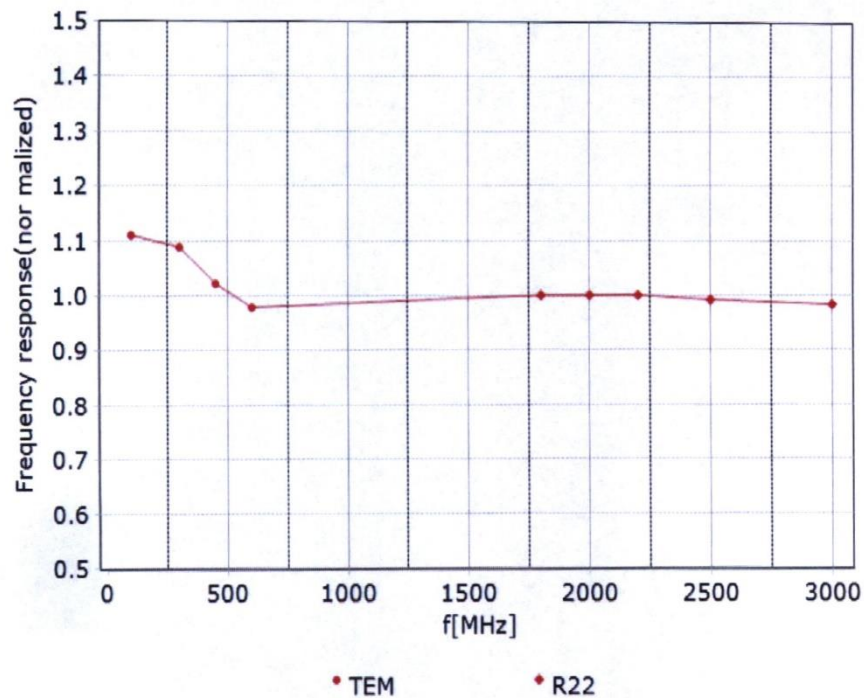

Uncertainty of Frequency Response of E-field:  $\pm 7.4\%$  ( $k=2$ )




In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Receiving Pattern ( $\Phi$ ), $\theta=0^\circ$


**f=600 MHz, TEM**

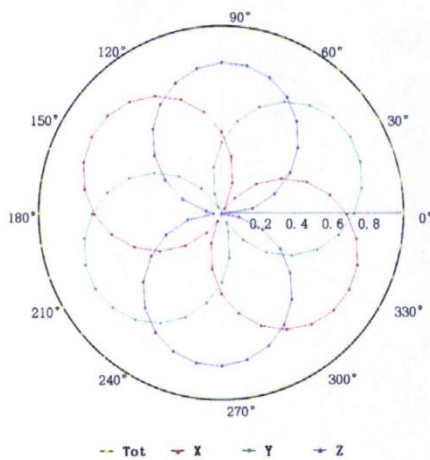

**f=1800 MHz, R22**

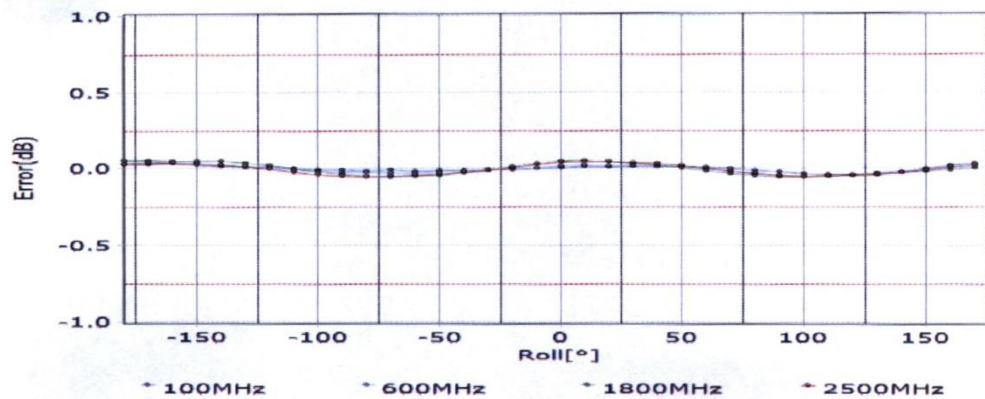
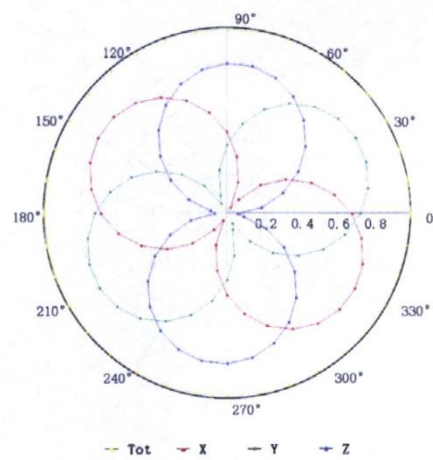


Uncertainty of Axial Isotropy Assessment:  $\pm 1.2\%$  ( $k=2$ )



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Dynamic Range f(SAR<sub>head</sub>) (TEM cell, f = 900 MHz)

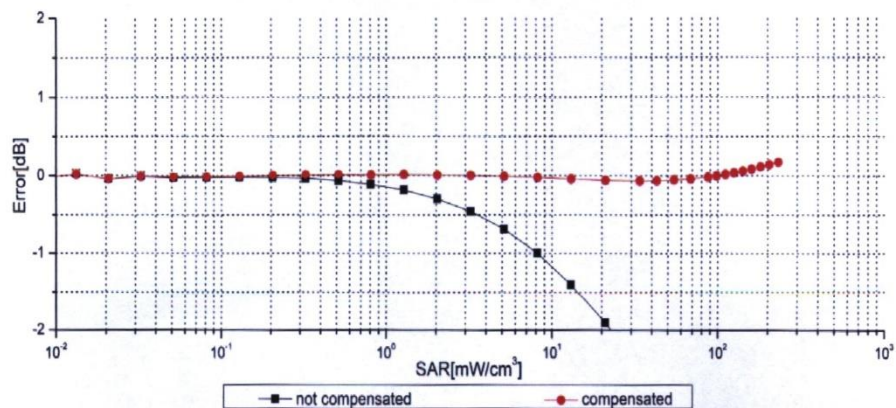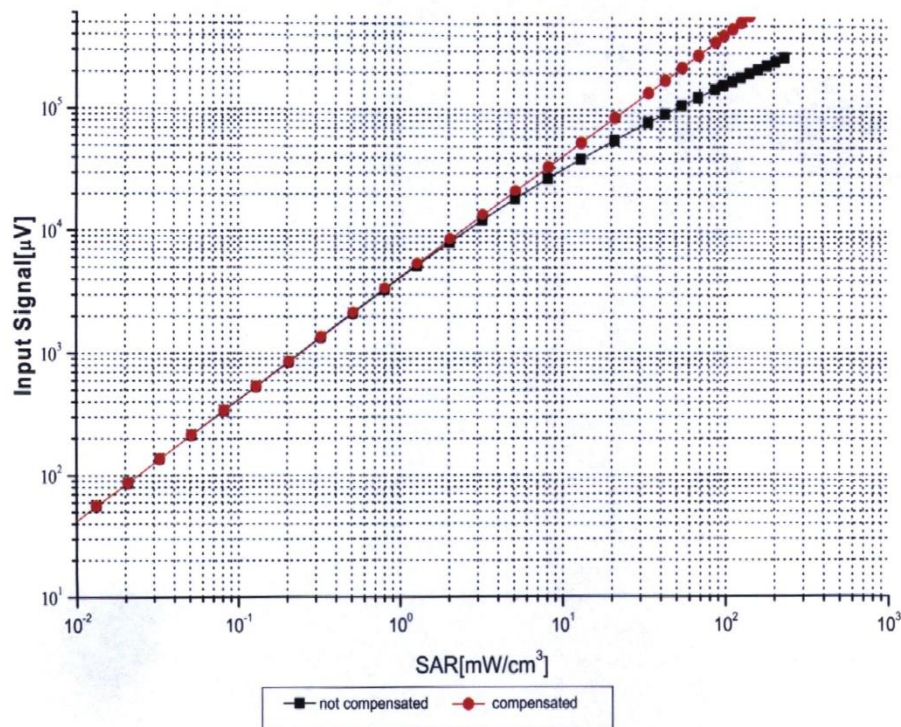

Uncertainty of Linearity Assessment:  $\pm 0.9\%$  ( $k=2$ )

Certificate No:24J02Z000266

Page 7 of 9



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>


## Conversion Factor Assessment

f=750 MHz,WGLS R9(H\_convF)

f=1750 MHz,WGLS R22(H\_convF)

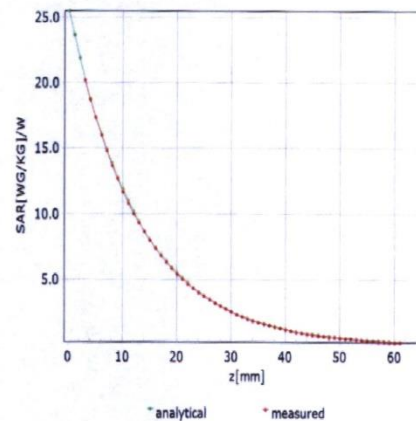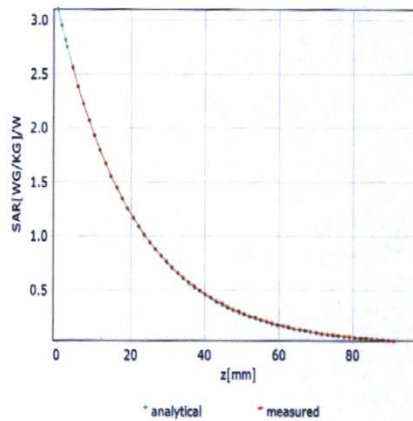

## Deviation from Isotropy in Liquid

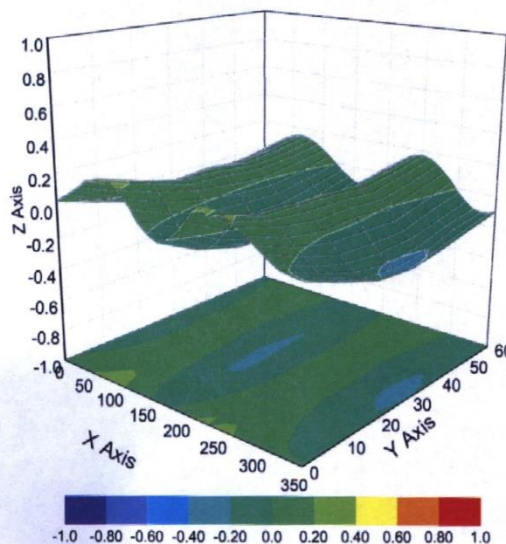

Uncertainty of Spherical Isotropy Assessment:  $\pm 3.2\%$  ( $k=2$ )



No. 24T04Z102293-001



In Collaboration with

**s p e a g**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:3846

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | 16.2       |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disable    |
| Probe Overall Length                          | 337mm      |
| Probe Body Diameter                           | 10mm       |
| Tip Length                                    | 9mm        |
| Tip Diameter                                  | 2.5mm      |
| Probe Tip to Sensor X Calibration Point       | 1mm        |
| Probe Tip to Sensor Y Calibration Point       | 1mm        |
| Probe Tip to Sensor Z Calibration Point       | 1mm        |
| Recommended Measurement Distance from Surface | 1.4mm      |




No. 24T04Z102293-001

## Probe 7673 Calibration Certificate

|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |                                                                       |                                                                                                                                                                        |                                                                                                    |
|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------|
|  In Collaboration with<br><b>s p e a g</b><br>CALIBRATION LABORATORY                                                                                                                                                                                                                                                                                                                                      |                                                                       |   | 中国认可<br>国际互认<br>校准<br>CALIBRATION<br>CNAS L0570                                                    |
| Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China<br>Tel: +86-10-62304633-2117<br>E-mail: emf@caict.ac.cn      http://www.caict.ac.cn                                                                                                                                                                                                                                                                                                                                   |                                                                       |                                                                                                                                                                        |                                                                                                    |
| Client                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     | CTTL                                                                  | Certificate No: 24J02Z000429                                                                                                                                           |                                                                                                    |
| <b>CALIBRATION CERTIFICATE</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                             |                                                                       |                                                                                                                                                                        |                                                                                                    |
| Object                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     | EX3DV4 - SN : 7673                                                    |                                                                                                                                                                        |                                                                                                    |
| Calibration Procedure(s)                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | FF-Z11-004-02<br>Calibration Procedures for Dosimetric E-field Probes |                                                                                                                                                                        |                                                                                                    |
| Calibration date:                                                                                                                                                                                                                                                                                                                                                                                                                                                                          | July 29, 2024                                                         |                                                                                                                                                                        |                                                                                                    |
| <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> |                                                                       |                                                                                                                                                                        |                                                                                                    |
| Primary Standards                                                                                                                                                                                                                                                                                                                                                                                                                                                                          | ID #                                                                  | Cal Date(Calibrated by, Certificate No.)                                                                                                                               | Scheduled Calibration                                                                              |
| Power Meter NRP2                                                                                                                                                                                                                                                                                                                                                                                                                                                                           | 106277                                                                | 19-Oct-23(CTTL, No.J23X11026)                                                                                                                                          | Oct-24                                                                                             |
| Power sensor NRP8S                                                                                                                                                                                                                                                                                                                                                                                                                                                                         | 104291                                                                | 19-Oct-23(CTTL, No.J23X11026)                                                                                                                                          | Oct-24                                                                                             |
| Power sensor NRP8S                                                                                                                                                                                                                                                                                                                                                                                                                                                                         | 104292                                                                | 19-Oct-23(CTTL, No.J23X11026)                                                                                                                                          | Oct-24                                                                                             |
| Reference 10dBAttenuator                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | 18N50W-10dB                                                           | 19-Jan-23(CTTL, No.J23X00212)                                                                                                                                          | Jan-25                                                                                             |
| Reference 20dBAttenuator                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | 18N50W-20dB                                                           | 19-Jan-23(CTTL, No.J23X00211)                                                                                                                                          | Jan-25                                                                                             |
| Reference Probe EX3DV4                                                                                                                                                                                                                                                                                                                                                                                                                                                                     | SN 7307                                                               | 28-May-24(SPEAG, No.EX-7307_May24)                                                                                                                                     | May-25                                                                                             |
| DAE4                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       | SN 1555                                                               | 24-Aug-23(SPEAG, No.DAE4-1555_Aug23)                                                                                                                                   | Aug-24                                                                                             |
| Secondary Standards                                                                                                                                                                                                                                                                                                                                                                                                                                                                        | ID #                                                                  | Cal Date(Calibrated by, Certificate No.)                                                                                                                               | Scheduled Calibration                                                                              |
| SignalGenerator MG3700A                                                                                                                                                                                                                                                                                                                                                                                                                                                                    | 6201052605                                                            | 12-Jun-24(CTTL, No.24J02X005419)                                                                                                                                       | Jun-25                                                                                             |
| SignalGenerator APSIN26G                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | 181-33A6D0700-1959                                                    | 26-Mar-24(CTTL, No.24J02X002468)                                                                                                                                       | Mar-25                                                                                             |
| Network Analyzer E5071C                                                                                                                                                                                                                                                                                                                                                                                                                                                                    | MY46110673                                                            | 25-Dec-23(CTTL, No.J23X13425)                                                                                                                                          | Dec-24                                                                                             |
| Reference 10dBAttenuator                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | BT0520                                                                | 11-May-23(CTTL, No.J23X04061)                                                                                                                                          | May-25                                                                                             |
| Reference 20dBAttenuator                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | BT0267                                                                | 11-May-23(CTTL, No.J23X04062)                                                                                                                                          | May-25                                                                                             |
| OCP DAK-12                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 | SN 1174                                                               | 25-Oct-23(SPEAG, No.OCP-DAK12-1174_Oct23)                                                                                                                              | Oct-24                                                                                             |
| Calibrated by:                                                                                                                                                                                                                                                                                                                                                                                                                                                                             | Name<br>Yu Zongying                                                   | Function<br>SAR Test Engineer                                                                                                                                          | Signature<br> |
| Reviewed by:                                                                                                                                                                                                                                                                                                                                                                                                                                                                               | Name<br>Lin Jun                                                       | Function<br>SAR Test Engineer                                                                                                                                          |                                                                                                    |
| Approved by:                                                                                                                                                                                                                                                                                                                                                                                                                                                                               | Name<br>Qi Dianyuan                                                   | Function<br>SAR Project Leader                                                                                                                                         |                                                                                                    |
| Issued: August 05, 2024                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |                                                                       |                                                                                                                                                                        |                                                                                                    |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.                                                                                                                                                                                                                                                                                                                                                                            |                                                                       |                                                                                                                                                                        |                                                                                                    |

Certificate No: 24J02Z000429

Page 1 of 9



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

### Glossary:

|                       |                                                                                                                                               |
|-----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                   | tissue simulating liquid                                                                                                                      |
| NORM <sub>x,y,z</sub> | sensitivity in free space                                                                                                                     |
| ConvF                 | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                    |
| DCP                   | diode compression point                                                                                                                       |
| CF                    | crest factor (1/duty_cycle) of the RF signal                                                                                                  |
| A,B,C,D               | modulation dependent linearization parameters                                                                                                 |
| Polarization $\Phi$   | $\Phi$ rotation around probe axis                                                                                                             |
| Polarization $\theta$ | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), $i$<br>$\theta=0$ is normal to probe axis |


Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta=0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A,B,C** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn http://www.caict.ac.cn

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:7673

### Basic Calibration Parameters

|                                      | Sensor X | Sensor Y | Sensor Z | Unc ( $k=2$ ) |
|--------------------------------------|----------|----------|----------|---------------|
| Norm( $\mu V/(V/m)^2$ ) <sup>A</sup> | 0.62     | 0.63     | 0.60     | $\pm 10.0\%$  |
| DCP(mV) <sup>B</sup>                 | 109.4    | 111.6    | 108.0    |               |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A<br>dB | B<br>dB $\sqrt{\mu V}$ | C   | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>( $k=2$ ) |
|-----|---------------------------|---|---------|------------------------|-----|---------|----------|-------------------------------|
| 0   | CW                        | X | 0.0     | 0.0                    | 1.0 | 0.00    | 214.8    | $\pm 2.1\%$                   |
|     |                           | Y | 0.0     | 0.0                    | 1.0 |         | 218.1    |                               |
|     |                           | Z | 0.0     | 0.0                    | 1.0 |         | 207.9    |                               |

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X, Y, Z do not affect the  $E^2$ -field uncertainty inside TSL (see Page 4).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:7673

### Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 41.9                               | 0.89                            | 10.45   | 10.45   | 10.45   | 0.23               | 1.09                    | ± 12.7%     |
| 900                  | 41.5                               | 0.97                            | 10.03   | 10.03   | 10.03   | 0.21               | 1.24                    | ± 12.7%     |
| 1450                 | 40.5                               | 1.20                            | 8.74    | 8.74    | 8.74    | 0.18               | 1.04                    | ± 12.7%     |
| 1750                 | 40.1                               | 1.37                            | 8.45    | 8.45    | 8.45    | 0.25               | 1.02                    | ± 12.7%     |
| 1900                 | 40.0                               | 1.40                            | 8.10    | 8.10    | 8.10    | 0.25               | 1.04                    | ± 12.7%     |
| 2000                 | 40.0                               | 1.40                            | 8.15    | 8.15    | 8.15    | 0.26               | 1.05                    | ± 12.7%     |
| 2300                 | 39.5                               | 1.67                            | 7.85    | 7.85    | 7.85    | 0.58               | 0.69                    | ± 12.7%     |
| 2450                 | 39.2                               | 1.80                            | 7.60    | 7.60    | 7.60    | 0.57               | 0.71                    | ± 12.7%     |
| 2600                 | 39.0                               | 1.96                            | 7.44    | 7.44    | 7.44    | 0.64               | 0.67                    | ± 12.7%     |
| 3300                 | 38.2                               | 2.71                            | 6.93    | 6.93    | 6.93    | 0.47               | 0.88                    | ± 13.9%     |
| 3500                 | 37.9                               | 2.91                            | 6.73    | 6.73    | 6.73    | 0.45               | 1.00                    | ± 13.9%     |
| 3700                 | 37.7                               | 3.12                            | 6.48    | 6.48    | 6.48    | 0.35               | 1.20                    | ± 13.9%     |
| 3900                 | 37.5                               | 3.32                            | 6.44    | 6.44    | 6.44    | 0.30               | 1.52                    | ± 13.9%     |
| 4100                 | 37.2                               | 3.53                            | 6.43    | 6.43    | 6.43    | 0.35               | 1.25                    | ± 13.9%     |
| 4200                 | 37.1                               | 3.63                            | 6.33    | 6.33    | 6.33    | 0.30               | 1.52                    | ± 13.9%     |
| 4400                 | 36.9                               | 3.84                            | 6.23    | 6.23    | 6.23    | 0.30               | 1.52                    | ± 13.9%     |
| 4600                 | 36.7                               | 4.04                            | 6.18    | 6.18    | 6.18    | 0.35               | 1.40                    | ± 13.9%     |
| 4800                 | 36.4                               | 4.25                            | 6.07    | 6.07    | 6.07    | 0.35               | 1.55                    | ± 13.9%     |
| 4950                 | 36.3                               | 4.40                            | 5.74    | 5.74    | 5.74    | 0.35               | 1.55                    | ± 13.9%     |
| 5250                 | 35.9                               | 4.71                            | 5.18    | 5.18    | 5.18    | 0.40               | 1.52                    | ± 13.9%     |
| 5600                 | 35.5                               | 5.07                            | 4.60    | 4.60    | 4.60    | 0.40               | 1.52                    | ± 13.9%     |
| 5750                 | 35.4                               | 5.22                            | 4.71    | 4.71    | 4.71    | 0.40               | 1.55                    | ± 13.9%     |


<sup>C</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequency up to 6 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Certificate No:24J02Z000429

Page 4 of 9




Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

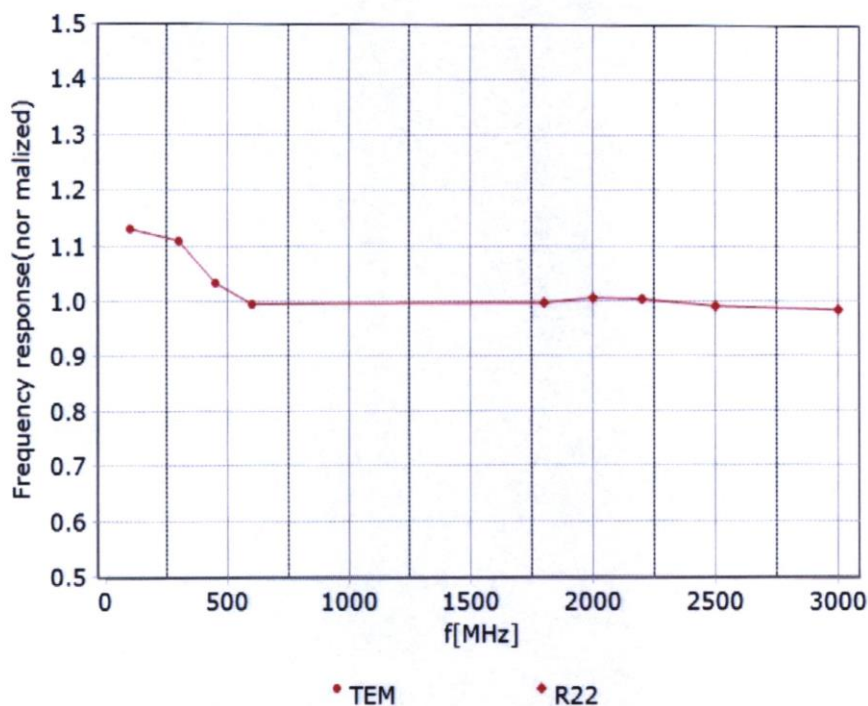

Uncertainty of Frequency Response of E-field:  $\pm 7.4\%$  ( $k=2$ )






Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Receiving Pattern ( $\Phi$ ), $\theta=0^\circ$

**f=600 MHz, TEM**



**f=1800 MHz, R22**

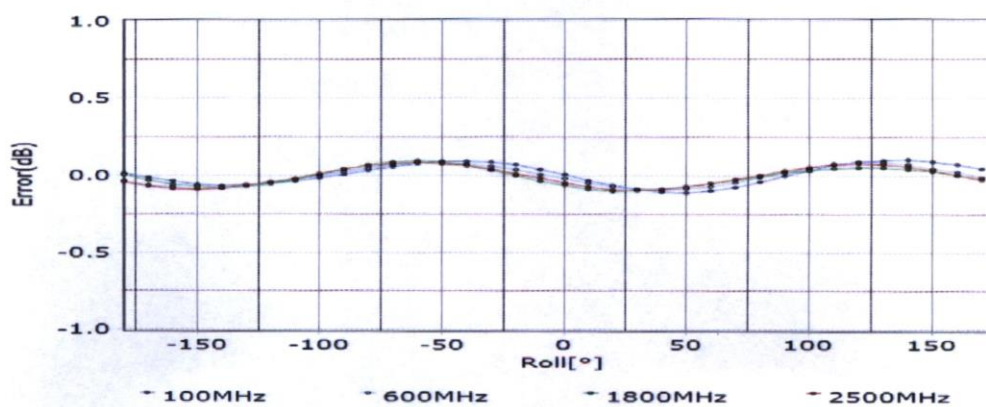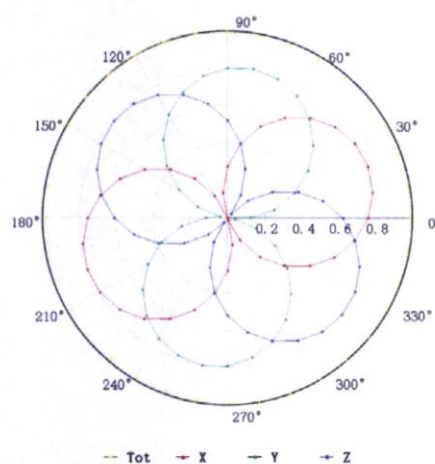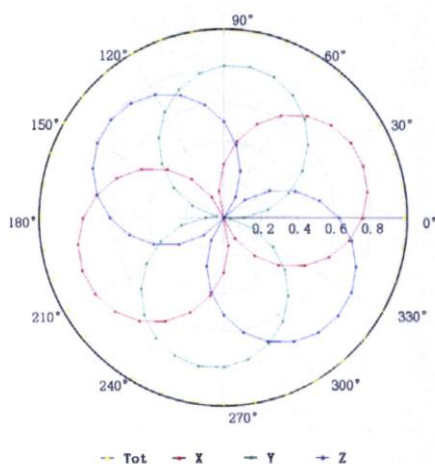


Uncertainty of Axial Isotropy Assessment:  $\pm 1.2\%$  ( $k=2$ )

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Dynamic Range f(SAR<sub>head</sub>) (TEM cell, f = 900 MHz)

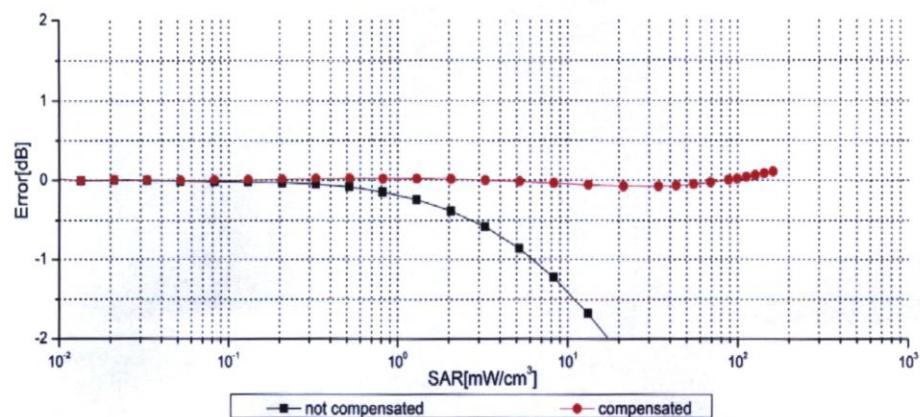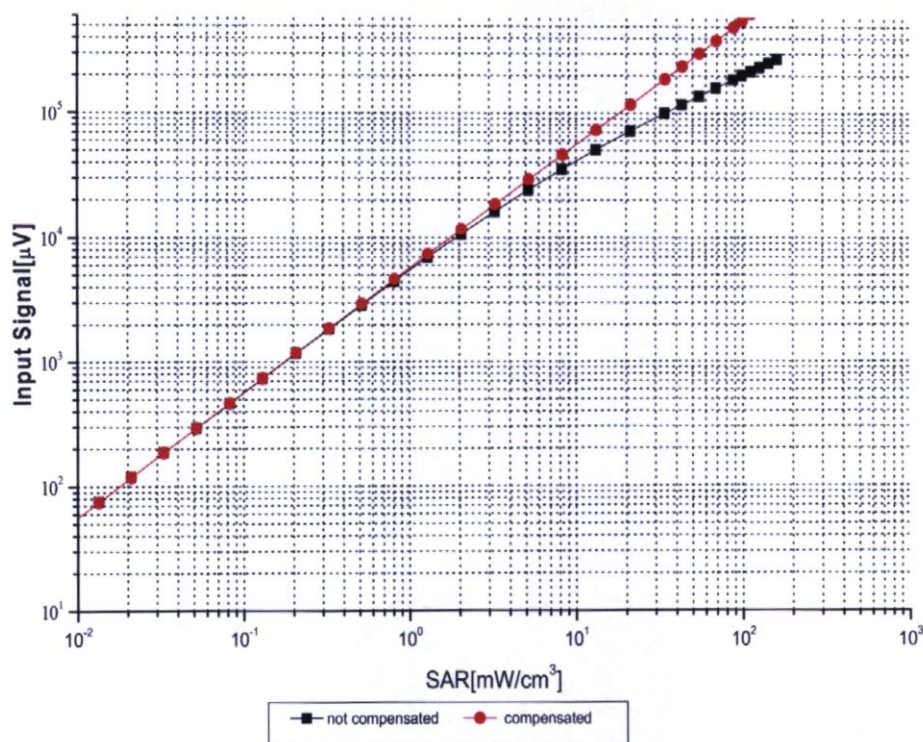

Uncertainty of Linearity Assessment:  $\pm 0.9\%$  ( $k=2$ )





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>


## Conversion Factor Assessment

$f=750\text{ MHz}$ , WGLS R9(H\_convF)

$f=1750\text{ MHz}$ , WGLS R22(H\_convF)

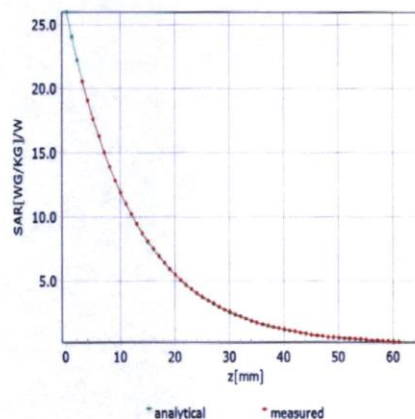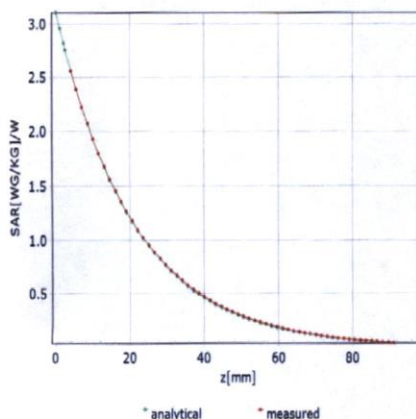

## Deviation from Isotropy in Liquid

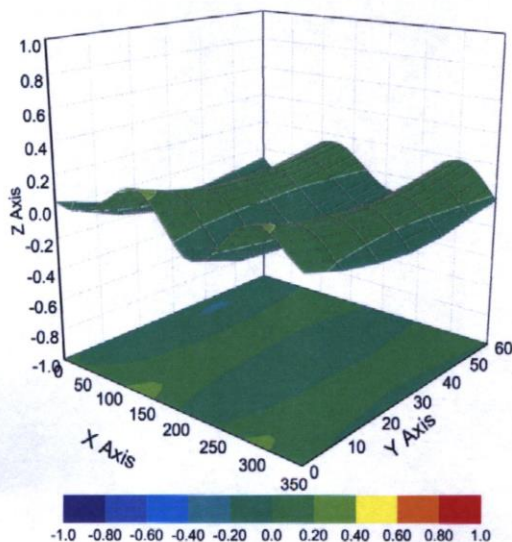

Uncertainty of Spherical Isotropy Assessment:  $\pm 3.2\%$  ( $k=2$ )