

DASY5 Validation Report for Body TSL

Date: 24.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: IndexSAR; Serial: IndexSAR - SN:1S2571

Communication System: UID 0 - CW ; Frequency: 5200 MHz, Frequency: 5500 MHz, Frequency: 5800 MHz

Medium parameters used: $f = 5200$ MHz; $\sigma = 5.4$ S/m; $\epsilon_r = 48.9$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5500$ MHz; $\sigma = 5.79$ S/m; $\epsilon_r = 48.4$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5800$ MHz; $\sigma = 6.21$ S/m; $\epsilon_r = 47.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(4.91, 4.91, 4.91); Calibrated: 28.12.2012, ConvF(4.43, 4.43, 4.43); Calibrated: 28.12.2012, ConvF(4.38, 4.38, 4.38); Calibrated: 28.12.2012;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1f37); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 55.464 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 26.1 W/kg

SAR(1 g) = 6.74 W/kg; SAR(10 g) = 1.92 W/kg

Maximum value of SAR (measured) = 15.5 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 53.036 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 27.8 W/kg

SAR(1 g) = 6.59 W/kg; SAR(10 g) = 1.89 W/kg

Maximum value of SAR (measured) = 15.8 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan,


dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 50.674 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 30.0 W/kg

SAR(1 g) = 6.44 W/kg; SAR(10 g) = 1.79 W/kg

Maximum value of SAR (measured) = 15.9 W/kg

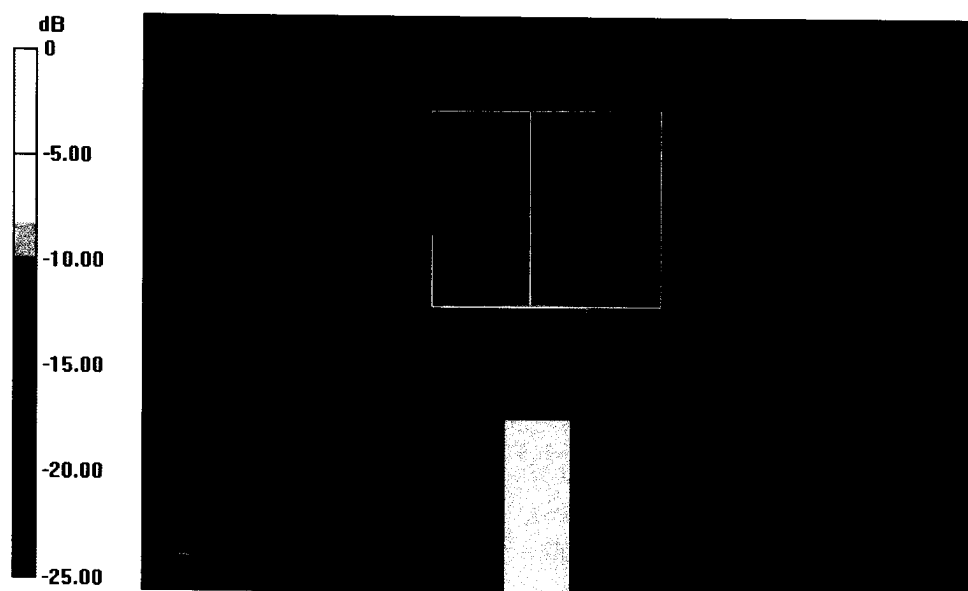

0 dB = 15.9 W/kg = 12.01 dBW/kg

Impedance Measurement Plot for Body TSL

24 Jul 2013 15:03:52

CH1 S11 1 U FS

1: 41.676 Ω -26.406 Ω 1.1591 pF


5 200.000 000 MHz

*
Del

Cor

Avg
16

H1d

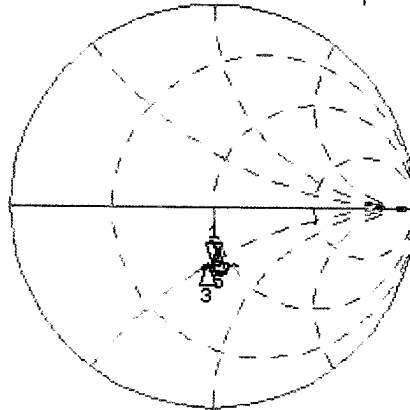

CH1 Markers

3: 39.045 Ω
-25.248 Ω
5.50000 GHz

5: 46.773 Ω
-22.291 Ω
5.80000 GHz

CH2 S11 LOG

5 dB/REF -20 dB


1: -10.745 dB

5 200.000 000 MHz

Cor

Avg
16

H1d

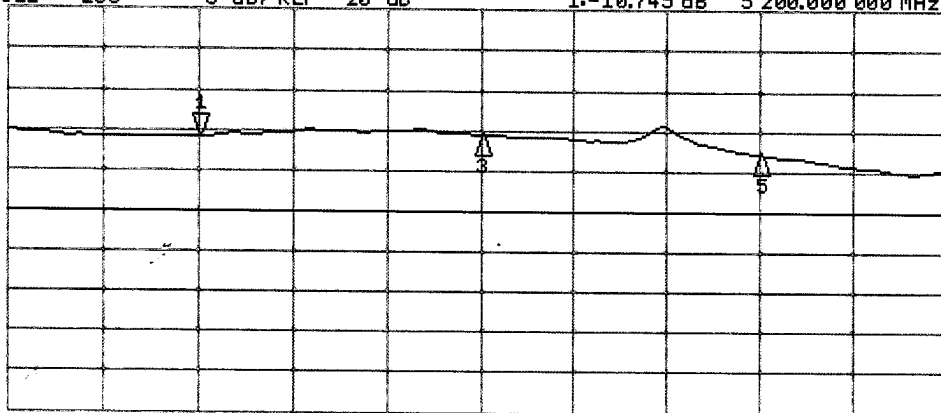

CH2 Markers

3: -10.536 dB
5.50000 GHz

5: -12.888 dB
5.80000 GHz

START 5 000.000 000 MHz

STOP 5 800.000 000 MHz



APPENDIX E - MEASURED FLUID DIELECTRIC PARAMETERS

Title

SubTitle

June 17, 2014 04:12 PM

Frequency	e'	e''
2.400000000 GI	50.946'	14.8684
2.402000000 GI	50.939'	14.8920
2.404000000 GI	50.928'	14.8994
2.406000000 GI	50.928'	14.9158
2.408000000 GI	50.924'	14.9291
2.410000000 GI	50.909'	14.9400
2.412000000 GI	50.889'	14.9581
2.414000000 GI	50.878'	14.9587
2.416000000 GI	50.876'	14.9617
2.418000000 GI	50.865'	14.9807
2.420000000 GI	50.836'	14.9912
2.422000000 GI	50.822'	15.0086
2.424000000 GI	50.816'	15.0070
2.426000000 GI	50.799'	15.0064
2.428000000 GI	50.805'	15.0153
2.430000000 GI	50.790'	15.0246
2.432000000 GI	50.778'	15.0367
2.434000000 GI	50.775'	15.0531
2.436000000 GI	50.750'	15.0516
2.438000000 GI	50.735'	15.0607
2.440000000 GI	50.728'	15.0524
2.442000000 GI	50.726'	15.0786
2.444000000 GI	50.711'	15.0761
2.446000000 GI	50.708'	15.0708
2.448000000 GI	50.707'	15.0885
2.450000000 GI	50.702'	15.0849
2.452000000 GI	50.696'	15.0981
2.454000000 GI	50.698'	15.1154
2.456000000 GI	50.693'	15.1385
2.458000000 GI	50.682'	15.1537
2.460000000 GI	50.674'	15.1654
2.462000000 GI	50.667'	15.1901
2.464000000 GI	50.664'	15.2028
2.466000000 GI	50.651'	15.2133
2.468000000 GI	50.647'	15.2245

2.470000000 GI	50.637	15.2312
2.472000000 GI	50.619	15.2405
2.474000000 GI	50.621	15.2626
2.476000000 GI	50.599	15.2689
2.478000000 GI	50.583	15.2795
2.480000000 GI	50.568	15.3083
2.482000000 GI	50.557	15.3233
2.484000000 GI	50.543	15.3354
2.486000000 GI	50.532	15.3406
2.488000000 GI	50.526	15.3650
2.490000000 GI	50.515	15.3651
2.492000000 GI	50.491	15.3832
2.494000000 GI	50.472	15.3941
2.496000000 GI	50.460	15.3810
2.498000000 GI	50.449	15.4042
2.500000000 GI	50.442	15.3941

Title

SubTitle

August 15, 2014 09:17 AM

Frequency	e'	e''
5.000000000 GI	47.408	17.3486
5.020000000 GI	47.375	17.3428
5.040000000 GI	47.324	17.3940
5.060000000 GI	47.245	17.4331
5.080000000 GI	47.230	17.4594
5.100000000 GI	47.208	17.5254
5.120000000 GI	47.189	17.5271
5.140000000 GI	47.192	17.5459
5.160000000 GI	47.116	17.5702
5.180000000 GI	47.068	17.5878
5.200000000 GI	47.010	17.6387
5.220000000 GI	46.989	17.6385
5.240000000 GI	47.003	17.6733
5.260000000 GI	46.940	17.6813
5.280000000 GI	46.908	17.6871
5.300000000 GI	46.827	17.7458
5.320000000 GI	46.764	17.7820
5.340000000 GI	46.776	17.8383
5.360000000 GI	46.805	17.8585
5.380000000 GI	46.779	17.8437
5.400000000 GI	46.718	17.8718
5.420000000 GI	46.662	17.8641
5.440000000 GI	46.617	17.9383
5.460000000 GI	46.567	17.9775
5.480000000 GI	46.570	17.9816
5.500000000 GI	46.565	17.9916
5.520000000 GI	46.488	17.9800
5.540000000 GI	46.438	18.0157
5.560000000 GI	46.375	18.0766
5.580000000 GI	46.351	18.0911
5.600000000 GI	46.343	18.1045
5.620000000 GI	46.307	18.0970
5.640000000 GI	46.274	18.1469
5.660000000 GI	46.186	18.1928
5.680000000 GI	46.153	18.2091

5.700000000 GI	46.139%	18.2459
5.720000000 GI	46.117%	18.2016
5.740000000 GI	46.065%	18.1610
5.760000000 GI	45.922%	18.1858
5.780000000 GI	45.901%	18.2575
5.800000000 GI	45.878%	18.3276
5.820000000 GI	45.882%	18.3880
5.840000000 GI	45.866%	18.3926
5.860000000 GI	45.826%	18.3588
5.880000000 GI	45.765%	18.3544
5.900000000 GI	45.695%	18.4146
5.920000000 GI	45.605%	18.4601
5.940000000 GI	45.617%	18.5262
5.960000000 GI	45.617%	18.5303
5.980000000 GI	45.617%	18.5273
6.000000000 GI	45.549%	18.5624



APPENDIX F – PHANTOM CERTIFICATE OF CONFORMITY

Certificate of conformity / First Article Inspection

Item	SAM Twin Phantom V4.0
Type No	QD 000 P40 C
Series No	TP-1150 and higher
Manufacturer / Origin	Untersee Composites Hauptstr. 69 CH-8559 Fruthwilen Switzerland

Tests

The series production process used allows the limitation to test of first articles.

Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series units (called samples).

Test	Requirement	Details	Units tested
Shape	Compliance with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness	Compliant with the requirements according to the standards	2mm +/- 0.2mm in specific areas; 6mm +/- 0.2mm at ERP	First article, Samples
Material parameters	Dielectric parameters for required frequencies	200 MHz – 3 GHz Relative permittivity < 5 Loss tangent < 0.05.	Material sample TP 104-5
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards if handled and cleaned according to the instructions	DEGMBE based simulating liquids	Pre-series, First article, Samples

Standards

[1] CENELEC EN 50361

[2] IEEE Std 1528-200x Draft CD 1.1 (Dec 02)

[3] IEC 62209/CD (Nov 02)

(*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of [1] and [3].

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standard [1] and draft standards [2] and [3].

Date

7.8.2003

Signature / Stamp

s p e a g

Schmid & Partner Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 1 245 9700, Fax +41 1 245 9779
 info@speag.com, http://www.speag.com



APPENDIX G - DAE CALIBRATION CERTIFICATE



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **MET Laboratories**

Certificate No: **DAE3-584_Jul13**

CALIBRATION CERTIFICATE

Object **DAE3 - SD 000 D03 AA - SN: 584**

Calibration procedure(s) **QA CAL-06.v26**
Calibration procedure for the data acquisition electronics (DAE)

Calibration date: **July 18, 2013**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	02-Oct-12 (No:12728)	Oct-13
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	07-Jan-13 (in house check)	In house check: Jan-14
Calibrator Box V2.1	SE UMS 006 AA 1002	07-Jan-13 (in house check)	In house check: Jan-14

Calibrated by:	Name	Function	Signature
	Dominique Steffen	Technician	
Approved by:	Fin Bomholt	Deputy Technical Manager	

Issued: July 18, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary

DAE	data acquisition electronics
Connector angle	information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
 - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
 - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
 - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
 - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
 - *Power consumption:* Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 μ V , full range = -100...+300 mV

Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.662 $\pm$ 0.02% (k=2)	404.844 $\pm$ 0.02% (k=2)	404.267 $\pm$ 0.02% (k=2)
Low Range	3.93273 $\pm$ 1.50% (k=2)	3.98110 $\pm$ 1.50% (k=2)	3.97938 $\pm$ 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	141.0 ° $\pm$ 1 °
---	-------------------

Appendix

1. DC Voltage Linearity

High Range		Reading (μV)	Difference (μV)	Error (%)
Channel X	+ Input	199996.51	-1.40	-0.00
Channel X	+ Input	20001.72	1.16	0.01
Channel X	- Input	-19998.74	2.23	-0.01
Channel Y	+ Input	199995.49	-2.08	-0.00
Channel Y	+ Input	20001.55	1.15	0.01
Channel Y	- Input	-19997.38	3.75	-0.02
Channel Z	+ Input	199996.10	-1.20	-0.00
Channel Z	+ Input	19999.08	-1.38	-0.01
Channel Z	- Input	-19999.72	1.40	-0.01

Low Range		Reading (μV)	Difference (μV)	Error (%)
Channel X	+ Input	2002.82	1.92	0.10
Channel X	+ Input	202.17	0.93	0.46
Channel X	- Input	-198.65	-0.18	0.09
Channel Y	+ Input	2002.22	1.54	0.08
Channel Y	+ Input	200.42	-0.71	-0.35
Channel Y	- Input	-199.73	-1.09	0.55
Channel Z	+ Input	2000.94	0.28	0.01
Channel Z	+ Input	200.01	-1.13	-0.56
Channel Z	- Input	-200.29	-1.60	0.80

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	3.04	1.31
	- 200	-0.45	-1.35
Channel Y	200	3.69	2.42
	- 200	-3.59	-3.54
Channel Z	200	-7.37	-7.51
	- 200	5.30	5.09

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	-0.18	-3.67
Channel Y	200	6.93	-	-0.17
Channel Z	200	7.39	5.46	-

IMPORTANT NOTICE

USAGE OF THE DAE 3

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

Battery Exchange: The battery cover of the DAE3 unit is connected to a fragile 3-pin battery connector. Customer is responsible to apply outmost caution not to bend or damage the connector when changing batteries.

Shipping of the DAE: Before shipping the DAE to SPEAG for calibration the customer shall remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts transportation. The package shall be marked to indicate that a fragile instrument is inside.

E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, Customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

Important Note:

Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.

Important Note:

Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.

Important Note:

To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16109	15852
Channel Y	16158	16754
Channel Z	16279	16611

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M Ω

	Average (μ V)	min. Offset (μ V)	max. Offset (μ V)	Std. Deviation (μ V)
Channel X	1.30	-0.50	3.30	0.53
Channel Y	-0.18	-1.65	1.35	0.50
Channel Z	-0.26	-1.48	1.14	0.47

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9