


APPENDIX B EUT TEST POSITION PHOTOS

Liquid depth $\geq 15\text{cm}$


Phantom: SAM (30deg probe tilt) with CRP v5.0_20150321; Type: QD000P40CD; Serial: TP:1874




Head Left Cheek Setup Photo

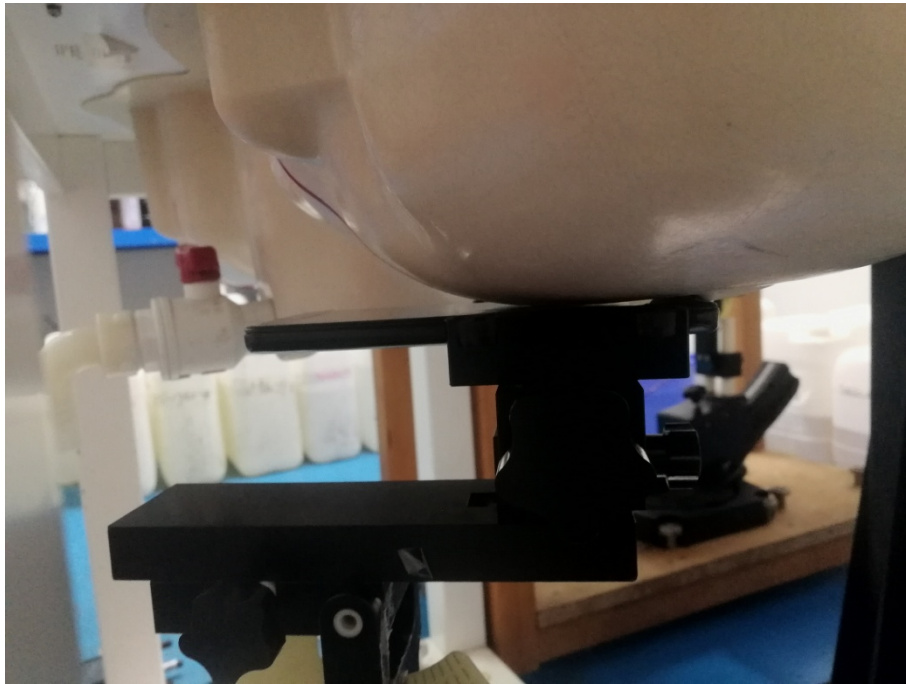


Head Left Tilt Setup Photo

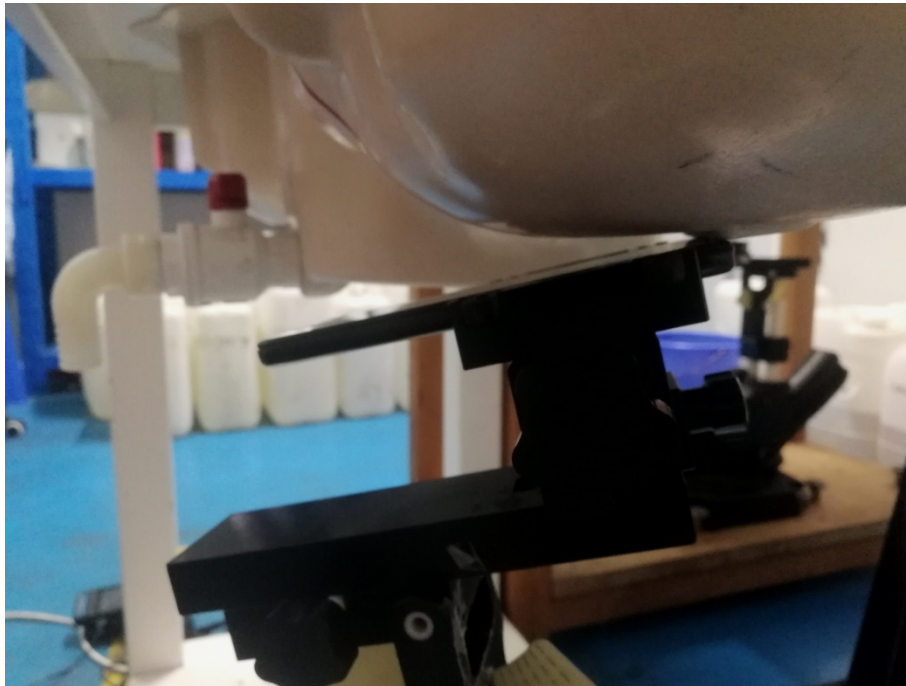


Head Right Cheek Setup Photo

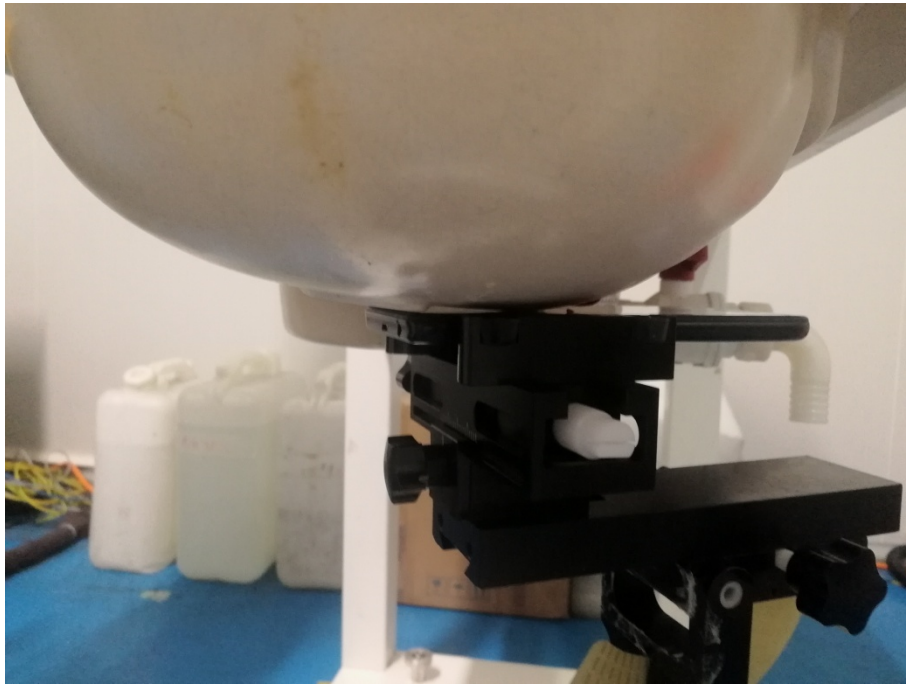


Head Right Tilt Setup Photo

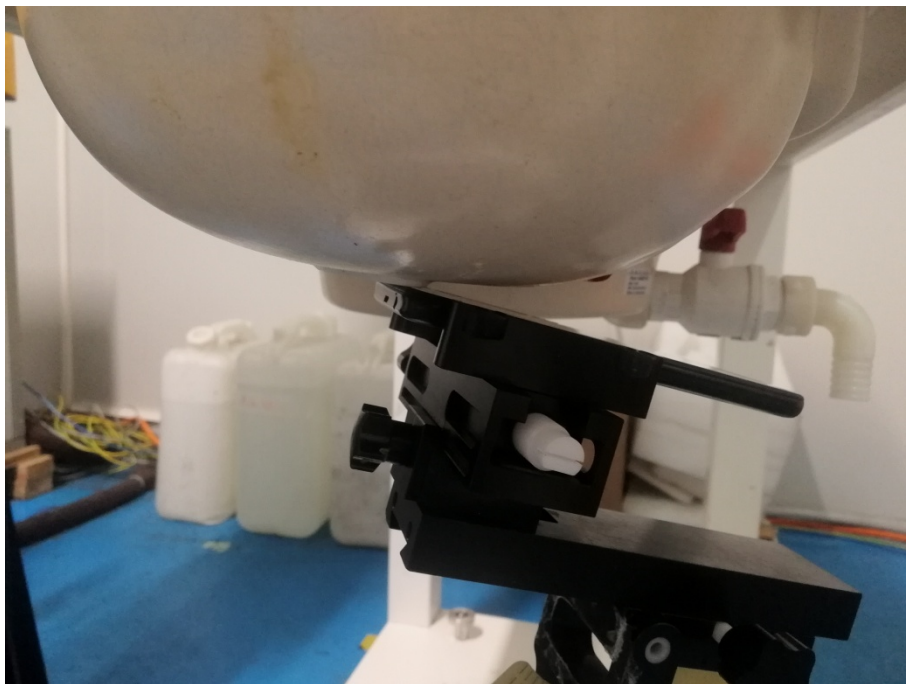


Body (Worn) Back Setup Photo (10mm)

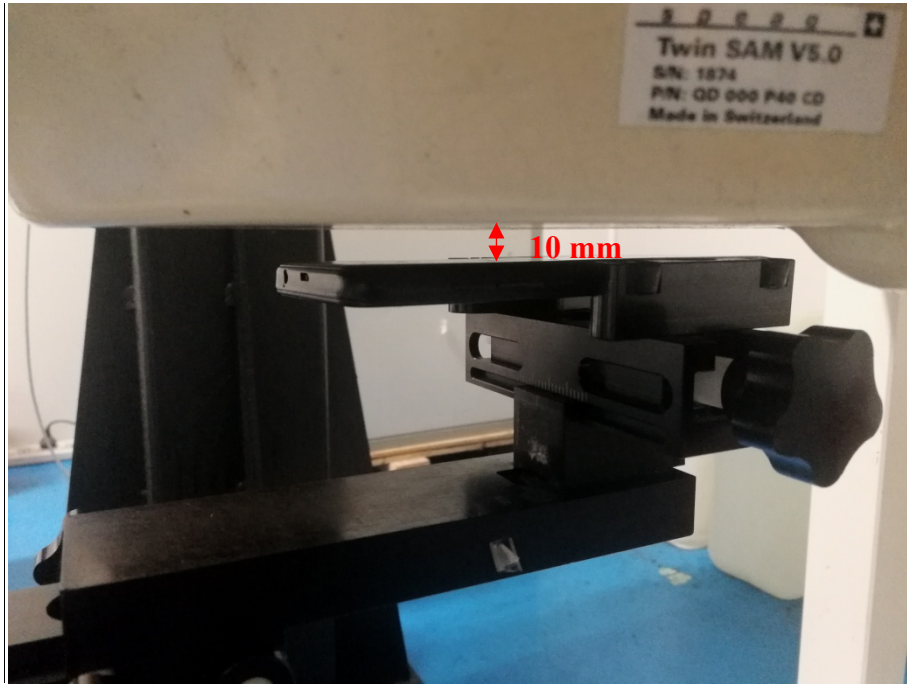


Body (Worn) Front Setup Photo (10mm)

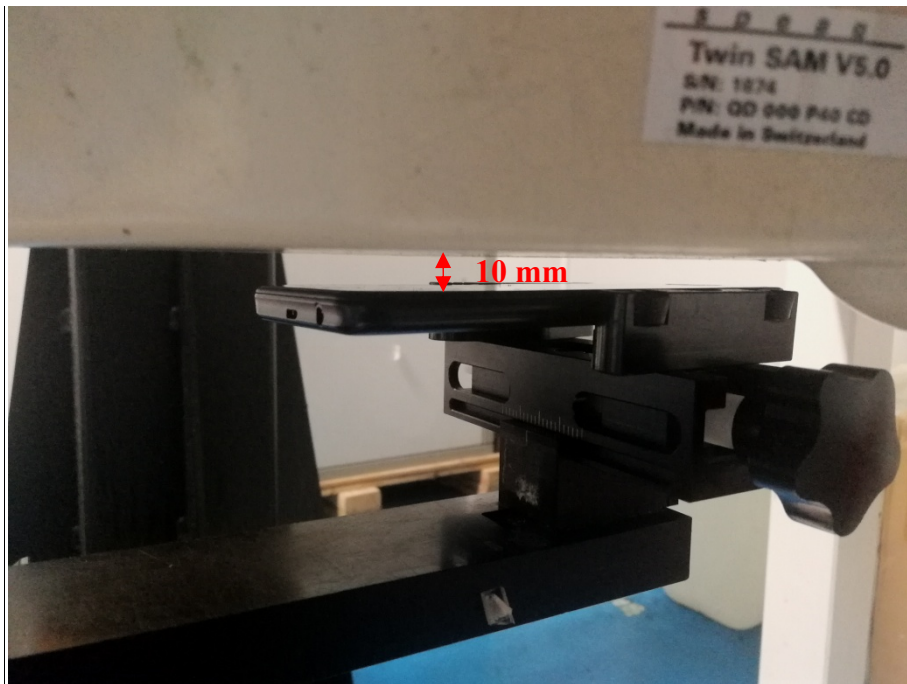

Body Left Setup Photo (10mm)

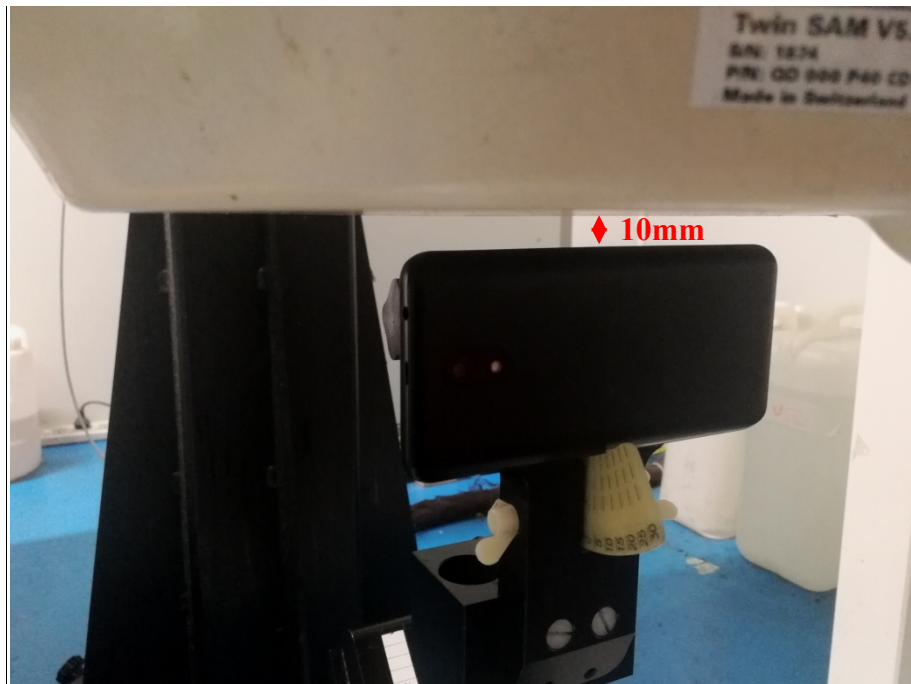

Body Right Setup Photo (10mm)

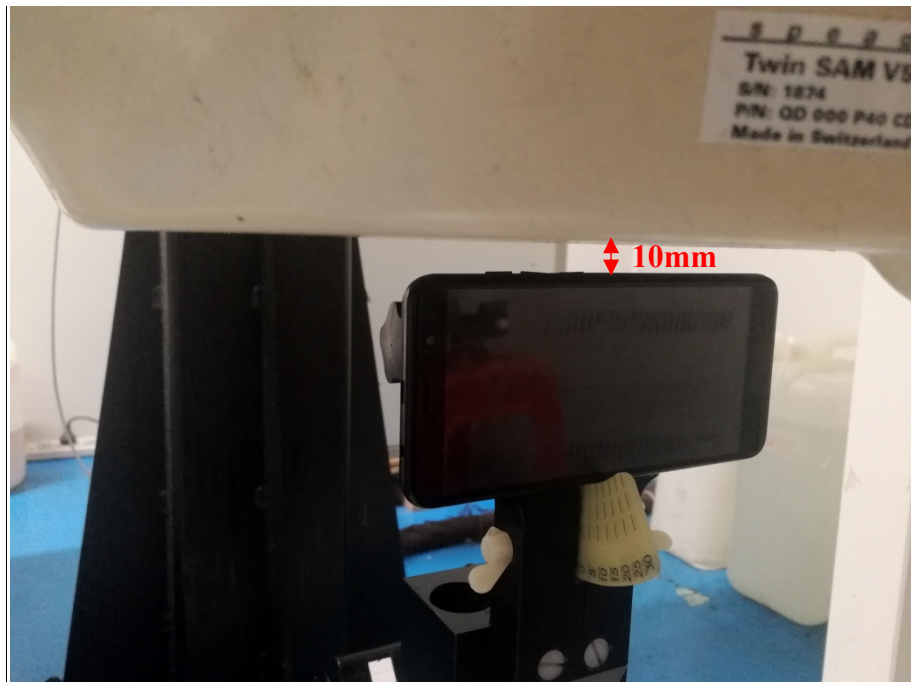

Body Bottom Setup Photo (10mm)



Body Top Setup Photo (10mm)

