



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY5 Validation Report for Head TSL

Date: 2023-08-23

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1245

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz,
Frequency: 5750 MHz

Medium parameters used: $f = 5250$ MHz; $\sigma = 4.627$ S/m; $\epsilon_r = 35.17$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5600$ MHz; $\sigma = 5$ S/m; $\epsilon_r = 34.58$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5750$ MHz; $\sigma = 5.162$ S/m; $\epsilon_r = 34.36$; $\rho = 1000$ kg/m³

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(5.5, 5.5, 5.5) @ 5250 MHz; ConvF(5.01, 5.01, 5.01) @ 5600 MHz; ConvF(5.15, 5.15, 5.15) @ 5750 MHz; Calibrated: 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan,**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.63 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 31.2 W/kg

SAR(1 g) = 7.84 W/kg; SAR(10 g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.4%

Maximum value of SAR (measured) = 18.5 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan,**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.43 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 35.6 W/kg

SAR(1 g) = 8.15 W/kg; SAR(10 g) = 2.3 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.4%

Maximum value of SAR (measured) = 19.7 W/kg




In Collaboration with
s p e a g
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>


Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan,
dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 61.00 V/m; Power Drift = -0.03 dB
Peak SAR (extrapolated) = 36.0 W/kg
SAR(1 g) = 7.83 W/kg; SAR(10 g) = 2.19 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 61%
Maximum value of SAR (measured) = 19.8 W/kg

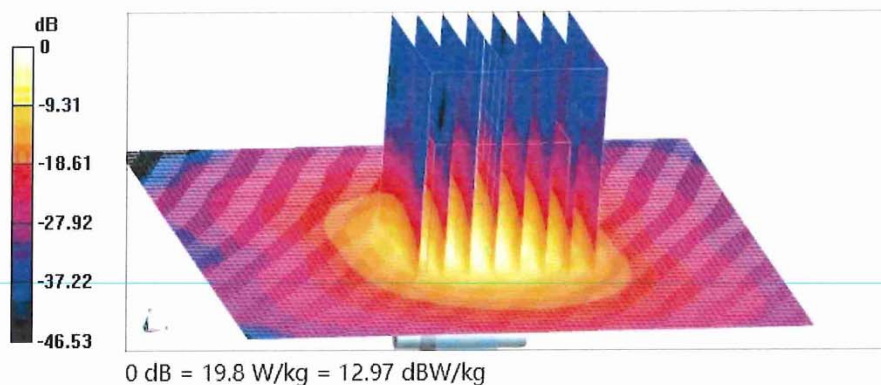



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caic.ac.cn>

Impedance Measurement Plot for Head TSL

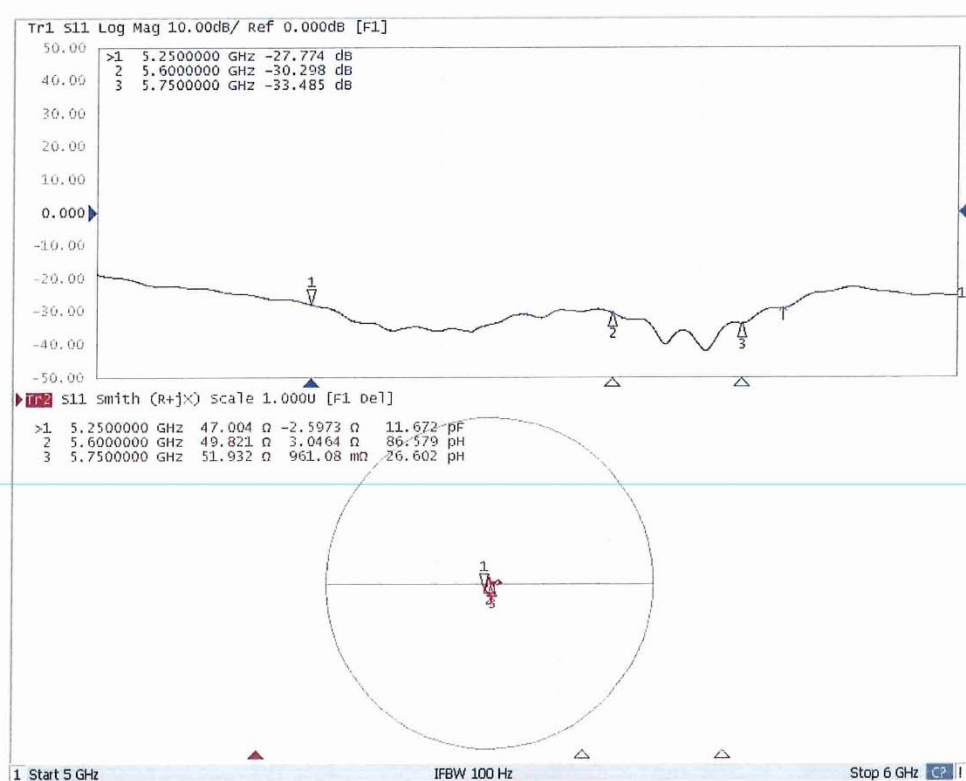


RETURN LOSS&IMPEDANCE MEASUREMENT**D750V3 - SN: 1230 Extended Dipole Calibrations**

Per FCC KDB 865664 D01, calibration intervals of up to 3 years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements.

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20 dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from calibration date.

D750V3 - SN:1230						
750MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedence(Ω)	Delta (Ω)	Imaginary Impedence(Ω)	Delta (Ω)
2023/3/24	-30.332	/	53.013	/	0.869	/
2024/3/23	-31.662	4.385	49.870	-3.143	-2.606	-3.475

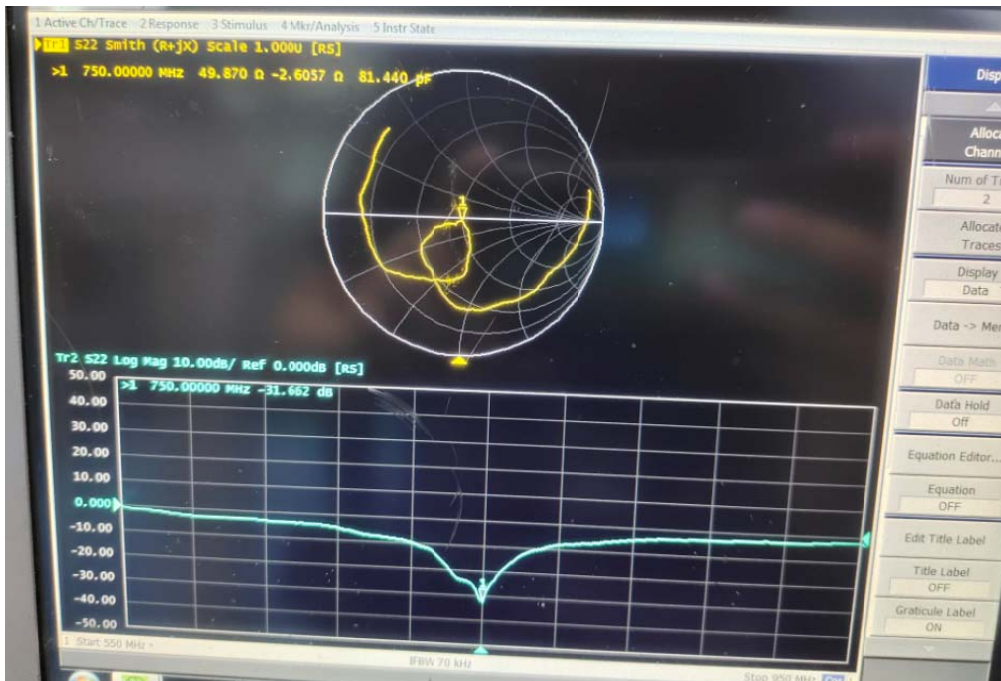

	Name	Signature
Calibrated By:	Karl Gong	<i>Karl Gong</i>


D900V2 - SN: 1d217 Extended Dipole Calibrations

Per FCC KDB 865664 D01, calibration intervals of up to 3 years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements.

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20 dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from calibration date.

D900V2 - SN:1d217						
900MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedance(Ω)	Delta (Ω)	Imaginary Impedance(Ω)	Delta (Ω)
2023/3/24	-50.111	/	50.312	/	-0.032	/
2024/3/23	-49.309	1.6	49.663	-0.649	-0.057	-0.025

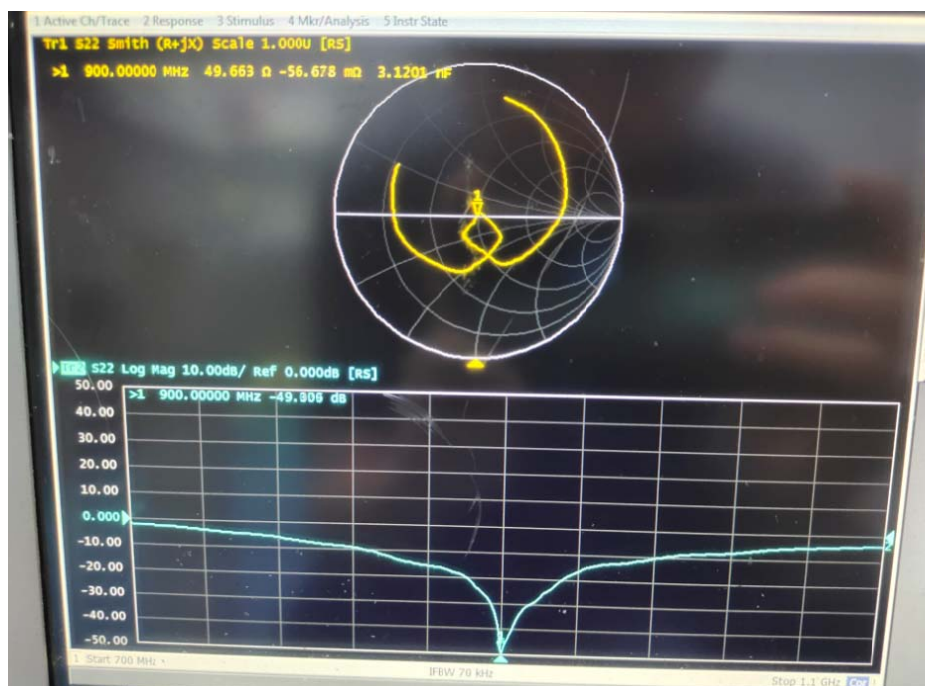

	Name	Signature
Calibrated By:	Karl Gong	Karl Gong

D1750V2 - SN: 1200 Extended Dipole Calibrations

Per FCC KDB 865664 D01, calibration intervals of up to 3 years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements.

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20 dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from calibration date.

D1750V2 - SN:1200						
1750MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedance(Ω)	Delta (Ω)	Imaginary Impedance(Ω)	Delta (Ω)
2023/3/27	-26.957	/	48.910	/	3.066	/
2024/3/26	-29.696	10.161	48.606	-3.04	2.914	-0.152



	Name	Signature
Calibrated By:	Karl Gong	Karl Gong


D1900V2 - SN: 5d251 Extended Dipole Calibrations

Per FCC KDB 865664 D01, calibration intervals of up to 3 years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements.

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20 dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from calibration date.

D1900V2 - SN:5d251						
1900MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedance(Ω)	Delta (Ω)	Imaginary Impedance(Ω)	Delta (Ω)
2023/3/27	-23.715	/	49.490	/	6.481	/
2024/3/26	-23.536	-0.755	45.694	-3.796	4.627	-1.854

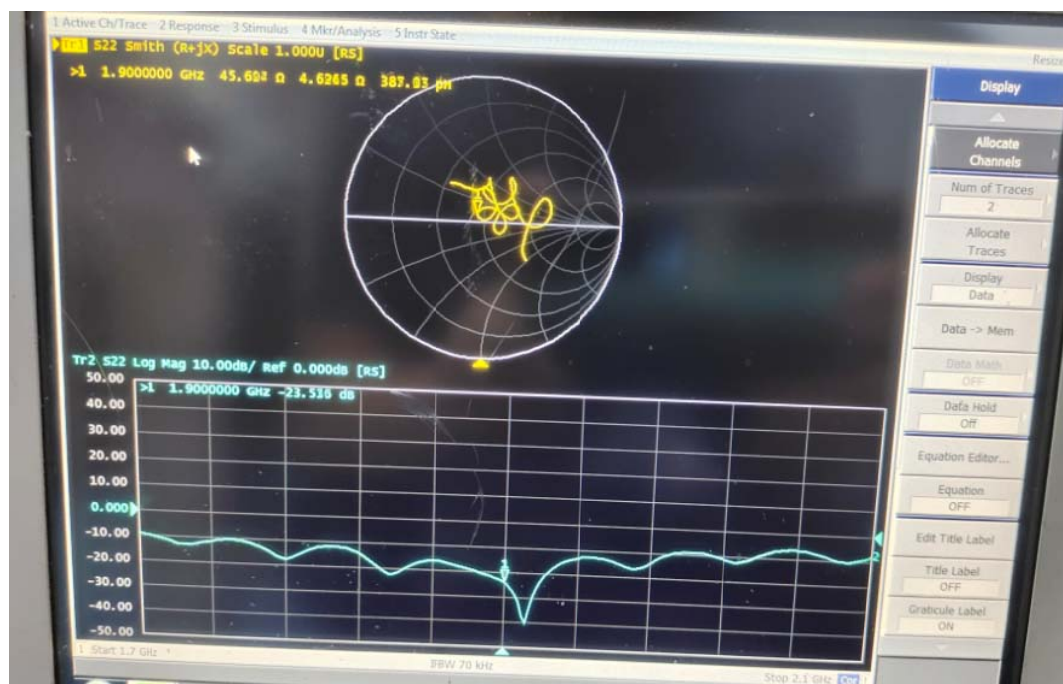

	Name	Signature
Calibrated By:	Karl Gong	Karl Gong


D2450V2 - SN: 1102 Extended Dipole Calibrations

Per FCC KDB 865664 D01, calibration intervals of up to 3 years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements.

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20 dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from calibration date.

D2450V2 - SN:1102						
2450MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedance(Ω)	Delta (Ω)	Imaginary Impedance(Ω)	Delta (Ω)
2023/3/27	-24.556	/	53.856	/	4.795	/
2024/3/26	-27.581	12.319	54.335	0.479	0.453	-4.342

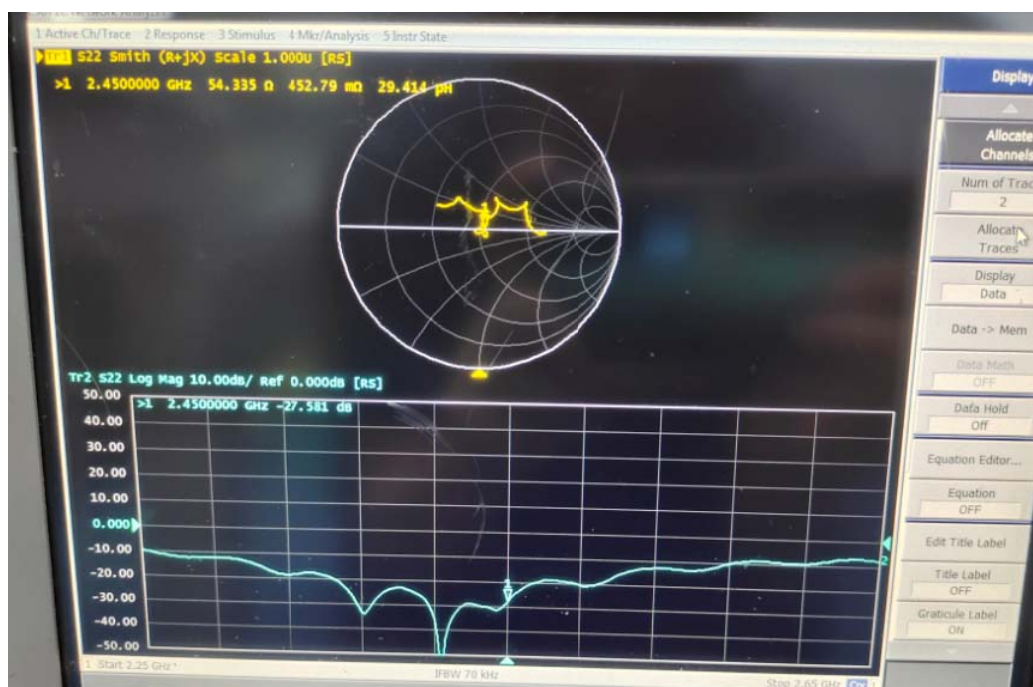

	Name	Signature
Calibrated By:	Karl Gong	Karl Gong


D2600V2 - SN: 1206 Extended Dipole Calibrations

Per FCC KDB 865664 D01, calibration intervals of up to 3 years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements.

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20 dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from calibration date.

D2600V2 - SN:1026						
2600MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedance(Ω)	Delta (Ω)	Imaginary Impedance(Ω)	Delta (Ω)
2023/3/27	-32.698	/	48.148	/	1.322	/
2024/3/26	-29.186	-10.741	52.646	4.498	2.431	1.109

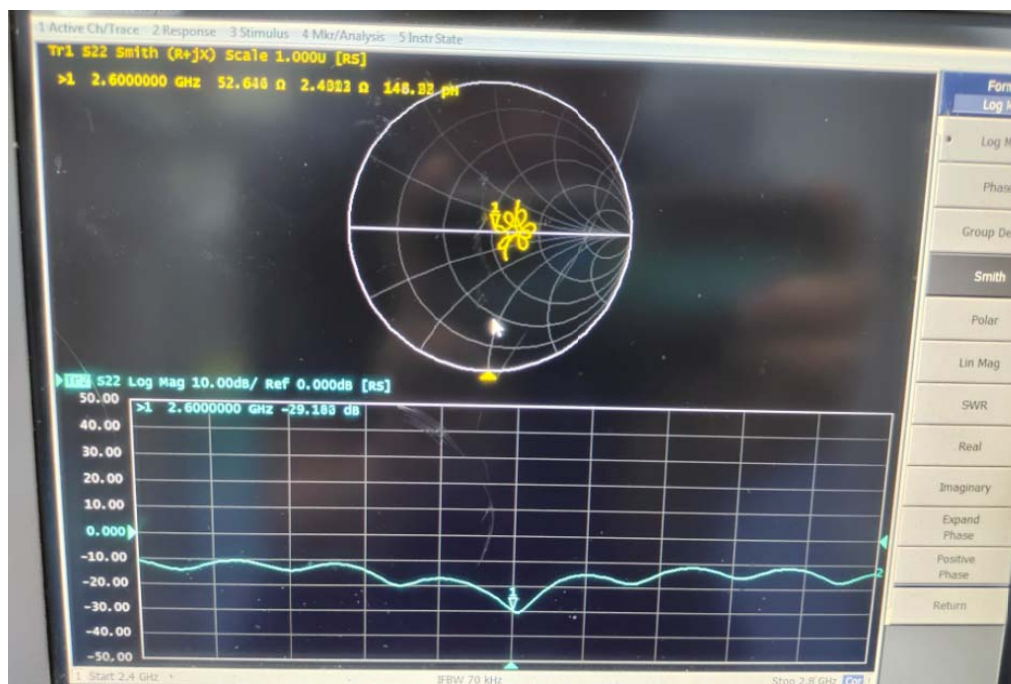

	Name	Signature
Calibrated By:	Karl Gong	Karl Gong



D5GHzV2 - SN: 1245 Extended Dipole Calibrations


Per FCC KDB 865664 D01, calibration intervals of up to 3 years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements.

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20 dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from calibration date.

D5GHzV2-SN:1245						
5250MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedence(Ω)	Delta (Ω)	Imaginary Impedence(Ω)	Delta (Ω)
2023/8/23	-27.774	/	47.004	/	-2.5973	/
2024/8/20	-25.515	-8.13	51.281	4.277	1.8032	4.4005
5600MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedence(Ω)	Delta (Ω)	Imaginary Impedence(Ω)	Delta (Ω)
2023/8/23	-30.298	/	49.821	/	3.0464	/
2024/8/20	-33.499	10.57	50.527	0.706	2.0683	-0.9781
5750MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedence(Ω)	Delta (Ω)	Imaginary Impedence(Ω)	Delta (Ω)
2023/8/23	-33.485	/	51.932	/	0.9611	/
2024/8/20	-29.979	-10.47	47.897	-4.035	2.2950	1.3339

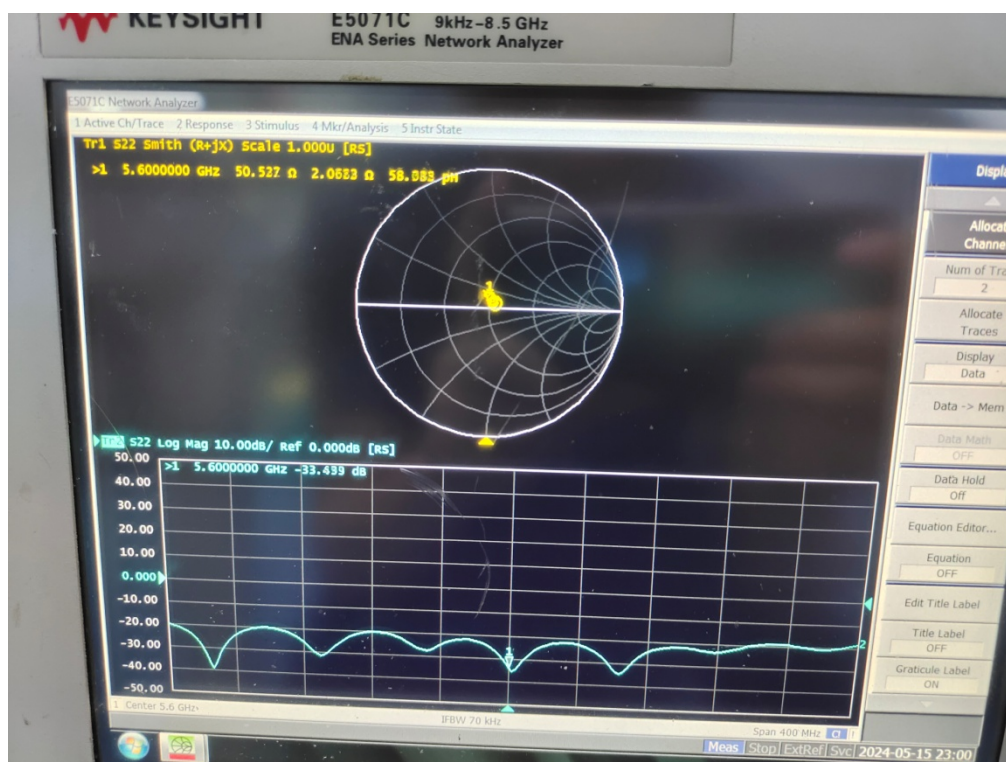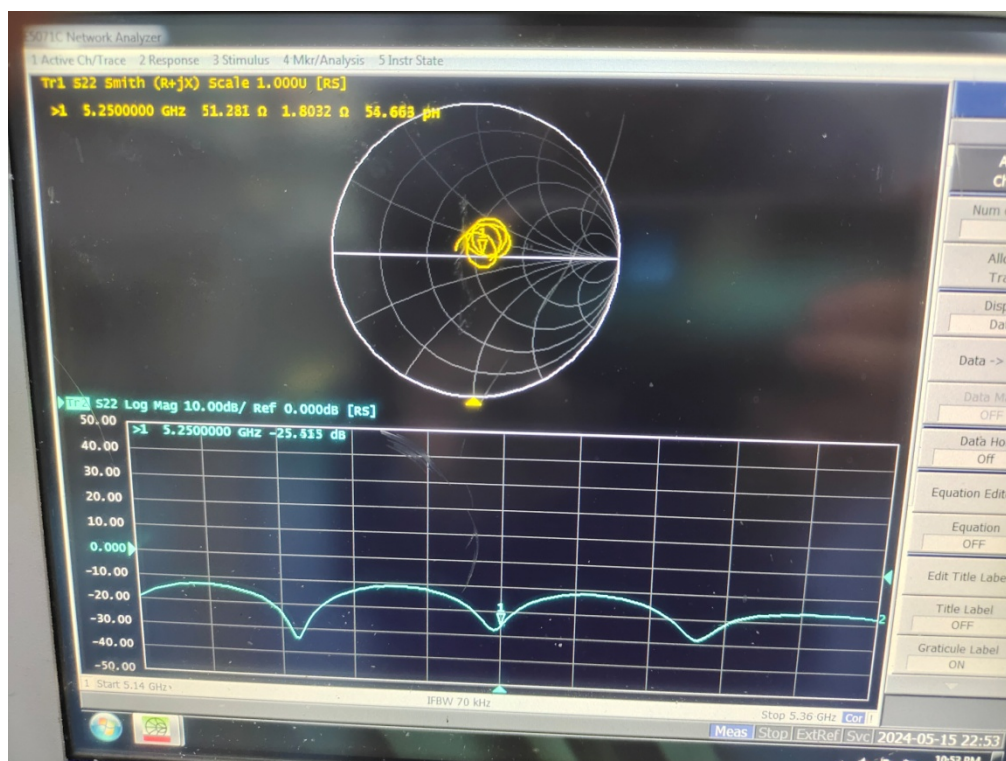

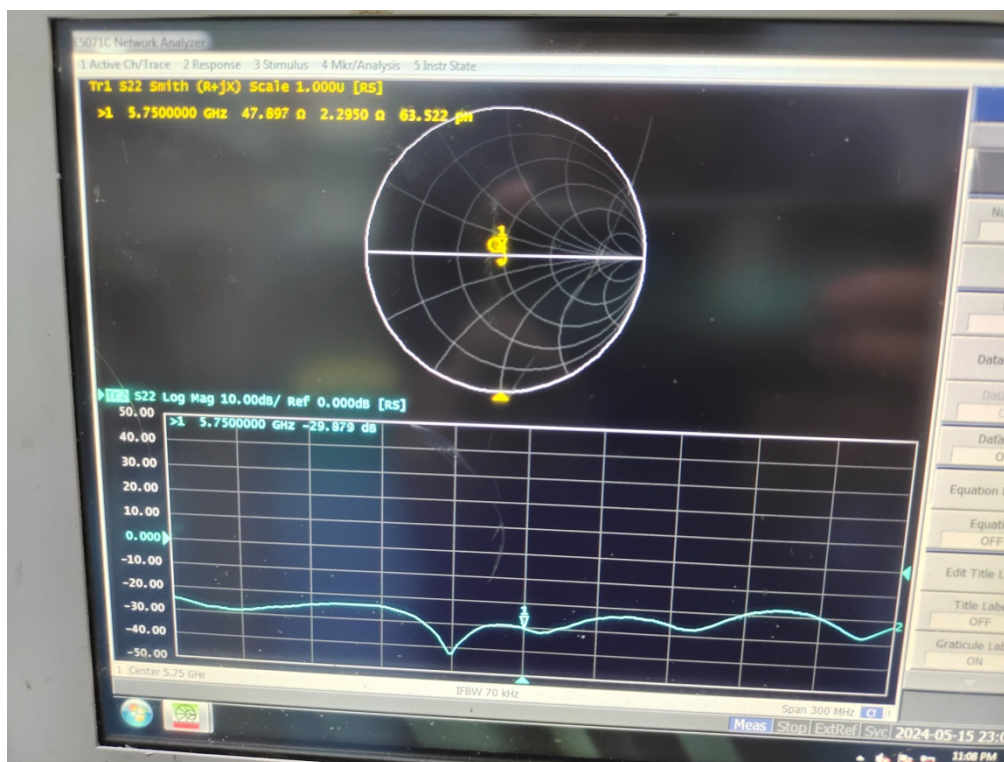

	Name	Signature
Calibrated By:	Karl Gong	Karl Gong