

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid



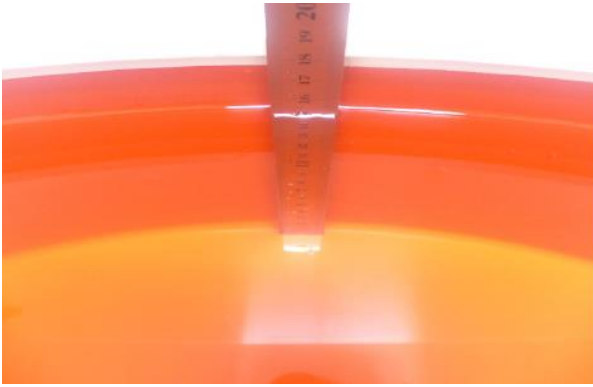
Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1800	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 2600
	

Photo 7: Tissue Simulant Liquid for Head 5GHz

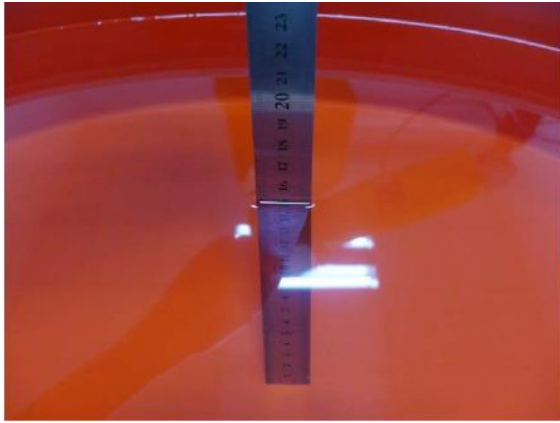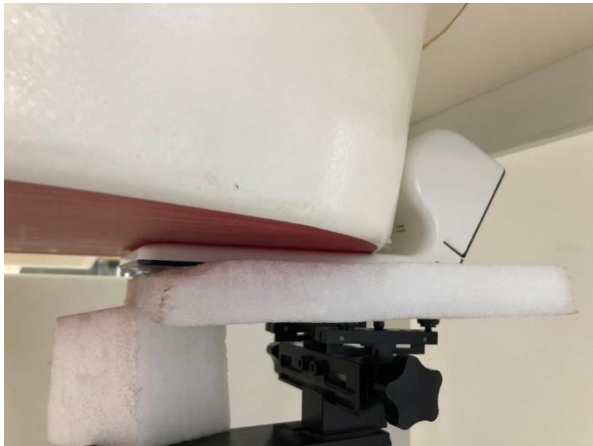

3.

Photographs of EUT test position

Photo 8: Right side 0mm	Photo 9: Back side 0mm
 A photograph showing the right side of a white electronic device (EUT) placed on a white foam block. A red curved object is visible above the device. The device has a black screen and a white label on the side.	 A photograph showing the back side of the same white electronic device (EUT) placed on a white foam block. A red curved object is visible above the device. The device is connected to a black cable.

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.