

Date: 2025-05-13

**System Check\_Head\_6500MHz****DUT: D6.5GHzV2 - SN1026**

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used:  $f = 6500.000$  MHz;  $\sigma = 6.03$  S/m;  $\epsilon_r = 33.9$ 

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.74, 5.63, 5.69); Calibrated: 2024-09-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2024-07-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

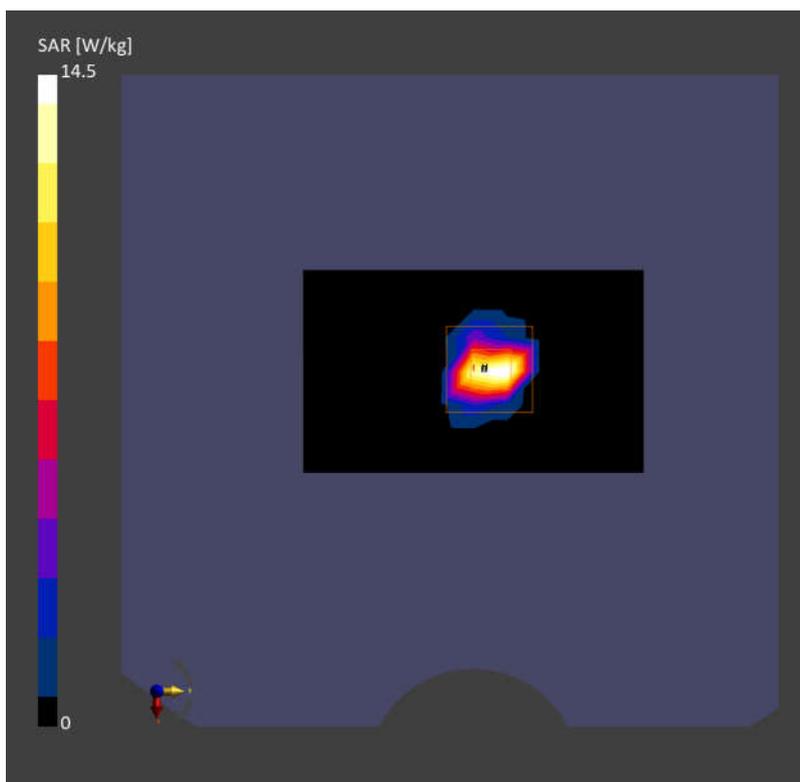
**Pin=50mW/Area Scan (51.0 mm x 85.0 mm):** Measurement Grid: 8.5 mm x 8.5 mm  
SAR (1g) = 10.6 W/kg; SAR (10g) = 2.27 W/kg;**Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 14.5 W/kg; SAR (10g) = 2.72 W/kg

Smallest distance from peaks to all points 3 dB below = 4.6 mm

Ratio of SAR at M2 to SAR at M1 = 53.1 %

psAPD (4.0cm<sup>2</sup>, sq) = 65.8 [W/m<sup>2</sup>]

Measurement Report for Source 10G, FRONT, Validation band, CW, Channel 10000 (10000.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]
Source 10G,	100.0 x 100.0 x 105.0

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor
5G	FRONT, 10.00	Validation band	CW, 0--	10000.0, 10000	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave - 1065	Air -	EUmmWW4 - SN9553_F1-55GHz, 2024-11-15	DAE4 Sn1650, 2024-11-25

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0
MAIA	N/A

Measurement Results

Scan Type	5G Scan
Date	2025-06-04
Avg. Area [cm <sup>2</sup> ]	4.00
psPDn+ [W/m <sup>2</sup> ]	98.7
psPDtot+ [W/m <sup>2</sup> ]	99.3
psPDmod+ [W/m <sup>2</sup> ]	102
E <sub>max</sub> [V/m]	238
Power Drift [dB]	0.02

