

Date: 2025/6/1

System Check_750MHz

D750V3-SN:1099

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 43.2$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(9.81, 8.75, 9.26); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 2.28 W/kg; SAR (10g) = 1.46 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.23 W/kg; SAR (10g) = 1.44 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

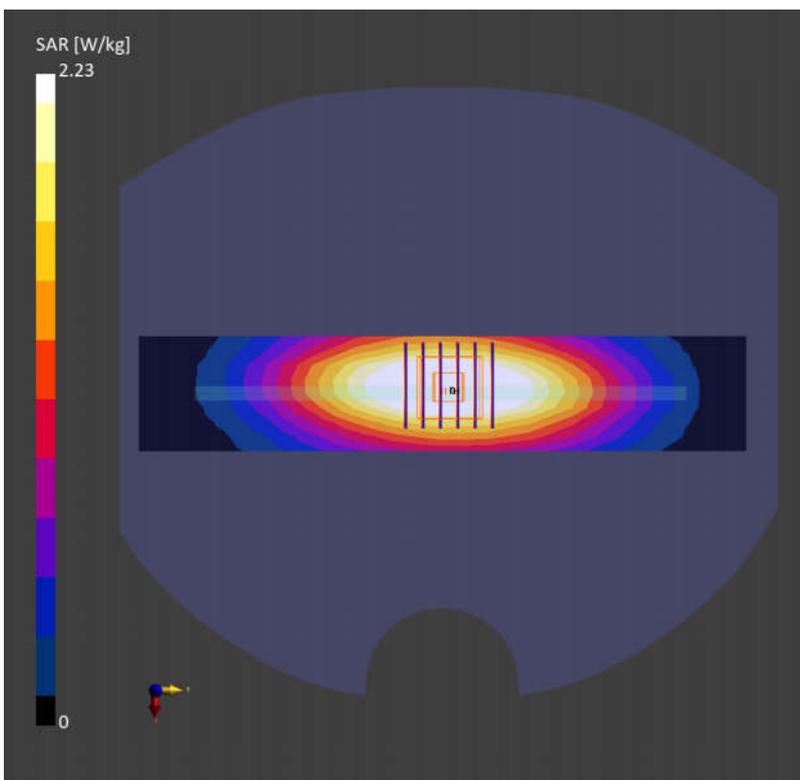

Date: 2025/6/1

System Check_835MHz**D835V2-SN:4d162**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.890$ S/m; $\epsilon_r = 41.5$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(9.4, 8.38, 8.87); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (60.0 mm x 210.0 mm): Measurement Grid: 15.0 mm x 15.0 mm
SAR (1g) = 2.43 W/kg; SAR (10g) = 1.59 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.41 W/kg; SAR (10g) = 1.57 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.6 %

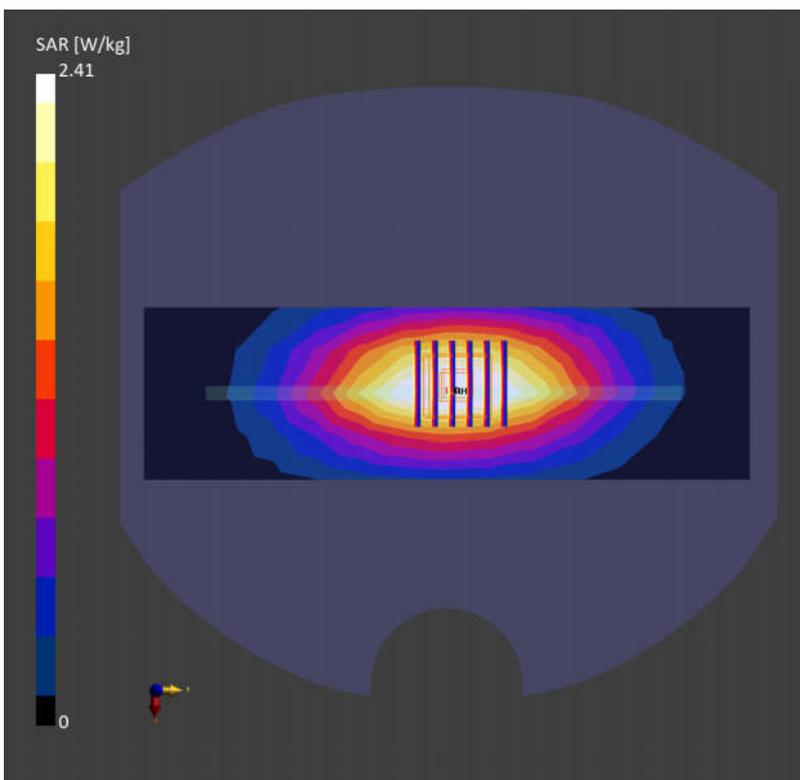

Date: 2025/6/1

System Check_1750MHz**D1750V2-SN:1137**

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.7$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.94, 7.08, 7.50); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (36.0 mm x 120.0 mm): Measurement Grid: 3.0 mm x 15.0 mm
SAR (1g) = 8.51 W/kg; SAR (10g) = 4.63 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 8.48 W/kg; SAR (10g) = 4.58 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.8 %

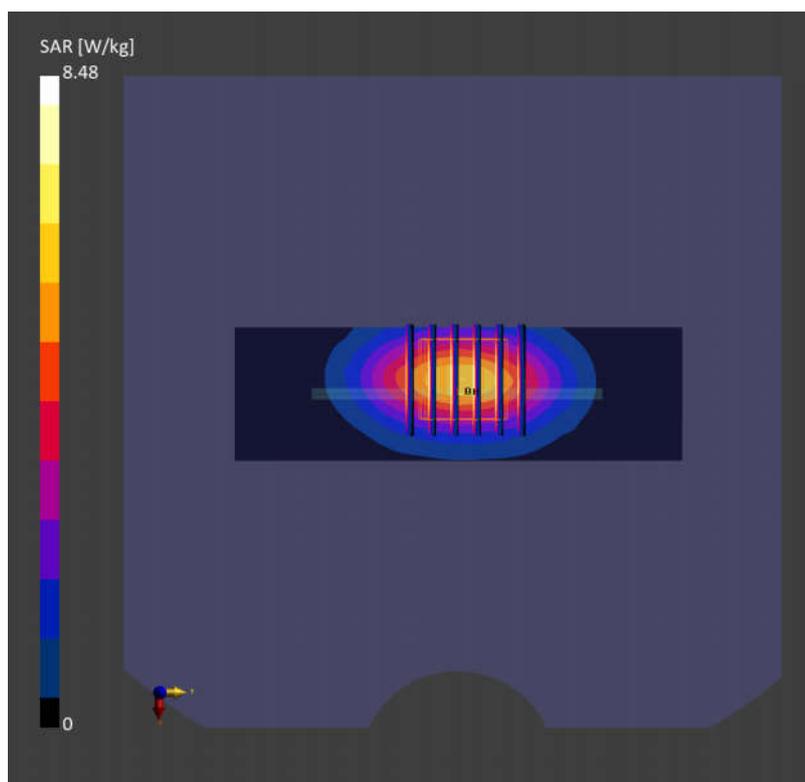

Date: 2025/6/1

System Check_1900MHz

D1900V2-SN:5d182

Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 41.6$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.95, 7.09, 7.51); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 10.4 W/kg; SAR (10g) = 5.42 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 10.3 W/kg; SAR (10g) = 5.31 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

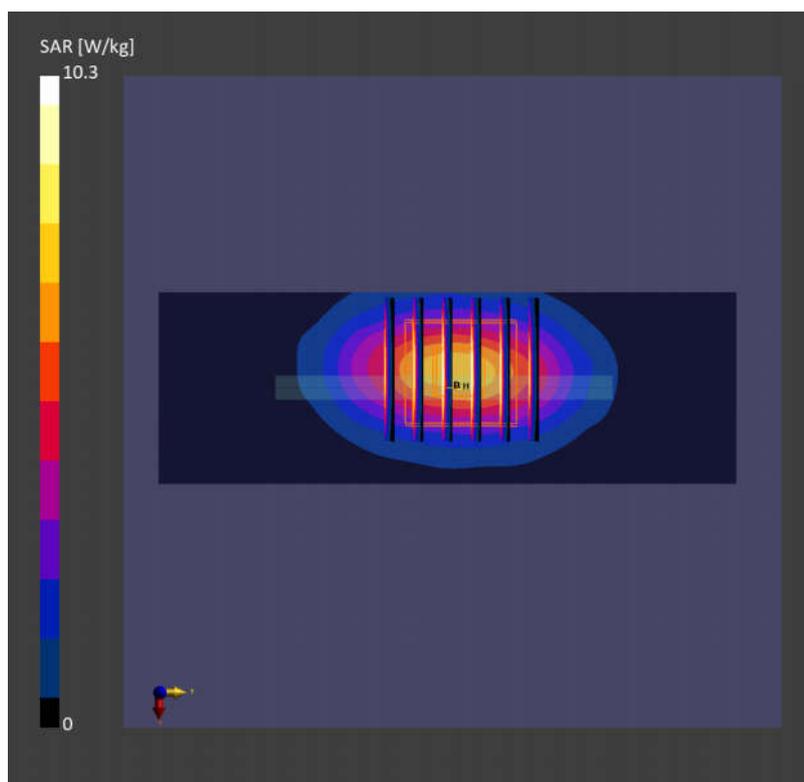

Date: 2025/6/1

System Check_2600MHz

D2600V2-SN:1070

Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 37.7$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.68, 6.85, 7.26); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 13.6 W/kg; SAR (10g) = 6.21 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 13.5 W/kg; SAR (10g) = 6.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.4 %

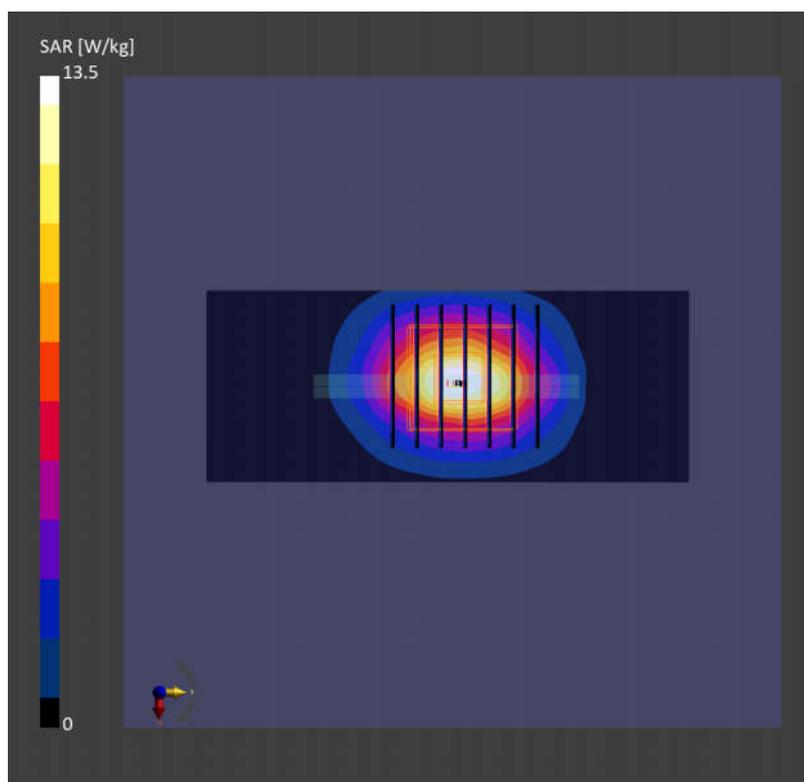

Date: 2025/6/1

System Check_3700MHz**D3700V2-SN:1008**

Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.08$ S/m; $\epsilon_r = 37.4$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.92, 6.17, 6.53); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 6.85 W/kg; SAR (10g) = 2.58 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 6.82 W/kg; SAR (10g) = 2.54 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.3 %

