

Date: 2025-07-05

System Check_Head_750MHz**DUT: D750V3 - SN1087**


Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1
Medium: HSL_750_250705 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.890$ S/m; $\epsilon_r = 42.9$
Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.71, 11.46, 9.89); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 0.406 W/kg; SAR (10g) = 0.275 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 0.419 W/kg; SAR (10g) = 0.276 W/kg
Smallest distance from peaks to all points 3 dB below = 13.7 mm
Ratio of SAR at M2 to SAR at M1 = 87.5 %

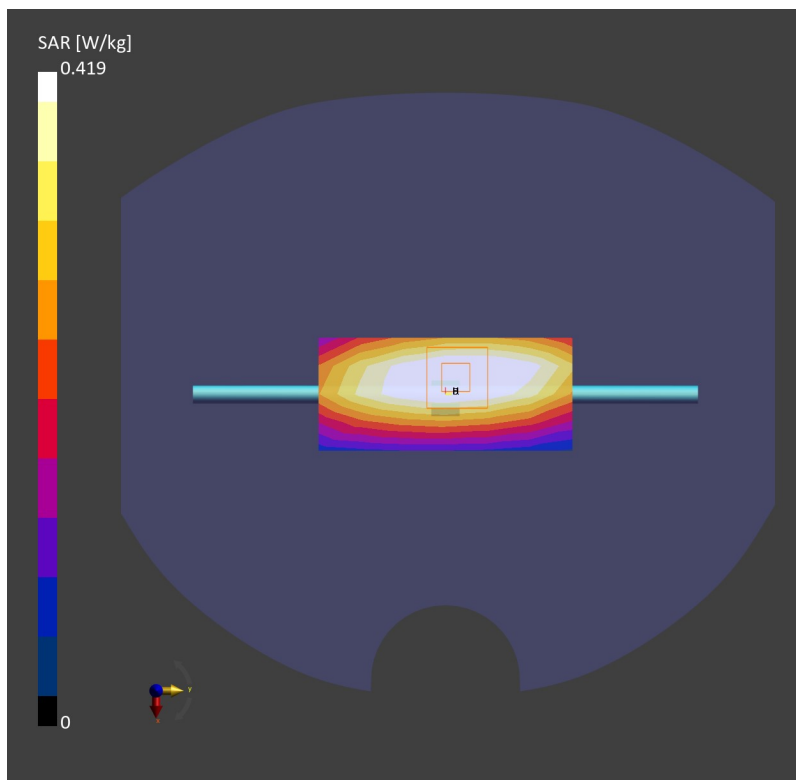

Date: 2025-07-13

System Check_Head_750MHz**DUT: D750V3 - SN1087**


Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1
Medium: HSL_750_250713 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.892$ S/m; $\epsilon_r = 42.9$
Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.71, 11.46, 9.89); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 0.406 W/kg; SAR (10g) = 0.275 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 0.421 W/kg; SAR (10g) = 0.277 W/kg
Smallest distance from peaks to all points 3 dB below = 13.7 mm
Ratio of SAR at M2 to SAR at M1 = 88.0 %

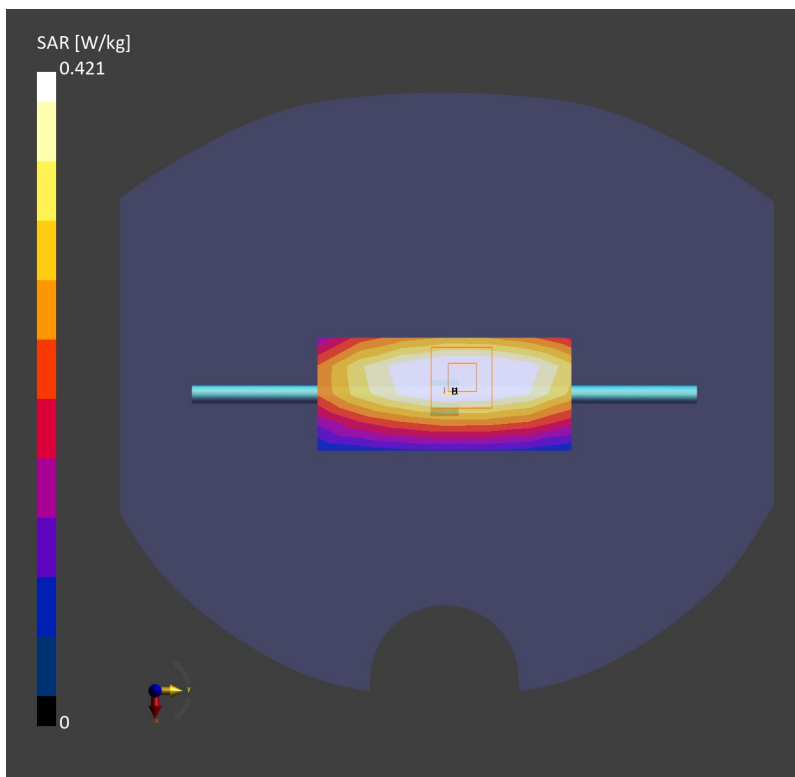

Date: 2025-08-01

System Check_Head_750MHz**DUT: D750V3 - SN1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL_750_250801 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.887$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.71, 11.46, 9.89); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.404 W/kg; SAR (10g) = 0.273 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm
x 1.5 mm

Power Drift = -0.07 dB

SAR (1g) = 0.403 W/kg; SAR (10g) = 0.276 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 90.6 %

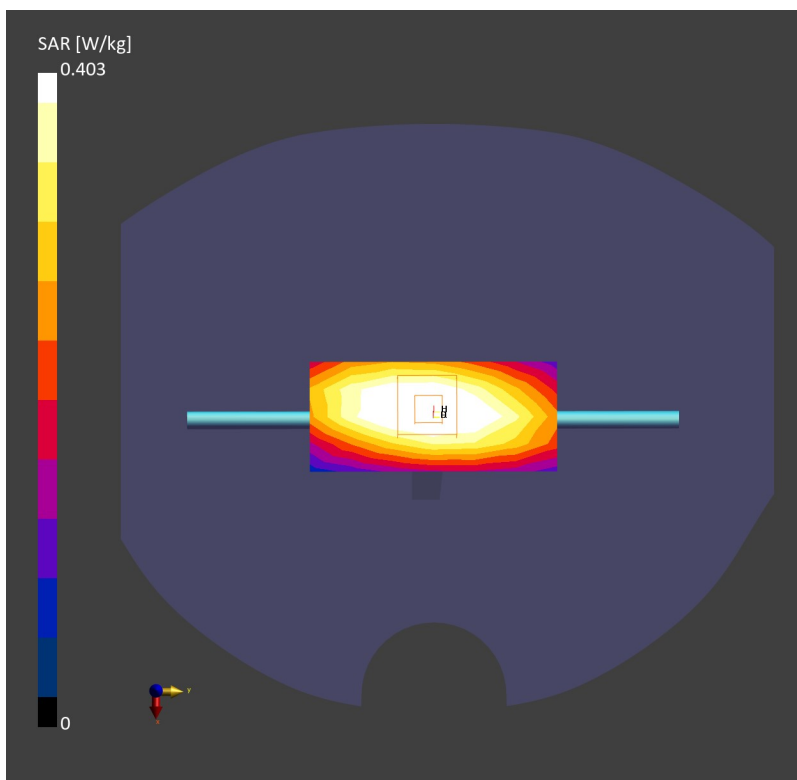

Date: 2025-07-06

System Check_Head_835MHz**DUT: D835V2 - SN4d162**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_835_250706 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.914$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.47, 11.17, 9.64); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.440 W/kg; SAR (10g) = 0.292 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.14 dB

SAR (1g) = 0.432 W/kg; SAR (10g) = 0.289 W/kg

Smallest distance from peaks to all points 3 dB below = 17.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.9 %

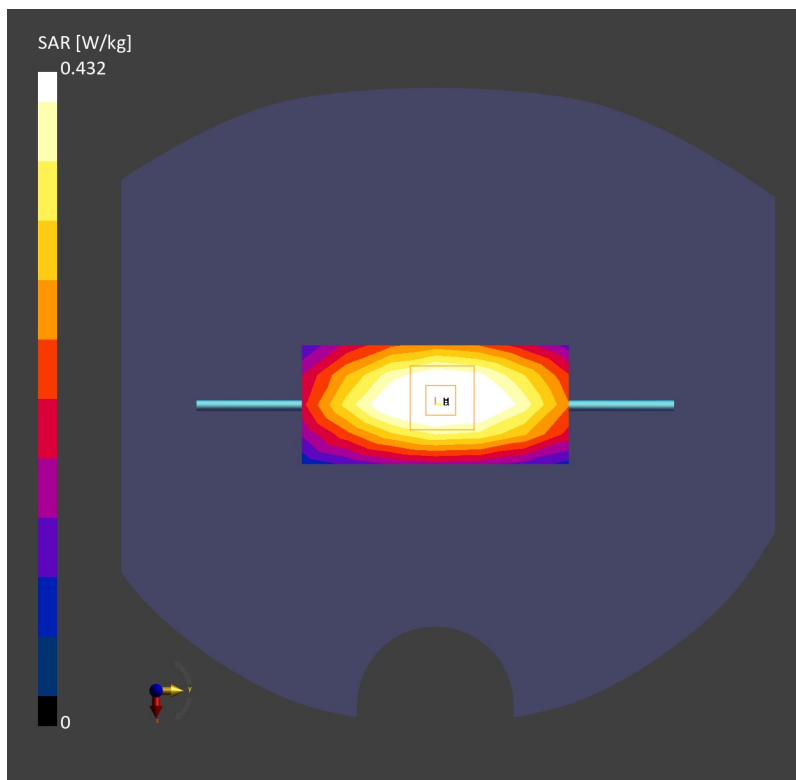

Date: 2025-07-14

System Check_Head_835MHz**DUT: D835V2 - SN4d162**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_835_250714 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.920$ S/m; $\epsilon_r = 42.6$


Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.47, 11.17, 9.64); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 0.415 W/kg; SAR (10g) = 0.276 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 0.423 W/kg; SAR (10g) = 0.284 W/kg
Smallest distance from peaks to all points 3 dB below = 17.0 mm
Ratio of SAR at M2 to SAR at M1 = 89.8 %

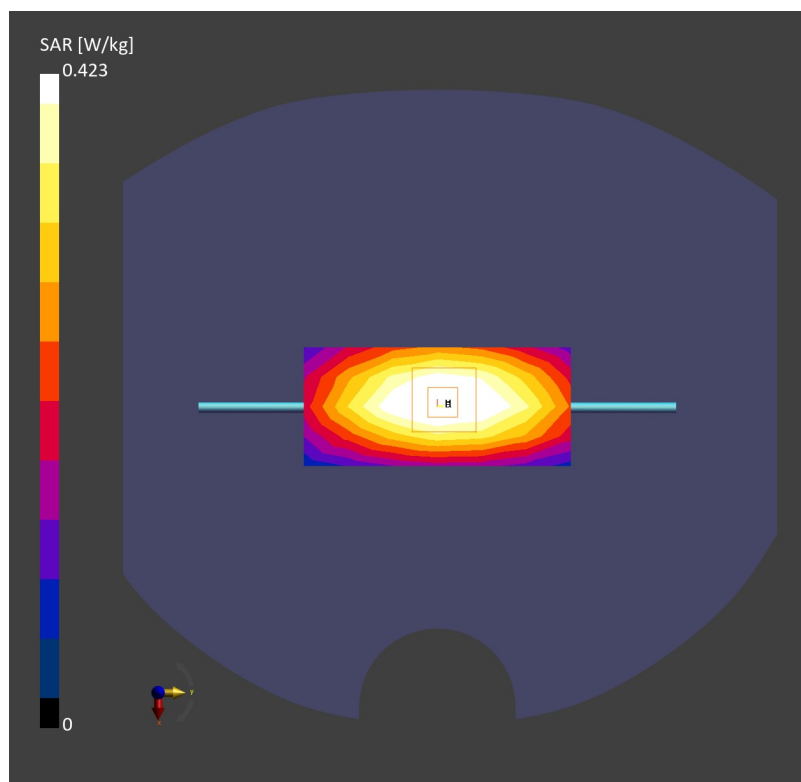

Date: 2025-08-02

System Check_Head_835MHz**DUT: D835V2 - SN4d162**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_835_250802 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.915$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.47, 11.17, 9.64); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.478 W/kg; SAR (10g) = 0.308 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm
x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 0.486 W/kg; SAR (10g) = 0.308 W/kg

Smallest distance from peaks to all points 3 dB below = 15.8 mm

Ratio of SAR at M2 to SAR at M1 = 90.9 %

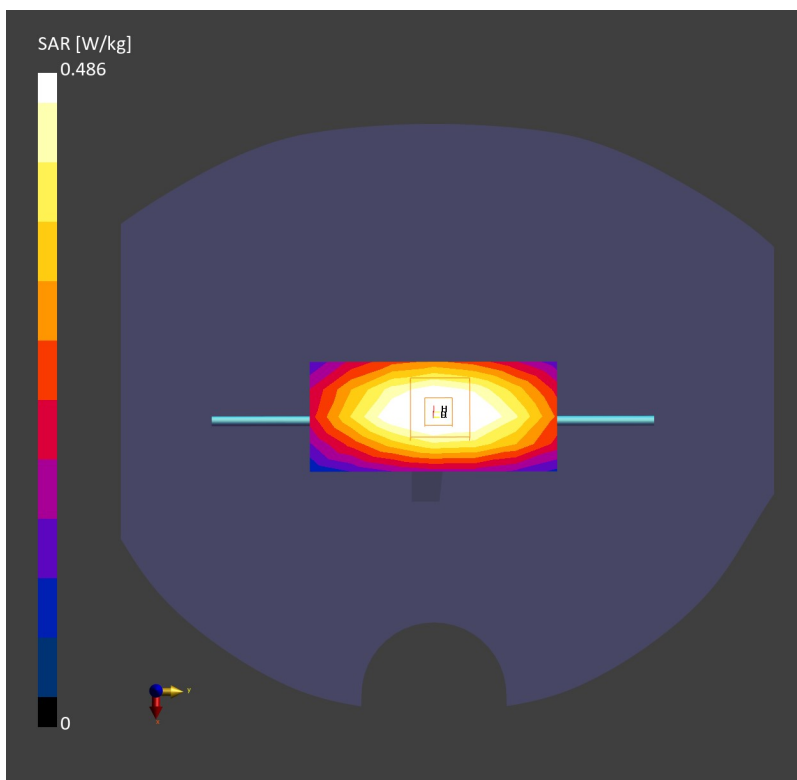

Date: 2025-07-07

System Check_Head_1750MHz**DUT: D1750V2 - SN1090**


Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1
Medium: HSL_1750_250707 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.6$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.83, 9.23, 7.96); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.73 W/kg; SAR (10g) = 0.928 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 1.75 W/kg; SAR (10g) = 0.962 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 86.3 %

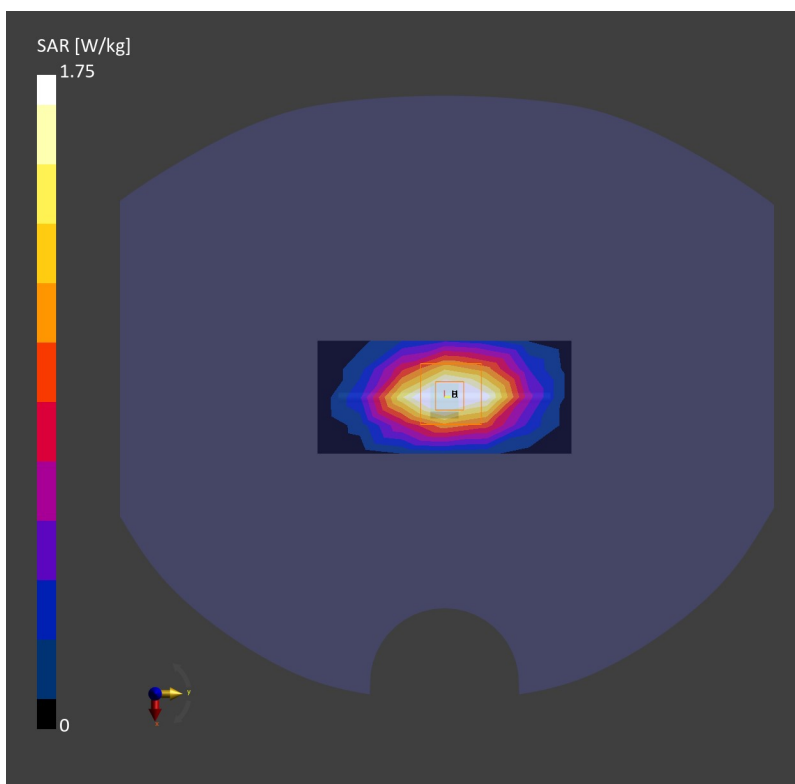

Date: 2025-07-15

System Check_Head_1750MHz**DUT: D1750V2 - SN1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1
Medium: HSL_1750_250715 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.7$


Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.83, 9.23, 7.96); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.65 W/kg; SAR (10g) = 0.912 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 1.74 W/kg; SAR (10g) = 0.958 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 87.3 %

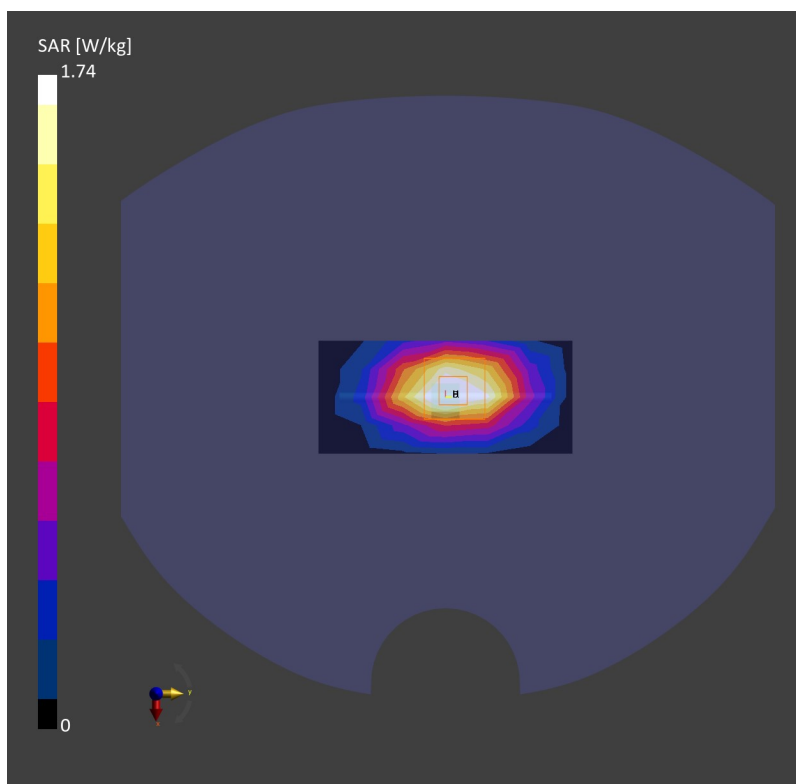

Date: 2025-08-03

System Check_Head_1750MHz**DUT: D1750V2 - SN1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: HSL_1750_250803 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.83, 9.23, 7.96); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.90 W/kg; SAR (10g) = 1.05 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm
x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.5 %

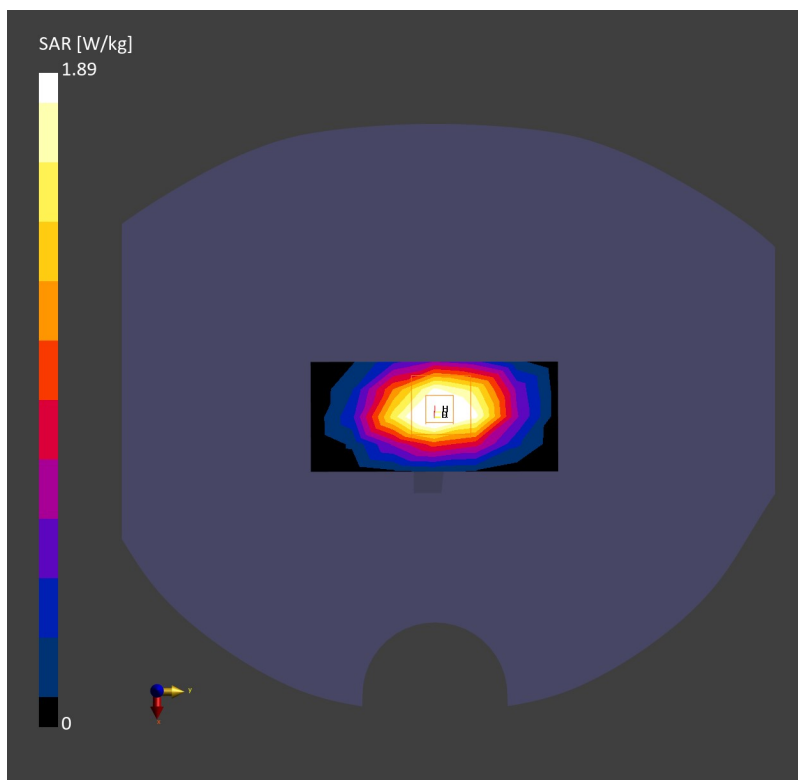

Date: 2025-07-08

System Check_Head_1900MHz**DUT: D1900V2 - SN5d170**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL_1900_250708 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.58, 8.94, 7.72); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.97 W/kg; SAR (10g) = 1.03 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 1.97 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

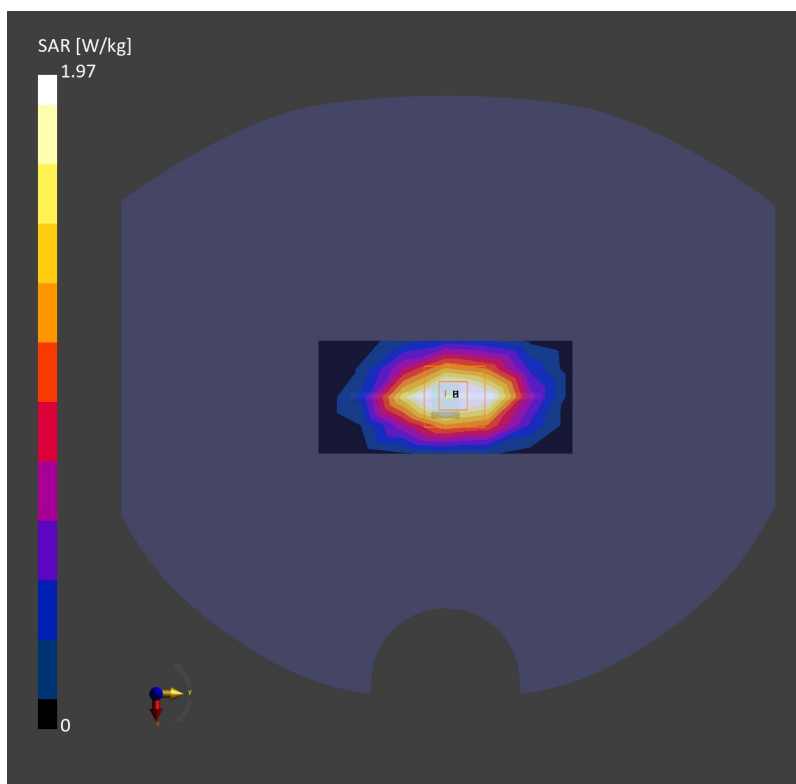

Date: 2025-07-16

System Check_Head_1900MHz**DUT: D1900V2 - SN5d170**


Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1
Medium: HSL_1900_250716 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.1$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.58, 8.94, 7.72); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.01 W/kg; SAR (10g) = 1.05 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 2.04 W/kg; SAR (10g) = 1.11 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 86.9 %

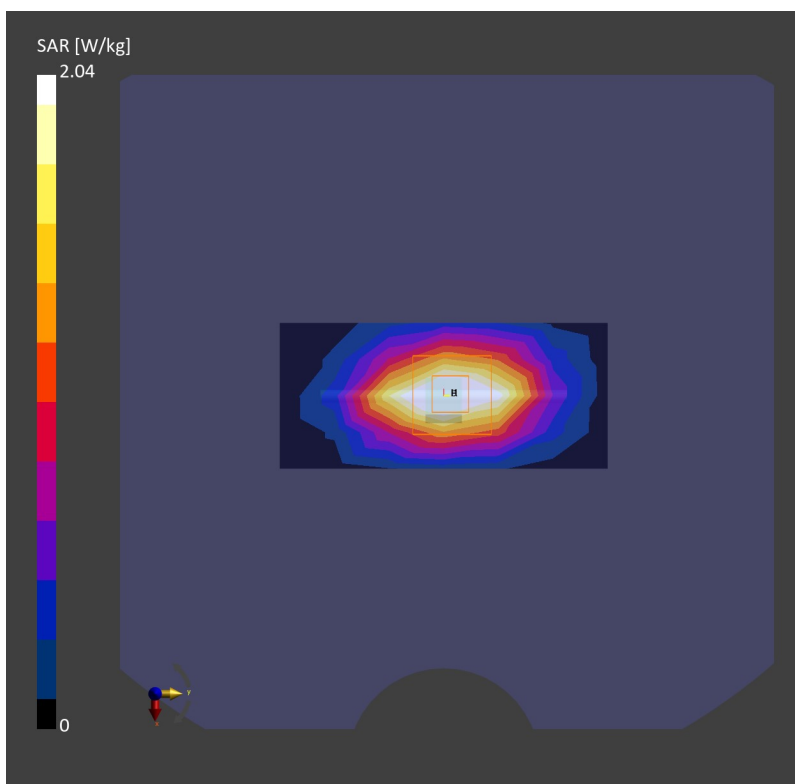

Date: 2025-08-04

System Check_Head_1900MHz**DUT: D1900V2 - SN5d170**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL_1900_250804 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.58, 8.94, 7.72); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 1.03 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm
x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.02 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.1 %

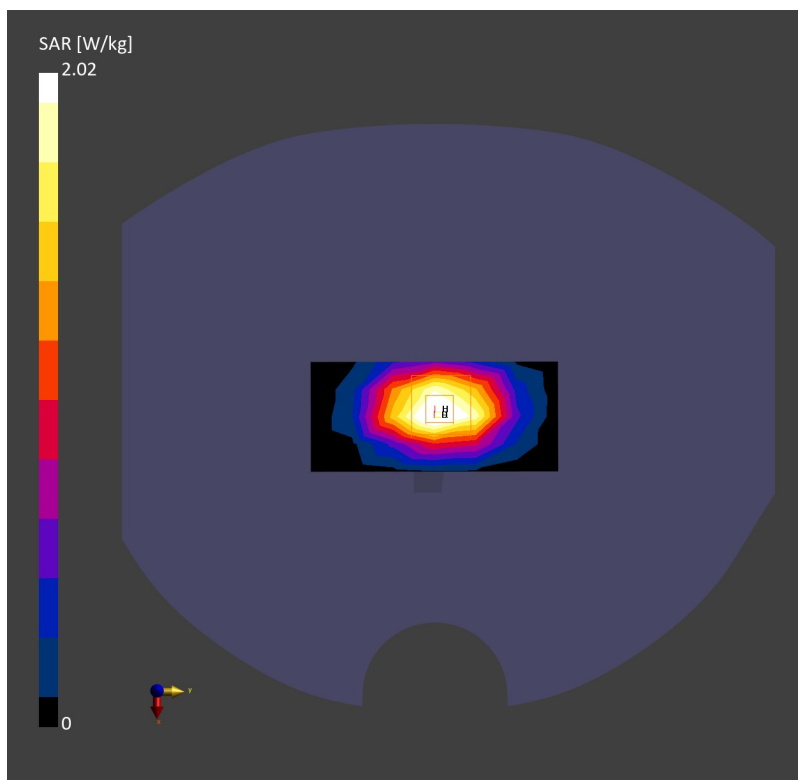

Date: 2025-07-17

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**


Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1
Medium: HSL_2450_250717 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.77$ S/m; $\epsilon_r = 39.3$
Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(7.36, 7.16, 6.91); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.66 W/kg; SAR (10g) = 1.23 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.10 dB
SAR (1g) = 2.74 W/kg; SAR (10g) = 1.31 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 82.4 %

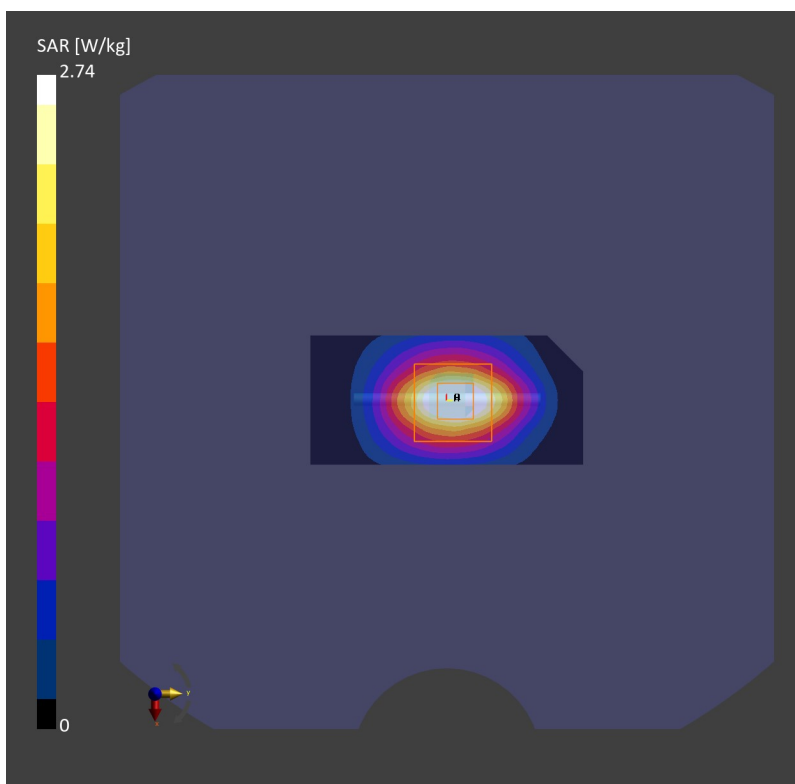

Date: 2025-07-09

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**


Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1
Medium: HSL_2600_250709 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 38.8$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.23, 8.53, 7.36); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.47 W/kg; SAR (10g) = 1.13 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.59 W/kg; SAR (10g) = 1.20 W/kg
Smallest distance from peaks to all points 3 dB below = 8.1 mm
Ratio of SAR at M2 to SAR at M1 = 82.5 %

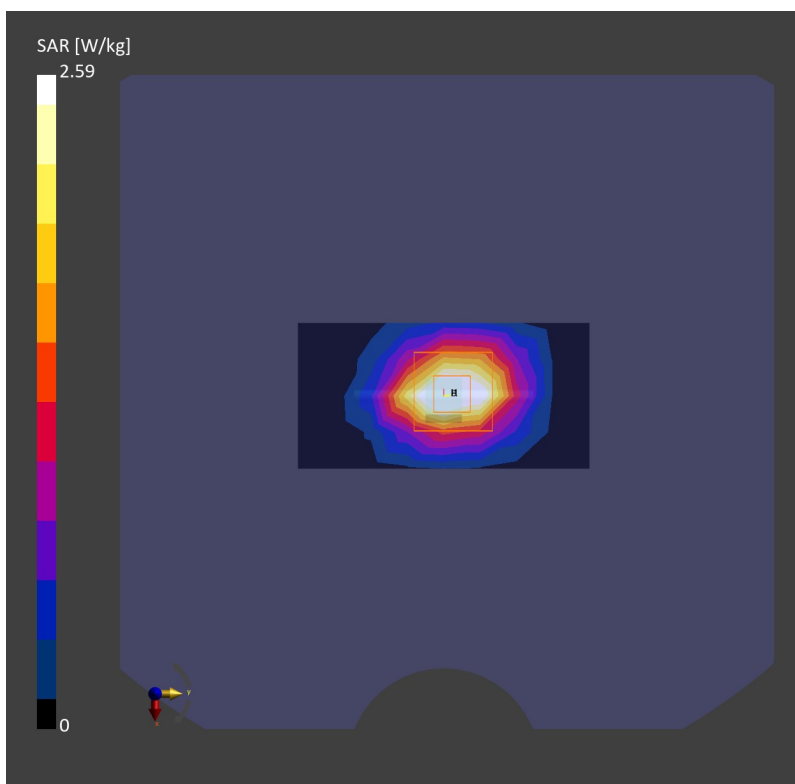

Date: 2025-07-17

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**


Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1
Medium: HSL_2600_250717 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.92$ S/m; $\epsilon_r = 38.8$
Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.23, 8.53, 7.36); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.50 W/kg; SAR (10g) = 1.14 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.61 W/kg; SAR (10g) = 1.21 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 82.3 %

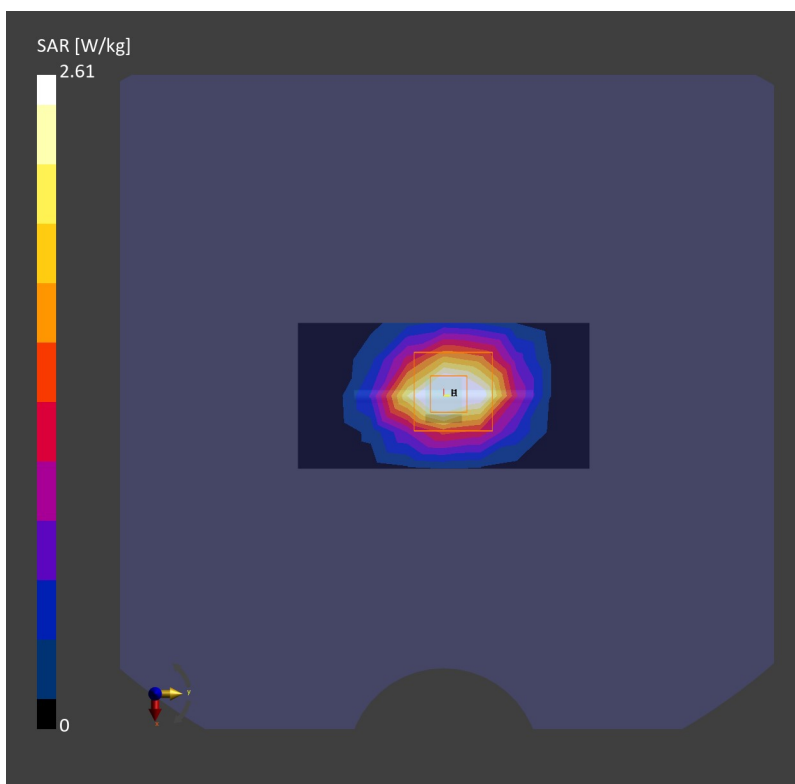

Date: 2025-08-05

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600_250805 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.92$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.23, 8.53, 7.36); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.12 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm
x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.60 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

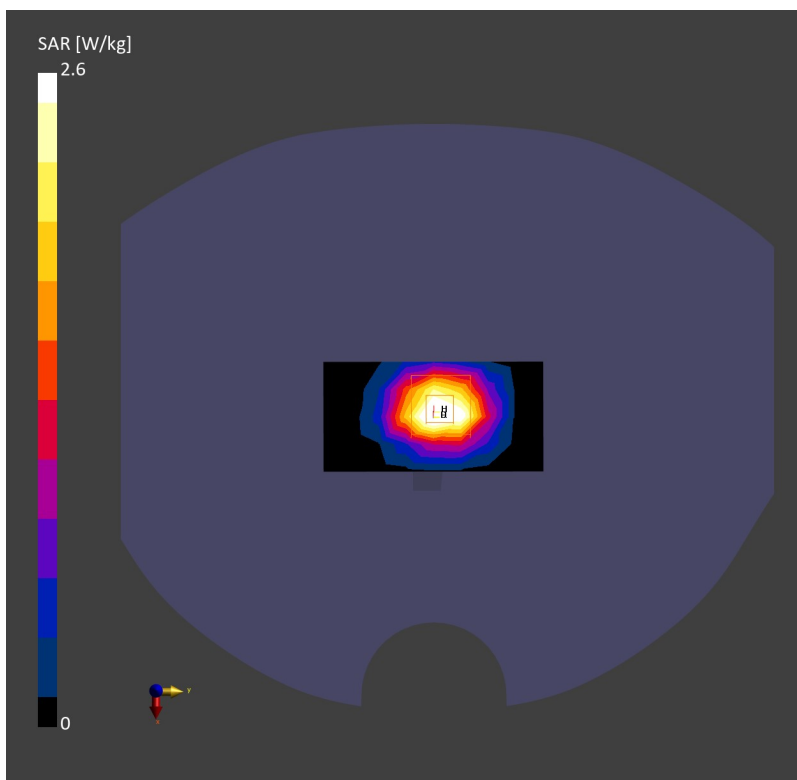

Date: 2025-07-10

System Check_Head_3500MHz**DUT: D3500V2 - SN1037**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1
Medium: HSL_3500_250710 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.97$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.79, 8.01, 6.91); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.03 W/kg; SAR (10g) = 1.17 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0mm
x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.2 %

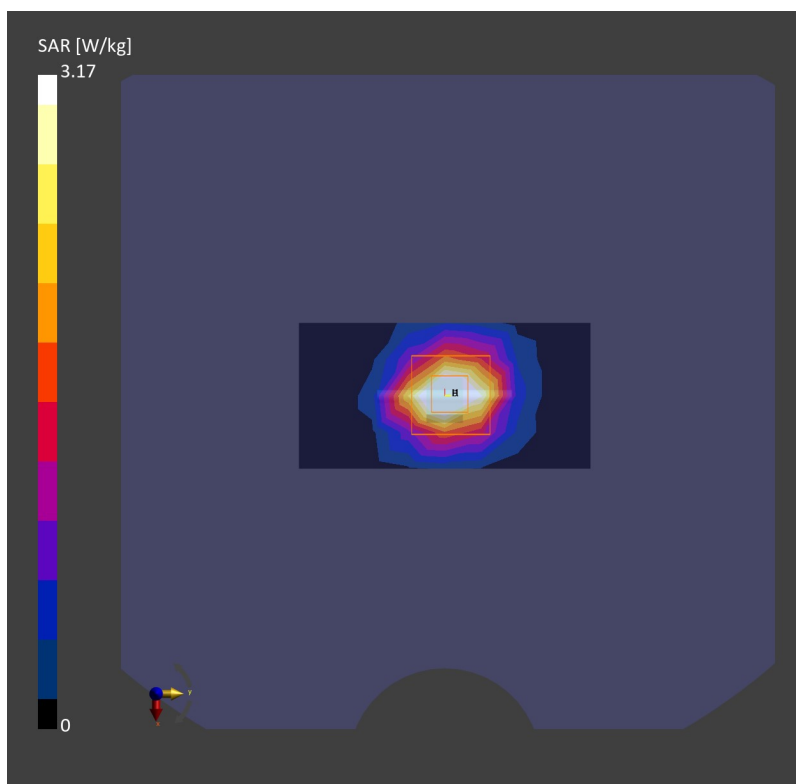

Date: 2025-07-18

System Check_Head_3500MHz**DUT: D3500V2 - SN1037**


Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1
 Medium: HSL_3500_250718 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.96$ S/m; $\epsilon_r = 37.6$
 Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.79, 8.01, 6.91); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
 SAR (1g) = 3.06 W/kg; SAR (10g) = 1.20 W/kg;

Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0mm
 x 1.4 mm
 Power Drift = 0.04 dB
 SAR (1g) = 3.32 W/kg; SAR (10g) = 1.31 W/kg
 Smallest distance from peaks to all points 3 dB below = 8.0 mm
 Ratio of SAR at M2 to SAR at M1 = 77.9 %

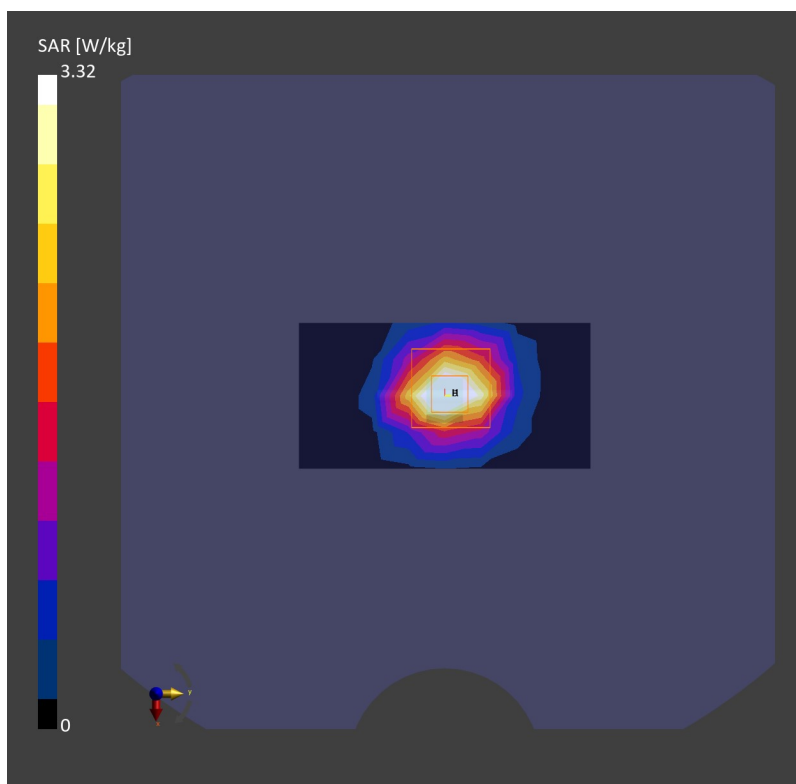

Date: 2025-07-11

System Check_Head_3700MHz**DUT: D3700V2 - SN1008**

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1
Medium: HSL_3700_250711 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.20$ S/m; $\epsilon_r = 37.5$


Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.84, 8.06, 6.96); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.97 W/kg; SAR (10g) = 1.15 W/kg;

Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0mm
x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 3.24 W/kg; SAR (10g) = 1.26 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 76.8 %

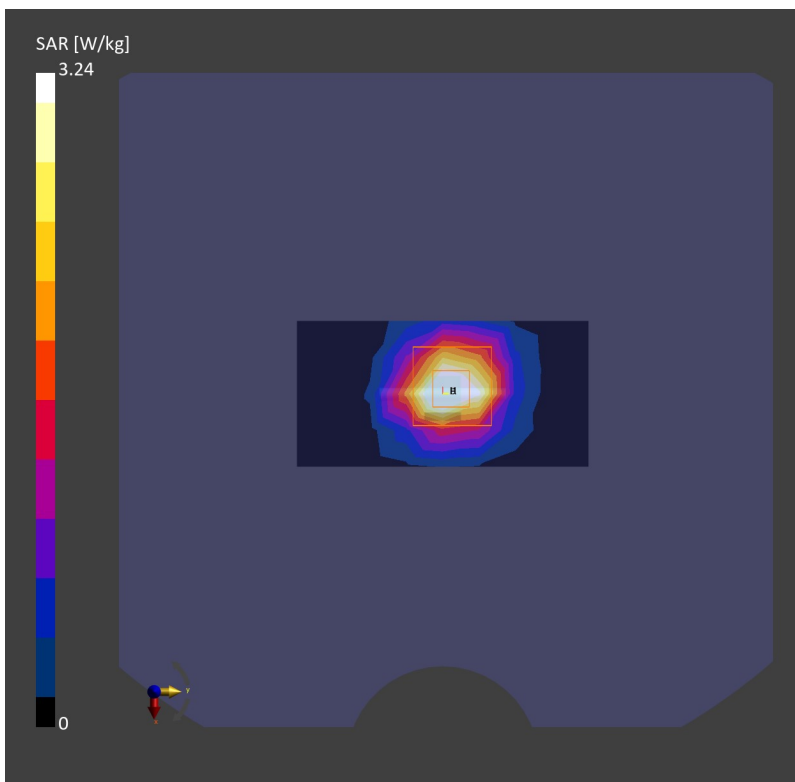

Date: 2025-07-19

System Check_Head_3700MHz**DUT: D3700V2 - SN1008**

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1
Medium: HSL_3700_250719 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.16$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.84, 8.06, 6.96); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.92 W/kg; SAR (10g) = 1.13 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0mm
x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.19 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.7 %

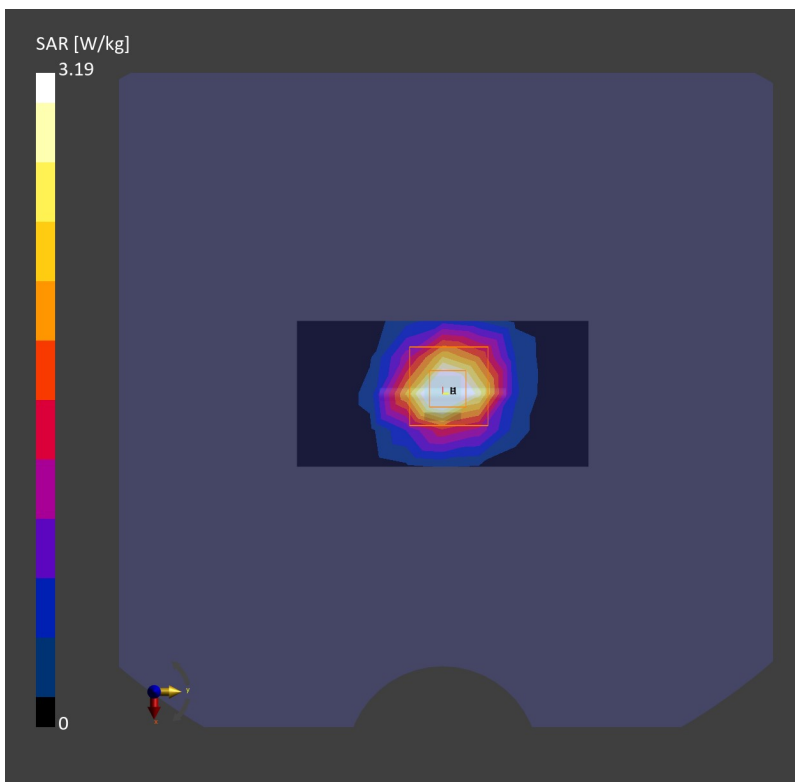

Date: 2025-07-12

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**


Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1
Medium: HSL_3900_250712 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.38$ S/m; $\epsilon_r = 37.3$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.66, 7.85, 6.77); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.52 W/kg; SAR (10g) = 1.33 W/kg;

Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0mm
x 1.4 mm
Power Drift = 0.03 dB
SAR (1g) = 3.56 W/kg; SAR (10g) = 1.23 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 78.0 %

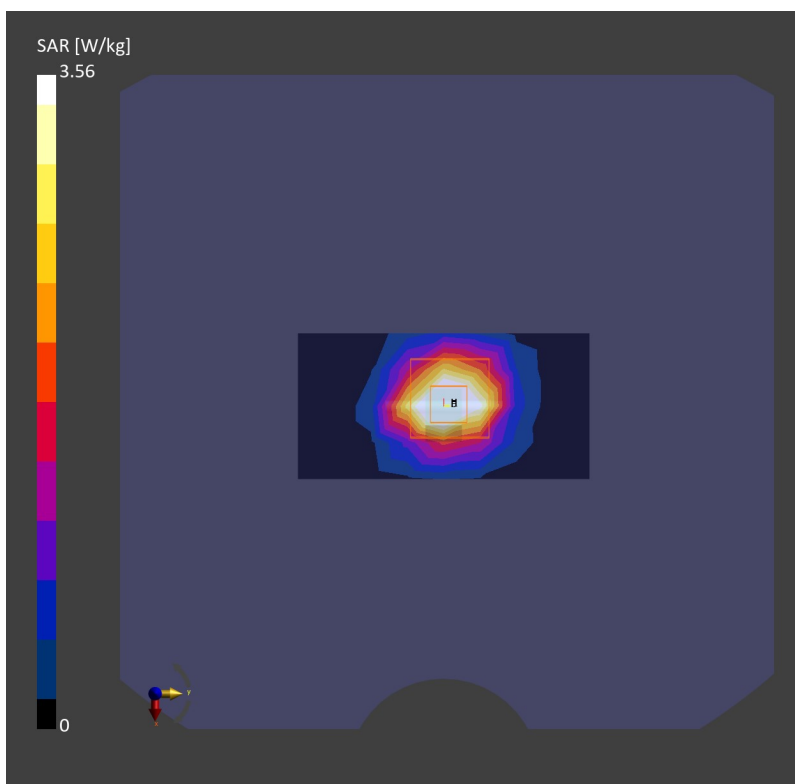

Date: 2025-07-20

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**


Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1
Medium: HSL_3900_250720 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.37$ S/m; $\epsilon_r = 37.4$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.66, 7.85, 6.77); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.51 W/kg; SAR (10g) = 1.33 W/kg;

Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0mm
x 1.4 mm
Power Drift = 0.03 dB
SAR (1g) = 3.55 W/kg; SAR (10g) = 1.22 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 78.3 %

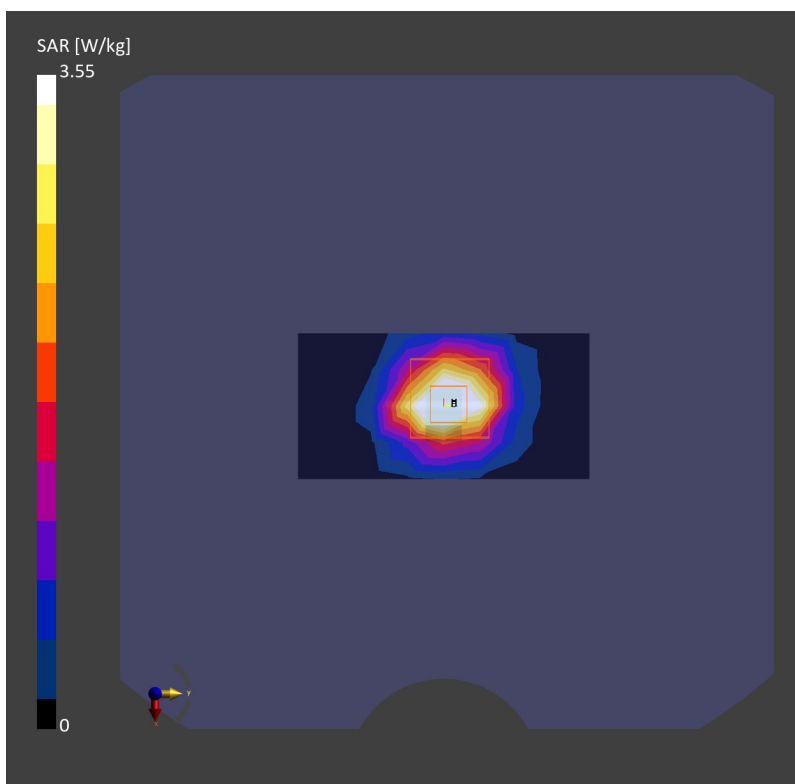

Date: 2025-07-18

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**


Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1
Medium: HSL_5250_250718 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.65$ S/m; $\epsilon_r = 36.2$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(5.93, 5.77, 5.57); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.28 W/kg; SAR (10g) = 0.993 W/kg;

Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.03 dB
SAR (1g) = 3.99 W/kg; SAR (10g) = 1.16 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 63.9 %

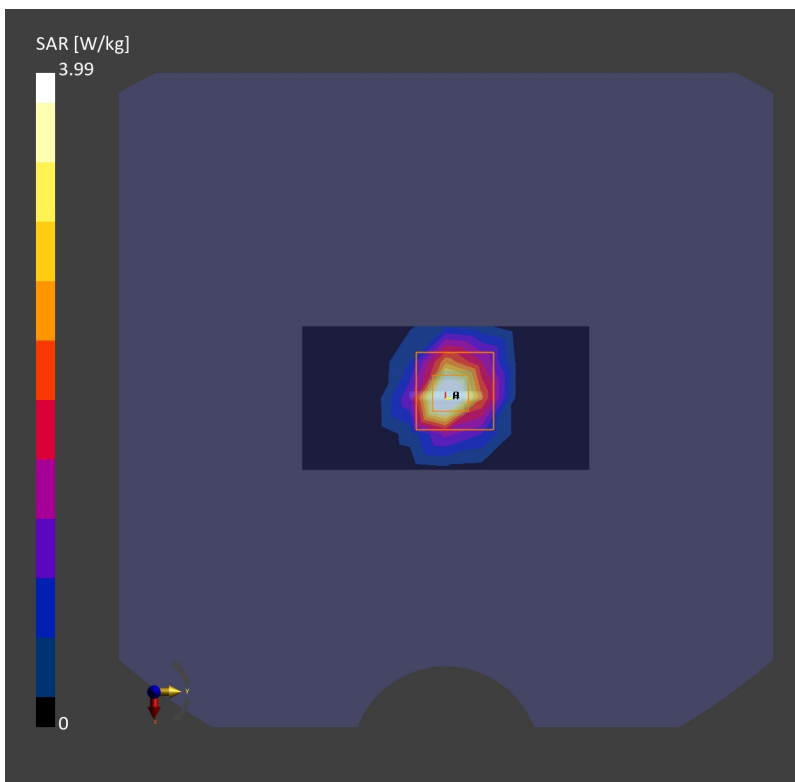

Date: 2025-07-19

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1
Medium: HSL_5600_250719 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.00$ S/m; $\epsilon_r = 35.7$


Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(5.42, 5.27, 5.08); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.44 W/kg; SAR (10g) = 1.02 W/kg;

Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.06 dB
SAR (1g) = 4.21 W/kg; SAR (10g) = 1.20 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 60.7 %

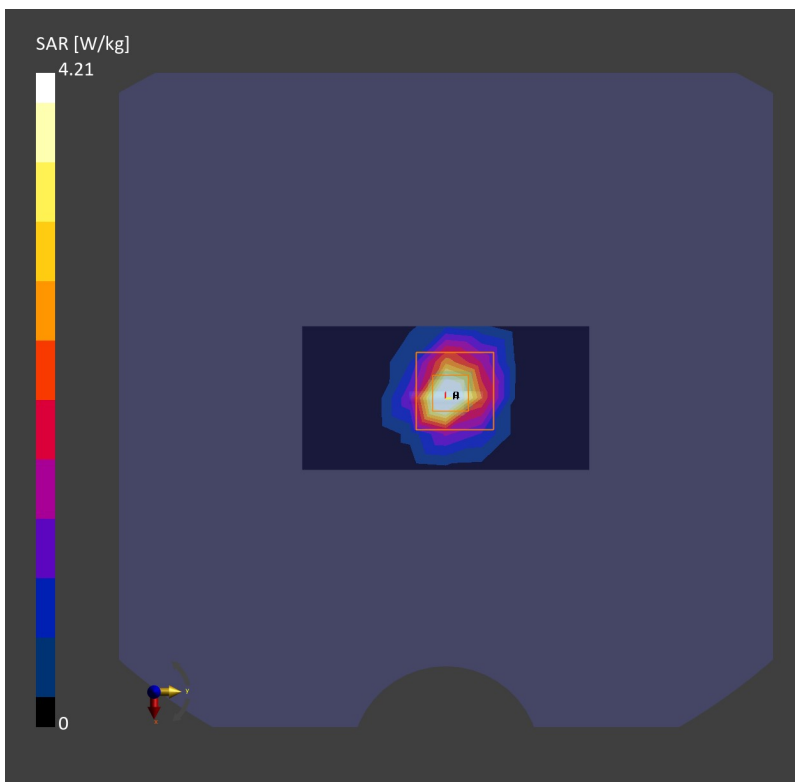

Date: 2025-07-20

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1
Medium: HSL_5750_250720 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.20$ S/m; $\epsilon_r = 35.6$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(5.53, 5.38, 5.19); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.04 W/kg; SAR (10g) = 0.949 W/kg;

Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.03 dB
SAR (1g) = 3.88 W/kg; SAR (10g) = 1.11 W/kg
Smallest distance from peaks to all points 3 dB below = 6.5 mm
Ratio of SAR at M2 to SAR at M1 = 58.4 %

