



DASY/EASY – Parameters of Probe: EX3DV4 – SN:3962

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	10.16	10.16	10.16	0.40	0.80	±12.1%
835	41.5	0.90	9.85	9.85	9.85	0.13	1.47	±12.1%
1750	40.1	1.37	8.50	8.50	8.50	0.20	1.08	±12.1%
1900	40.0	1.40	8.21	8.21	8.21	0.28	1.02	±12.1%
2300	39.5	1.67	7.95	7.95	7.95	0.48	0.73	±12.1%
2450	39.2	1.80	7.60	7.60	7.60	0.47	0.77	±12.1%
2600	39.0	1.96	7.42	7.42	7.42	0.63	0.68	±12.1%
3300	38.2	2.71	7.48	7.48	7.48	0.65	0.69	±13.3%
3500	37.9	2.91	7.07	7.07	7.07	0.49	0.83	±13.3%
3700	37.7	3.12	6.67	6.67	6.67	0.54	0.81	±13.3%
3900	37.5	3.32	6.56	6.56	6.56	0.35	1.21	±13.3%
4100	37.2	3.53	6.46	6.46	6.46	0.40	1.20	±13.3%
4400	36.9	3.84	6.33	6.33	6.33	0.35	1.35	±13.3%
4600	36.7	4.04	6.15	6.15	6.15	0.40	1.40	±13.3%
4800	36.4	4.25	5.98	5.98	5.98	0.45	1.35	±13.3%
4950	36.3	4.40	5.82	5.82	5.82	0.40	1.35	±13.3%
5250	35.9	4.71	5.56	5.56	5.56	0.45	1.20	±13.3%
5600	35.5	5.07	4.82	4.82	4.82	0.45	1.50	±13.3%
5750	35.4	5.22	4.88	4.88	4.88	0.50	1.40	±13.3%


^C Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.




Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

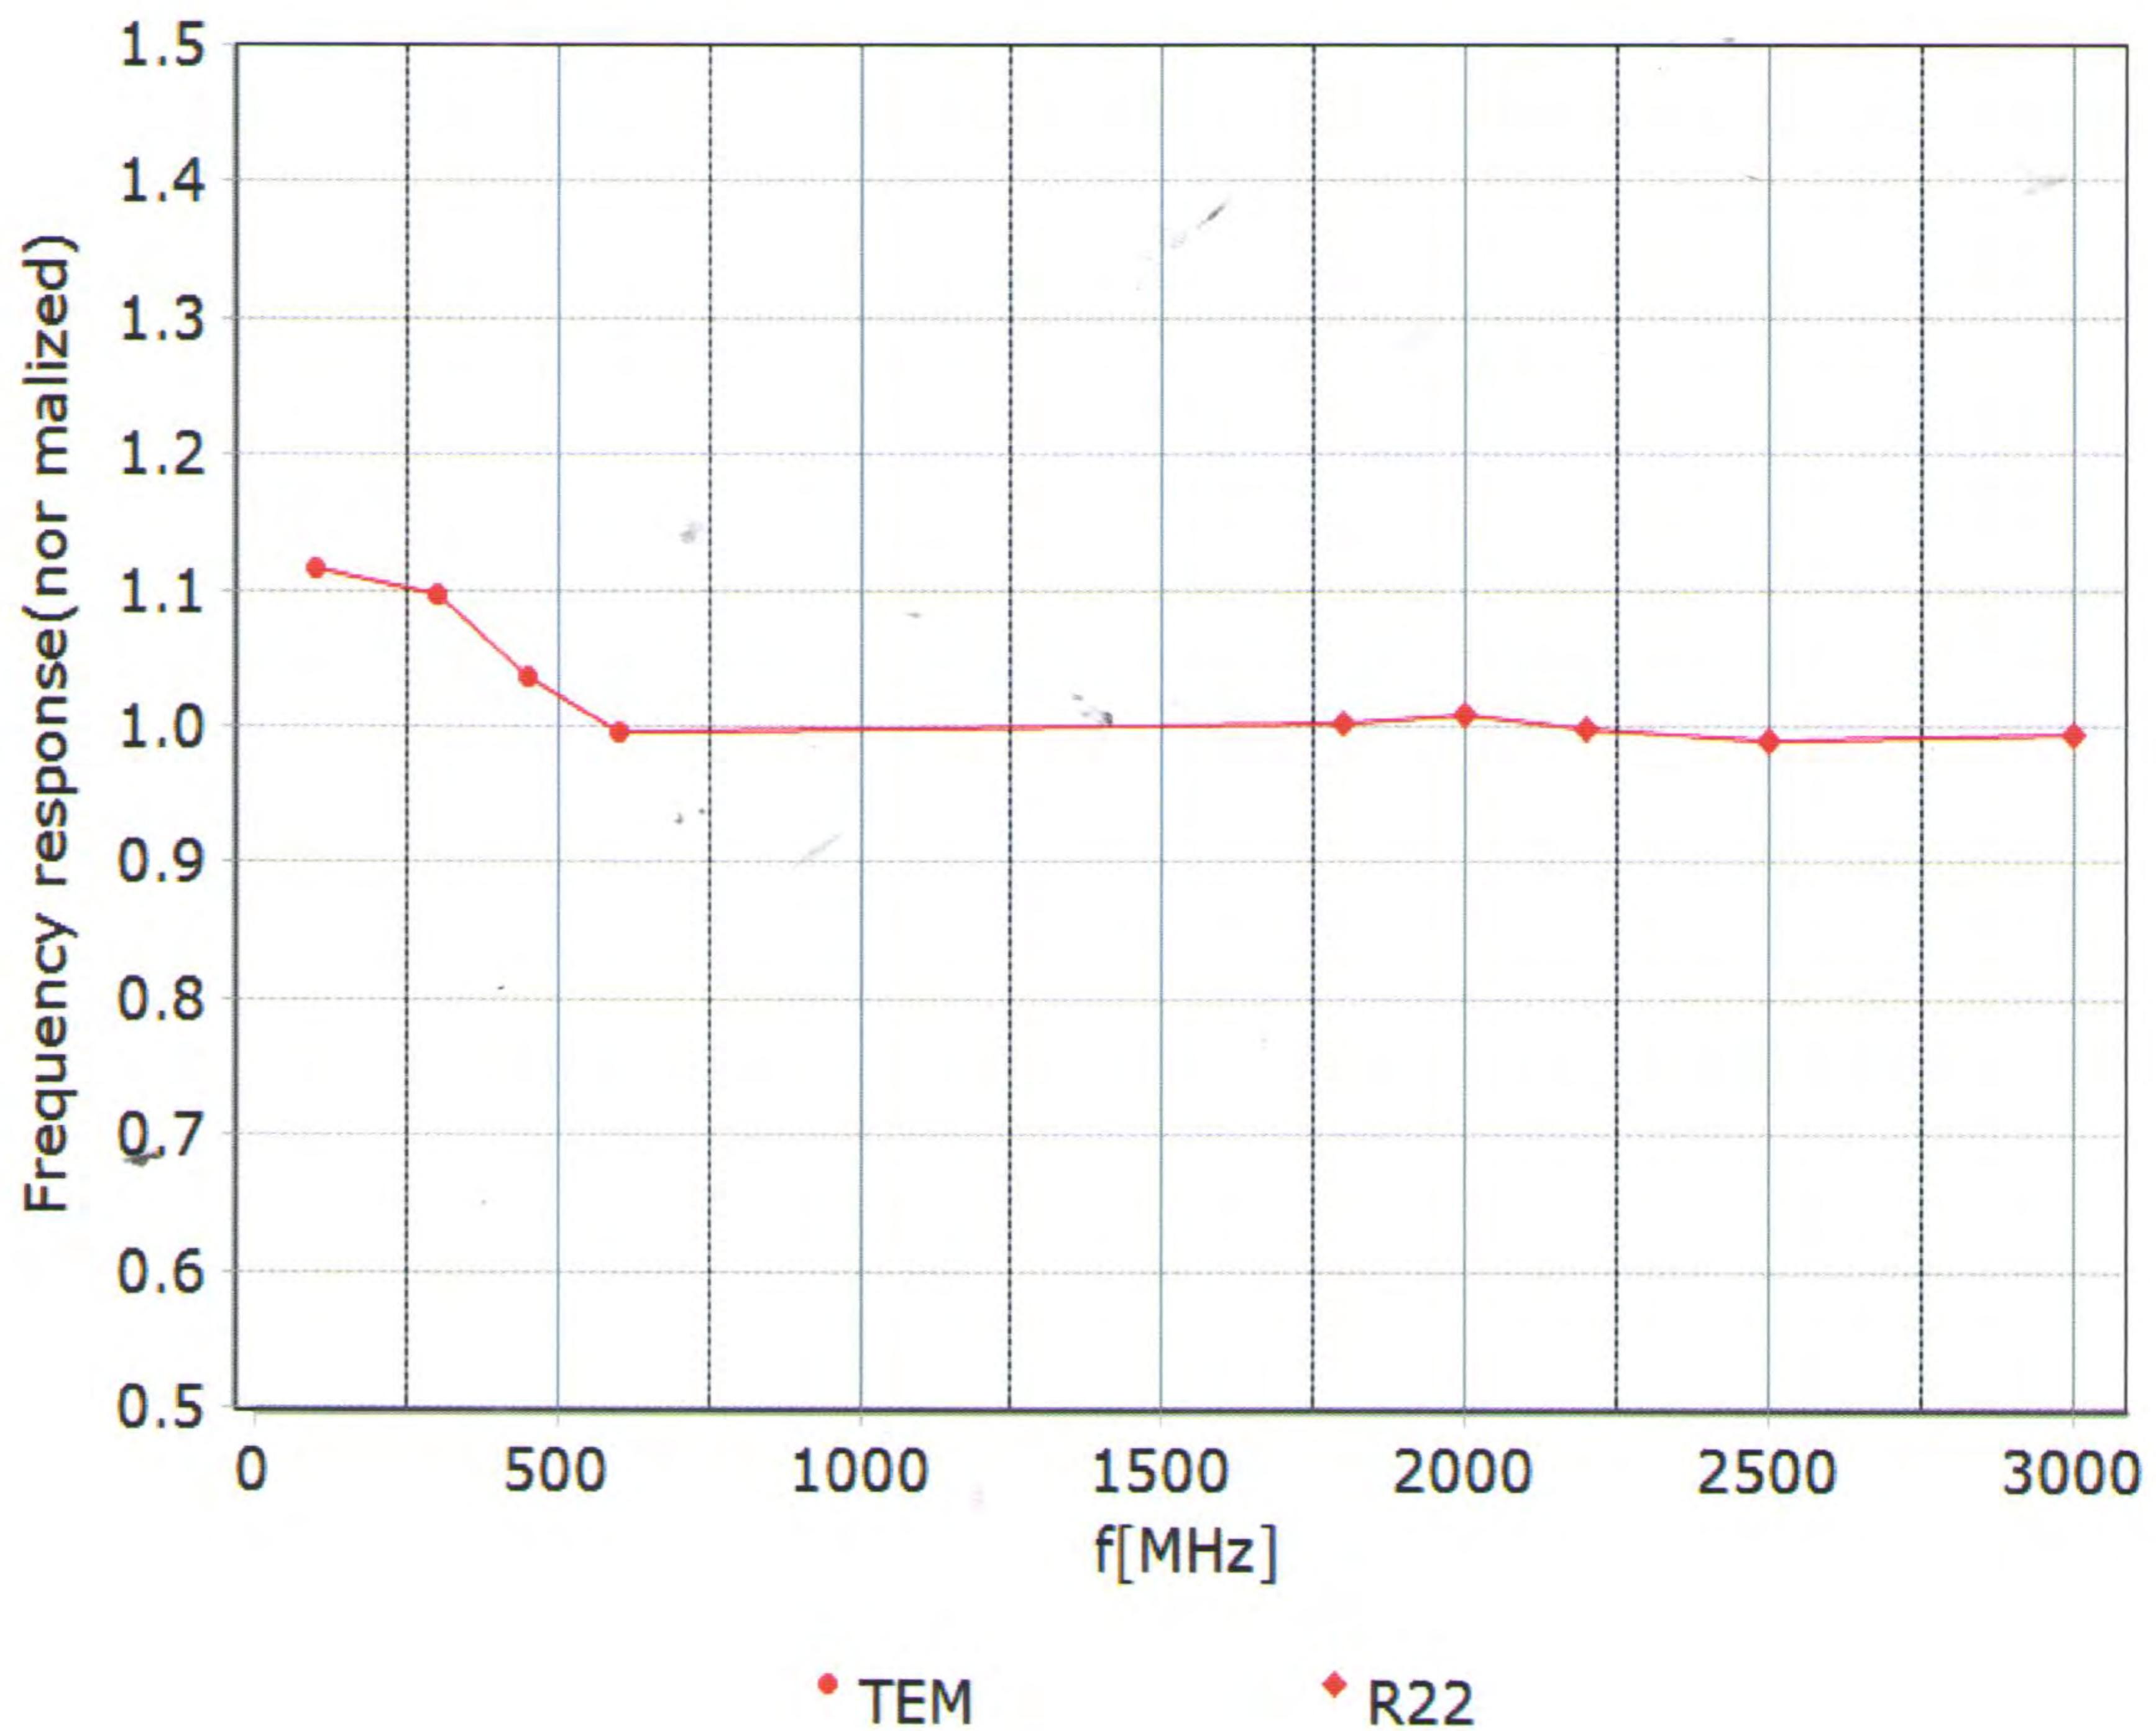



Uncertainty of Frequency Response of E-field: $\pm 7.4\%$ (k=2)

Receiving Pattern (Φ), $\theta=0^\circ$

f=600 MHz, TEM


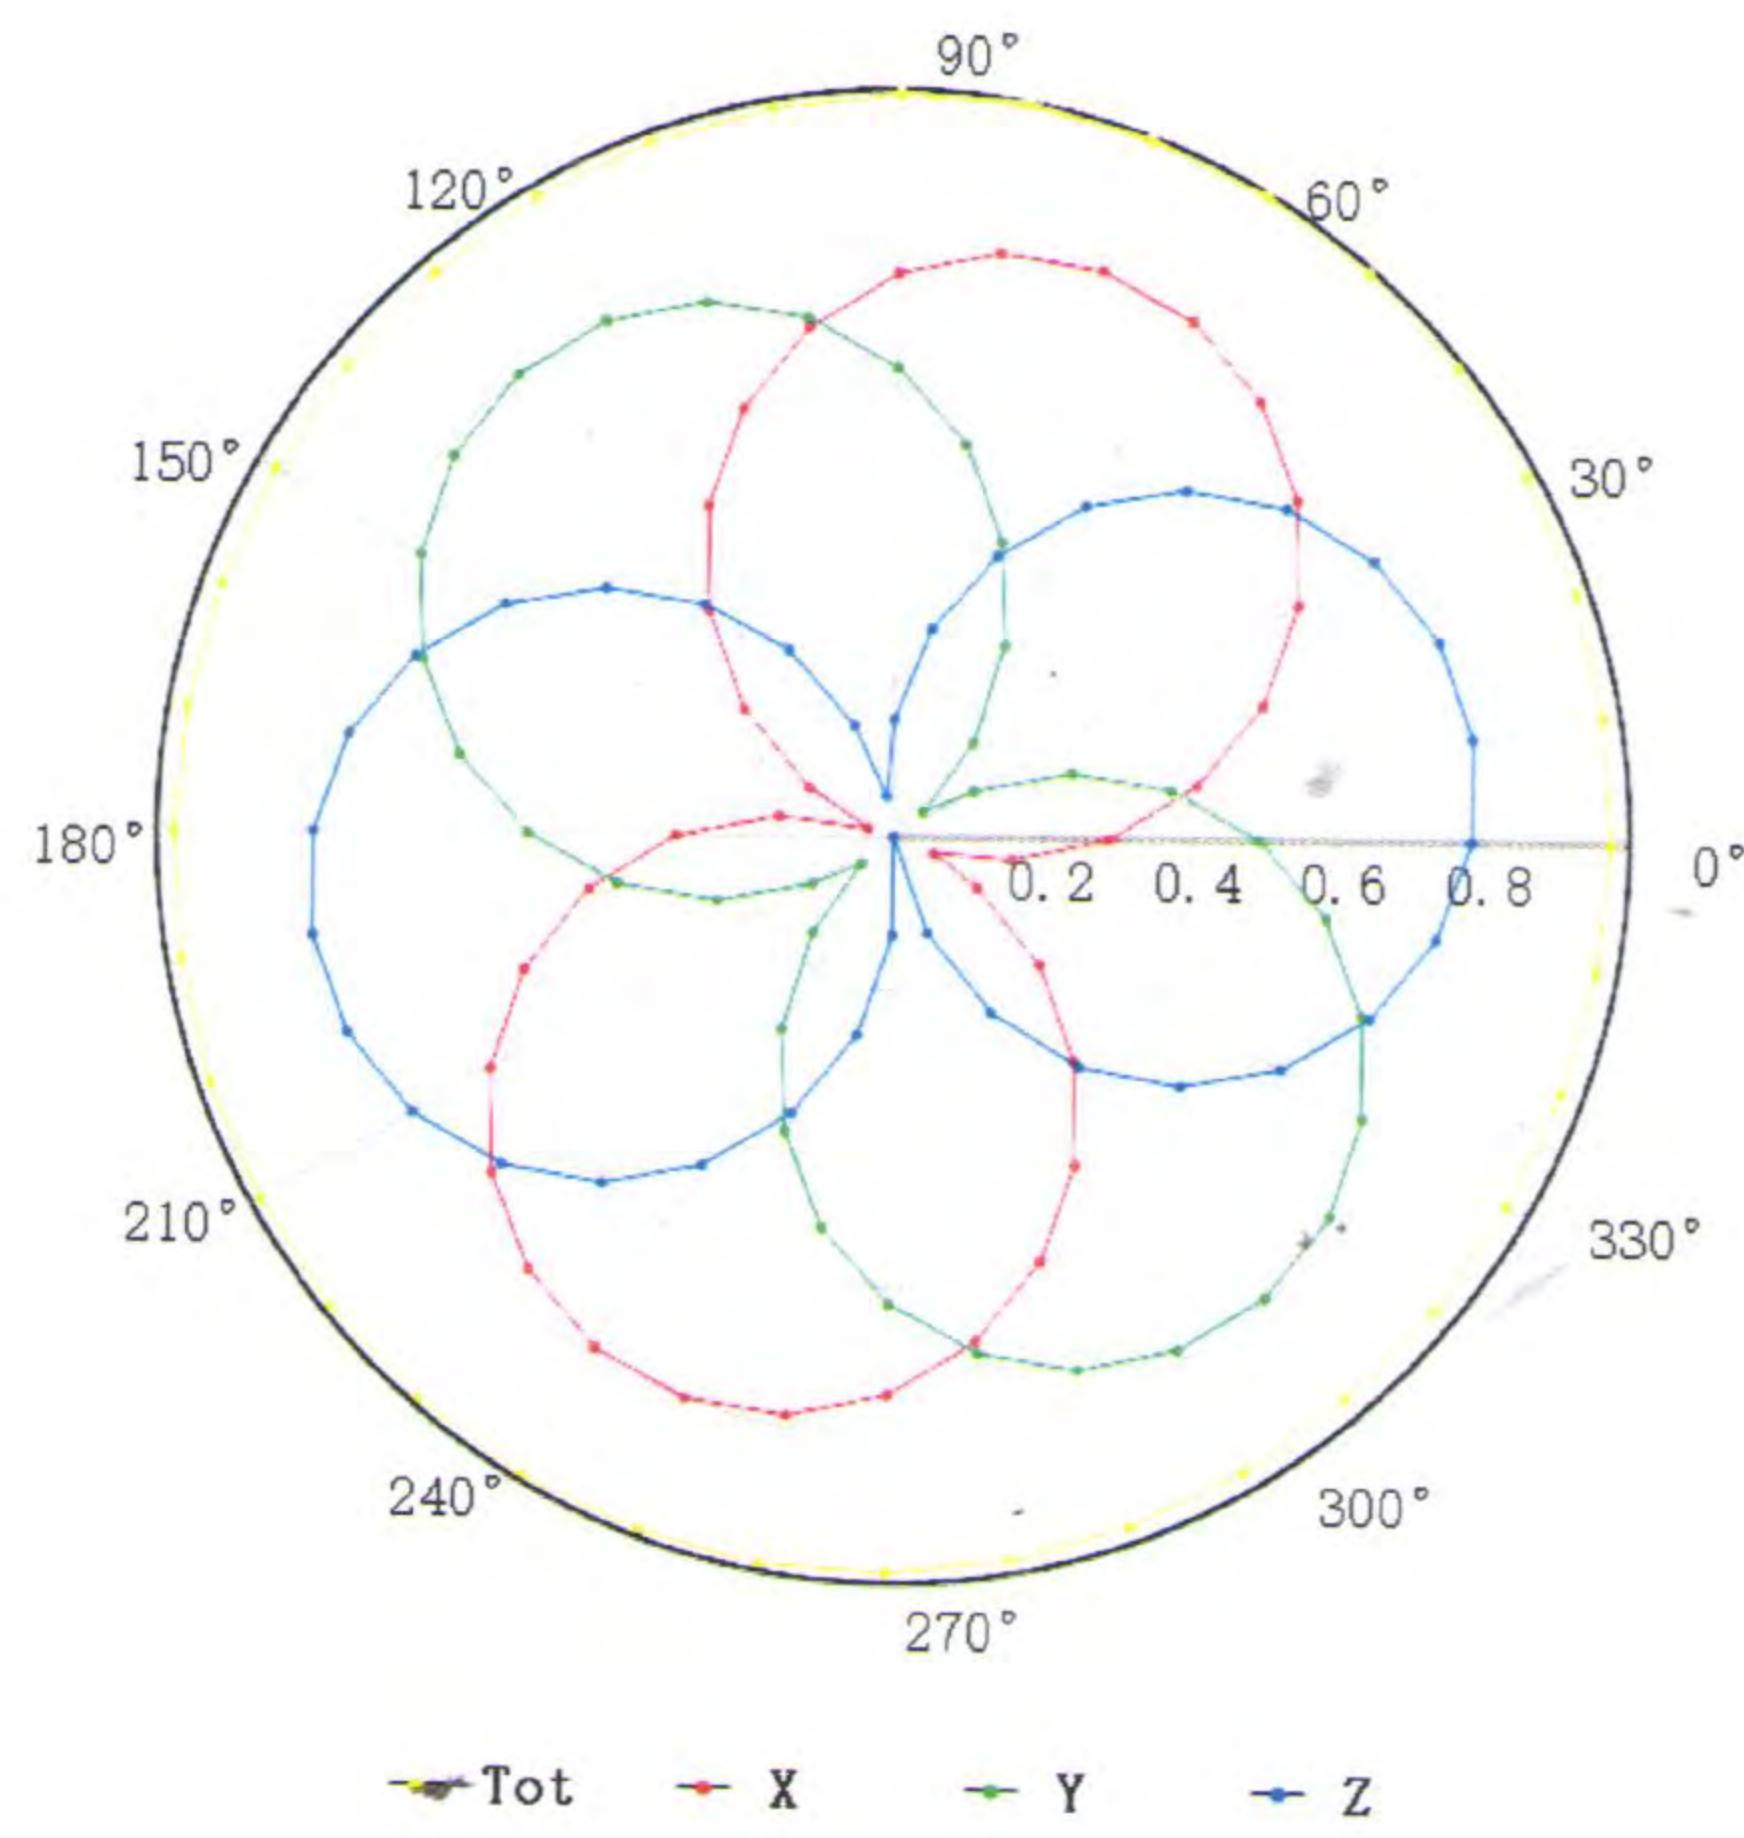


f=1800 MHz, R22

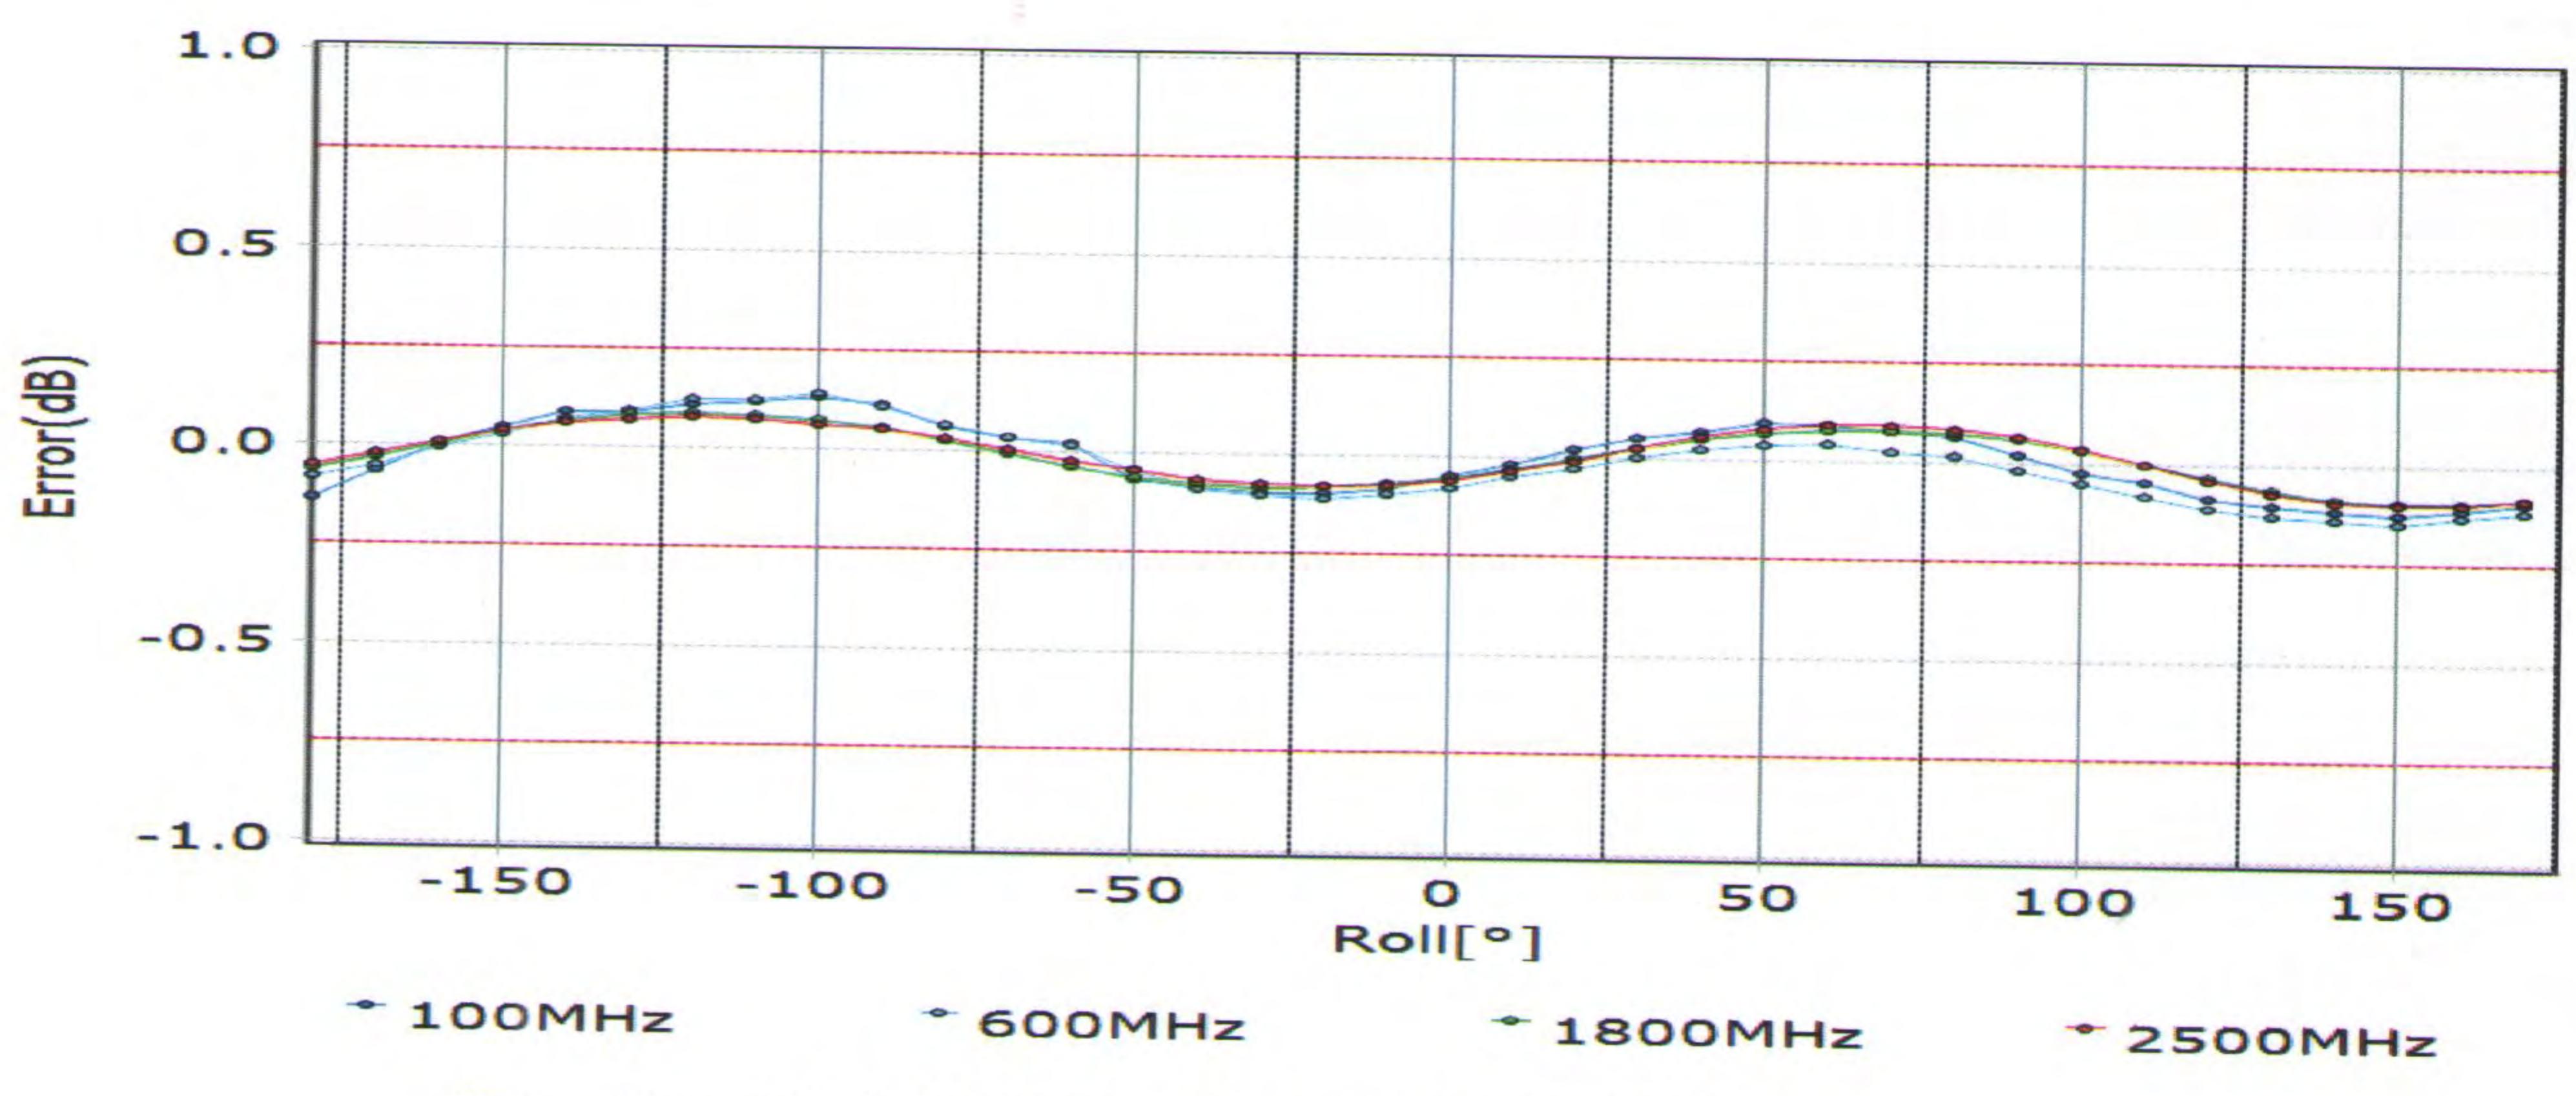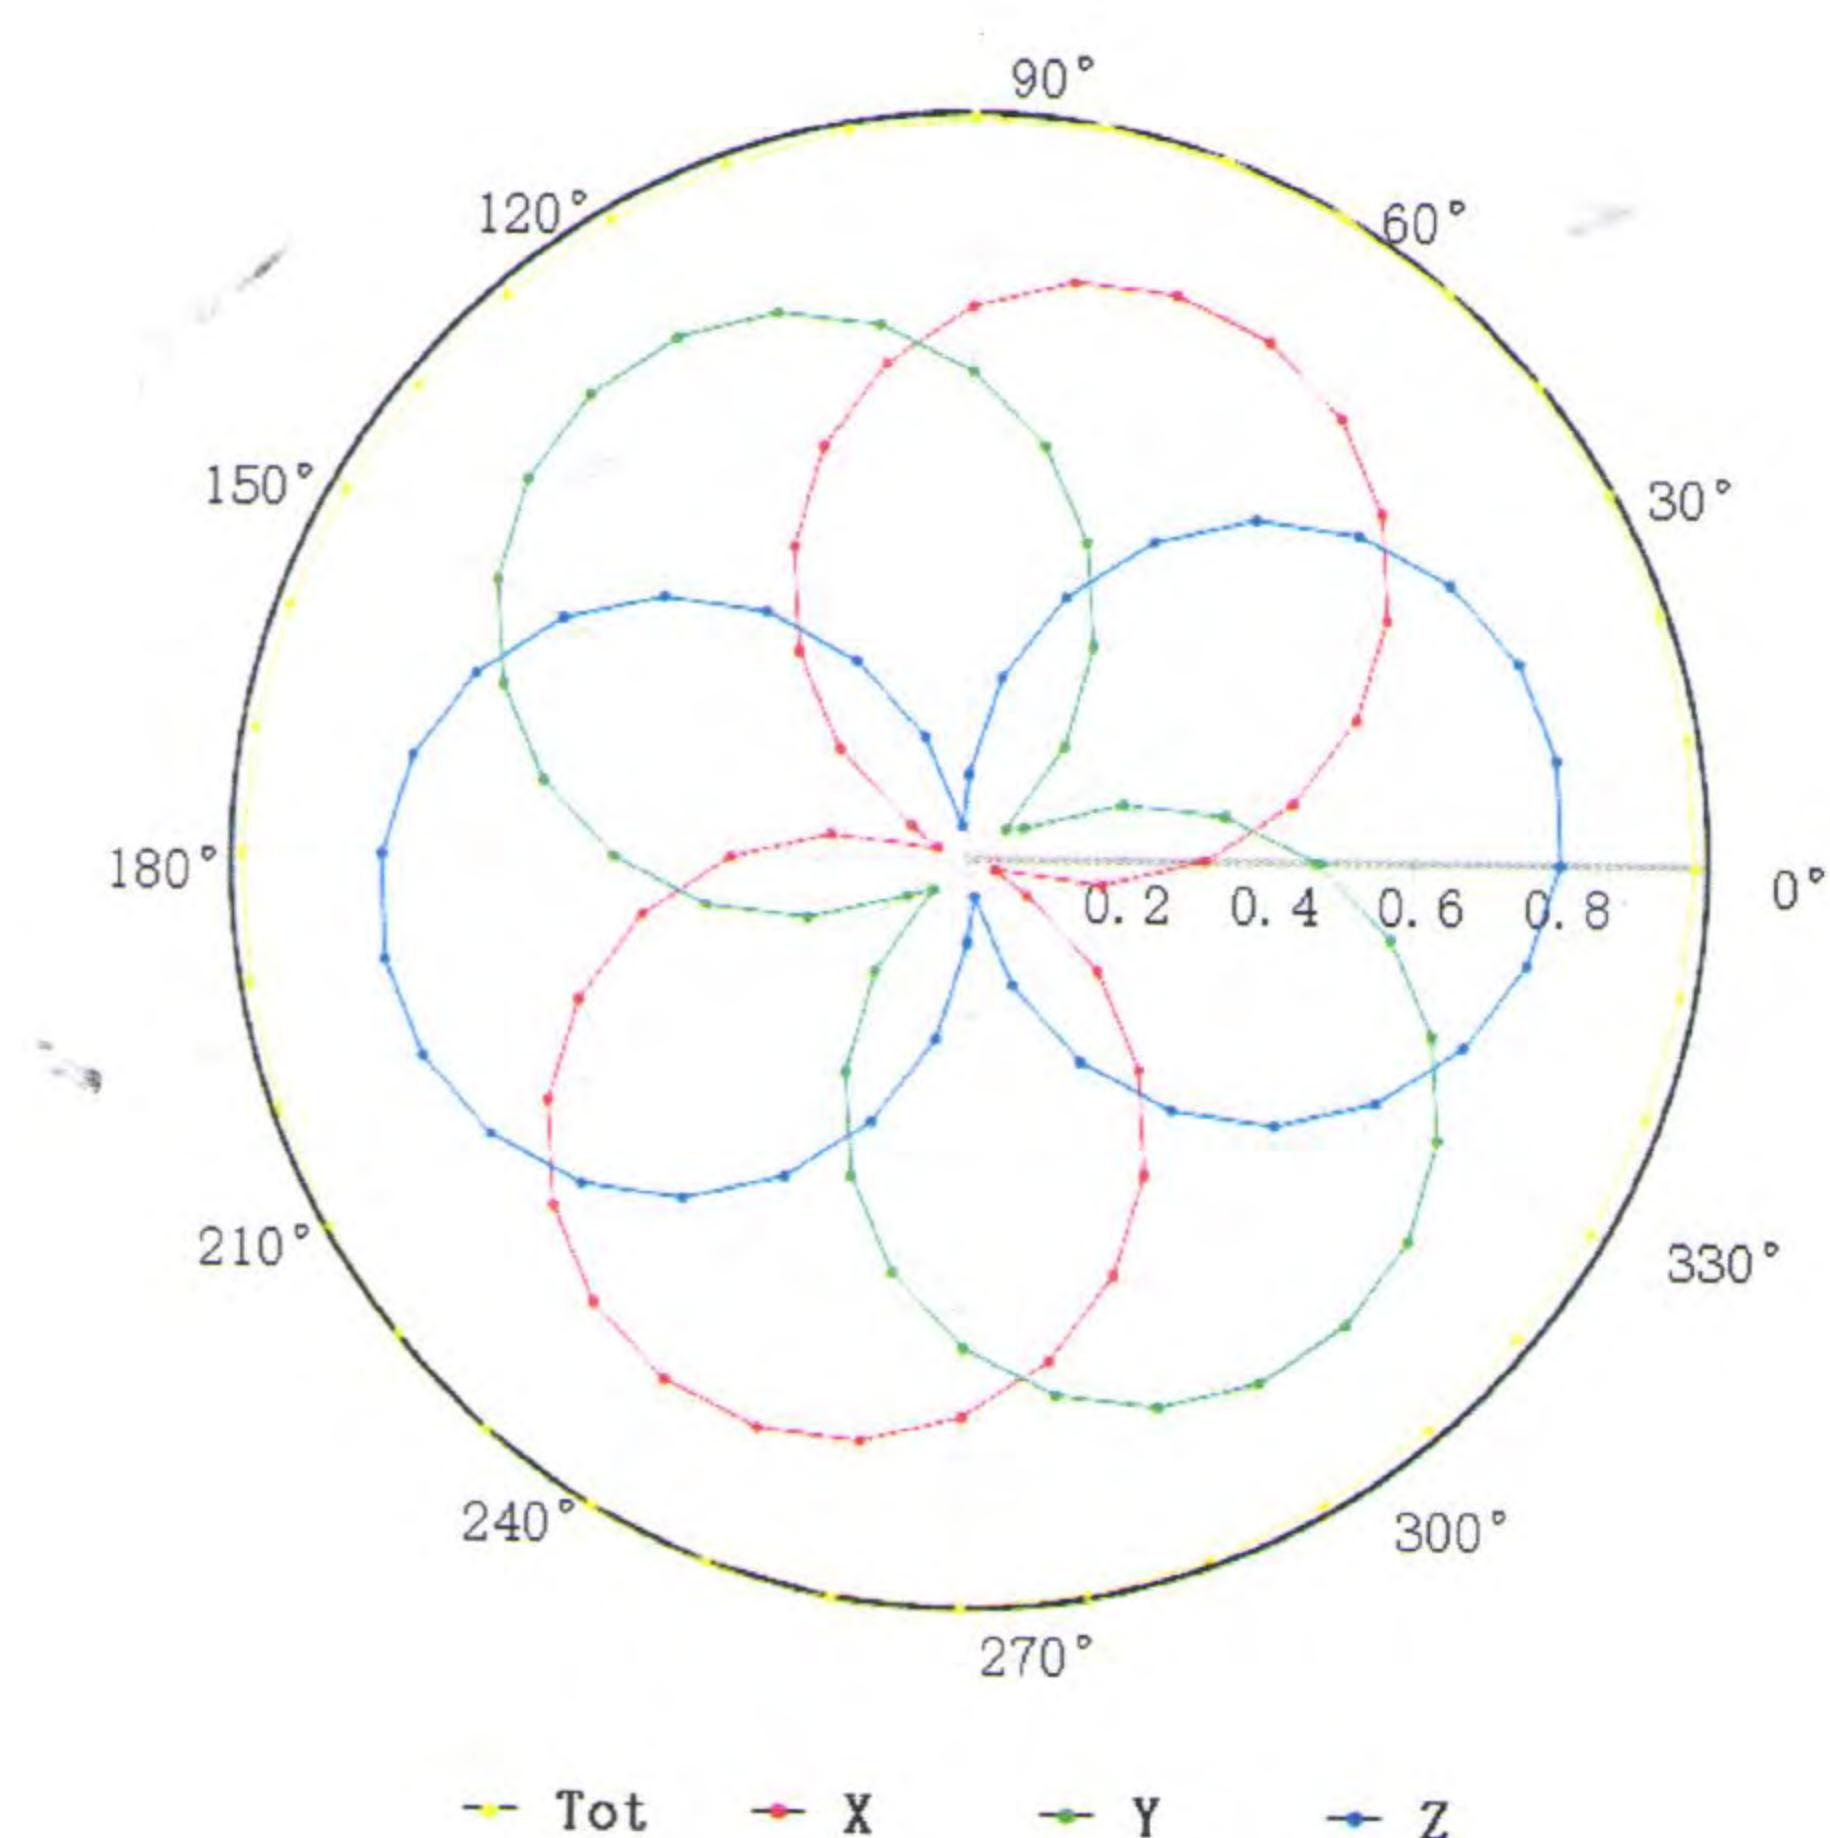

Uncertainty of Axial Isotropy Assessment: $\pm 1.2\%$ (k=2)

Dynamic Range f(SAR_{head}) (TEM cell, f = 900 MHz)

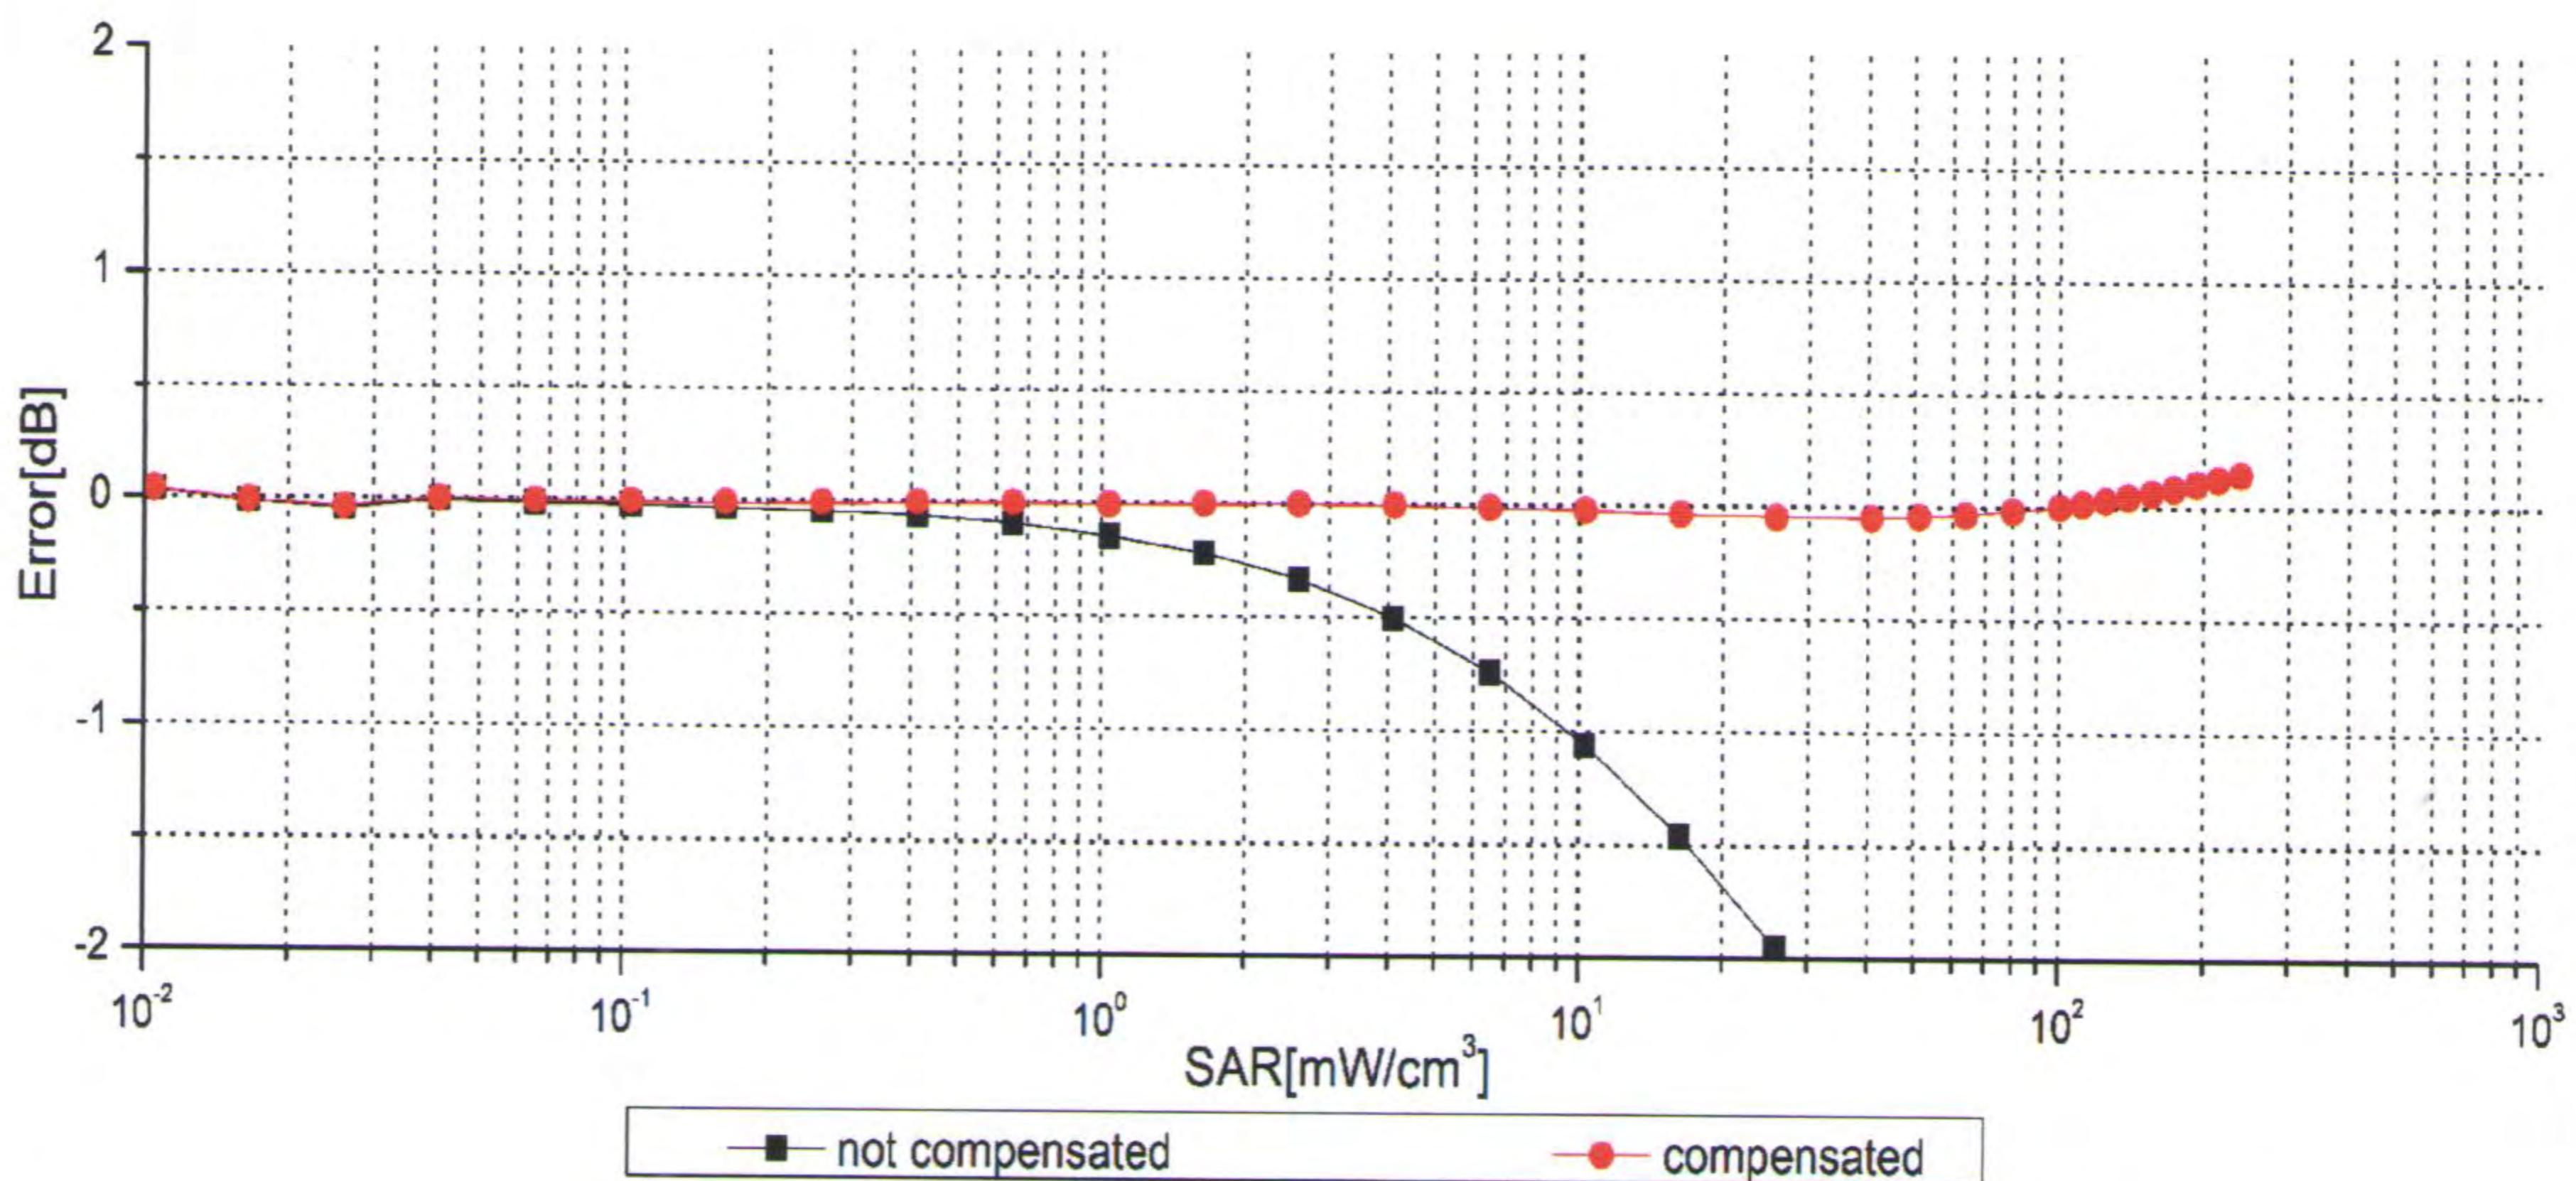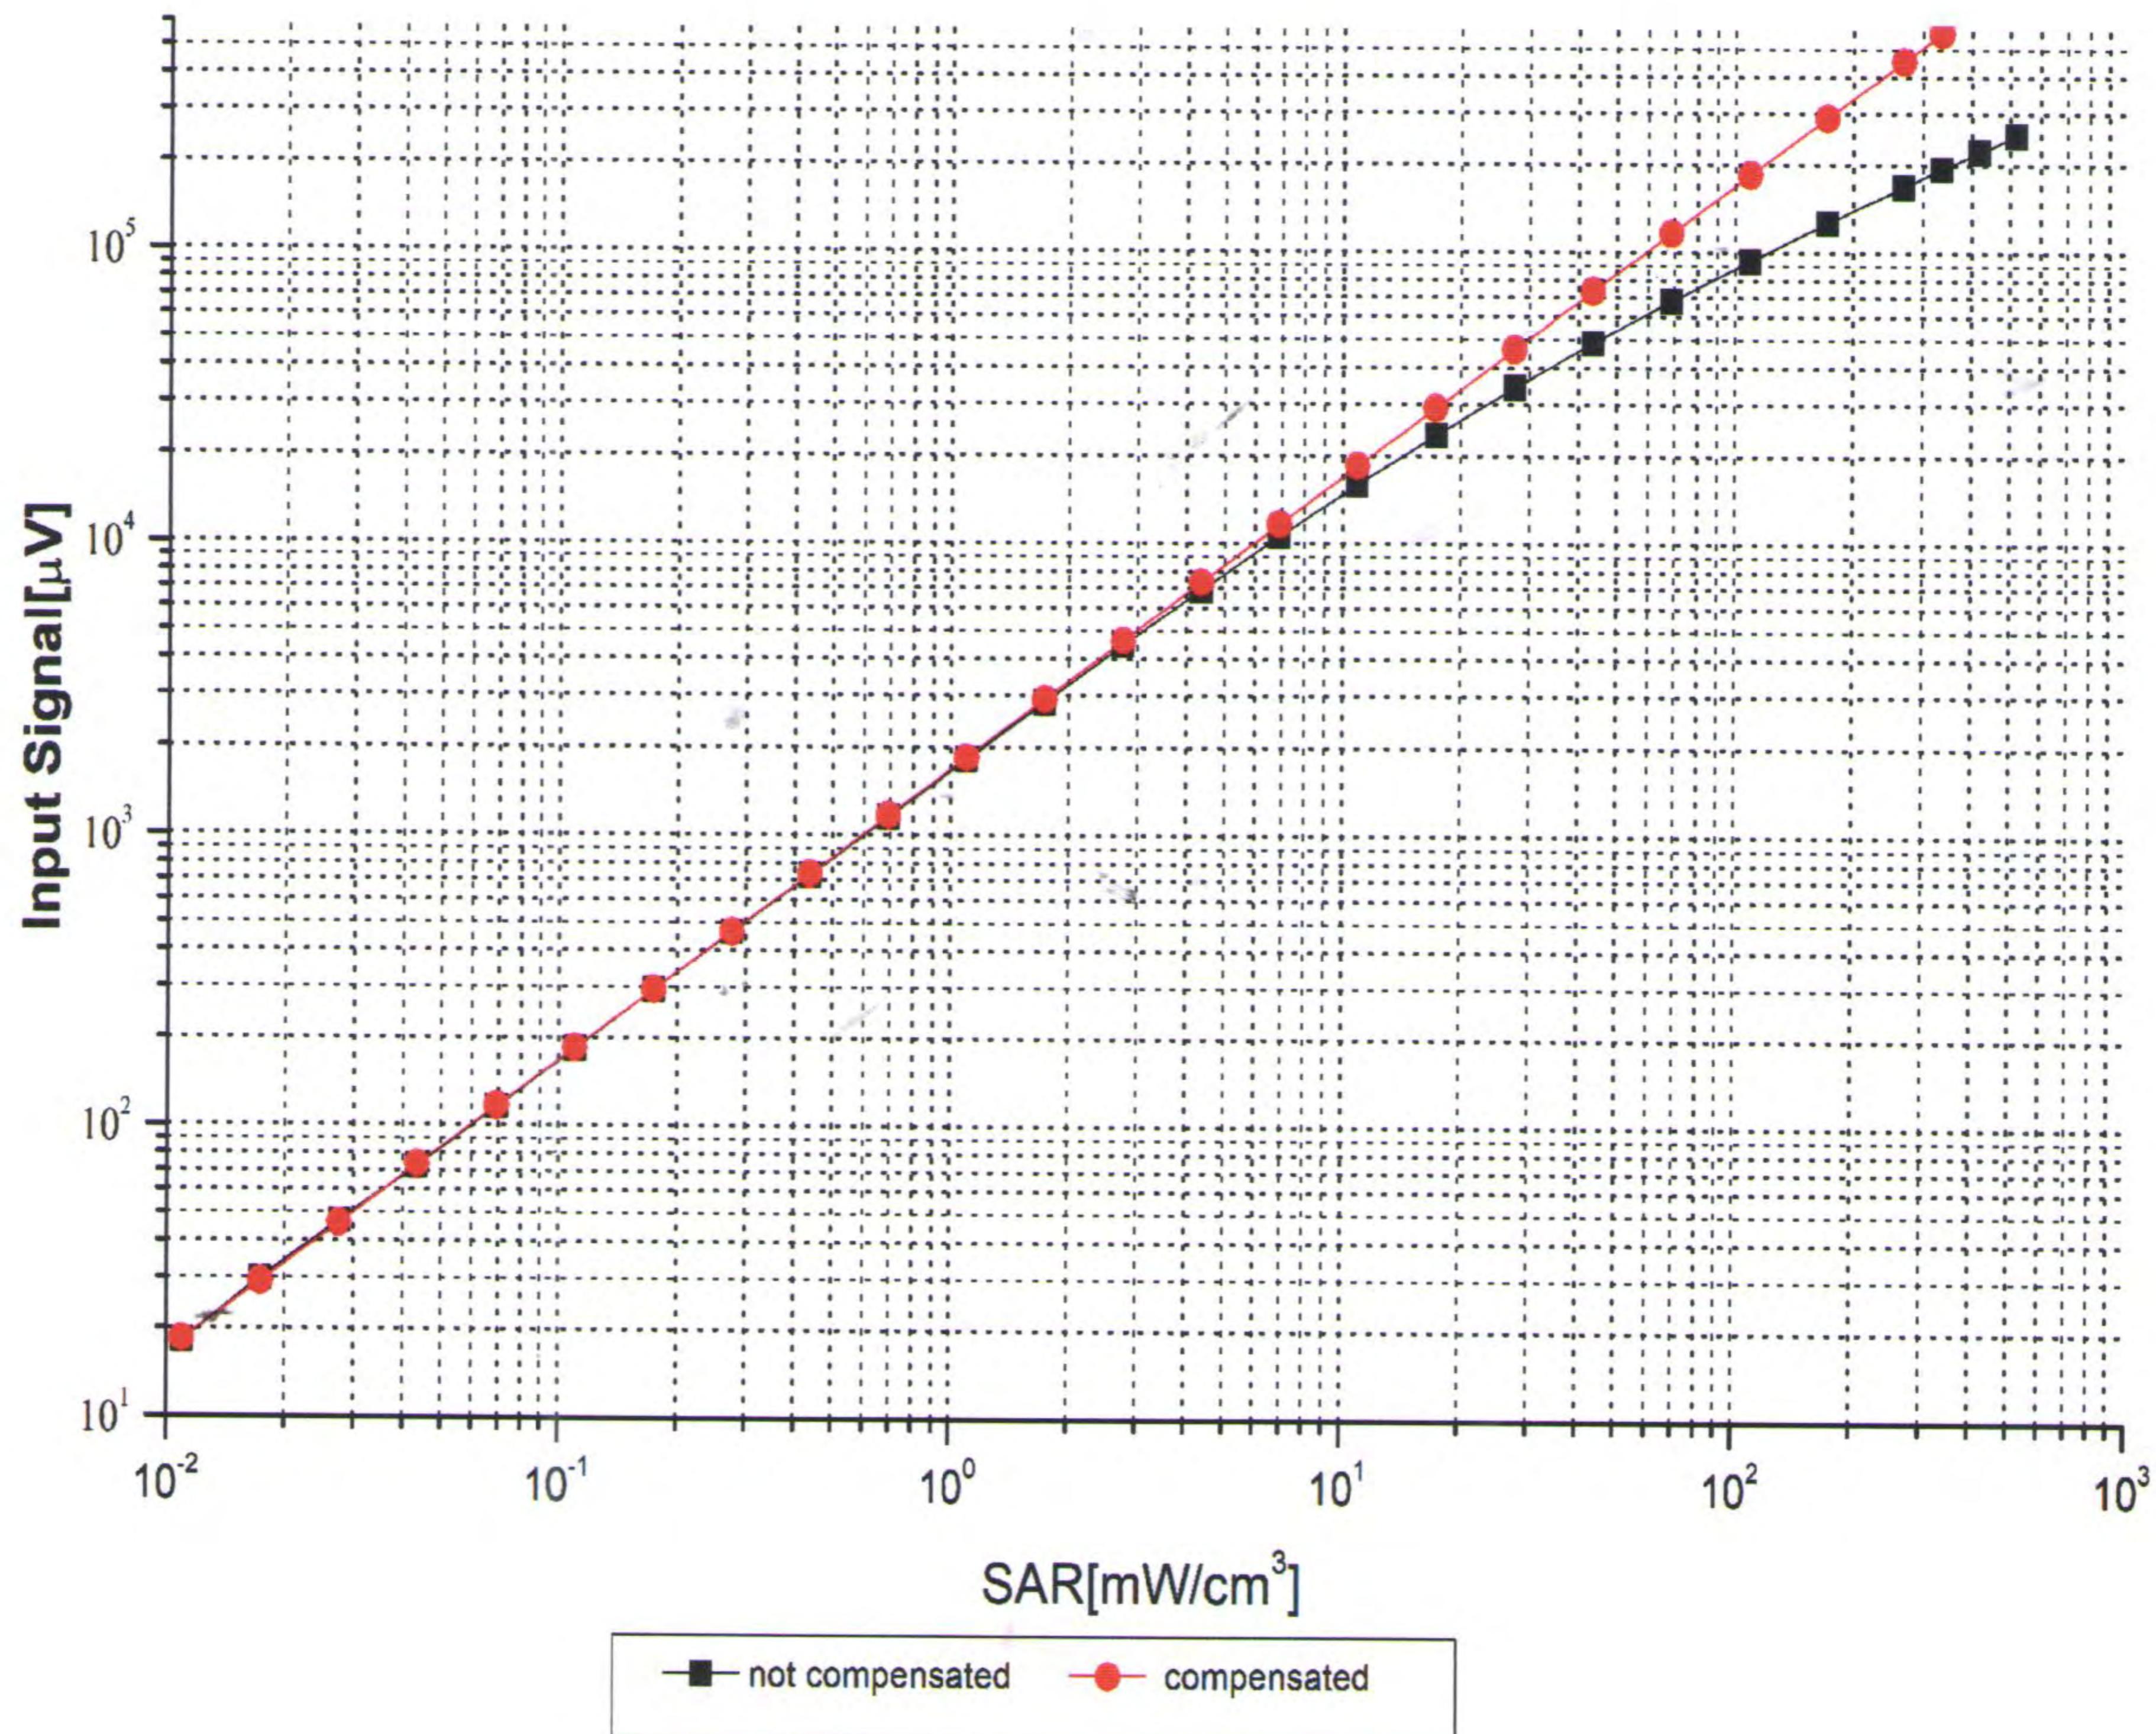



Uncertainty of Linearity Assessment: $\pm 0.9\%$ ($k=2$)




Conversion Factor Assessment

$f=835 \text{ MHz, WGLS R9(H_convF)}$

$f=1750 \text{ MHz, WGLS R22(H_convF)}$

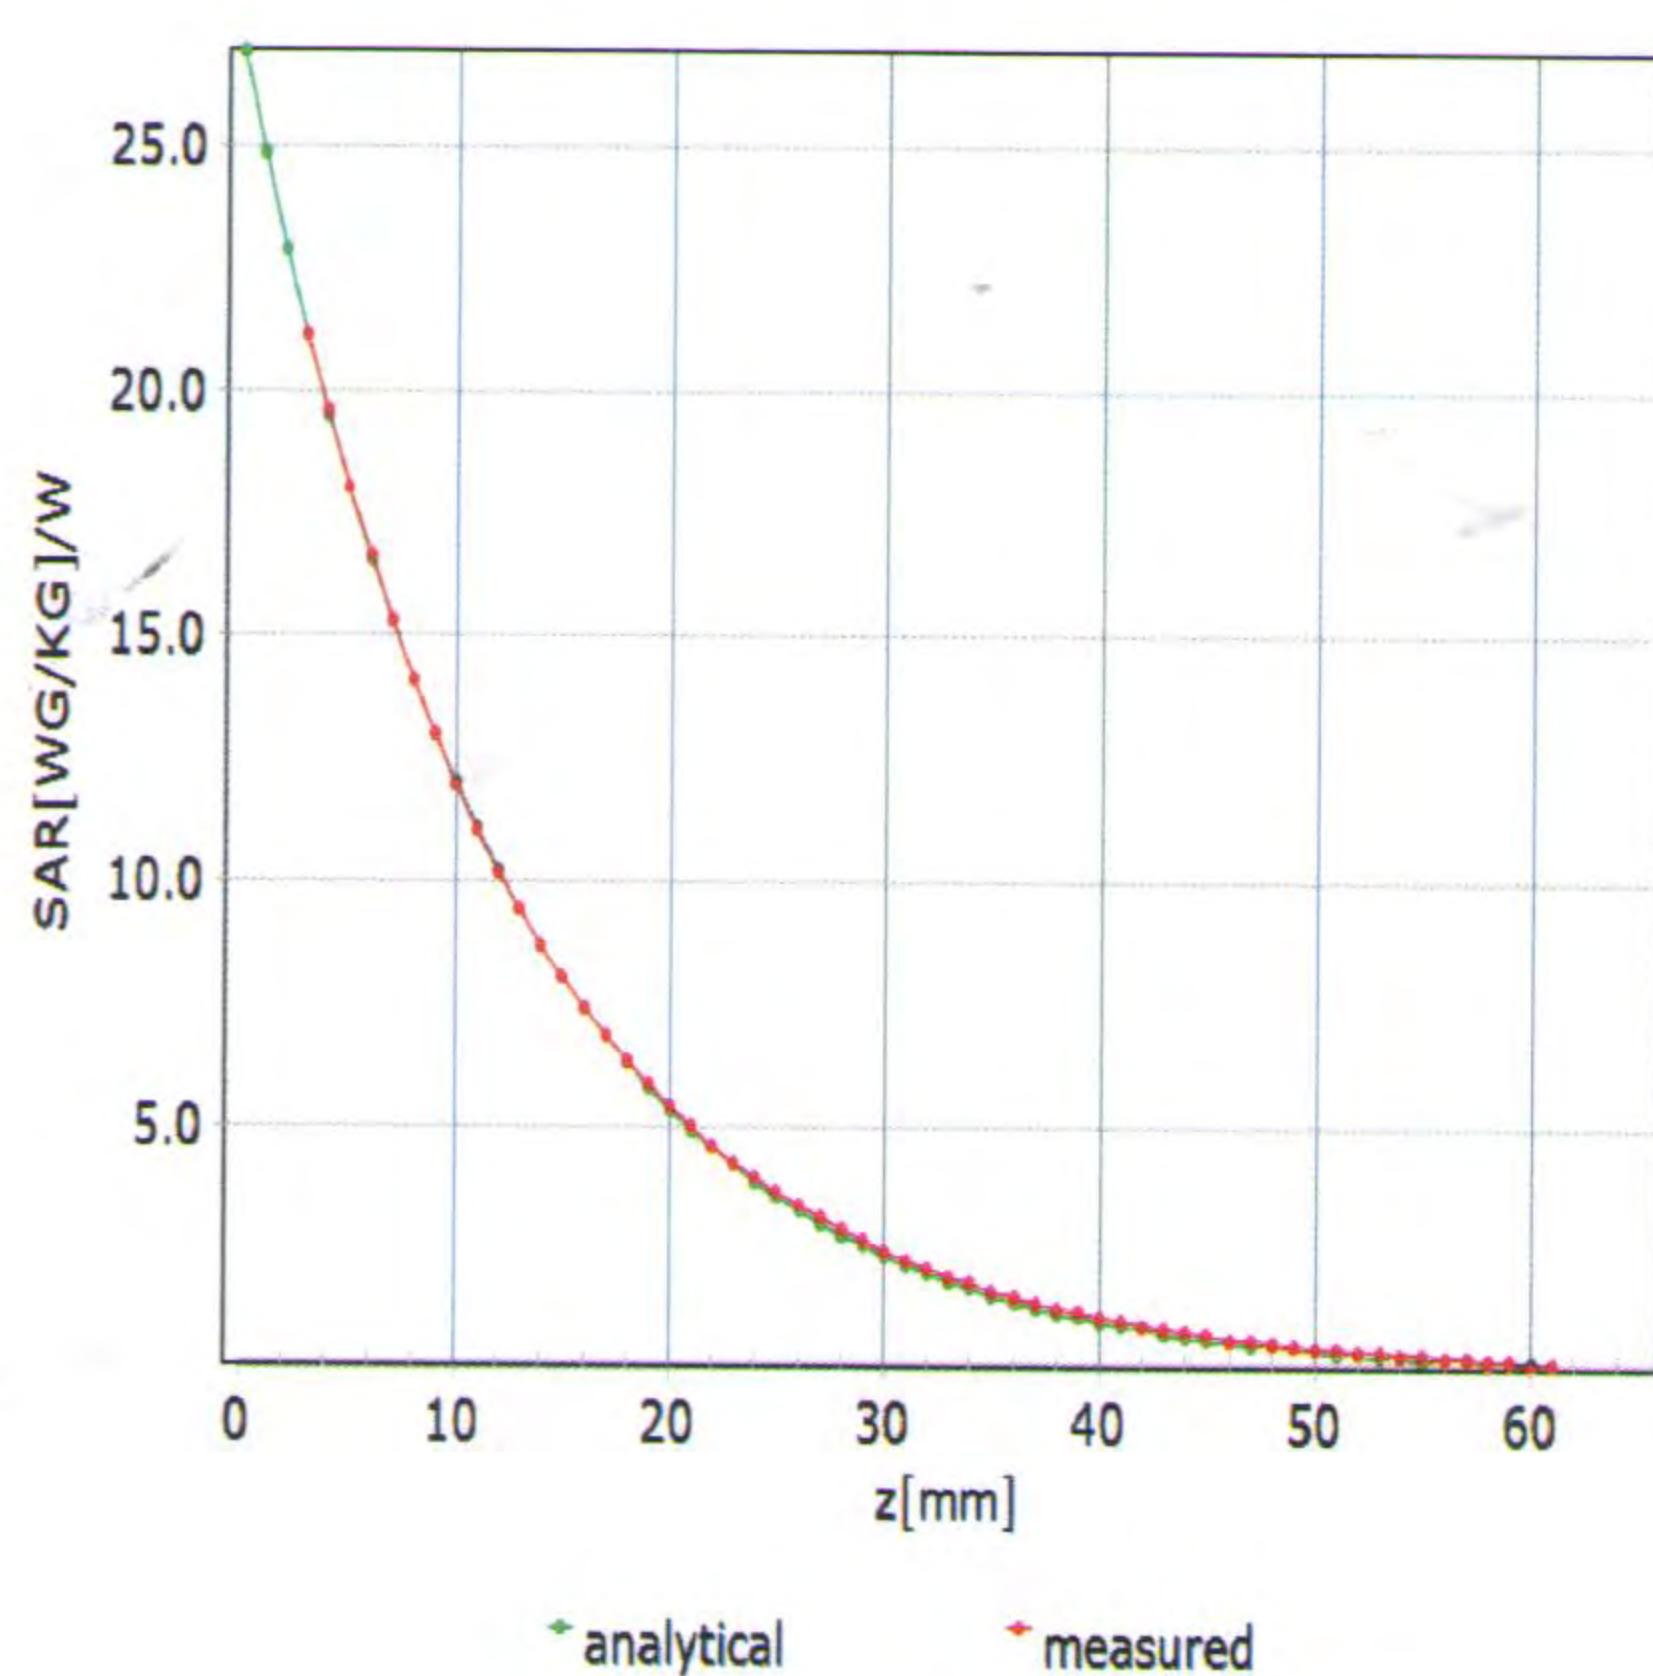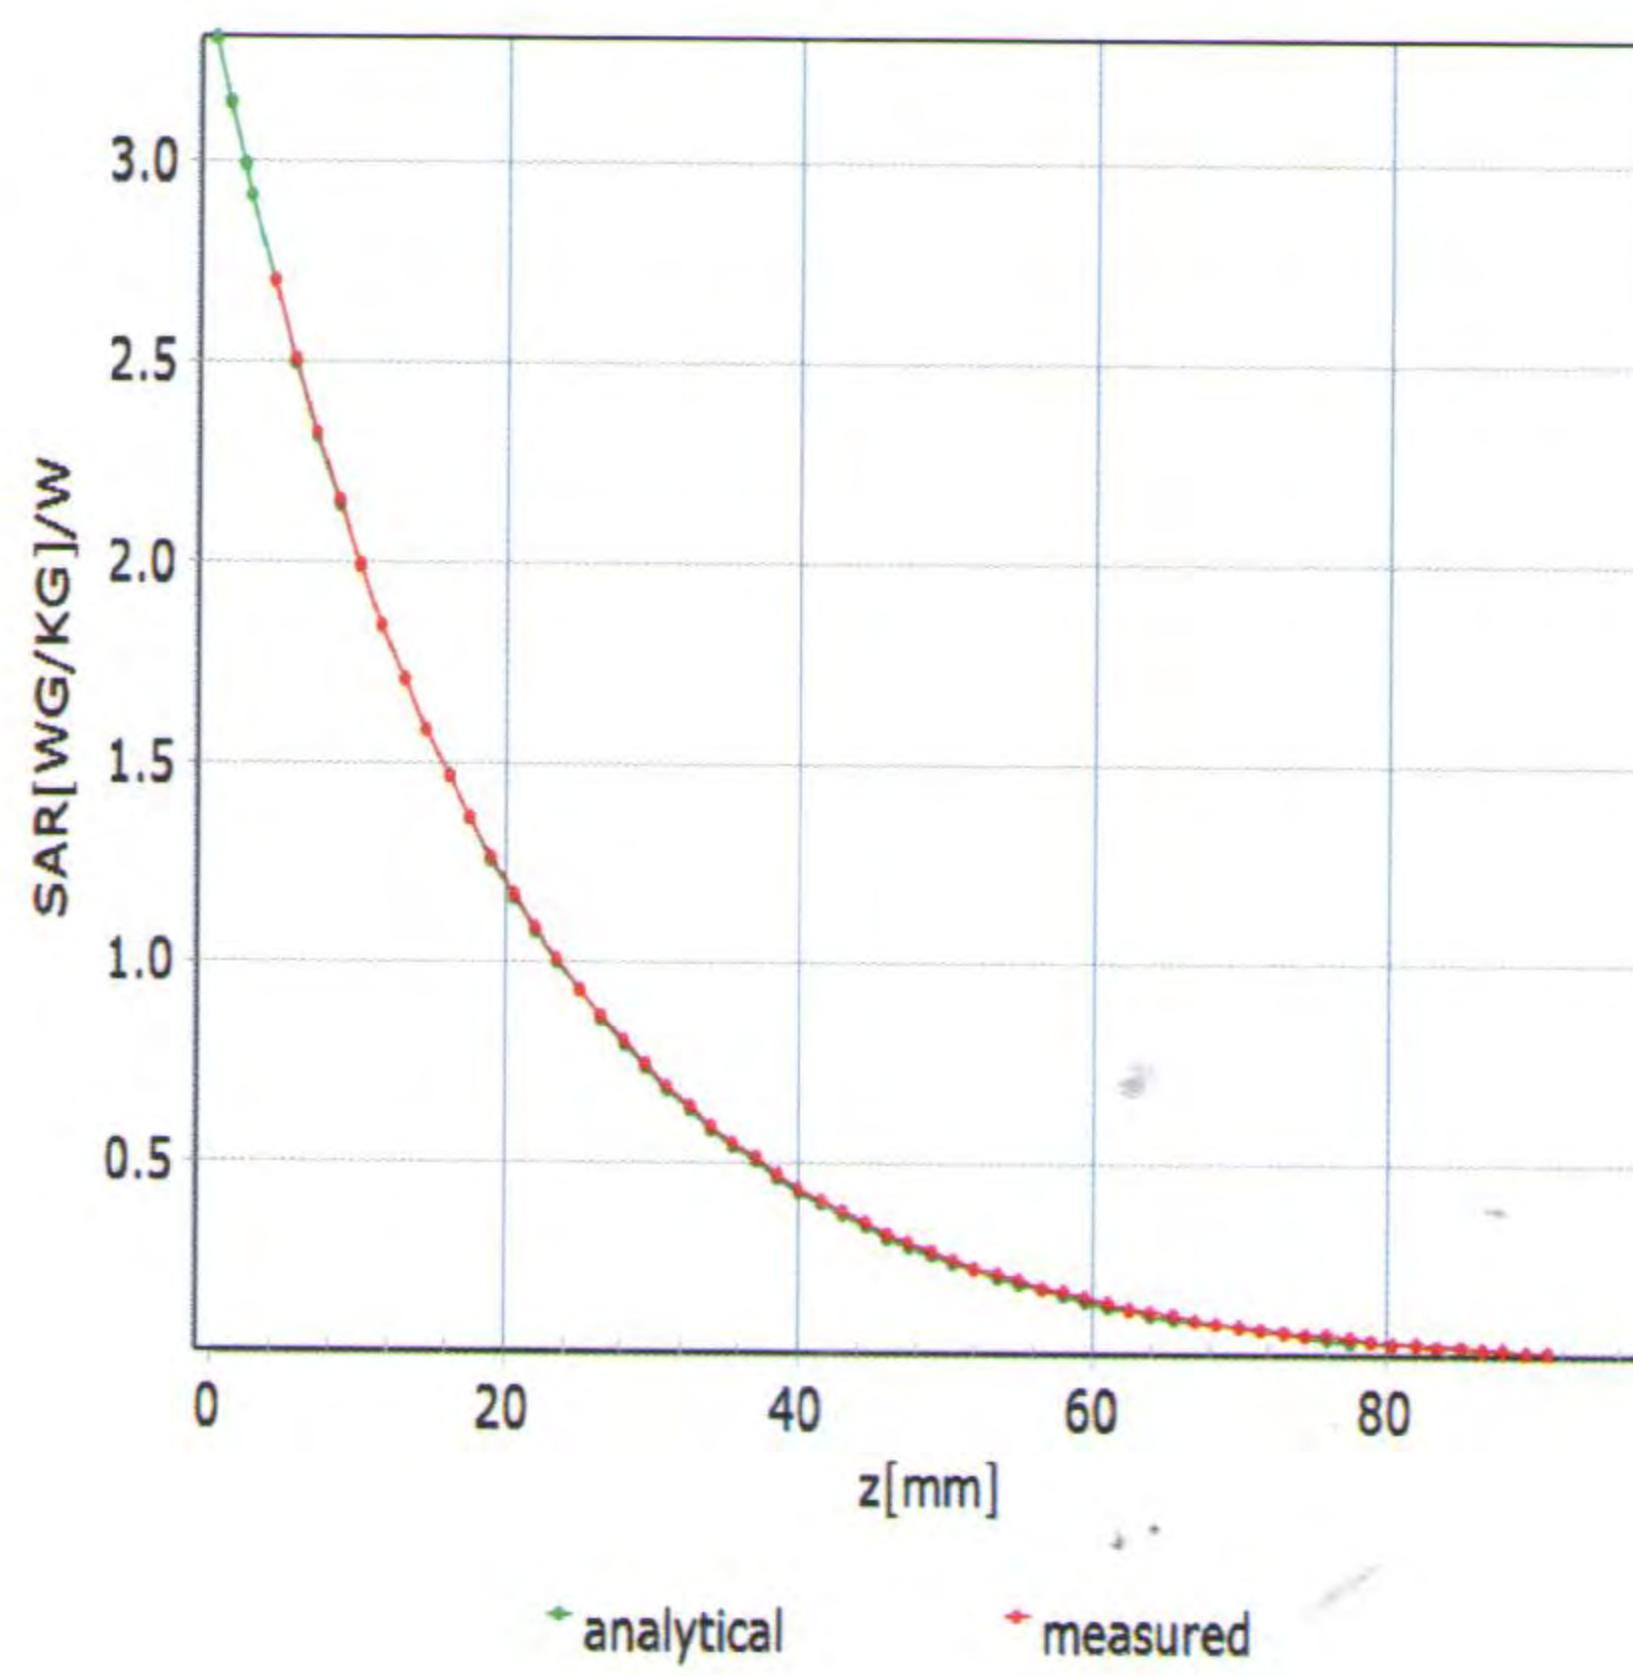

Deviation from Isotropy in Liquid

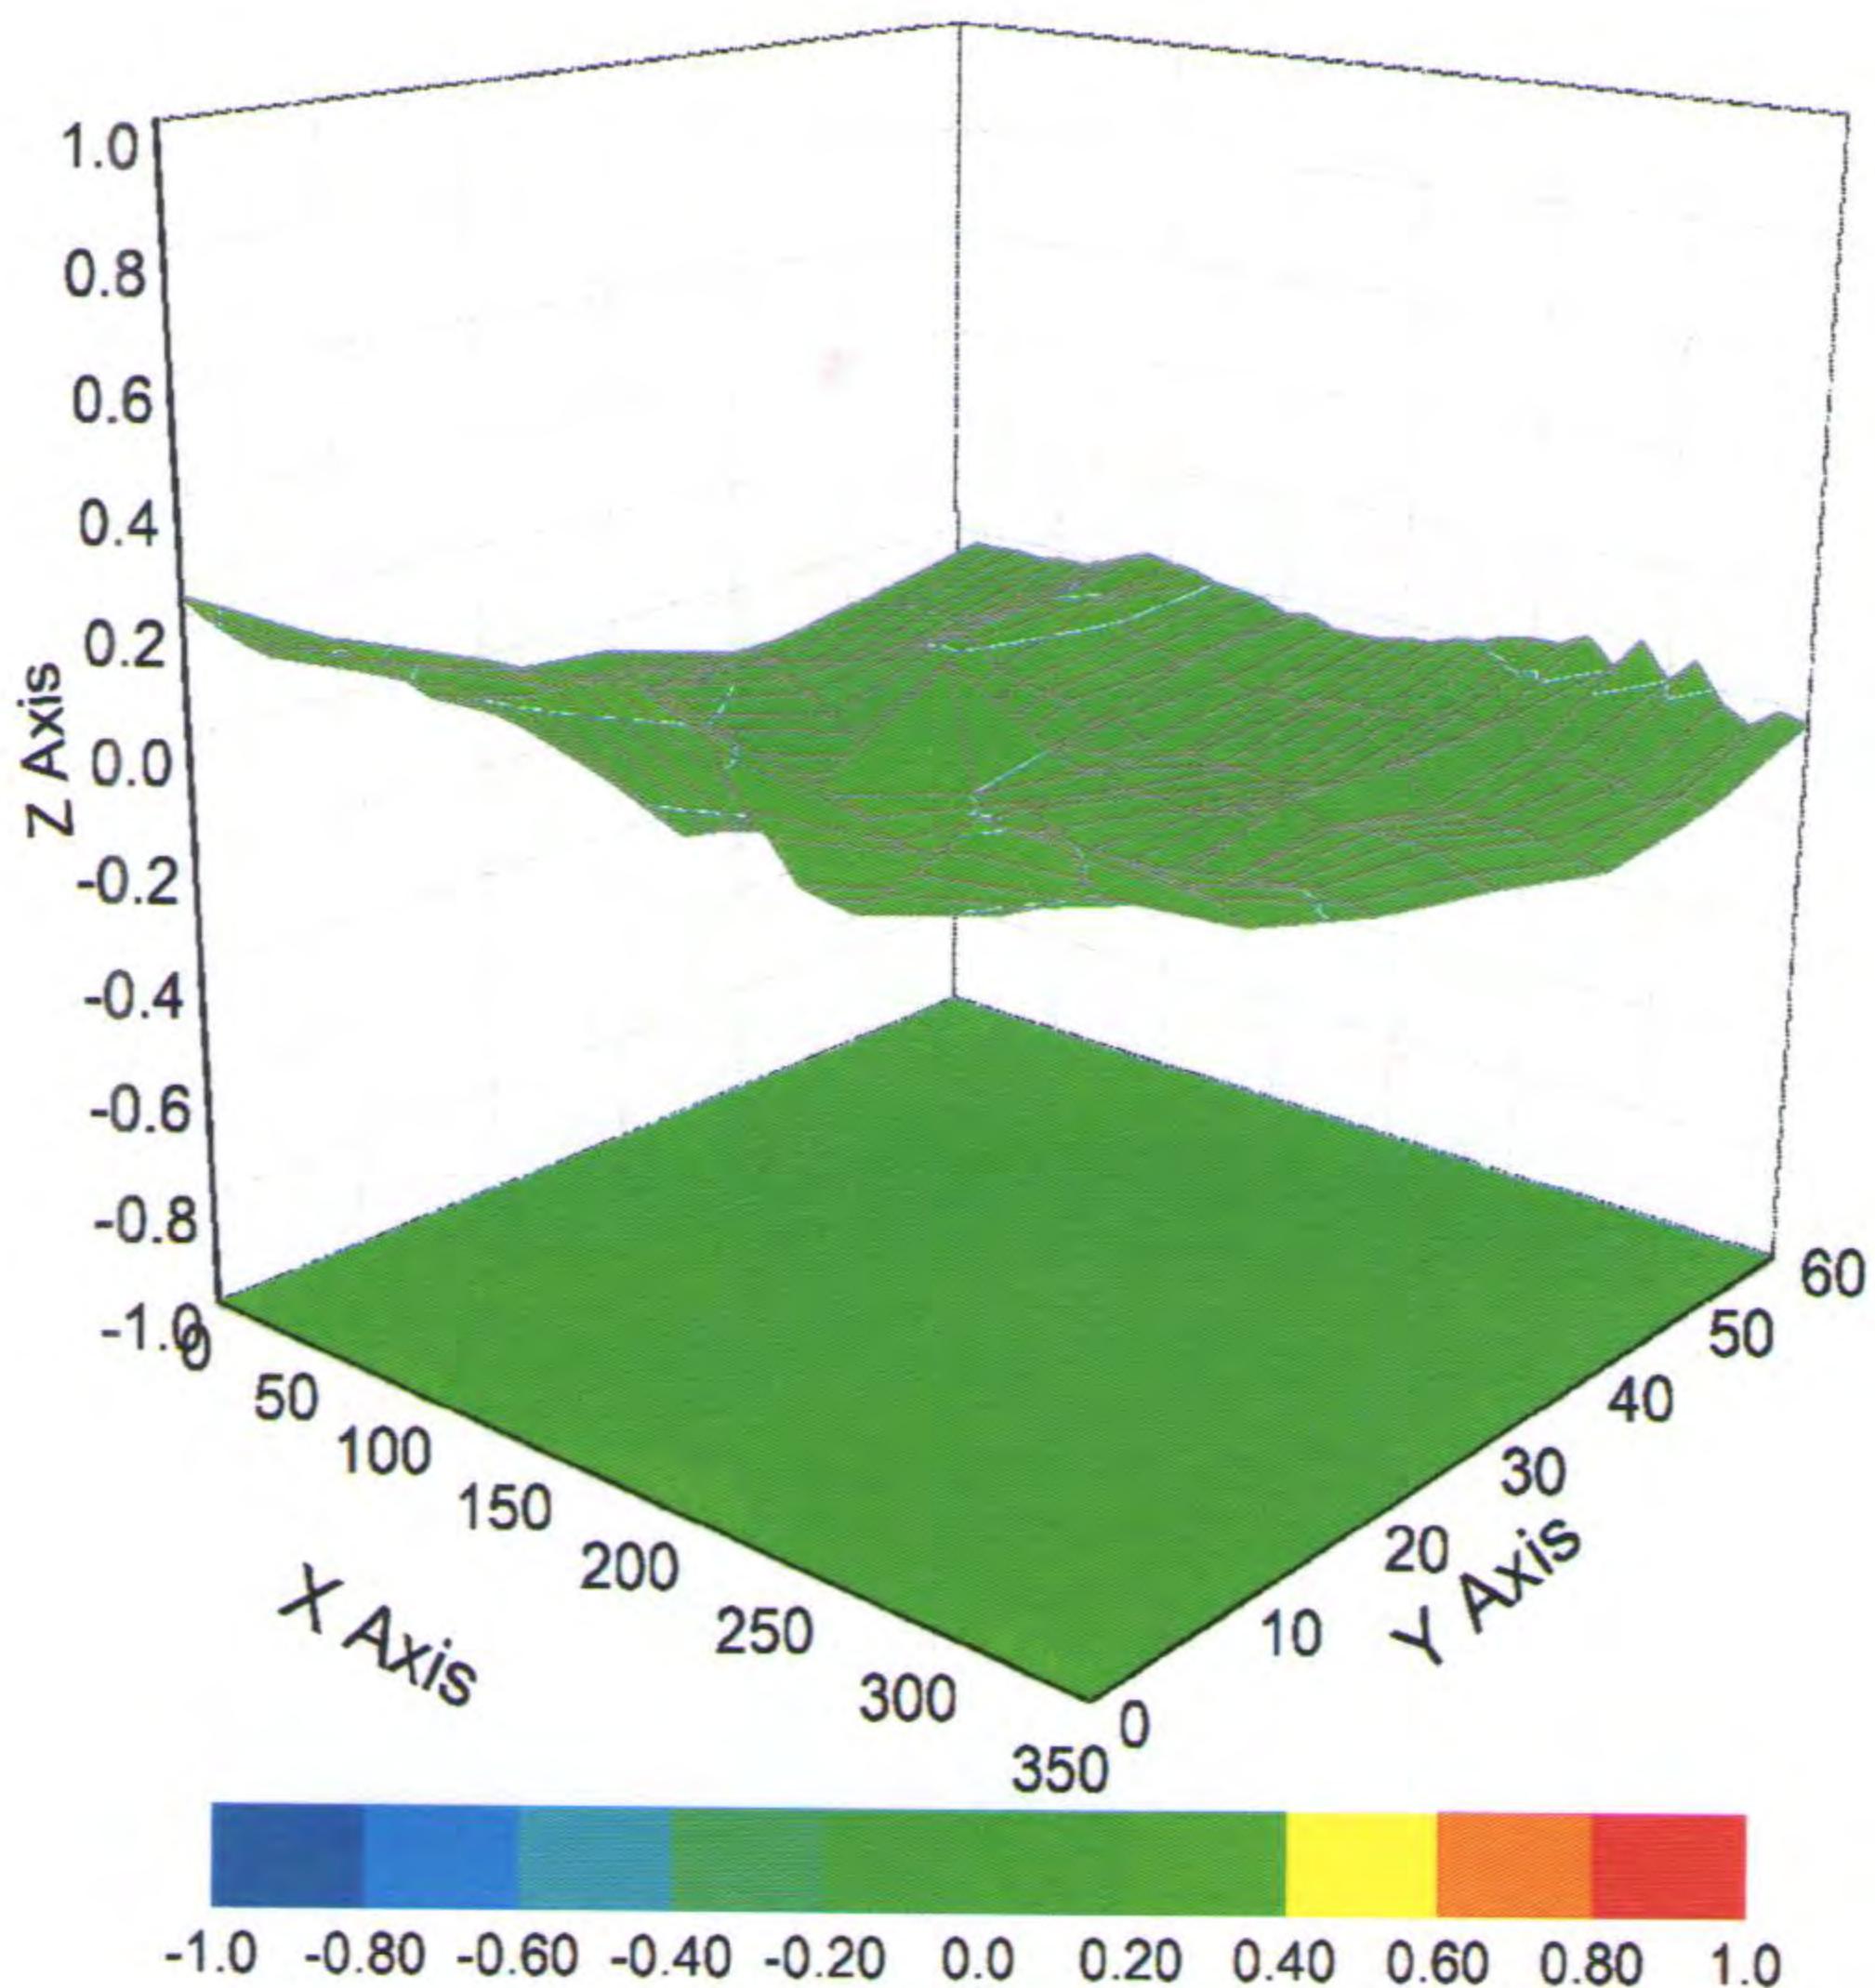

Uncertainty of Spherical Isotropy Assessment: $\pm 3.2\% (K=2)$



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504
E-mail: ctl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3962

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	151.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	10mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm

Dipole D835V2 SN 4d105				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2019-12-17	-26.0	/	49.5	/
2020-12-16	-27.0	3.85%	51.4	1.9Ω


Dipole D2450V2 SN 733				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2019-12-17	-27.2	/	52.2	/
2020-12-16	-27.8	2.21%	53.4	1.2Ω

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

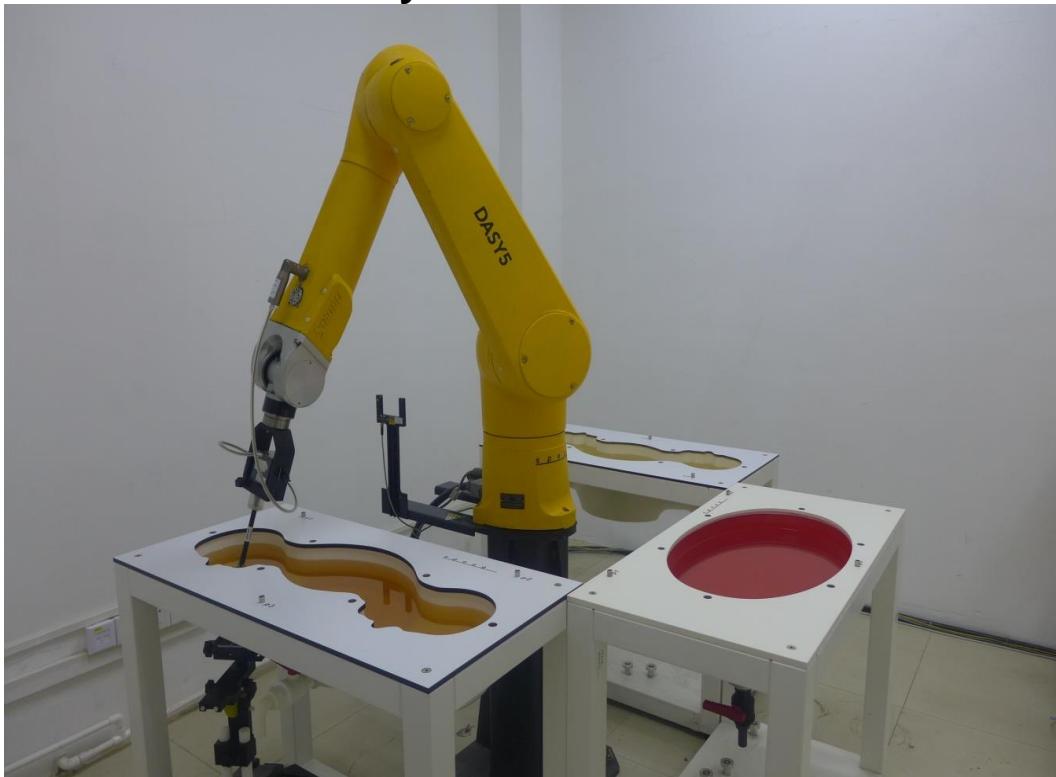

2. Photographs of Tissue Simulate Liquid


Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
	NA

3. Photographs of EUT test position

Photo 2: Front side 5mm	Photo 3: Back side 5mm
	
Photo 4: Left side 5mm	Photo 5: Right side 5mm
	
Photo 6: Top side 5mm	Photo 7: Bottom side 5mm
	

Photo 8: Front side 5mm with back cover	NA
	NA

4. EUT Constructional Details

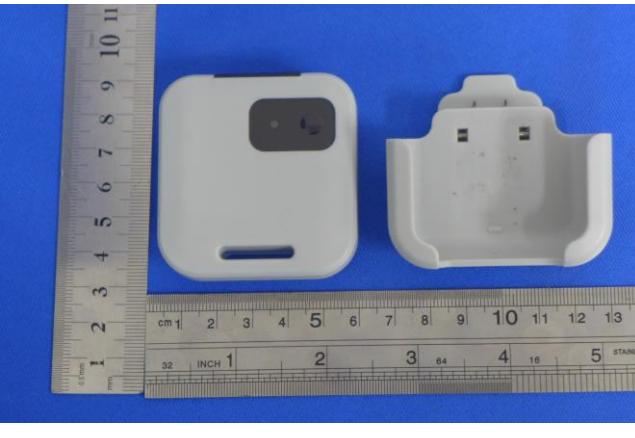Photo 9: Front View	Photo 10: Back View
 A photograph of the front view of the EUT (Electronic Unit Under Test). The device is white with a black camera lens on the top left. It has a small blue rectangular slot on the bottom left. The EUT is placed next to a metal ruler with markings in millimeters (mm) and inches (INCH). The ruler shows measurements from 0 to 12 cm and 0 to 5 inches.	 A photograph of the back view of the EUT. The device is white with a black camera lens on the top left. It has a small blue rectangular slot on the bottom left. The EUT is placed next to a metal ruler with markings in millimeters (mm) and inches (INCH). The ruler shows measurements from 0 to 10 cm and 0 to 4 inches.
Photo 11: Front View With back cover	NA
 A photograph showing the front view of the EUT with its back cover removed. The internal components are visible, including a white plastic frame and a blue rectangular component. The EUT is placed next to a metal ruler with markings in millimeters (mm) and inches (INCH). The ruler shows measurements from 0 to 13 cm and 0 to 5 inches.	NA