| REVISION | | | | | |
|---|---|---|---|---|---|
| REV | DESCRIPTION | ECO NUMBER | DATE | DRFT | APRV |
| A | INITIAL PRODUCTION RELEASE | 20-00675 | 7/17/2020 | TY | KV |
| B | UPDATE FCC LABEL CONTENT | 21-00755 | 1/15/2021 | TY | AR |




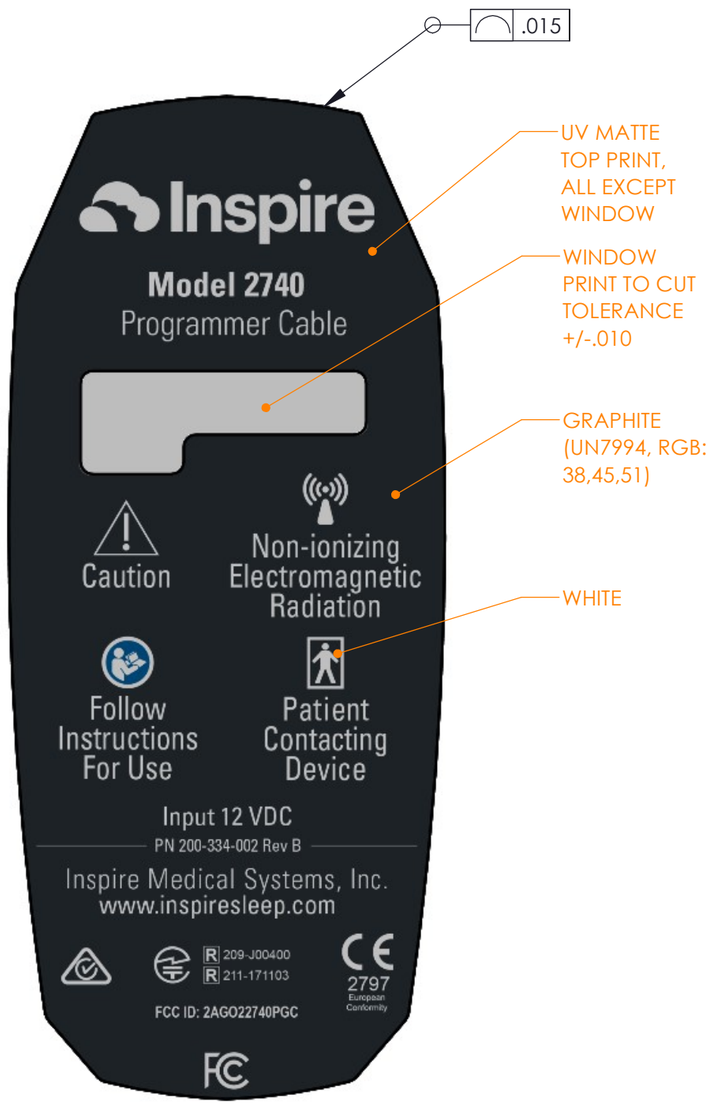


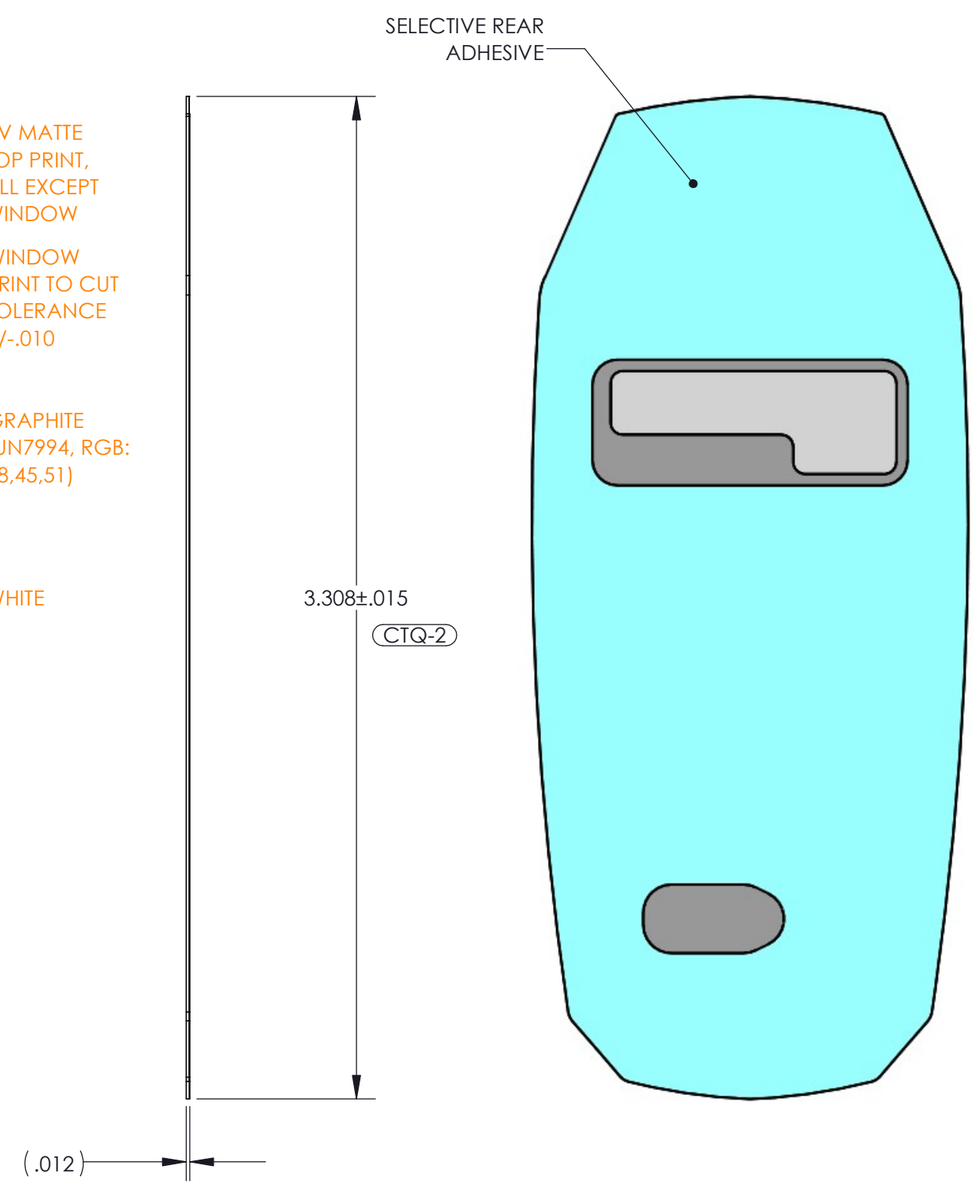


NOTES:

CTQ-1 1. MATERIAL: 10 MIL MARNOT XL HARDCOATED CLEAR GLOSS PC WITH 3M 7952MP REAR ADHESIVE (2 MIL). MATERIAL CERTIFICATION TO BE PROVIDED WITH EACH LOT.

2. SEE ART FILES FOR COMPLETE GEOMETRY DEFINITION. P/N'S 200-334-001 & 200-334-002 HAVE THE SAME GEOMETRY WITH DIFFERENT ART AND SHARE THIS DRAWING (200-334-002 SHOWN).

3. CTQ ARE CRITICAL INSPECTION DIMENSIONS (2).

4. UNLESS OTHERWISE SPECIFIED GENERAL TOLERANCES APPLY: CUT-TO-CUT & PRINT-TO-CUT ±.020, PRINT TO PRINT ±.010.

5. THE PARTS SHALL BE PACKAGED IN A MANNER THAT PREVENTS DAMAGE OR CONTAMINATION FROM FOREIGN MATERIAL. EACH MANUFACTURING LOT SHALL BE LABELED IN ACCORDANCE WITH INSPIRE SPEC 700-006-000.

6. UPON APPROVAL BY INSPIRE MEDICAL SYSTEMS OF THE INITIAL DESIGN, ANY PROCESS CHANGES, DESIGN CHANGES, PACKAGING CHANGES, RAW MATERIAL CHANGES, OR DEVIATIONS CONSIDERED BY THE MANUFACTURER MUST BE SUBMITTED TO INSPIRE IN WRITNG FOR PRE-APPROVAL. THE INFORMATION SUBMITTED SHALL INCLUDE A COMPLETE DESCRIPTION OF THE CHANGE AND THE EFFECT THE CHANGE WILL HAVE ON ALL THE CHARACTERISTICS OF THE DEVICE/MATERIAL. UPON REQUEST, THE MANUFACTURER SHALL SUBMIT SAMPLES OF THE PROPOSED DEVICE/MATERIAL FOR EVALUATION AND APPROVAL BY INSPIRE MEDICAL SYSTEMS.

| IMS P/N | REV | DESCRIPTION |
|---|---|---|
| 200-334-001 | B | BACK LABEL, PROGRAMMER CABLE, US |
| 200-334-002 | B | BACK LABEL, PROGRAMMER CABLE, GLOBAL |

PROPERTY AND CONFIDENTIAL
The information contained in this drawing is the sole property of Inspire. Any reproduction in part or as a whole without the express written permission of Inspire is strictly prohibited.

Inspire Medical Systems, Inc.
Golden Valley, MN USA

TITLE: BACK LABEL, PROGRAMMER CABLE

X.X ±.1
X.XX ±.01
X.XXX ±.005
ANGLES ±2.0°
All dimensions in inches unless otherwise noted

| DOCUMENT CREATED BY: | DATE | APPROVED | DATE |
|---|---|---|---|
| T. YOCH | 11/25/2019 | A. RASMUSSEN | 11/25/2019 |

| SIZE | DWG NO. | REV. | SHEET |
|---|---|---|---|
| B | 200-334-000 | B | 1 OF 1 |