


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

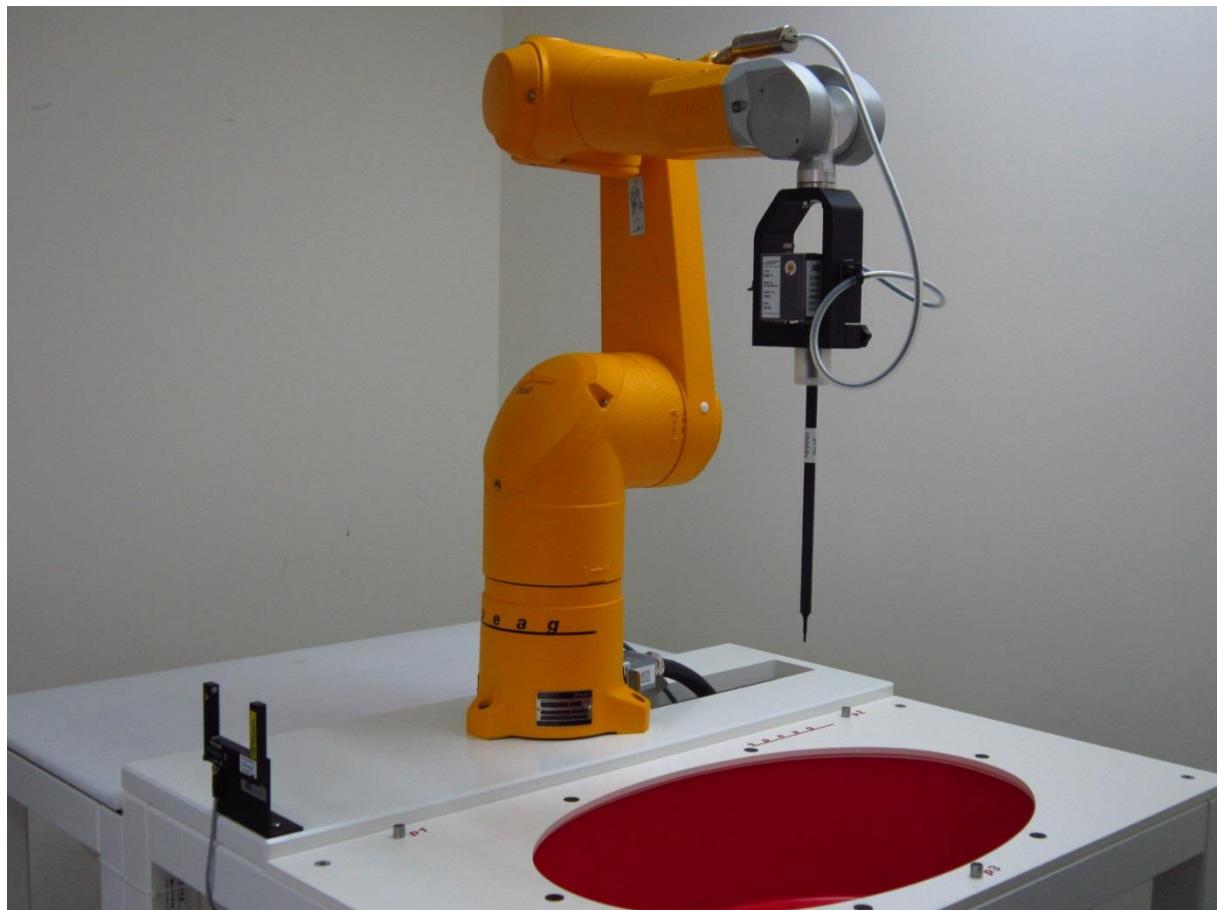

2. Photographs of Tissue Simulate Liquid

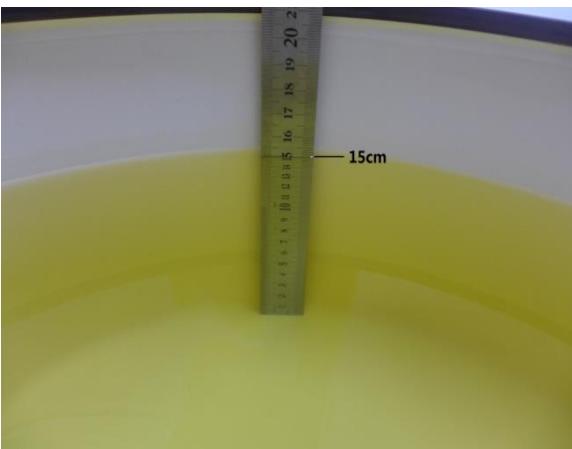
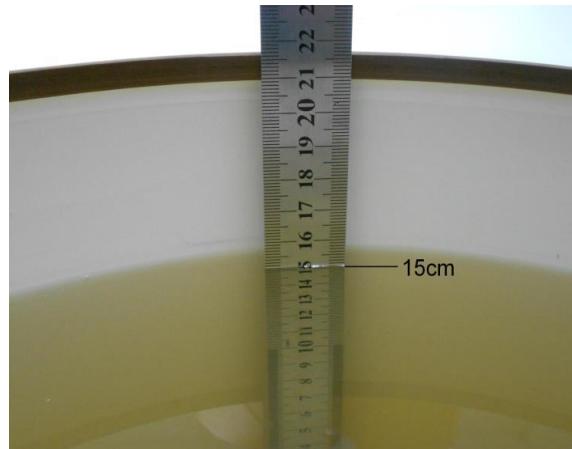
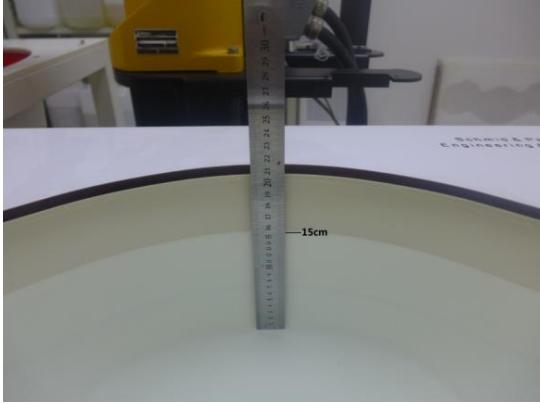
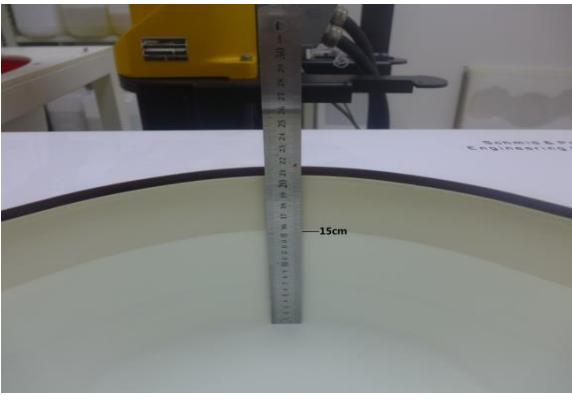
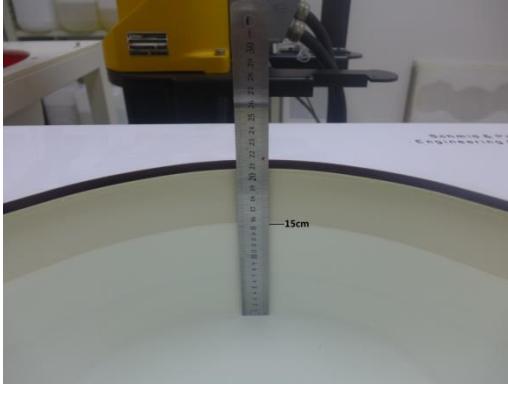
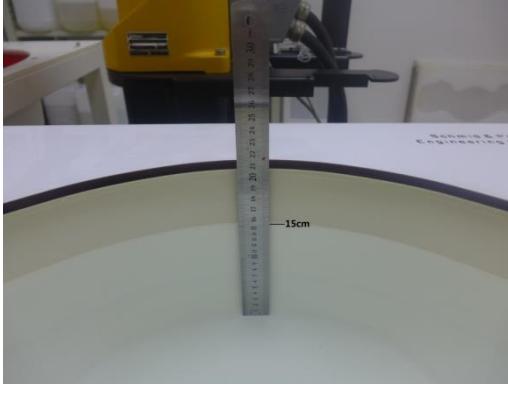
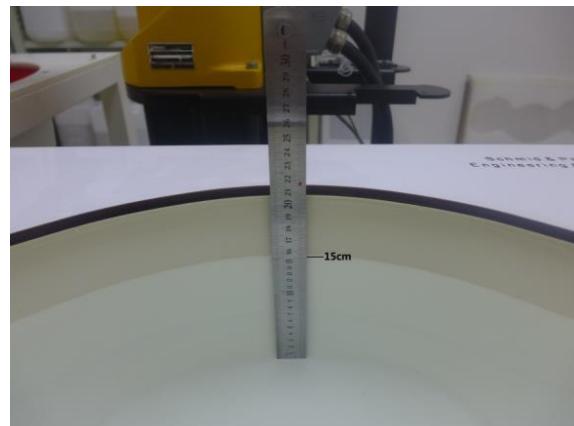
Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1800	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 2600
	

Photo 7: Tissue Simulant Liquid for Head5GHz

3. Photographs of EUT test position

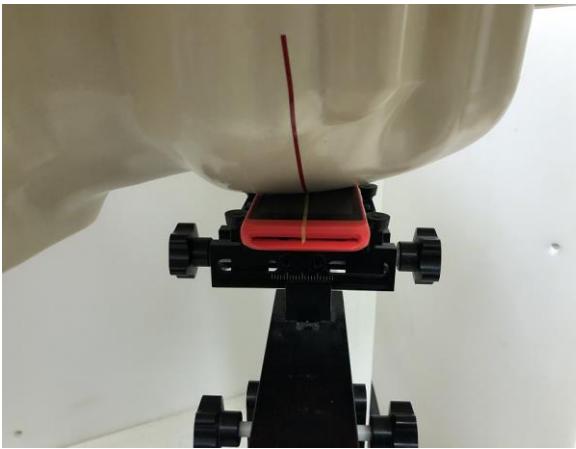
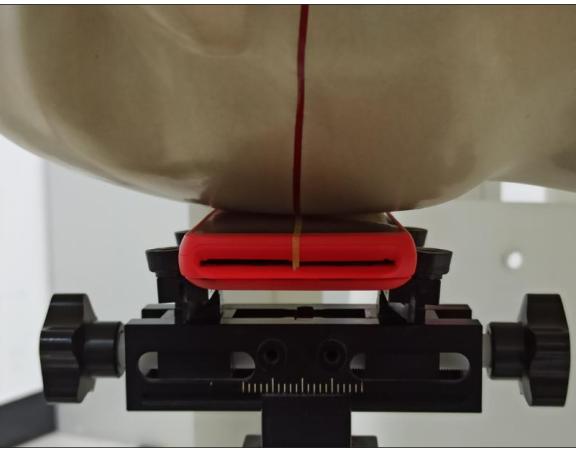
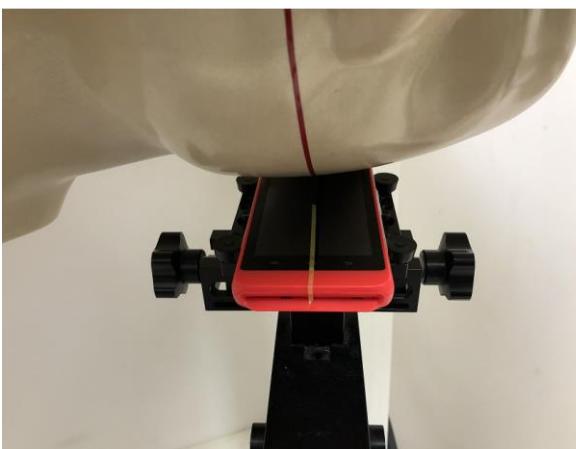
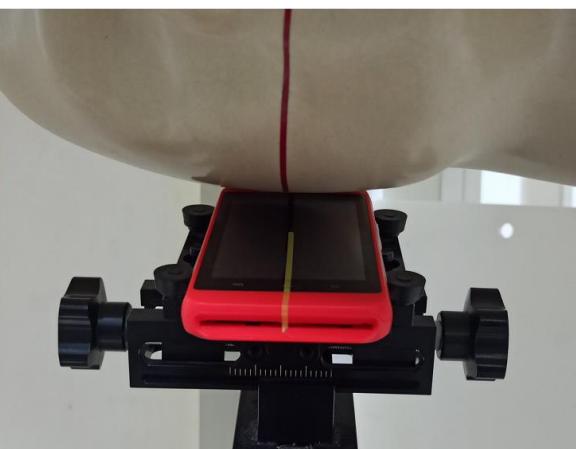
Photo 8: Left cheek 0mm	Photo 9: Right cheek 0mm
	
Photo 10: Left tilted	Photo 11: Right tilted
	
Photo 12: Front side 10mm	Photo 13: Back side 10mm
	

Photo 14: Left side 10mm	Photo 15: Right side 10mm
	
Photo 16: Top side 10mm	Photo 17: Bottom side 10mm
	

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.