

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750

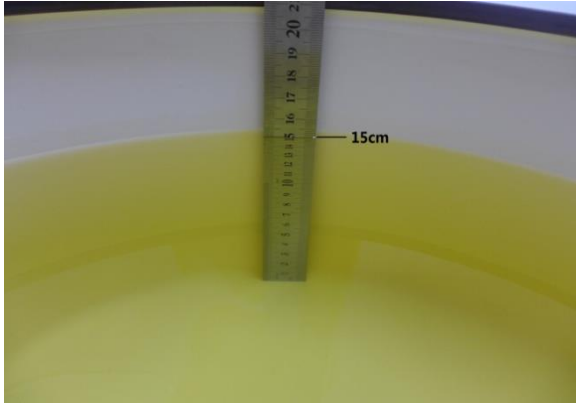


Photo 2: Tissue Simulant Liquid for Head 835

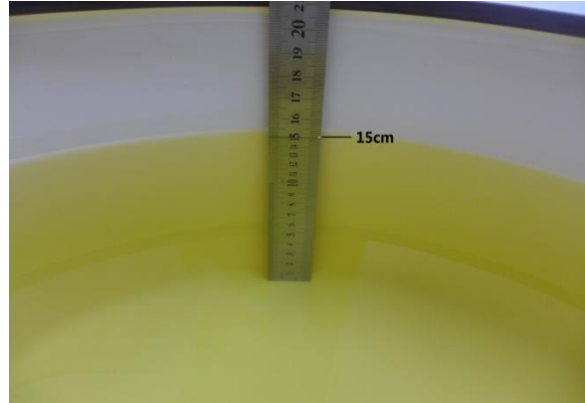


Photo 3: Tissue Simulant Liquid for Head 900

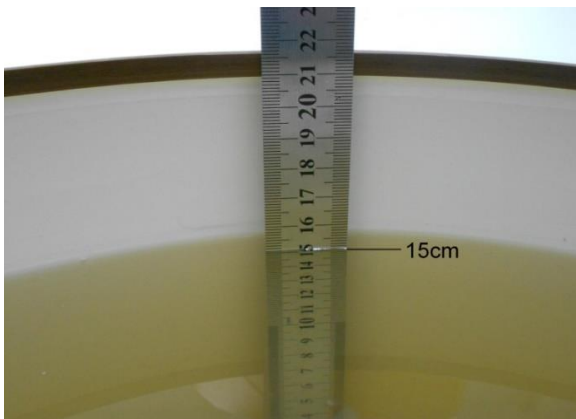


Photo 4: Tissue Simulant Liquid for Head 1800

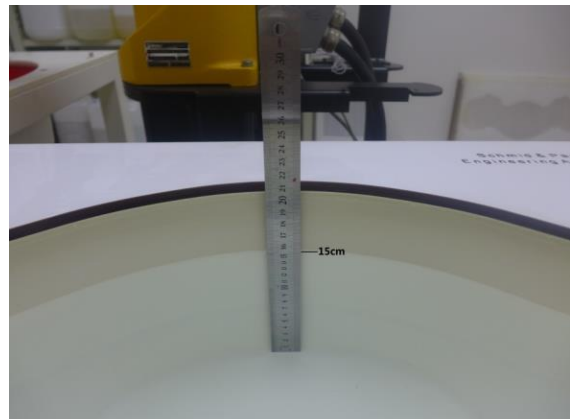


Photo 5: Tissue Simulant Liquid for Head 2000

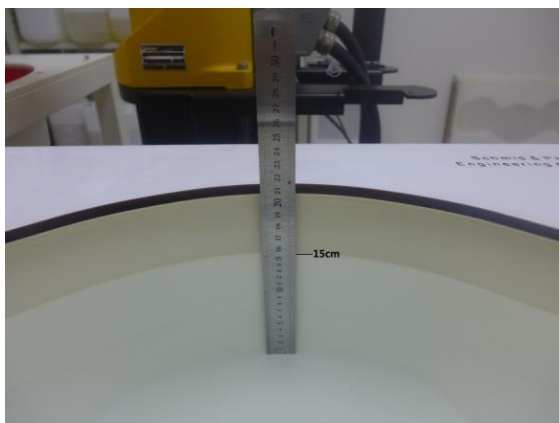


Photo 6: Tissue Simulant Liquid for Head 2300

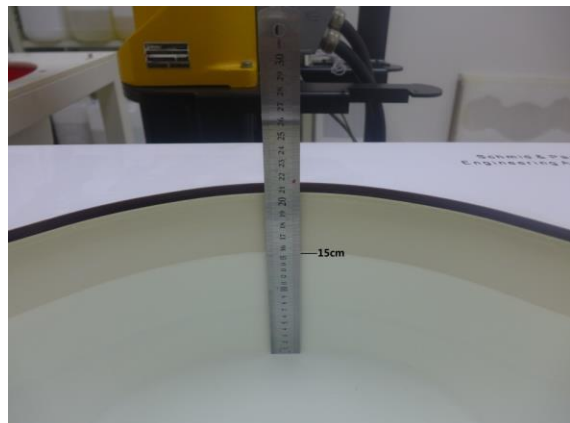


Photo 7: Tissue Simulant Liquid for Head 2450

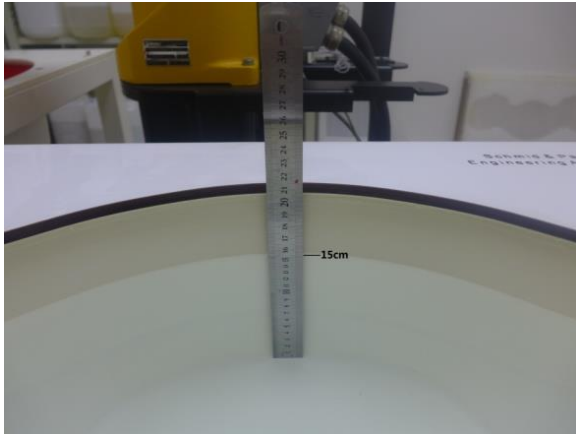


Photo 8: Tissue Simulant Liquid for Head 2600


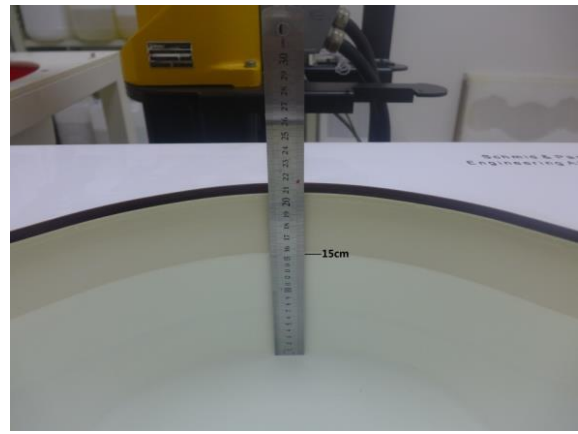


Photo 9: Tissue Simulant Liquid for Head 5GHz

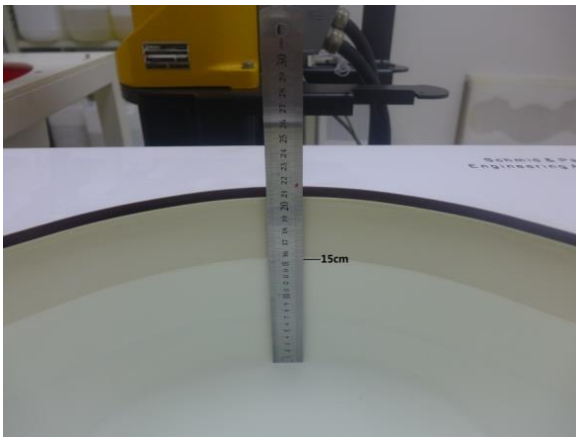

3. Photographs of EUT test position


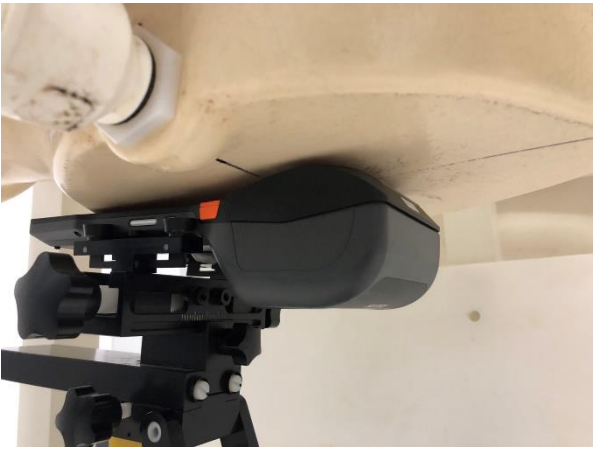
Photo 10: Front side 0mm	Photo 11: Back side 0mm
	
Photo 12: Left side 0mm	Photo 13: Right side 0mm
	
Photo 14: Top side 0mm	Photo 15: Bottom side 0mm
	

Photo 16: Handheld Back 0mm

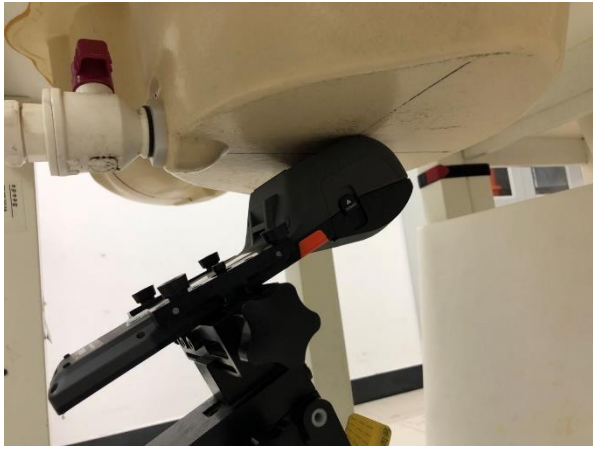

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.