



TEST REPORT

Report Number. : R13999443-EP1

Applicant : INFOBIONIC
400 TOTTEN POND RD STE 315
WALTHAM, MA 02451, USA

Model : 01854 REV B

FCC ID : 2AHLC01855

EUT Description : WIRELESS AMBULATORY ECG MONITORING AND DETECTION
SYSTEM

Test Standard(s) : FCC CFR47 PART 22H, PART 24,
PART 27, AND PART 90R

Date Of Issue:
2021-12-06

Prepared by:
UL LLC
12 Laboratory Dr.
Research Triangle Park, NC 27709 U.S.A.
TEL: (919) 549-1400



Revision History


Rev.	Issue Date	Revisions	Revised By
V1	2021-12-06	Initial Release	Brian Kiewra

TABLE OF CONTENTS



1. RADIATED SETUP.....4

2. SETUP PHOTOS5

1. RADIATED SETUP

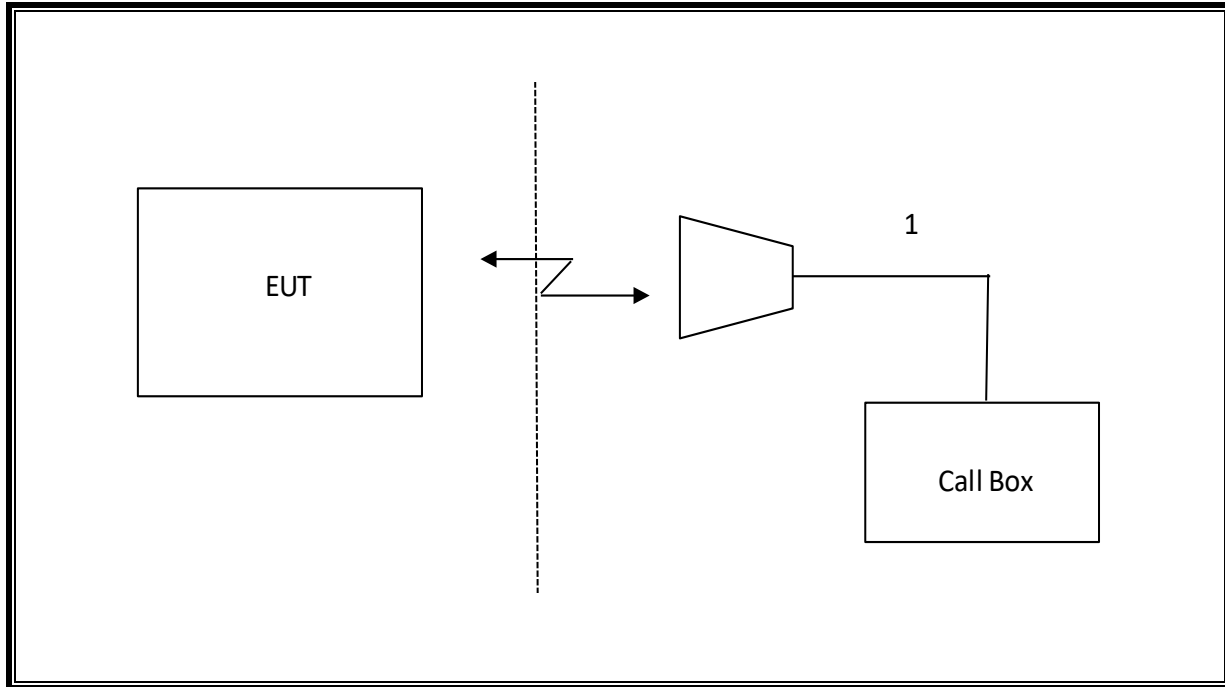

2. SETUP PHOTOS

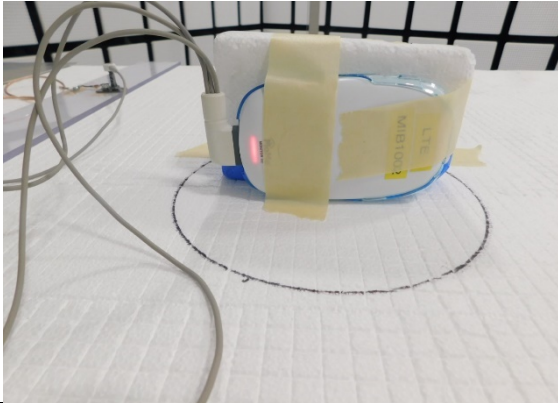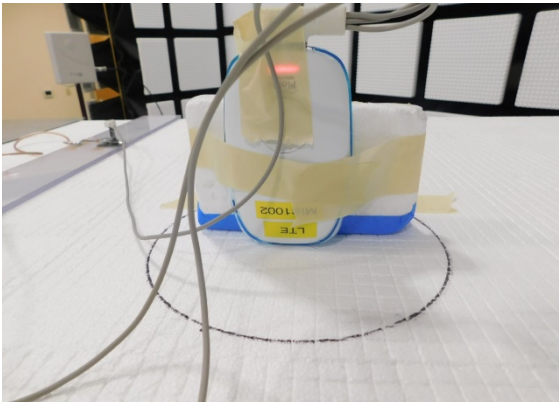
RADIATED RF MEASUREMENT SETUP FOR PORTABLE CONFIGURATION	
	
X-AXIS PHOTO	Y-AXIS PHOTO
	
Z-AXIS FRONT PHOTO	




B1G FRONT PHOTO (Bands 5, 12, 13, 14, and 71)




B1G BACK PHOTO (Bands 5, 12, 13, 14, and 71)

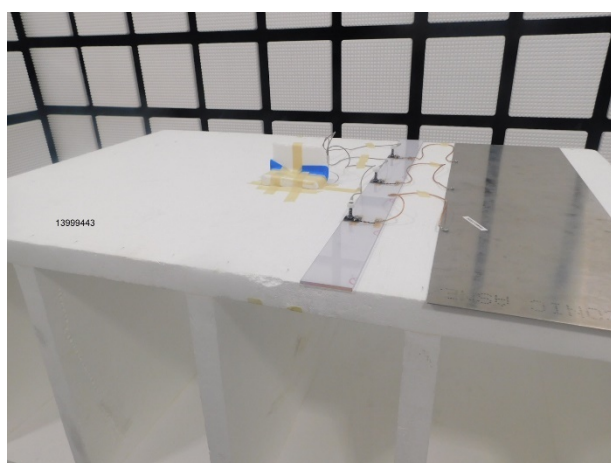


A1G FRONT PHOTO (Bands 5, 12, 13, 14, and 71)

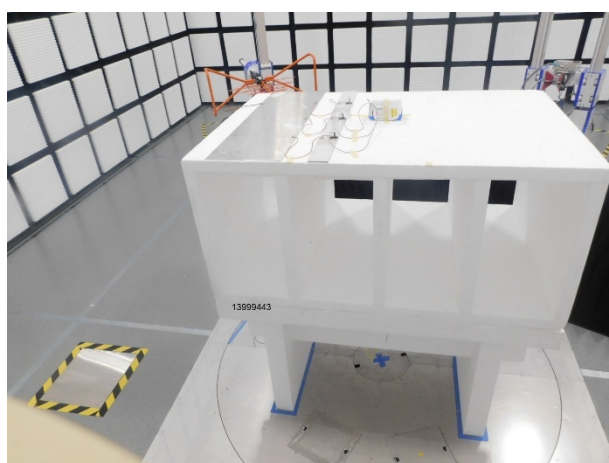


A1G BACK PHOTO (Bands 5, 12, 13, 14, and 71)

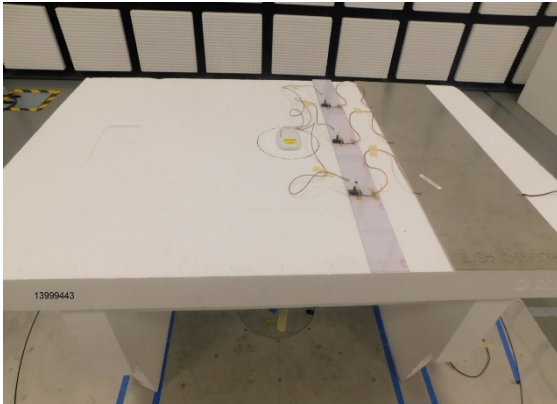


B1G FRONT PHOTO (Bands 2, 4, and 66)

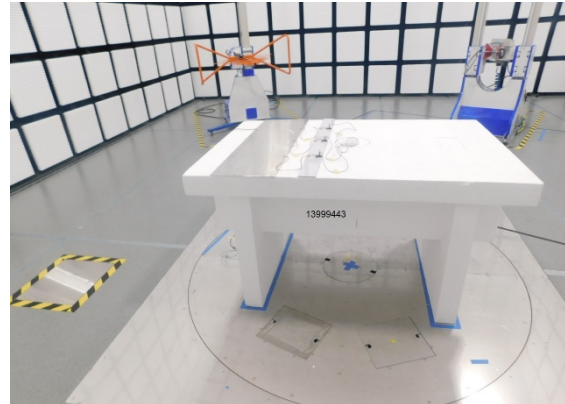

B1G BACK PHOTO (Bands 2, 4, and 66)

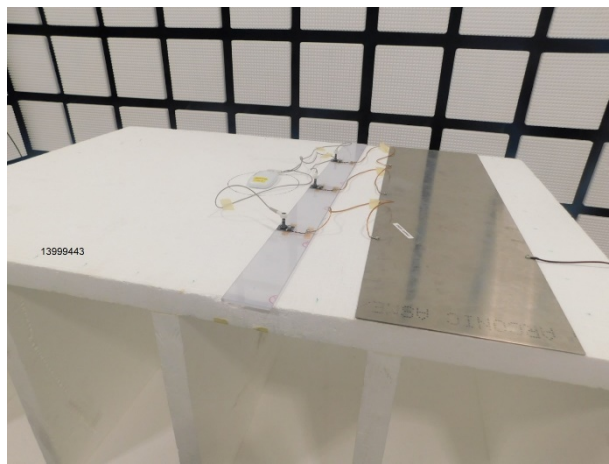

A1G FRONT PHOTO (Bands 2, 4, and 66)

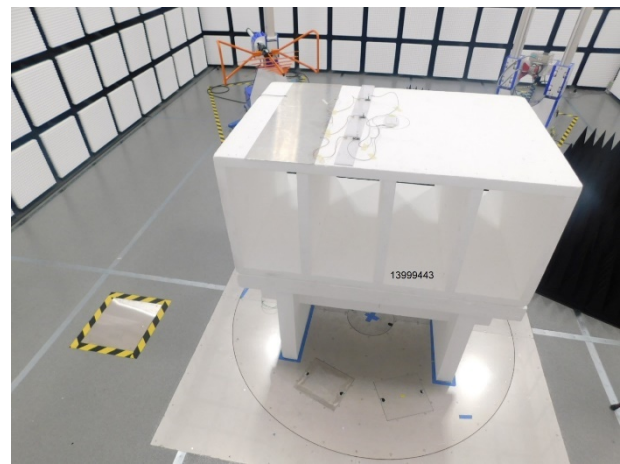

A1G BACK PHOTO (Bands 2, 4, and 66)

END OF REPORT