

Date: 2024-12-21

**System Check\_Head\_750MHz****DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_750\_241221 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.893$  S/m;  $\epsilon_r = 41.5$ 

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.06, 8.49, 8.31); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.431 W/kg; SAR (10g) = 0.288 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.435 W/kg; SAR (8g) = 0.314 W/kg; SAR (10g) = 0.300 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 90.8 %

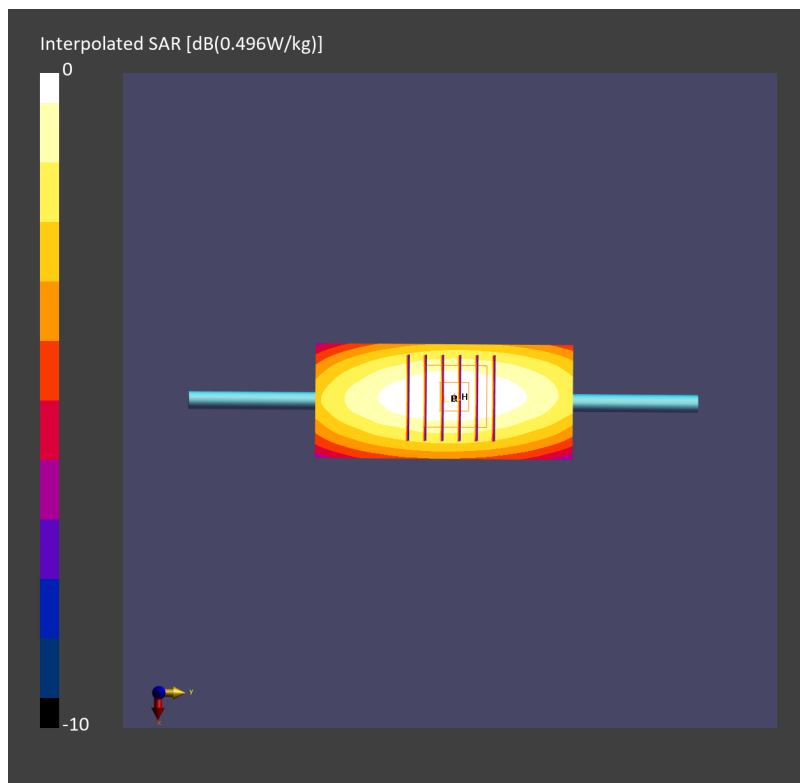

Date: 2024-12-24

**System Check\_Head\_750MHz****DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_750\_241224 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.897$  S/m;  $\epsilon_r = 42.2$ 

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.280 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 0.414 W/kg; SAR (8g) = 0.292 W/kg; SAR (10g) = 0.278 W/kg

Smallest distance from peaks to all points 3 dB below = 24.8 mm

Ratio of SAR at M2 to SAR at M1 = 90.4 %

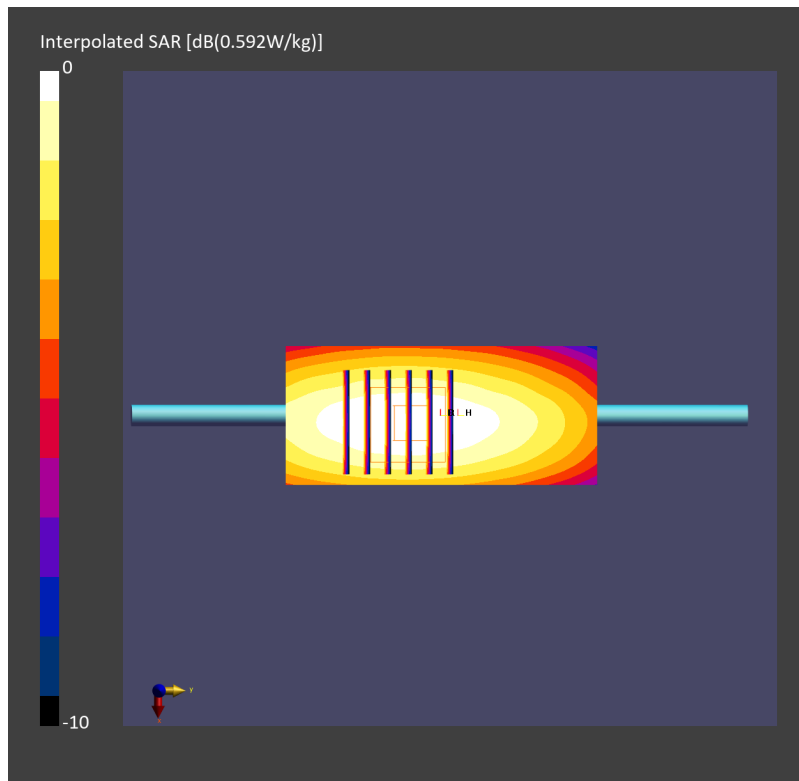

Date: 2025-01-12

**System Check\_Head\_750MHz****DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_750\_250112 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.892$  S/m;  $\epsilon_r = 41.8$ 

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(8.7, 8.49, 8.82); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.431 W/kg; SAR (10g) = 0.288 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.435 W/kg; SAR (8g) = 0.306 W/kg; SAR (10g) = 0.290 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

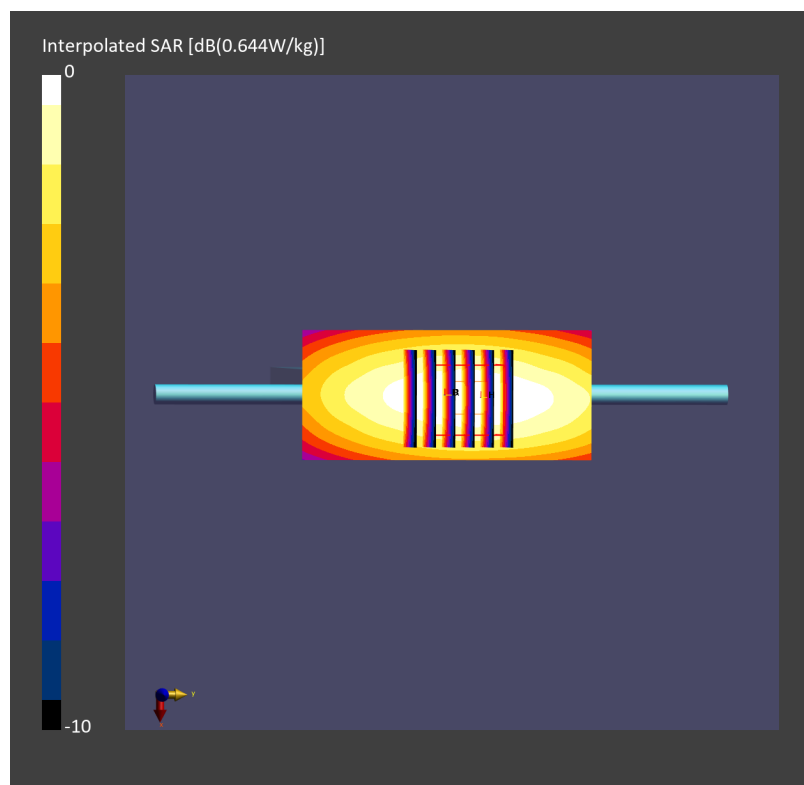

Date: 2025-01-13

**System Check\_Head\_750MHz****DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_750\_250113 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.886$  S/m;  $\epsilon_r = 42.9$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2024-05-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.384 W/kg; SAR (10g) = 0.260 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.397 W/kg; SAR (8g) = 0.282 W/kg; SAR (10g) = 0.269 W/kg

Smallest distance from peaks to all points 3 dB below = &gt; 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

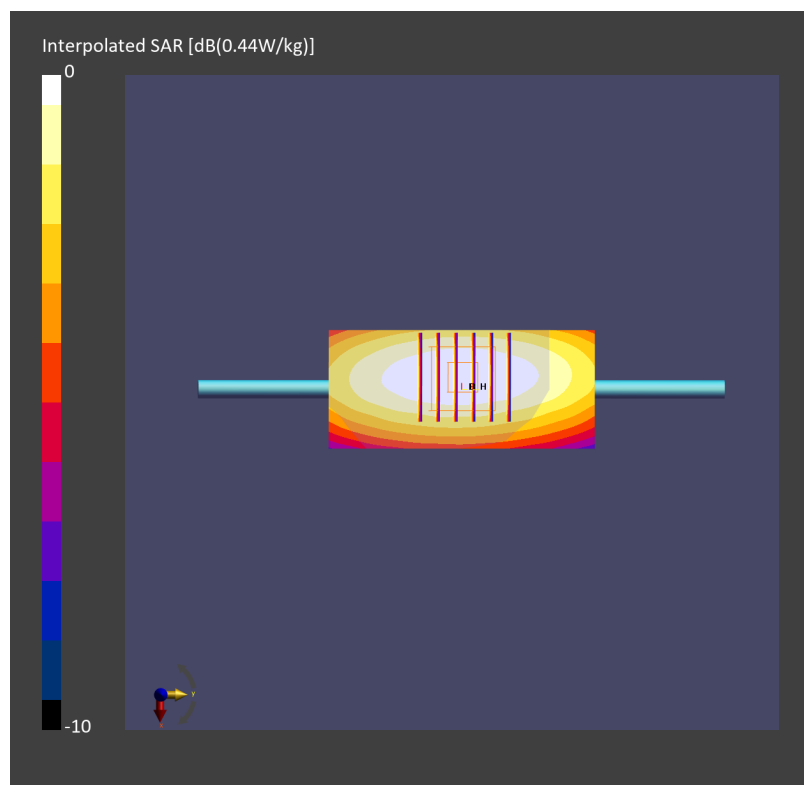

Date: 2024-12-21

**System Check\_Head\_850MHz****DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL\_850\_241221 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.927$  S/m;  $\epsilon_r = 41.2$ 

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(7.92, 8.34, 8.16); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.495 W/kg; SAR (10g) = 0.325 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.06 dB

SAR (1g) = 0.498 W/kg; SAR (8g) = 0.356 W/kg; SAR (10g) = 0.339 W/kg

Smallest distance from peaks to all points 3 dB below = 19.6 mm

Ratio of SAR at M2 to SAR at M1 = 90.0 %

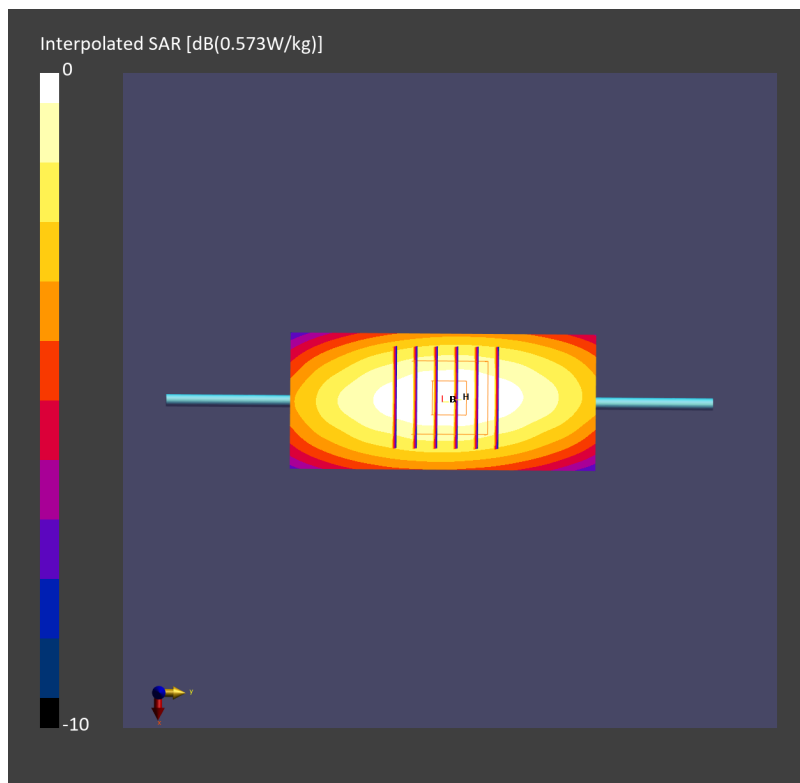

Date: 2024-12-24

**System Check\_Head\_850MHz****DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL\_850\_241224 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.932$  S/m;  $\epsilon_r = 41.9$ 

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.49, 9.77, 9.84); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.477 W/kg; SAR (10g) = 0.314 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.475 W/kg; SAR (8g) = 0.331 W/kg; SAR (10g) = 0.314 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

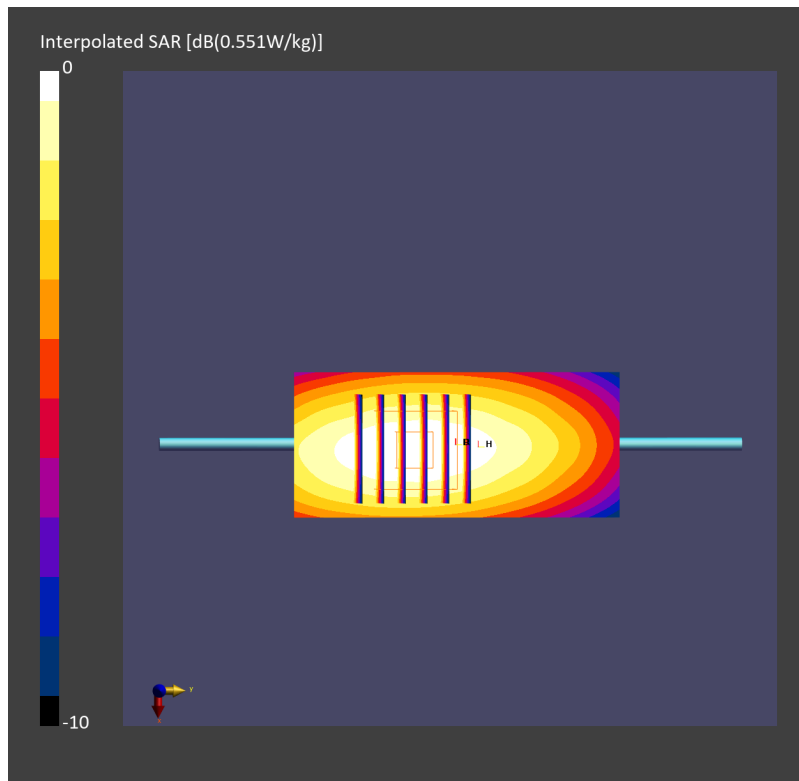

Date: 2025-01-12

**System Check\_Head\_835MHz****DUT: D835V2 - SN499**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL\_850\_250112 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.914$  S/m;  $\epsilon_r = 41.3$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(8.44, 8.25, 8.69); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.471 W/kg; SAR (10g) = 0.311 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 0.477 W/kg; SAR (8g) = 0.336 W/kg; SAR (10g) = 0.319 W/kg

Smallest distance from peaks to all points 3 dB below = &gt; 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

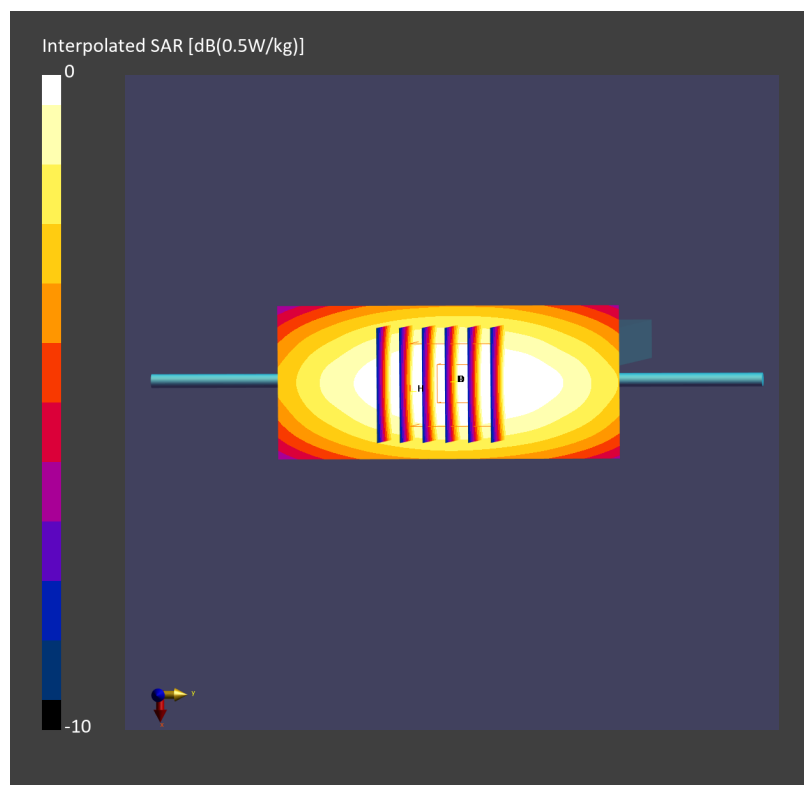

Date: 2024-12-22

**System Check\_Head\_1750MHz****DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL\_1750\_241222 Medium parameters used:  $f = 1750.000$  MHz;  $\sigma = 1.36$  S/m;  $\epsilon_r = 40.6$ 

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.82, 7.18, 7.03); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.83 W/kg; SAR (10g) = 0.975 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 1.82 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 87.7 %

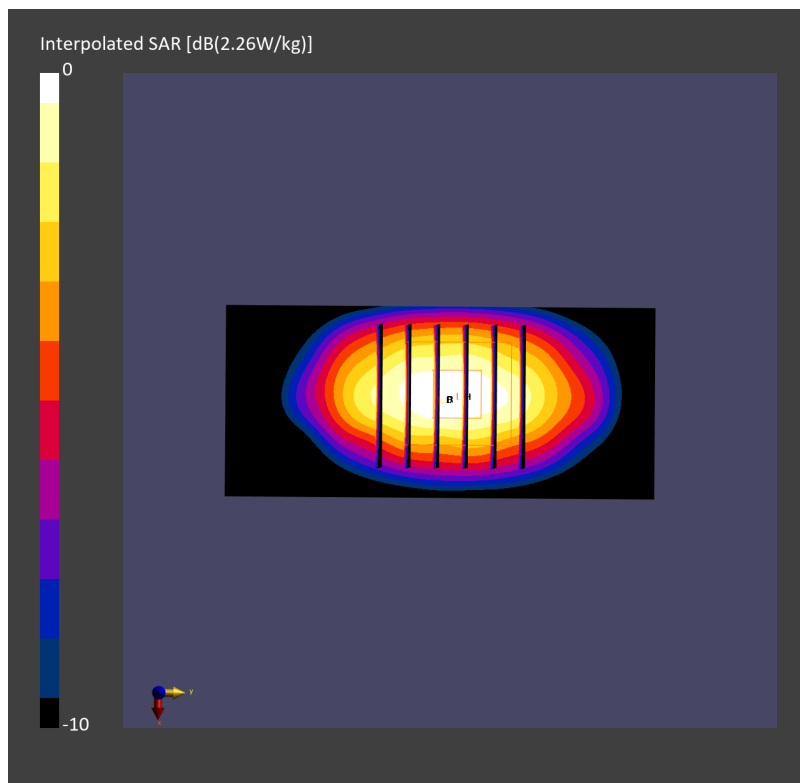

Date: 2024-12-25

**System Check\_Head\_1750MHz****DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL\_1750\_241225 Medium parameters used:  $f = 1750.000$  MHz;  $\sigma = 1.38$  S/m;  $\epsilon_r = 40.8$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.14, 8.24, 8.22); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 0.995 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.86 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

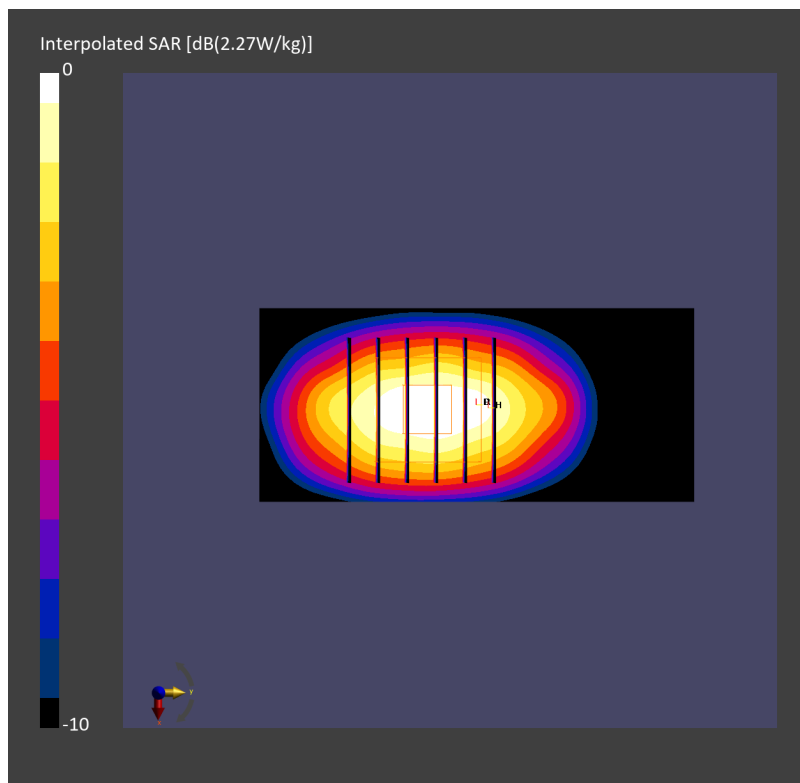

Date: 2025-01-08

**System Check\_Head\_1750MHz****DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL\_1750\_250108 Medium parameters used:  $f = 1750.000$  MHz;  $\sigma = 1.36$  S/m;  $\epsilon_r = 40.5$ 

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.86, 7.67, 8.57); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.954 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.74 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.936 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 86.2 %

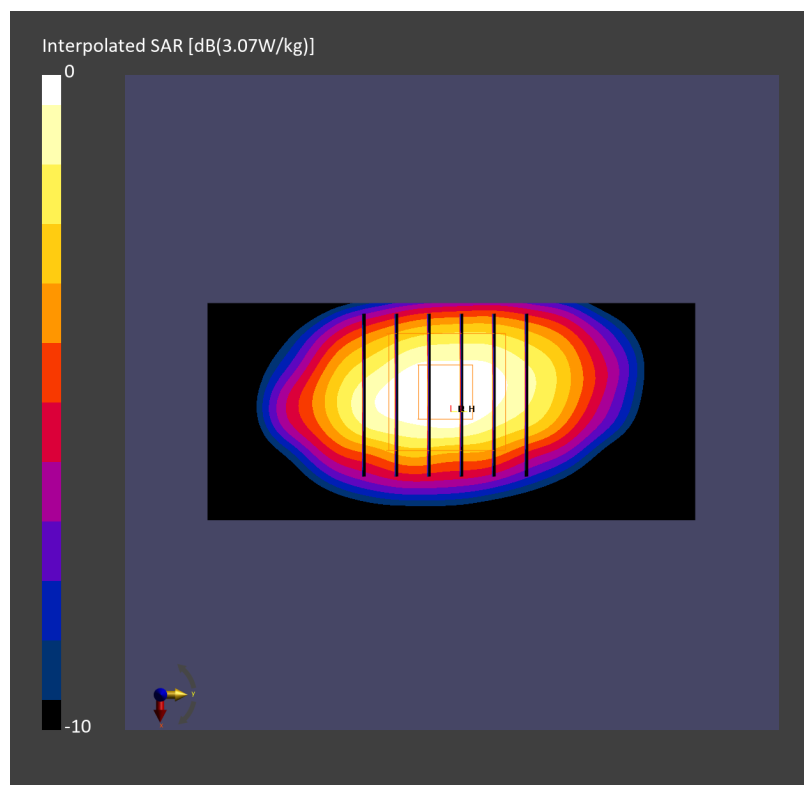

Date: 2024-12-22

**System Check\_Head\_1900MHz****DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL\_1900\_241222 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.44$  S/m;  $\epsilon_r = 39.1$ 

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.72, 7.08, 6.92); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.98 W/kg; SAR (10g) = 1.04 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.99 W/kg; SAR (8g) = 1.17 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 87.5 %

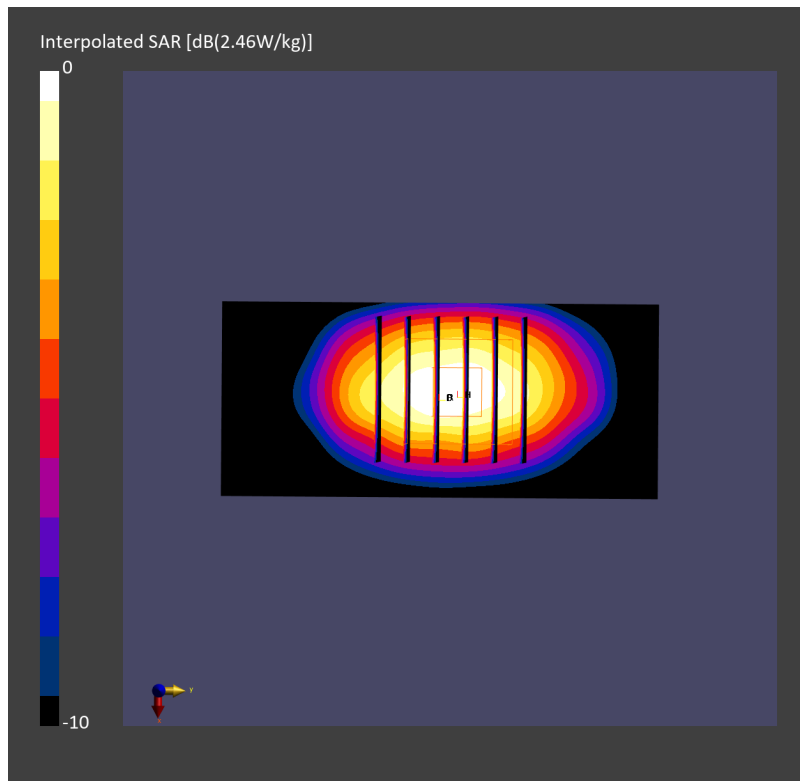

Date: 2024-12-25

**System Check\_Head\_1900MHz****DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL\_1900\_241225 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.45$  S/m;  $\epsilon_r = 39.3$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.7, 7.85, 7.85); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 1.00 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.93 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 86.0 %

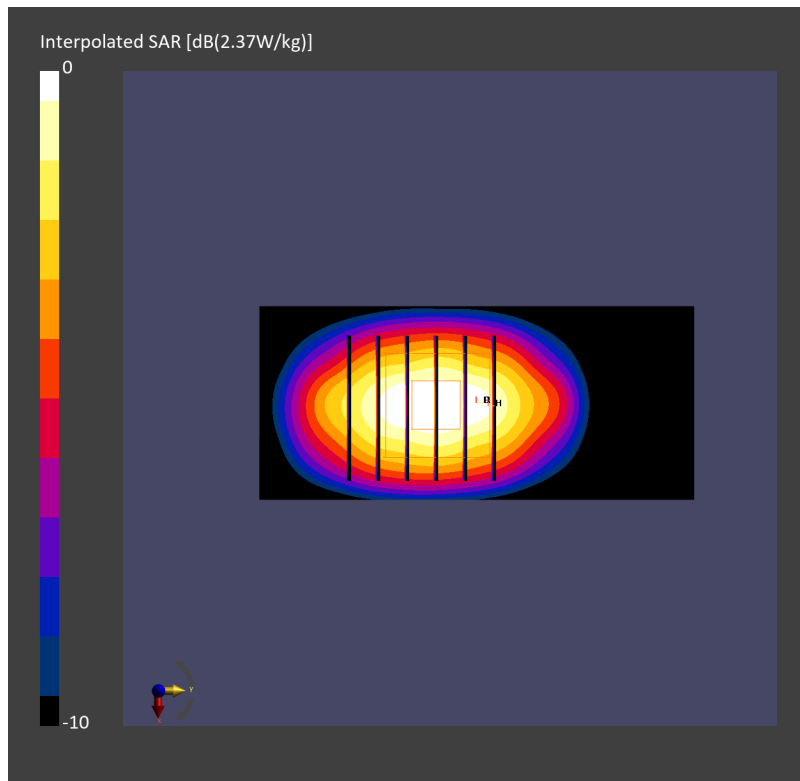

Date: 2025-01-08

**System Check\_Head\_1900MHz****DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL\_1900\_250108 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.44$  S/m;  $\epsilon_r = 39.0$ 

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.62, 7.44, 8.32); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.01 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.90 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 0.999 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.9 %

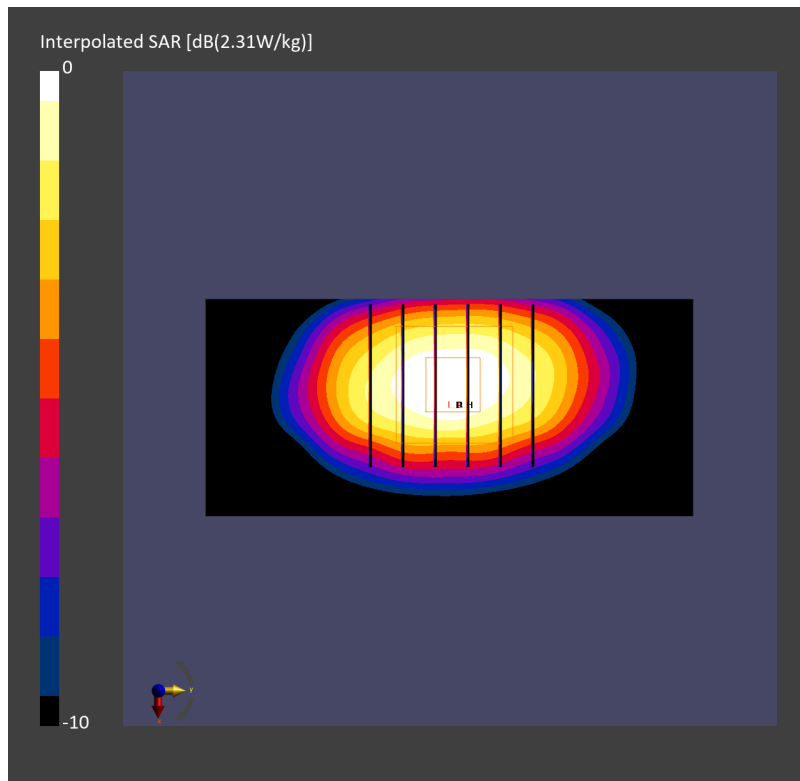

Date: 2024-12-23

**System Check\_Head\_2300MHz****DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL\_2300\_241223 Medium parameters used:  $f = 2300.000$  MHz;  $\sigma = 1.59$  S/m;  $\epsilon_r = 40.4$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.55, 6.9, 6.76); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.19 W/kg; SAR (10g) = 1.04 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.19 W/kg; SAR (8g) = 1.20 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

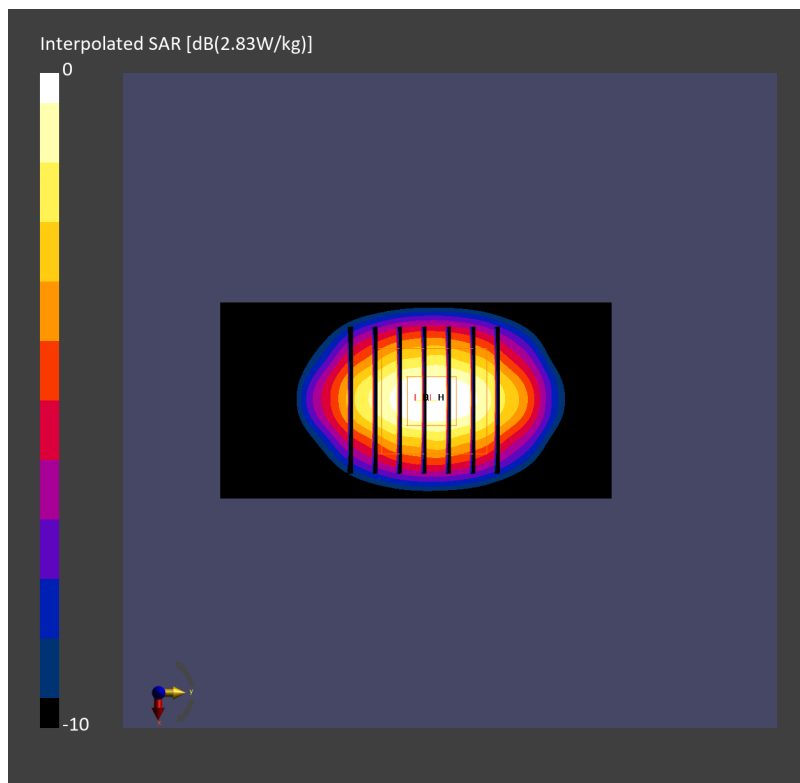

Date: 2024-12-26

**System Check\_Head\_2300MHz****DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL\_2300\_241226 Medium parameters used:  $f = 2300.000$  MHz;  $\sigma = 1.62$  S/m;  $\epsilon_r = 40.7$ 

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.36, 7.47, 7.48); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.30 W/kg; SAR (10g) = 1.09 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.28 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

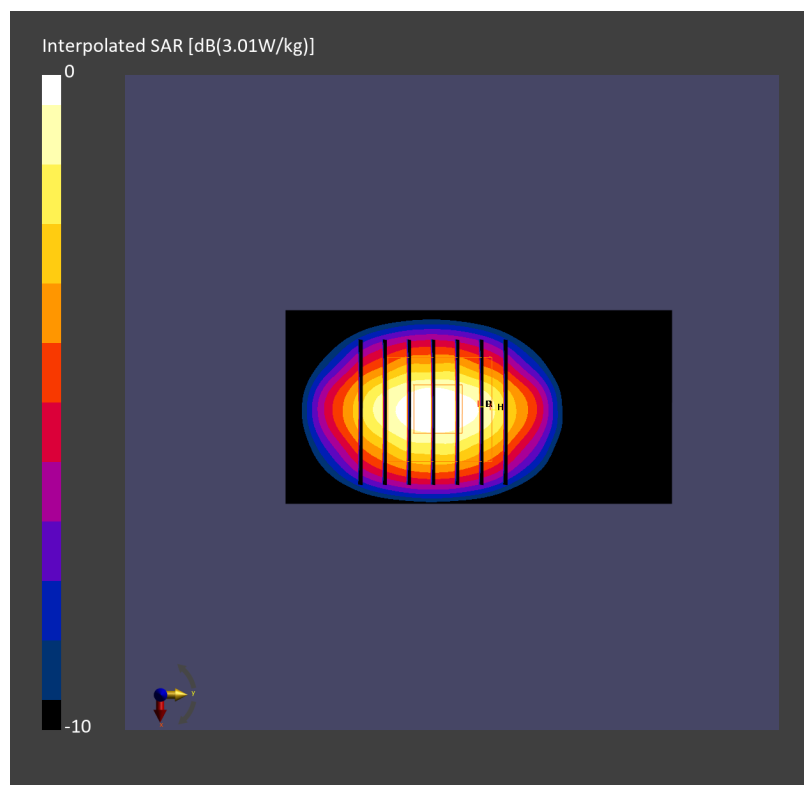

Date: 2024-12-23

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_241223 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.91$  S/m;  $\epsilon_r = 39.2$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.24, 6.57, 6.44); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.19 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.67 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.3 %

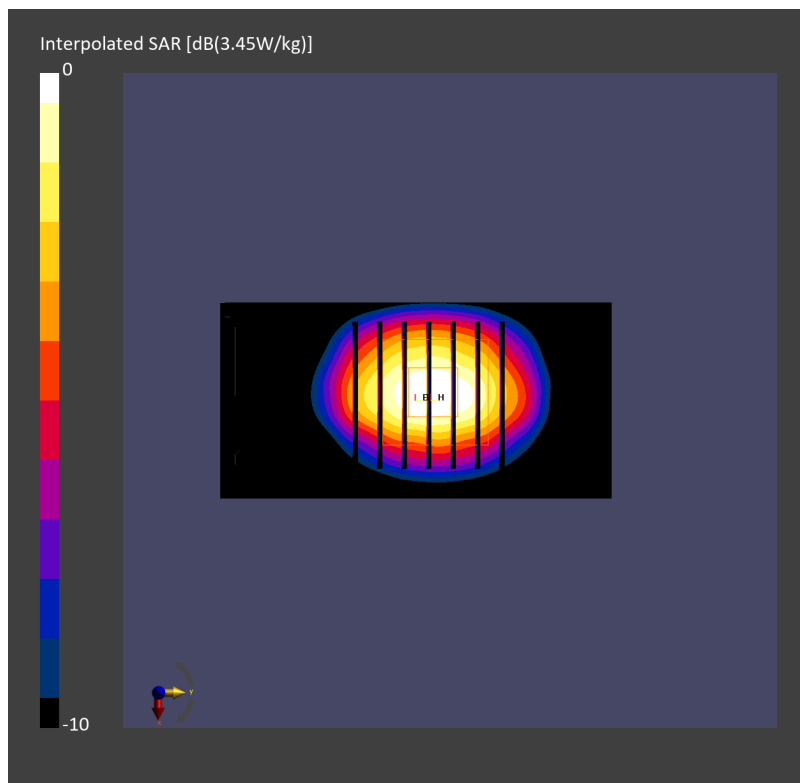

Date: 2024-12-26

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_241226 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.97$  S/m;  $\epsilon_r = 39.6$ 

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.33, 7.44, 7.46); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.63 W/kg; SAR (10g) = 1.20 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.65 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

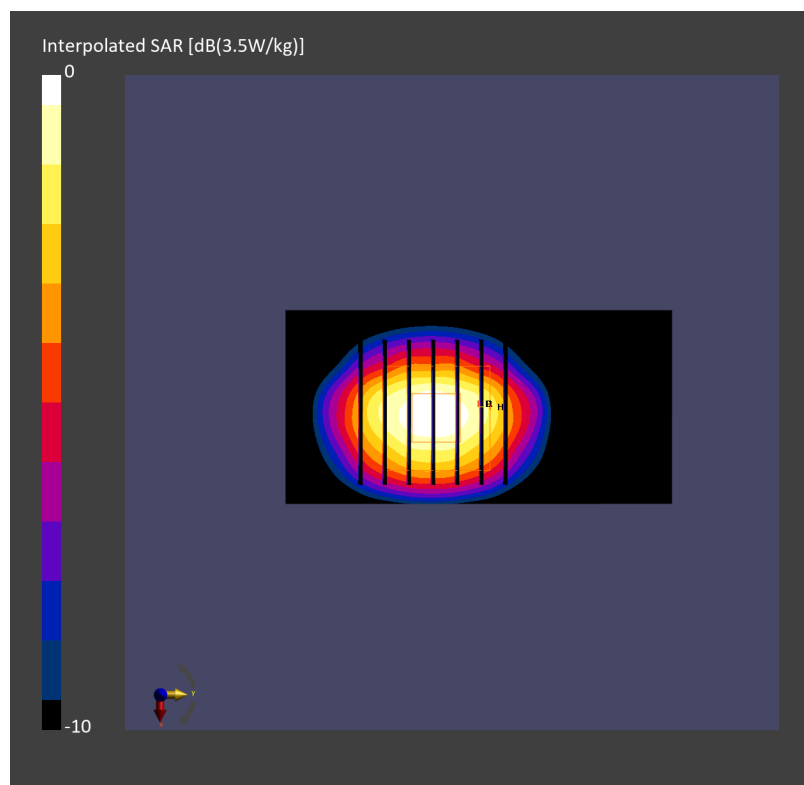

Date: 2025-01-10

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_250110 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 2.00$  S/m;  $\epsilon_r = 38.4$ 

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.52, 6.78, 6.82); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.26 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.78 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 80.5 %

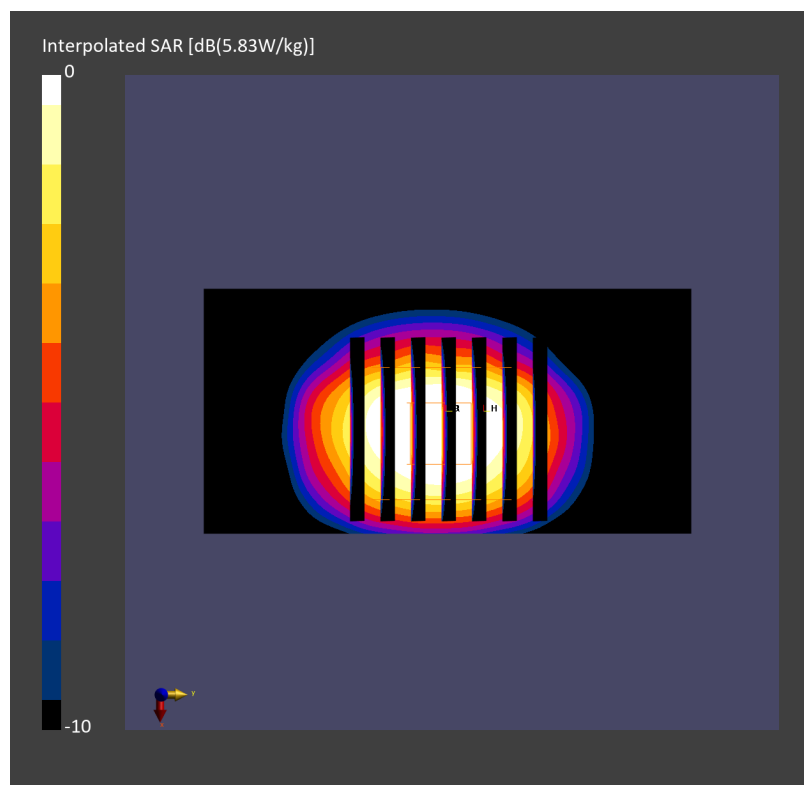

Date: 2025-01-14

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_250114 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.98$  S/m;  $\epsilon_r = 38.6$ 

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.52, 6.78, 6.82); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.64 W/kg; SAR (10g) = 1.17 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.62 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

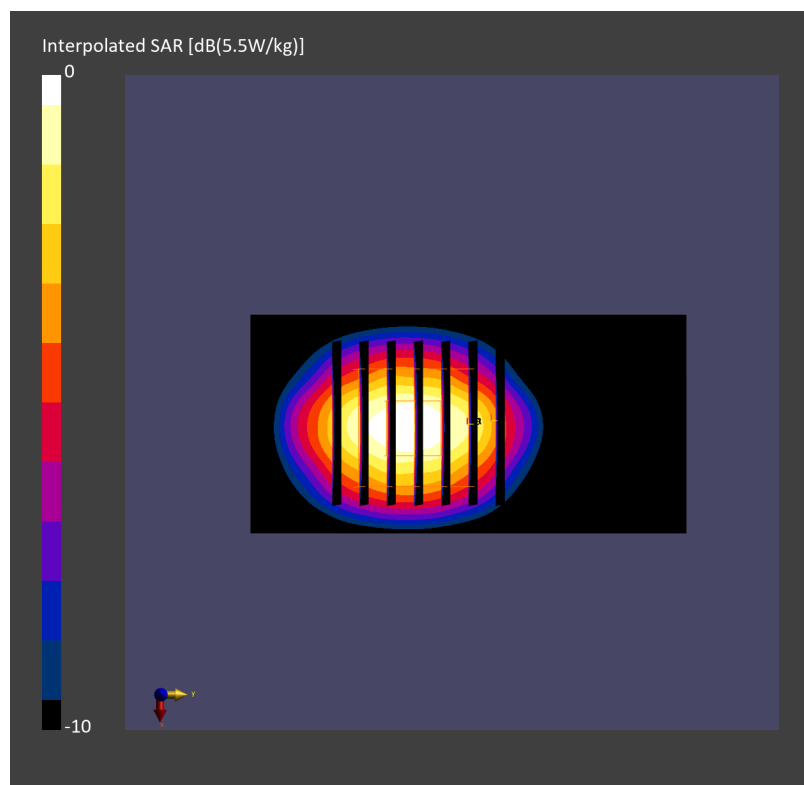

Date: 2025-01-15

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_250115 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.99$  S/m;  $\epsilon_r = 38.7$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.52, 6.78, 6.82); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.18 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.64 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

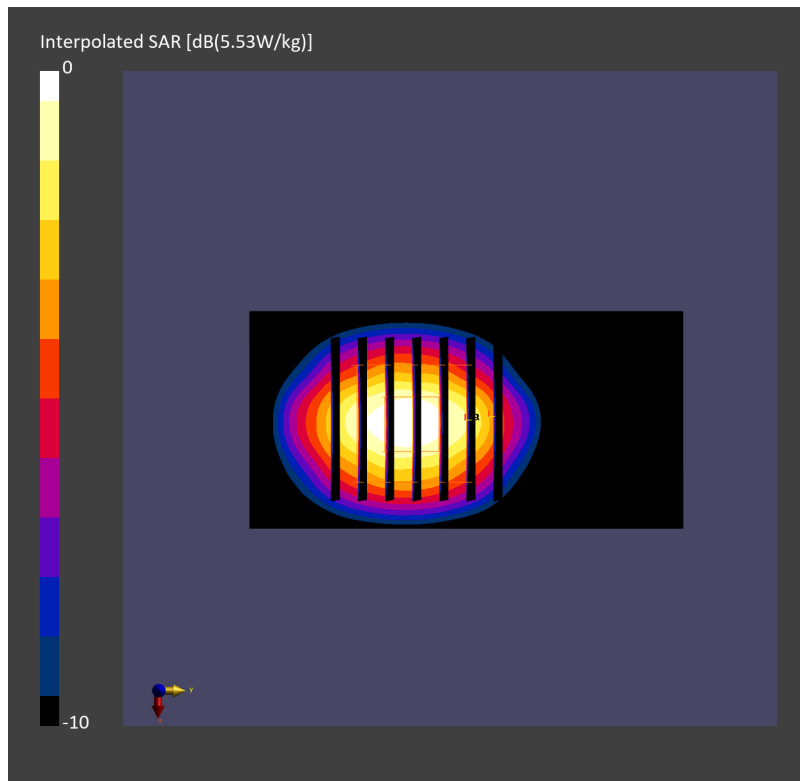

Date: 2025-01-16

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_250116 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 2.00$  S/m;  $\epsilon_r = 38.7$ 

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.52, 6.78, 6.82); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.19 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.66 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.6 %

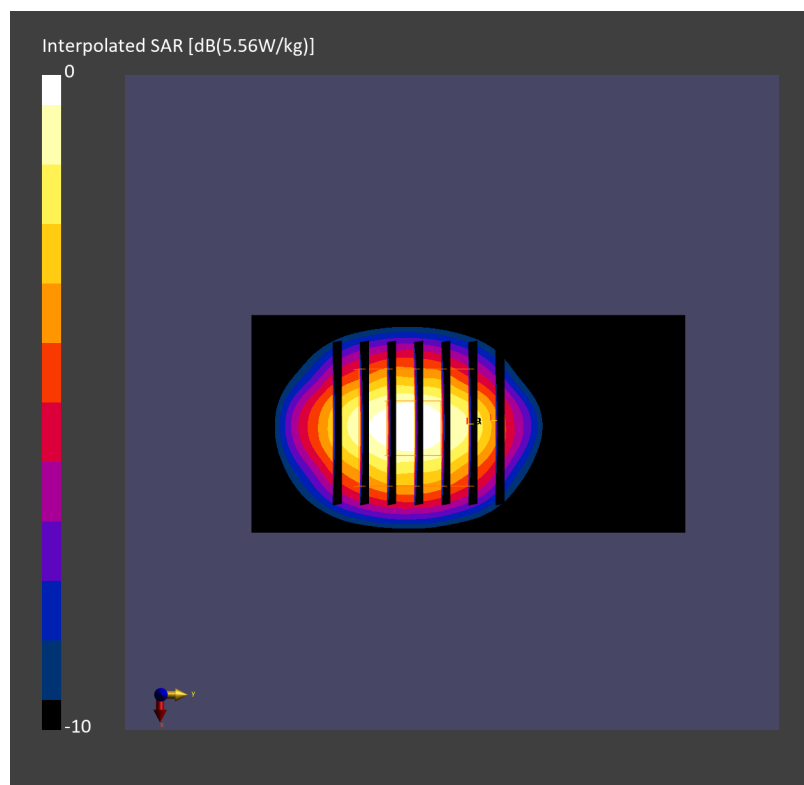

Date: 2024-12-24

**System Check\_Head\_3500MHz****DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_3500\_241224 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.91$  S/m;  $\epsilon_r = 37.9$ 

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.42, 5.71, 5.59); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.40 W/kg; SAR (10g) = 1.30 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.44 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.0 %

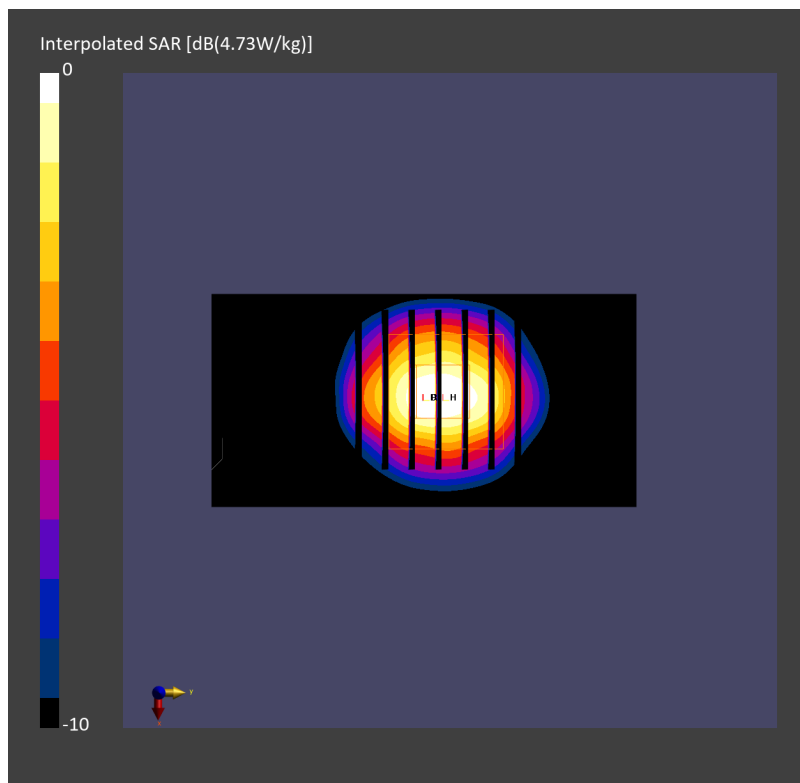

Date: 2024-12-27

**System Check\_Head\_3500MHz****DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_3500\_241227 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 3.00$  S/m;  $\epsilon_r = 37.8$ 

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.94, 7.01, 6.98); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.27 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.3 %

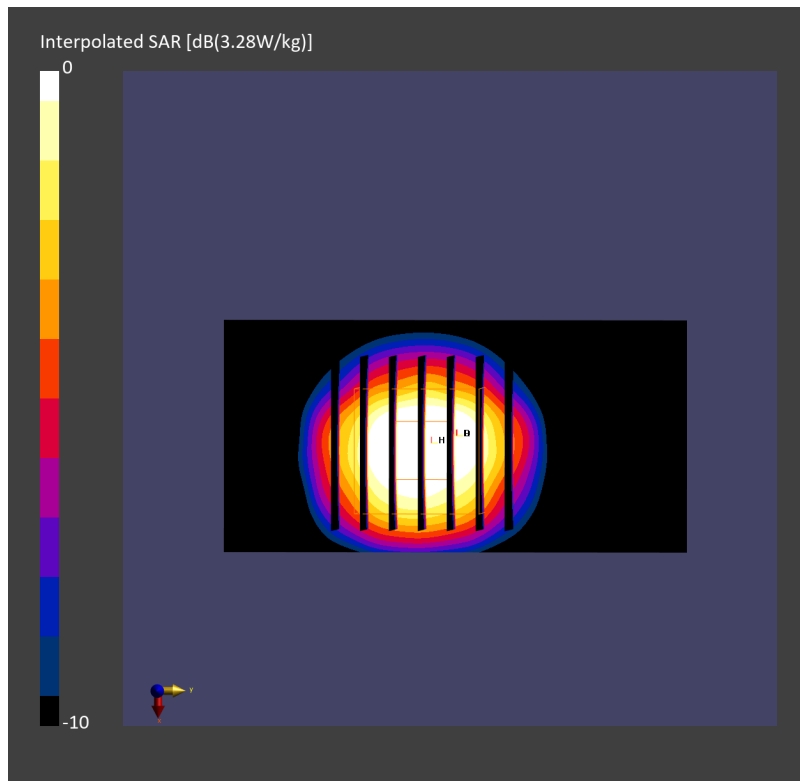

Date: 2025-01-10

**System Check\_Head\_3500MHz****DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_3500\_250110 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.89$  S/m;  $\epsilon_r = 37.9$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.34, 6.42, 6.99); Calibrated: 2024-05-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2024-05-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.26 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.29 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

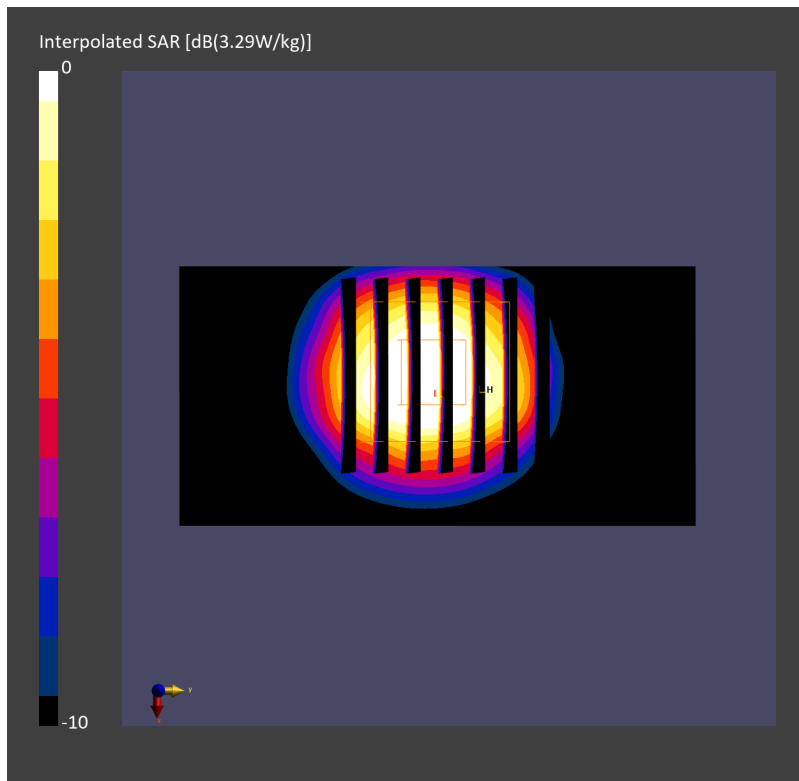

Date: 2025-01-11

**System Check\_Head\_3500MHz****DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_3500\_250111 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.94$  S/m;  $\epsilon_r = 38.1$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.2, 6.41, 6.45); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.03 W/kg; SAR (10g) = 1.14 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.08 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.5 %

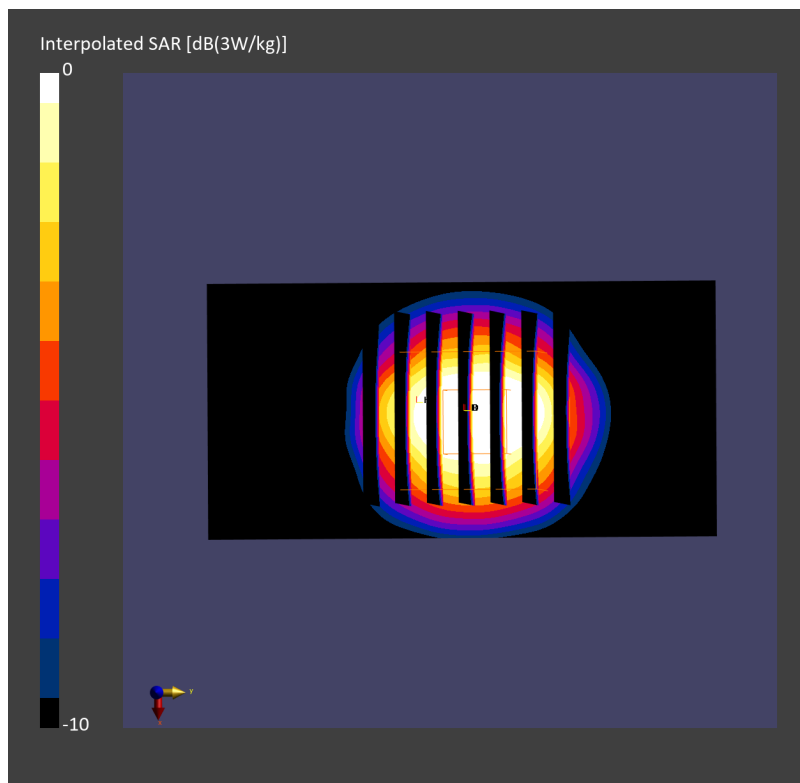

Date: 2025-01-17

**System Check\_Head\_3500MHz****DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_3500\_250117 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.95$  S/m;  $\epsilon_r = 37.9$ 

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.2, 6.41, 6.45); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.20 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.19 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.7 %

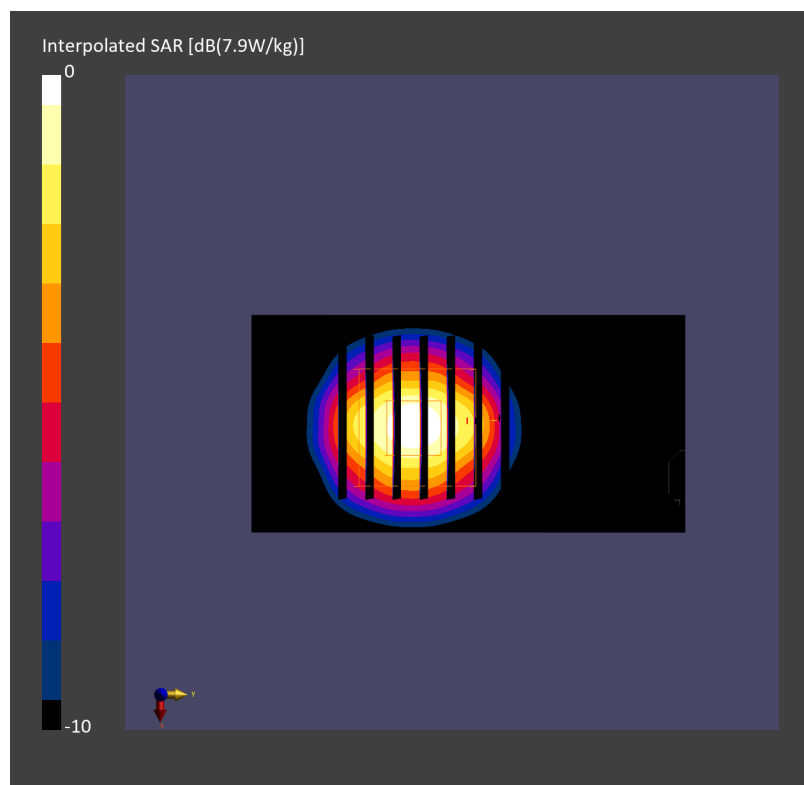

Date: 2025-01-18

**System Check\_Head\_3500MHz****DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_3500\_250118 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.97$  S/m;  $\epsilon_r = 38.0$ 

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.2, 6.41, 6.45); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.20 W/kg; SAR (10g) = 1.21 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.20 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 78.0 %

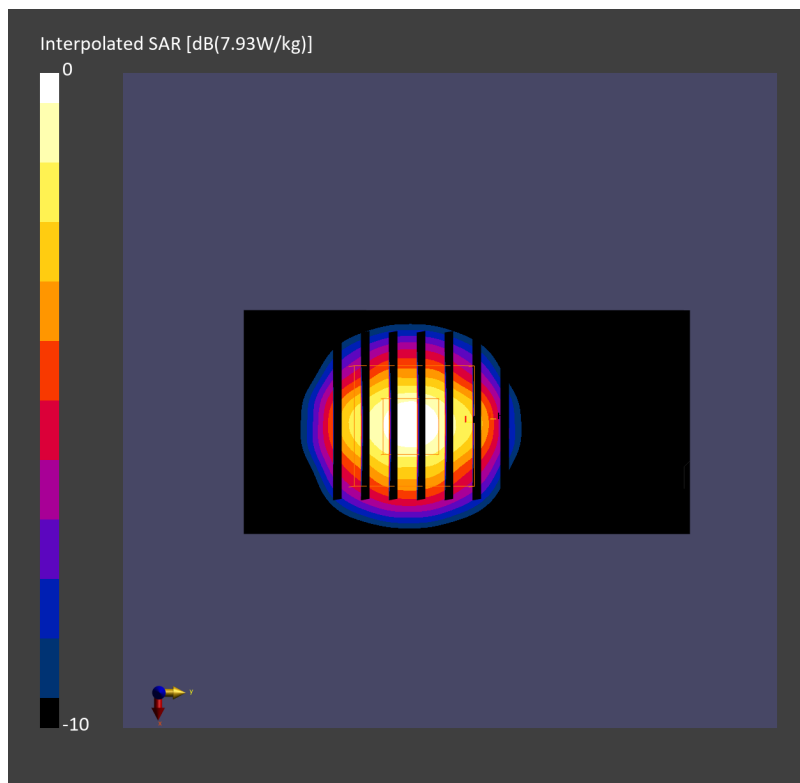

Date: 2024-12-24

**System Check\_Head\_3700MHz****DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_3700\_241224 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 3.11$  S/m;  $\epsilon_r = 37.7$ 

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.49, 5.79, 5.66); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 1.26 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.41 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.2 %

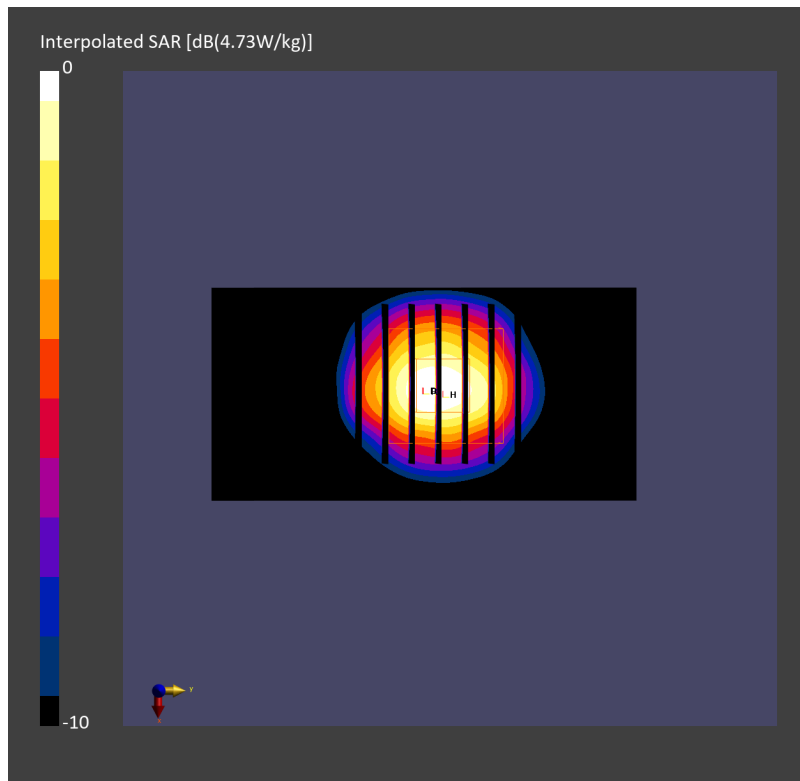

Date: 2024-12-27

**System Check\_Head\_3700MHz****DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_3700\_241227 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 3.16$  S/m;  $\epsilon_r = 37.5$ 

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.95, 6.98, 7.0); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.09 W/kg; SAR (10g) = 1.18 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.15 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.4 %

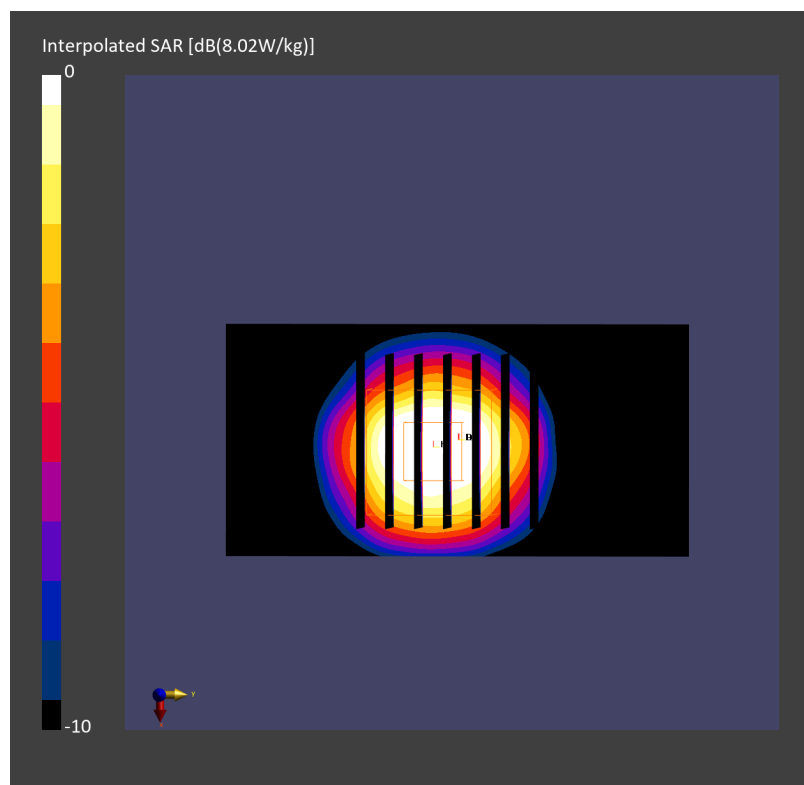

Date: 2025-01-10

**System Check\_Head\_3700MHz****DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_3700\_250110 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 3.08$  S/m;  $\epsilon_r = 37.8$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.22, 6.3, 6.87); Calibrated: 2024-05-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2024-05-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.05 W/kg; SAR (10g) = 1.20 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.21 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

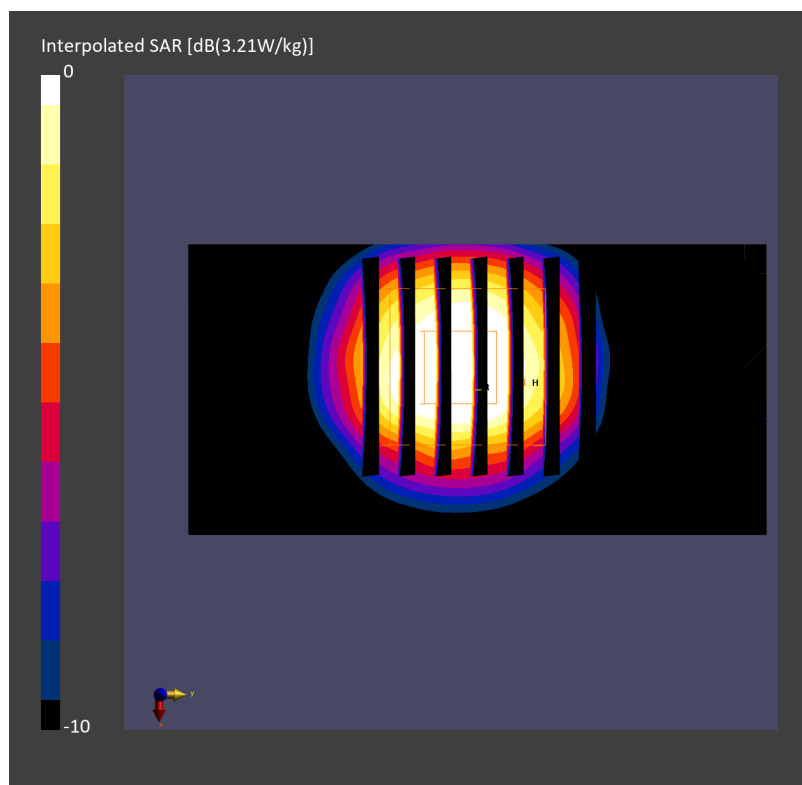

Date: 2025-01-11

**System Check\_Head\_3700MHz****DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_3700\_250111 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 3.10$  S/m;  $\epsilon_r = 37.8$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.14, 6.36, 6.41); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.14 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.10 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

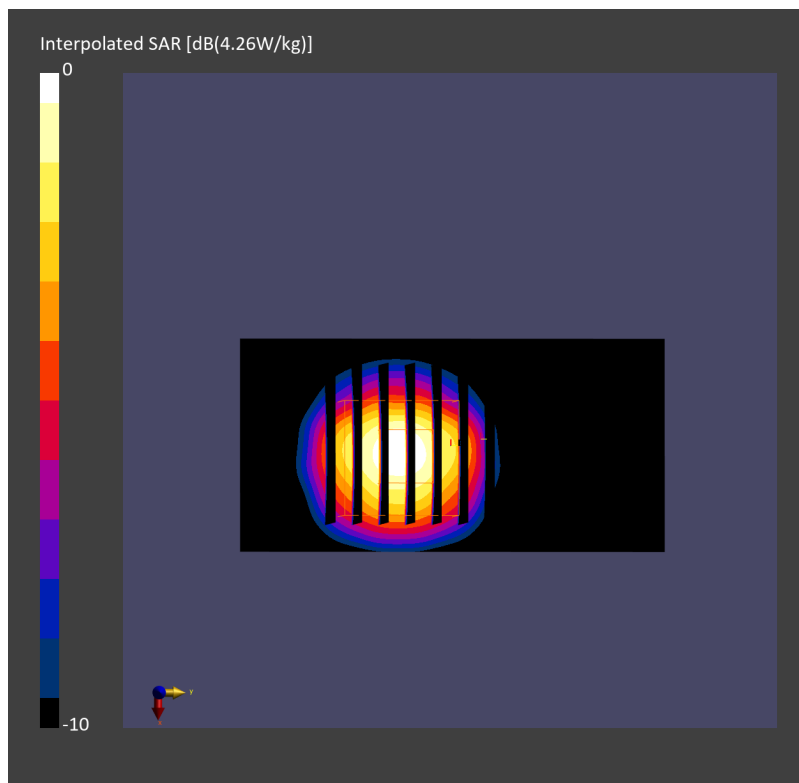

Date: 2025-01-19

**System Check\_Head\_3700MHz****DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_3700\_250119 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 3.15$  S/m;  $\epsilon_r = 38.0$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.14, 6.36, 6.41); Calibrated: 2024-03-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.15 W/kg; SAR (10g) = 1.18 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.18 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.0 %

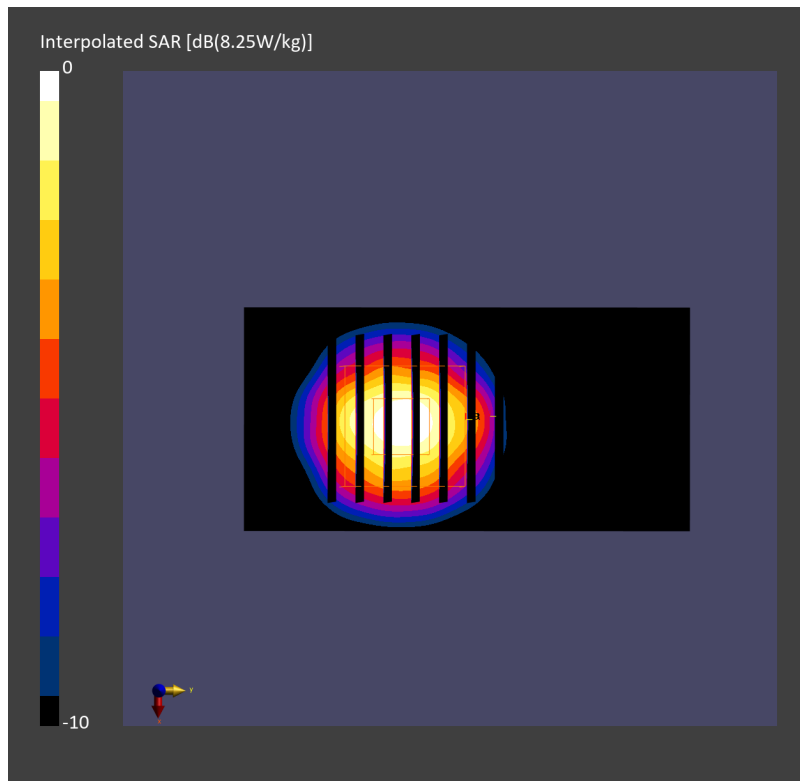

Date: 2024-12-24

**System Check\_Head\_3900MHz****DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_3900\_241224 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.32$  S/m;  $\epsilon_r = 37.5$ 

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.38, 5.66, 5.54); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.16 W/kg; SAR (10g) = 1.14 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.27 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.5 %

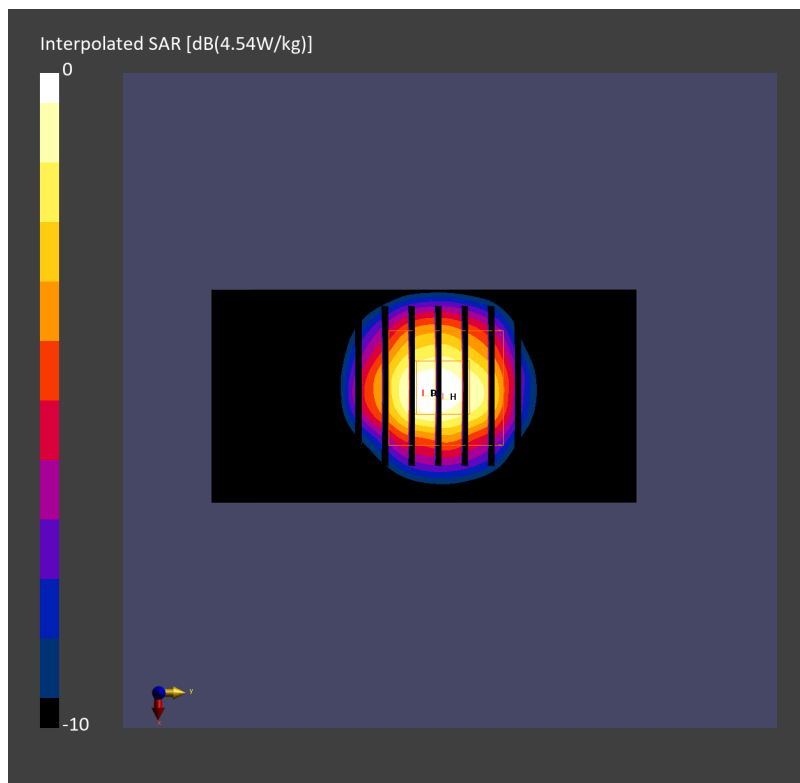

Date: 2024-12-27

**System Check\_Head\_3900MHz****DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_3900\_241227 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.33$  S/m;  $\epsilon_r = 37.3$ 

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.52, 6.53, 6.5); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2024-09-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.05 W/kg; SAR (10g) = 1.11 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.13 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

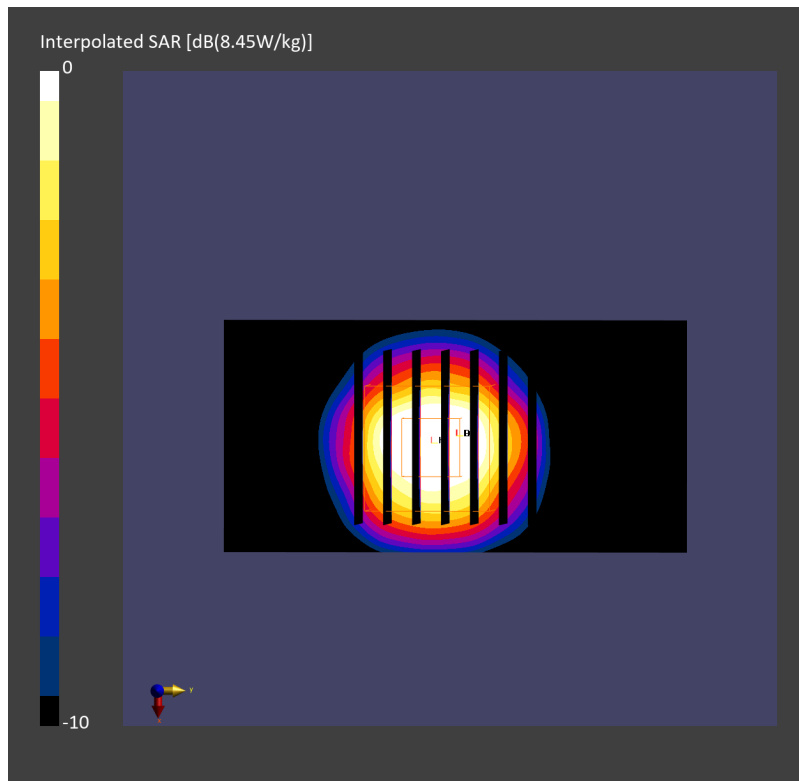

Date: 2025-01-20

**System Check\_Head\_3900MHz****DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_3900\_250120 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.33$  S/m;  $\epsilon_r = 37.7$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(6.48, 6.2, 6.35); Calibrated: 2024-06-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2024-02-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.11 W/kg;

**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.12 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.4 %

