

Date: 2025-01-27

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250127 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.893$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(10.07, 10.07, 10.07); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.280 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.05 dB

SAR (1g) = 0.426 W/kg; SAR (8g) = 0.302 W/kg; SAR (10g) = 0.281 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

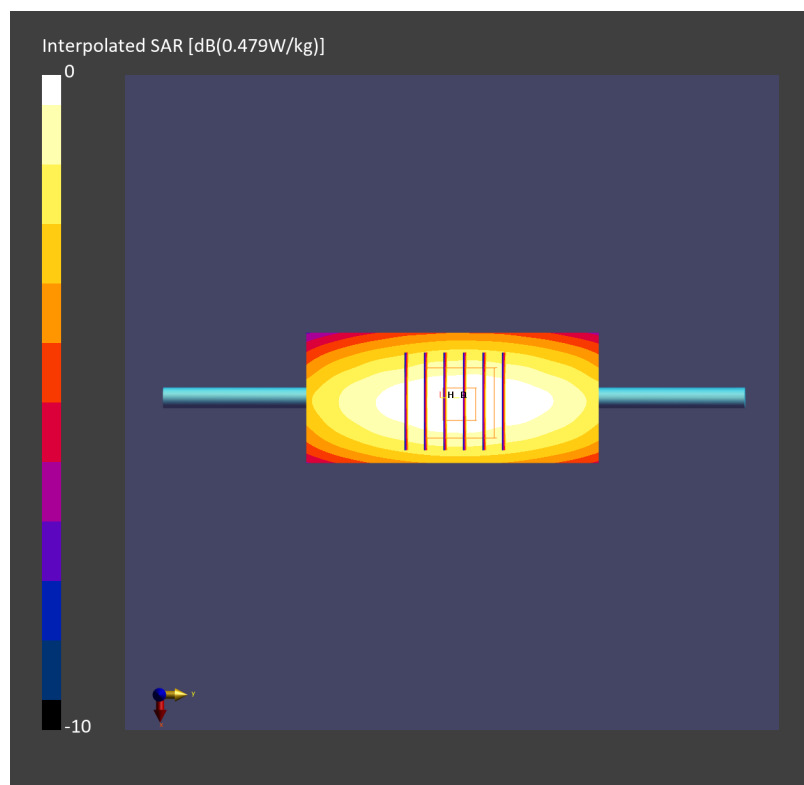

Date: 2025-01-28

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250128 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.895$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(10.07, 10.07, 10.07); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.421 W/kg; SAR (10g) = 0.281 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 0.430 W/kg; SAR (8g) = 0.303 W/kg; SAR (10g) = 0.291 W/kg

Smallest distance from peaks to all points 3 dB below = 19.6 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

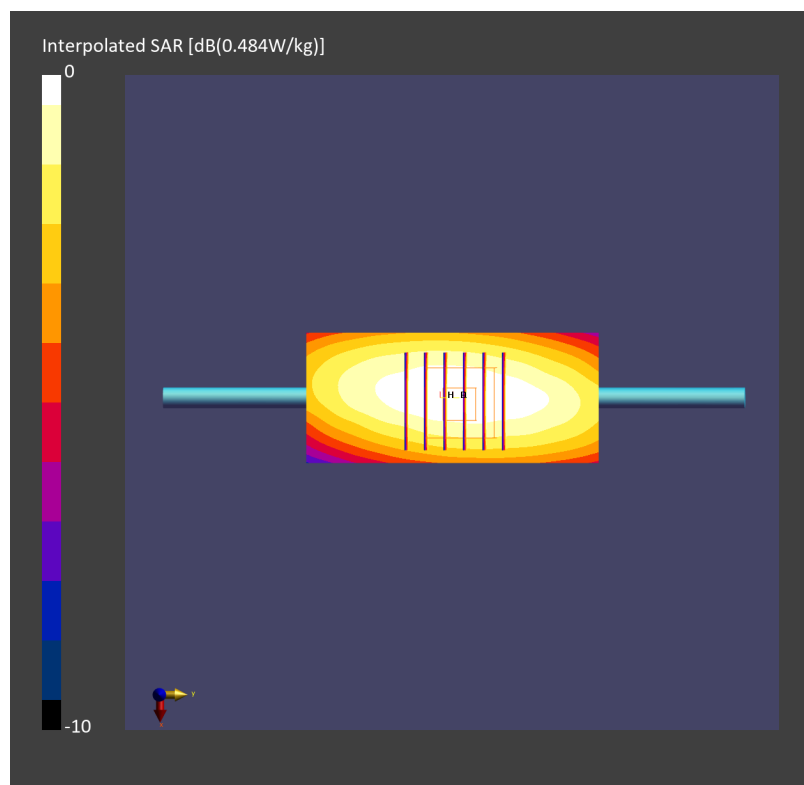

Date: 2025-01-29

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250129 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.890$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(10.07, 10.07, 10.07); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.420 W/kg; SAR (10g) = 0.281 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 0.429 W/kg; SAR (8g) = 0.302 W/kg; SAR (10g) = 0.288 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

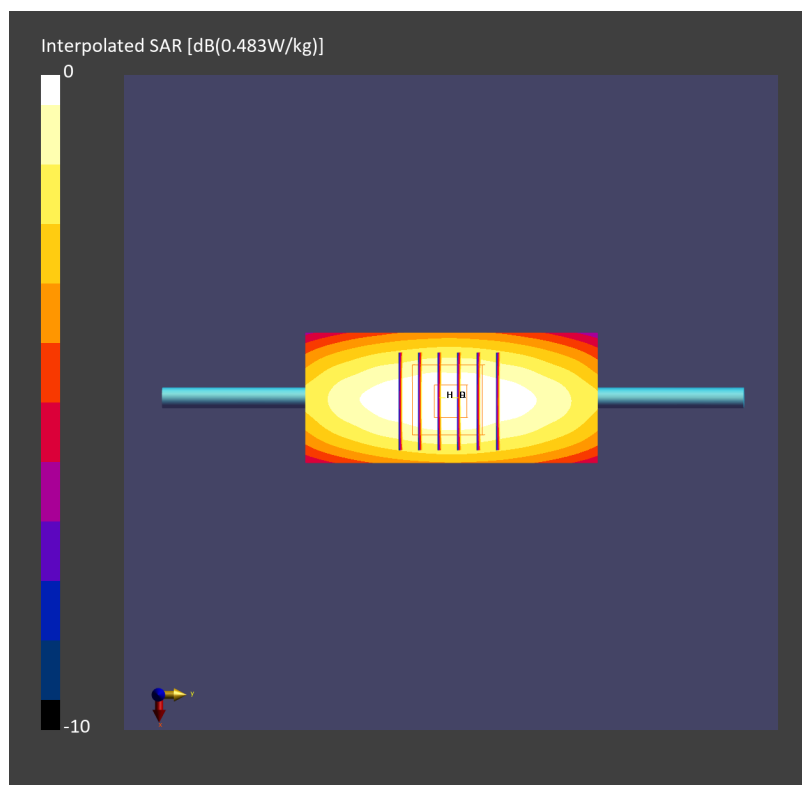

Date: 2025-01-30

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250130 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.887$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(10.07, 10.07, 10.07); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.424 W/kg; SAR (10g) = 0.285 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.434 W/kg; SAR (8g) = 0.307 W/kg; SAR (10g) = 0.292 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.0 %

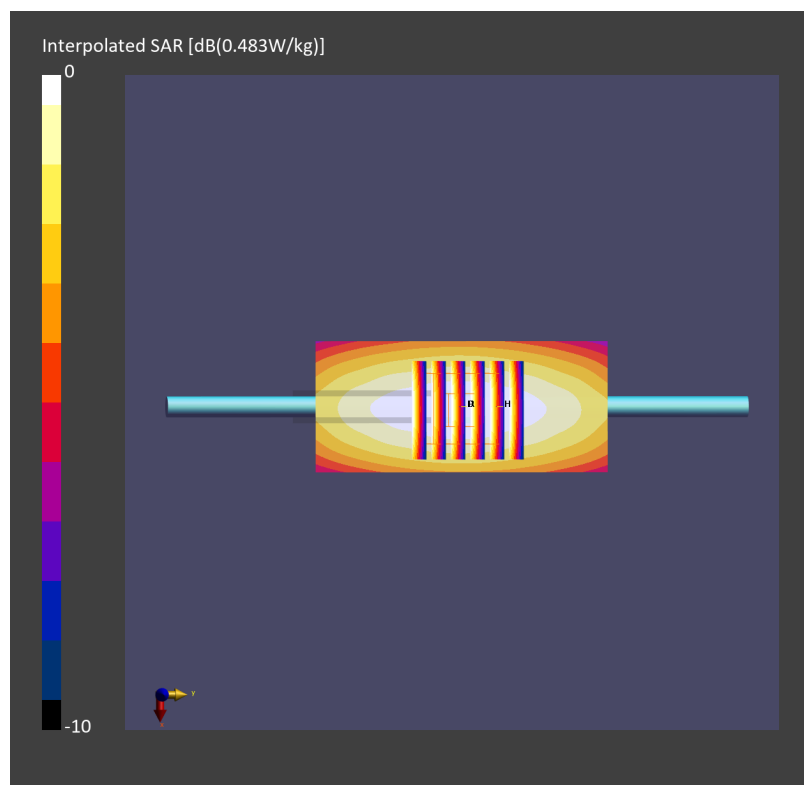

Date: 2025-01-31

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250131 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.921$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(9.92, 9.92, 9.92); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.451 W/kg; SAR (10g) = 0.297 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 0.464 W/kg; SAR (8g) = 0.324 W/kg; SAR (10g) = 0.308 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

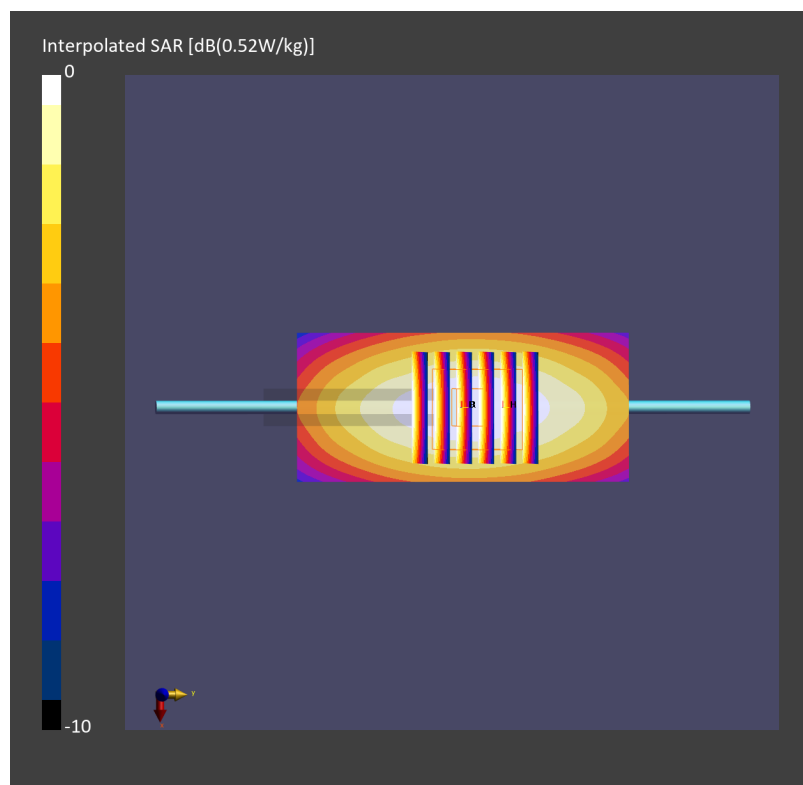

Date: 2025-02-01

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250201 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.918$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(9.92, 9.92, 9.92); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.449 W/kg; SAR (10g) = 0.296 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.463 W/kg; SAR (8g) = 0.323 W/kg; SAR (10g) = 0.307 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

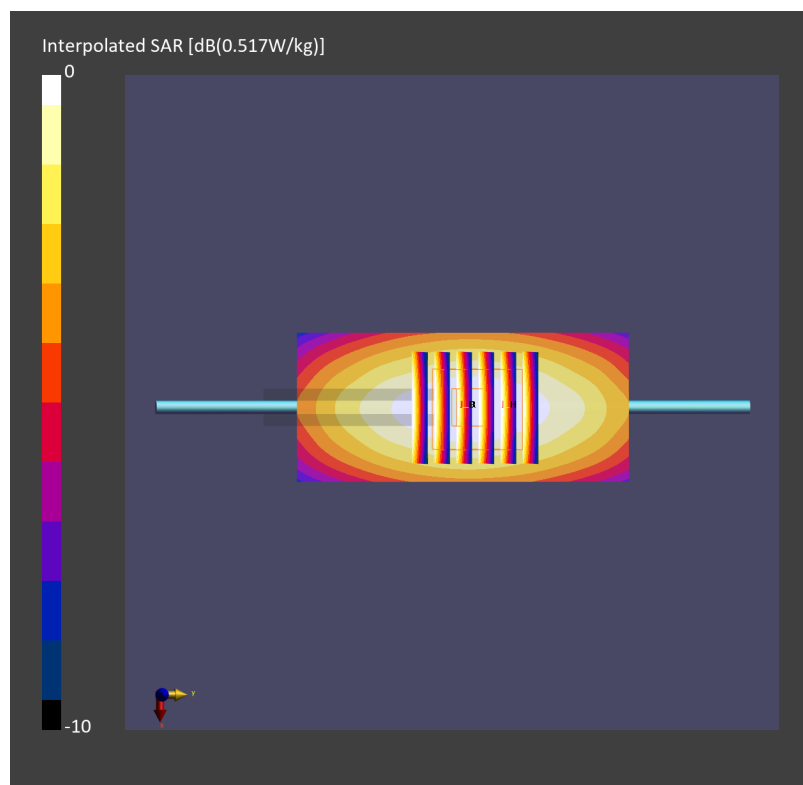

Date: 2025-02-03

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250203 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(9.03, 9.03, 9.03); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.71 W/kg; SAR (10g) = 0.909 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.964 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 82.5 %

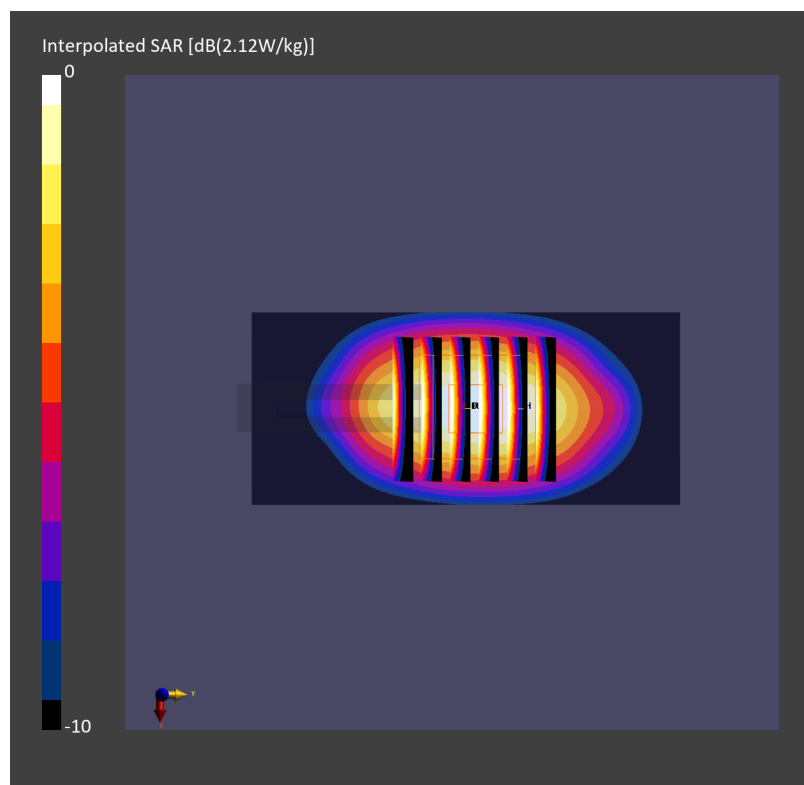

Date: 2025-02-04

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250204 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(9.03, 9.03, 9.03); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.72 W/kg; SAR (10g) = 0.915 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 1.79 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.970 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 82.6 %

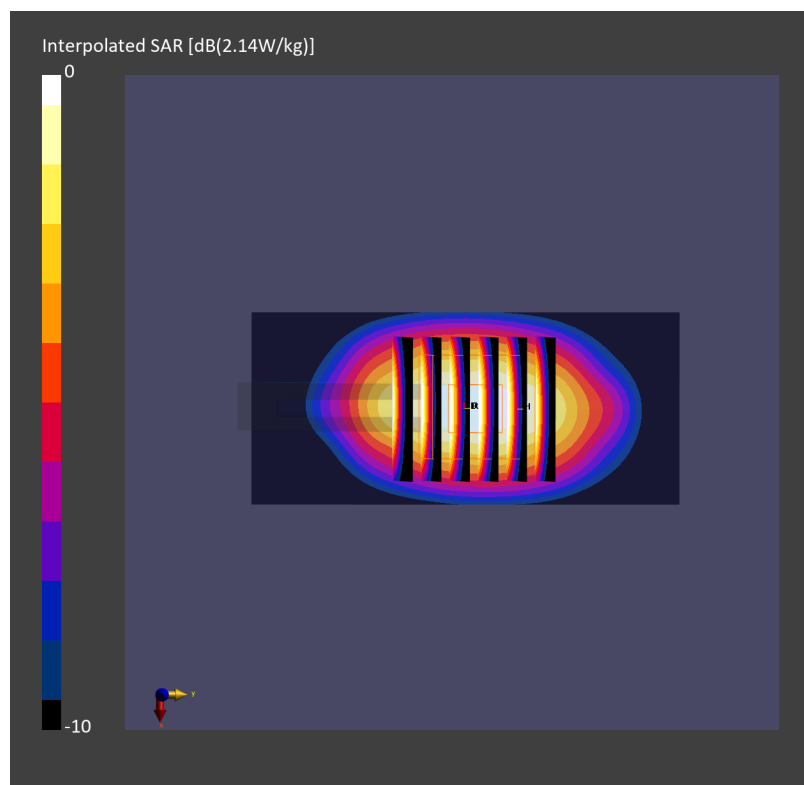

Date: 2025-02-06

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250206 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(8.73, 8.73, 8.73); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.77 W/kg; SAR (10g) = 0.918 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.84 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.977 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

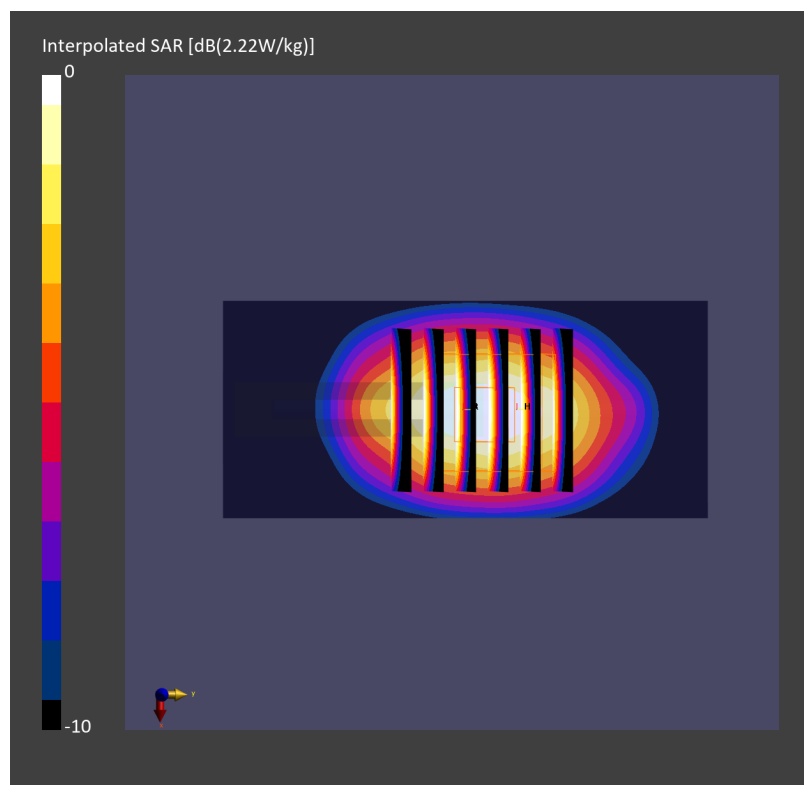

Date: 2025-02-07

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250207 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(8.73, 8.73, 8.73); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.83 W/kg; SAR (10g) = 0.953 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.90 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.4 %

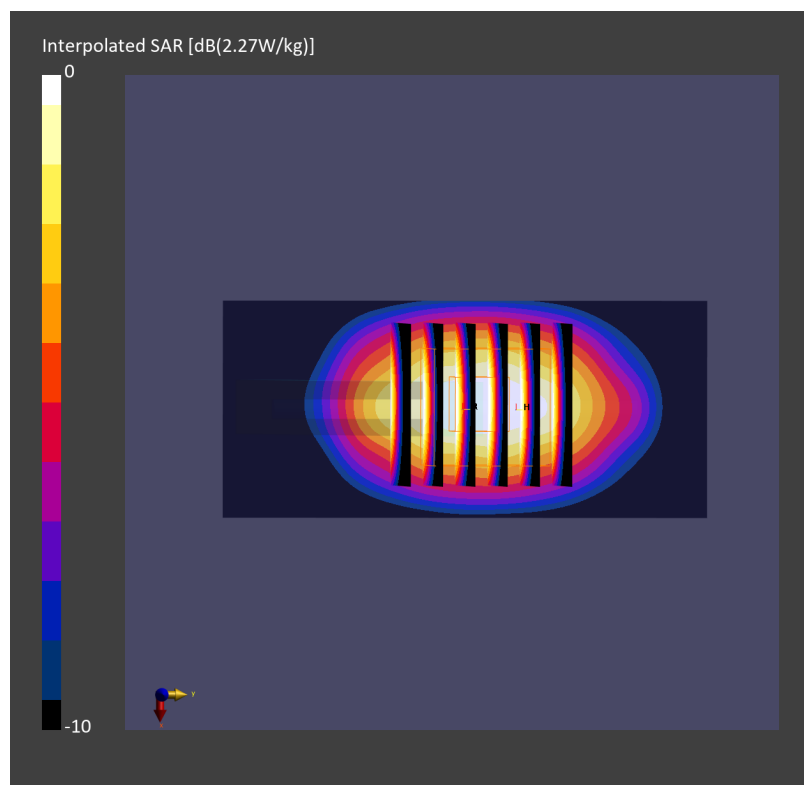

Date: 2025-02-09

System Check_Head_2300MHz**DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250209 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.66$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(8.18, 8.18, 8.18); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.16 W/kg; SAR (10g) = 0.993 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.31 W/kg; SAR (8g) = 1.22 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

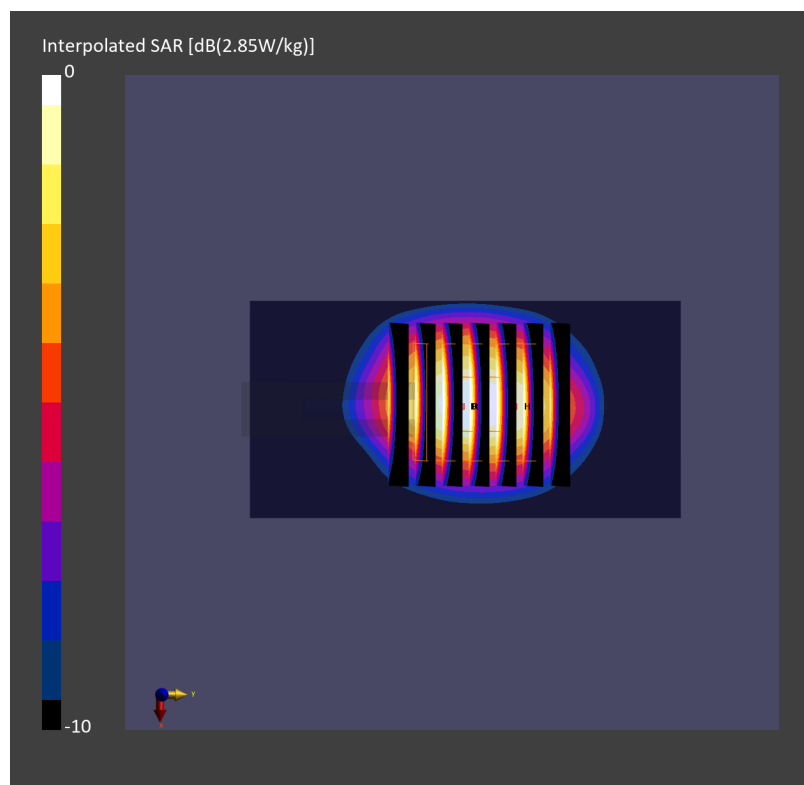

Date: 2025-02-11

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250211 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(7.75, 7.75, 7.75); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.20 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.81 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.9 %

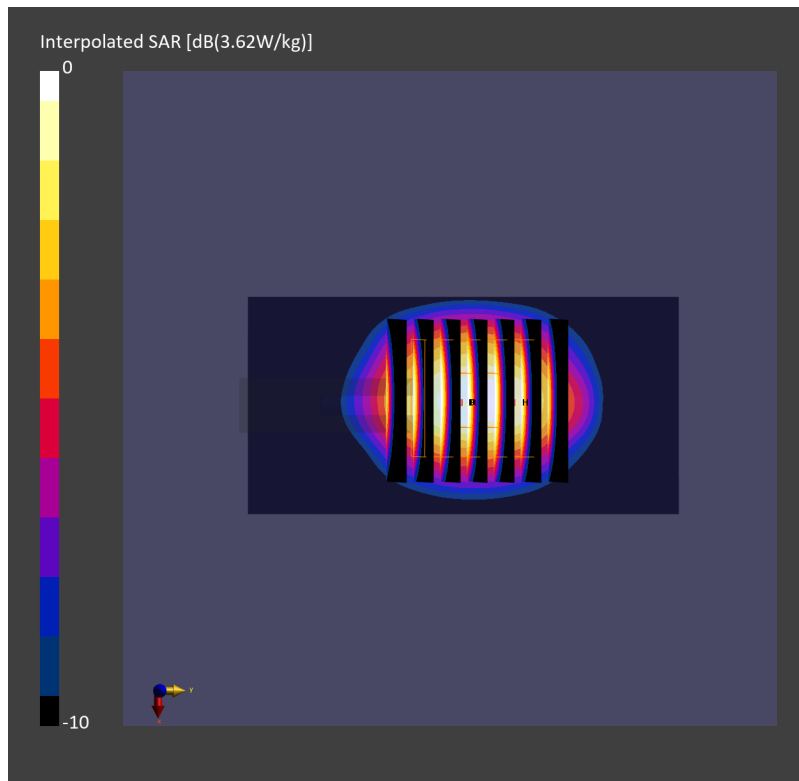

Date: 2025-02-12

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250212 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.02$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(7.75, 7.75, 7.75); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2024-09-16
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-Laptop; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.21 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 2.81 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.8 %

