

System Check_Head_2450MHz

DUT:D2450V2 - SN:1040

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.38, 8.38, 8.38); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2022-11-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.60 W/kg; SAR (10g) = 1.21 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.53 W/kg; SAR (10g) = 1.18 W/kg;

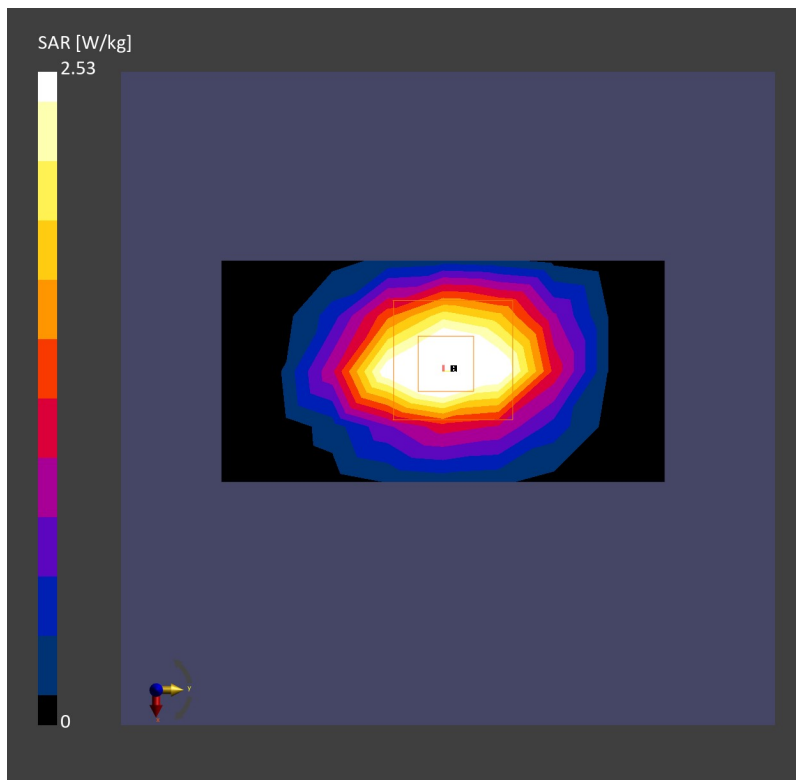

System Check_Head_5250MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.56$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.18, 6.18, 6.18); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2022-11-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 0.987 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.82 W/kg; SAR (10g) = 1.09 W/kg;

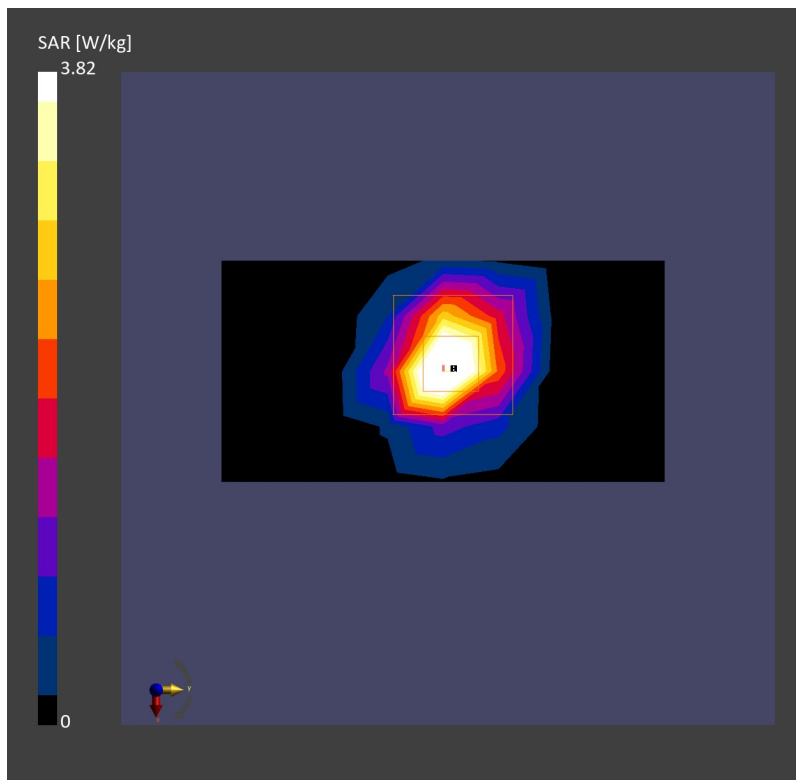

System Check_Head_5750MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.12$ S/m; $\epsilon_r = 34.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.57, 5.57, 5.57); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2022-11-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 0.960 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.81 W/kg; SAR (10g) = 1.09 W/kg;

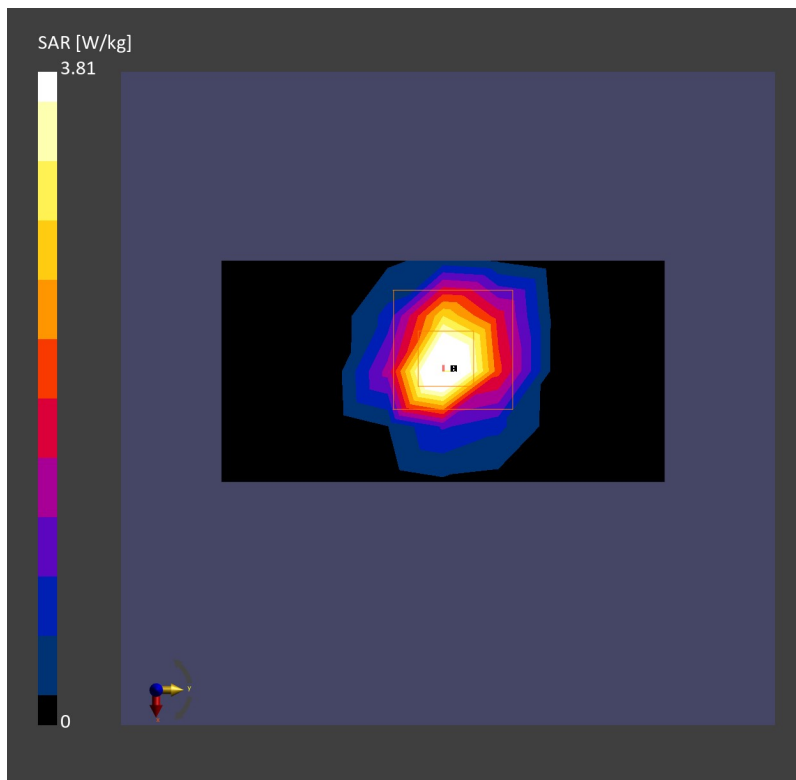

System Check_Right Head_2450MHz

DUT:D2450V2 - SN:1095

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C


DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.38, 8.38, 8.38); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2022-11-24
- Phantom: SAM-HeadStand V10.0; Serial: 1031
- Measurement Software: cDASY6 V6.6.0.13926

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.74 W/kg; SAR (10g) = 1.25 W/kg

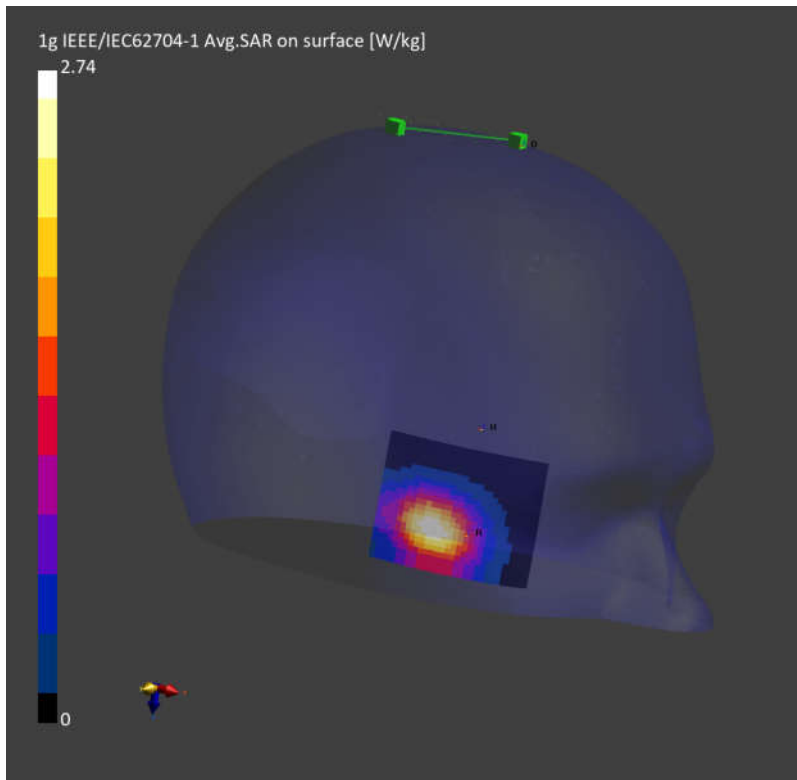

System Check_Right Head_5800MHz

DUT:D5GHzV2 - SN:1365

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.31$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C


DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.57, 5.57, 5.57); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2022-11-24
- Phantom: SAM-HeadStand V10.0; Serial: 1031
- Measurement Software: cDASY6 V6.6.0.13926

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 0.909 W/kg; SAR (10g) = 0.324 W/kg

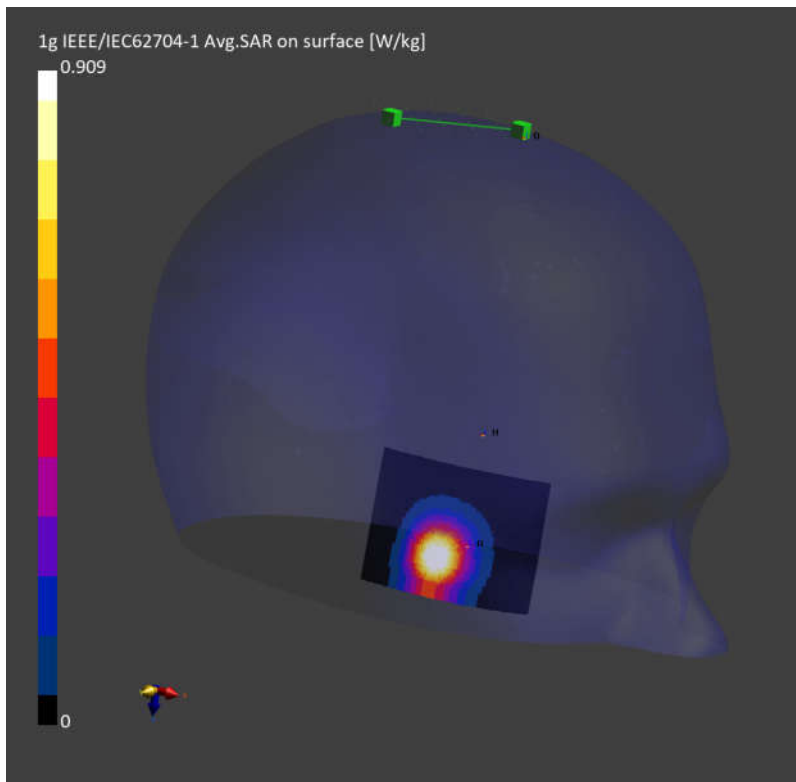

System Check_Left Head_2450MHz

DUT:D2450V2 - SN:1095

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C


DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.38, 8.38, 8.38); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2022-11-24
- Phantom: SAM-HeadStand V10.0; Serial: 1031
- Measurement Software: cDASY6 V6.6.0.13926

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.64 W/kg; SAR (10g) = 1.20 W/kg

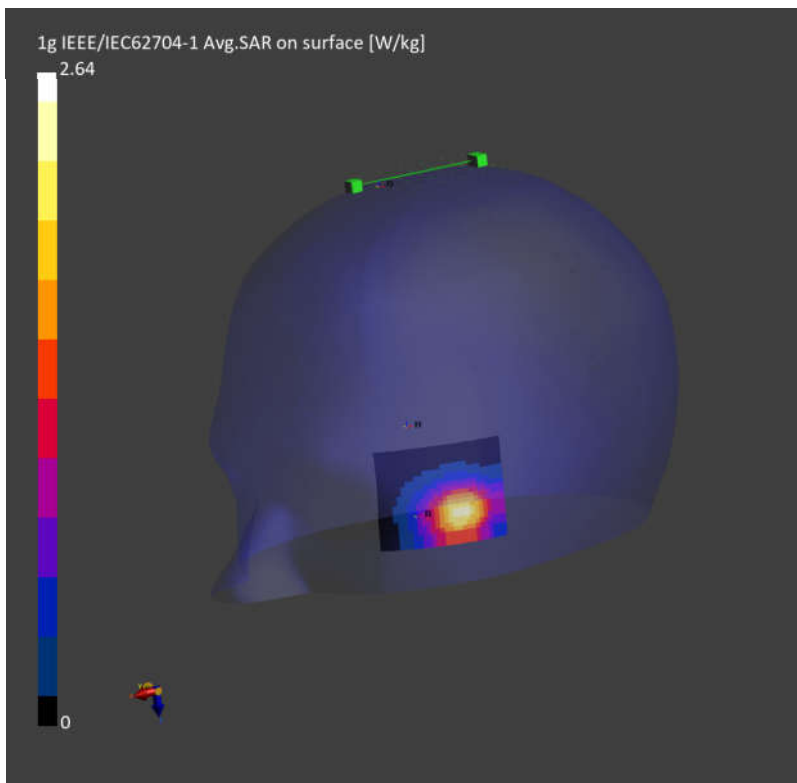

System Check_Left Head_5800MHz

DUT:D5GHzV2 - SN:1365

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.31$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.57, 5.57, 5.57); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2022-11-24
- Phantom: SAM-HeadStand V10.0; Serial: 1031
- Measurement Software: cDASY6 V6.6.0.13926

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 0.933 W/kg; SAR (10g) = 0.325 W/kg

