Appendix A: Test result of conducted Test

Conducted Average Output Power

Result Table

Mode	Channel	Meas.Level [dBm]	Av.Power [dBm]	Verdict
11B	LCH	14.71	14.71	PASS
11B	MCH	14.11	14.11	PASS
11B	HCH	14.59	14.59	PASS
11G	LCH	12.44	12.44	PASS
11G	MCH	14.3	14.3	PASS
11G	HCH	14.2	14.2	PASS
11N20SISO	LCH	12.56	12.56	PASS
11N20SISO	MCH	12.2	12.2	PASS
11N20SISO	HCH	12.05	12.05	PASS

Test Graph

Graphs			
11B/LCH			
11B/MCH			

11B/HCH			
11G/LCH			
11G/MCH			

11G/HCH			
11N20SISO/LCH			
11N20SISO/MCH		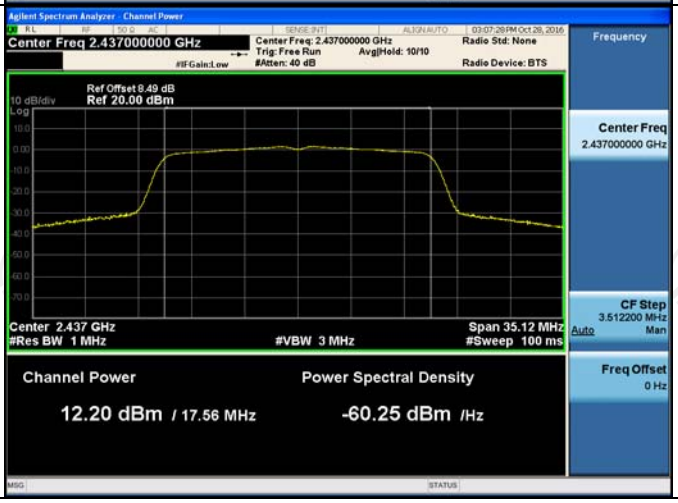	

11N20SISO/HCH			

6dB Occupied Bandwidth

Result Table

Mode	Channel	6dB Bandwidth [MHz]	99% OBW [MHz]	Verdict
11B	LCH	9.071	12.549	PASS
11B	MCH	9.061	12.515	PASS
11B	HCH	10.01	12.494	PASS
11G	LCH	15.34	16.396	PASS
11G	MCH	15.13	16.398	PASS
11G	HCH	15.86	16.422	PASS
11N20SISO	LCH	13.80	17.558	PASS
11N20SISO	MCH	15.13	17.561	PASS
11N20SISO	HCH	15.08	17.564	PASS

Test Graph

Graphs			
11B/LCH			
11B/MCH			

11B/HCH			
11G/LCH			
11G/MCH		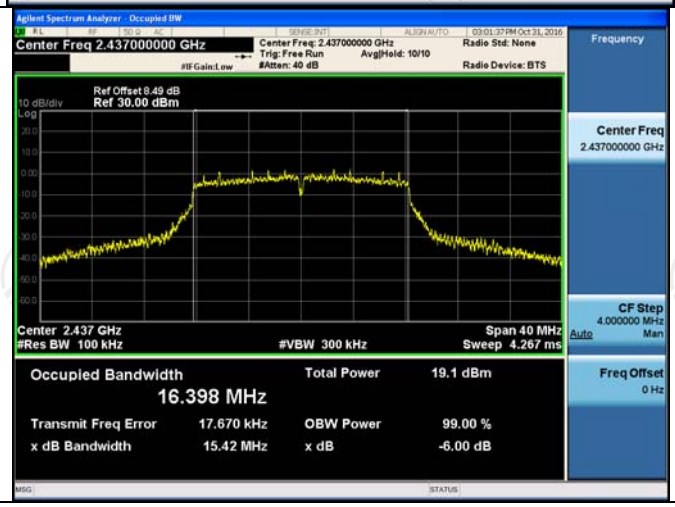	

11G/HCH			
11N20SISO/LCH			
11N20SISO/MCH			

11N20SISO/HCH		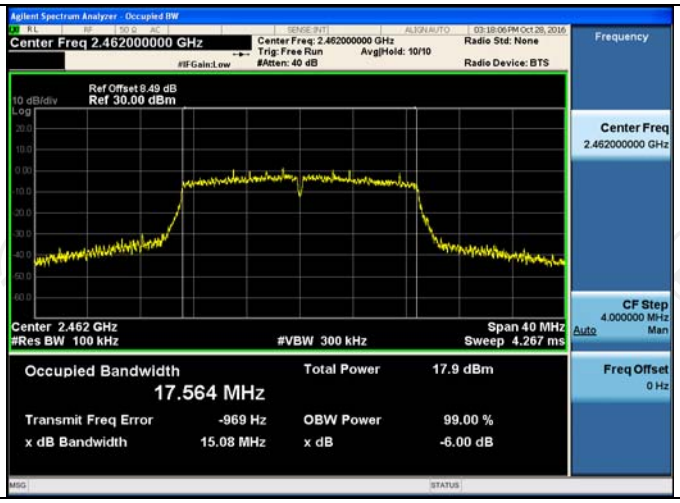	

Band-edge for RF Conducted Emissions

Result Table

Mode	Channel	Carrier Power [dBm]	Max.Spurious Level [dBm]	Limit [dBm]	Verdict
11B	LCH	5.919	-41.376	-24.08	PASS
11B	HCH	5.309	-40.623	-24.69	PASS
11G	LCH	2.256	-41.405	-27.74	PASS
11G	HCH	3.169	-40.393	-26.83	PASS
11N20SISO	LCH	1.850	-41.235	-28.15	PASS
11N20SISO	HCH	1.812	-40.141	-28.19	PASS

Test Graph

Graphs		
11B/LCH		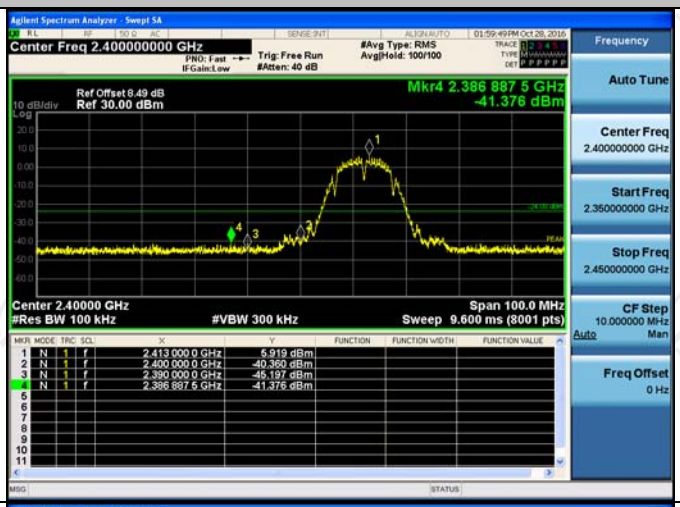
11B/HCH		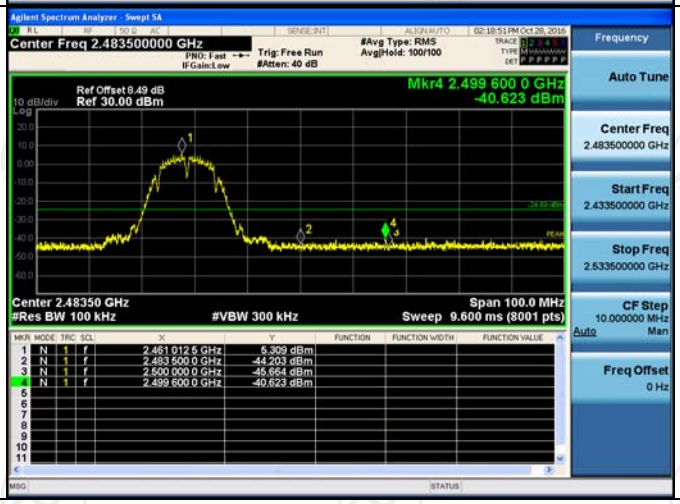

11G/LCH		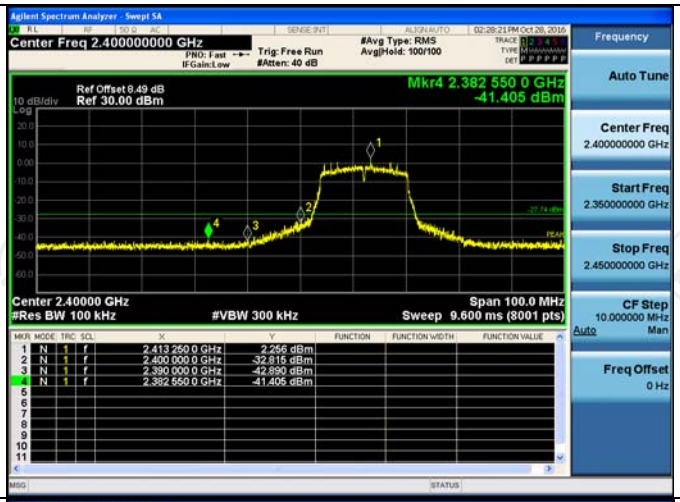	
11G/HCH		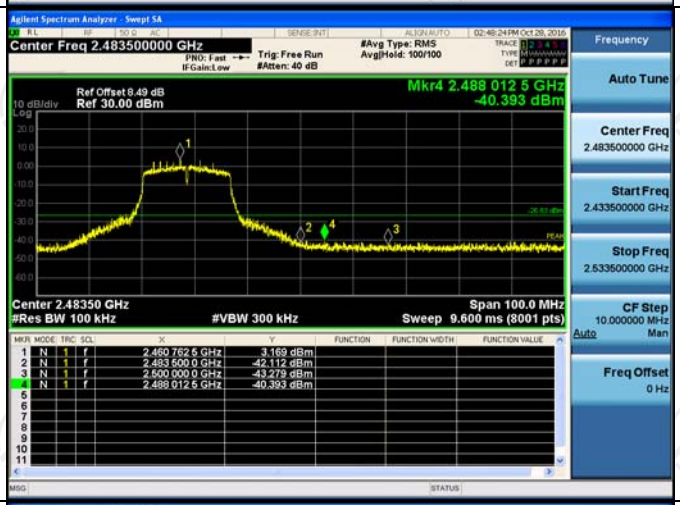	
11N20SISO/LCH		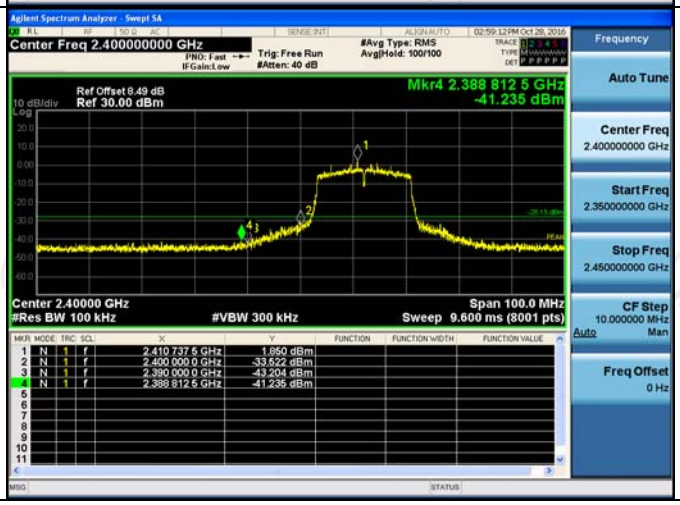	

11N20SISO/HCH		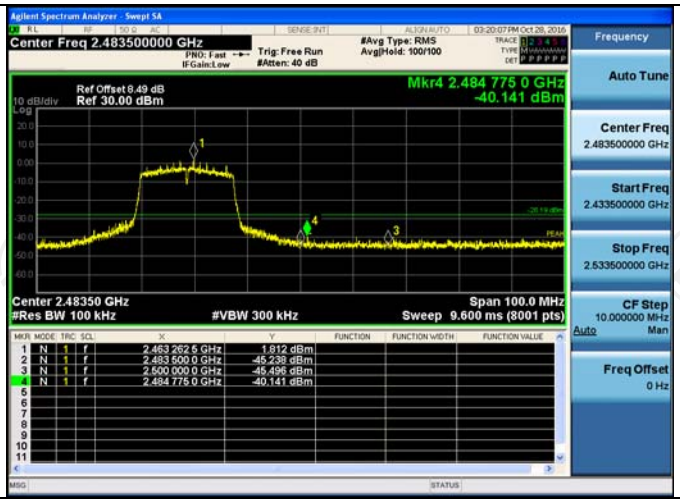	

RF Conducted Spurious Emissions

Result Table

Mode	Channel	Pref [dBm]	Puw [dBm]	Verdict
11B	LCH	5.394	<Limit	PASS
11B	MCH	4.455	<Limit	PASS
11B	HCH	5.383	<Limit	PASS
11G	LCH	1.89	<Limit	PASS
11G	MCH	4.242	<Limit	PASS
11G	HCH	3.981	<Limit	PASS
11N20SISO	LCH	1.834	<Limit	PASS
11N20SISO	MCH	2.132	<Limit	PASS
11N20SISO	HCH	1.298	<Limit	PASS

Test Graph

11B_LCH_Graphs			
Pref/11B/LCH			
Puw/11B/LCH		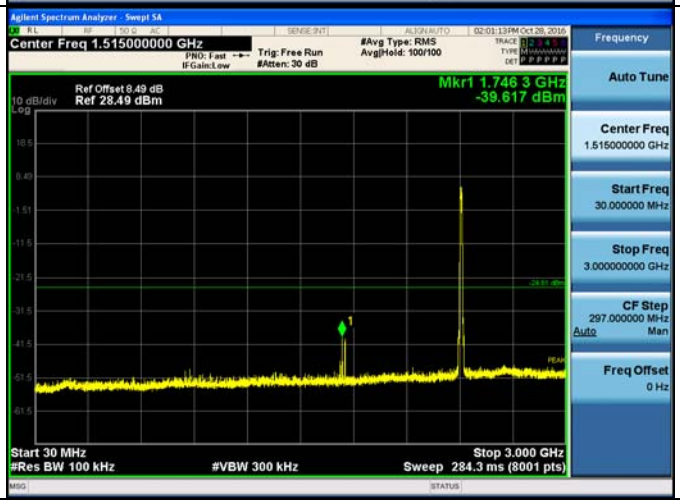	

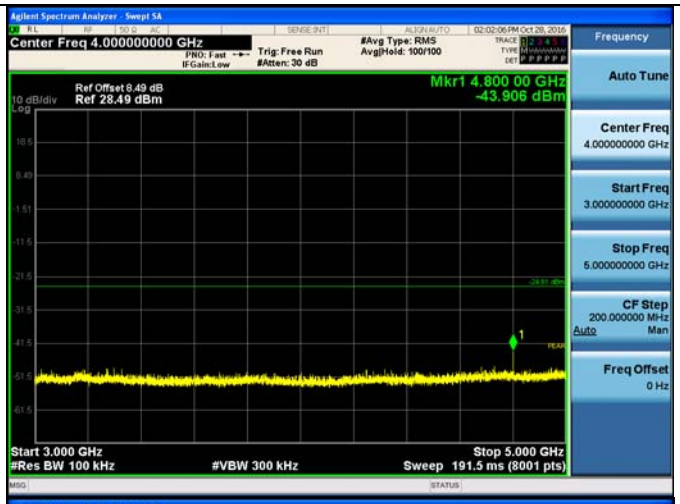
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 4.800 00 GHz
-43.906 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz

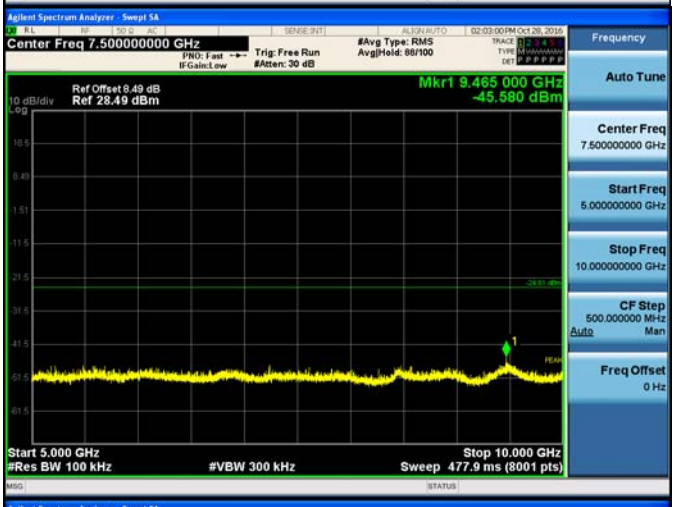
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 9.465 000 GHz
-45.580 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 14.567 500 GHz
-44.912 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		

11B_MCH_Graphs		
Pref/11B/MCH		
Puw/11B/MCH		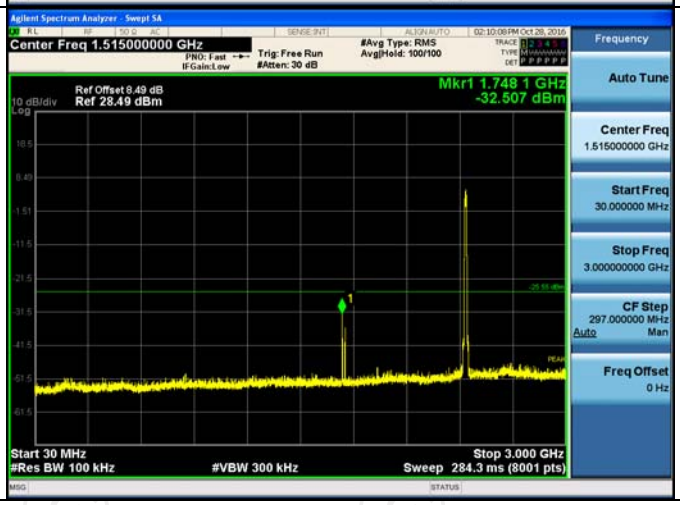

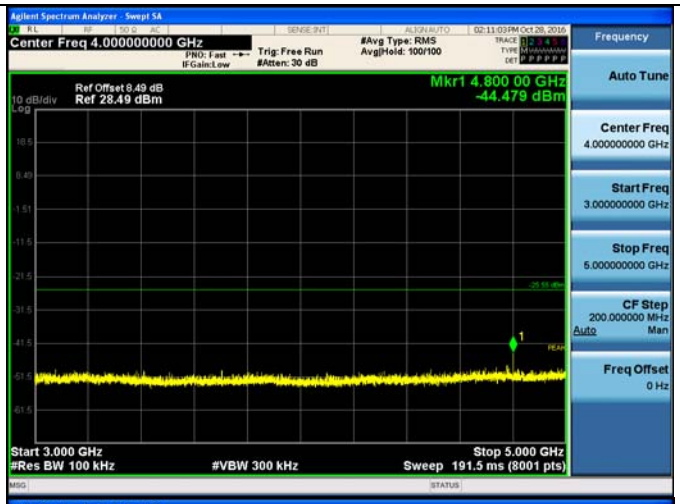
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 4.800 00 GHz
-44.479 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz

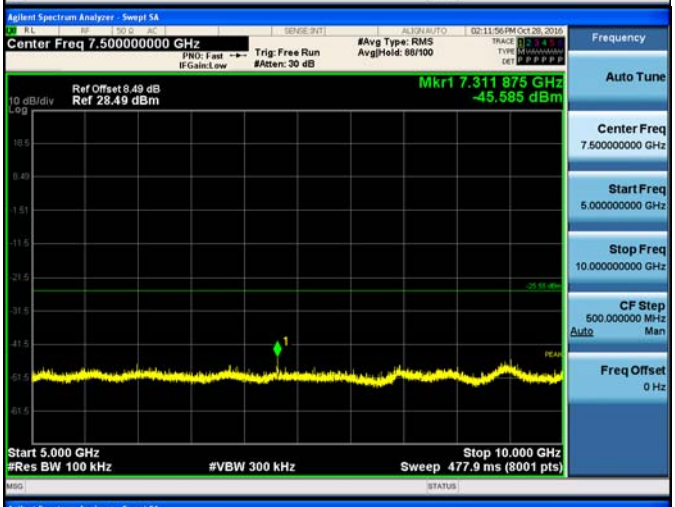
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 7.311 875 GHz
-45.585 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 13.538 750 GHz
-45.257 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		

11B_HCH_Graphs		
Pref/11B/HCH		
Puw/11B/HCH		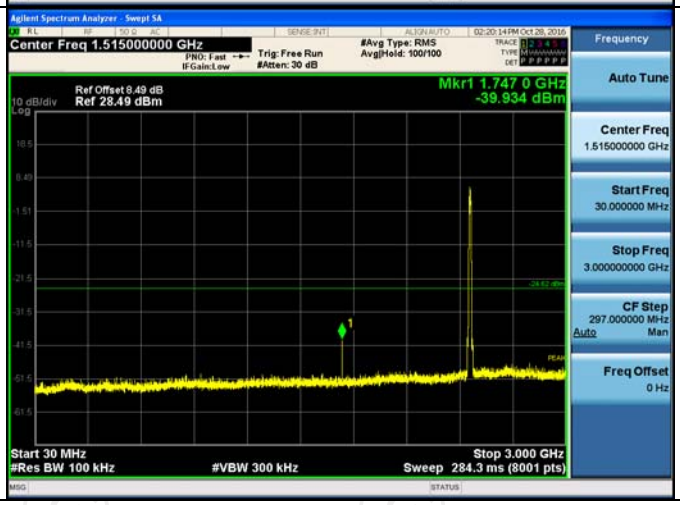

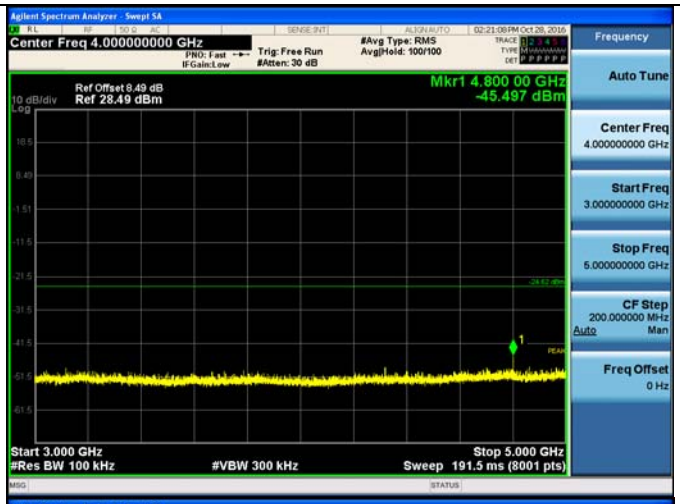
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
02:21:08 PM Oct 28, 2016
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Log
Mkr1 4.800 00 GHz
-45.497 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
MSG
STATUS

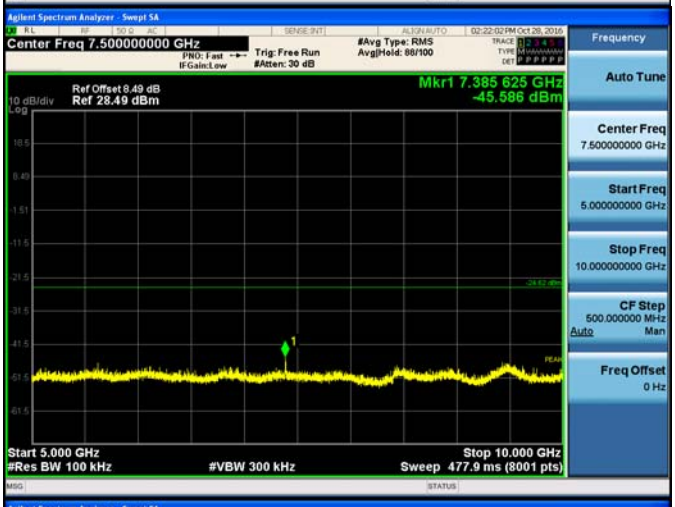
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
02:22:02 PM Oct 28, 2016
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Log
Mkr1 7.385 625 GHz
-45.586 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
02:23:26 PM Oct 28, 2016
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Log
Mkr1 14.546 250 GHz
-45.386 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS

		

11G_LCH_Graphs		
Pref/11G/LCH		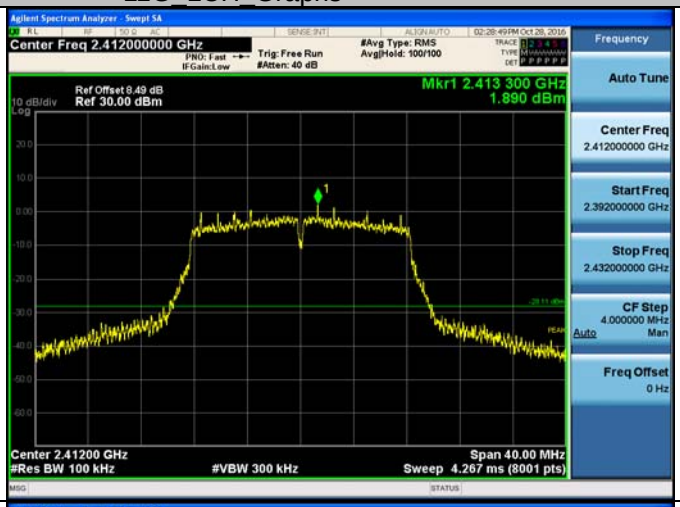
Puw/11G/LCH		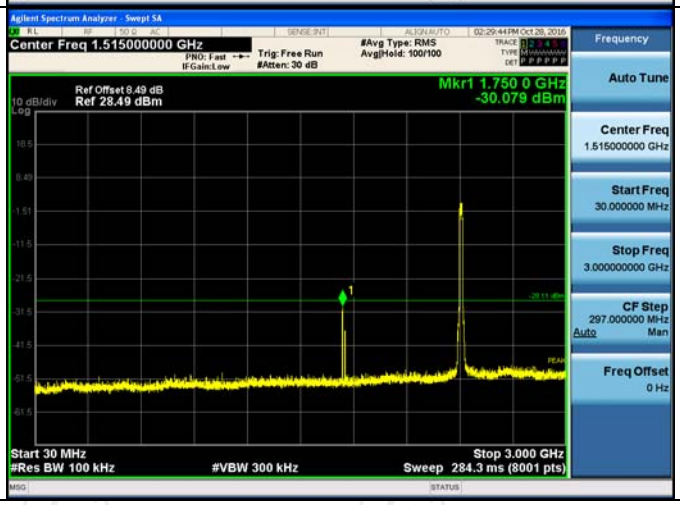

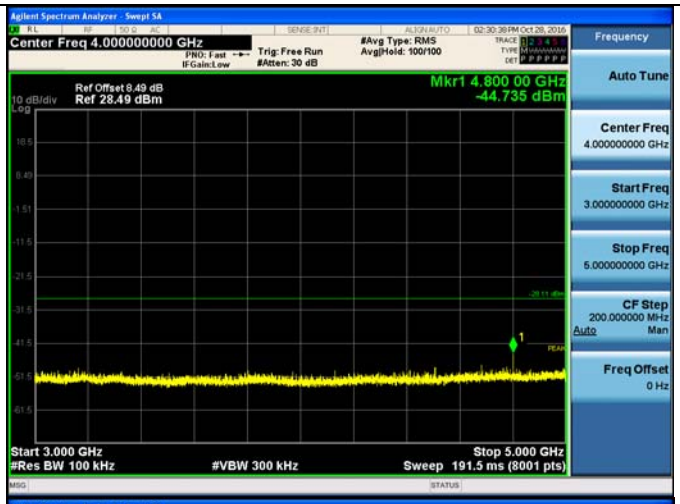
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 4.800 00 GHz
-44.735 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 89/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 9.480 625 GHz
-47.050 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 14.523 750 GHz
-44.997 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		

11G_MCH_Graphs		
Pref/11G/MCH		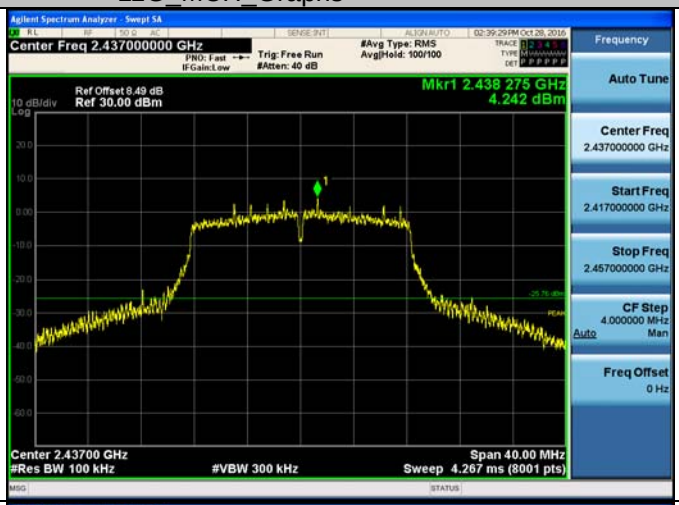
Puw/11G/MCH		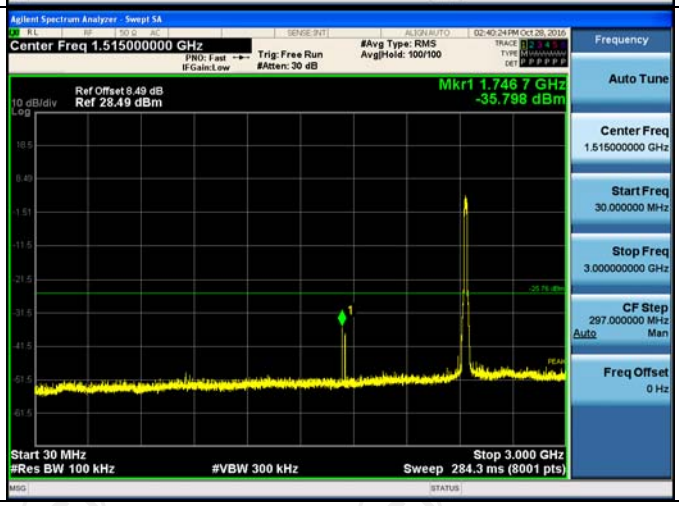

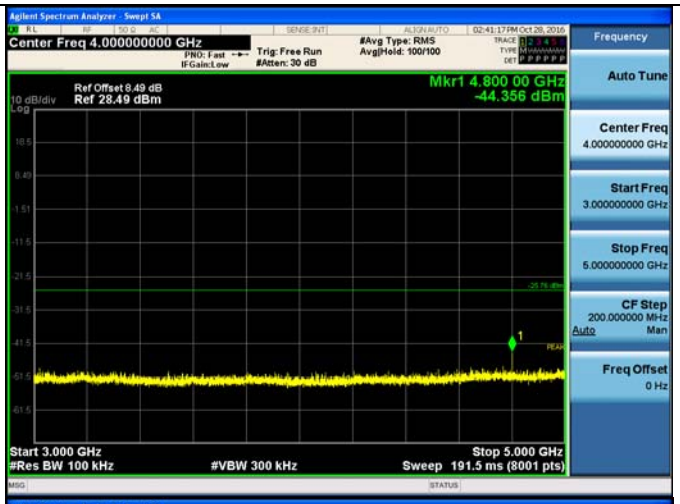
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
02:41:17 PM Oct 28, 2016
Frequency
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Log
Mkr1 4.800 00 GHz
-44.356 dBm
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
MSG
STATUS


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
02:42:12 PM Oct 28, 2016
Frequency
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Log
Mkr1 9.496 250 GHz
-46.967 dBm
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
02:43:36 PM Oct 28, 2016
Frequency
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Log
Mkr1 14.570 625 GHz
-46.001 dBm
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS

		

11G_HCH_Graphs		
Pref/11G/HCH		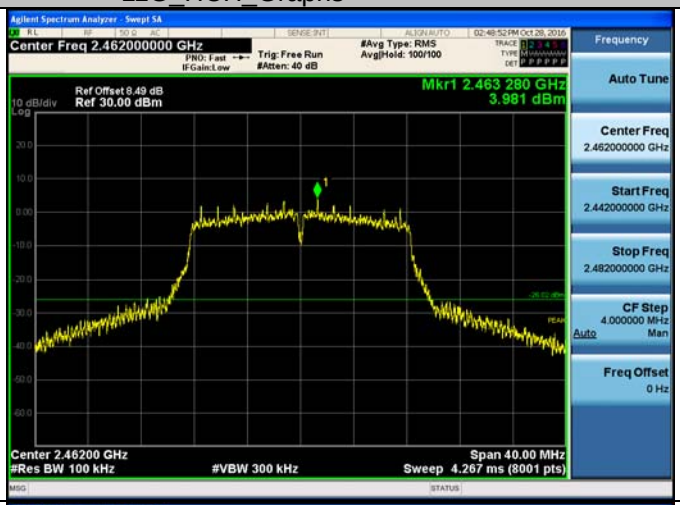
Puw/11G/HCH		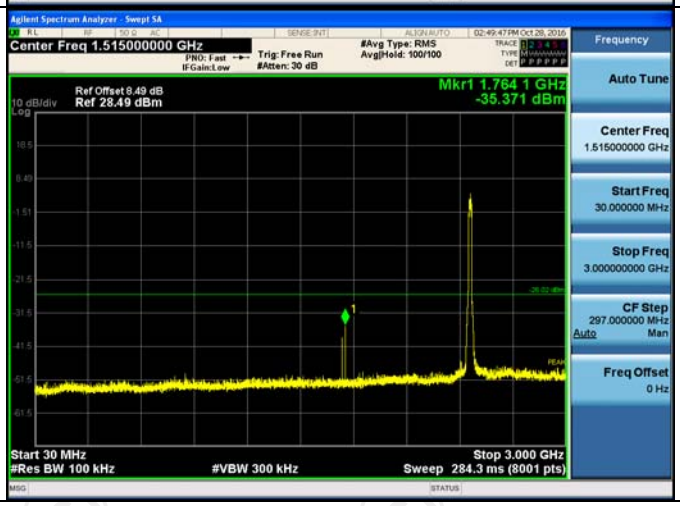

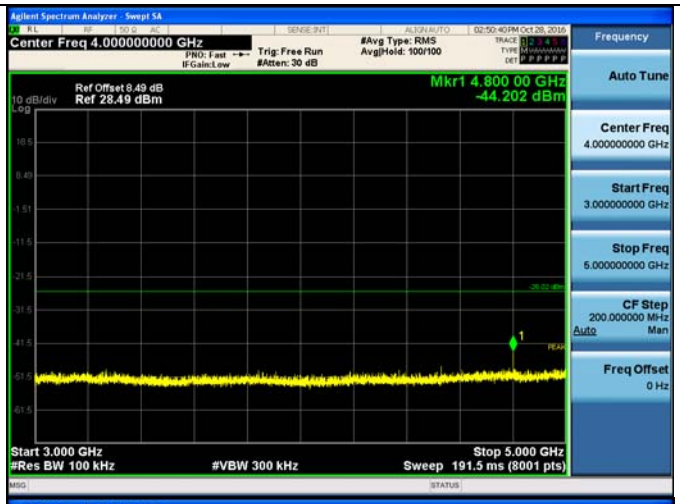
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 4.800 00 GHz
-44.202 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)

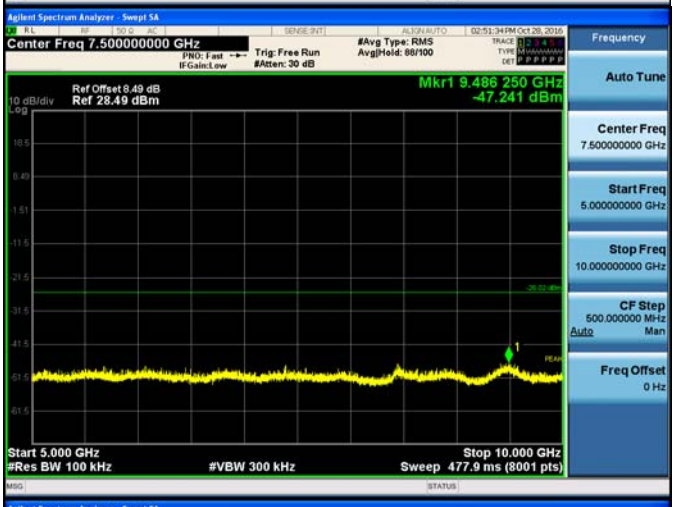
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 9.486 250 GHz
-47.241 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 14.564 375 GHz
-44.597 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		

11N20SISO_LCH_Graphs		
Pref/11N20SISO/LCH		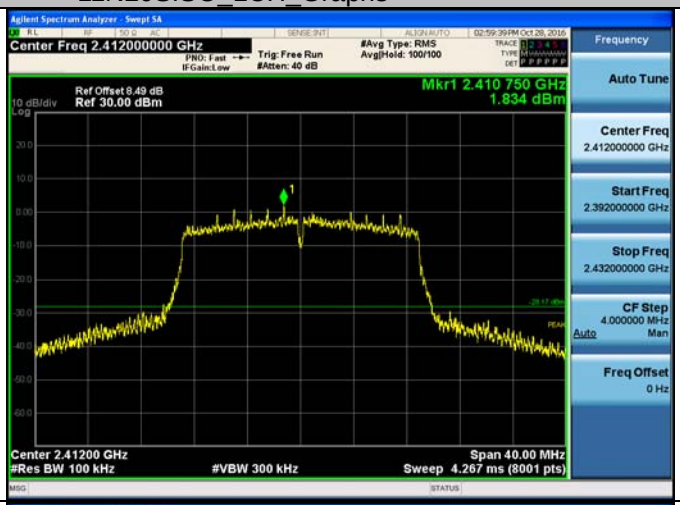
/11N20SISO/LCH		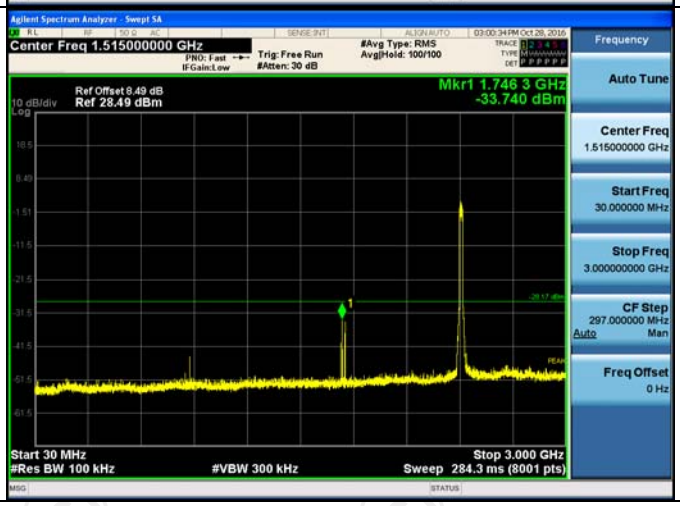

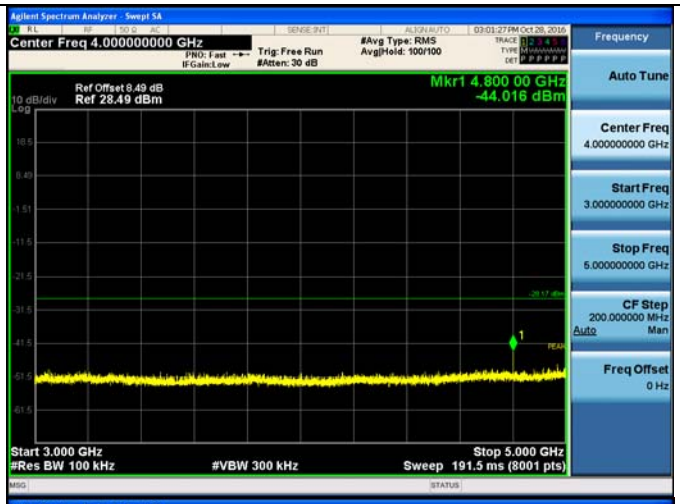
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 4.800 00 GHz
-44.016 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz

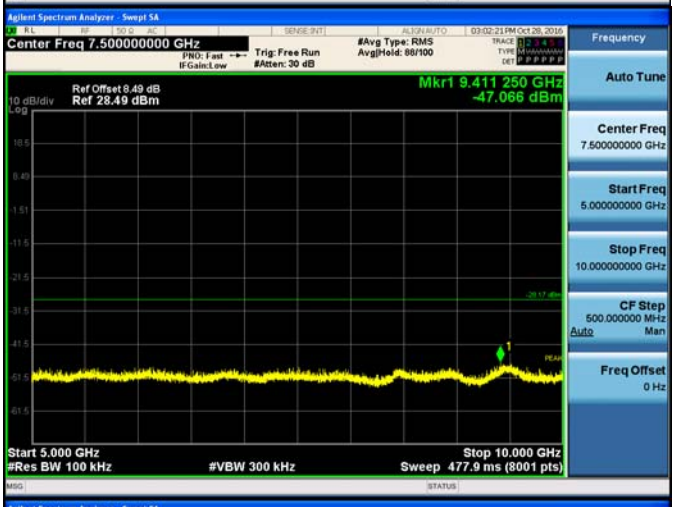
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 9.411 250 GHz
-47.066 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 14.571 875 GHz
-44.256 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		

11N20SISO_MCH_Graphs		
Pref/11N20SISO/MCH		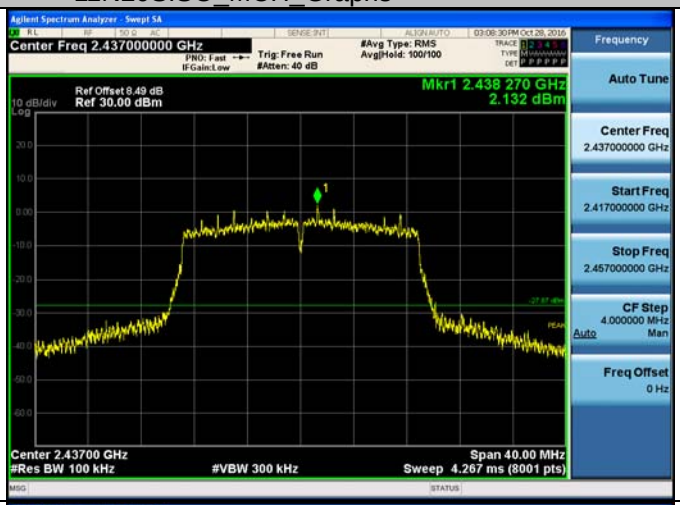
Puw/11N20SISO/MCH		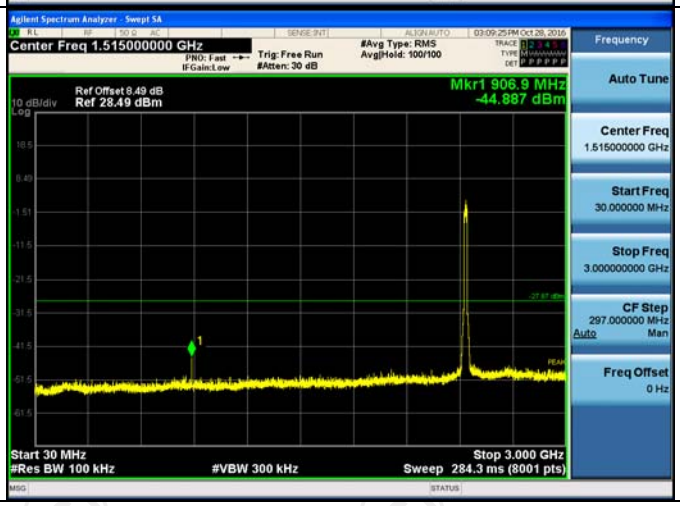

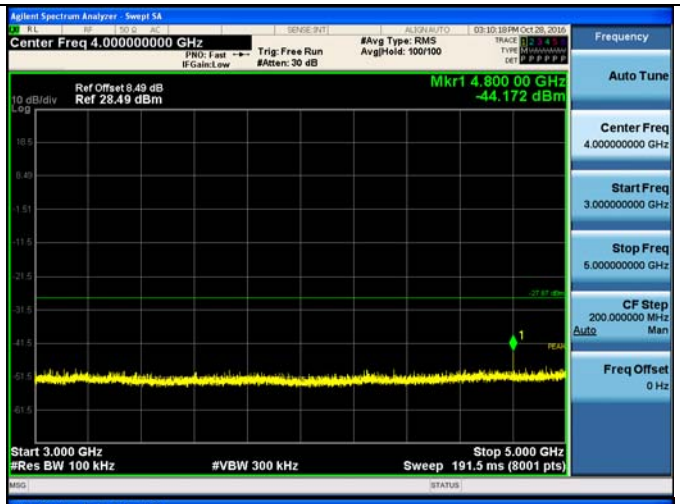
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 4.800 00 GHz
-44.172 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 9.513 125 GHz
-46.597 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 14.584 375 GHz
-45.476 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		

11N20SISO_HCH_Graphs		
Pref/11N20SISO/HCH		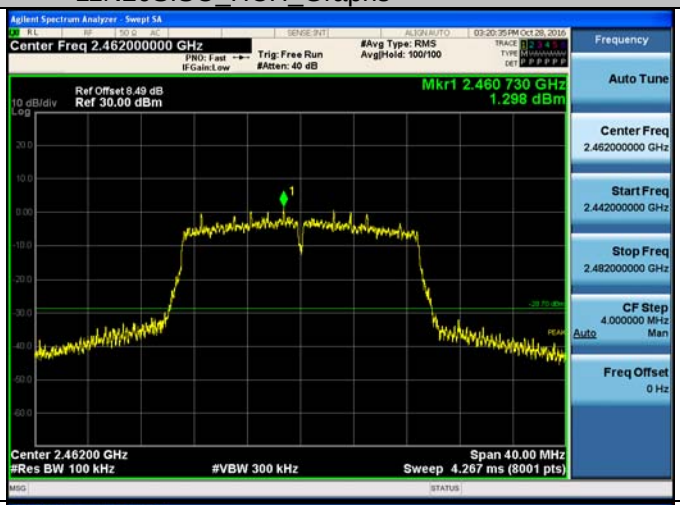
Puw/11N20SISO/HCH		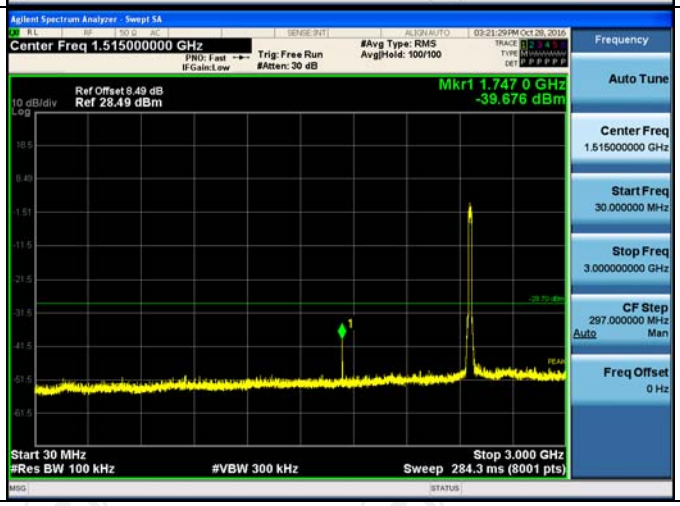

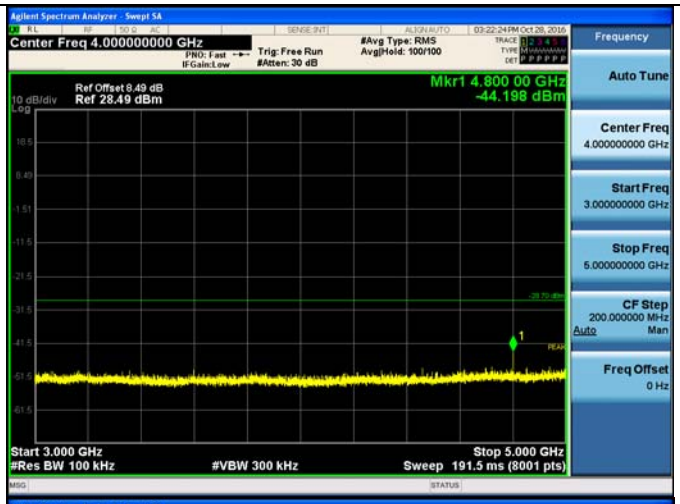
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 4.800 00 GHz
-44.198 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)

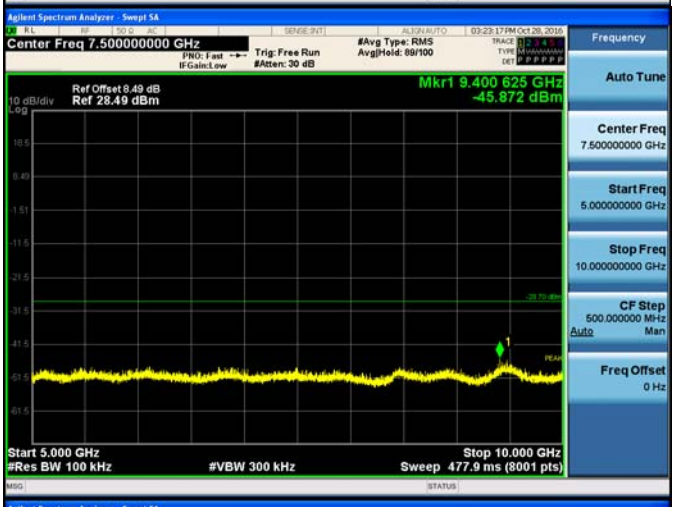
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 89/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 9.400 625 GHz
-45.872 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 8.49 dB
10 dB/div
Ref 28.49 dBm
Mkr1 14.545 000 GHz
-44.261 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

	

Agilent Spectrum Analyzer - Swept SA
Center Freq 20.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 32 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 8.49 dB
10 dB/div
Ref 30.00 dBm
Log
Mkr1 24.646 25 GHz
-37.240 dBm
Start 15.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.000 GHz
Sweep 955.7 ms (8001 pts)
Frequency
Auto Tune
Center Freq
20.000000000 GHz
Start Freq
15.000000000 GHz
Stop Freq
25.000000000 GHz
CF Step
1.000000000 GHz
Auto
Man
Freq Offset
0 Hz

Power Spectral Density

Result Table

Mode	Channel	Meas.Level [dBm]	Av.PSD [dBm]	Verdict
11B	LCH	-11.834	-11.816	PASS
11B	MCH	-10.967	-10.949	PASS
11B	HCH	-10.623	-10.605	PASS
11G	LCH	-16.470	-16.345	PASS
11G	MCH	-13.915	-13.790	PASS
11G	HCH	-14.971	-14.846	PASS
11N20SISO	LCH	-16.046	-15.904	PASS
11N20SISO	MCH	-17.509	-17.375	PASS
11N20SISO	HCH	-17.474	-17.340	PASS

Test Graph

Graphs			
11B/LCH		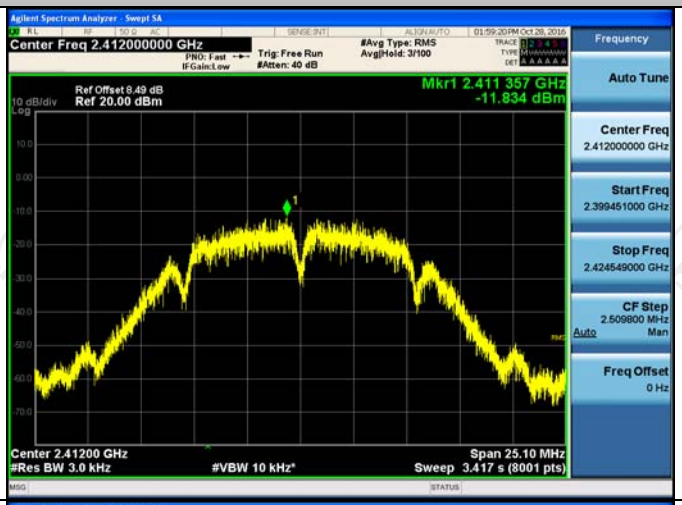	
11B/MCH		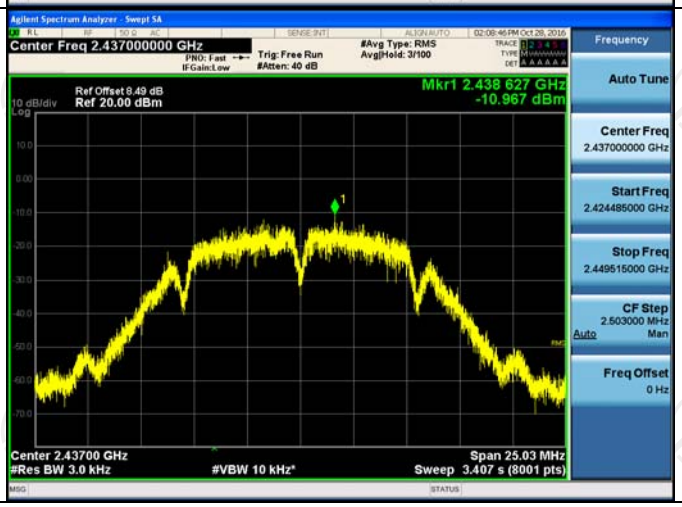	

11B/HCH		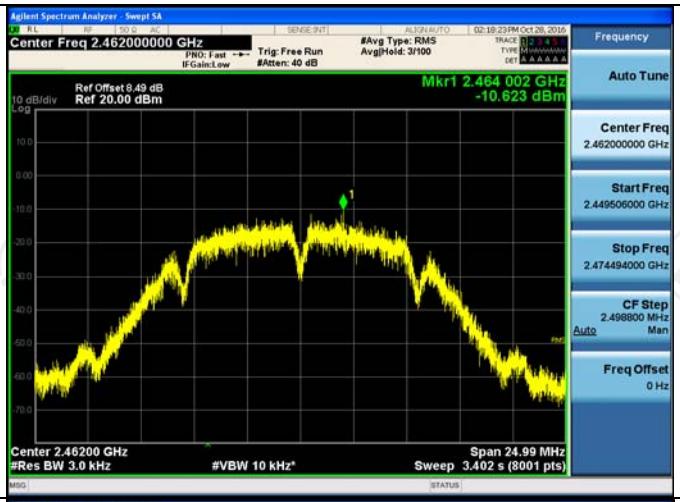	
11G/LCH		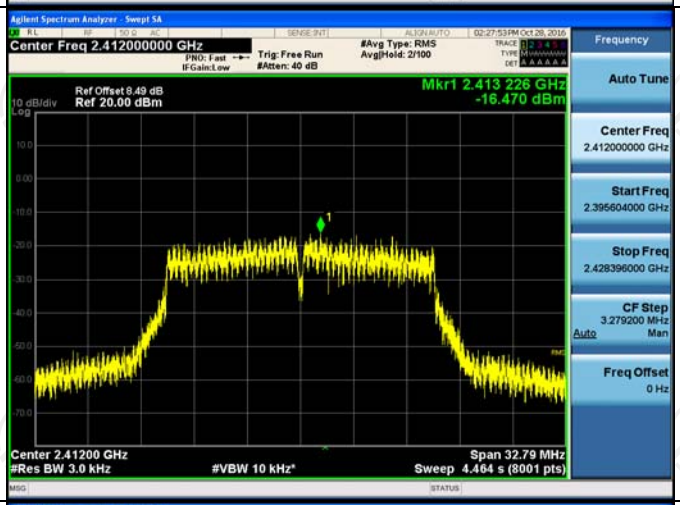	
11G/MCH		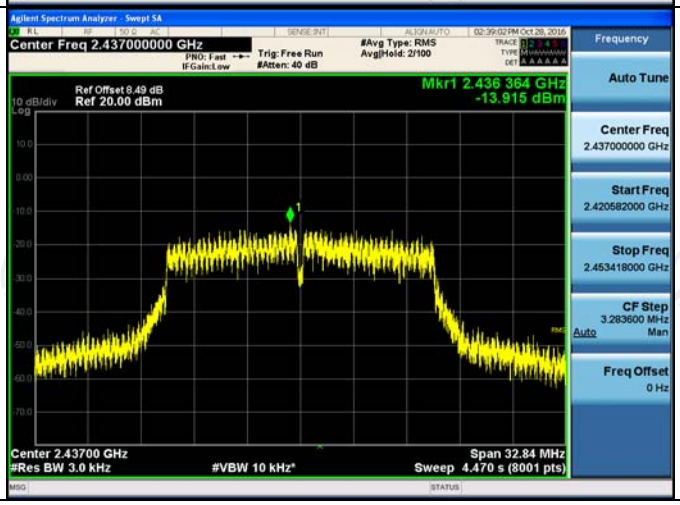	

11G/HCH		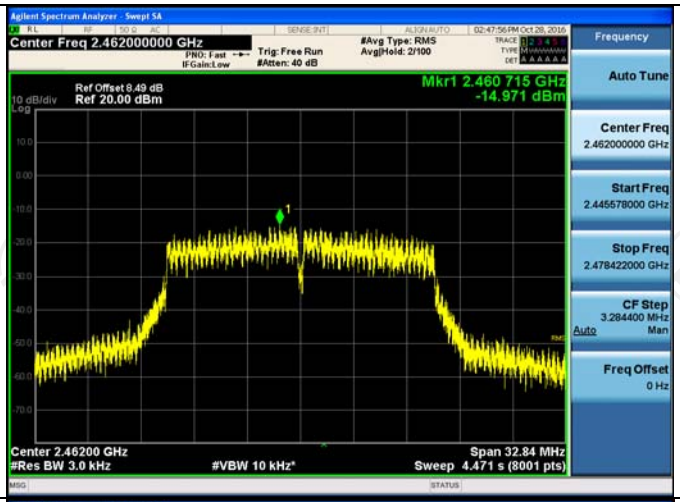	
11N20SISO/LCH		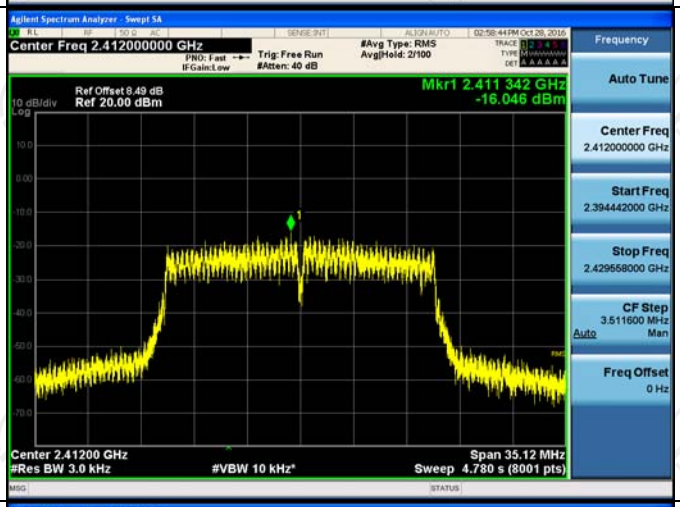	
11N20SISO/MCH		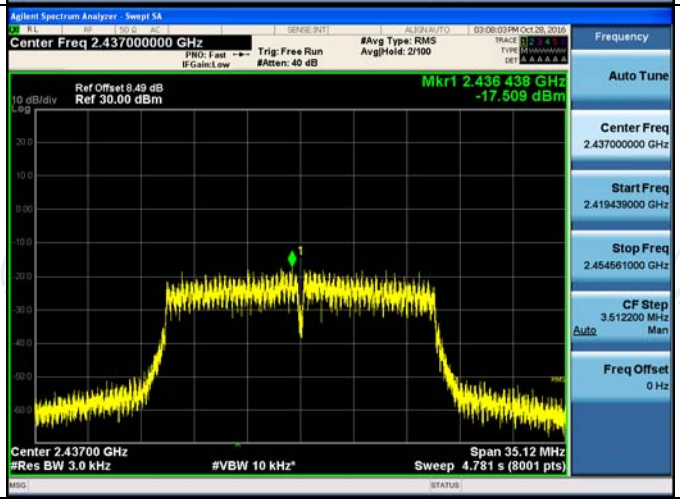	

11N20SISO/HCH