


FCC ID Label

The FCC ID and will be placed on the equipment as shown in the photograph below.

19.7*37mm

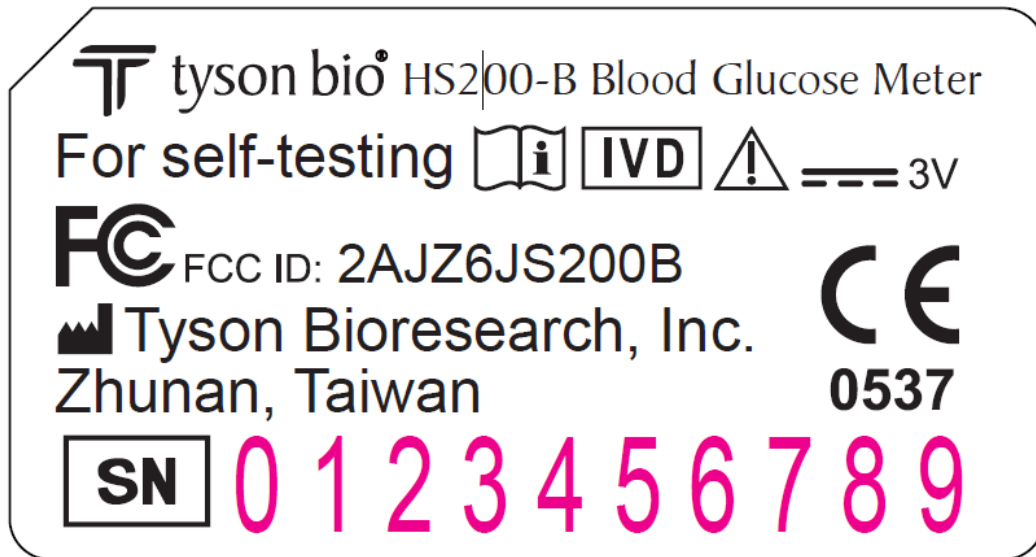


19.7*37mm




FCC ID Label

19.7*37mm

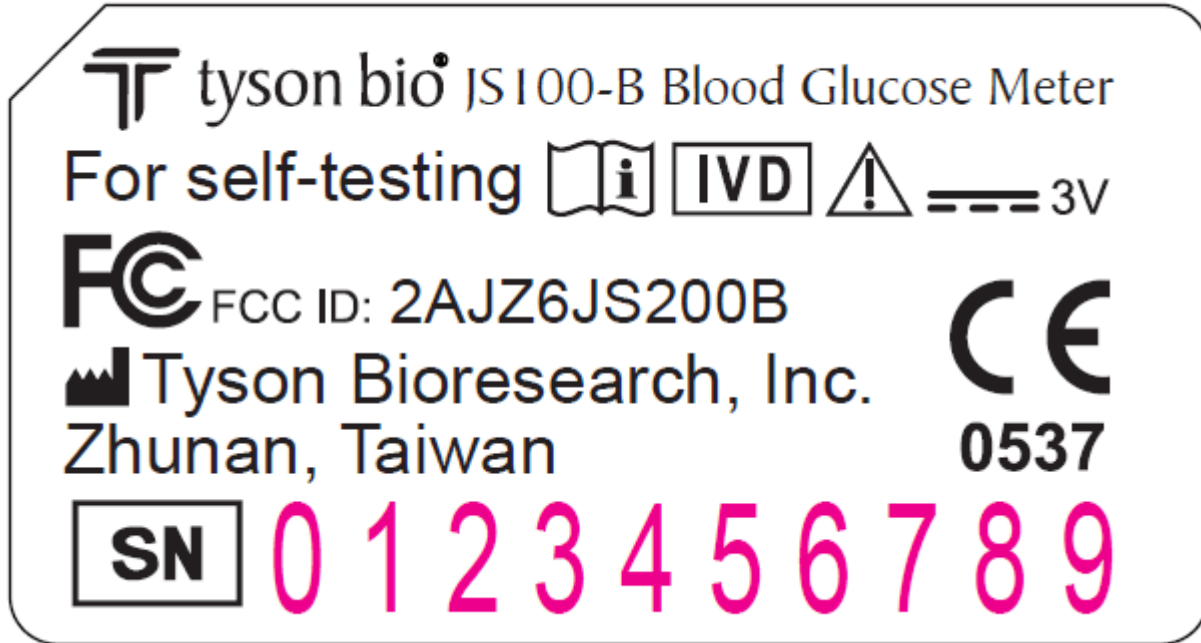

19.7*37mm

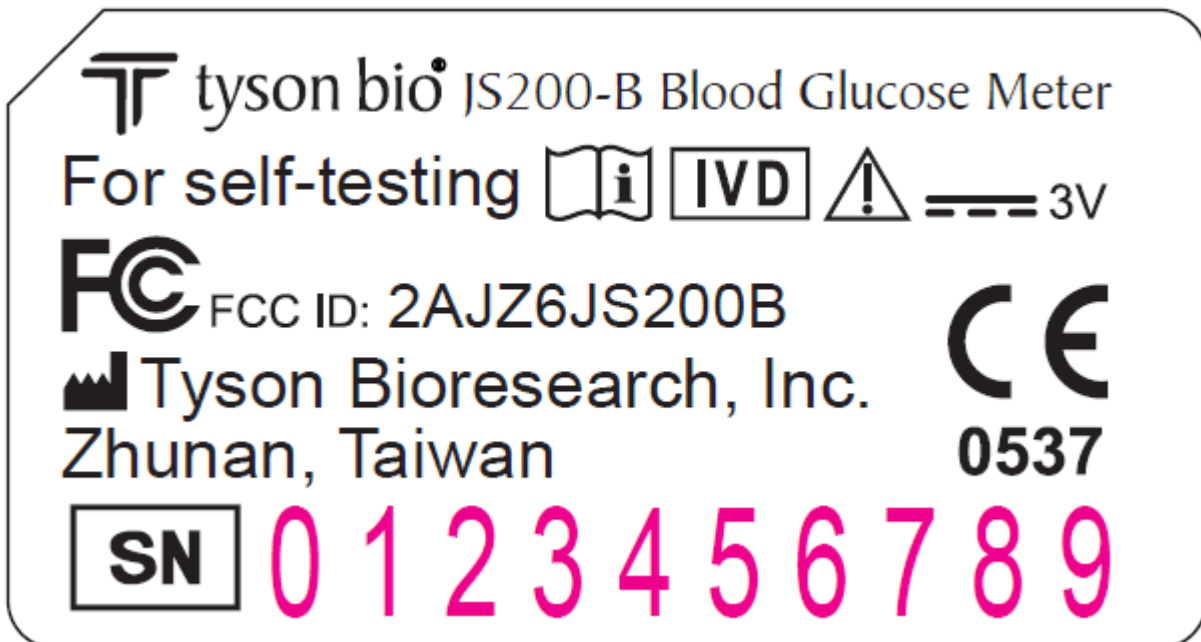

FCC ID Label

rossmax HS200
 Blood Glucose Meter For self-testing

 Tyson Bioresearch, Inc. Zhunan, Taiwan

 Medical Device Safety Service GmbH

Schiffgraben 41, D-30175 Hannover,
 Germany

mg/dL

IVD

CE
0537
3V

FCC FCC ID: 2AJZ6JS200B

SN YYMPXXXXXXXXXX

RL5HS20000000000XX

rossmax JS200
 Blood Glucose Meter For self-testing

 Tyson Bioresearch, Inc. Zhunan, Taiwan

 Medical Device Safety Service GmbH

Schiffgraben 41, D-30175 Hannover,
 Germany

mg/dL

IVD

CE
0537
3V

FCC FCC ID: 2AJZ6JS200B

SN : YYMPXXXXXXXXXX

RL5JS2000000000010