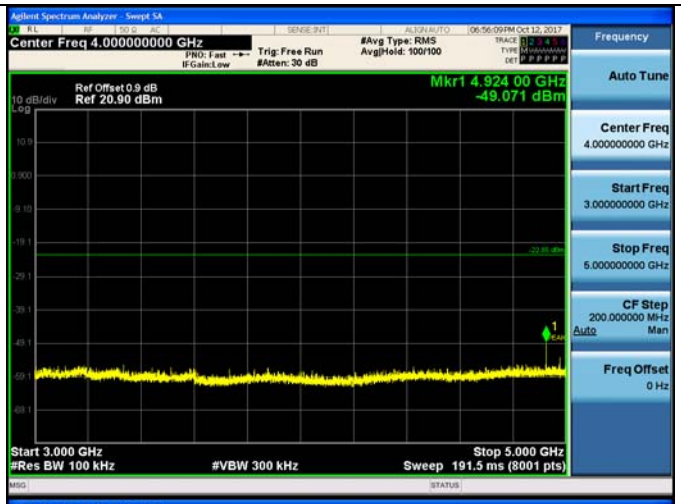
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 4.924 00 GHz
-49.071 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz

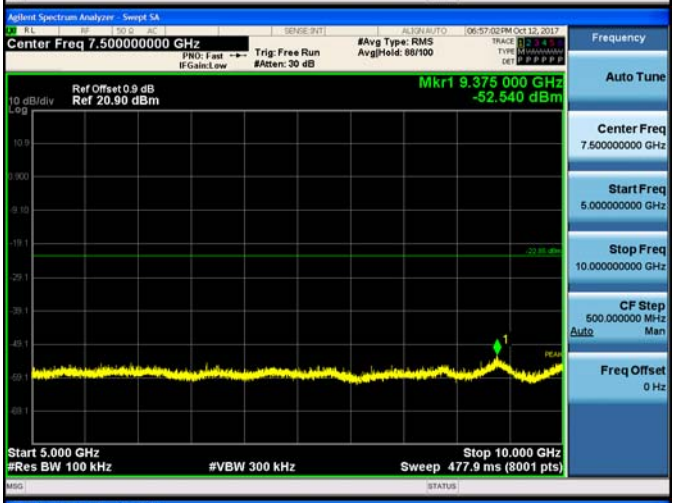
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 9.375 000 GHz
-52.540 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 14.946 875 GHz
-49.963 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		

11G_LCH_Graphs		
Pref/11G/LCH		
Puw/11G/LCH		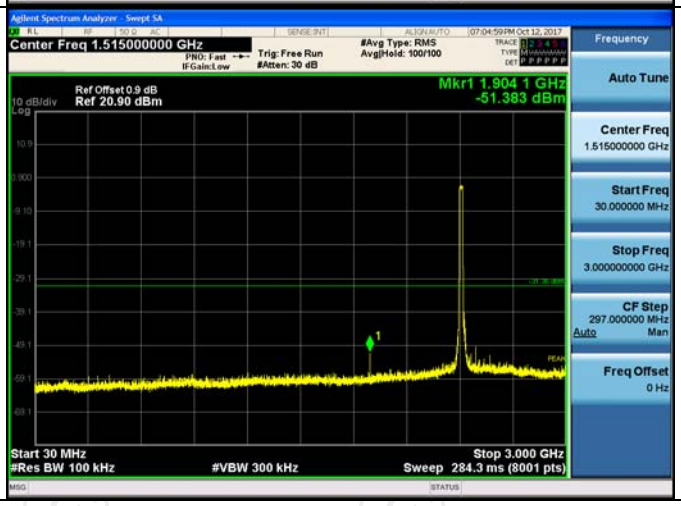


Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 4.986 25 GHz
-54.409 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 9.373 125 GHz
-53.183 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 14.982 500 GHz
-50.878 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		

11G_MCH_Graphs		
Pref/11G/MCH		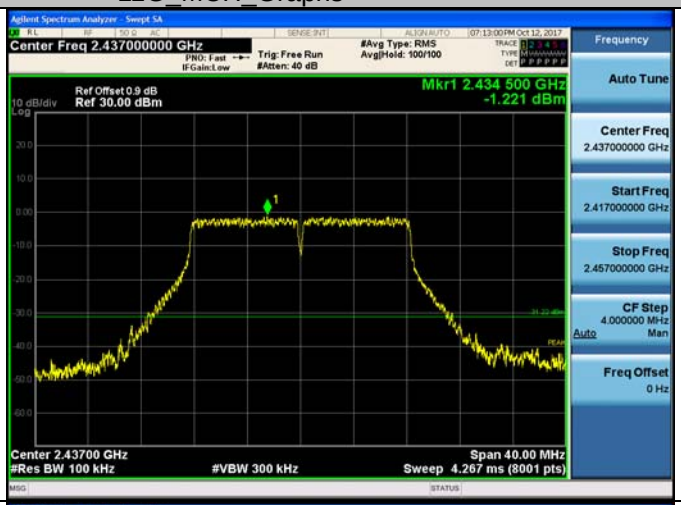
Puw/11G/MCH		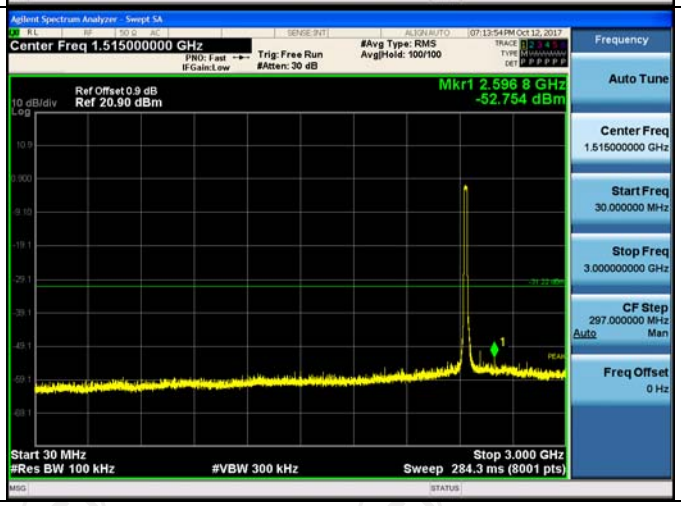

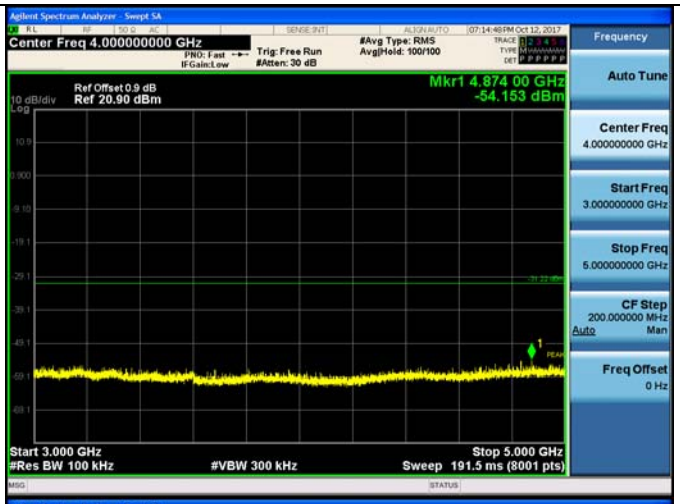
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
07:14:48 PM Oct 12, 2017
Frequency
Mkr1 4.874 00 GHz
-54.153 dBm
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
MSG
STATUS

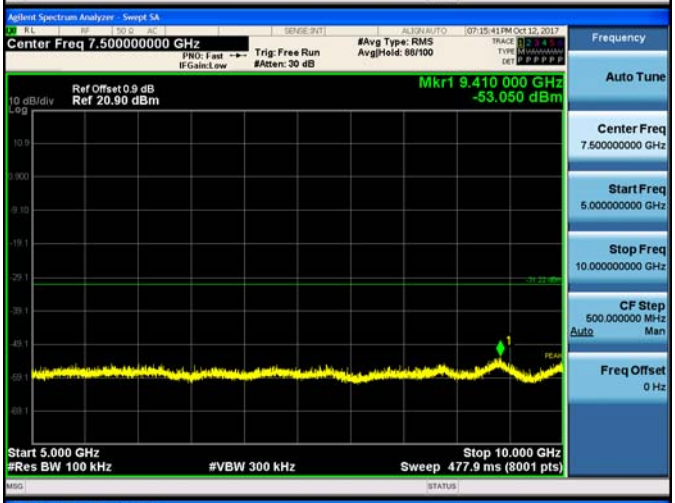
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
07:15:41 PM Oct 12, 2017
Frequency
Mkr1 9.410 000 GHz
-53.050 dBm
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
07:17:05 PM Oct 12, 2017
Frequency
Mkr1 14.992 500 GHz
-51.000 dBm
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS

		

11G_HCH_Graphs		
Pref/11G/HCH		
Puw/11G/HCH		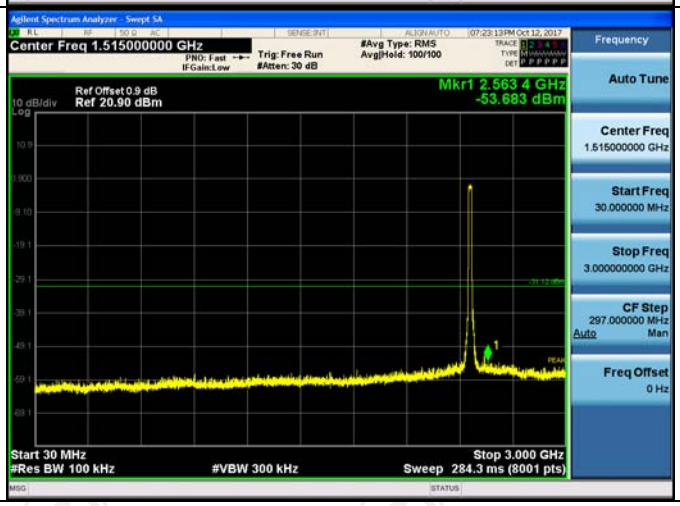


Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 4.915 00 GHz
-55.023 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 89/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 9.405 625 GHz
-53.017 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 14.989 375 GHz
-51.155 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		

11N20SISO_LCH_Graphs		
Pref/11N20SISO/LCH		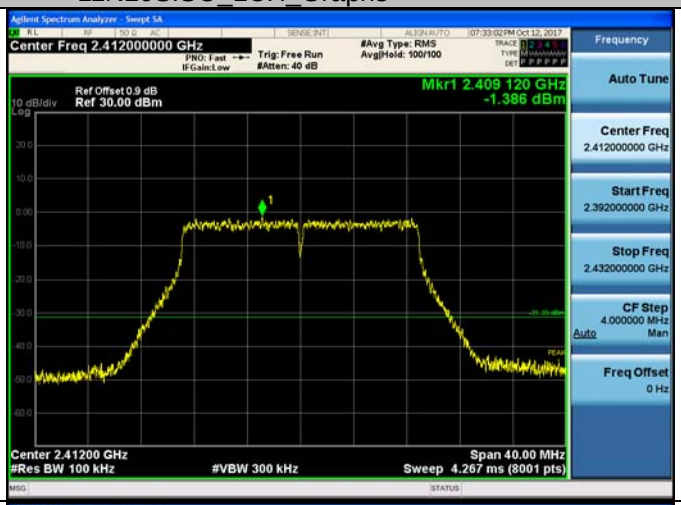
/11N20SISO/LCH		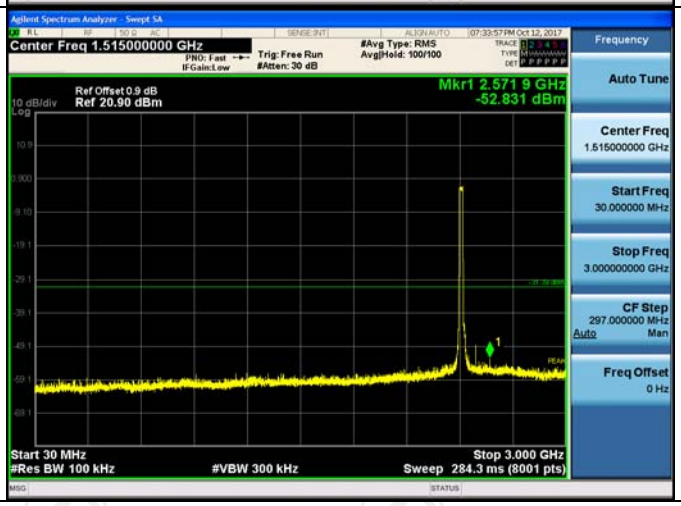

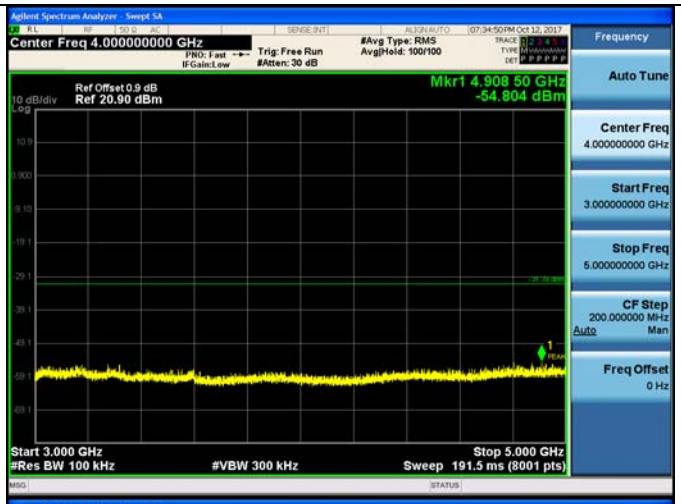
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 4.908 50 GHz
-54.804 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 7.234 375 GHz
-53.169 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 14.980 000 GHz
-51.032 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		

11N20SISO_MCH_Graphs		
Pref/11N20SISO/MCH		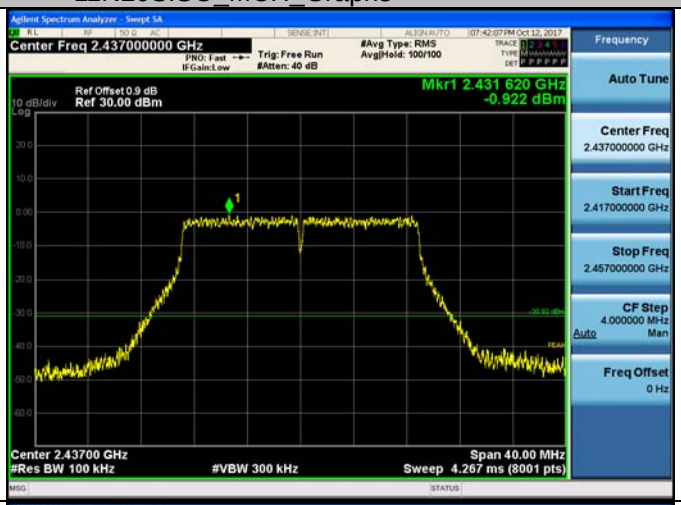
Puw/11N20SISO/MCH		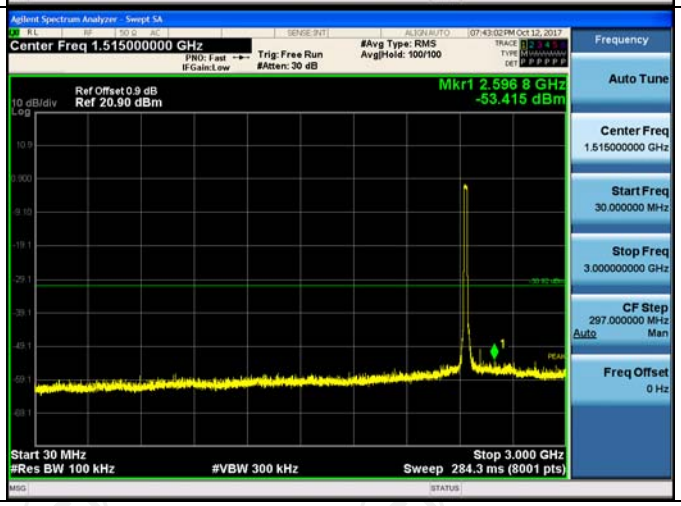

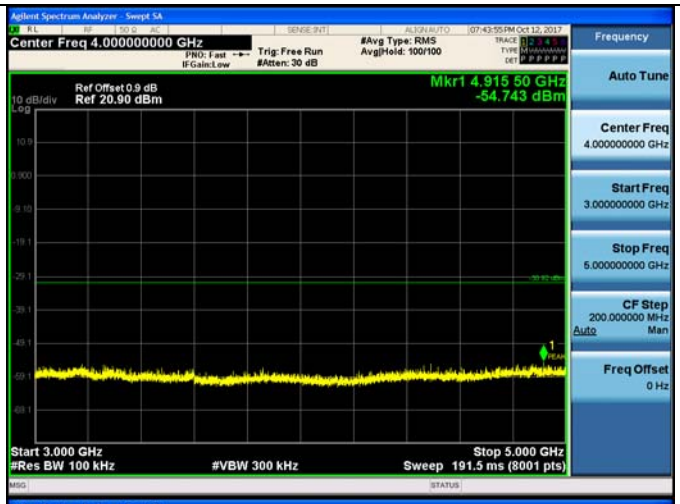
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 4.915 50 GHz
-54.743 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 9.381 875 GHz
-53.009 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 14.980 625 GHz
-50.993 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		

11N20SISO_HCH_Graphs		
Pref/11N20SISO/HCH		
Puw/11N20SISO/HCH		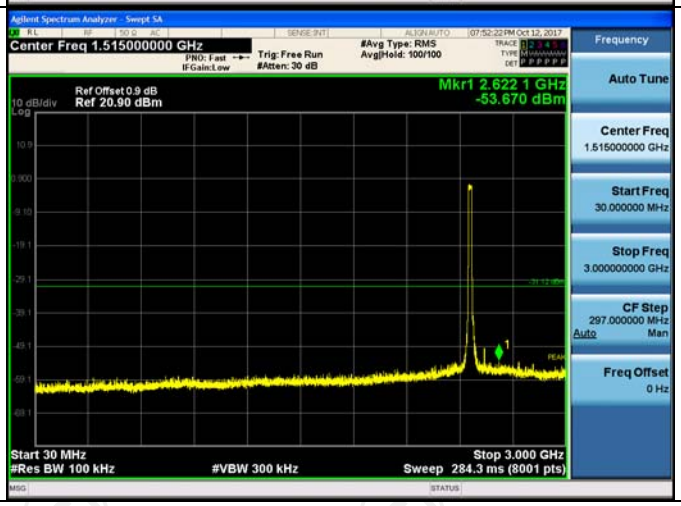

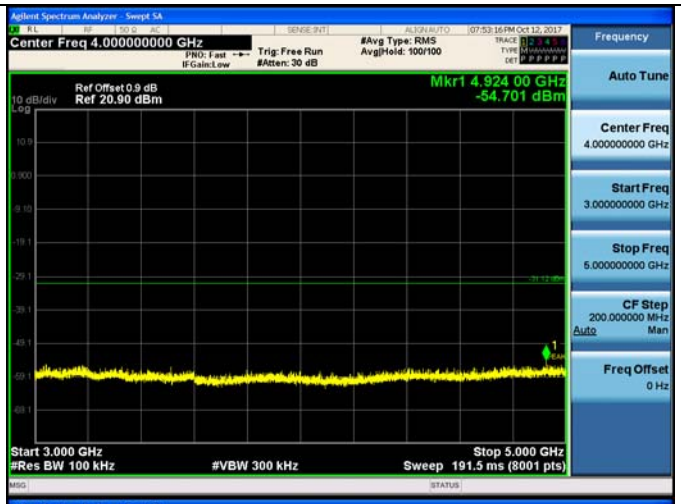
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 4.924 00 GHz
-54.701 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)

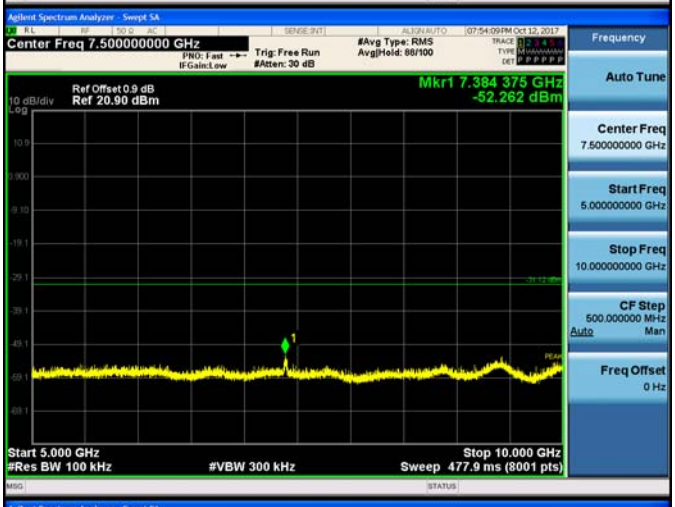
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 7.384 375 GHz
-52.262 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 14.697 500 GHz
-50.770 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		

11N40SISO_LCH_Graphs		
Pref/11N40SISO/LCH		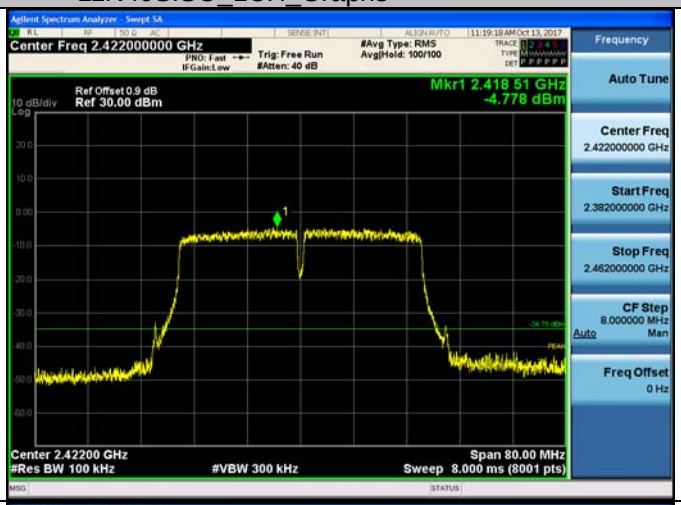
Puw/11N40SISO/LCH		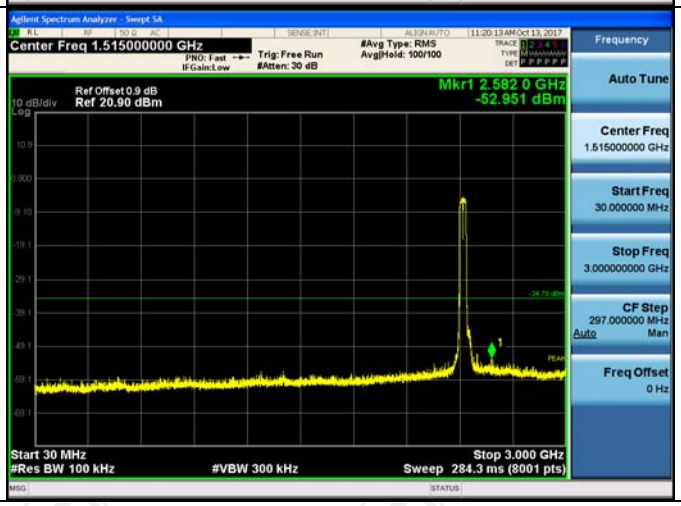

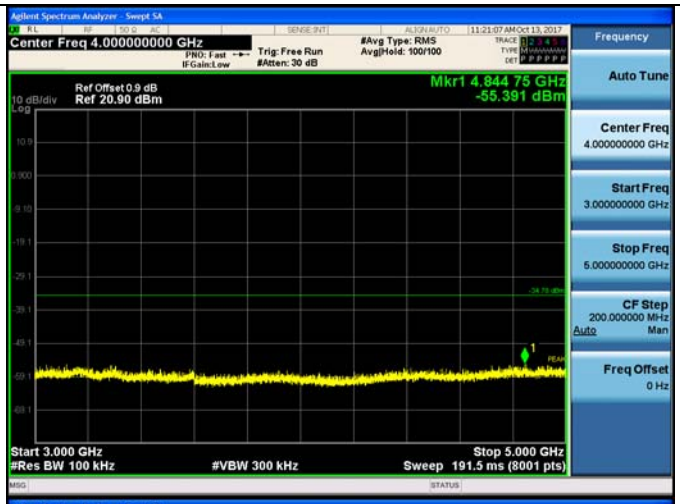
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:21:07 AM Oct 13, 2017
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 4.844 75 GHz
-55.391 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 89/100
11:22:00 AM Oct 13, 2017
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 8.899 375 GHz
-53.828 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:23:24 AM Oct 13, 2017
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 14.998 125 GHz
-51.022 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		

11N40SISO_MCH_Graphs		
Pref/11N40SISO/MCH		
Puw/11N40SISO/MCH		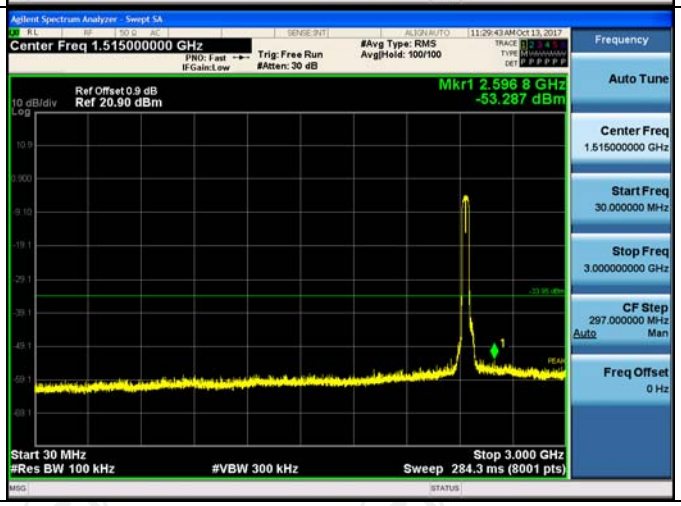

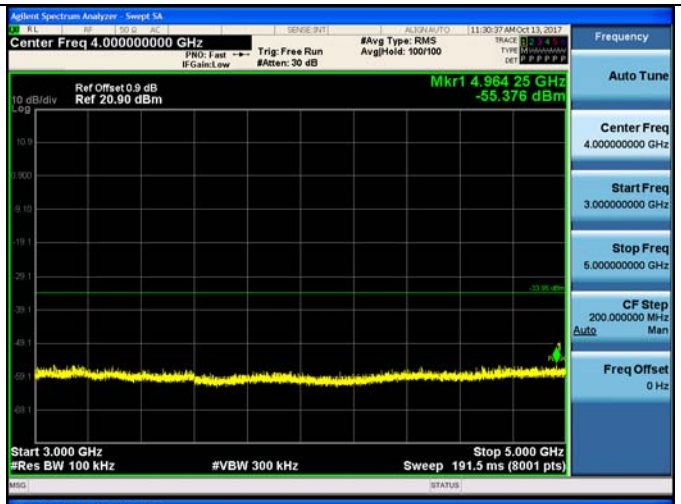
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:30:37 AM Oct 13, 2017
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 4.964 25 GHz
-55.376 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
MSG
STATUS


Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 89/100
11:31:31 AM Oct 13, 2017
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 9.395 000 GHz
-53.031 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:32:54 AM Oct 13, 2017
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 14.995 625 GHz
-51.063 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS

		

11N40SISO_HCH_Graphs		
Pref/11N40SISO/HCH		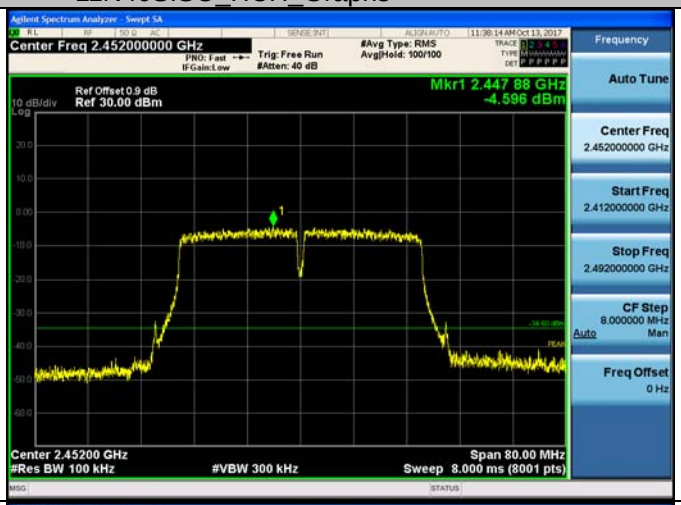
Puw/11N40SISO/HCH		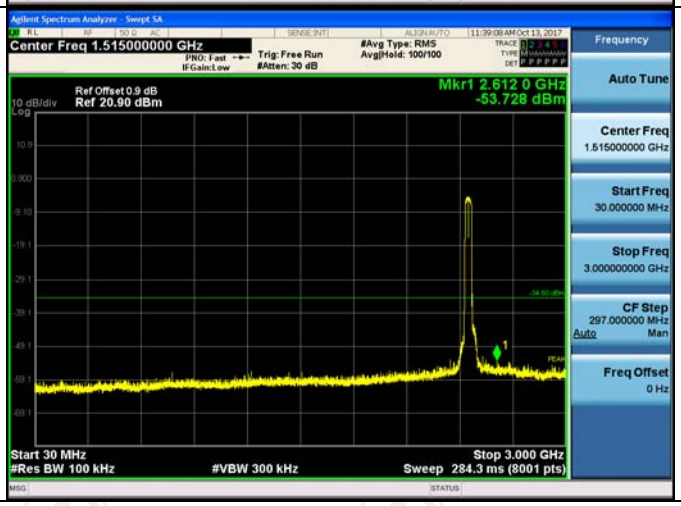


Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:40:02 AM Oct 13, 2017
Frequency
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 4.904 00 GHz
-55.307 dBm
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
MSG
STATUS

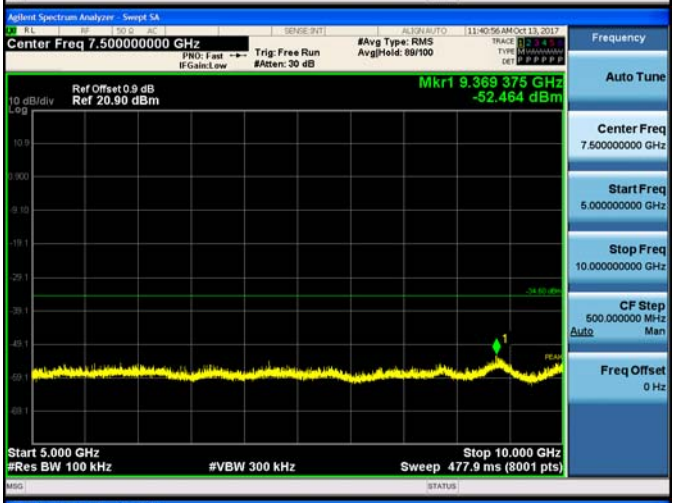
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 89/100
11:40:56 AM Oct 13, 2017
Frequency
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 9.369 375 GHz
-52.464 dBm
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:42:19 AM Oct 13, 2017
Frequency
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Log
Mkr1 14.924 375 GHz
-51.187 dBm
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
MSG
STATUS


Agilent Spectrum Analyzer - Swept SA
Center Freq 20.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 32 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:44:23 AM Oct 13, 2017
Ref Offset 0.9 dB
10 dB/div
Ref 22.90 dBm
Log
Mkr1 24.993 75 GHz
-40.829 dBm
Start 15.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.000 GHz
Sweep 955.7 ms (8001 pts)
Frequency
Auto Tune
Center Freq
20.000000000 GHz
Start Freq
15.000000000 GHz
Stop Freq
25.000000000 GHz
CF Step
1.000000000 GHz
Auto
Man
Freq Offset
0 Hz

Power Spectral Density

Result Table

Mode	Channel	Meas.Level [dBm]	Verdict
11B	LCH	-15.935	PASS
11B	MCH	-15.384	PASS
11B	HCH	-15.182	PASS
11G	LCH	-19.408	PASS
11G	MCH	-19.191	PASS
11G	HCH	-19.133	PASS
11N20SISO	LCH	-18.019	PASS
11N20SISO	MCH	-18.270	PASS
11N20SISO	HCH	-19.262	PASS
11N40SISO	LCH	-23.475	PASS
11N40SISO	MCH	-21.927	PASS
11N40SISO	HCH	-23.348	PASS

Test Graph

Graphs		
11B/LCH		
11B/MCH		

Hotline: 400-6611-140 Tel: 86-755-27673339 Fax: 86-755-27673332 http://www.tct-lab.com

11B/HCH			
11G/LCH		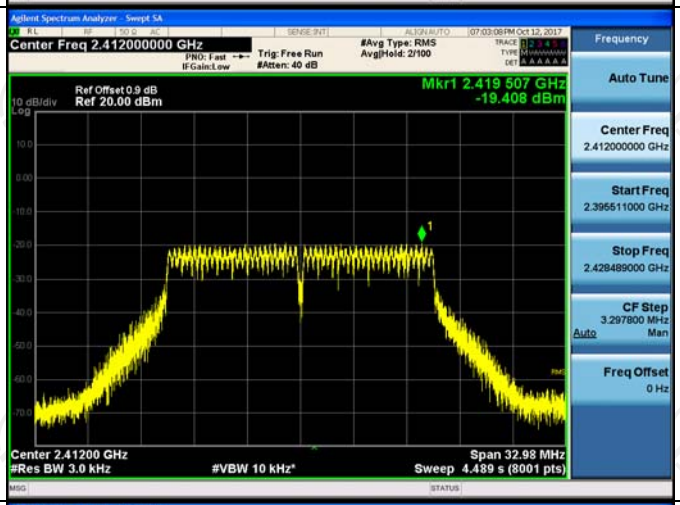	
11G/MCH		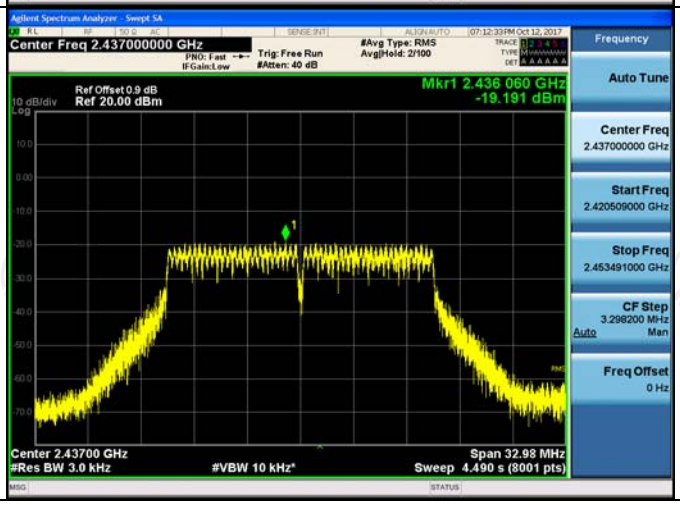	

11G/HCH		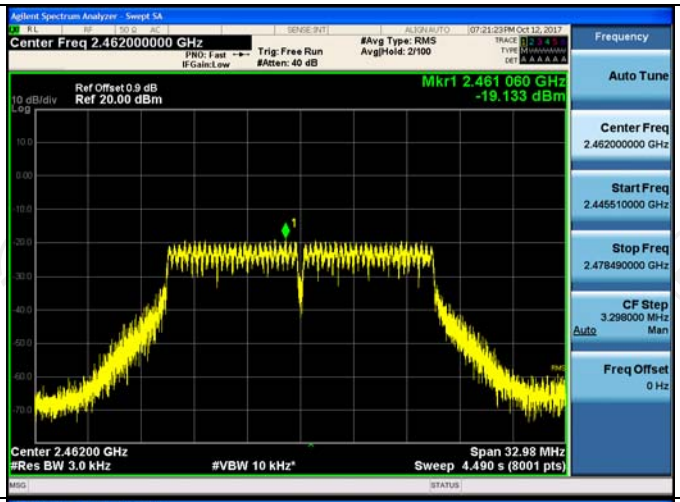	
11N20SISO/LCH		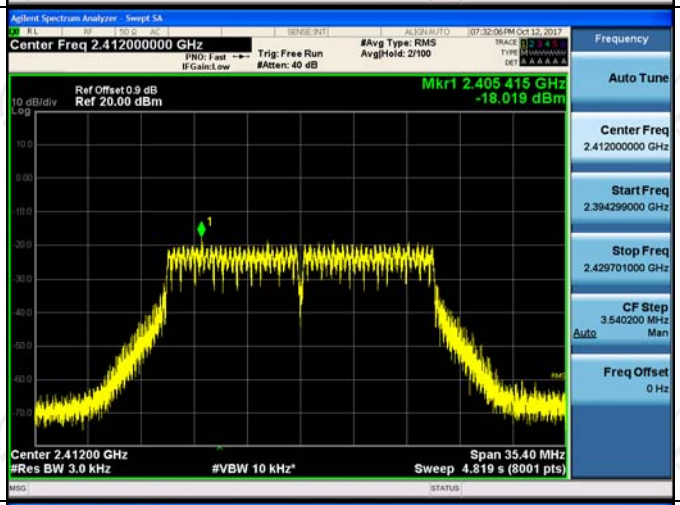	
11N20SISO/MCH		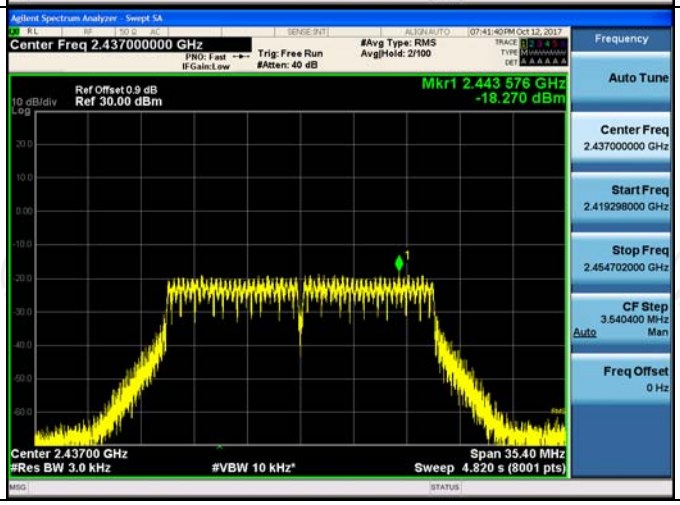	

11N20SISO/HCH		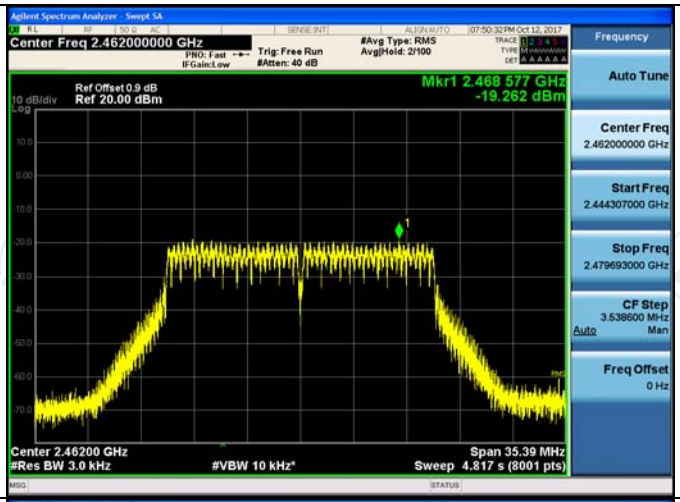	
11N40SISO/LCH		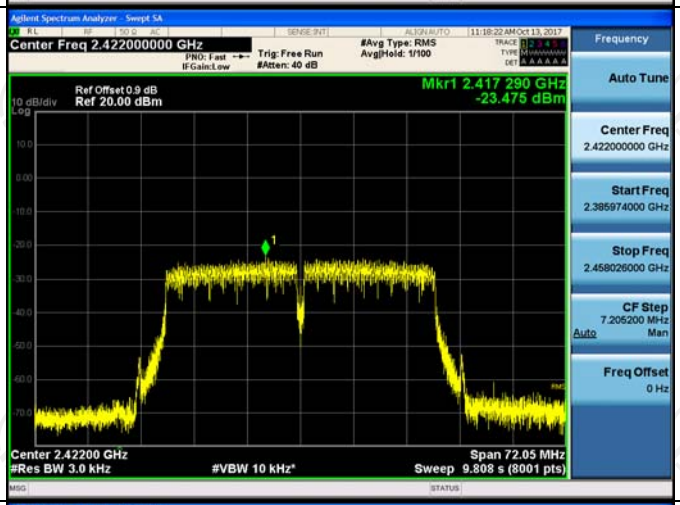	
11N40SISO/MCH		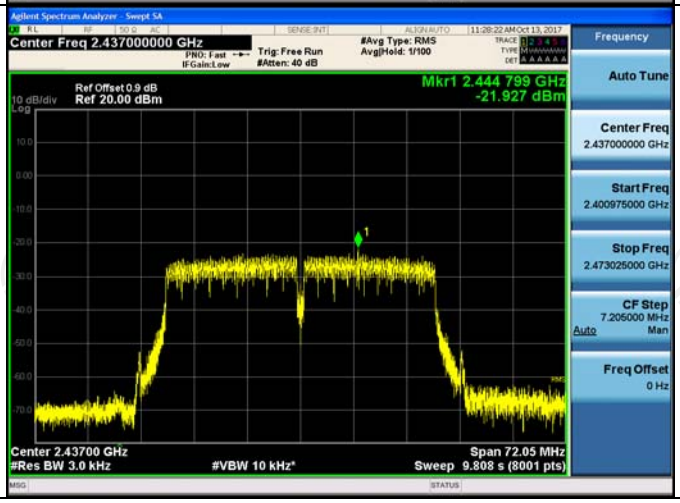	

11N40SISO/HCH		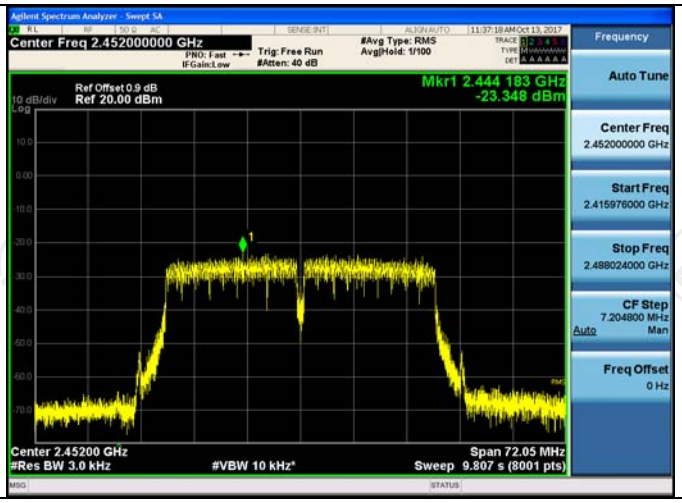	

Appendix B: Photographs of Test Setup

Refer to test report TCT170922E056

Appendix C: Photographs of EUT

Refer to test report TCT170922E056

********END OF REPORT********

Hotline: 400-6611-140 Tel: 86-755-27673339 Fax: 86-755-27673332 http://www.tct-lab.com