



849 NW State Road 45  
Newberry, FL 32669 USA  
Ph.: 888.472.2424 or  
352.472.5500  
Fax: 352.472.2030  
Email: [info@timcoengr.com](mailto:info@timcoengr.com)  
Website: [www.timcoengr.com](http://www.timcoengr.com)

## FCC PART 15.249 & IC RSS-210

### UNLICENSED INTENTIONAL RADIATOR

### TEST REPORT

|                             |   |
|-----------------------------|---|
| <b>Applicant</b>            | IRADIMED  |
| <b>Address</b>              | 1025 WILLA SPRINGS DRIVE<br>WINTER SPRINGS FL 32708 |
| <b>FCC ID</b>               | 2AKRU-IRM00   |
| <b>IC</b>                   | 22312-IRM00   |
| <b>Model Number</b>         | 3880  |
| <b>Product Description</b>  | NON-MAGNETIC PATIENT MONITOR                        |
| <b>Date Sample Received</b> | 12/8/2016   |
| <b>Final Test Date</b>      | 03/10/2017  |
| <b>Tested By</b>            | Tim Royer   |
| <b>Approved By</b>          | Cory Leverett                                       |

| Report Number        | Version Number | Description  | Issue Date |
|----------------------|----------------|--|------------|
| 2451AUT16TestReport_ | Rev1           | Initial Issue                                      | 01/30/2017 |
|                      | Rev2           | Retest Bandege, update with spectral plot pg 11,12 | 03/10/2010 |

THE ATTACHED REPORT SHALL NOT BE REPRODUCED EXCEPT IN FULL  
WITHOUT THE WRITTEN APPROVAL OF TIMCO ENGINEERING, INC.



## TABLE OF CONTENTS

|   |    |
|---|----|
| GENERAL INFORMATION .....                                 | 4  |
| EUT Specification .....                                   | 4  |
| Test Supporting Equipment .....                           | 4  |
| RESULTS SUMMARY .....                                     | 5  |
| OCCUPIED BANDWIDTH .....                                  | 6  |
| Test Data:    Measurement Table.....                      | 6  |
| Test Data:    Low end of band Plot.....                   | 7  |
| Test Data:    Middle of band Plot .....                   | 8  |
| Test Data:    High end of band Plot .....                 | 9  |
| BANDEDGE .....  | 10 |
| Test Data:    Lower Bandedge Plot.....                    | 11 |
| Test Data:    Upper Bandedge Plot .....                   | 12 |
| RADIATED SPURIOUS EMISSIONS .....                         | 13 |
| Test Data:    Measurement Table.....                      | 15 |
| AC POWER LINE CONDUCTED EMISSIONS .....                   | 16 |
| Test Data:    Powerline 1 Peak Plot .....                 | 17 |
| Test Data:    Powerline 2 Peak Plot .....                 | 18 |
| Test Data:    Powerline 2 Quasi-Peak / Average Plot ..... | 19 |
| EMC EQUIPMENT LIST .....                                  | 20 |

## GENERAL REMARKS

The attached report shall not be reproduced except in full without the written permission of Timco Engineering Inc.

### Summary

The device under test does:

- Fulfill the general approval requirements as identified in this test report and was selected by the customer.
- Not fulfill the general approval requirements as identified in this test report

### Attestations

This equipment has been tested in accordance with the standards identified in this test report. To the best of my knowledge and belief, these tests were performed using the measurement procedures described in this report.

All instrumentation and accessories used to test products for compliance to the indicated standards are calibrated regularly in accordance with ISO 17025 requirements.

I attest that the necessary measurements were made at:

**Timco Engineering Inc.**  
**849 NW State Road 45**  
**Newberry, FL 32669**



**Tested by:**

Name and Title: Tim Royer, Project Manager/Testing Engineer

**Date: 03/10/2017**



**Reviewed and approved by:**

Name and Title: Cory Leverett, Engineering Project Manager

**Date: 03/10/2017**

Applicant: IRADIMED CORPORATION  
FCC ID: 2AKRU-IRM00  
IC: 22312-IRM00  
Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)



## GENERAL INFORMATION

### EUT Specification

|                      |   |   |  |
|----------------------|---|---|--|
| Regulatory Standards | FCC Title 47 CFR Part 15.249<br>IC RSS-210 Issue 8 A2.9 & RSS-GEN Issue 4             |   |  |
| FCC ID               | <b>2AKRU-IRM00</b>  |   |  |
| IC                   | <b>22312-IRM00</b>  |   |  |
| Model                | 3880  |   |  |
| EUT Description      | NON-MAGNETIC PATIENT MONITOR  |   |  |
| Modulation Types     | Mode 1: GFSK  |   |  |
| Operating Frequency  | TX: 2404 – 2434 MHz   | RX: 2404 – 2434 MHz                     |  |
| EUT Power Source     | <input type="checkbox"/> 110–120Vac/50– 60Hz  |   |  |
|                      | <input type="checkbox"/> DC Power   |   |  |
|                      | <input checked="" type="checkbox"/> Battery Operated 14.7 VDC with external AC supply |   |  |
| Test Item            | <input type="checkbox"/> Prototype  | <input type="checkbox"/> Pre-Production | <input checked="" type="checkbox"/> Production |
| Type of Equipment    | <input type="checkbox"/> Fixed  | <input type="checkbox"/> Mobile         | <input checked="" type="checkbox"/> Portable   |
| Antenna Connector    | None  |   |  |
| Antenna              | Integral  |   |  |
| Test Conditions      | Temperature: 24-26°C<br>Relative humidity: 50-65%                                     |   |  |
| Measurement Standard | ANSI C63.10-2013<br>ANSI C63.4-2014 (Radiated Site Validation)                        |   |  |

### Test Supporting Equipment

| Device                               | Manufacturer | Model     | S/N | Supplied By | Used For                                      |
|--------------------------------------|--------------|-----------|-----|-------------|---|
| MRI Wireless ECG Module              | Iradimed     | ePod 3881 | na  | Applicant   | Terminate charging port for emissions testing |
| MRI Wireless SpO <sub>2</sub> Module | Iradimed     | oPod 3882 | na  | Applicant   |   |



## RESULTS SUMMARY

| FCC Rule Part No. | IC Standard Ref.  | Requirement               | Test Item                        | Result |
|-------------------|-------------------|---------------------------|----------------------------------|--------|
| 2.1049            | RSS-GEN 6.6       | Occupied Bandwidth        | 99% Bandwidth                    | ---    |
| 15.249(a)(c)      | RSS-210 § A2.9(a) | Fundamental and Harmonics | Radiated Spurious Emissions      | Pass   |
| 15.249(d)(e)      | RSS-247 § 5.5     | Spurious Emissions        | Bandedge                         | Pass   |
|                   |                   |                           | Radiated Spurious Emissions      | Pass   |
| 15.207(a)         | RSS-GEN § 8.8     | AC Conducted Emissions    | AC Powerline Conducted Emissions | Pass   |

### Notes:

Applicant: IRADIMED CORPORATION  
FCC ID: 2AKRU-IRM00  
IC: 22312-IRM00  
Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)

Page 5 of 20

## OCCUPIED BANDWIDTH


**Rules Part No.:** FCC 2.1049, IC RSS GEN § 6.6

**FCC Requirements:** Reporting only

**IC Requirements:** Reporting Only

**Test Method:** THE TEST PROCEDURES USED ARE DETAILED IN THE STANDARD LISTED ABOVE.

**Setup:**

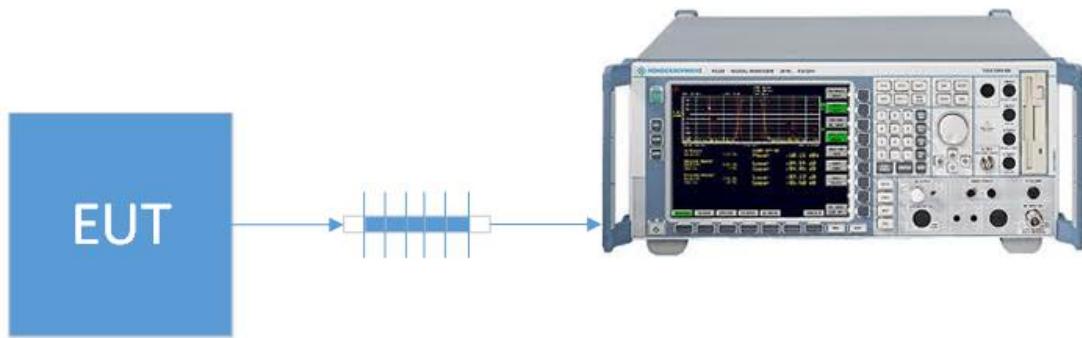


**Test Data:** **Measurement Table**

| Tuned Frequency (MHz) | BW (KHz) |
|-----------------------|----------|
| 2404                  | 861.44   |
| 2420                  | 950.36   |
| 2434                  | 867.00   |

**RESULTS:**

## OCCUPIED BANDWIDTH

**Test Data:** Low end of band Plot

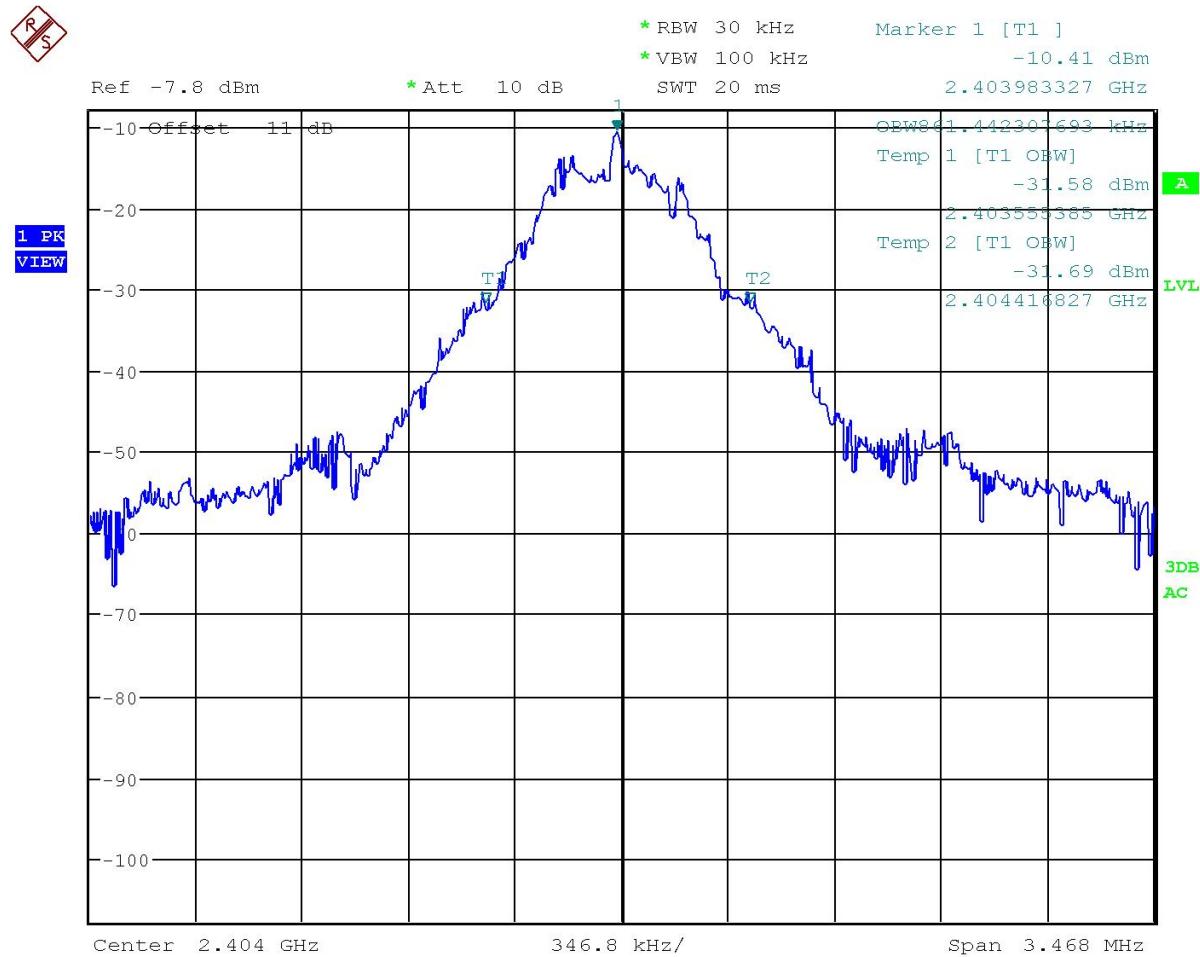

Date: 16.JAN.2017 11:36:10

**RESULTS: Meets Requirements**


Applicant: IRADIMED CORPORATION  
 FCC ID: 2AKRU-IRM00  
 IC: 22312-IRM00  
 Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)

Page 7 of 20

## OCCUPIED BANDWIDTH

**Test Data: Middle of band Plot**

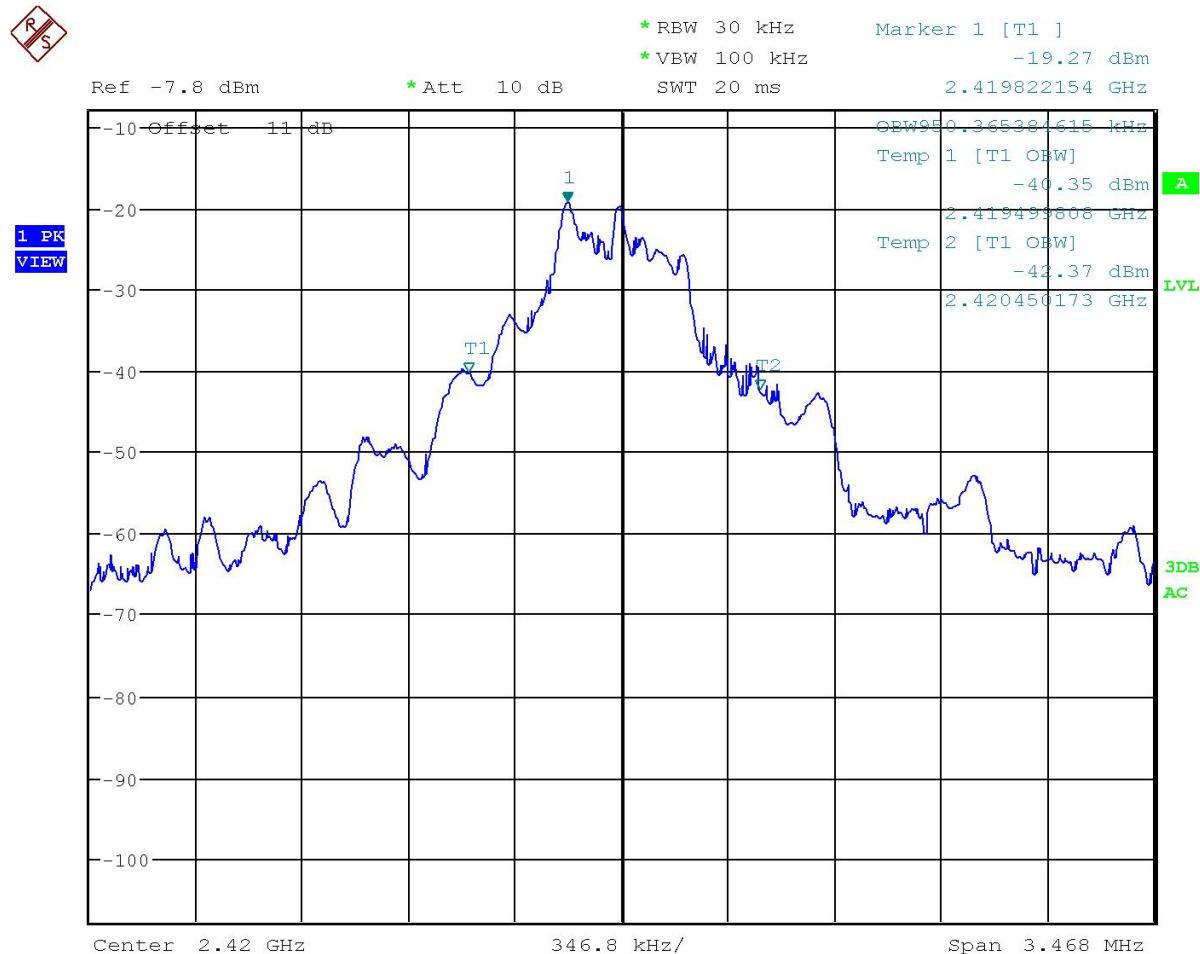

Date: 16.JAN.2017 14:14:50


**RESULTS: Meets Requirements**

Applicant: IRADIMED CORPORATION  
 FCC ID: 2AKRU-IRM00  
 IC: 22312-IRM00  
 Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)

## OCCUPIED BANDWIDTH

**Test Data:** High end of band Plot

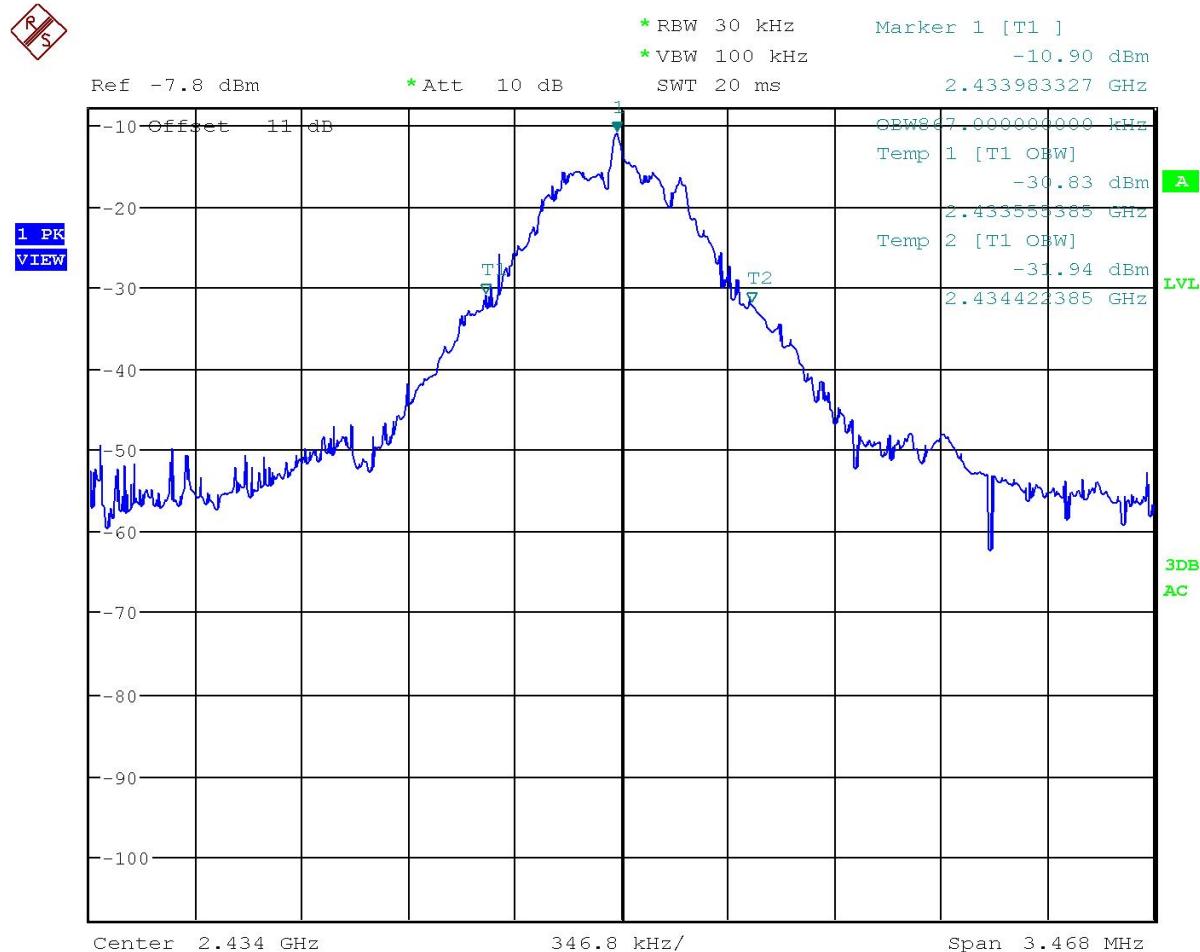

Date: 16.JAN.2017 11:33:48

## RESULTS: Meets Requirements

Applicant: IRADIMED CORPORATION  
 FCC ID: 2AKRU-IRM00  
 IC: 22312-IRM00  
 Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)


## BANDEDGE


**Rule Part No.:** FCC 15.249(d), IC RSS 210 § A2.9(b)

**Requirements:** Emissions must be at least 50 dB down from the highest emission level Within the authorized band as measured with a 100 kHz RBW, or to the limits of 15.209.

**Test Method:** THE TEST PROCEDURES USED ARE DETAILED IN THE STANDARD LISTED ABOVE.

**Setup:**

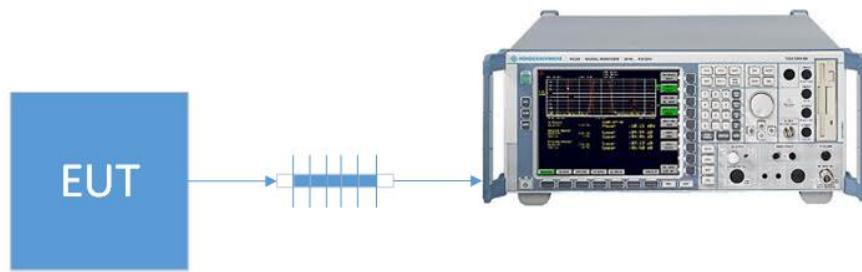

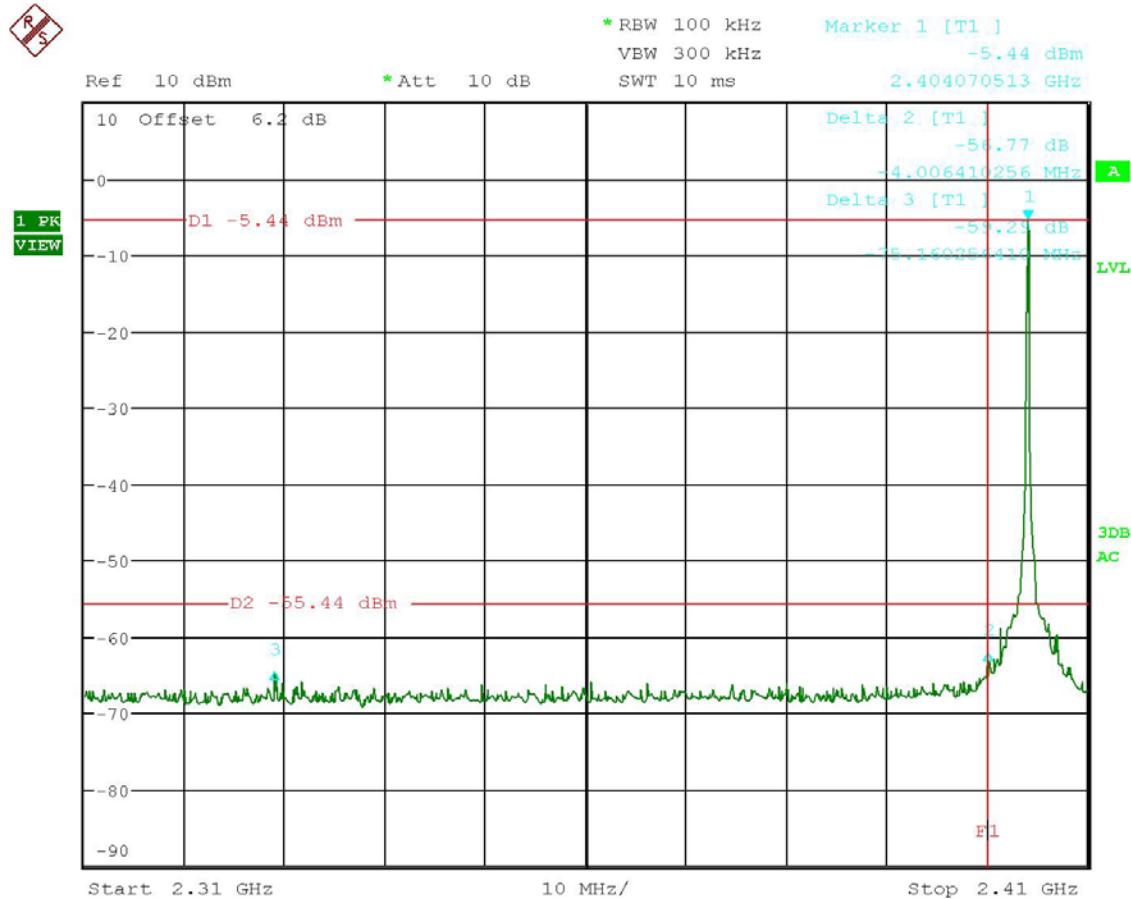**BANDEDGE**
**Test Data: Lower Bandedge Plot**


Date: 10.MAR.2017 10:49:49


**Results Meet Requirements**

Applicant: IRADIMED CORPORATION  
 FCC ID: 2AKRU-IRM00  
 IC: 22312-IRM00  
 Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)

## BANDEDGE

### Test Data: Upper Bandedge Plot

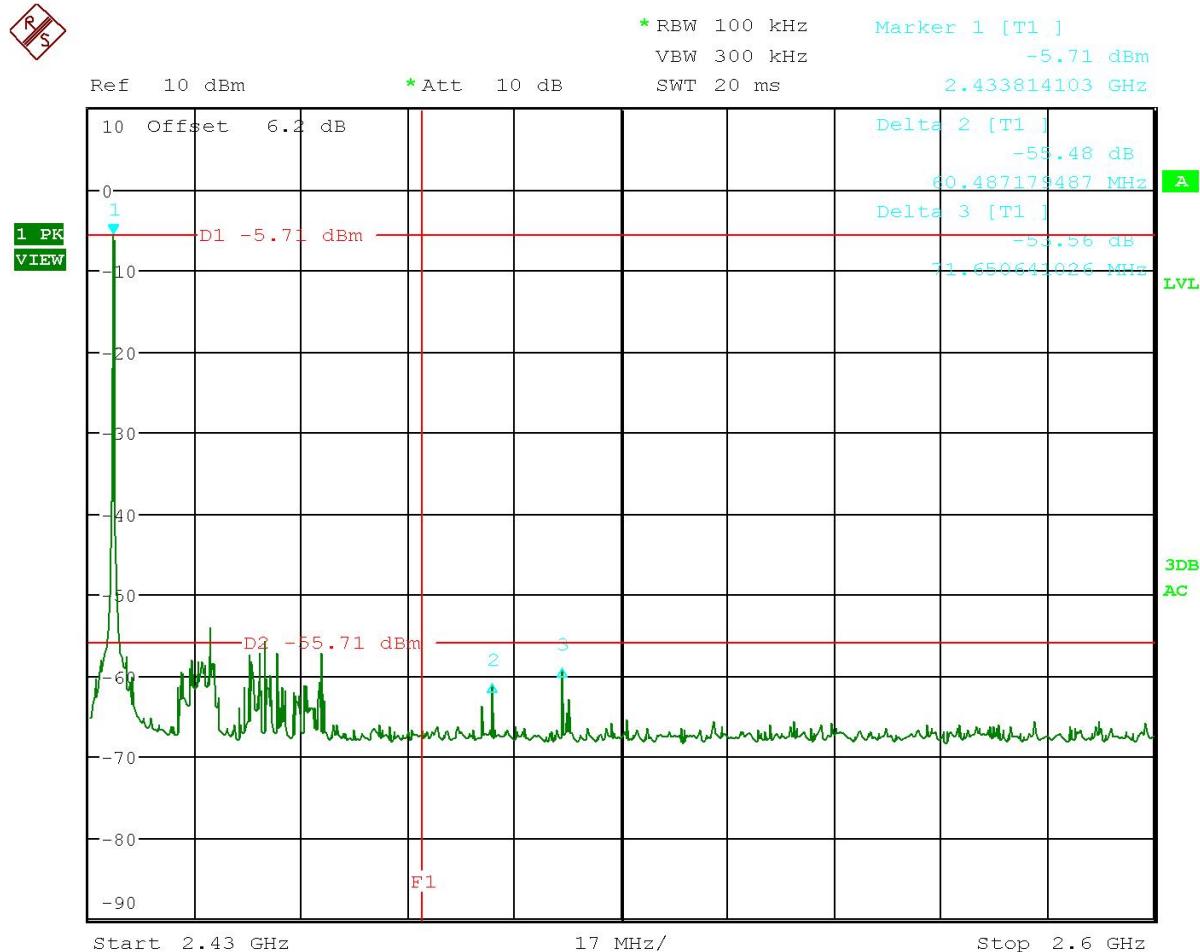

Date: 10.MAR.2017 10:48:15

### Results Meet Requirements

Applicant: IRADIMED CORPORATION  
 FCC ID: 2AKRU-IRM00  
 IC: 22312-IRM00  
 Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)

## RADIATED SPURIOUS EMISSIONS

**Rules Part No.:** FCC part 15.249 (a)(c)(d)(e)

**Requirements:** the field strength of emissions from intentional radiators operated within these frequency bands shall comply with the following:

As shown in §15.35(b), for frequencies above 1000 MHz, the field strength limits of this section are based on average limits. However, the peak field strength of any emission shall not exceed the maximum permitted average limits specified above by more than 20 dB under any condition of modulation

Field strength limits are specified at a distance of 3 meters

Emissions radiated outside of the specified frequency bands, except for harmonics, shall be attenuated by at least 50 dB below the level of the fundamental or to the general radiated emission limits in §15.209, whichever is the lesser attenuation.

| Frequency                    | Limits                              |
|------------------------------|-------------------------------------|
| Part 15.209                  |                                     |
| 9 to 490 kHz                 | 2400/F (kHz) $\mu$ V/m @ 300 meters |
| 490 to 1705 kHz              | 24000/F (kHz) $\mu$ V/m @ 30 meters |
| 1705 kHz to 30 MHz           | 29.54 dB $\mu$ V/m @ 30 meters      |
| 30 – 88                      | 40.0 dB $\mu$ V/m @ 3 meters        |
| 80 – 216                     | 43.5 dB $\mu$ V/m @ 3 meters        |
| 216 – 960                    | 46.0 dB $\mu$ V/m @ 3 meters        |
| Above 960                    | 54.0 dB $\mu$ V/m @ 3 meters        |
| Part 15.249                  |                                     |
| Fundamental 902 – 928 MHz    | 94.0 dB $\mu$ V/m @ 3 meters        |
| Fundamental 2.4 – 2.4835 GHz | 94.0 dB $\mu$ V/m @ 3 meters        |
| Harmonics                    | 54.0 dB $\mu$ V/m @ 3 meters        |

**Test Method:** ANSI C63.4 § Annex D Validation of radiated emissions standard test sites  
ANSI C63.10 § 6.3 Common requirements radiated emissions  
ANSI C63.10 § 6.4 Emissions below 30 MHz  
ANSI C63.10 § 6.5 Emissions between 30 & 1000 MHz  
ANSI C63.10 § 6.6 Emissions above 1 GHz

### Field Strength Calculation:

The field strength at 3m was established by adding the meter reading of the spectrum analyzer (which is set to read in units of dB $\mu$ V) to the antenna correction factor supplied by the antenna manufacturer plus the coax loss. The antenna correction factors are stated in terms of dB. The gain of the preselector was accounted for in the spectrum analyzer meter reading.


Example:

$$\begin{array}{llll}
\text{Freq (MHz)} & \text{Meter Reading} & + \text{ACF} & + \text{CL} = \text{FS} \\
33 & 20 \text{ dB}\mu\text{V} & + 10.36 \text{ dB} & + 0.5 = 30.86 \text{ dB}\mu\text{V/m @ 3m}
\end{array}$$


## RADIATED SPURIOUS EMISSIONS

### Setup:


#### Emissions below 30 MHz

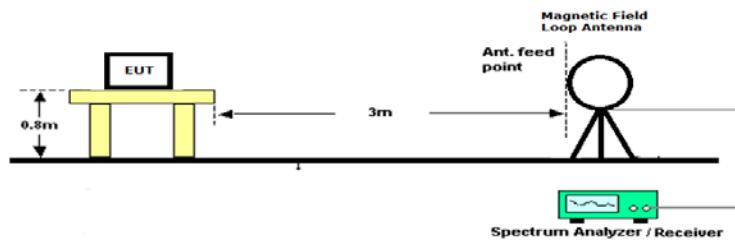

#### Emissions 30 – 1000 MHz

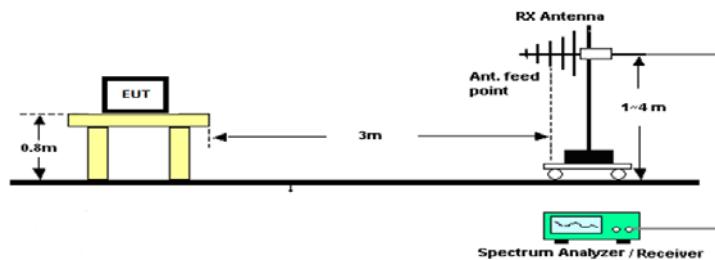

#### Emissions above 1 GHz

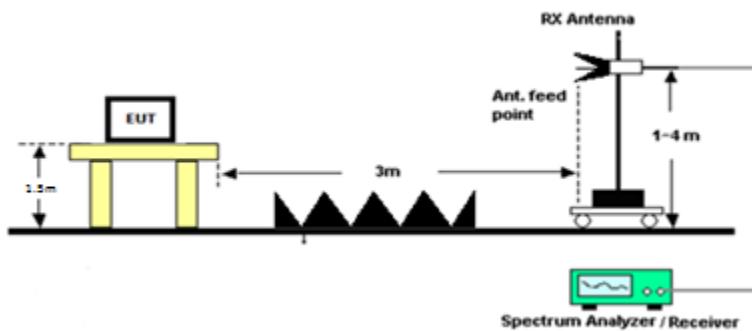



## RADIATED SPURIOUS EMISSIONS

**Notes:** The EUT was checked in three orthogonal planes as required, a setup photo is provided to show the orientation of the worst case position.

Only emissions within 20dB of the limit are reported.

The spectrum was measured from 9 KHz to 25 GHz

### Test Data: Measurement Table

| Tuned Freq (MHz) | Emission Frequency (MHz) | Detector (QP/PK/AV) | Meter Reading (dBuV) | Antenna Polarity (H/V) | Coax Loss (dB) | Correction Factor (dB/M) | Field Strength (dBuV/M) | Limit (dBuV/M) | Margin (dB) |
|------------------|--------------------------|---------------------|----------------------|------------------------|----------------|--------------------------|-------------------------|----------------|-------------|
| 2404.00          | 276.92                   | PK                  | 20.44                | V                      | 1.95           | 15.07                    | 37.46                   | 46.00          | 8.54        |
| 2404.00          | 287.18                   | PK                  | 19.70                | H                      | 1.98           | 14.26                    | 35.94                   | 46.00          | 10.06       |
| 2404.00          | 747.43                   | PK                  | 18.31                | H                      | 3.15           | 21.25                    | 42.71                   | 46.00          | 3.29        |
| 2404.00          | 826.90                   | PK                  | 20.11                | V                      | 3.30           | 21.79                    | 45.20                   | 46.00          | 0.80        |
| 2404.00          | 2344.85                  | PK                  | 12.92                | H                      | 5.62           | 32.12                    | 50.66                   | 54.00          | 3.34        |
| 2404.00          | 2399.70                  | PK                  | 13.21                | V                      | 5.64           | 32.21                    | 51.06                   | 54.00          | 2.94        |
| 2404.00          | 2404.00                  | PK                  | 51.50                | V                      | 5.69           | 32.41                    | 89.60                   | 94.00          | 4.40        |
| 2404.00          | 4808.00                  | PK                  | 6.84                 | H                      | 8.07           | 33.99                    | 48.90                   | 54.00          | 5.10        |
| 2404.00          | 7212.00                  | PK                  | 7.48                 | V                      | 9.92           | 35.42                    | 52.82                   | 54.00          | 1.18        |
| 2404.00          | 9616.00                  | PK                  | -4.06                | H                      | 11.43          | 36.83                    | 44.20                   | 54.00          | 9.80        |
| 2420.00          | 343.58                   | PK                  | 20.54                | V                      | 2.14           | 13.84                    | 36.52                   | 46.00          | 9.48        |
| 2420.00          | 365.38                   | PK                  | 20.39                | H                      | 2.19           | 14.69                    | 37.27                   | 46.00          | 8.73        |
| 2420.00          | 729.48                   | PK                  | 18.67                | H                      | 3.12           | 20.21                    | 42.00                   | 46.00          | 4.00        |
| 2420.00          | 739.74                   | PK                  | 20.40                | V                      | 3.14           | 20.67                    | 44.21                   | 46.00          | 1.79        |
| 2420.00          | 2420.00                  | PK                  | 52.87                | V                      | 5.71           | 32.46                    | 91.04                   | 94.00          | 2.96        |
| 2420.00          | 4840.00                  | PK                  | 10.46                | H                      | 8.10           | 33.96                    | 52.52                   | 54.00          | 1.48        |
| 2420.00          | 7260.00                  | PK                  | -3.56                | H                      | 9.96           | 35.52                    | 41.92                   | 54.00          | 12.08       |
| 2420.00          | 9680.00                  | PK                  | -8.91                | V                      | 11.47          | 36.96                    | 39.52                   | 54.00          | 14.48       |
| 2434.00          | 339.74                   | PK                  | 20.44                | V                      | 2.13           | 13.69                    | 36.26                   | 46.00          | 9.74        |
| 2434.00          | 405.13                   | PK                  | 20.20                | V                      | 2.30           | 15.30                    | 37.80                   | 46.00          | 8.20        |
| 2434.00          | 730.76                   | PK                  | 19.41                | V                      | 3.12           | 20.20                    | 42.73                   | 46.00          | 3.27        |
| 2434.00          | 771.79                   | PK                  | 18.82                | V                      | 3.20           | 21.89                    | 43.91                   | 46.00          | 2.09        |
| 2434.00          | 2434.00                  | PK                  | 53.80                | V                      | 5.73           | 32.50                    | 92.03                   | 94.00          | 1.97        |
| 2434.00          | 2486.00                  | PK                  | 12.84                | V                      | 5.78           | 32.66                    | 51.28                   | 54.00          | 2.72        |
| 2434.00          | 2486.80                  | PK                  | 13.37                | H                      | 5.79           | 32.66                    | 51.82                   | 54.00          | 2.18        |
| 2434.00          | 4868.00                  | PK                  | 6.72                 | V                      | 8.12           | 33.93                    | 48.77                   | 54.00          | 5.23        |
| 2434.00          | 7302.00                  | PK                  | 6.45                 | V                      | 9.99           | 35.60                    | 52.04                   | 54.00          | 1.96        |
| 2434.00          | 9736.00                  | PK                  | -4.53                | H                      | 11.51          | 37.04                    | 44.02                   | 54.00          | 9.98        |

### Results: Meets Requirements

Applicant: IRADIMED CORPORATION  
FCC ID: 2AKRU-IRM00  
IC: 22312-IRM00  
Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)

## AC POWER LINE CONDUCTED EMISSIONS

**Rules Part No.:** FCC 15.207(a), IC RSS Gen § 8.8


**Requirements:**

| Frequency (MHz) | Quasi Peak Limits (dB $\mu$ V) | Average Limits (dB $\mu$ V) |
|-----------------|--------------------------------|-----------------------------|
| 0.15 – 0.5      | 66 – 56 *                      | 56 – 46 *                   |
| 0.5 – 5.0       | 56                             | 46                          |
| 5.0 – 30        | 60                             | 50                          |

\* Decrease with logarithm of frequency

**Test Method:** ANSI C63.10 § 6.2 Test Method for AC power-line conducted emissions


**Setup:**

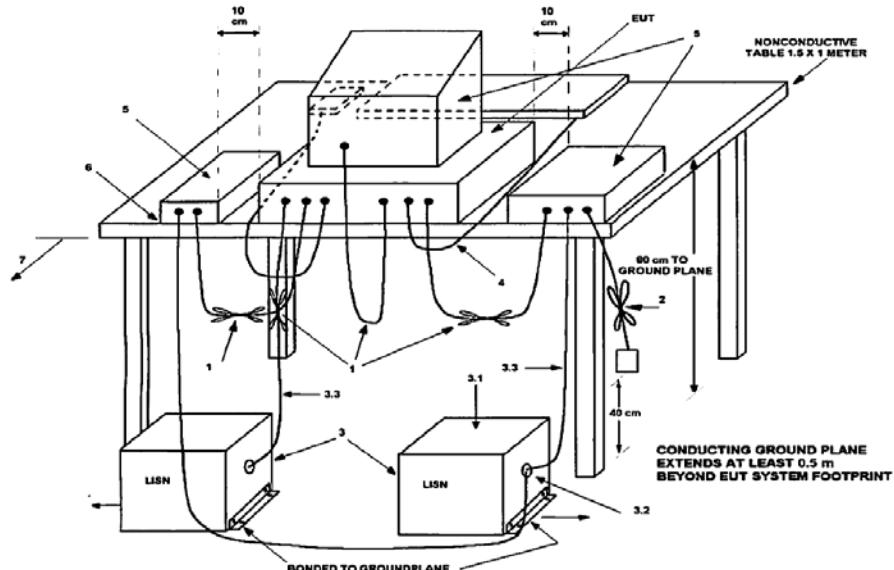

## AC POWER LINE CONDUCTED EMISSIONS

**Notes:** The following plots represent the emissions read for power line Conducted. Both lines were observed.

### Test Data: Powerline 1 Peak Plot

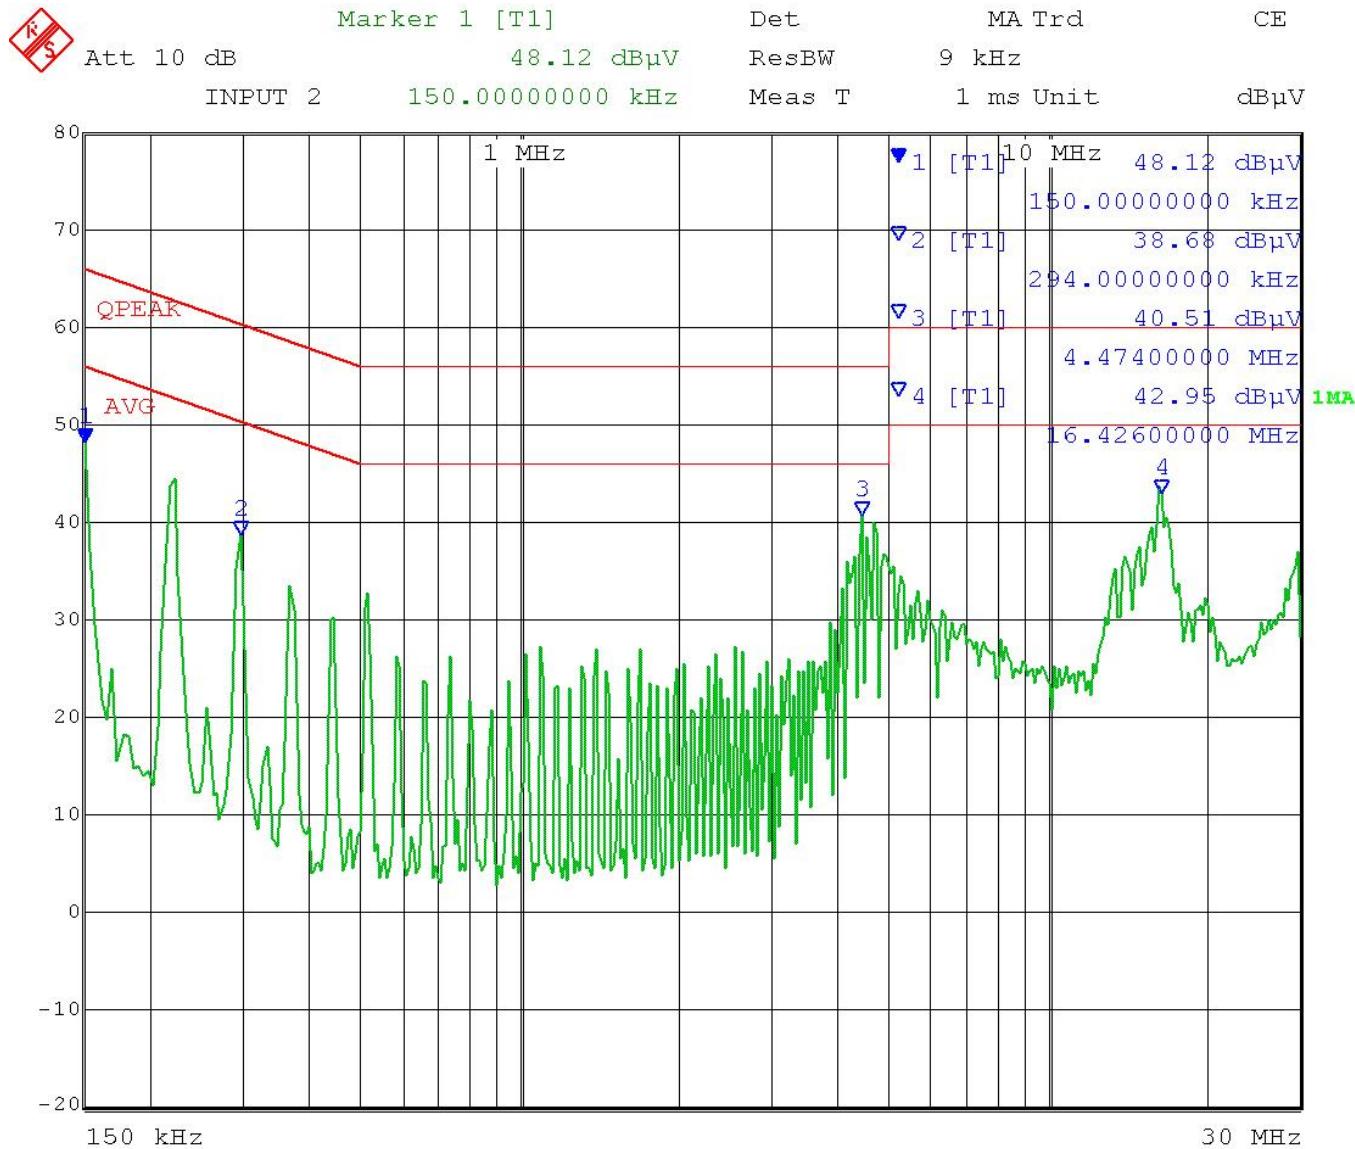


Date: 24.JAN.2017 08:38:40

Applicant: IRADIMED CORPORATION  
 FCC ID: 2AKRU-IRM00  
 IC: 22312-IRM00  
 Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)

## AC POWER LINE CONDUCTED EMISSIONS

### Test Data: Powerline 2 Peak Plot

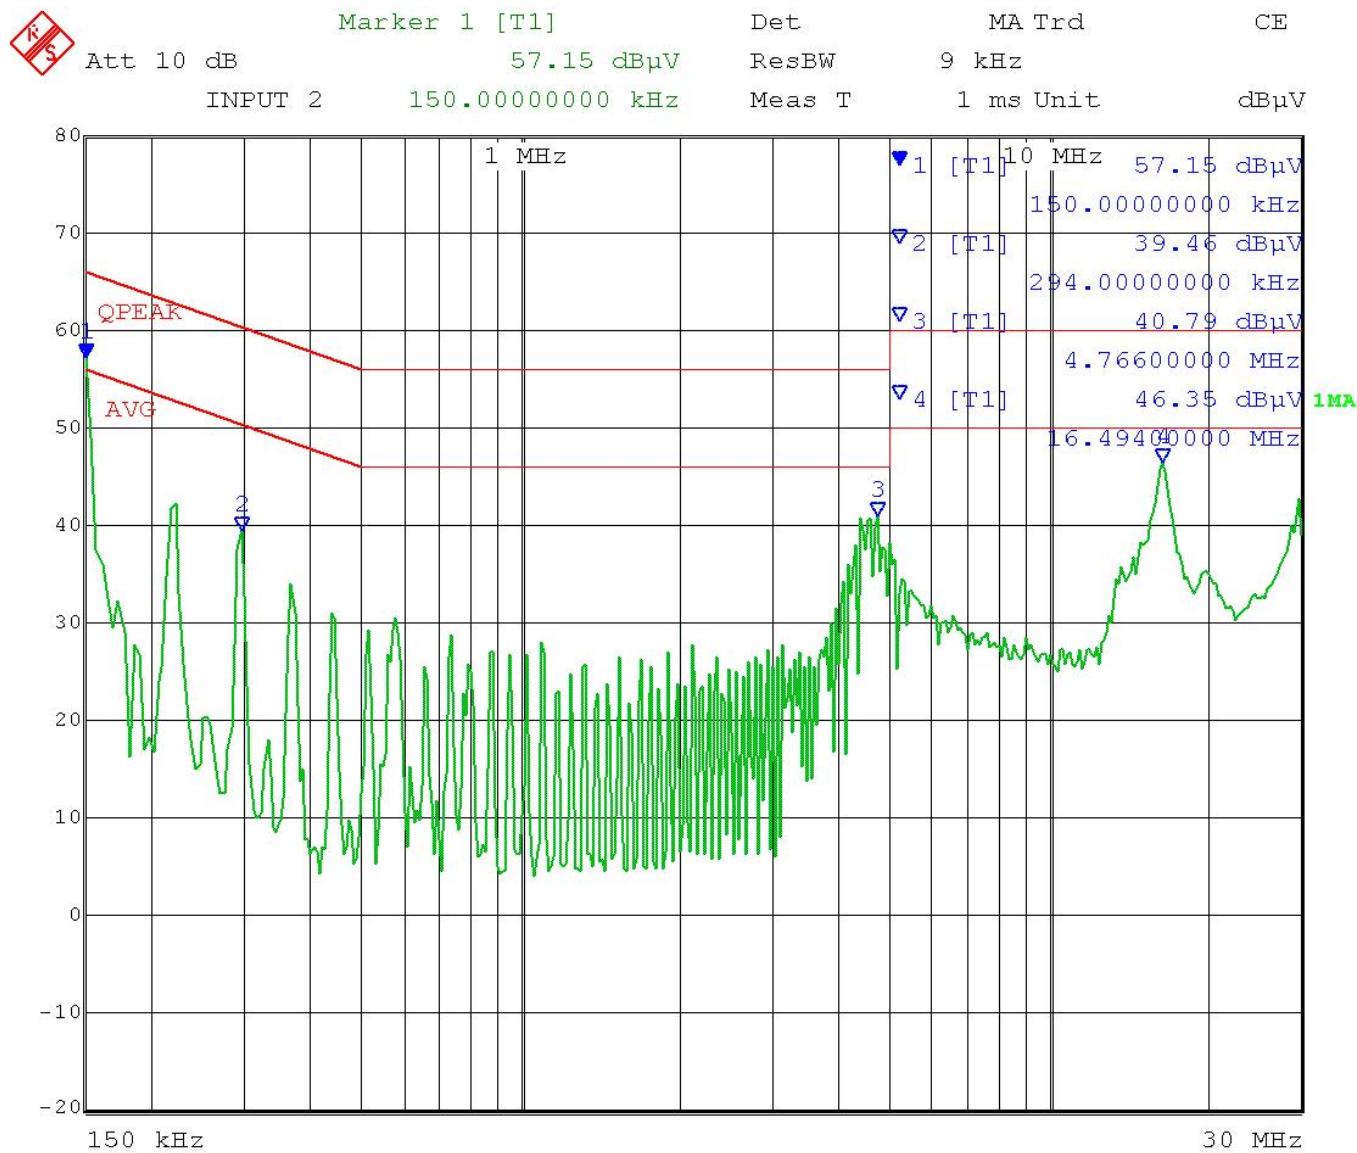

Date: 24.JAN.2017 08:37:05


### RESULTS: Meets Requirements

Applicant: IRADIMED CORPORATION  
 FCC ID: 2AKRU-IRM00  
 IC: 22312-IRM00  
 Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)

## AC POWER LINE CONDUCTED EMISSIONS

### Test Data: Powerline 2 Quasi-Peak / Average Plot

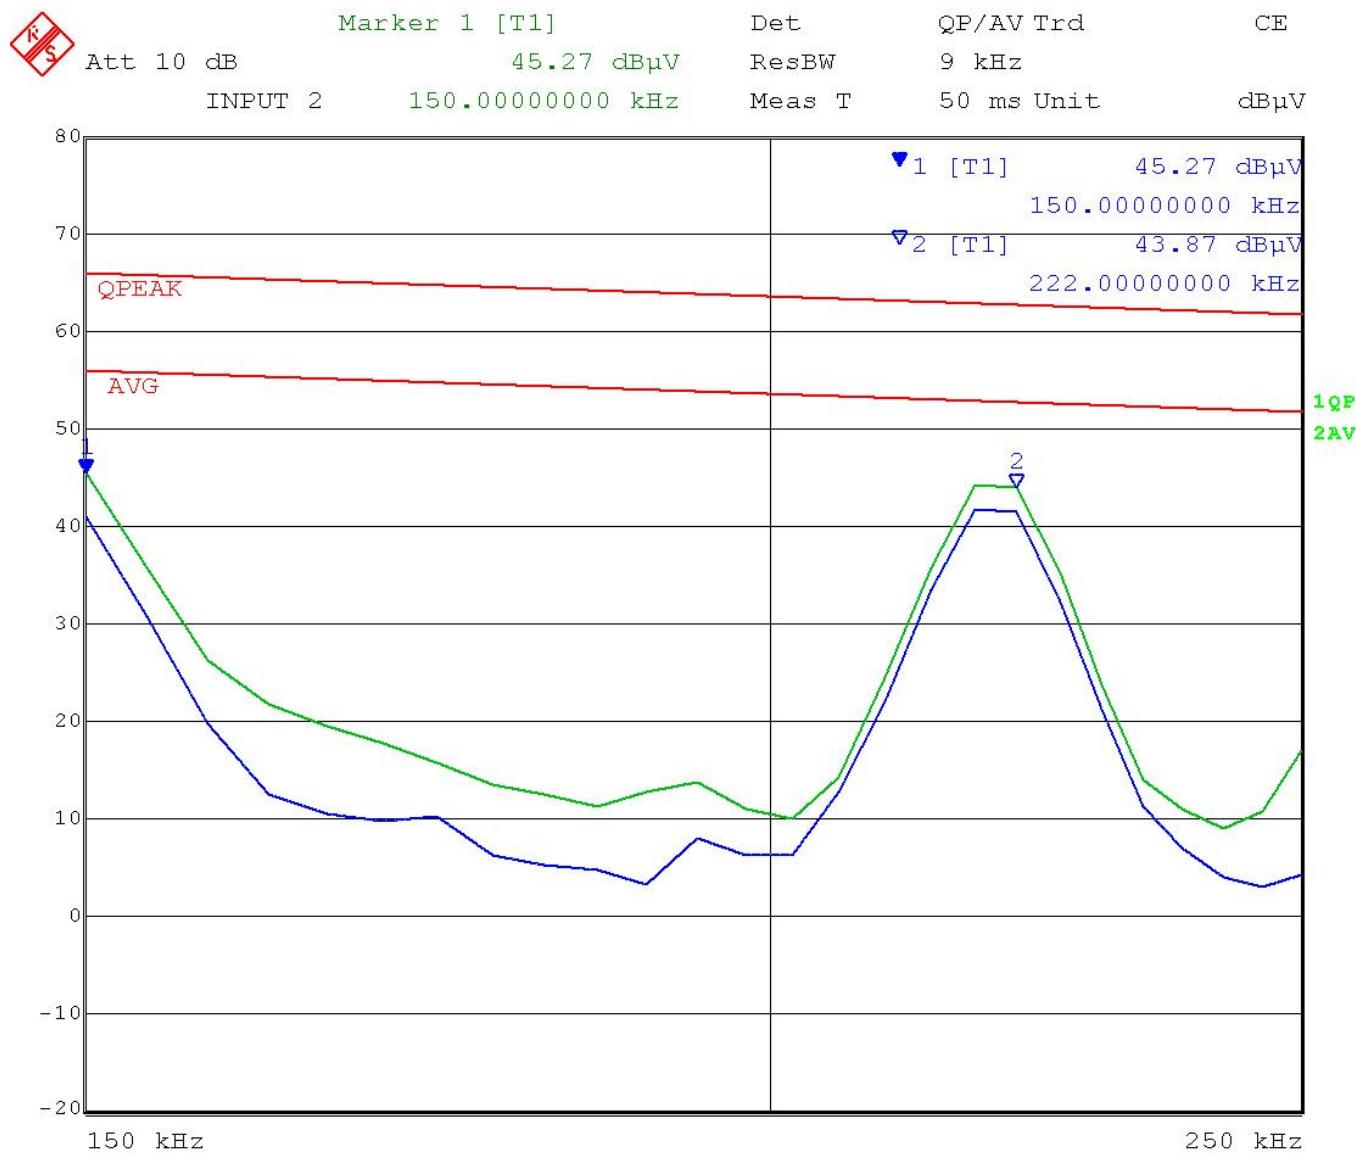

Date: 24.JAN.2017 08:41:02

### RESULTS: Meets Requirements

Applicant: IRADIMED CORPORATION  
 FCC ID: 2AKRU-IRM00  
 IC: 22312-IRM00  
 Report: 2451AUT16TestReport\_Rev2

[Table of Contents](#)



## EMC EQUIPMENT LIST

| Device  | Manufacturer         | Model                         | Serial Number                            | Cal/Char Date | Due Date |
|---|----------------------|-------------------------------|--|---------------|----------|
| LISN (Primary)                                | Electro-Metrics      | EM-7820                       | 2682                                     | 05/08/15      | 05/08/17 |
| Coaxial Cable - BMBM-1000-00 Silver           | Semflex              | LISN Cable                    | BMBM-1000-00                             | 01/14/15      | 01/14/17 |
| Antenna: Biconical 1096 Chamber               | Eaton                | 94455-1                       | 1096                                     | 07/14/15      | 07/14/17 |
| Antenna: Log-Periodic 1122                    | Electro-Metrics      | LPA-25                        | 1122                                     | 07/14/15      | 07/14/17 |
| Antenna: Standard Gain Horn 18.0-26.3 GHz     | Systron Donner       | DBE-520-20                    | Not Serialized                           | NA            | NA       |
| Antenna: Standard Gain Horn 12.4-18.0 GHz     | ATM                  | 62-442-6                      | D262108-01                               | NA            | NA       |
| CHAMBER                                       | Panashield           | 3M                            | N/A                                      | 04/25/16      | 12/31/17 |
| Antenna: Double-Ridged Horn/ETS Horn 2        | ETS-Lindgren Chamber | 3117                          | 00041534                                 | 02/25/15      | 02/25/17 |
| Software: Field Strength Program              | Timco                | N/A                           | Version 4.0                              | NA            | NA       |
| Antenna: Active Loop                          | ETS-Lindgren         | 6502                          | 00062529                                 | 11/18/15      | 11/18/17 |
| EMI Test Receiver R & S ESU 40 Chamber        | Rohde & Schwarz      | ESU 40                        | 100320                                   | 04/01/16      | 04/01/18 |
| Coaxial Cable - Chamber 3 cable set (Primary) | Micro-Coax           | Chamber 3 cable set (Primary) | KMKG-0244-01; KMKG-0670-00; KFKF-0198-01 | 08/08/16      | 08/08/18 |
| Pre-amp                                       | RF-LAMBDA            | RNLA00M45GA                   | NA                                       | 01/04/16      | 01/04/18 |
| Band Reject Filter 2.4 GHz                    | Micro-Tronics        | BRM50702-02                   | -G042                                    | 9/27/16       | 9/27/18  |
| High Pass Filter 18GHz                        | Micro-Tronics        | HPS18771                      | -002                                     | 9/27/16       | 9/27/18  |
| Bore-sight Antenna Positioning Tower          | Sunol Sciences       | TLT2                          | N/A                                      | NA            | NA       |

### \*EMI RECEIVER SOFTWARE VERSION

The receiver firmware used was version 4.43 Service Pack 3

**END OF TEST REPORT**