

BT

DUT:HA-NP1T

Communication System: BT; Frequency: 2480 MHz;Duty Cycle: 1:1.3020
Medium: H2450 Medium parameters used: $f = 2480 \text{ MHz}$; $\sigma = 1.78 \text{ S/m}$; $\epsilon_r = 40.05$; $\rho = 1000 \text{ kg/m}^3$
Ambient Temperature : $22.0 \text{ }^\circ\text{C}$; Liquid Temperature : $21.8 \text{ }^\circ\text{C}$


DASY5 Configuration:
- Probe: EX3DV4 - SN3970; Calibrated: 2024/6/25;
- Electronics: DAE4 Sn1418; Calibrated: 2024/5/17
- Phantom: SAM; Type: QD000P40CD; Serial: TP:1794
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Left Head/Front-DH5/Area Scan (6x7x1): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$

Maximum value of SAR (measured) = 0.0245 W/kg

Left Head/Front-DH5/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 0.792 V/m ; Power Drift = 0.11 dB
Peak SAR (extrapolated) = 0.210 W/kg
SAR(1 g) = 0.012 W/kg ; SAR(10 g) = 0.00481 W/kg
Maximum value of SAR (measured) = 0.026 W/kg

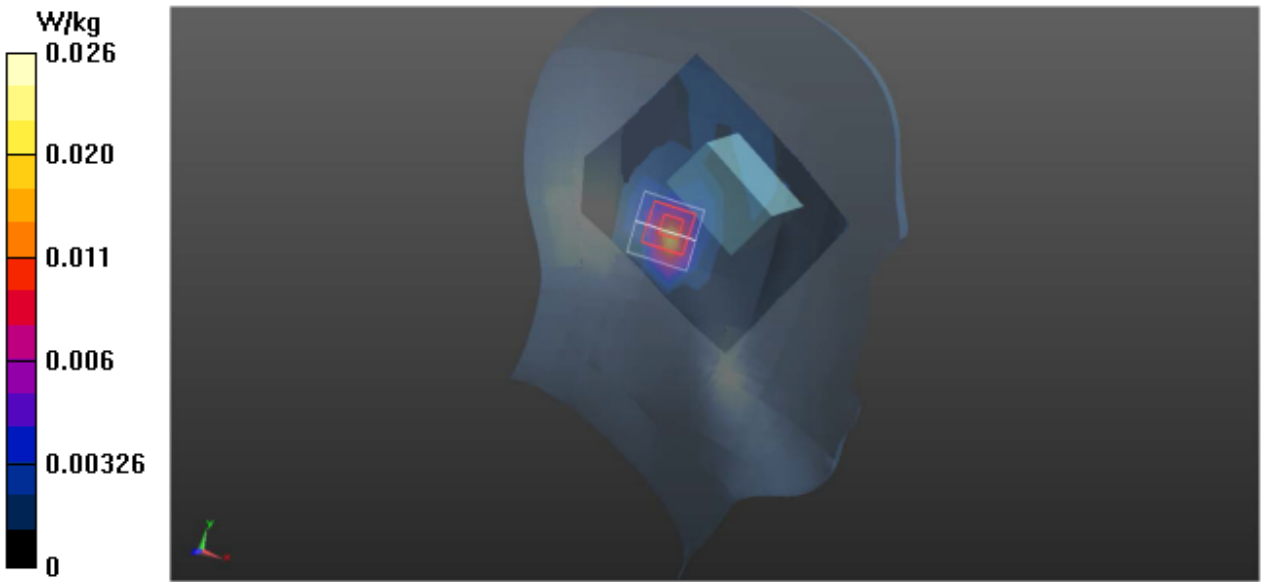

BT

DUT: HA-NP1T

Communication System:BT; Frequency: 2480 MHz;Duty Cycle: 1:1.3020
Medium: H2450 Medium parameters used: $f = 2480\text{ MHz}$; $\sigma = 1.78\text{ S/m}$; $\epsilon_r = 40.05$; $\rho = 1000\text{ kg/m}^3$
Ambient Temperature : $22.0\text{ }^{\circ}\text{C}$; Liquid Temperature : $21.8\text{ }^{\circ}\text{C}$

- DASY5 Configuration:
- Probe: EX3DV4 - SN3970; Calibrated: 2024/6/25;
 - Electronics: DAE4 Sn1418; Calibrated: 2024/5/17
 - Phantom: SAM; Type: QD000P40CD; Serial: TP:1794
 - Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Front-3DH5/Area Scan (7x7x1): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$

Maximum value of SAR (measured) = 0.0088 W/kg

Front-3DH5/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 0.741 V/m ; Power Drift = 0.16 dB
Peak SAR (extrapolated) = 0.0410 W/kg
SAR(1 g) = 0.019 W/kg ; SAR(10 g) = 0.00921 W/kg
Maximum value of SAR (measured) = 0.015 W/kg

