

Appendix C for KSCR221100226101

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date
Dipole	☐	1	CLA150	4025	2021/04/26
	☐	2	D450V3	1103	2021/04/21
	☐	3	D750V3	1188	2022/03/29
	☐	4	D835V2	4d114	2022/03/31
	☐	5	D900V2	1d079	2022/06/07
	☐	6	D1800V2	2d170	2022/03/31
	☐	7	D1900V2	5d136	2022/06/07
	☐	8	D2000V2	1041	2022/06/06
	☐	9	D2300V2	1096	2022/03/31
	☒	10	D2450V2	817	2022/04/01
	☐	11	D2600V2	1158	2022/03/31
	☐	12	D5GHzV2	1095	2022/06/01
DAE	☒	13	DAE4	1245	2022/05/30
Probe	☒	14	EX3DV4	7346	2022/03/30



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1 Dipole

1.1 CLA150 - SN 4025

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Client: SGS-CN (Audeon)		Certificate No.: CLA150-4025_Apr21	
CALIBRATION CERTIFICATE			
Object: CLA150 - SN: 4025			
Calibration procedure(s): QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz			
Calibration date: April 26, 2021			
The calibration certificate documents the traceability to national standards, which require the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and on part of the certificate.			
All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.			
Calibration Equipment Used (M&E critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 10475	09-Apr-21 (No. 217-03001/03002)	Apr-22
Power sensor NRP Z01	SN: 10384	09-Apr-21 (No. 217-03001)	Apr-22
Power sensor NRP Z01	SN: 10385	09-Apr-21 (No. 217-03002)	Apr-22
Reference 20 dB Attenuator	SN: C23602 (C03)	09-Apr-21 (No. 217-03003)	Apr-22
Type-N mismatch combination	SN: 310907 / 0007	09-Apr-21 (No. 217-03004)	Apr-22
Reference Probe EX300A	SN: 3877	30-Dec-20 (No. 203-3077_Dec20)	Dec-21
EXE4	SN: 661	19-Jan-20 (No. 19459-659_Jan20)	Jan-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter S4419E	SN: G341303024	09-Apr-15 (in house check Jun-20)	In house check Jun-20
Power sensor E4113A	SN: MY4169007	09-Apr-15 (in house check Jun-20)	In house check Jun-20
Power sensor E4113A	SN: 00010210	09-Apr-15 (in house check Jun-20)	In house check Jun-20
RF generator HP 8594C	SN: U504001709	04-Aug-19 (in house check Jun-20)	In house check Jun-20
Network Analyzer Agilent T8368A	SN: U541000477	31-Mar-14 (in house check Oct-19)	In house check Oct-21
Calibrated by:	Janis Johannes Katsch	Function: Laboratory Technician	Signature:
Approved by:	Kajsa Polovic	Technical Manager	Signature:
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: April 26, 2021			
Certificate No: CLA150-4025_Apr21		Page 1 of 5	

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Glossary:			
TSL	Issue simulating liquid		
ConvF	sensitivity in TSL / NORM x,y,z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013			
b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016			
c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010			
d) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
e) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.			
• Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the reported SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: CLA150-4025_Apr21		Page 2 of 5	

Measurement Conditions		
DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELIA Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz ± 1 MHz	

Head TSL parameters			
The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	52.3	0.75 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL		
SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.90 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.88 W/kg ± 19.4 % (k=2)
SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.60 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)	
Antenna Parameters with Head TSL	
Impedance, transformed to feed point	47.9 Ω ± 1.5 Ω
Return Loss	-31.4 dB
Additional EUT Data	
Manufactured by	SPLEAG

Certificate No: CLA150-4025_Apr21	
Page 3 of 6	Page 4 of 6




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn

t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

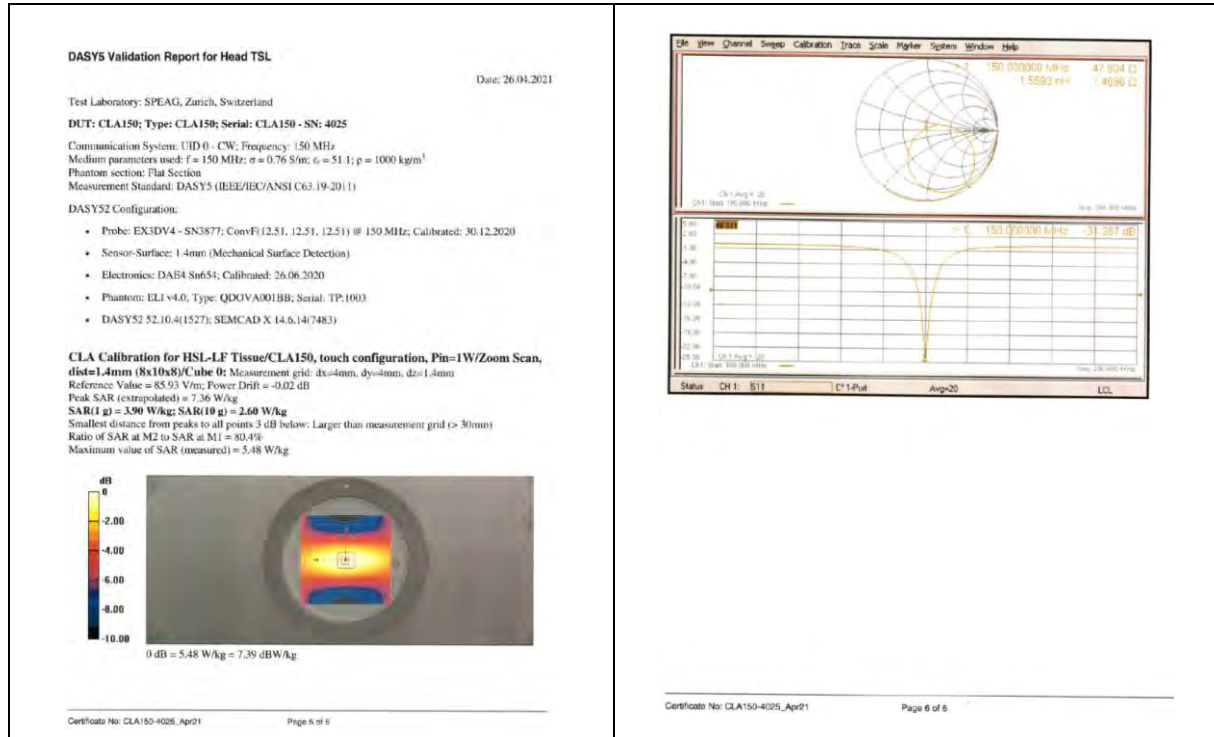

1.2 D450V3 - SN 1103

Calibration Laboratory of Schmid & Partner Engineering AG
Zugstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aiden)** Certificate No: **D450V3-1103_Apr21**

CALIBRATION CERTIFICATE

Object: **D450V3 - SN: 1103**

Calibration procedure(s): **QA CAL-15-V9**
Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 2) °C and humidity < 75%.

Calibration Equipment used (MTE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN 104779	09-Apr-21 (No. 217-030110300)	Apr-22
Power sensor MHP-291	SN 103344	09-Apr-21 (No. 217-03011)	Apr-22
Power sensor MHP-291	SN 103345	09-Apr-21 (No. 217-03015)	Apr-22
Reference 20 dB Attenuator	SN C2552 (200)	09-Apr-21 (No. 217-03049)	Apr-22
Type-N measurement connection	SN 310822 / 06327	09-Apr-21 (No. 217-03044)	Apr-22
Reference Probe EX3DV4	SN 3877	30-Dec-20 (No. EX3-2077 Dec20)	Dec-21
DA54	SN 454	06-Jun-20 (No. DA54-664-Jun20)	Jun-21

Secondary Standards

ID #	Cal Date (In House)	Scheduled Check
Power meter E41188	06-Apr-19 (In house check Jun-20)	In house check Jun-20
Power sensor E4112A	06-Apr-19 (In house check Jun-20)	In house check Jun-20
Power sensor E4112A	06-Apr-19 (In house check Jun-20)	In house check Jun-20
RF generator HP 8440C	06-Aug-19 (In house check Jun-20)	In house check Jun-20
Network Analyzer Agilent E8358A	31-Mar-14 (In house check Dec-20)	In house check Oct-21

Calibrated by: **Kuba Fomke** Function: **Laboratory Technician**

Approved by: **Kuba Fomke** Technical Manager

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D450V3-1103_Apr21 Page 1 of 6

Calibration Laboratory of Schmid & Partner Engineering AG
Zugstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aiden)** Certificate No: **D450V3-1103_Apr21**

Glossary:

TSL: Issue simulating liquid sensitivity in TSL / NORM x,y,z

ConvF: not applicable or not measured

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC 61010-1:2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300

中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn

t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Measurement Conditions		
DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V82.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELJ Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters			
The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.57 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	43.1 ± 6 %	0.07 mho/m ± 8 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL		
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.55 W/kg ± 18.1 % (k=2)

SAR result with Head TSL		
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	0.757 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg ± 17.6 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)		
Antenna Parameters with Head TSL		
Impedance, transformed to feed point	57.1 Ω - j2.8 jΩ	
Return Loss	-23.0 dB	

General Antenna Parameters and Design	
Electrical Delay (one direction)	1.346 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data	
Manufactured by	SPEAG

Certificate No: D450V3-1103_Apr21		
Page 3 of 6		

Certificate No: D450V3-1103_Apr21		
Page 4 of 6		

DASY5 Validation Report for Head TSL		
Test Laboratory: SPEAG, Zurich, Switzerland		
DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103		
Communication System: UTD 0 - CW; Frequency: 450 MHz		
Medium parameters used: f = 450 MHz, α = 0.87 S/m; ε _r = 43.1; ρ = 1000 kg/m ³		
Phantom section: Flat Section		
Measurement Standard: DASY5 (IEC/IEC/ANSI C63.19-2011)		
DASY52 Configuration:		
- Probe: EX3DV4 - SN3877; ConvF [10.64, 10.64] @ 450 MHz; Calibrated: 30.12.2020 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DAE4 Sn654; Calibrated: 26.06.2020 - Phantom: ELJ v4.0; Type: QDOVA001BB; Serial: TP:1003 - DASY52 52.10.4 (1527); SEMCAD X (4.6.14/7483)		
Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:		
Measurement grid: dx=5mm, dy=5mm, dz=5mm		
Reference Value = 39.18 V/m; Power Dfitt = -0.08 dB		
Peak SAR (extrapolated) = 1.76 W/kg		
SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.767 W/kg		
Smallest distance from peaks to all points 3 dB below: Larger than measurement grid		
Ratio of SAR at M2 to SAR at M1 = 64.9%		
Maximum value of SAR (measured) = 1.53 W/kg		

Certificate No: D450V3-1103_Apr21		
Page 5 of 6		

Certificate No: D450V3-1103_Apr21		
Page 6 of 6		



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.3 D750V3 - SN 1188

TTL Speag CALIBRATION LABORATORY		CAICT																					
Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191 Tel: +86-10-4239613-2172 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com		Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191 Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com																					
Client: SGS-CN		Certificate No: Z22-60103																					
CALIBRATION CERTIFICATE																							
Object: D750V3 - SN: 1188																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 28, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility; environment temperature (22±3)°C and humidity <70%.																							
Calibration Equipment used (M&TE critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>104277</td><td>24-Sep-21 (CTTL No.J21X08328)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP88</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08328)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX30V4</td><td>SN 7307</td><td>26-May-21 (SPEAG No.EX3-7307_May21)</td><td>May-22</td></tr><tr><td>DAE4</td><td>SN 1556</td><td>12-Jan-22 (CTTL-SPEAG No.Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	104277	24-Sep-21 (CTTL No.J21X08328)	Sep-22	Power sensor NRP88	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22	Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	104277	24-Sep-21 (CTTL No.J21X08328)	Sep-22																				
Power sensor NRP88	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22																				
Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22																				
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator S4436C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.J22X00406)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY46110673</td><td>14-Jan-22 (CTTL No.J22X00406)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator S4436C	MY48071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator S4436C	MY48071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23																				
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23																				
Calibrated by: Zhao Jing SAR Test Engineer		Signature: [Signature]																					
Reviewed by: Lin Hao SAR Test Engineer		Signature: [Signature]																					
Approved by: Qi Dianyun SAR Project Leader		Signature: [Signature]																					
Issued: April 3, 2022																							
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-60103		Page 1 of 6																					

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com		Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version		DASY52	
Extrapolation		Advanced Extrapolation	
Phantom		Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL		15 mm with Spacer	
Zoom Scan Resolution		dx, dy, dz = 5 mm	
Frequency		750 MHz ± 1 MHz	
Head TSL parameters The following parameters and calculations were applied:			
Temperature		22.0 °C	
Permittivity		42.0	
Conductivity		0.90 mho/m	
Nominal Head TSL parameters		(22.0 ± 0.2) °C	
Measured Head TSL parameters		(22.0 ± 0.2) °C	
Head TSL temperature change during test		<1.0 °C	
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL		Condition	
SAR measured		250 mW input power	
SAR for nominal Head TSL parameters		normalized to 1W	
SAR averaged over 10 cm ² (10 g) of Head TSL		Condition	
SAR measured		250 mW input power	
SAR for nominal Head TSL parameters		normalized to 1W	


TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com		Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point		53.60- 1.13jΩ	
Return Loss		>28.7dB	
General Antenna Parameters and Design			
Electrical Delay (one direction)		0.947 ns	
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when placed according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by		SPEAG	
Certificate No: Z22-60103		Page 1 of 6	



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

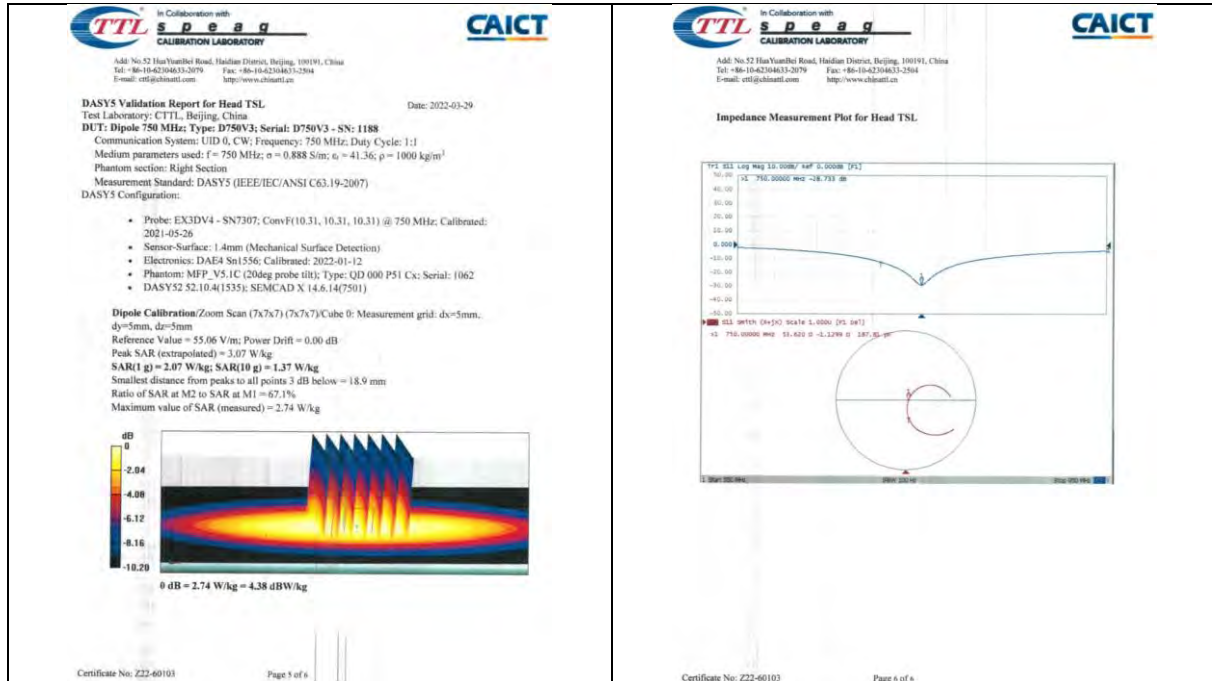

1.4 D835V2 - SN 4d114

TTL Speaq In Collaboration with **CAICT**
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@chinaul.com.cn http://www.chinaul.com

Client: **SGS-CN** Certificate No: **Z22-60104**

CALIBRATION CERTIFICATE

Object: **D835V2 - SN: 4d114**

Calibration Procedure(s): **FF-211-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No J21X08326)	Sep-22
Power sensor NRPBS	104281	24-Sep-21 (CTTL No J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No J22X00409)	Jan-23
Network Analyzer E5071C	MY46110873	14-Jan-22 (CTTL No J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer

Reviewed by: **Lin Hao** SAR Test Engineer

Approved by: **Qi Dianyuan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: Z22-60104 Page 1 of 6

TTL Speaq In Collaboration with **CAICT**
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@chinaul.com.cn http://www.chinaul.com

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 668664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the space to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60104 Page 2 of 6




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com			
Measurement Conditions DASY system configuration, as far as not given on page 1			
DASY Version	DASY52	VS2 10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	835 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	41.5	0.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 0.5	0.81 mho/m ± 0.5%
Head TSL temperature change during last	< 1.0 °C	—	—
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.37 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	9.40 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.54 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60104 Page 1 of 6			

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com			
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.70 - j2.22Ω		
Return Loss	-25.3dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.307 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60104 Page 1 of 6			

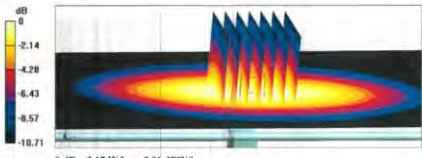In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com			
DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-03-31			
DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 40114 Communication System: UTD 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz; σ = 0.907 S/m; ε _r = 40.98; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:			
- Probe: EX3DV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2021-05-26 - Sensor Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA64 Sn1556; Calibrated: 2022-01-12 - Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(153); SEMCAD X 14.6.14(7501)			
Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.88 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 3.56 W/kg SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg Smallest distance from peaks to all points 3 dB below = 15.8 mm Ratio of SAR at M2 to SAR at M1 = 66.2% Maximum value of SAR (measured) = 3.17 W/kg			
			
Certificate No: Z22-60104 Page 1 of 6			

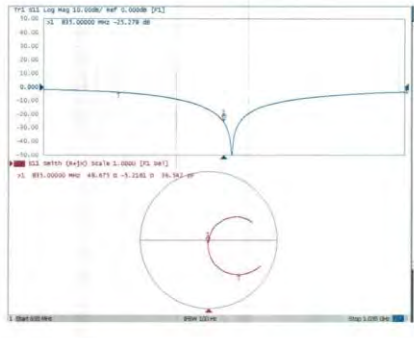In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com			
Impedance Measurement Plot for Head TSL			
			
Certificate No: Z22-60104 Page 6 of 6			



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.5 D900V2 - SN 1d079

TTL In Collaboration with SPS CALIBRATION LABORATORY Address: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42346323-117 E-mail: cti@sgs.com.cn Client: SGS-CN Certificate No: Z22-60184 CALIBRATION CERTIFICATE Object: D900V2 - SN: 1d079 Calibration Procedure(s): PF-Z11-003-01 Calibration Procedures for dipole validation kits Calibration date: June 7, 2022 The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility, environment temperature (23±1°C) and humidity <70%. Calibration Equipment used (MATE critical for calibration) <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter: NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor: NRP85</td> <td>104291</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe: EX32V4</td> <td>SN 7484</td> <td>26-Jan-22 (SPEAG No. EX3-7484_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1586</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator: E2438C</td> <td>MY48071430</td> <td>13-Jan-22 (CTTL No. J22X00406)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer: E5071C</td> <td>MY48110473</td> <td>14-Jan-22 (CTTL No. J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> Calibrated by: Zhao Jing SAR Test Engineer Reviewed by: Lin Hao SAR Test Engineer Approved by: Qi Dianyan SAR Project Leader Issued: June 13, 2022 This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Certificate No: Z22-60184 Page 1 of 4	Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter: NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Power sensor: NRP85	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Reference Probe: EX32V4	SN 7484	26-Jan-22 (SPEAG No. EX3-7484_Jan22)	Jan-23	DAE4	SN 1586	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator: E2438C	MY48071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23	Network Analyzer: E5071C	MY48110473	14-Jan-22 (CTTL No. J22X00406)	Jan-23	TTL In Collaboration with SPS CALIBRATION LABORATORY Address: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42346323-117 E-mail: cti@sgs.com.cn Glossary: TSL: Issue simulating liquid ConvF: sensitivity in TSL / NORM.y,z NVA: not applicable or not measured Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" Additional Documentation: c) DASYS45 System Handbook Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. Certificate No: Z22-60184 Page 1 of 4																																		
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																																
Power Meter: NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																																
Power sensor: NRP85	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																																
Reference Probe: EX32V4	SN 7484	26-Jan-22 (SPEAG No. EX3-7484_Jan22)	Jan-23																																																																
DAE4	SN 1586	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23																																																																
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																																
Signal Generator: E2438C	MY48071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23																																																																
Network Analyzer: E5071C	MY48110473	14-Jan-22 (CTTL No. J22X00406)	Jan-23																																																																
TTL In Collaboration with SPS CALIBRATION LABORATORY Address: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42346323-117 E-mail: cti@sgs.com.cn Measurement Conditions DASY system configuration, as far as not given on page 1: <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY2</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Tight Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>0x, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> Head TSL parameters The following parameters and calculations were applied: <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>41.5</td> <td>0.97 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>42.1 ± 6 %</td> <td>0.98 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><+1.0 °C</td> <td>—</td> <td>—</td> </tr> </tbody> </table> SAR result with Head TSL <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.76 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>11.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.75 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>7.09 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> Certificate No: Z22-60184 Page 1 of 4	DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Tight Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	0x, dy, dz = 5 mm		Frequency	900 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 mho/m ± 6 %	Head TSL temperature change during test	<+1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.76 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.75 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)	TTL In Collaboration with SPS CALIBRATION LABORATORY Address: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42346323-117 E-mail: cti@sgs.com.cn Appendix (Additional assessments outside the scope of CNAS L0670) Antenna Parameters with Head TSL <table border="1"> <thead> <tr> <th></th> <th>48 (10-9-450)</th> </tr> </thead> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td></td> </tr> <tr> <td>Return Loss</td> <td>-23.3 dB</td> </tr> </tbody> </table> General Antenna Parameters and Design <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>1.312 ns</th> </tr> </thead> <tbody> <tr> <td></td> <td></td> </tr> </tbody> </table> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard serringid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> <tbody> <tr> <td></td> <td></td> </tr> </tbody> </table> Certificate No: Z22-60184 Page 1 of 6		48 (10-9-450)	Impedance, transformed to feed point		Return Loss	-23.3 dB	Electrical Delay (one direction)	1.312 ns			Manufactured by	SPEAG		
DASY Version	DASY2	52.10.4																																																																	
Extrapolation	Advanced Extrapolation																																																																		
Phantom	Tight Flat Phantom 5.1C																																																																		
Distance Dipole Center - TSL	15 mm	with Spacer																																																																	
Zoom Scan Resolution	0x, dy, dz = 5 mm																																																																		
Frequency	900 MHz ± 1 MHz																																																																		
	Temperature	Permittivity	Conductivity																																																																
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m																																																																
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 mho/m ± 6 %																																																																
Head TSL temperature change during test	<+1.0 °C	—	—																																																																
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																																		
SAR measured	250 mW input power	2.76 W/kg																																																																	
SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)																																																																	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																																		
SAR measured	250 mW input power	1.75 W/kg																																																																	
SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)																																																																	
	48 (10-9-450)																																																																		
Impedance, transformed to feed point																																																																			
Return Loss	-23.3 dB																																																																		
Electrical Delay (one direction)	1.312 ns																																																																		
Manufactured by	SPEAG																																																																		




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgs.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

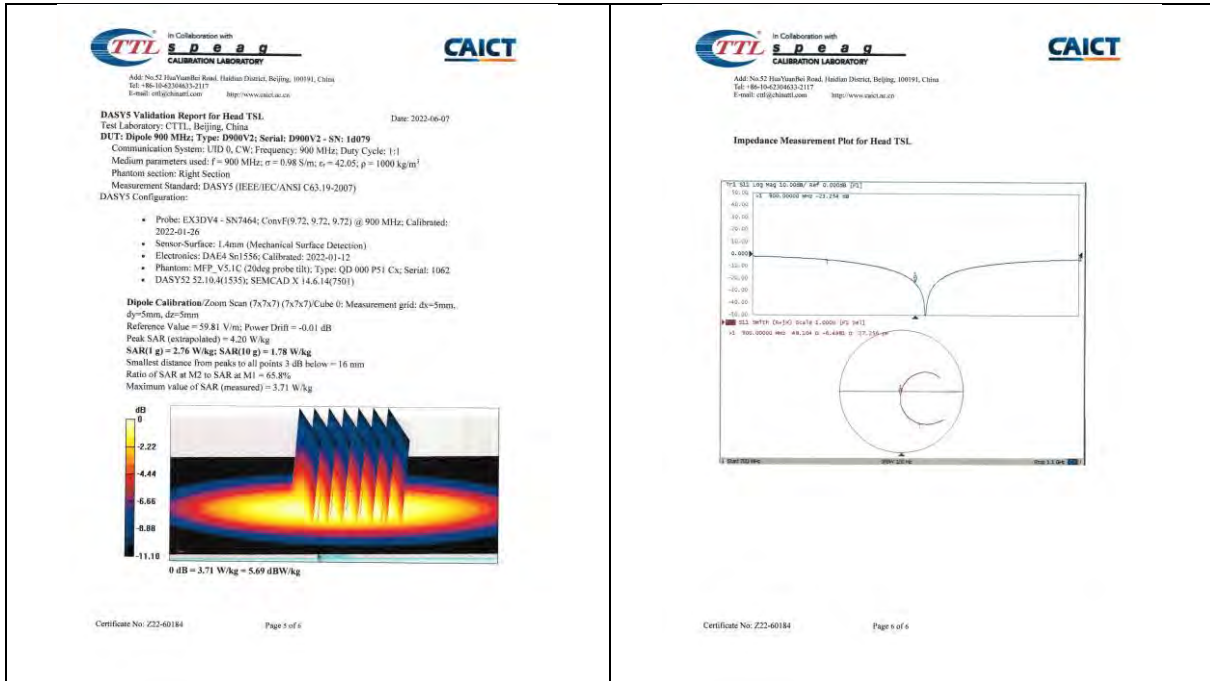

1.6 D1800V2 - SN 2d170

TTL Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117
E-mail: cti@china.ttl.com

CAICT

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Lin Hao** SAR Test Engineer
Approved by: **Qi Diqian** SAR Project Leader

Issued: April 6, 2022
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

TTL Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117
E-mail: cti@china.ttl.com

CAICT

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORM_{x,y,z}
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:
c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

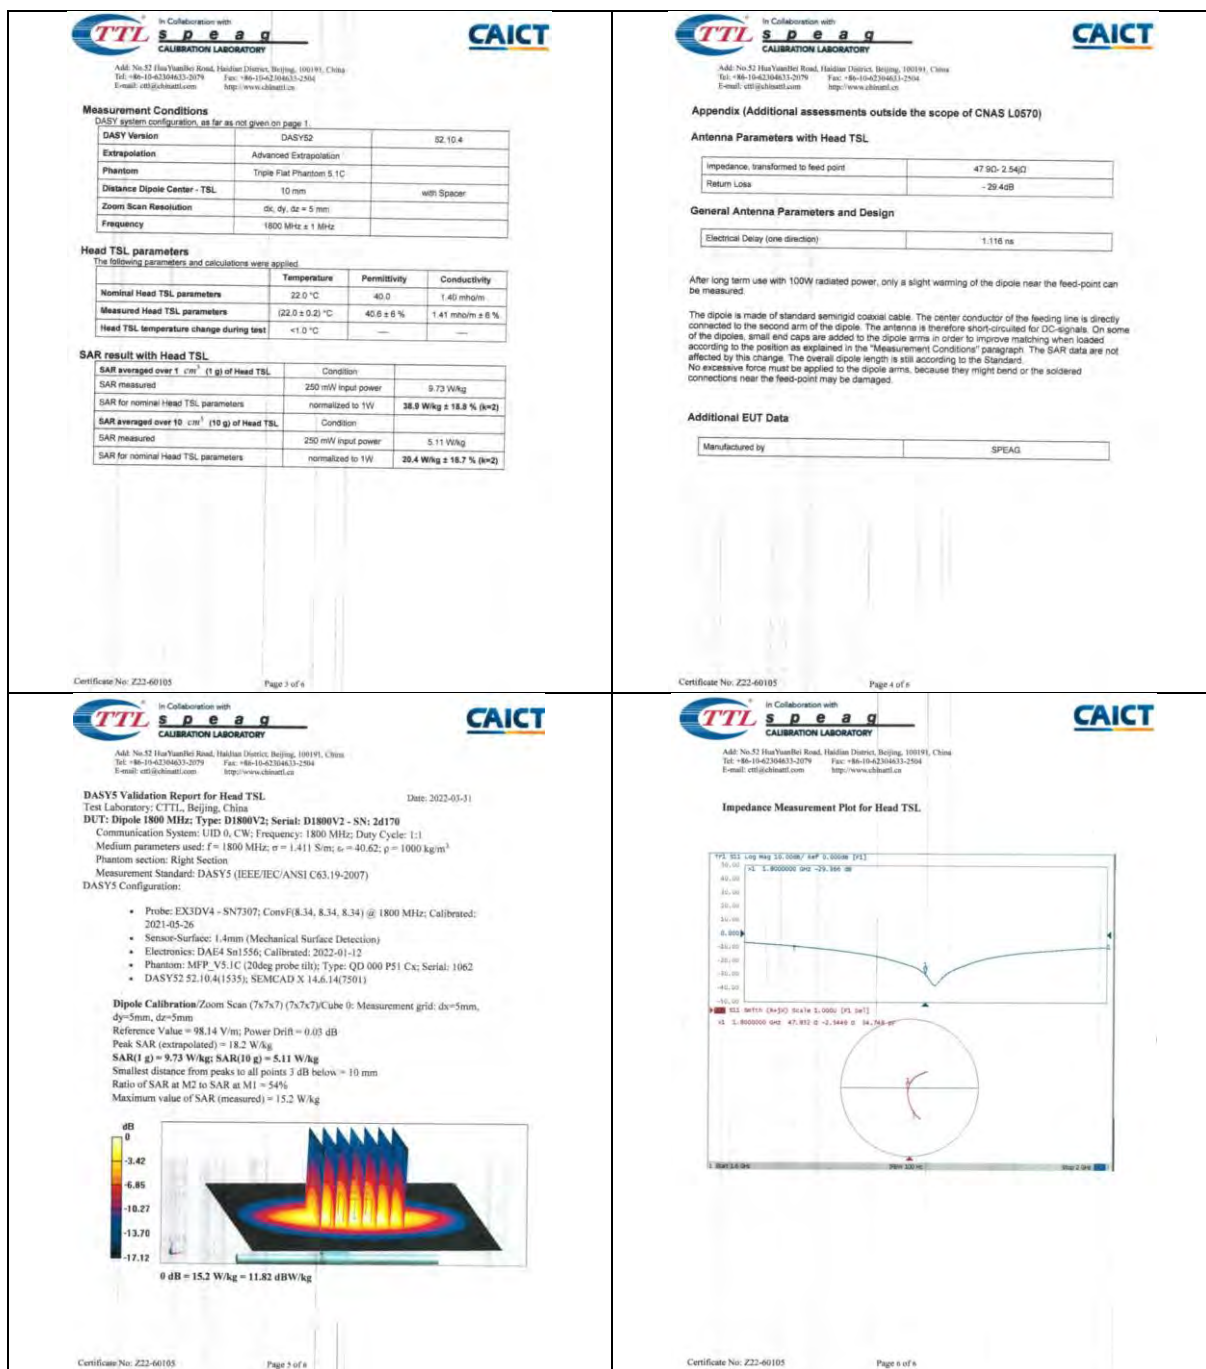

1.7 D1900V2 - SN 5d136

TTL S P E A G CALIBRATION LABORATORY		CAICT																					
Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4226403-2117 E-mail: csl@sgs.com.cn		Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4226403-2117 E-mail: csl@sgs.com.cn																					
Client: SGS-CN		Certificate No: Z22-60185																					
CALIBRATION CERTIFICATE																							
Object: D1900V2 - SN 5d136																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: June 7, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility, environment temperature (23±1)°C and humidity <70%.																							
Calibration Equipment used (M&E critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>106277</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP85</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX3DV4</td><td>SN 7404</td><td>28-Jan-22 (SPEAG No EX3-7404_Jan22)</td><td>Jan-23</td></tr><tr><td>DAEA</td><td>SN 1558</td><td>12-Jan-22 (CTTL-SPEAG No Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7404	28-Jan-22 (SPEAG No EX3-7404_Jan22)	Jan-23	DAEA	SN 1558	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Reference Probe EX3DV4	SN 7404	28-Jan-22 (SPEAG No EX3-7404_Jan22)	Jan-23																				
DAEA	SN 1558	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator E4438C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr><tr><td>Network Analyser E5071C</td><td>MY48110073</td><td>14-Jan-22 (CTTL No.J22X00406)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyser E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00406)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Network Analyser E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00406)	Jan-23																				
Calibrated by: Name: Zhao Jing, Function: SAR Test Engineer, Signature: [Signature]																							
Reviewed by: Lin Hao, SAR Test Engineer, Signature: [Signature]																							
Approved by: Qi Dianyan, SAR Project Leader, Signature: [Signature]																							
Issued: June 13, 2022																							
The calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-60185		Page 1 of 8																					

TTL S P E A G CALIBRATION LABORATORY		CAICT																			
Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4226403-2117 E-mail: csl@sgs.com.cn		Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4226403-2117 E-mail: csl@sgs.com.cn																			
Measurement Conditions QASY system configuration, as far as not given on page 1:																					
<table border="1"><thead><tr><th>DASY Version</th><th>DASY152</th><th>52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>1900 MHz ± 1 MHz</td><td></td></tr></tbody></table>				DASY Version	DASY152	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	1900 MHz ± 1 MHz	
DASY Version	DASY152	52.10.4																			
Extrapolation	Advanced Extrapolation																				
Phantom	Triple Flat Phantom 5.1C																				
Distance Dipole Center - TSL	10 mm	with Spacer																			
Zoom Scan Resolution	dx, dy, dz = 5 mm																				
Frequency	1900 MHz ± 1 MHz																				
Head TSL parameters The following parameters and calculations were applied:																					
<table border="1"><thead><tr><th>Nominal Head TSL parameters</th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td></td><td>22.0 °C</td><td>46.0</td><td>1.40 nS/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.5) °C</td><td>39.9 ± 0.5 %</td><td>1.39 nS/m ± 0.5 %</td></tr><tr><td>Head TSL temperature change during test</td><td>+1.0 °C</td><td></td><td></td></tr></tbody></table>				Nominal Head TSL parameters	Temperature	Permittivity	Conductivity		22.0 °C	46.0	1.40 nS/m	Measured Head TSL parameters	(22.0 ± 0.5) °C	39.9 ± 0.5 %	1.39 nS/m ± 0.5 %	Head TSL temperature change during test	+1.0 °C				
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																		
	22.0 °C	46.0	1.40 nS/m																		
Measured Head TSL parameters	(22.0 ± 0.5) °C	39.9 ± 0.5 %	1.39 nS/m ± 0.5 %																		
Head TSL temperature change during test	+1.0 °C																				
SAR result with Head TSL																					
<table border="1"><thead><tr><th>SAR averaged over 1 cm² (1 g) of Head TSL</th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR measured</td><td>250 mW input power</td><td>9.65 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>40.0 W/kg ± 16.8 % (k=2)</td></tr></tbody></table>				SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		SAR measured	250 mW input power	9.65 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 16.8 % (k=2)									
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition																				
SAR measured	250 mW input power	9.65 W/kg																			
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 16.8 % (k=2)																			
<table border="1"><thead><tr><th>SAR averaged over 10 cm² (10 g) of Head TSL</th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR measured</td><td>250 mW input power</td><td>5.18 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>20.8 W/kg ± 16.7 % (k=2)</td></tr></tbody></table>				SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.18 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 16.7 % (k=2)									
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition																				
SAR measured	250 mW input power	5.18 W/kg																			
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 16.7 % (k=2)																			


TTL S P E A G CALIBRATION LABORATORY		CAICT					
Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4226403-2117 E-mail: csl@sgs.com.cn		Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4226403-2117 E-mail: csl@sgs.com.cn					
Appendix (Additional assessments outside the scope of CNAS L0570)							
Antenna Parameters with Head TSL							
<table border="1"><thead><tr><th>Impedance, transformed to feed point</th><th>51.0Ω ± 1.5Ω(j)</th></tr></thead><tbody><tr><td>Return Loss</td><td>22.4dB</td></tr></tbody></table>				Impedance, transformed to feed point	51.0Ω ± 1.5Ω(j)	Return Loss	22.4dB
Impedance, transformed to feed point	51.0Ω ± 1.5Ω(j)						
Return Loss	22.4dB						
General Antenna Parameters and Design							
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>1.109 ns</th></tr></thead></table>				Electrical Delay (one direction)	1.109 ns		
Electrical Delay (one direction)	1.109 ns						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.							
The dipole is made of standard semirigid coaxial cable. The feeder conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small caps are added to the dipole arms in order to improve matching when loaded according to the position as specified in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.							
Additional EUT Data							
<table border="1"><thead><tr><th>Manufacturer by</th><th>SPEAG</th></tr></thead></table>				Manufacturer by	SPEAG		
Manufacturer by	SPEAG						



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgs.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

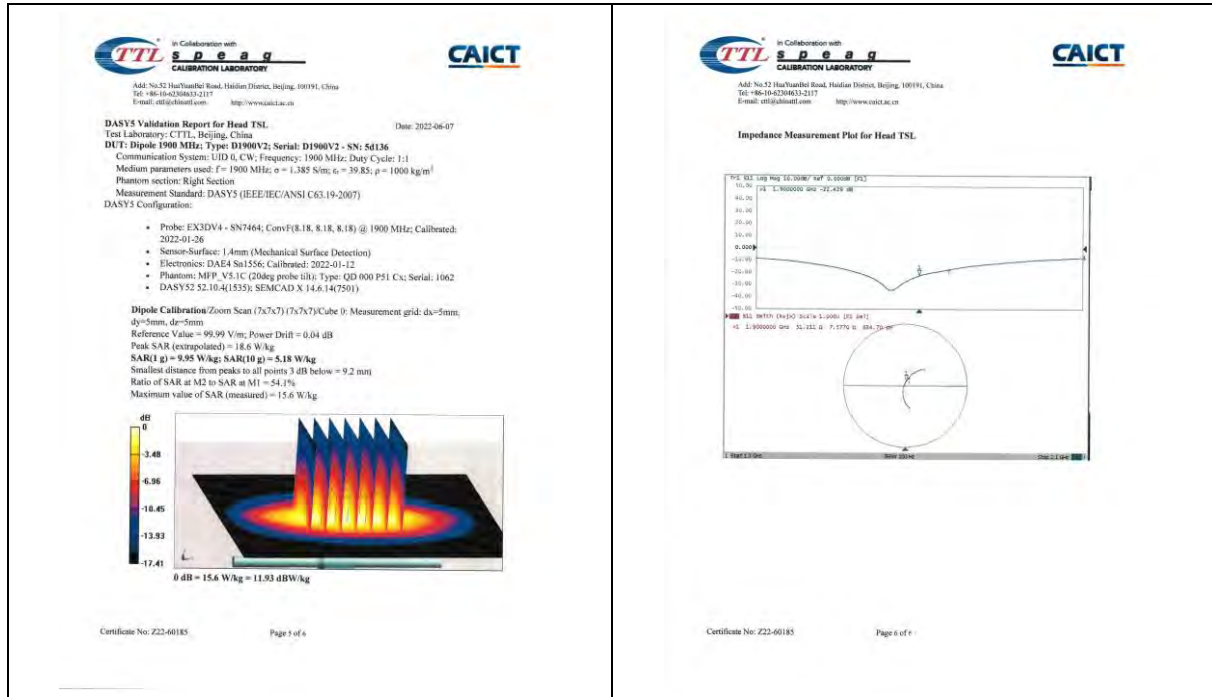

1.8 D2000V2 - SN 1041

Calibration Certificate
 Client: SGS-CN Certificate No: Z22-60186
 Object: D2000V2 - SN 1041
 Calibration Procedure(s): FF-Z11-003-01
 Calibration date: June 5, 2022
 This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.
 All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.
 Calibration Equipment used (MATE critical for calibration):

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08328)	Sep-22
Power sensor NRP5	104291	24-Sep-21 (CTTL No. J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464, Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. Z22X00408)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. Z22X00408)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer
 Reviewed by: Lin Hao SAR Test Engineer
 Approved by: Qi Danyuan SAR Project Leader
 Issued: June 13, 2022
 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Glossary:
 TSL: Issue simulating liquid
 ConvF: sensitivity in TSL / NORMx.y.z
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
 a) IEC/IEEE 62209-1528, Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices: Part 1528 Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz), October 2020
 b) KDB 865564, "SAR Measurement Requirements for 100 MHz to 6 GHz"
 Additional Documentation:
 c) DASY4/S System Handbook

Methods Applied and Interpretation of Parameters:
 • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
 • Antenna Parameter with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
 • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance data is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
 • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
 • SAR measured: SAR measured at the stated antenna input power.
 • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
 • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.



The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

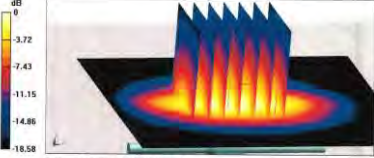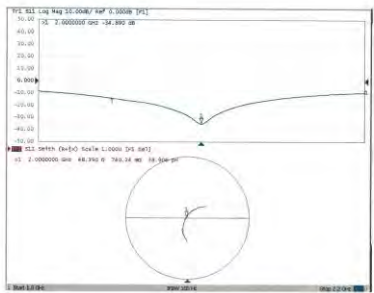In Collaboration with TTL s p e a g CALIBRATION LABORATORY CAICT Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6204832-2117 E-mail: emc@chinaict.com.cn http://www.chinaict.com.cn Measurement Conditions DASY system configuration, as for as not given on page 1. <table border="1"><tr><td>DASY Version</td><td>DASYV2</td><td>52.10.4</td></tr><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom S.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>2000 MHz ± 1 MHz</td><td></td></tr></table> Head TSL parameters The following parameters and calculations were applied: <table border="1"><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr><tr><td>Nominal Head TSL parameters</td><td>22.9 °C</td><td>40.0</td><td>1.40 mho/cm</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>40.2 ± 0.6 %</td><td>1.36 mho/cm ± 0.6 %</td></tr><tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td></td><td></td></tr></table> SAR result with Head TSL <table border="1"><tr><th></th><th>Condition</th><th></th></tr><tr><td>SAR averaged over 1 cm² (1 g) of Head TSL</td><td>250 mW input power</td><td>10.4 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>41.8 W/kg ± 15.8 % (n=2)</td></tr><tr><td>SAR averaged over 10 cm² (10 g) of Head TSL</td><td>Condition</td><td></td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>250 mW input power</td><td>5.30 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>21.3 W/kg ± 18.7 % (n=2)</td></tr></table> Certificate No: Z22-60186 Page 3 of 6	DASY Version	DASYV2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom S.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2000 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.9 °C	40.0	1.40 mho/cm	Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 0.6 %	1.36 mho/cm ± 0.6 %	Head TSL temperature change during test	<1.0 °C				Condition		SAR averaged over 1 cm ² (1 g) of Head TSL	250 mW input power	10.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 15.8 % (n=2)	SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		SAR for nominal Head TSL parameters	250 mW input power	5.30 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)	In Collaboration with TTL s p e a g CALIBRATION LABORATORY CAICT Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6204832-2117 E-mail: emc@chinaict.com.cn http://www.chinaict.com.cn Appendix (Additional assessments outside the scope of CNAS L0570) Antenna Parameters with Head TSL <table border="1"><tr><td>Impedance, transformed to feed point</td><td>48.4Ω ± 0.74Ω</td></tr><tr><td>Return Loss</td><td>-34.8dB</td></tr></table> General Antenna Parameters and Design <table border="1"><tr><td>Electrical Delay (one direction)</td><td>1.08 ns</td></tr></table> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and large are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data <table border="1"><tr><td>Manufactured by</td><td>SPEAG</td></tr></table> Certificate No: Z22-60186 Page 8 of 8	Impedance, transformed to feed point	48.4Ω ± 0.74Ω	Return Loss	-34.8dB	Electrical Delay (one direction)	1.08 ns	Manufactured by	SPEAG
DASY Version	DASYV2	52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom S.1C																																																												
Distance Dipole Center - TSL	10 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	2000 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.9 °C	40.0	1.40 mho/cm																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 0.6 %	1.36 mho/cm ± 0.6 %																																																										
Head TSL temperature change during test	<1.0 °C																																																												
	Condition																																																												
SAR averaged over 1 cm ² (1 g) of Head TSL	250 mW input power	10.4 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 15.8 % (n=2)																																																											
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition																																																												
SAR for nominal Head TSL parameters	250 mW input power	5.30 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)																																																											
Impedance, transformed to feed point	48.4Ω ± 0.74Ω																																																												
Return Loss	-34.8dB																																																												
Electrical Delay (one direction)	1.08 ns																																																												
Manufactured by	SPEAG																																																												
In Collaboration with TTL s p e a g CALIBRATION LABORATORY CAICT Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6204832-2117 E-mail: emc@chinaict.com.cn http://www.chinaict.com.cn DASY Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041 Communication System: UTD 0; CW; Frequency: 2000 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε = 40.21; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7464; ConvF(R2, R2, R2) @ 2000 MHz; Calibrated: 2022-01-26 - Sensor Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA64 Sn1556; Calibrated: 2022-01-12 - Phantom: MPP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY5: S2.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube (0; Measurement grid: dx=5mm, dy=5mm, dz=5mm) Reference Value = 103.4 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 19.6 W/kg SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg Smallest distance from peaks to all points 3 dB below = 9.1 mm Ratio of SAR at M2 to SAR at M1 = 51.0% Maximum value of SAR (measured) = 16.3 W/kg  0 dB = 16.3 W/kg = 12.12 dBW/kg Certificate No: Z22-60186 Page 5 of 6	In Collaboration with TTL s p e a g CALIBRATION LABORATORY CAICT Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6204832-2117 E-mail: emc@chinaict.com.cn http://www.chinaict.com.cn Impedance Measurement Plot for Head TSL  Certificate No: Z22-60186 Page 6 of 6																																																												



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No. 10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgs.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

1.9 D2300V2 - SN 1096

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2512 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Client: SGS-CN		Certificate No: Z22-60106	
CALIBRATION CERTIFICATE			
Object	D2300V2 - SN 1096		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX330V4	SN 7307	26-May-21 (SPEAG No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory			
Certificate No: Z22-60106		Page 1 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2300 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 9 %	1.70 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	—	
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	12.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.88 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60106		Page 3 of 6	


TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.20 - 4.50j		
Return Loss	-26.6dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.083 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when backed according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60106		Page 4 of 6	



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

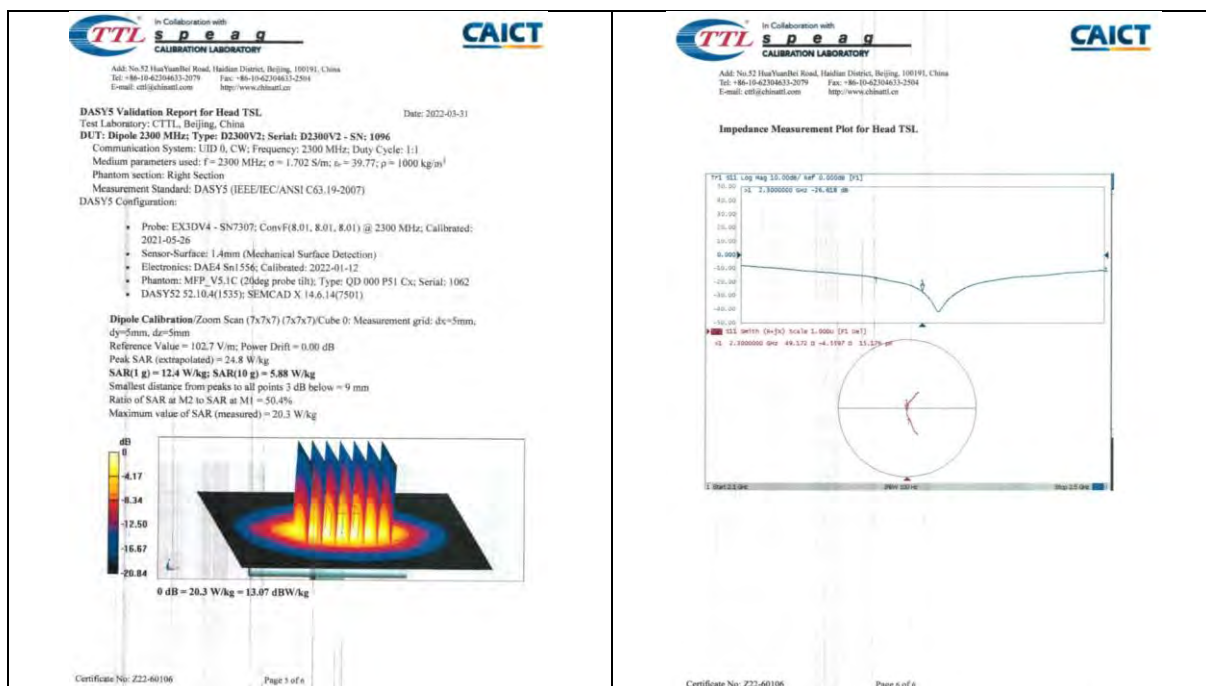

1.10 D2450V2 - SN 817

TTL Speaq
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-3079 Fax: +86-10-62504633-2504
E-mail: csl@china.ttl.com http://www.china.ttl.com

CAICT

Client: **SGS-CN** Certificate No: **Z22-60107**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN 817**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **April 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements [B]. The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor: NRP8S	104291	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe EX3DV4	SN 7307	25-May-21(SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1555	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Liu Hao** SAR Test Engineer
Approved by: **Qi Dianyan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 5

TTL Speaq
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-3079 Fax: +86-10-62504633-2504
E-mail: csl@china.ttl.com http://www.china.ttl.com

CAICT

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMix.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 5 GHz"

Additional Documentation:
c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor: $k=2$, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 5





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

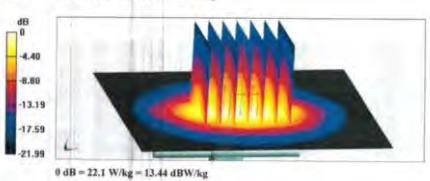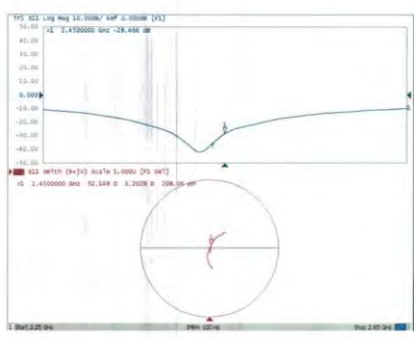TTL Speaq CALIBRATION LABORATORY		CAICT	
In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaul.com.cn http://www.chinaul.com.cn			
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2450 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 8 %
Head TSL temperature change during test	+1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	13.2 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	6.15 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-40107 Page 3 of 6			
TTL Speaq CALIBRATION LABORATORY		CAICT	
In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaul.com.cn http://www.chinaul.com.cn			
DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-04-01 DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; σ = 1.79 S/m; ε = 39.52; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7307; ConvF(7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA14 Snt1556; Calibrated: 2022-01-12 - Phantom: MFP, V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 104.6 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 27.0 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg Smallest distance from peaks to all points 3 dB below = 8.9 mm Ratio of SAR at M2 to SAR at M1 = -49.2% Maximum value of SAR (measured) = 22.1 W/kg			
			
Certificate No: Z22-40107 Page 4 of 6			
TTL Speaq CALIBRATION LABORATORY		CAICT	
In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaul.com.cn http://www.chinaul.com.cn			
Impedance Measurement Plot for Head TSL			
			
Certificate No: Z22-40107 Page 5 of 6			



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.11 D2600V2 - SN 1158

TTL S p e a g CALIBRATION LABORATORY		CAICT																					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.cn																					
Client: SGS-CN		Certificate No: Z22-40108																					
CALIBRATION CERTIFICATE																							
Object: D2600V2 - SN: 1158																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 31, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.																							
Calibration Equipment used (MSTE critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>102377</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP8S</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX30V4</td><td>SN 7307</td><td>26-May-21 (SPEAG No EX3-7307_May21)</td><td>May-22</td></tr><tr><td>DAE4</td><td>SN 1556</td><td>12-Jan-22 (CTTL-SPEAG No Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	102377	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	102377	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22																				
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator E5438C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.Z22X00406)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY48110673</td><td>14-Jan-22 (CTTL No.Z22X00406)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E5438C	MY48071430	13-Jan-22 (CTTL No.Z22X00406)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X00406)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator E5438C	MY48071430	13-Jan-22 (CTTL No.Z22X00406)	Jan-23																				
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X00406)	Jan-23																				
<table border="1"><thead><tr><th>Calibrated by:</th><th>Name</th><th>Function</th><th>Signature</th></tr></thead><tbody><tr><td></td><td>Zhao Jing</td><td>SAR Test Engineer</td><td></td></tr><tr><td>Reviewed by:</td><td>Lin Hao</td><td>SAR Test Engineer</td><td></td></tr><tr><td>Approved by:</td><td>Qi Dianyan</td><td>SAR Project Leader</td><td></td></tr></tbody></table>				Calibrated by:	Name	Function	Signature		Zhao Jing	SAR Test Engineer		Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Dianyan	SAR Project Leader					
Calibrated by:	Name	Function	Signature																				
	Zhao Jing	SAR Test Engineer																					
Reviewed by:	Lin Hao	SAR Test Engineer																					
Approved by:	Qi Dianyan	SAR Project Leader																					
Issued: April 6, 2022																							
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-40108		Page 1 of 6																					

TTL S p e a g CALIBRATION LABORATORY		CAICT																						
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.cn																						
In Collaboration with		In Collaboration with																						
CALIBRATION LABORATORY		CALIBRATION LABORATORY																						
CAICT		CAICT																						
Measurement Conditions DASY system configuration, as far as not given on page 1:																								
<table border="1"><thead><tr><th>DASY Version</th><th>DASY52</th><th>52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>2600 MHz ± 1 MHz</td><td></td></tr></tbody></table>				DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2600 MHz ± 1 MHz				
DASY Version	DASY52	52.10.4																						
Extrapolation	Advanced Extrapolation																							
Phantom	Triple Flat Phantom 5.1C																							
Distance Dipole Center - TSL	10 mm	with Spacer																						
Zoom Scan Resolution	dx, dy, dz = 5 mm																							
Frequency	2600 MHz ± 1 MHz																							
Head TSL parameters The following parameters and calculations were applied:																								
<table border="1"><thead><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>38.0</td><td>1.96 mho/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>38.7 ± 6 %</td><td>1.96 mho/m ± 6 %</td></tr><tr><td>Head TSL temperature change during test</td><td>±1.0 °C</td><td>—</td><td>—</td></tr></tbody></table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	38.0	1.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 6 %	Head TSL temperature change during test	±1.0 °C	—	—					
	Temperature	Permittivity	Conductivity																					
Nominal Head TSL parameters	22.0 °C	38.0	1.96 mho/m																					
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 6 %																					
Head TSL temperature change during test	±1.0 °C	—	—																					
SAR result with Head TSL																								
<table border="1"><thead><tr><th></th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR averaged over 1 cm² (1 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>13.7 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>54.8 W/kg ± 18.8 % (k=2)</td></tr><tr><td>SAR averaged over 10 cm² (10 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>6.12 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>24.5 W/kg ± 18.7 % (k=2)</td></tr></tbody></table>					Condition		SAR averaged over 1 cm ² (1 g) of Head TSL			SAR measured	250 mW input power	13.7 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL			SAR measured	250 mW input power	6.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)
	Condition																							
SAR averaged over 1 cm ² (1 g) of Head TSL																								
SAR measured	250 mW input power	13.7 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)																						
SAR averaged over 10 cm ² (10 g) of Head TSL																								
SAR measured	250 mW input power	6.12 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)																						

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.cn	
In Collaboration with		In Collaboration with	
CALIBRATION LABORATORY		CALIBRATION LABORATORY	
CAICT		CAICT	
Glossary: TSL tissue simulating liquid ConvF sensitivity in TSL / NORMx.y.z N/A not applicable or not measured			
Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 665864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation: c) DASY4/S System Handbook			
Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • MY for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-40108		Page 2 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.cn					
In Collaboration with		In Collaboration with					
CALIBRATION LABORATORY		CALIBRATION LABORATORY					
CAICT		CAICT					
Appendix (Additional assessments outside the scope of CNAS L0570)							
Antenna Parameters with Head TSL							
<table border="1"><thead><tr><th>Impedance, transformed to feed point</th><th>49.90 - j6.49Ω</th></tr></thead><tbody><tr><td>Return Loss</td><td>-23.9dB</td></tr></tbody></table>				Impedance, transformed to feed point	49.90 - j6.49Ω	Return Loss	-23.9dB
Impedance, transformed to feed point	49.90 - j6.49Ω						
Return Loss	-23.9dB						
General Antenna Parameters and Design							
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>1.053 ns</th></tr></thead></table>				Electrical Delay (one direction)	1.053 ns		
Electrical Delay (one direction)	1.053 ns						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.							
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.							
Additional EUT Data							
<table border="1"><thead><tr><th>Manufactured by</th><th>SPEAG</th></tr></thead></table>				Manufactured by	SPEAG		
Manufactured by	SPEAG						
Certificate No: Z22-40108		Page 3 of 6					




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

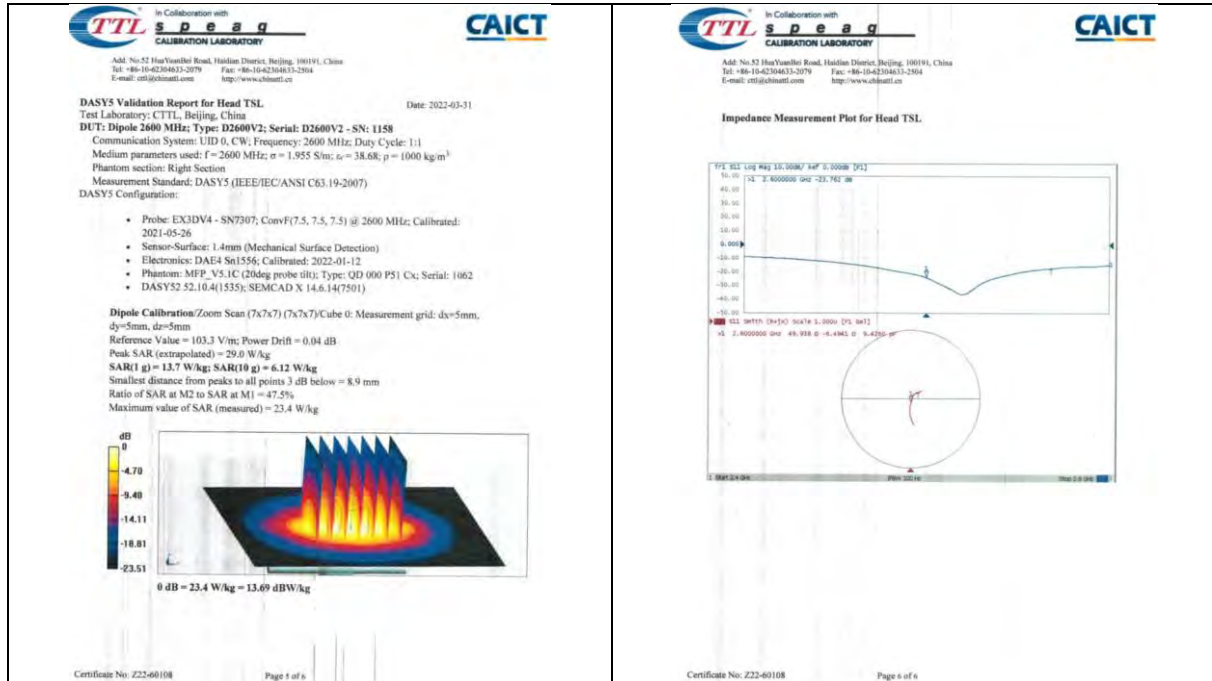

1.12 D5GHZV2 - SN 1095

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@ttspeaq.com http://www.ttspeaq.com

CAICT

Client: SGS-CN Certificate No: Z22-60187

CALIBRATION CERTIFICATE

Object: D5GHZV2 - SN 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kit

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.

Calibration Equipment used (MSTE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CCTL No. J21008328)	Sep-22
Power sensor NRP8	104291	24-Sep-21 (CCTL No. J21008328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464, Jan22)	Jan-23
DA64	SN 1556	12-Jan-22 (CCTL-SPEAG No. Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E438C	MY48071430	13-Jan-22 (CCTL No. J22000409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CCTL No. J22000406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyan SAR Project Leader

Issued: June 9, 2022

This calibration Certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@ttspeaq.com http://www.ttspeaq.com

CAICT

Glossary:

TSL: Issue simulating liquid

CompF: sensitivity in TSL + NORM k₂ z

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance station is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 7 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

TTL Calibration Laboratory		CAICT	
In Collaboration with s p e a g Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62420217 E-mail: info@speag.com http://www.speag.com		In Collaboration with s p e a g Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62420217 E-mail: info@speag.com http://www.speag.com	
Measurement Conditions SAR system configuration, as for as not given on page 1.			
DASY Version	DASY2		52.10.4
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom S.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	
Frequency	500 MHz ± 1 MHz 800 MHz ± 1 MHz 1500 MHz ± 1 MHz 5600 MHz ± 1 MHz		

Head TSL parameters at 5200MHz			
The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 5 %	4.73 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	—	—

SAR result with Head TSL at 5200MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL			
SAR measured	Condition		
SAR for nominal Head TSL parameters	100 mW input power	7.94 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL			
SAR measured	Condition		
SAR for nominal Head TSL parameters	100 mW input power	2.27 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)	

Head TSL parameters at 5500MHz			
The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.8	4.88 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 5 %	4.84 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	—	—

SAR result with Head TSL at 5500MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL			
SAR measured	Condition		
SAR for nominal Head TSL parameters	100 mW input power	8.26 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	82.5 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL			
SAR measured	Condition		
SAR for nominal Head TSL parameters	100 mW input power	2.34 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)	

Certificate No: Z22-60187 Page 4 of 10





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

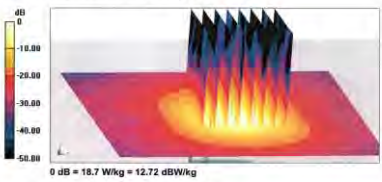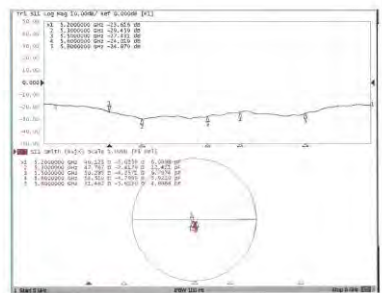TTL In Collaboration with CAICT CALIBRATION LABORATORY Add: No.52 Huayuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@caict.ac.cn http://www.caict.ac.cn General Antenna Parameters and Design Electrical Delay (one direction): 1.021 ns After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semirigid coaxial cable. The carrier conductor of the feeding line is directly connected to the second arm of the dipole. This antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data Manufactured by: SPEAG Certificate No: Z22-60187 Page 1 of 6	TTL In Collaboration with CAICT CALIBRATION LABORATORY Add: No.52 Huayuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@caict.ac.cn http://www.caict.ac.cn DASY5 Validation Report for Head TSL (Date: 2022-09-01) Test Laboratory: CTTL, Beijing, China DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095 Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: $f = 5200$ MHz; $\sigma = 4.82$ S/m; $\epsilon = 35.39$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5300$ MHz; $\sigma = 4.73$ S/m; $\epsilon = 35.19$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5500$ MHz; $\sigma = 4.939$ S/m; $\epsilon = 34.83$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5600$ MHz; $\sigma = 5.051$ S/m; $\epsilon = 34.89$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5800$ MHz; $\sigma = 5.247$ S/m; $\epsilon = 34.42$; $\rho = 1000$ kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C38.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5.5, 5.5, 5.5) @ 5800 MHz; Calibrated: 2022-01-28 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA84 Sn1556; Calibrated: 2022-01-12 - Phantom: MPF_V5.1G (20deg probe kit); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.73 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 19.3 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg Certificate No: Z22-60187 Page 2 of 6
TTL In Collaboration with CAICT CALIBRATION LABORATORY Add: No.52 Huayuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@caict.ac.cn http://www.caict.ac.cn Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.28 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.3 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg  Certificate No: Z22-60187 Page 3 of 6	TTL In Collaboration with CAICT CALIBRATION LABORATORY Add: No.52 Huayuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@caict.ac.cn http://www.caict.ac.cn Impedance Measurement Plot for Head TSL  Certificate No: Z22-60187 Page 4 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

2 DAE4 - SN 1245

Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland Phone +41 (0)43 9702, Fax +41 (0)43 9775 info@sgs.ch, info@sgs.cn s p e a g IMPORTANT NOTICE USAGE OF THE DAE4 The DAE4 unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE4. Special attention shall be given to the following points: Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE4 to wear out. Shipping of the DAE4: Before shipping the DAE4 to SPEAG for calibration, remove the batteries and pack the DAE4 in an anti-static bag. This anti-static bag shall then be packed into a larger box or container which protects the DAE4 from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside. E-stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE4 carefully and keep the DAE4 unit in a non-dusty environment if not used for measurements. Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect. DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file. Important Note: Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer. Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure. Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE. TN_EH190306AE_DAE4.docx 07.03.2019	Calibration Laboratory of Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Client: SGS-CN (Auden) Certificate No.: DAE4-1245_May22 Accreditation No.: SCS 0108 CALIBRATION CERTIFICATE Object: DAE4 - SD 000 D04 BM - SN: 1245 Calibration procedure(s): QA CAL-06 v30 Calibration procedure for the data acquisition electronics (DAE) Calibration date: May 30, 2022 This calibration certificate documents the traceability to national standards, which include the physical units of measurement (SI). The measurement and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 1) °C and humidity < 70%. Calibration Equipment used (MATE critical for calibration) <table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Due Date (Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Kathrein Multimeter Type 2001</td><td>SN: 0810278</td><td>31-Aug-21 (No: 31368)</td><td>Aug-22</td></tr></tbody></table> <table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Check Date (in hours)</th><th>Scheduled Check</th></tr></thead><tbody><tr><td>Auto DAE Calibration Unit</td><td>SE LWS 05A AA 1001</td><td>24-Jan-22 (in hours check)</td><td>In house check: Jan-22</td></tr><tr><td>Calibrator Box V2.1</td><td>SE LWS 00B AA 1002</td><td>24-Jan-22 (in hours check)</td><td>In house check: Jan-22</td></tr></tbody></table> Calibrated by: Dominique Steiner Function: Laboratory Technician Signature: <i>[Signature]</i> Approved by: (Ben Kuhn) Technical Manager Signature: <i>[Signature]</i> This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Certificate No.: DAE4-1245_May22 Page 1 of 5	Primary Standards	ID #	Due Date (Certificate No.)	Scheduled Calibration	Kathrein Multimeter Type 2001	SN: 0810278	31-Aug-21 (No: 31368)	Aug-22	Secondary Standards	ID #	Check Date (in hours)	Scheduled Check	Auto DAE Calibration Unit	SE LWS 05A AA 1001	24-Jan-22 (in hours check)	In house check: Jan-22	Calibrator Box V2.1	SE LWS 00B AA 1002	24-Jan-22 (in hours check)	In house check: Jan-22
Primary Standards	ID #	Due Date (Certificate No.)	Scheduled Calibration																		
Kathrein Multimeter Type 2001	SN: 0810278	31-Aug-21 (No: 31368)	Aug-22																		
Secondary Standards	ID #	Check Date (in hours)	Scheduled Check																		
Auto DAE Calibration Unit	SE LWS 05A AA 1001	24-Jan-22 (in hours check)	In house check: Jan-22																		
Calibrator Box V2.1	SE LWS 00B AA 1002	24-Jan-22 (in hours check)	In house check: Jan-22																		
Calibration Laboratory of Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108 Glossary DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system. Methods Applied and Interpretation of Parameters • DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. • Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. • The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty. • DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. • Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. • Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage. • AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage. • Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. • Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance. • Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement. • Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. • Power consumption: Typical value for information. Supply currents in various operating modes. Certificate No.: DAE4-1245_May22 Page 2 of 5	DC Voltage Measurement AD - Converter Resolution nominal High Range: 1LSB = 6.1 μV, full range = -190...+320 mV Low Range: 1LSB = 61 μV, full range = -1...+32 mV DASY measurement parameters: Auto Zero-Time: 3 sec; Measuring time: 3 sec <table border="1"><thead><tr><th>Calibration Factors</th><th>X</th><th>Y</th><th>Z</th></tr></thead><tbody><tr><td>High Range</td><td>405.265 ± 0.02% (k=2)</td><td>403.974 ± 0.02% (k=2)</td><td>406.092 ± 0.02% (k=2)</td></tr><tr><td>Low Range</td><td>3.99534 ± 1.50% (k=2)</td><td>3.99508 ± 1.50% (k=2)</td><td>4.01015 ± 1.50% (k=2)</td></tr></tbody></table> Connector Angle <table border="1"><thead><tr><th>Connector Angle to be used in DASY system</th><th>30.0° ± 1°</th></tr></thead></table> Certificate No.: DAE4-1245_May22 Page 3 of 5	Calibration Factors	X	Y	Z	High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)	Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)	Connector Angle to be used in DASY system	30.0° ± 1°						
Calibration Factors	X	Y	Z																		
High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)																		
Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)																		
Connector Angle to be used in DASY system	30.0° ± 1°																				



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgsgroup.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	19994.45	1.52	0.00
Channel X + Input	20004.58	2.22	0.01
Channel X - Input	-20001.14	1.12	-0.01
Channel Y + Input	19994.72	1.58	0.00
Channel Y + Input	20001.22	-1.00	-0.00
Channel Y - Input	-20003.05	-1.57	0.01
Channel Z + Input	19992.44	0.19	0.00
Channel Z + Input	20003.09	0.58	0.00
Channel Z - Input	-20001.73	-0.27	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2001.91	0.41	0.02
Channel X + Input	202.54	0.65	0.32
Channel X - Input	-197.86	0.07	-0.04
Channel Y + Input	2002.05	0.58	0.03
Channel Y + Input	201.27	-0.67	-0.28
Channel Y - Input	-196.23	-0.06	0.03
Channel Z + Input	2001.96	0.08	0.00
Channel Z + Input	200.09	-1.03	-0.76
Channel Z - Input	-199.85	-1.57	0.79

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X	200	-5.87	-7.69
	-200	9.12	7.79
Channel Y	200	-8.68	-9.28
	-200	8.52	6.36
Channel Z	200	-5.36	-5.60
	-200	3.58	3.08

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	4.07	-3.14
Channel Y	200	9.36	-	4.07
Channel Z	200	10.11	7.14	-

Certificate No: DAE4-1245_May22

Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15984	17040
Channel Y	16562	16768
Channel Z	16035	15968

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input (mV)	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	1.00	-0.15	1.93	0.45
Channel Y	-0.18	-1.28	0.94	0.45
Channel Z	-0.58	-2.81	0.58	0.60

6. Input Offset Current

Nominal input circuitry offset current on all channels: <25nA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+8	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1245_May22

Page 5 of 5

3 EX3DV4 - SN 7346

Calibration Laboratory of Schmid & Partner Engineering AG
Zürcherstrasse 6, 8004 Zürich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **Auden** Certificate No: **EX3-7346_May22**

Accreditation No.: SCS 0108

Calibration Certificate

Object: **EX3DV4 - SN 7346**

Calibration procedure: **QA CAL-01 vs. QA CAL-14 vs. QA CAL-23 vs. QA CAL-25-V**
Calibration procedure for domestic E-field probes

Calibration date: **March 30, 2022**

This calibration certificate documents the traceability to national standards, which requires the physical units of measurement (SI). The measurement and the uncertainty with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 0.5 °C and humidity < 70%).

Calibration Equipment used (MPE: usual for calibration):

Primary Standards	SI	Cal Date (Certificate No.)	Scheduled Calibration
Power meter M4P	SR 10479	08-Apr-21 (No. 217-0501-0303)	Apr-22
Power sensor HP-291	SR 10304	08-Apr-21 (No. 217-0501-0303)	Apr-22
Power sensor MPT-291	SR 10304	08-Apr-21 (No. 217-0501-0303)	Apr-22
Reference DUT attenuator	SR C2202 (20)	08-Apr-21 (No. 217-0501-0303)	Apr-22
DASA	SR 460	13-Dec-21 (No. DAE4-0453-0401)	Dec-22
Reference Probe (S202)	SR 3013	17-Dec-21 (No. E53-0013-0001)	Dec-22

Secondary Standards

SI	Check Date (in house)	Scheduled Date
Power meter E4419B	08-Apr-21 (in house check Jan-22)	in house check Jan-22
Power sensor E4419A	08-Apr-21 (in house check Jan-22)	in house check Jan-22
Power sensor E4419A	08-Apr-21 (in house check Jan-22)	in house check Jan-22
SR 3001 (100)	08-Apr-21 (in house check Jan-22)	in house check Jan-22
RF generator HP 8446C	08-Apr-21 (in house check Jan-22)	in house check Jan-22
Network Analyzer B 8700A	07-Mar-14 (in house check Dec-20)	in house check Dec-20

Calibrated by: **Heidi** Function: **Calibration Technician** Signature: *[Signature]*

Approved by: **Steven Koller** Deputy Manager Signature: *[Signature]*

This calibration certificate and not the reproduced image of it is valid without approval of the laboratory.

Certificate No: EX3-7346_May22 Page 1 of 24

Calibration Laboratory of Schmid & Partner Engineering AG
Zürcherstrasse 6, 8004 Zürich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **Auden** Certificate No: **EX3-7346_May22**

Accreditation No.: SCS 0108

Glossary:

- TSL: traceability
- NORM.y.z: sensitivity in free space
- DCP: code compression point
- CF: crest factor (10:1, cycle of the RF signal)
- A, B, C, D: modulation dependent measurement parameters
- Polarization: y: rotation around probe axis; z: rotation around axis that is in the plane normal to probe axis (in measurement center); i.e., $\theta = 15^\circ$ normal to probe axis
- Connector Angle: (information used in DASY system to align probe sensor X to the robot coordinate system)

Calibration is Performed According to the Following Standards:

- IEC 61010-1:2011, Measurement Procedure for the Assessment of Specific Absorption Rate (SAR) Exposure to Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices, Part 1: SAR Measurement, Implementation And Procedures (Frequency Range of 4 MHz to 10 GHz); October 2020
- ISO 9001:2015, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM.y.z: Assessed for E-field polarization $\theta = 0^\circ$ (1 = 1000 MHz in TEM-cell; 1 = 1000 MHz R22 waveguide). NORM.y.z are only reference values, i.e., the uncertainties of NORM.y.z does not affect the E-field uncertainty mode TSL (see below Conf).
- NORM(y.z) = NORM.y.z * Frequency response (see Frequency Response Chart). The uncertainty is included in the stated uncertainty of Conf.
- DCP.y.z: DCP is a nominal measurement parameter assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAC: PAC is the Peak to Average Ratio that is not calculated but determined based on the signal characteristics.
- A.y.z, B.y.z, C.y.z, D.y.z, V(y.z), A, B, C, D are numerical measurement parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VRF is the maximum calibration range assessed in RMS voltage across the probe.
- Conf: Conf and Boundary Effect Parameters: Assessed in the probe using E-field (or Temperature Transfer Standard for f < 400 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 400 MHz. The same values are used for assessment of the parameters applied by boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are NORM.y.z * Conf. The uncertainty of NORM.y.z is not given for Conf. A frequency dependent Conf is used in DASY version 4.4 and higher which allows assessing the validity from ≈ 50 MHz to ≈ 100 MHz.
- Sensor geometry (3D resolution from geometry) in a field of low gradients measured using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (see probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information given by determining the NORM(y.z) uncertainty required.

Certificate No: EX3-7346_May22 Page 2 of 24



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgsgroup.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

EX3DV4 - SN:7346										March 30, 2022									
DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346										DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346									
Basic Calibration Parameters										Sensor Model Parameters									
Norm. $\Delta V/V$ (mV/V) ¹										C1 C2 C3 C4 C5 C6 C7 C8 C9 C10 C11 C12 C13 C14 C15 C16									
DOP (mV/V)										ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹ ms.V ¹									
101.4 0.45 0.47 0.61 0.81 1.02 1.16 1.31 1.46 1.61 1.76 1.91 2.06 2.21 2.36 2.51										X 39.2 291.80 35.10 5.63 0.33 5.02 1.42 0.12 1.01 37.1 270.84 34.12 6.29 0.30 5.01 1.82 0.05 1.01 9.7 69.74 33.37 4.96 0.30 4.94 0.61 0.00 1.00									
Calibration Results for Modulation Response										Other Probe Parameters									
UID Communication System Name										Sensor Arrangement									
A B C D E F G H I J K L M N O P Q R S T U V W X Y Z										Triangular									
10000 AAA										Connector Angle (°)									
10000 AAA										-166.1									
10000 AAA										Mechanical Surface Detection Mode									
10000 AAA										enabled									
10000 AAA										Optical Surface Detection Mode									
10000 AAA										disabled									
10000 AAA										Probe Overall Length									
10000 AAA										237 mm									
10000 AAA										Probe Body Diameter									
10000 AAA										10 mm									
10000 AAA										Tip Length									
10000 AAA										9 mm									
10000 AAA										Tip Diameter									
10000 AAA										2.5 mm									
10000 AAA										Probe Tip to Sensor X Calibration Point									
10000 AAA										1 mm									
10000 AAA										Probe Tip to Sensor Y Calibration Point									
10000 AAA										1 mm									
10000 AAA										Probe Tip to Sensor Z Calibration Point									
10000 AAA										1 mm									
10000 AAA										Recommended Measurement Distance from Surface									
10000 AAA										1.4 mm									
Note: For details on UID parameters see Appendix										Note: Measurement distance from surface can be increased to 3.4 mm for an Area Scan job.									
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.																			
1) The uncertainties of Norm. $\Delta V/V$ and DOP are not affected by the field uncertainty within 10% (see Page 2 of 2).																			
2) Humidity measurement parameter, uncertainty not required.																			
3) Uncertainty is determined using the value. (Uncertainty from head response according to the distribution and is determined by the square of the field value).																			
Certificate No: EX3-7346_Mar22										Page 3 of 34									
EX3DV4 - SN:7346										March 30, 2022									
DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346										DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346									
Calibration Parameter Determined in Head Tissue Simulating Media										Calibration Parameter Determined in Head Tissue Simulating Media									
f (MHz) Relative Permittivity ¹ Conductivity (S/m) ² Coref X Coref Y Coref Z Alpha ³ Depth (mm) Unc. (k=2)										f (MHz) Relative Permittivity ¹ Conductivity (S/m) ² Coref X Coref Y Coref Z Alpha ³ Depth (mm) Unc. (k=2)									
750 41.9 0.89 10.56 10.56 10.56 0.55 0.85 ± 12.0 %										6500 34.5 6.07 5.30 5.30 5.30 0.20 2.50 ± 18.0 %									
835 41.5 0.90 10.12 10.12 10.12 0.42 0.96 ± 12.0 %																			
900 41.5 0.97 10.10 10.10 10.10 0.53 0.80 ± 12.0 %																			
1450 40.5 1.20 9.26 9.26 9.26 0.50 0.80 ± 12.0 %																			
1750 40.1 1.37 8.83 8.83 8.83 0.34 0.86 ± 12.0 %																			
1900 40.0 1.40 8.48 8.48 8.48 0.35 0.86 ± 12.0 %																			
2000 40.0 1.40 8.35 8.35 8.35 0.34 0.86 ± 12.0 %																			
2300 39.5 1.67 7.86 7.86 7.86 0.39 0.90 ± 12.0 %																			
2450 39.2 1.80 7.63 7.63 7.63 0.41 0.90 ± 12.0 %																			
2600 39.0 1.96 7.33 7.33 7.33 0.44 0.90 ± 12.0 %																			
3300 38.2 2.71 7.15 7.15 7.15 0.30 1.35 ± 13.1 %																			
3500 37.8 2.81 7.14 7.14 7.14 0.30 1.35 ± 13.1 %																			
3750 37.7 3.12 6.85 6.85 6.85 0.30 1.35 ± 13.1 %																			
3900 37.5 3.32 6.71 6.71 6.71 0.40 1.60 ± 13.1 %																			
4100 37.2 3.53 6.58 6.58 6.58 0.40 1.60 ± 13.1 %																			
4200 37.1 3.63 6.30 6.30 6.30 0.40 1.70 ± 13.1 %																			
4400 36.9 3.84 6.24 6.24 6.24 0.40 1.70 ± 13.1 %																			
4600 36.7 4.04 6.11 6.11 6.11 0.40 1.70 ± 13.1 %																			
4800 36.4 4.25 5.98 5.98 5.98 0.40 1.80 ± 13.1 %																			
4900 36.3 4.40 5.84 5.84 5.84 0.40 1.80 ± 13.1 %																			
5200 36.0 4.66 5.25 5.25 5.25 0.40 1.80 ± 13.1 %																			
5300 35.9 4.78 5.12 5.12 5.12 0.40 1.80 ± 13.1 %																			
5500 35.6 4.96 4.85 4.85 4.85 0.40 1.80 ± 13.1 %																			
5600 35.5 5.07 4.70 4.70 4.70 0.40 1.80 ± 13.1 %																			
5800 35.3 5.27 4.75 4.75 4.75 0.40 1.80 ± 13.1 %																			
1) Frequency validity above 300 MHz is 100 MHz only for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the Coref uncertainty at calibration frequency and the uncertainty for the indicated frequency band.										1) Frequency validity above 6 GHz is 100 MHz. The uncertainty is the RSS of the Coref uncertainty at calibration frequency and the uncertainty for the indicated frequency band.									
2) As frequencies > 30 GHz, the validity of tissue parameters (ρ and σ) can be related to a 10% if liquid compensation formula is applied to measured GHz values. The uncertainty is the RSS of the Coref uncertainty for indicated target tissue parameters.										2) As frequencies > 30 GHz, the validity of tissue parameters (ρ and σ) can be related to a 10% if liquid compensation formula is applied to measured GHz values. The uncertainty is the RSS of the Coref uncertainty for indicated target tissue parameters.									
3) Apparent depth is determined during calibration. SPICAD warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.										3) Apparent depth is determined during calibration. SPICAD warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.									
Certificate No: EX3-7346_Mar22										Page 5 of 24									
EX3DV4 - SN:7346										March 30, 2022									
DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346										DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346									
Calibration Parameter Determined in Head Tissue Simulating Media										Calibration Parameter Determined in Head Tissue Simulating Media									
f (MHz) Relative Permittivity ¹ Conductivity (S/m) ² Coref X Coref Y Coref Z Alpha ³ Depth (mm) Unc. (k=2)										f (MHz) Relative Permittivity ¹ Conductivity (S/m) ² Coref X Coref Y Coref Z Alpha ³ Depth (mm) Unc. (k=2)									
6500 34.5 6.07 5.30 5.30 5.30 0.20 2.50 ± 18.0 %																			
1) Frequency validity above 300 MHz is 100 MHz only for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the Coref uncertainty at calibration frequency and the uncertainty for the indicated frequency band.										1) Frequency validity above 6 GHz is 100 MHz. The uncertainty is the RSS of the Coref uncertainty at calibration frequency and the uncertainty for the indicated frequency band.									
2) As frequencies > 30 GHz, the validity of tissue parameters (ρ and σ) can be related to a 10% if liquid compensation formula is applied to measured GHz values. The uncertainty is the RSS of the Coref uncertainty for indicated target tissue parameters.										2) As frequencies > 30 GHz, the validity of tissue parameters (ρ and σ) can be related to a 10% if liquid compensation formula is applied to measured GHz values. The uncertainty is the RSS of the Coref uncertainty for indicated target tissue parameters.									
3) Apparent depth is determined during calibration. SPICAD warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.										3) Apparent depth is determined during calibration. SPICAD warrants that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.									
Certificate No: EX3-7346_Mar22										Page 6 of 24									




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

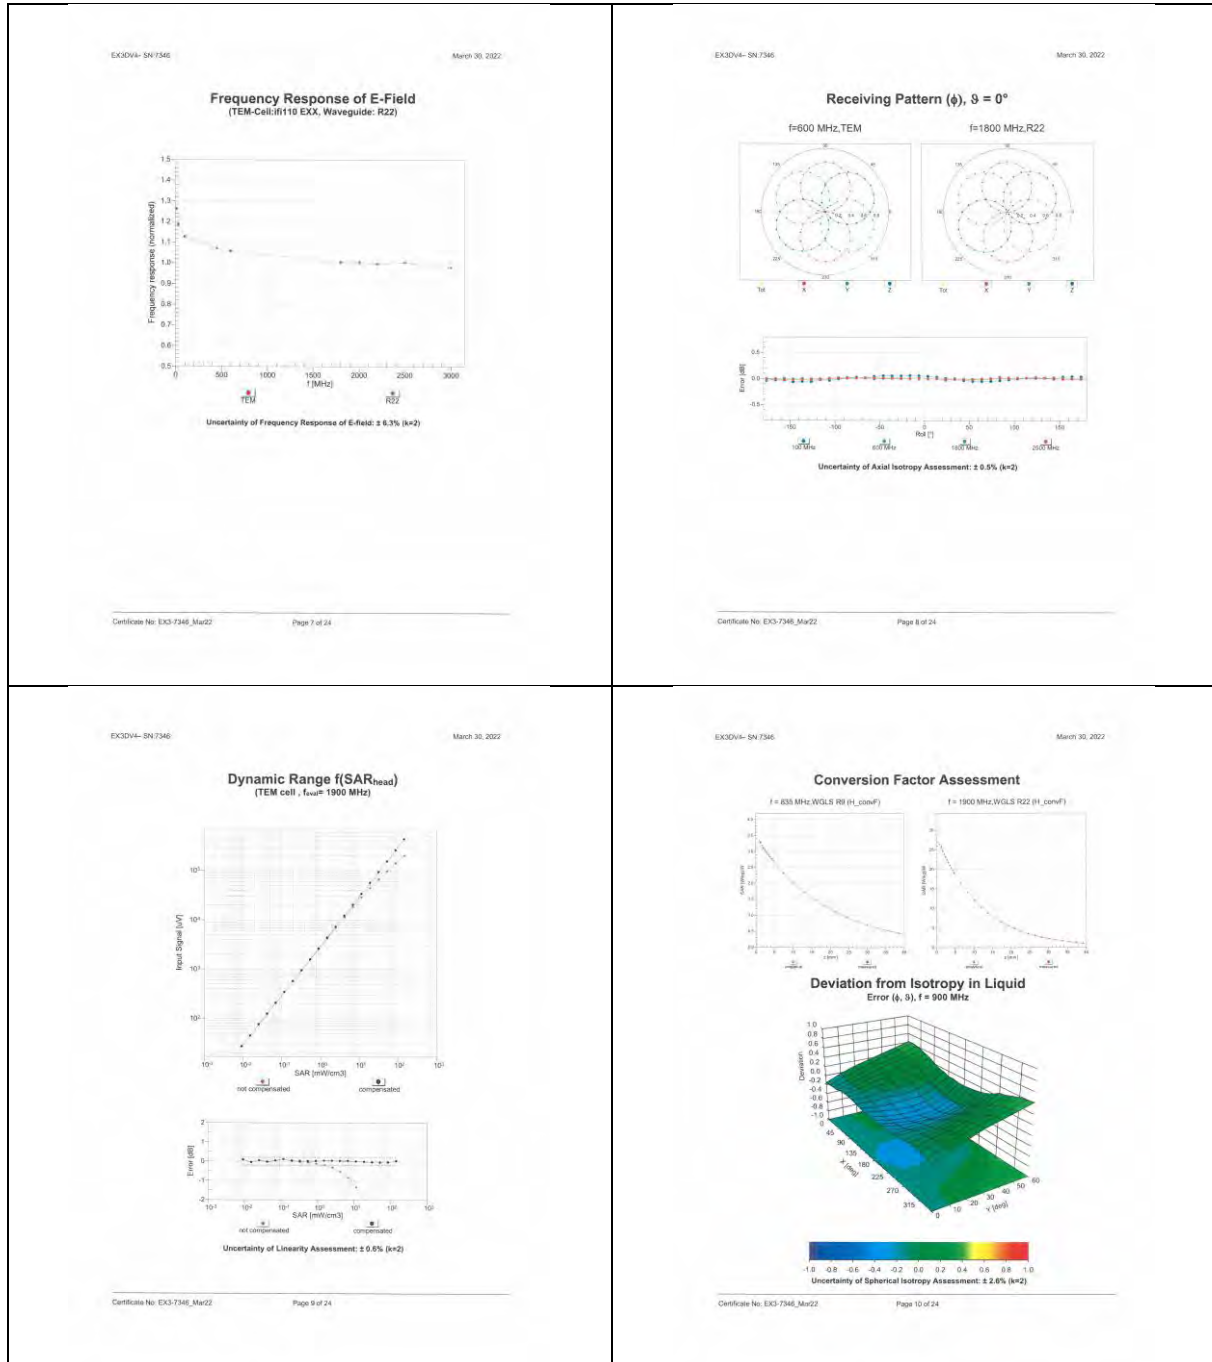

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

EX3034-EN7346										March 30, 2022									
Append: Modulation Calibration Parameters										March 30, 2022									
Uplink	Res	Communication System Name	Stream	PAIR	Mod	PAIR	Mod	PAIR	Mod	Uplink	Res	Communication System Name	Stream	PAIR	Mod	PAIR	Mod	PAIR	Mod
10000	CA	IEEE 802.11n HT Channel 39 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10000	CA	IEEE 802.11n HT Channel 39 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10001	CA	IEEE 802.11n HT Channel 40 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10001	CA	IEEE 802.11n HT Channel 40 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10002	CA	IEEE 802.11n HT Channel 41 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10002	CA	IEEE 802.11n HT Channel 41 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10003	CA	IEEE 802.11n HT Channel 42 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10003	CA	IEEE 802.11n HT Channel 42 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10004	CA	IEEE 802.11n HT Channel 43 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10004	CA	IEEE 802.11n HT Channel 43 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10005	CA	IEEE 802.11n HT Channel 44 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10005	CA	IEEE 802.11n HT Channel 44 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10006	CA	IEEE 802.11n HT Channel 45 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10006	CA	IEEE 802.11n HT Channel 45 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10007	CA	IEEE 802.11n HT Channel 46 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10007	CA	IEEE 802.11n HT Channel 46 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10008	CA	IEEE 802.11n HT Channel 47 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10008	CA	IEEE 802.11n HT Channel 47 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10009	CA	IEEE 802.11n HT Channel 48 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10009	CA	IEEE 802.11n HT Channel 48 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10010	CA	IEEE 802.11n HT Channel 49 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10010	CA	IEEE 802.11n HT Channel 49 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10011	CA	IEEE 802.11n HT Channel 50 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10011	CA	IEEE 802.11n HT Channel 50 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10012	CA	IEEE 802.11n HT Channel 51 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10012	CA	IEEE 802.11n HT Channel 51 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10013	CA	IEEE 802.11n HT Channel 52 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10013	CA	IEEE 802.11n HT Channel 52 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10014	CA	IEEE 802.11n HT Channel 53 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10014	CA	IEEE 802.11n HT Channel 53 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10015	CA	IEEE 802.11n HT Channel 54 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10015	CA	IEEE 802.11n HT Channel 54 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10016	CA	IEEE 802.11n HT Channel 55 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10016	CA	IEEE 802.11n HT Channel 55 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK
10017	CA	IEEE 802.11n HT Channel 56 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK	10017	CA	IEEE 802.11n HT Channel 56 (5MHz)	CA	1.00	QPSK	1.00	QPSK	1.00	QPSK

Member of the SGS Group (SGS SA)

EX3Dv4-SN7346	March 30, 2022	EX3Dv4-SN7346	March 30, 2022
10673 AAC IEEE 802.11ax (20MHz, MCS2, 90deg)	WLAN 8.78 9.96%	10729 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 9.54 9.96%
10674 AAC IEEE 802.11ax (20MHz, MCS3, 90deg)	WLAN 8.74 9.96%	10730 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.87 9.96%
10675 AAC IEEE 802.11ax (20MHz, MCS3, 90deg)	WLAN 8.80 9.96%	10731 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.80 9.96%
10676 AAC IEEE 802.11ax (20MHz, MCS5, 90deg)	WLAN 8.77 9.96%	10732 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%
10677 AAC IEEE 802.11ax (20MHz, MCS6, 90deg)	WLAN 8.73 9.96%	10733 AAC IEEE 802.11ax (20MHz, MCS6, 90deg)	WLAN 8.40 9.96%
10678 AAC IEEE 802.11ax (20MHz, MCS7, 90deg)	WLAN 8.78 9.96%	10734 AAC IEEE 802.11ax (20MHz, MCS7, 90deg)	WLAN 8.23 9.96%
10679 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.89 9.96%	10735 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.73 9.96%
10680 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.80 9.96%	10736 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.23 9.96%
10681 AAC IEEE 802.11ax (20MHz, MCS10, 90deg)	WLAN 8.62 9.96%	10737 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.39 9.96%
10682 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.63 9.96%	10738 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%
10683 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.42 9.96%	10739 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.23 9.96%
10684 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.25 9.96%	10740 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.48 9.96%
10685 AAC IEEE 802.11ax (20MHz, MCS2, 90deg)	WLAN 8.33 9.96%	10741 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.43 9.96%
10686 AAC IEEE 802.11ax (20MHz, MCS3, 90deg)	WLAN 8.28 9.96%	10742 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.43 9.96%
10687 AAC IEEE 802.11ax (20MHz, MCS4, 90deg)	WLAN 8.45 9.96%	10743 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.24 9.96%
10688 AAC IEEE 802.11ax (20MHz, MCS5, 90deg)	WLAN 8.29 9.96%	10744 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%
10689 AAC IEEE 802.11ax (20MHz, MCS6, 90deg)	WLAN 8.55 9.96%	10745 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10690 AAC IEEE 802.11ax (20MHz, MCS7, 90deg)	WLAN 8.29 9.96%	10746 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.71 9.96%
10691 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.25 9.96%	10747 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10692 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.29 9.96%	10748 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10693 AAC IEEE 802.11ax (20MHz, MCS10, 90deg)	WLAN 8.25 9.96%	10749 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.29 9.96%
10694 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.57 9.96%	10750 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.29 9.96%
10695 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.78 9.96%	10751 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10696 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10752 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10697 AAC IEEE 802.11ax (20MHz, MCS2, 90deg)	WLAN 8.63 9.96%	10753 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10698 AAC IEEE 802.11ax (20MHz, MCS3, 90deg)	WLAN 8.89 9.96%	10754 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 9.94 9.96%
10699 AAC IEEE 802.11ax (20MHz, MCS4, 90deg)	WLAN 8.82 9.96%	10755 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.94 9.96%
10700 AAC IEEE 802.11ax (20MHz, MCS5, 90deg)	WLAN 8.73 9.96%	10756 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.77 9.96%
10701 AAC IEEE 802.11ax (20MHz, MCS6, 90deg)	WLAN 8.86 9.96%	10757 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.77 9.96%
10702 AAC IEEE 802.11ax (20MHz, MCS7, 90deg)	WLAN 8.70 9.96%	10758 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.69 9.96%
10703 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.62 9.96%	10759 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.38 9.96%
10704 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.68 9.96%	10760 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%
10705 AAC IEEE 802.11ax (20MHz, MCS10, 90deg)	WLAN 8.69 9.96%	10761 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.28 9.96%
10706 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.68 9.96%	10762 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%
10707 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.32 9.96%	10763 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%
10708 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.55 9.96%	10764 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.54 9.96%
10709 AAC IEEE 802.11ax (20MHz, MCS2, 90deg)	WLAN 8.33 9.96%	10765 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.44 9.96%
10710 AAC IEEE 802.11ax (20MHz, MCS3, 90deg)	WLAN 8.29 9.96%	10766 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10711 AAC IEEE 802.11ax (20MHz, MCS4, 90deg)	WLAN 8.39 9.96%	10767 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10712 AAC IEEE 802.11ax (20MHz, MCS5, 90deg)	WLAN 8.67 9.96%	10768 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10713 AAC IEEE 802.11ax (20MHz, MCS6, 90deg)	WLAN 8.33 9.96%	10769 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10714 AAC IEEE 802.11ax (20MHz, MCS7, 90deg)	WLAN 8.28 9.96%	10770 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10715 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.45 9.96%	10771 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10716 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.30 9.96%	10772 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10717 AAC IEEE 802.11ax (20MHz, MCS10, 90deg)	WLAN 8.48 9.96%	10773 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10718 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.24 9.96%	10774 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10719 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.81 9.96%	10775 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10720 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.87 9.96%	10776 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10721 AAC IEEE 802.11ax (20MHz, MCS10, 90deg)	WLAN 8.78 9.96%	10777 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10722 AAC IEEE 802.11ax (20MHz, MCS3, 90deg)	WLAN 8.55 9.96%	10778 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10723 AAC IEEE 802.11ax (20MHz, MCS4, 90deg)	WLAN 8.70 9.96%	10779 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10724 AAC IEEE 802.11ax (20MHz, MCS5, 90deg)	WLAN 8.90 9.96%	10780 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10725 AAC IEEE 802.11ax (20MHz, MCS6, 90deg)	WLAN 8.74 9.96%	10781 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10726 AAC IEEE 802.11ax (20MHz, MCS7, 90deg)	WLAN 8.72 9.96%	10782 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10727 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.66 9.96%	10783 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10728 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.65 9.96%	10784 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%

Certificate No: EX3-T346-Muz2	Page 19 of 24	TestResult No: EX3-T346-Muz2	Page 19 of 24
EX3Dv4-SN7346	March 30, 2022	EX3Dv4-SN7346	March 30, 2022
10729 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 9.54 9.96%	10729 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 9.54 9.96%
10730 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.87 9.96%	10730 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.87 9.96%
10731 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.80 9.96%	10731 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.80 9.96%
10732 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%	10732 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%
10733 AAC IEEE 802.11ax (20MHz, MCS6, 90deg)	WLAN 8.40 9.96%	10733 AAC IEEE 802.11ax (20MHz, MCS6, 90deg)	WLAN 8.40 9.96%
10734 AAC IEEE 802.11ax (20MHz, MCS7, 90deg)	WLAN 8.23 9.96%	10734 AAC IEEE 802.11ax (20MHz, MCS7, 90deg)	WLAN 8.23 9.96%
10735 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.73 9.96%	10735 AAC IEEE 802.11ax (20MHz, MCS8, 90deg)	WLAN 8.73 9.96%
10736 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.23 9.96%	10736 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.23 9.96%
10737 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.39 9.96%	10737 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.39 9.96%
10738 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%	10738 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%
10739 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.23 9.96%	10739 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.23 9.96%
10740 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.48 9.96%	10740 AAC IEEE 802.11ax (20MHz, MCS9, 90deg)	WLAN 8.48 9.96%
10741 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.43 9.96%	10741 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.43 9.96%
10742 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.43 9.96%	10742 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.43 9.96%
10743 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.24 9.96%	10743 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.24 9.96%
10744 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%	10744 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.40 9.96%
10745 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%	10745 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10746 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.71 9.96%	10746 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.71 9.96%
10747 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%	10747 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10748 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%	10748 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10749 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.29 9.96%	10749 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.29 9.96%
10750 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.29 9.96%	10750 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.29 9.96%
10751 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%	10751 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10752 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10752 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10753 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%	10753 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.93 9.96%
10754 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 9.94 9.96%	10754 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 9.94 9.96%
10755 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.94 9.96%	10755 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.94 9.96%
10756 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.77 9.96%	10756 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.77 9.96%
10757 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.77 9.96%	10757 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.77 9.96%
10758 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.69 9.96%	10758 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.69 9.96%
10759 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.38 9.96%	10759 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.38 9.96%
10760 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%	10760 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%
10761 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.28 9.96%	10761 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.28 9.96%
10762 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%	10762 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%
10763 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%	10763 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.49 9.96%
10764 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.54 9.96%	10764 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.54 9.96%
10765 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.44 9.96%	10765 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.44 9.96%
10766 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10766 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10767 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10767 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10768 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10768 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10769 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10769 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10770 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10770 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10771 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10771 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10772 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10772 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10773 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10773 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10774 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10774 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10775 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10775 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10776 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10776 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10777 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10777 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10778 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10778 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10779 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10779 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10780 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10780 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10781 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10781 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10782 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10782 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10783 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10783 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%
10784 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%	10784 AAC IEEE 802.11ax (20MHz, MCS11, 90deg)	WLAN 8.91 9.96%

EXCIV4-SN 7346 March 30, 2022 15985 AAA 50 NR DL (CP-CFOM, TM 3.1, 40 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.54 ± 9.8 % 15986 AAA 50 NR DL (CP-CFOM, TM 3.1, 50 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.50 ± 9.8 % 15987 AAA 50 NR DL (CP-CFOM, TM 3.1, 60 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.50 ± 9.8 % 15988 AAA 50 NR DL (CP-CFOM, TM 3.1, 70 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.38 ± 9.8 % 15989 AAA 50 NR DL (CP-CFOM, TM 3.1, 80 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.33 ± 9.8 % 15990 AAA 50 NR DL (CP-CFOM, TM 3.1, 90 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.52 ± 9.8 % ¹ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value. Certificate No. EXC-7346_Mar22 Page 24 of 24	EXCIV4-SN 7346 March 30, 2022 15985 AAA 50 NR DL (CP-CFOM, TM 3.1, 40 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.54 ± 9.8 % 15986 AAA 50 NR DL (CP-CFOM, TM 3.1, 50 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.50 ± 9.8 % 15987 AAA 50 NR DL (CP-CFOM, TM 3.1, 60 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.50 ± 9.8 % 15988 AAA 50 NR DL (CP-CFOM, TM 3.1, 70 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.38 ± 9.8 % 15989 AAA 50 NR DL (CP-CFOM, TM 3.1, 80 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.33 ± 9.8 % 15990 AAA 50 NR DL (CP-CFOM, TM 3.1, 90 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.52 ± 9.8 % ¹ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value. Certificate No. EXC-7346_Mar22 Page 24 of 24
--	--

4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/26	-31.4	/	47.8	/
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/21	-23	/	57.1	/



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com