

FCC ID:

Nalu Medical Inc

Section 1. Test Setup Photos

1.1 Radiated emissions test setup

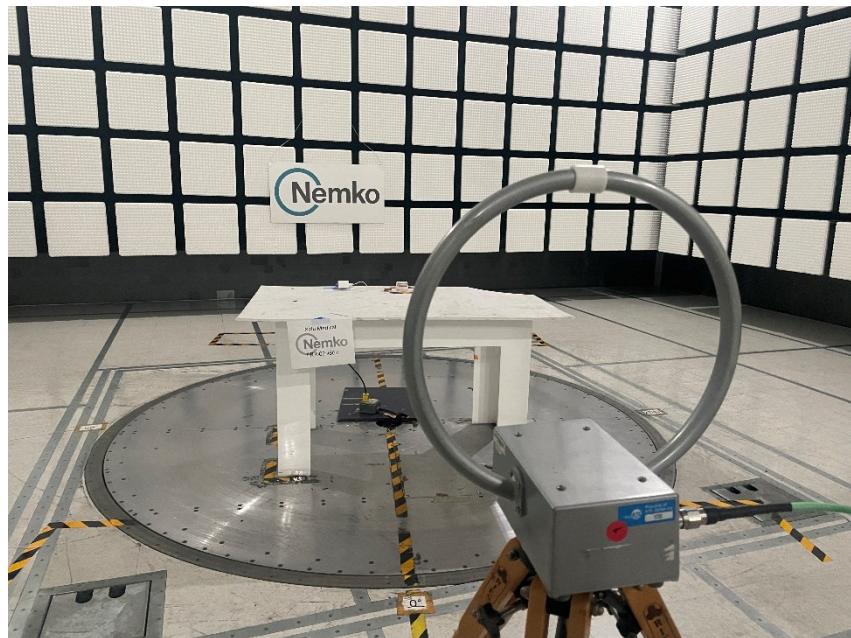


Figure 1 - Radiated emissions below 30 MHz (9 kHz – 30 MHz), 0 Degrees, front view



Figure 2 - Radiated emissions below 30 MHz (9 kHz – 30 MHz), 0 Degrees, rear view

FCC ID:

Nalu Medical Inc

1.2 Radiated emissions test setup, continued

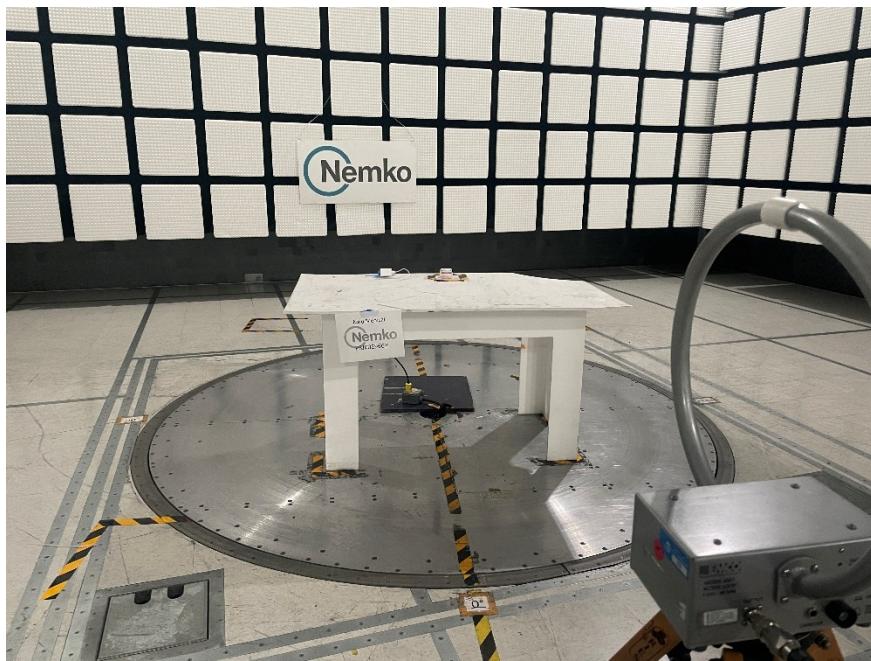


Figure 3 - Radiated emissions below 30 MHz (9 kHz – 30 MHz), 90 Degrees, front view

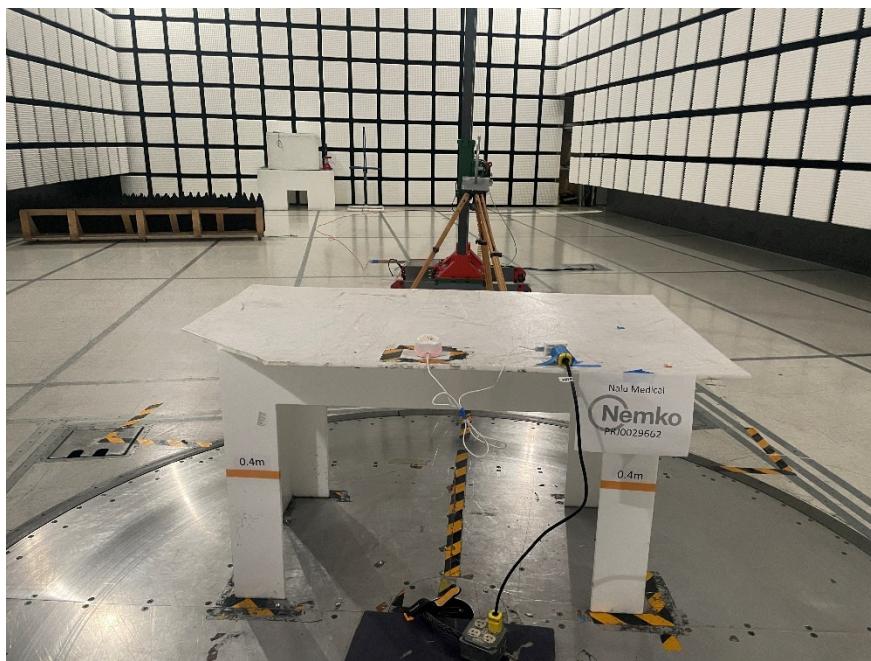


Figure 4 - Radiated emissions below 30 MHz (9 kHz – 30 MHz), 90 Degrees, rear view

FCC ID:

Nalu Medical Inc

1.2 Radiated emissions test setup, continued



Figure 5 - Radiated emissions below 1 GHz (30 – 1000 MHz), front view.



Figure 6 - Radiated emissions below 1 GHz (30 – 1000 MHz), rear view.

FCC ID:

Nalu Medical Inc

1.2 Conducted Emissions test Setup



Figure 7 – Test setup, front view.



Figure 8 – Test setup, side view.

FCC ID:

Nalu Medical Inc

1.3 Frequency stability setup



Figure 9 – Test setup, frequency stability.