



SAR
Dipole Performance Measurement
Report

EUT Type: SAR Validation Dipole and Waveguide

Model Name: DIP2G450

Brand Name: SATIMO

Test Conclusion: Pass

Test Date: 08 July 2022

Date of Issue: 11 July 2022

Testing Engineer : Shi fan-long

((Shifan. Long)

Technical Manager : Sean She

(Sean she)

Authorized Signatory : Bovey Yang

(Bovey Yang)





ISSUED BY
Shenzhen STS Test Services Co., Ltd.

1. Equipment List

Kind of Equipment	Manufacturer	Type No.	Serial No.	Last Calibration	Calibrated Until
PC	Acer	N/A	N/A	N/A	N/A
E-Field Probe	MVG	SSE2	SN 07/21 EPGO352	2022.02.28	2023.02.27
Dielectric Probe Kit	MVG	SCLMP	SN 32/14 OCPG67	2022.11.15	2023.11.14
Phantom1	MVG	SAM	SN 32/14 SAM115	N/A	N/A
Phantom3	MVG	SAM	SN 21/21 ELLI48	N/A	N/A
Attenuator	Agilent	99899	DC-18GHz	N/A	N/A
Directional coupler	Narda	4226-20	3305	N/A	N/A
Network Analyzer	Agilent	8753ES	US38432810	2022.09.28	2023.09.27
Multi Meter	Keithley	Multi Meter 2000	4050073	2022.09.29	2023.09.28
Signal Generator	Agilent	N5182A	MY50140530	2022.09.28	2023.09.27
Power Amplifier	DESAY	ZHL-42W	9638	2022.10.08	2023.10.07
Power Meter	R&S	NRP	100510	2022.09.28	2023.09.27
Power Sensor	R&S	NRP-Z11	101919	2022.09.28	2023.09.27
Temperature hygrometer	SuWei	SW-108	N/A	2022.09.30	2023.09.29
Thermograph	Elitech	RC-4	S/N EF7176501537	2022.09.30	2023.09.29



2. <Justification of the extended calibration>


Referring to KDB 865664 D01, if dipoles are verified in return loss < -20dB, (within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Head 2450 MHz				
Date of Measurement	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2020.07.14	-26.03	-	46.3	-
2021.07.11	-26.42	1.50	47.25	0.95
2022.07.08	-26.91	3.38	47.40	1.1

The return loss is < -20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Head 2450 MHz

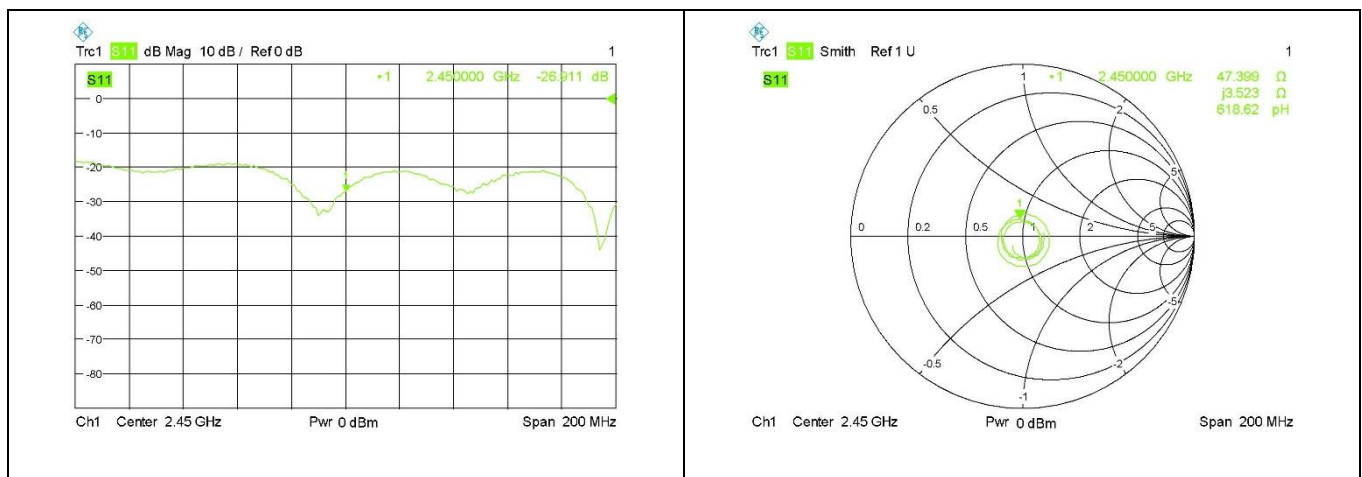



Body 2450 MHz				
Date of Measurement	Return Loss (dB)	Delta (%)	Impedance	Delta(ohm)
2020.07.14	-32.76	-	48.7	-
2021.07.11	-32.55	-0.64	47.25	-1.45
2022.07.08	-33.75	3.02	49.28	0.58

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>

Body 2450 MHz

