



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **DEKRA**  
Taoyuan City

Certificate No. **5G-Veri10-2006\_Apr24**

## CALIBRATION CERTIFICATE

Object **5G Verification Source 10 GHz - SN: 2006**

Calibration procedure(s) **QA CAL-45.v5**  
Calibration procedure for sources in air above 6 GHz

Calibration date: **April 18, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                | ID #           | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------------|----------------|-----------------------------------|------------------------|
| Reference Probe EUmWV3           | SN: 9374       | 04-Dec-23 (No. EUmWV3-Dec23)      | Dec-24                 |
| DAE4ip                           | SN: 1602       | 08-Nov-23 (No. DAE4ip-1602_Nov23) | Nov-24                 |
| Secondary Standards              | ID #           | Check Date (in house)             | Scheduled Check        |
| RF generator R&S SMF100A         | SN: 100184     | 29-Nov-23 (in house check Nov-23) | In house check: Nov-24 |
| Power sensor R&S NRP18S-10       | SN: 101258     | 29-Nov-23 (in house check Nov-23) | In house check: Nov-24 |
| Network Analyzer Keysight E5063A | SN: MY54504221 | 31-Oct-19 (in house check Oct-22) | In house check: Oct-25 |

|                |                             |                                   |                                                                                                    |
|----------------|-----------------------------|-----------------------------------|----------------------------------------------------------------------------------------------------|
| Calibrated by: | Name<br><b>Leif Klysner</b> | Function<br>Laboratory Technician | Signature<br> |
| Approved by:   | Sven Kühn                   | Technical Manager                 |               |

Issued: April 20, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

CW                      Continuous wave

## Calibration is Performed According to the Following Standards

- Internal procedure QA CAL-45, Calibration procedure for sources in air above 6 GHz.
- IEC/IEEE 63195-1, "Assessment of power density of human exposure to radio frequency fields from wireless devices in close proximity to the head and body (frequency range of 6 GHz to 300 GHz)", May 2022

## Methods Applied and Interpretation of Parameters

- *Coordinate System:* z-axis in the waveguide horn boresight, x-axis is in the direction of the E-field, y-axis normal to the others in the field scanning plane parallel to the horn flare and horn flange.
- *Measurement Conditions:* (1) 10 GHz: The radiated power is the forward power to the horn antenna minus ohmic and mismatch loss. The forward power is measured prior and after the measurement with a power sensor. During the measurements, the horn is directly connected to the cable and the antenna ohmic and mismatch losses are determined by far-field measurements. (2) 30, 45, 60 and 90 GHz: The verification sources are switched on for at least 30 minutes. Absorbers are used around the probe cub and at the ceiling to minimize reflections.
- *Horn Positioning:* The waveguide horn is mounted vertically on the flange of the waveguide source to allow vertical positioning of the EUmmW probe during the scan. The plane is parallel to the phantom surface. Probe distance is verified using mechanical gauges positioned on the flare of the horn.
- *E- field distribution:* E field is measured in two x-y-plane (10mm, 10mm +  $\lambda/4$ ) with a vectorial E-field probe. The E-field value stated as calibration value represents the E-field-maxima and the averaged (1cm<sup>2</sup> and 4cm<sup>2</sup>) power density values at 10mm in front of the horn.
- *Field polarization:* Above the open horn, linear polarization of the field is expected. This is verified graphically in the field representation.

## Calibrated Quantity

- Local peak E-field (V/m) and average of peak spatial components of the poynting vector (W/m<sup>2</sup>) averaged over the surface area of 1 cm<sup>2</sup> and 4cm<sup>2</sup> at the nominal operational frequency of the verification source. Both square and circular averaging results are listed.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                       |                               |      |
|---------------------------------------|-------------------------------|------|
| <b>DASY Version</b>                   | DASY8 Module mmWave           | V3.2 |
| <b>Phantom</b>                        | 5G Phantom                    |      |
| <b>Distance Horn Aperture - plane</b> | 10 mm                         |      |
| <b>Number of measured planes</b>      | 2 (10mm, 10mm + $\lambda/4$ ) |      |
| <b>Frequency</b>                      | 10 GHz $\pm$ 10 MHz           |      |

## Calibration Parameters, 10 GHz

### Circular Averaging

| Distance Horn Aperture to Measured Plane | <b><i>Prad'</i></b><br>(mW) | <b>Max E-field</b><br>(V/m) | Uncertainty<br>(k = 2) | Avg Power Density<br>Avg (psPDn+, psPDtot+, psPDmod+)<br>(W/m <sup>2</sup> ) |                         | Uncertainty<br>(k = 2) |
|------------------------------------------|-----------------------------|-----------------------------|------------------------|------------------------------------------------------------------------------|-------------------------|------------------------|
|                                          |                             |                             |                        | <b>1 cm<sup>2</sup></b>                                                      | <b>4 cm<sup>2</sup></b> |                        |
| 10 mm                                    | 138                         | <b>297</b>                  | 1.27 dB                | <b>237</b>                                                                   | <b>188</b>              | 1.28 dB                |

| Distance Horn Aperture to Measured Plane | <b><i>Prad'</i></b><br>(mW) | <b>Max E-field</b><br>(V/m) | Uncertainty<br>(k = 2) | Power Density<br>psPDn+, psPDtot+, psPDmod+<br>(W/m <sup>2</sup> ) |                         | Uncertainty<br>(k = 2) |
|------------------------------------------|-----------------------------|-----------------------------|------------------------|--------------------------------------------------------------------|-------------------------|------------------------|
|                                          |                             |                             |                        | <b>1 cm<sup>2</sup></b>                                            | <b>4 cm<sup>2</sup></b> |                        |
| 10 mm                                    | 138                         | <b>297</b>                  | 1.27 dB                | <b>236, 236, 239</b>                                               | <b>186, 186, 192</b>    | 1.28 dB                |

### Square Averaging

| Distance Horn Aperture to Measured Plane | <b><i>Prad'</i></b><br>(mW) | <b>Max E-field</b><br>(V/m) | Uncertainty<br>(k = 2) | Avg Power Density<br>Avg (psPDn+, psPDtot+, psPDmod+)<br>(W/m <sup>2</sup> ) |                         | Uncertainty<br>(k = 2) |
|------------------------------------------|-----------------------------|-----------------------------|------------------------|------------------------------------------------------------------------------|-------------------------|------------------------|
|                                          |                             |                             |                        | <b>1 cm<sup>2</sup></b>                                                      | <b>4 cm<sup>2</sup></b> |                        |
| 10 mm                                    | 138                         | <b>297</b>                  | 1.27 dB                | <b>237</b>                                                                   | <b>187</b>              | 1.28 dB                |

| Distance Horn Aperture to Measured Plane | <b><i>Prad'</i></b><br>(mW) | <b>Max E-field</b><br>(V/m) | Uncertainty<br>(k = 2) | Power Density<br>psPDn+, psPDtot+, psPDmod+<br>(W/m <sup>2</sup> ) |                         | Uncertainty<br>(k = 2) |
|------------------------------------------|-----------------------------|-----------------------------|------------------------|--------------------------------------------------------------------|-------------------------|------------------------|
|                                          |                             |                             |                        | <b>1 cm<sup>2</sup></b>                                            | <b>4 cm<sup>2</sup></b> |                        |
| 10 mm                                    | 138                         | <b>297</b>                  | 1.27 dB                | <b>236, 236, 239</b>                                               | <b>185, 186, 191</b>    | 1.28 dB                |

### Max Power Density

| Distance Horn Aperture to Measured Plane | <b><i>Prad'</i></b><br>(mW) | <b>Max E-field</b><br>(V/m) | Uncertainty<br>(k = 2) | Max Power Density<br>Sn, Stot,  Stot <br>(W/m <sup>2</sup> ) | Uncertainty<br>(k = 2) |
|------------------------------------------|-----------------------------|-----------------------------|------------------------|--------------------------------------------------------------|------------------------|
| 10 mm                                    | 138                         | <b>297</b>                  | 1.27 dB                | <b>257, 257, 257</b>                                         | 1.28 dB                |


<sup>1</sup> Assessed ohmic and mismatch loss plus numerical offset: 0.60 dB

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters

|                                      |                                 |
|--------------------------------------|---------------------------------|
| Impedance, transformed to feed point | 43.0 $\Omega$ - 0.65 j $\Omega$ |
| Return Loss                          | - 22.4 dB                       |

Impedance Measurement Plot

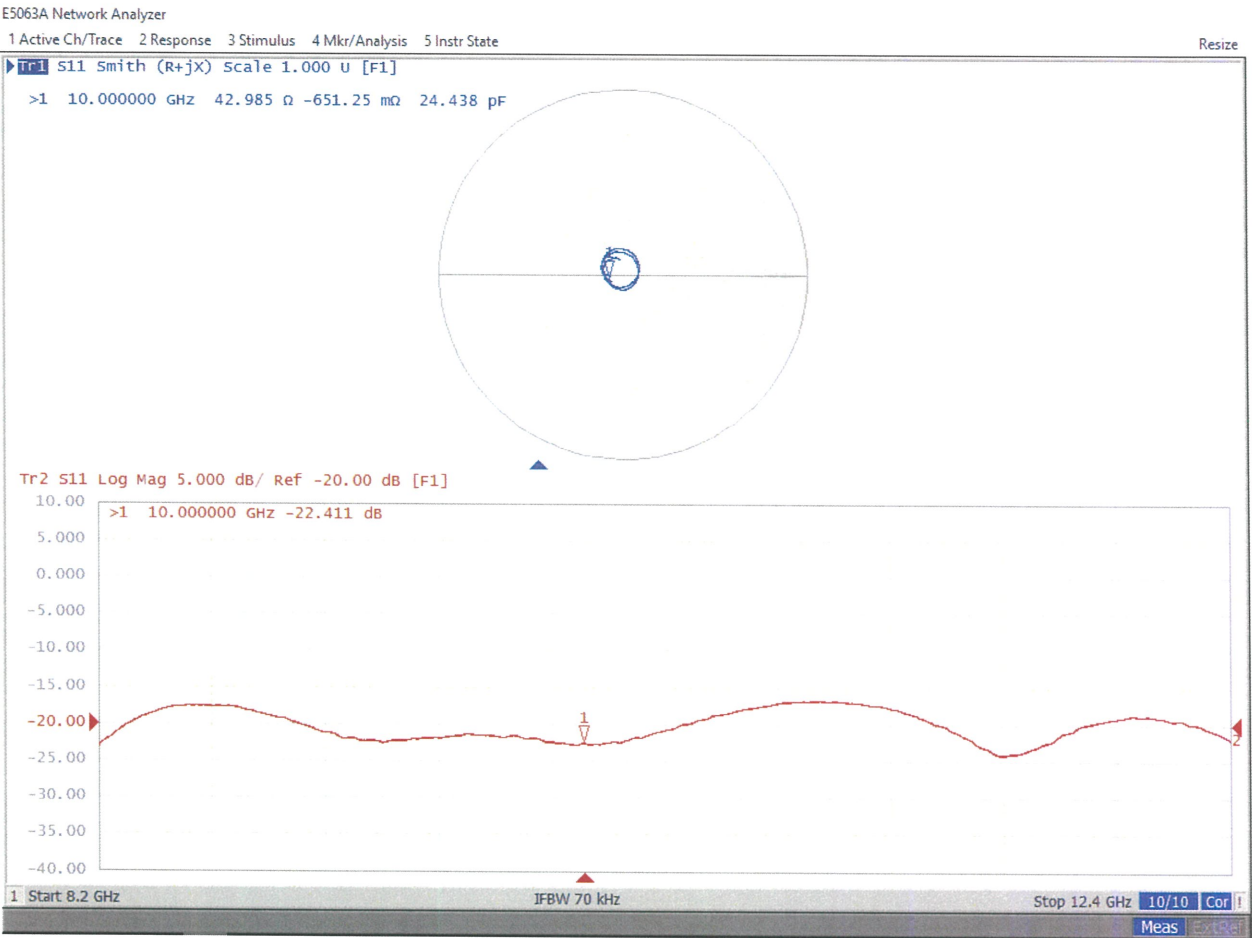



DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Properties

| Name, Manufacturer            | Dimensions [mm]       | IMEI     | DUT Type |
|-------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 100.0 | SN: 2006 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|--------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW     | 10000.0, 10000                  | 1.0               |

Hardware Setup


| Phantom               | Medium | Probe, Calibration Date               | DAE, Calibration Date     |
|-----------------------|--------|---------------------------------------|---------------------------|
| mmWave Phantom - 1002 | Air    | EUmmWV3 - SN9374_F1-55GHz, 2023-12-04 | DAE4ip Sn1602, 2023-11-08 |

Scan Setup

| Sensor Surface [mm] | 5G Scan               |
|---------------------|-----------------------|
| MAIA                | 10.0<br>MAIA not used |

Measurement Results

|                        | 5G Scan            |
|------------------------|--------------------|
| Date                   | 2024-04-18, 10:22  |
| Avg. Area [cm²]        | 1.00               |
| Avg. Type              | Circular Averaging |
| psPDn+ [W/m²]          | 236                |
| psPDtot+ [W/m²]        | 236                |
| psPDmod+ [W/m²]        | 239                |
| Max(Sn) [W/m²]         | 257                |
| Max(Stot) [W/m²]       | 257                |
| Max( Stot ) [W/m²]     | 257                |
| E <sub>max</sub> [V/m] | 297                |
| Power Drift [dB]       | -0.00              |

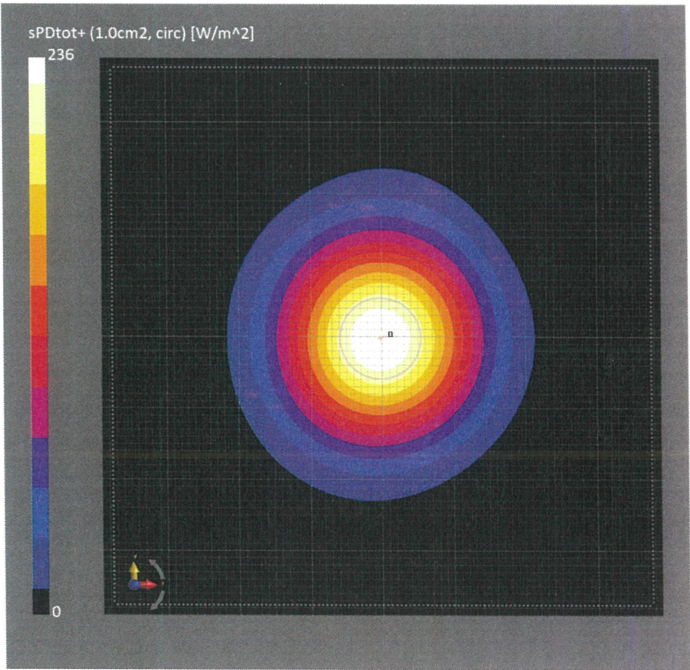

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Properties

|                               |                       |          |          |
|-------------------------------|-----------------------|----------|----------|
| Name, Manufacturer            | Dimensions [mm]       | IMEI     | DUT Type |
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 100.0 | SN: 2006 | -        |

Exposure Conditions

|                 |                              |                 |        |                                 |                   |
|-----------------|------------------------------|-----------------|--------|---------------------------------|-------------------|
| Phantom Section | Position, Test Distance [mm] | Band            | Group, | Frequency [MHz], Channel Number | Conversion Factor |
| 5G -            | 10.0 mm                      | Validation band | CW     | 10000.0, 10000                  | 1.0               |

Hardware Setup


|                       |        |                                       |                           |
|-----------------------|--------|---------------------------------------|---------------------------|
| Phantom               | Medium | Probe, Calibration Date               | DAE, Calibration Date     |
| mmWave Phantom - 1002 | Air    | EUmmWV3 - SN9374_F1-55GHz, 2023-12-04 | DAE4ip Sn1602, 2023-11-08 |

Scan Setup

|                     |               |
|---------------------|---------------|
| Sensor Surface [mm] | 5G Scan       |
| MAIA                | 10.0          |
|                     | MAIA not used |

Measurement Results

|                        |                    |
|------------------------|--------------------|
| Date                   | 5G Scan            |
| 2024-04-18, 10:22      |                    |
| Avg. Area [cm²]        | 4.00               |
| Avg. Type              | Circular Averaging |
| psPDn+ [W/m²]          | 186                |
| psPDtot+ [W/m²]        | 186                |
| psPDmod+ [W/m²]        | 192                |
| Max(Sn) [W/m²]         | 257                |
| Max(Stot) [W/m²]       | 257                |
| Max( Stot ) [W/m²]     | 257                |
| E <sub>max</sub> [V/m] | 297                |
| Power Drift [dB]       | -0.00              |

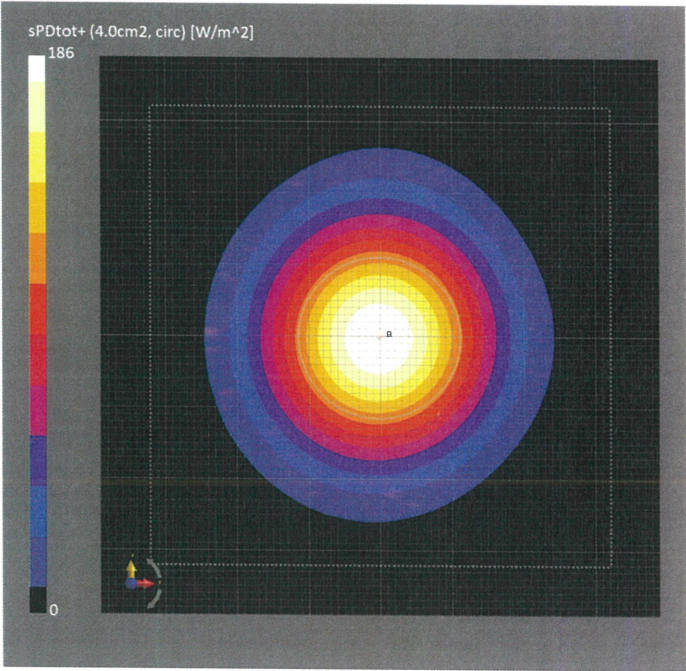

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Properties

| Name, Manufacturer            | Dimensions [mm]       | IMEI     | DUT Type |
|-------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 100.0 | SN: 2006 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|--------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW     | 10000.0, 10000                  | 1.0               |

Hardware Setup


| Phantom               | Medium | Probe, Calibration Date               | DAE, Calibration Date     |
|-----------------------|--------|---------------------------------------|---------------------------|
| mmWave Phantom - 1002 | Air    | EUmmWV3 - SN9374_F1-55GHz, 2023-12-04 | DAE4ip Sn1602, 2023-11-08 |

Scan Setup

| Sensor Surface [mm] | 5G Scan               |
|---------------------|-----------------------|
| MAIA                | 10.0<br>MAIA not used |

Measurement Results

| Date                   | 5G Scan           |
|------------------------|-------------------|
| 2024-04-18, 10:22      | 2024-04-18, 10:22 |
| Avg. Area [cm²]        | 1.00              |
| Avg. Type              | Square Averaging  |
| psPDn+ [W/m²]          | 236               |
| psPDtot+ [W/m²]        | 236               |
| psPDmod+ [W/m²]        | 239               |
| Max(Sn) [W/m²]         | 257               |
| Max(Stot) [W/m²]       | 257               |
| Max( Stot ) [W/m²]     | 257               |
| E <sub>max</sub> [V/m] | 297               |
| Power Drift [dB]       | -0.00             |

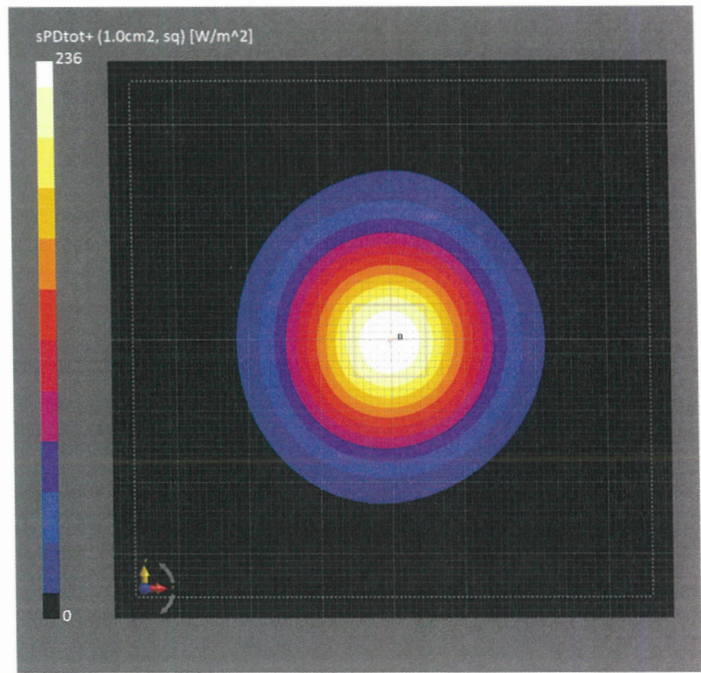



DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Properties

|                               |                       |          |          |
|-------------------------------|-----------------------|----------|----------|
| Name, Manufacturer            | Dimensions [mm]       | IMEI     | DUT Type |
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 100.0 | SN: 2006 | -        |

Exposure Conditions

|                 |                              |                 |        |                                 |                   |
|-----------------|------------------------------|-----------------|--------|---------------------------------|-------------------|
| Phantom Section | Position, Test Distance [mm] | Band            | Group, | Frequency [MHz], Channel Number | Conversion Factor |
| 5G -            | 10.0 mm                      | Validation band | CW     | 10000.0, 10000                  | 1.0               |

Hardware Setup

|                       |        |                                       |                           |
|-----------------------|--------|---------------------------------------|---------------------------|
| Phantom               | Medium | Probe, Calibration Date               | DAE, Calibration Date     |
| mmWave Phantom - 1002 | Air    | EUmmWV3 - SN9374_F1-55GHz, 2023-12-04 | DAE4ip Sn1602, 2023-11-08 |

Scan Setup

|                     |                       |
|---------------------|-----------------------|
| Sensor Surface [mm] | 5G Scan               |
| MAIA                | 10.0<br>MAIA not used |

Measurement Results

|                        |                   |
|------------------------|-------------------|
| Date                   | 5G Scan           |
| Avg. Area [cm²]        | 2024-04-18, 10:22 |
| Avg. Type              | 4.00              |
| psPDn+ [W/m²]          | Square Averaging  |
| psPDtot+ [W/m²]        | 185               |
| psPDmod+ [W/m²]        | 186               |
| Max(Sn) [W/m²]         | 191               |
| Max(Stot) [W/m²]       | 257               |
| Max( Stot ) [W/m²]     | 257               |
| E <sub>max</sub> [V/m] | 297               |
| Power Drift [dB]       | -0.00             |

