

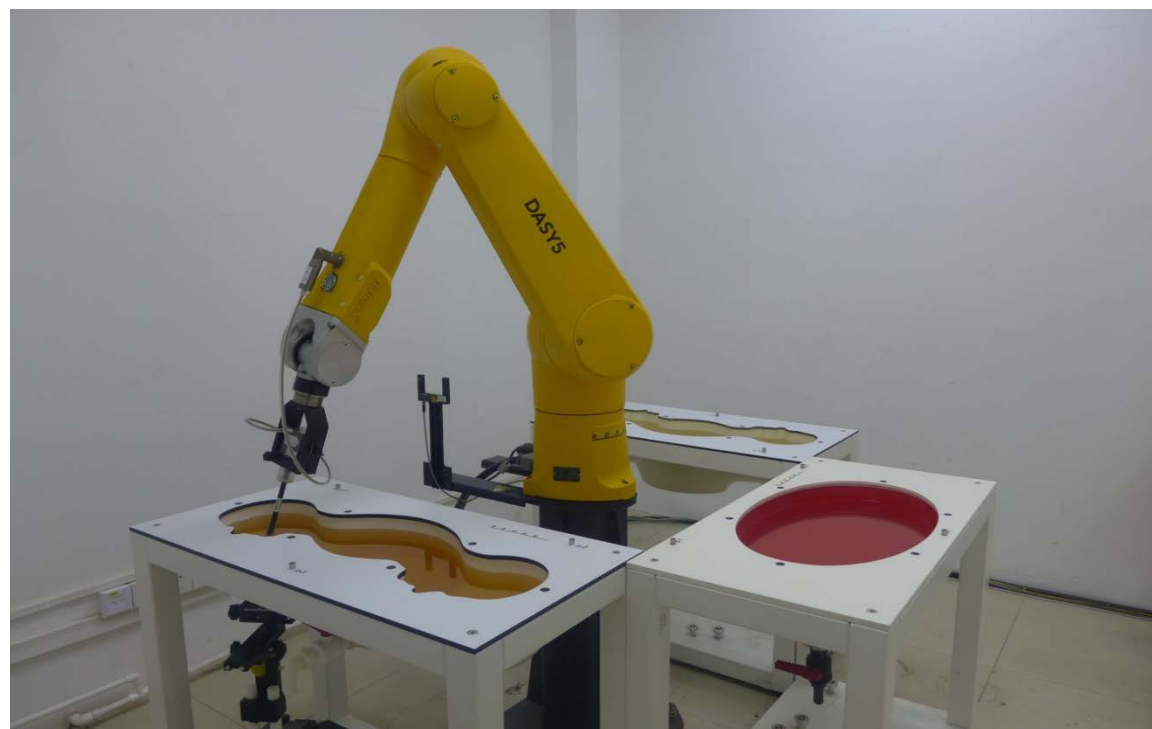


Appendix D

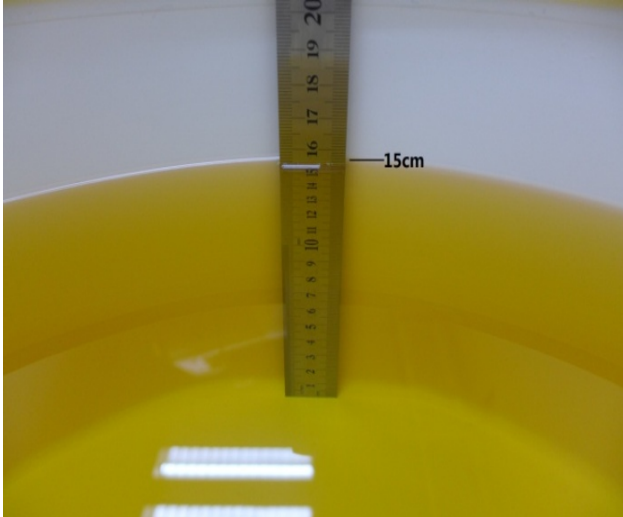
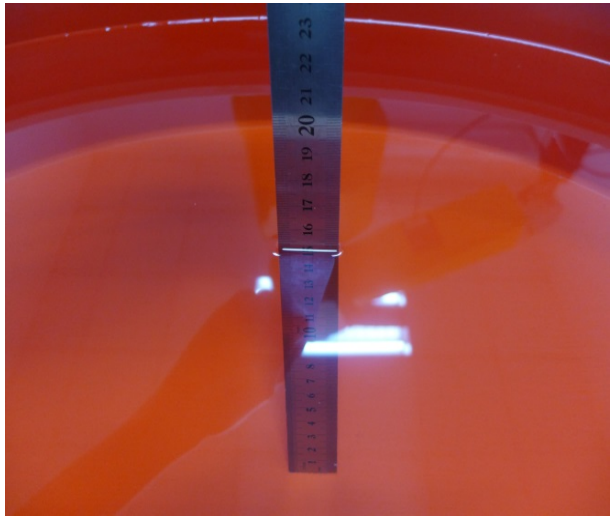
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

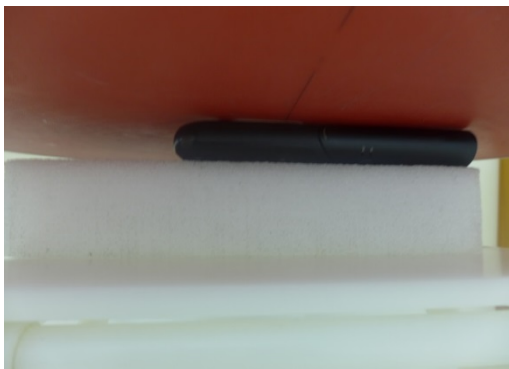
1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Body 2450	Photo 2: Tissue Simulant Liquid for Body 5G
 A photograph showing a yellow liquid in a white container. A ruler is placed vertically next to the liquid, and a horizontal line indicates a depth of 15cm.	 A photograph showing a red liquid in a white container. A ruler is placed vertically next to the liquid.

3. Photographs of EUT test position

Photo 3: Front side 0mm	Photo 4: Back side 0mm
	
Photo 5: Left side 0mm	Photo 6: Right side 0mm
	
Photo 7: Top side 0mm	NA
	NA

4. EUT Constructional Details

Photo 8: Front View	Photo 9: Back View
