

Figure 1: Front View of Trilogy EVO Device with front panel removed showing Display PCA and System PCA

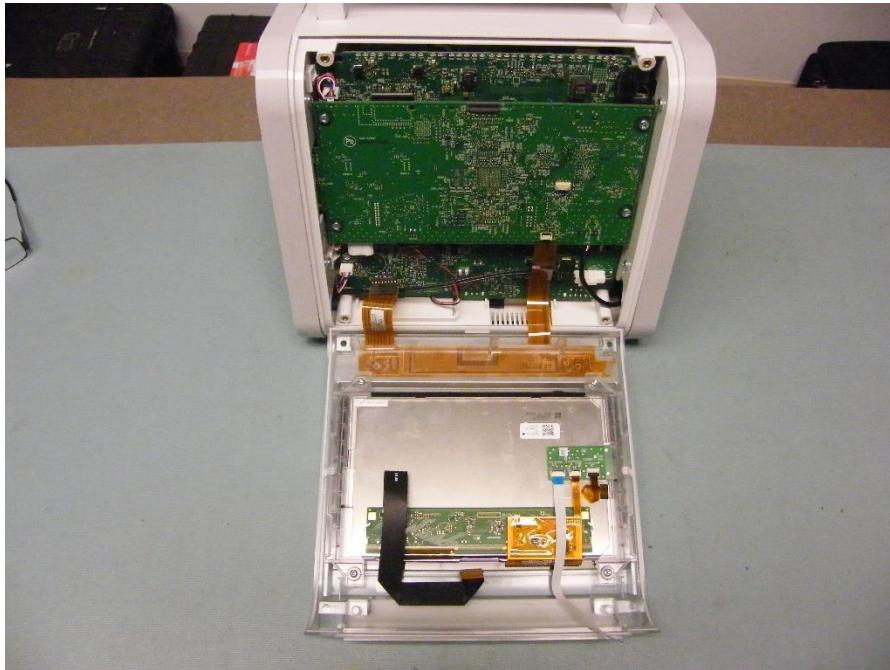


Figure 2: Trilogy EVO Device with front panel partially removed showing System PCA, Display PCA, Keypad and Display.



Philips-Respirronics
1740 Golden Mile Hwy
Monroeville, PA 15146

PHILIPS

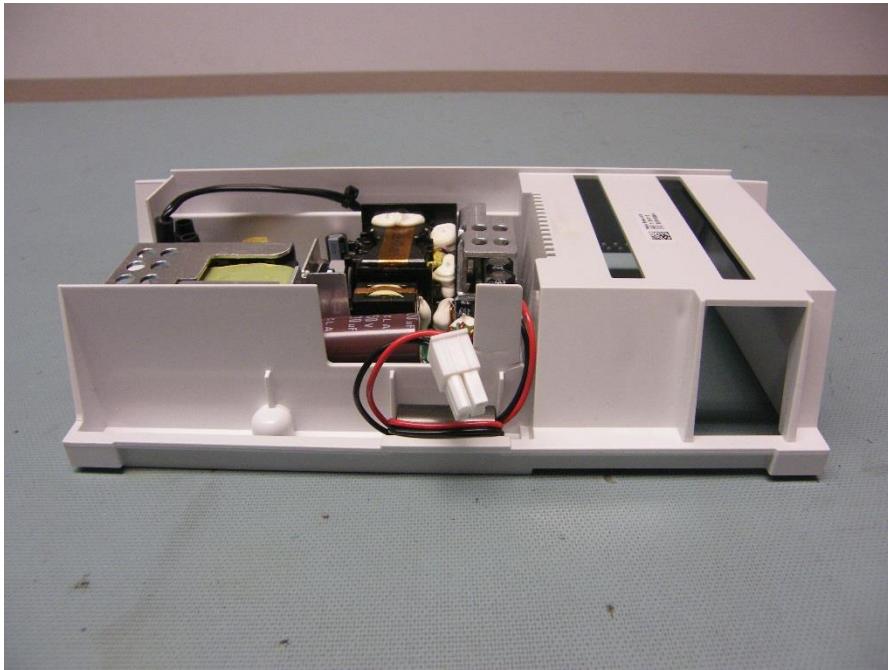


Figure 3: Trilogy Evo base showing power supply and Internal Battery compartment

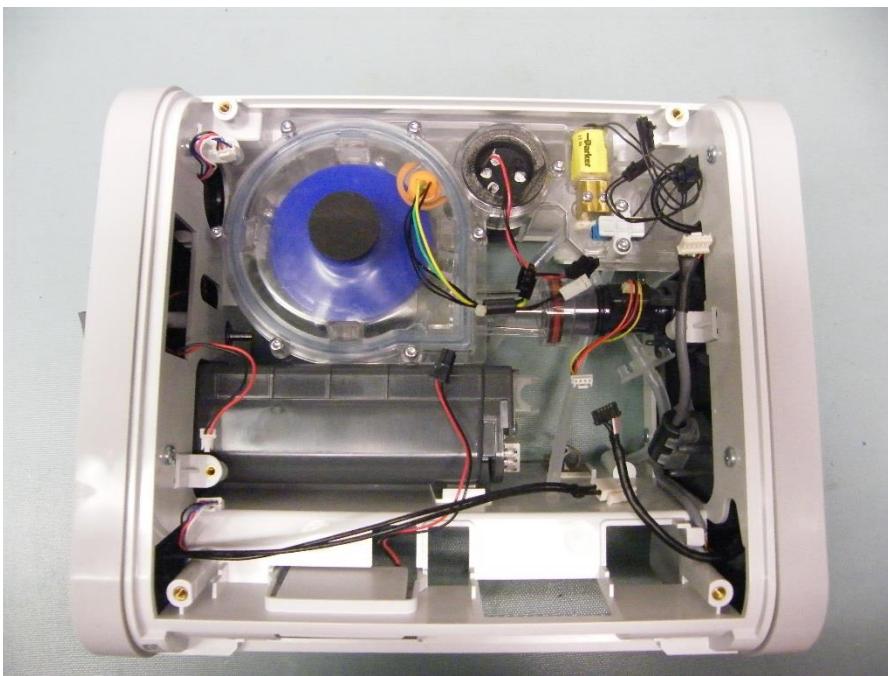


Figure 4: Rear View of Trilogy EVO showing Blower and Detachable Battery compartment.



Philips-Respirronics
1740 Golden Mile Hwy
Monroeville, PA 15146

PHILIPS

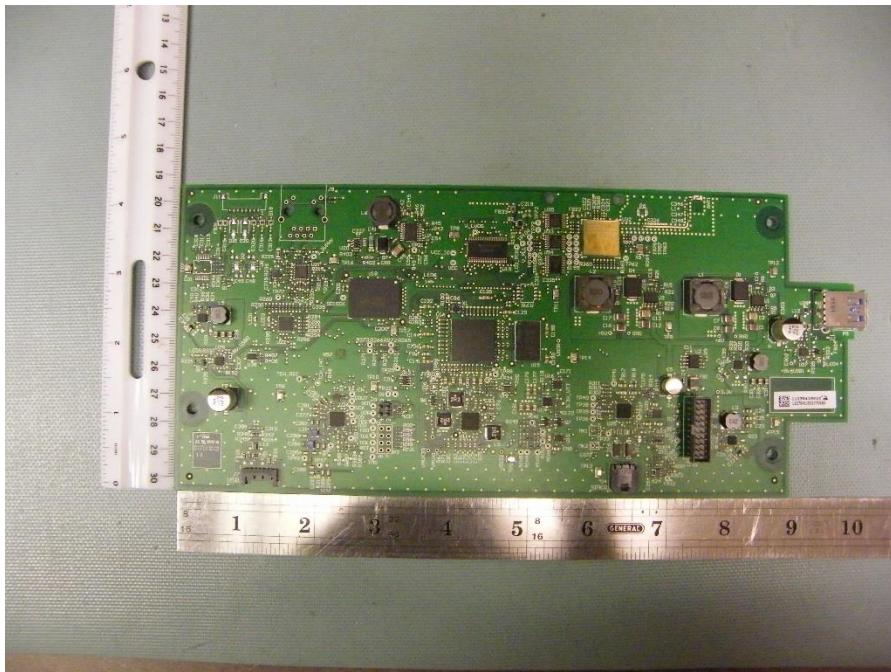


Figure 5: Top View of Trilogy EVO Display PCA

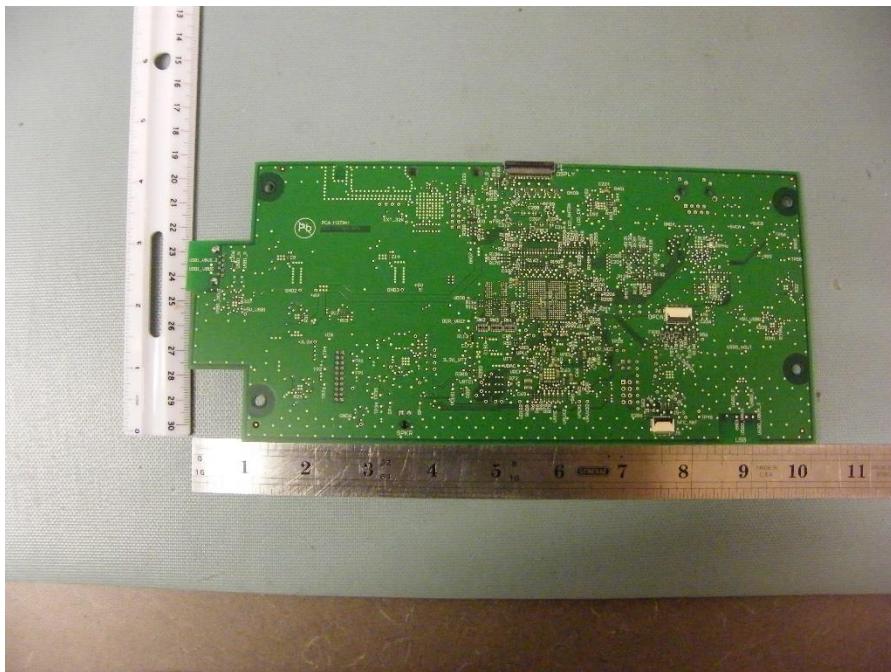


Figure 6: Top View of Trilogy EVO Display PCA



Philips-Respirronics
1740 Golden Mile Hwy
Monroeville, PA 15146

PHILIPS

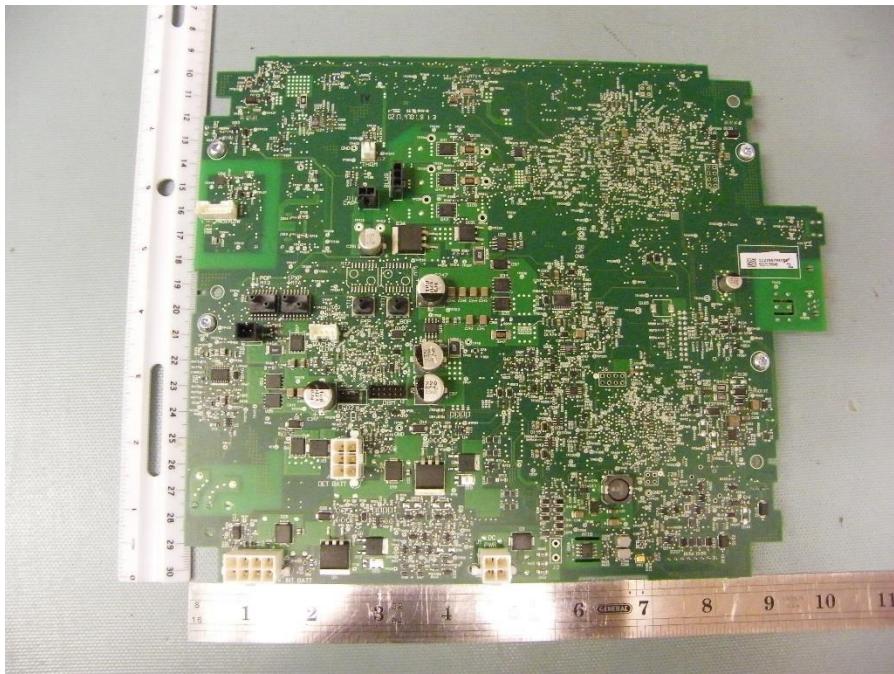


Figure 7: Top View of Trilogy EVO System PCA

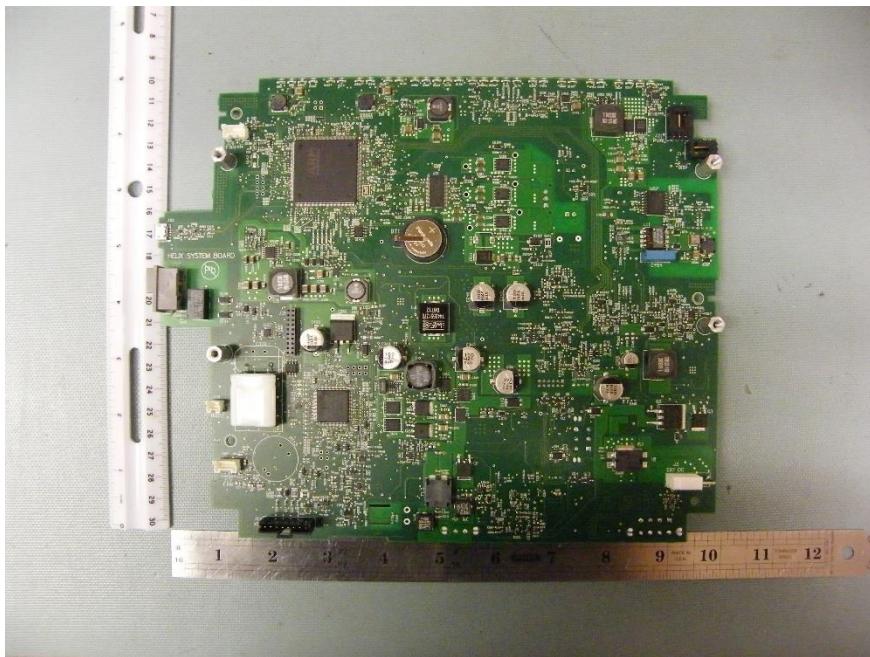


Figure 8: Bottom View of Trilogy EVO System PCA



Philips-Respirronics
1740 Golden Mile Hwy
Monroeville, PA 15146

PHILIPS



Figure 9: Rear View of OBM version Trilogy EVO with filter removed



Figure 10: Rear View of OBM version Trilogy EVO with OBM module removed



Philips-Respirronics
1740 Golden Mile Hwy
Monroeville, PA 15146

PHILIPS

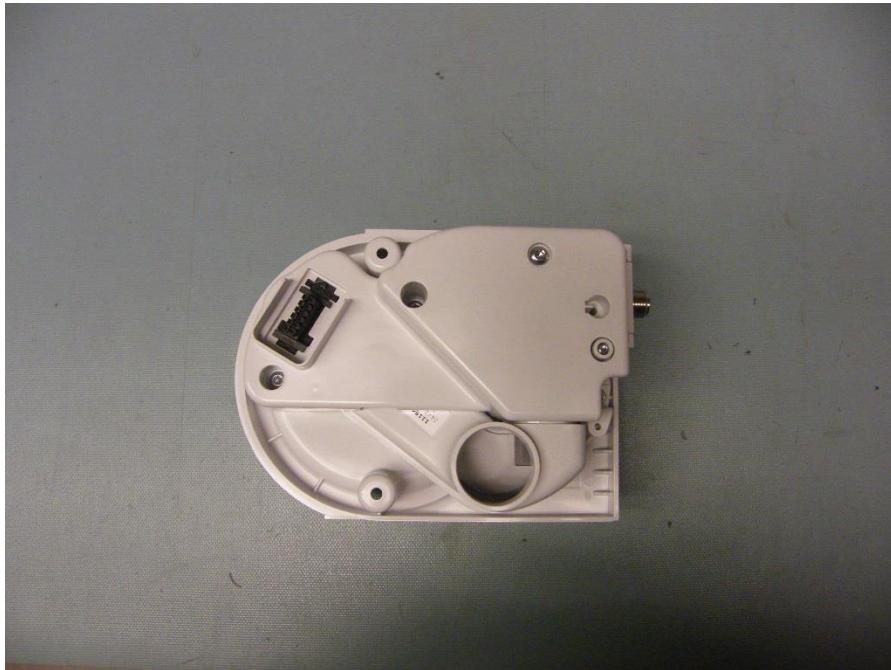


Figure 11: OBM module

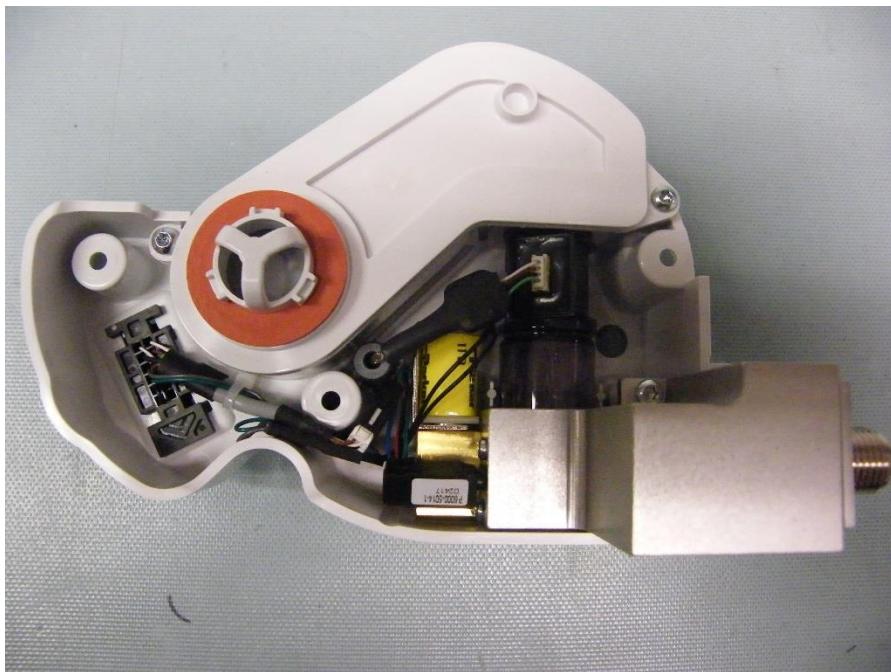


Figure 12: Interior View of OBM module



Philips-Respirronics
1740 Golden Mile Hwy
Monroeville, PA 15146

