

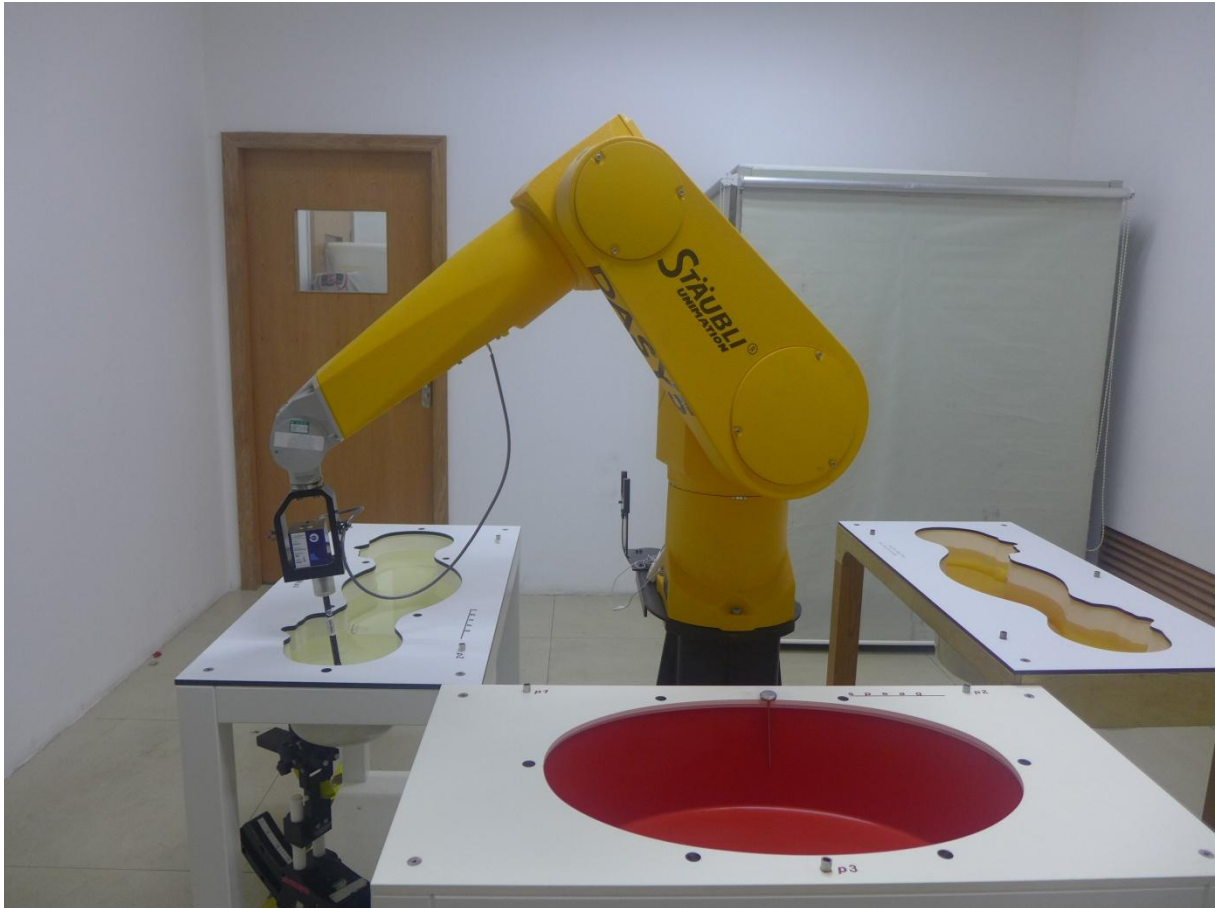


Appendix D

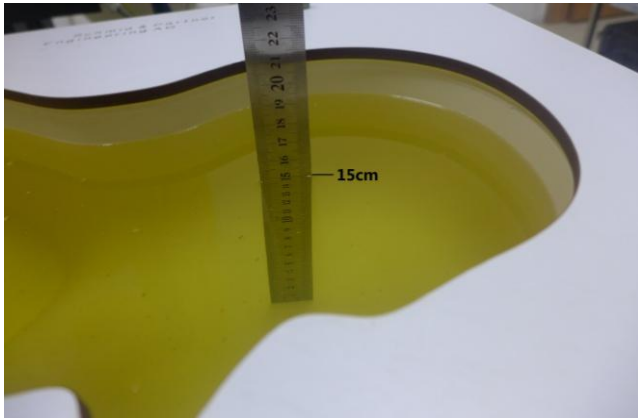
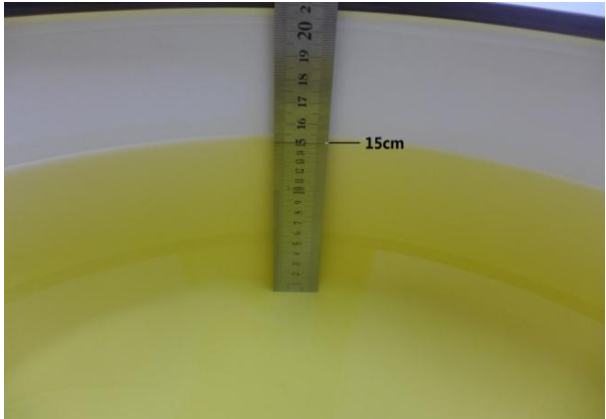
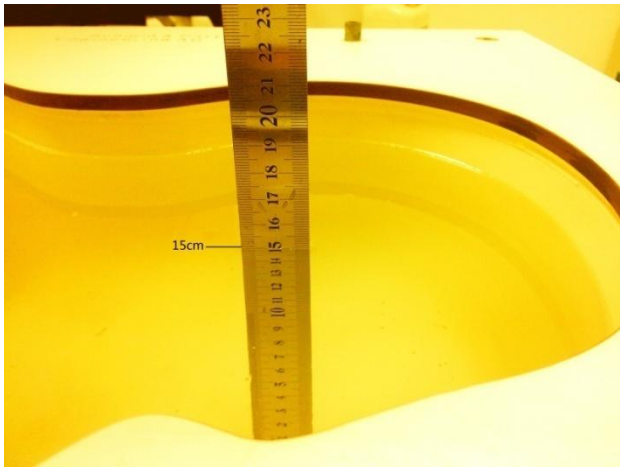
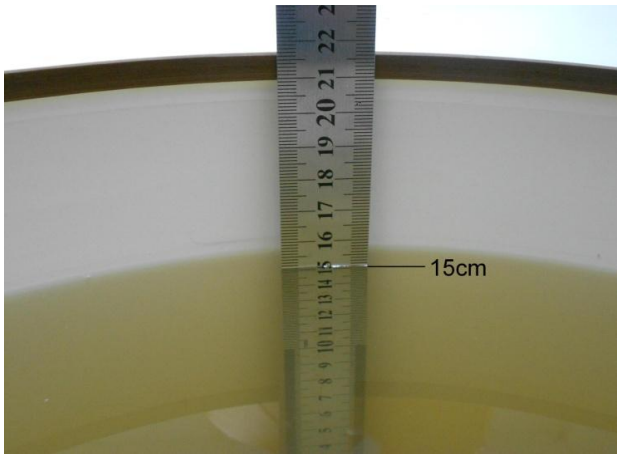
Photographs

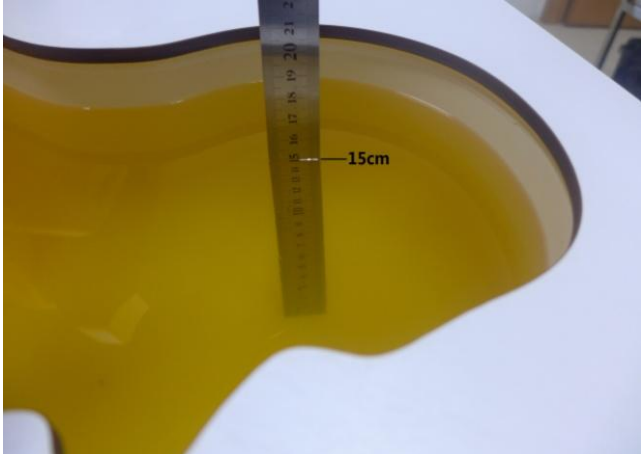
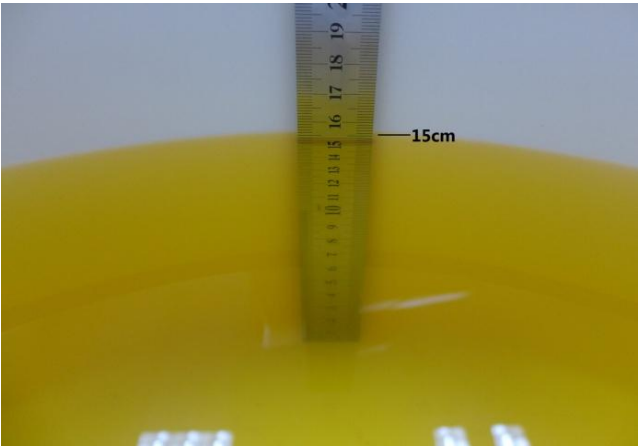
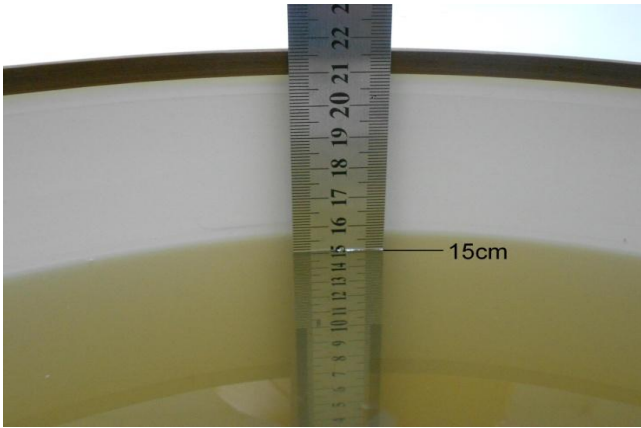
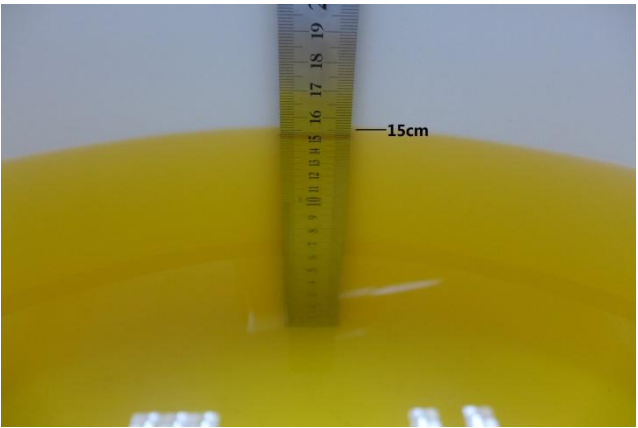
1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

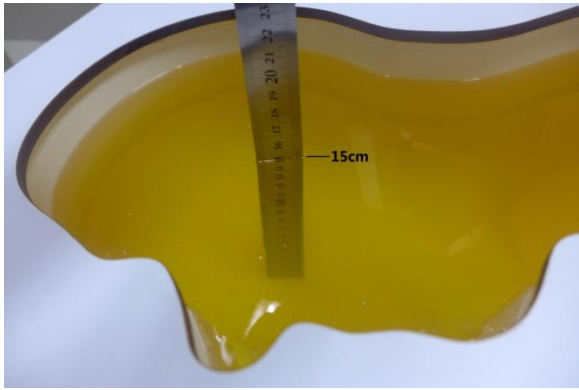
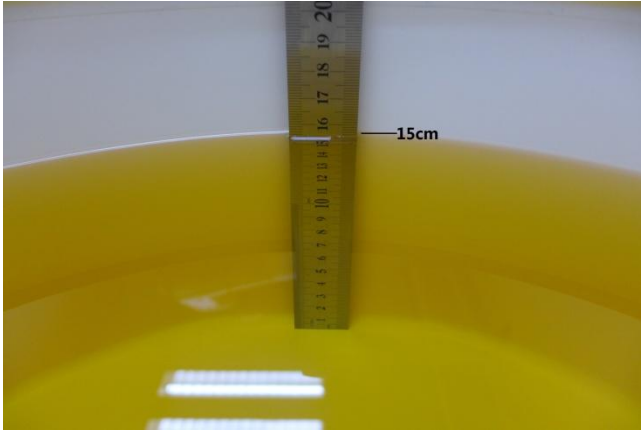
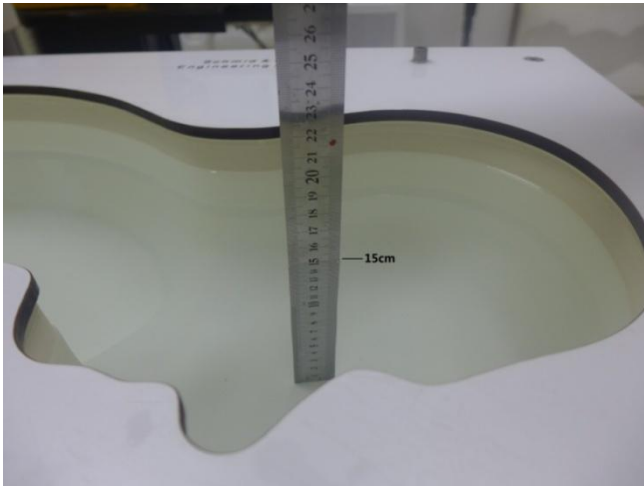
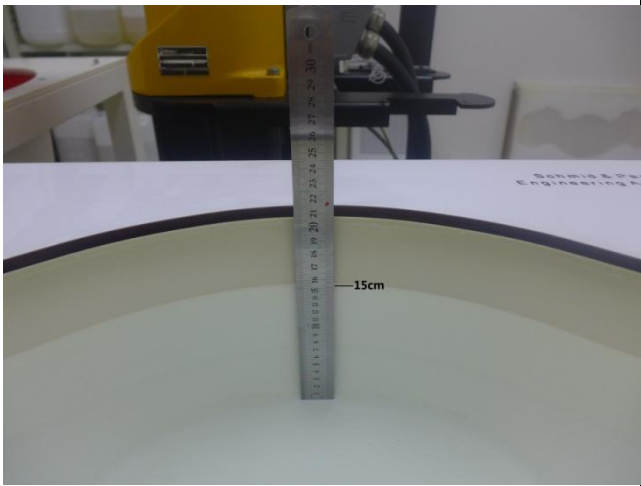
1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Body 750
	
Photo 3: Tissue Simulant Liquid for Head 835	Photo 4: Tissue Simulant Liquid for Body 835
	

<p>Photo 5: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 6: Tissue Simulant Liquid for Body 1750</p>
	
<p>Photo 7: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 8: Tissue Simulant Liquid for Body 1900</p>
	

<p>Photo 9: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 10: Tissue Simulant Liquid for Body 2450</p>
	
<p>Photo 11: Tissue Simulant Liquid for Head 5G</p>	<p>Photo 12: Tissue Simulant Liquid for Body 5G</p>
	

3. Photographs of EUT test position


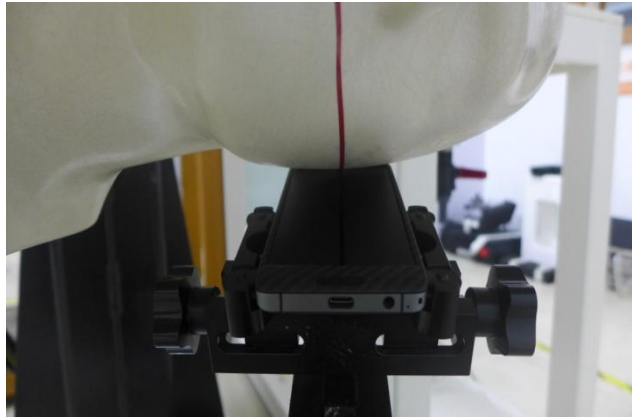
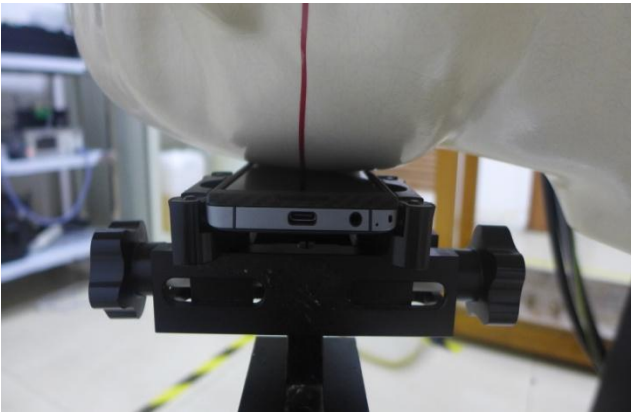
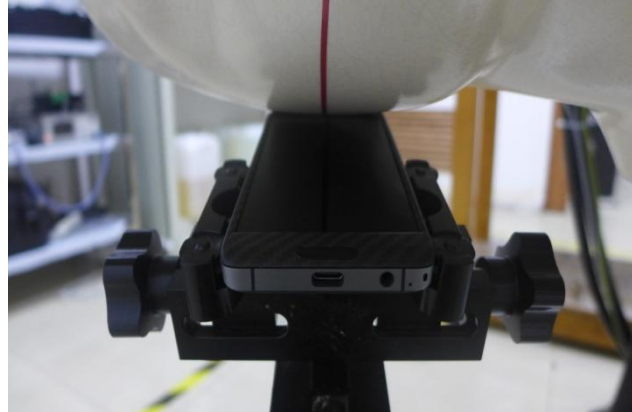


<p>Photo 13: Left touch cheek</p>	<p>Photo 14: Left tilted 15 degree</p>
	
<p>Photo 15: Right touch cheek</p>	<p>Photo 16: Right tilted 15 degree</p>
	
<p>Photo 17: Front side 15mm</p>	<p>Photo 18: Back side 15mm</p>
	

Photo 19: Front side 10mm

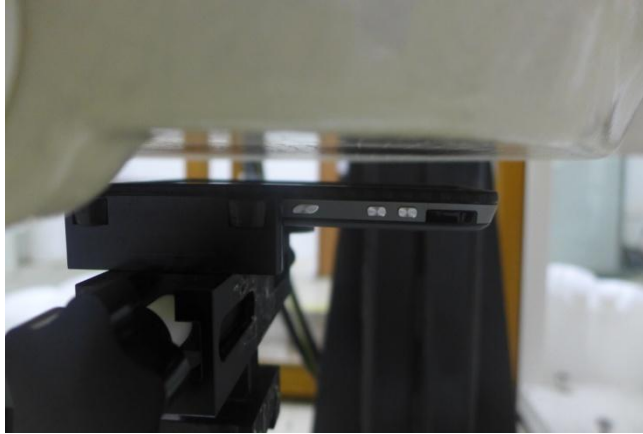


Photo 20: Back side 10mm



Photo 21: Left side 10mm



Photo 22: Right side 10mm



Photo 23: Top side 10mm

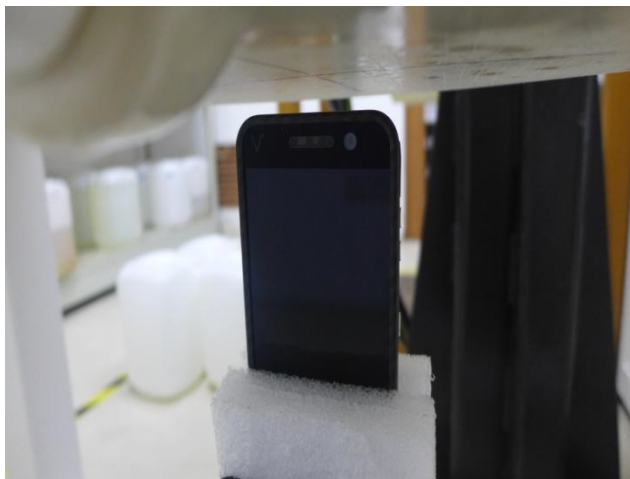
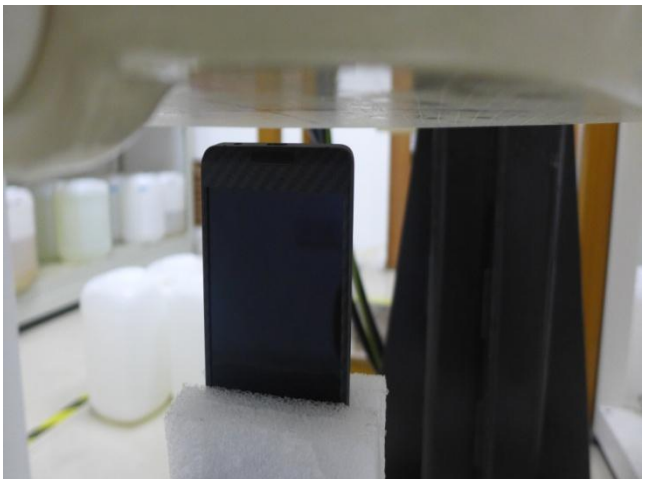




Photo 24: Bottom side 10mm



4. EUT Constructional Details

<p align="center">Photo 25: Front View</p>	<p align="center">Photo 26: Back View</p>
	
<p align="center">Photo 27: Accessory</p>	<p align="center">N/A</p>
	<p align="center">N/A</p>