



App E

Dipole calibration record

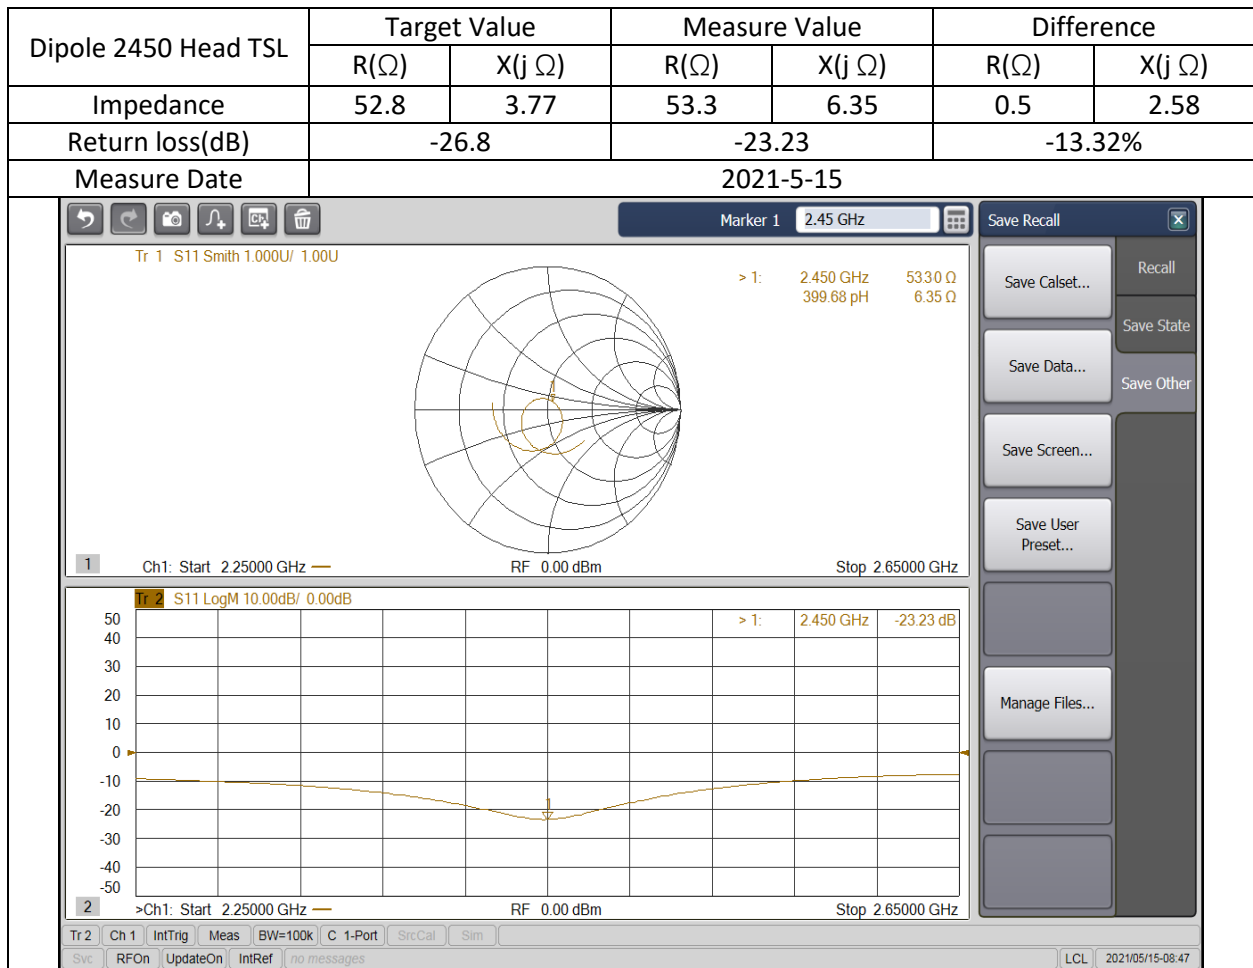

Dipole 5250 Head TSL	Target Value		Measure Value		Difference	
	R(Ω)	X(j Ω)	R(Ω)	X(j Ω)	R(Ω)	X(j Ω)
Impedance	51.3	-3.03	48.93	-2.33	-2.37	0.7
Return loss(dB)	-29.7		-28.02		-5.66%	
Measure Date	2021-5-15					

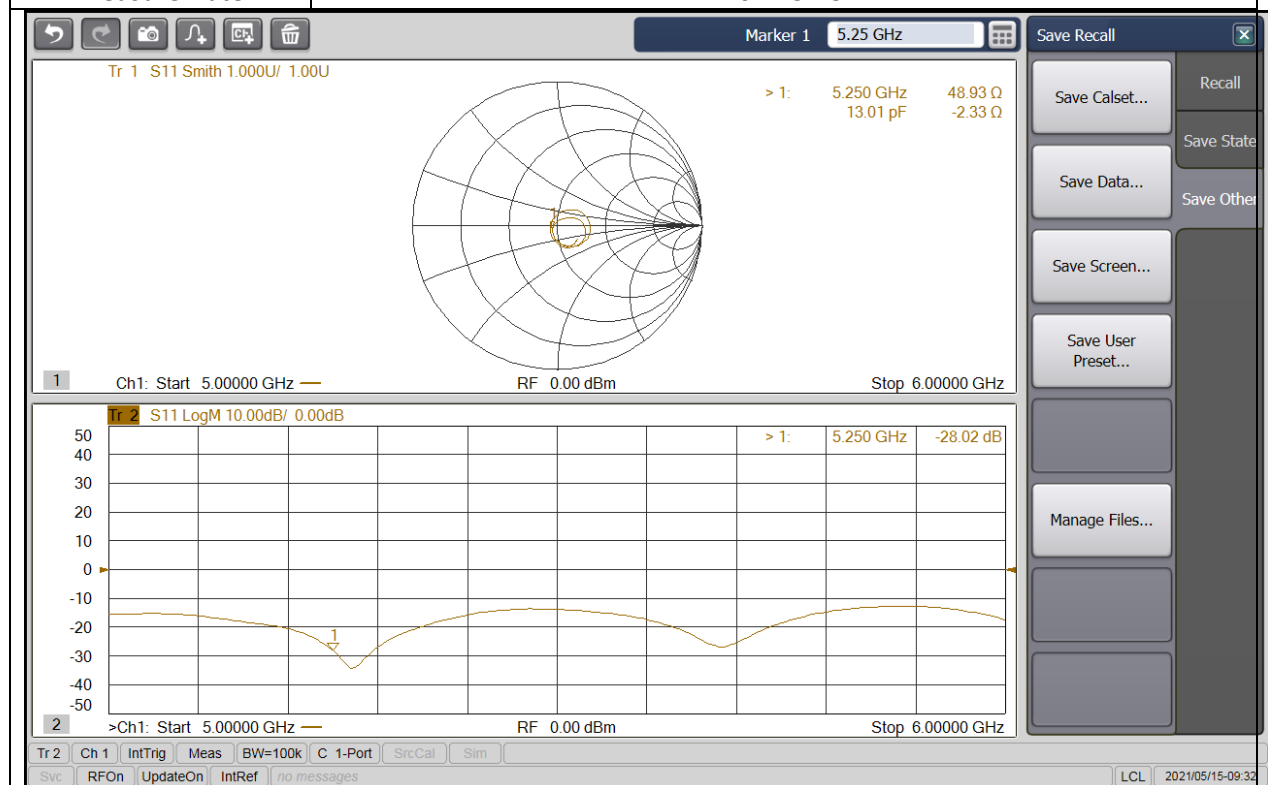

Dipole 5600 Head TSL	Target Value		Measure Value		Difference	
	R(Ω)	X(j Ω)	R(Ω)	X(j Ω)	R(Ω)	X(j Ω)
Impedance	53	1.64	50.78	-1.55	-2.22	-3.19
Return loss(dB)	-29.5		-35.19		19.29%	
Measure Date	2021-5-15					

