


Impedance Plot for SN 29/15 DIP 2G450-393
2450 Head

Calibrated impedance: $52.3\Omega + 3.4j\Omega$; Measurement impedance: $55.8\Omega + 1.6j\Omega$ (within 5Ω)



Calibrated return loss: -27.80dB; Measurement return loss: -24.53dB (within 20%)

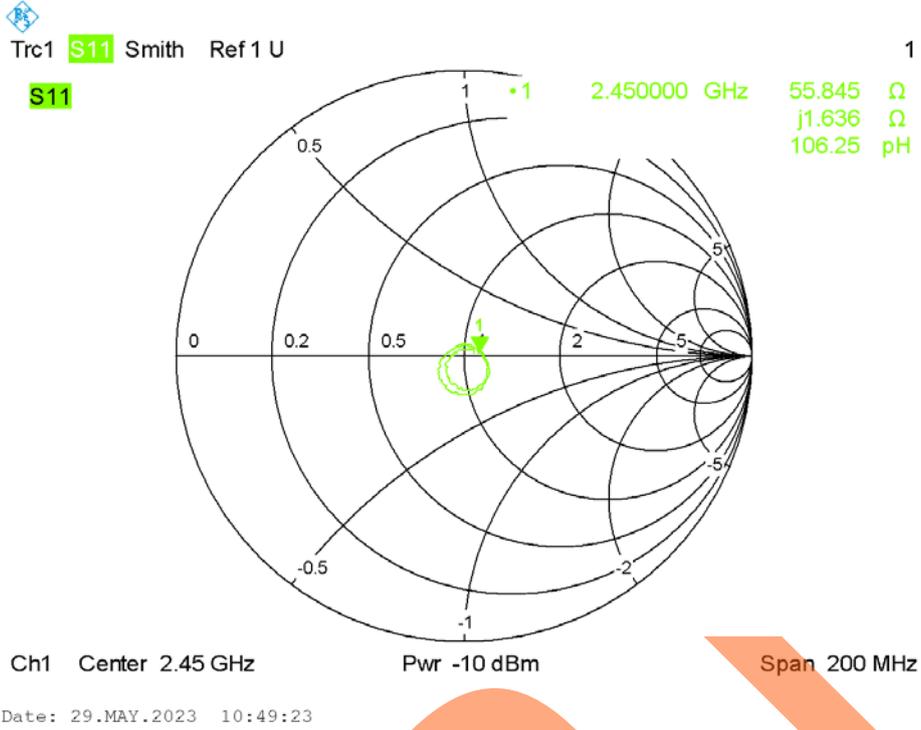